
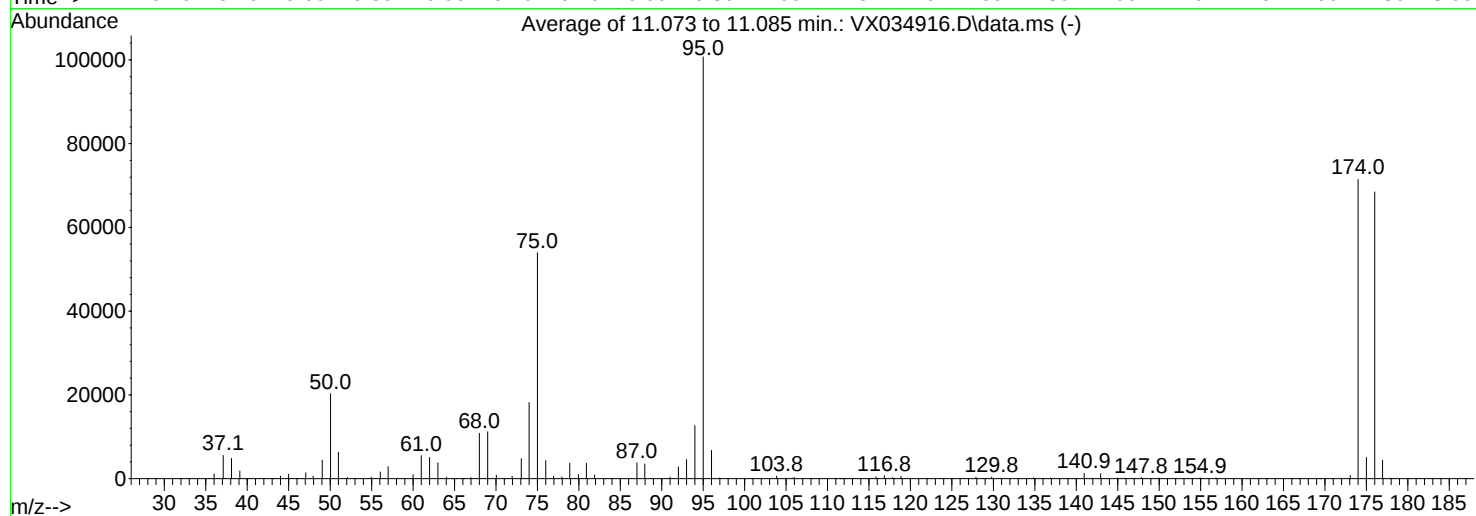


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040323\
Data File : VX034916.D
Acq On : 03 Apr 2023 08:43
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Title : SW846 8260
Last Update : Sat Apr 01 01:50:18 2023

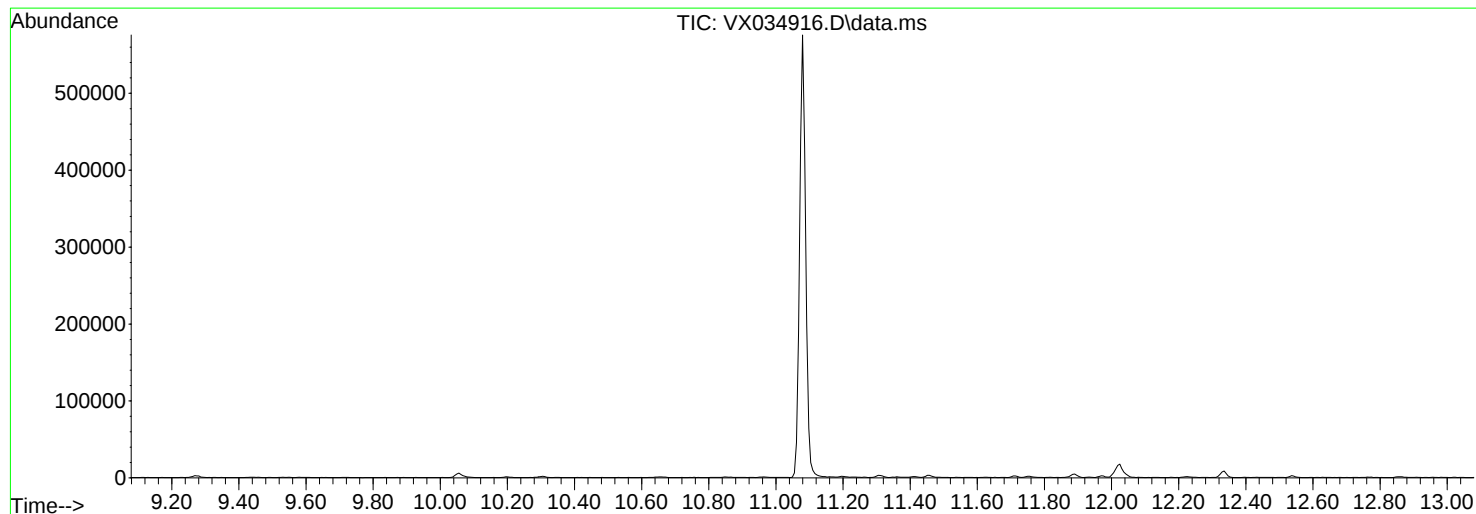

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	20277	PASS
75	95	30	60	53.5	53939	PASS
95	95	100	100	100.0	100733	PASS
96	95	5	9	6.7	6753	PASS
173	174	0.00	2	1.1	751	PASS
174	95	50	100	70.9	71467	PASS
175	174	5	9	7.1	5041	PASS
176	174	95	101	95.8	68485	PASS
177	176	5	9	6.4	4413	PASS