

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040325\
 Data File : VX045580.D
 Acq On : 03 Apr 2025 18:43
 Operator : JC/MD
 Sample : Q1676-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Storage-Blank-SOIL-REF-6

Quant Time: Apr 04 01:28:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	65833	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	129421	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	121603	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	51026	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	65866	54.710	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.420%
35) Dibromofluoromethane	5.385	113	47118	51.313	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.620%
50) Toluene-d8	8.647	98	162253	50.624	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.240%
62) 4-Bromofluorobenzene	11.079	95	60680	51.977	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	103.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040325\
Data File : VX045580.D
Acq On : 03 Apr 2025 18:43
Operator : JC/MD
Sample : Q1676-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SOIL-REF-6

Quant Time: Apr 04 01:28:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




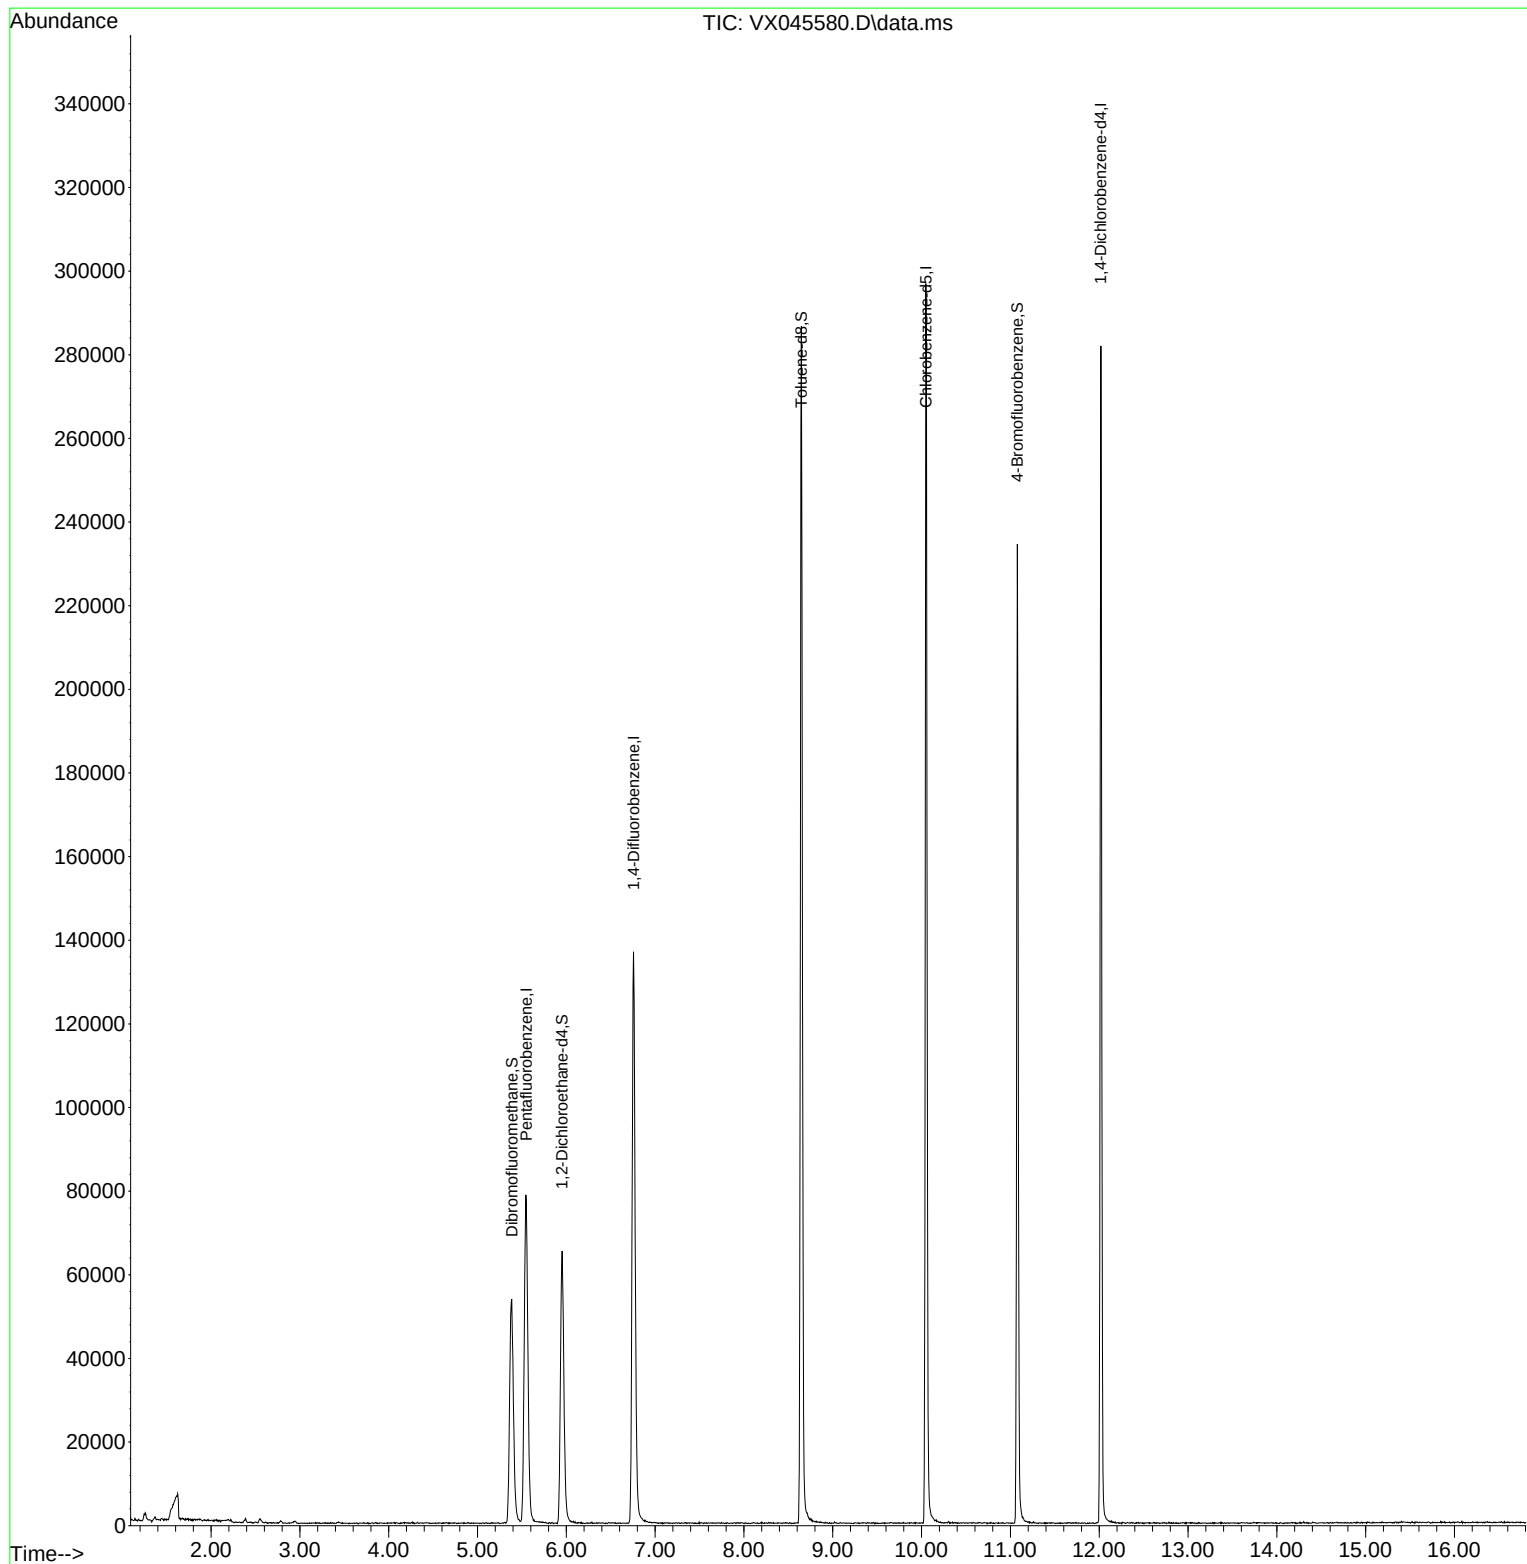


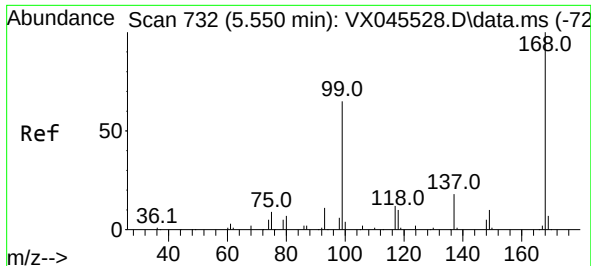

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SOIL-REF-6


Tgt Ion:168 Resp: 65833
Ion Ratio Lower Upper
168 100
99 67.7 52.3 78.5

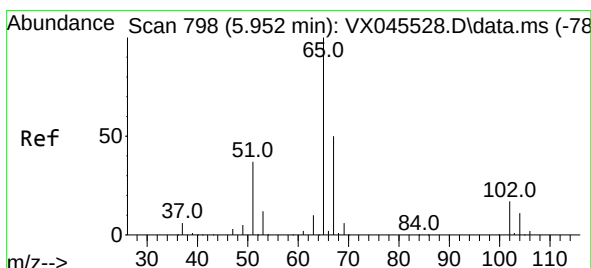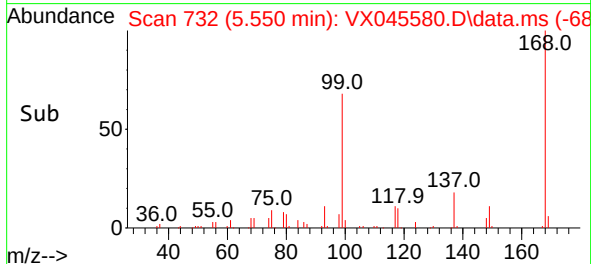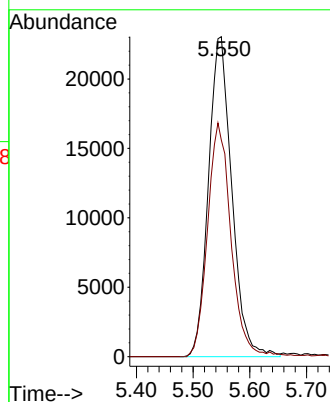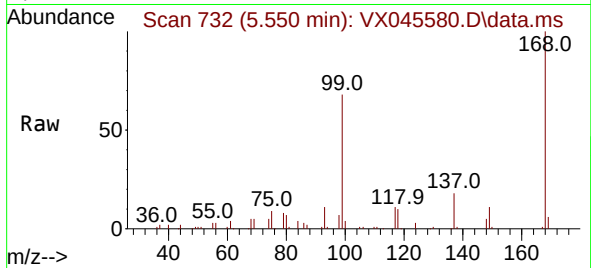

#33
1,2-Dichloroethane-d4
Concen: 54.710 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43

Tgt Ion: 65 Resp: 65866
Ion Ratio Lower Upper
65 100
67 49.4 0.0 99.0


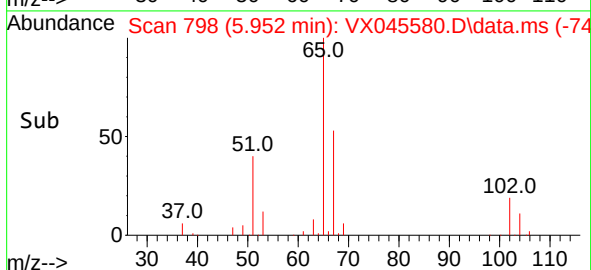
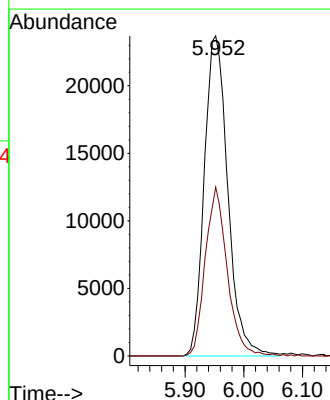
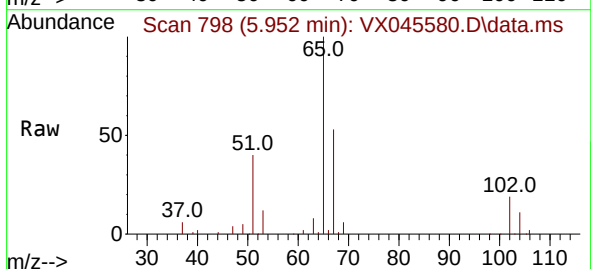


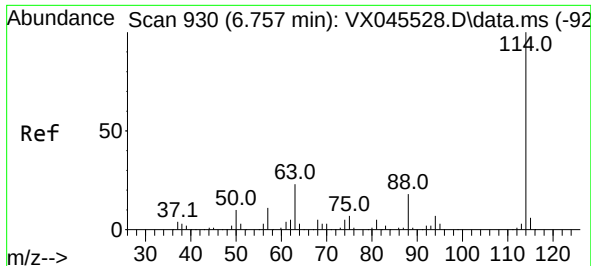

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SOIL-REF-6


Tgt Ion:114 Resp: 129421
Ion Ratio Lower Upper
114 100
63 23.9 0.0 46.8
88 17.9 0.0 35.4

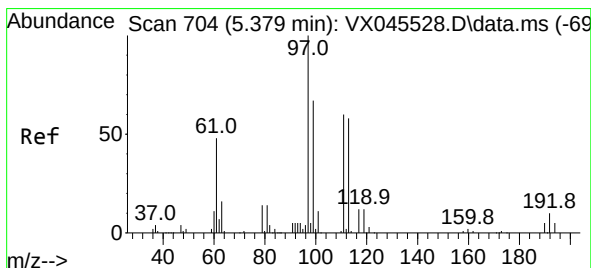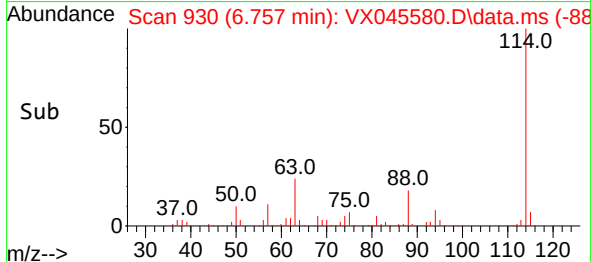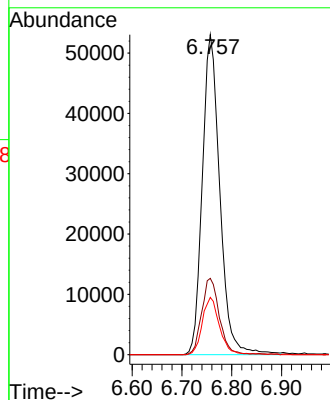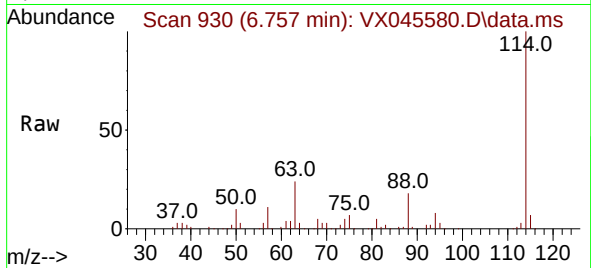

#35
Dibromofluoromethane
Concen: 51.313 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43

Tgt Ion:113 Resp: 47118
Ion Ratio Lower Upper
113 100
111 102.8 81.8 122.6
192 16.8 13.8 20.6


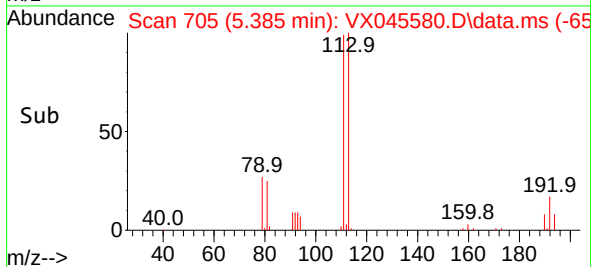
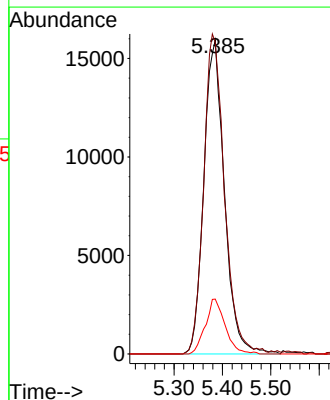
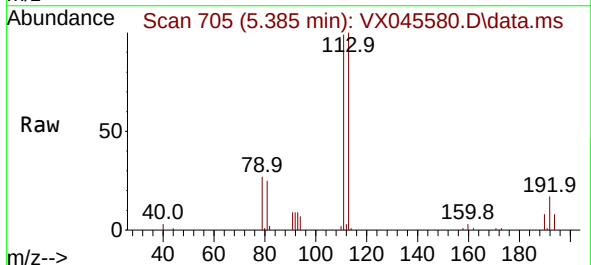


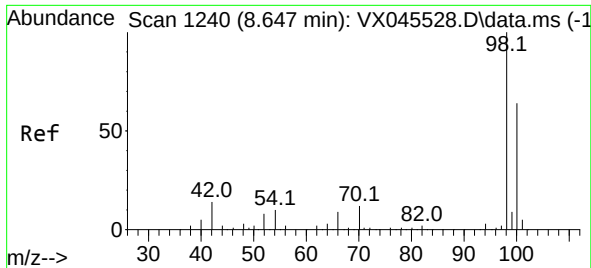

#50
Toluene-d8
Concen: 50.624 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43




Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SOIL-REF-6


Tgt Ion: 98 Resp: 162253
Ion Ratio Lower Upper
98 100
100 64.9 52.2 78.4

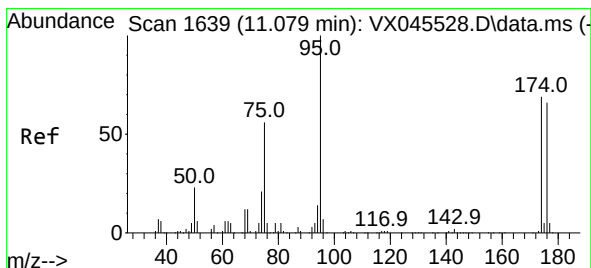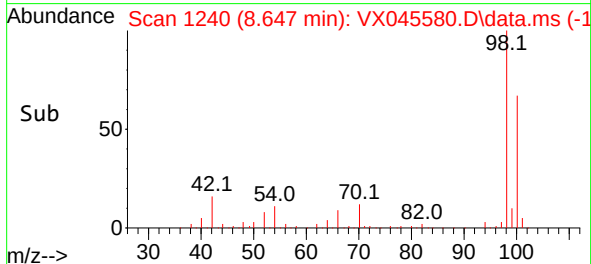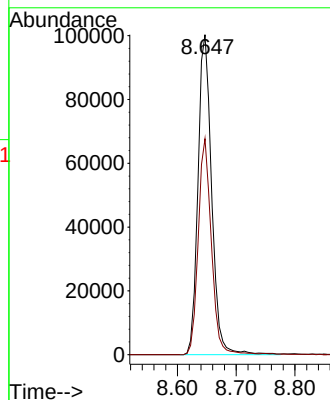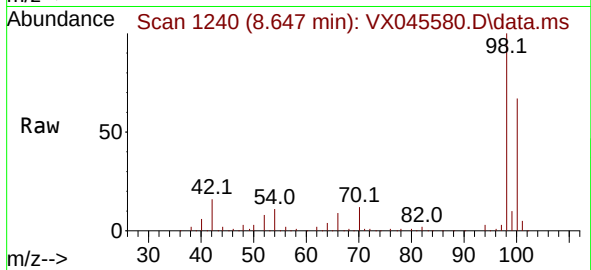

#62
4-Bromofluorobenzene
Concen: 51.977 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43

Tgt Ion: 95 Resp: 60680
Ion Ratio Lower Upper
95 100
174 67.6 0.0 135.8
176 64.9 0.0 131.4


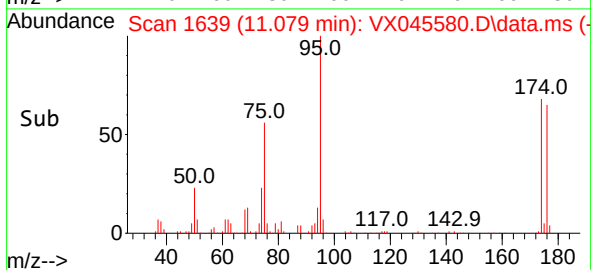
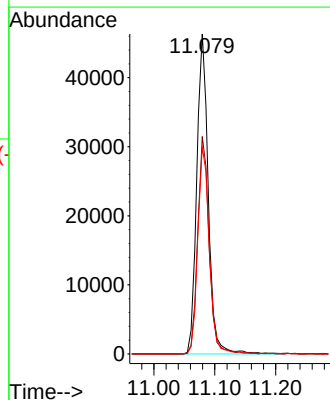
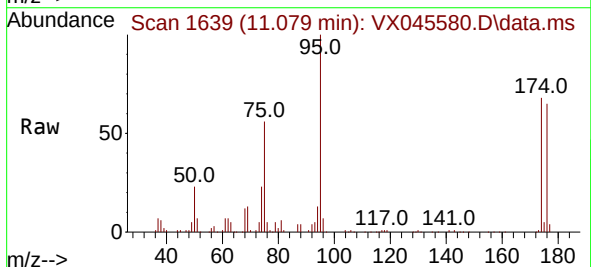


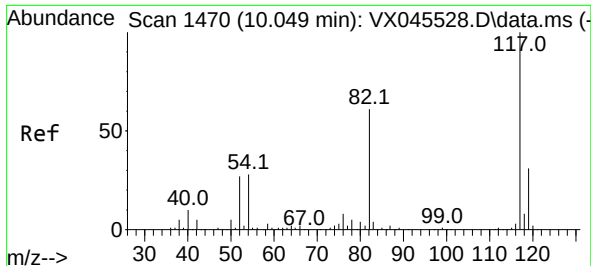

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43

Instrument :
MSVOA_X
ClientSampleId :
Storage-Blank-SOIL-REF-6

Tgt Ion:117 Resp: 121603
Ion Ratio Lower Upper
117 100
82 62.5 49.2 73.8
119 32.5 25.1 37.7

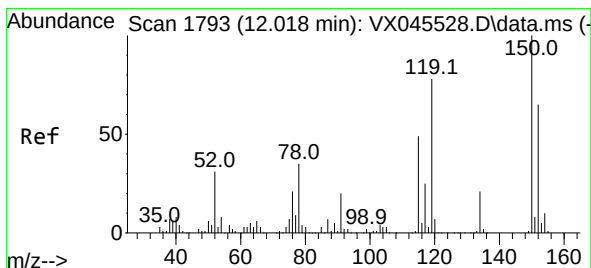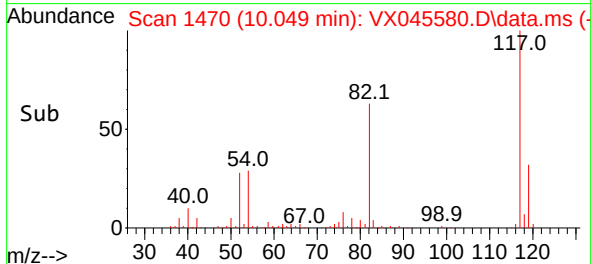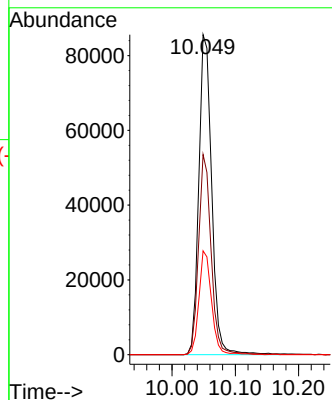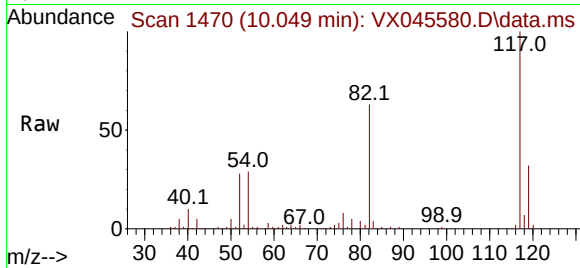

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045580.D
Acq: 03 Apr 2025 18:43

Tgt Ion:152 Resp: 51026
Ion Ratio Lower Upper
152 100
115 65.5 46.9 140.7
150 159.5 0.0 349.4

