

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\WX040419\
 Data File : VX008641.D
 Acq On : 04 Apr 2019 17:17
 Operator : JC/SP
 Sample : K2263-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Quant Time: Apr 05 07:08:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	224779	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	365875	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	308610	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	132496	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.09	65	150610	45.94	ug/l	0.02
Spiked Amount			Recovery	=	91.88%	
35) Dibromofluoromethane	5.51	113	98503	42.11	ug/l	0.00
Spiked Amount			Recovery	=	84.22%	
50) Toluene-d8	8.73	98	466127	50.04	ug/l	0.01
Spiked Amount			Recovery	=	100.08%	
62) 4-Bromofluorobenzene	11.13	95	149086	45.14	ug/l	0.00
Spiked Amount			Recovery	=	90.28%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.30	50	73654	22.292	ug/l #	69
5) Bromomethane	1.64	94	342	2.076	ug/l #	62
6) Chloroethane	1.95	64	3103	Below Cal	#	1
8) Diethyl Ether	2.18	74	1450	0.791	ug/l	93
10) Methyl Iodide	2.51	142	186	4.079	ug/l #	90
11) Tert butyl alcohol	3.04	59	17541	22.853	ug/l #	72
13) Acrolein	2.21	56	121095	318.177	ug/l #	1
14) Allyl chloride	2.81	41	763084	128.272	ug/l #	40
15) Acrylonitrile	3.17	53	39167	19.262	ug/l #	40
16) Acetone	2.44	43	26487	14.027	ug/l	95
17) Carbon Disulfide	2.59	76	47503	5.674	ug/l	97
18) Methyl Acetate	2.76	43	153986	33.623	ug/l #	56
19) Methyl tert-butyl Ether	3.20	73	3008	0.324	ug/l #	1
20) Methylene Chloride	2.78	84	59706	18.889	ug/l #	12
23) Vinyl Acetate	3.75	43	63715	6.388	ug/l #	78
24) 1,1-Dichloroethane	3.67	63	3290	0.580	ug/l #	85
25) 2-Butanone	4.68	43	32864	11.011	ug/l	98
26) 2,2-Dichloropropane	4.41	77	25186	6.299	ug/l #	53
28) Bromochloromethane	5.03	49	97	Below Cal	#	22
29) Tetrahydrofuran	5.17	42	890	0.449	ug/l #	66
30) Chloroform	5.28	83	54754	10.799	ug/l #	22
31) Cyclohexane	5.59	56	3520206	621.441	ug/l	99
36) 1,1-Dichloropropene	5.67	75	17787	4.447	ug/l #	51
37) Ethyl Acetate	4.90	43	2985	0.559	ug/l #	1
38) Carbon Tetrachloride	5.67	117	21818	6.591	ug/l #	16
39) Methylcyclohexane	7.46	83	1294122	261.939	ug/l	98
41) Methacrylonitrile	5.07	41	11677	3.805	ug/l #	41
42) 1,2-Dichloroethane	6.18	62	540034	126.430	ug/l #	75
43) Isopropyl Acetate	6.46	43	32582	3.896	ug/l #	63
45) 1,2-Dichloropropane	7.47	63	12294	3.615	ug/l #	1
46) Dibromomethane	7.63	93	961	0.487	ug/l #	1
47) Bromodichloromethane	7.84	83	3981	1.070	ug/l #	74
48) Methyl methacrylate	7.74	41	73000	17.257	ug/l #	56
49) 1,4-Dioxane	7.71	88	173	2.183	ug/l #	1

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX040419\
 Data File : VX008641.D
 Acq On : 04 Apr 2019 17:17
 Operator : JC/SP
 Sample : K2263-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Quant Time: Apr 05 07:08:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)


51) 4-Methyl-2-Pentanone	8.67	43	211800	39.344	ug/l	94
53) t-1,3-Dichloropropene	8.83	75	628286	150.821	ug/l #	1
55) 1,1,2-Trichloroethane	9.17	97	24100	8.547	ug/l #	17
56) Ethyl methacrylate	9.07	69	56425	11.060	ug/l #	29
58) 2-Chloroethyl Vinyl ether	8.26	63	3975	1.526	ug/l #	52
59) 2-Hexanone	9.51	43	863813	206.477	ug/l #	49
61) 1,2-Dibromoethane	9.67	107	41115	14.007	ug/l	99
65) Chlorobenzene	10.34	112	9900	1.447	ug/l #	58
67) Ethyl Benzene	10.26	91	14422283	1130.618	ug/l #	66
68) m/p-Xylenes	10.38	106	14713025	3207.903	ug/l #	52
69) o-Xylene	10.71	106	6084956	1368.996	ug/l	82
70) Styrene	10.71	104	363803	47.483	ug/l #	1
73) Isopropylbenzene	11.02	105	433220	39.454	ug/l	100
74) N-amyl acetate	10.90	43	56413	8.732	ug/l #	55
75) 1,1,2,2-Tetrachloroethane	11.23	83	41358	9.904	ug/l #	45
76) 1,2,3-Trichloropropane	11.33	75	5999	1.648	ug/l #	32
78) n-propylbenzene	11.36	91	1149884	89.939	ug/l	100
79) 2-Chlorotoluene	11.44	91	579770	74.935	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.51	105	1500989	162.849	ug/l	99
81) trans-1,4-Dichloro-2-buten	11.02	75	5298	4.012	ug/l #	1
82) 4-Chlorotoluene	11.51	91	161903	18.078	ug/l #	47
83) tert-Butylbenzene	11.81	119	543628	61.306	ug/l #	64
84) 1,2,4-Trimethylbenzene	11.81	105	4315371	462.384	ug/l	96
85) sec-Butylbenzene	11.81	105	4315371	409.700	ug/l #	58
86) p-Isopropyltoluene	12.02	119	66354	7.019	ug/l	97
89) n-Butylbenzene	12.38	91	117627	13.267	ug/l #	15
90) Hexachloroethane	12.67	117	32776	20.903	ug/l #	9
91) 1,2-Dichlorobenzene	12.39	146	993	0.212	ug/l #	1
92) 1,2-Dibromo-3-Chloropropan	13.02	75	2054	2.236	ug/l #	3
95) Naphthalene	13.83	128	603445	55.345	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\WX040419\
Data File : VX008641.D
Acq On : 04 Apr 2019 17:17
Operator : JC/SP
Sample : K2263-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Quant Time: Apr 05 07:08:11 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

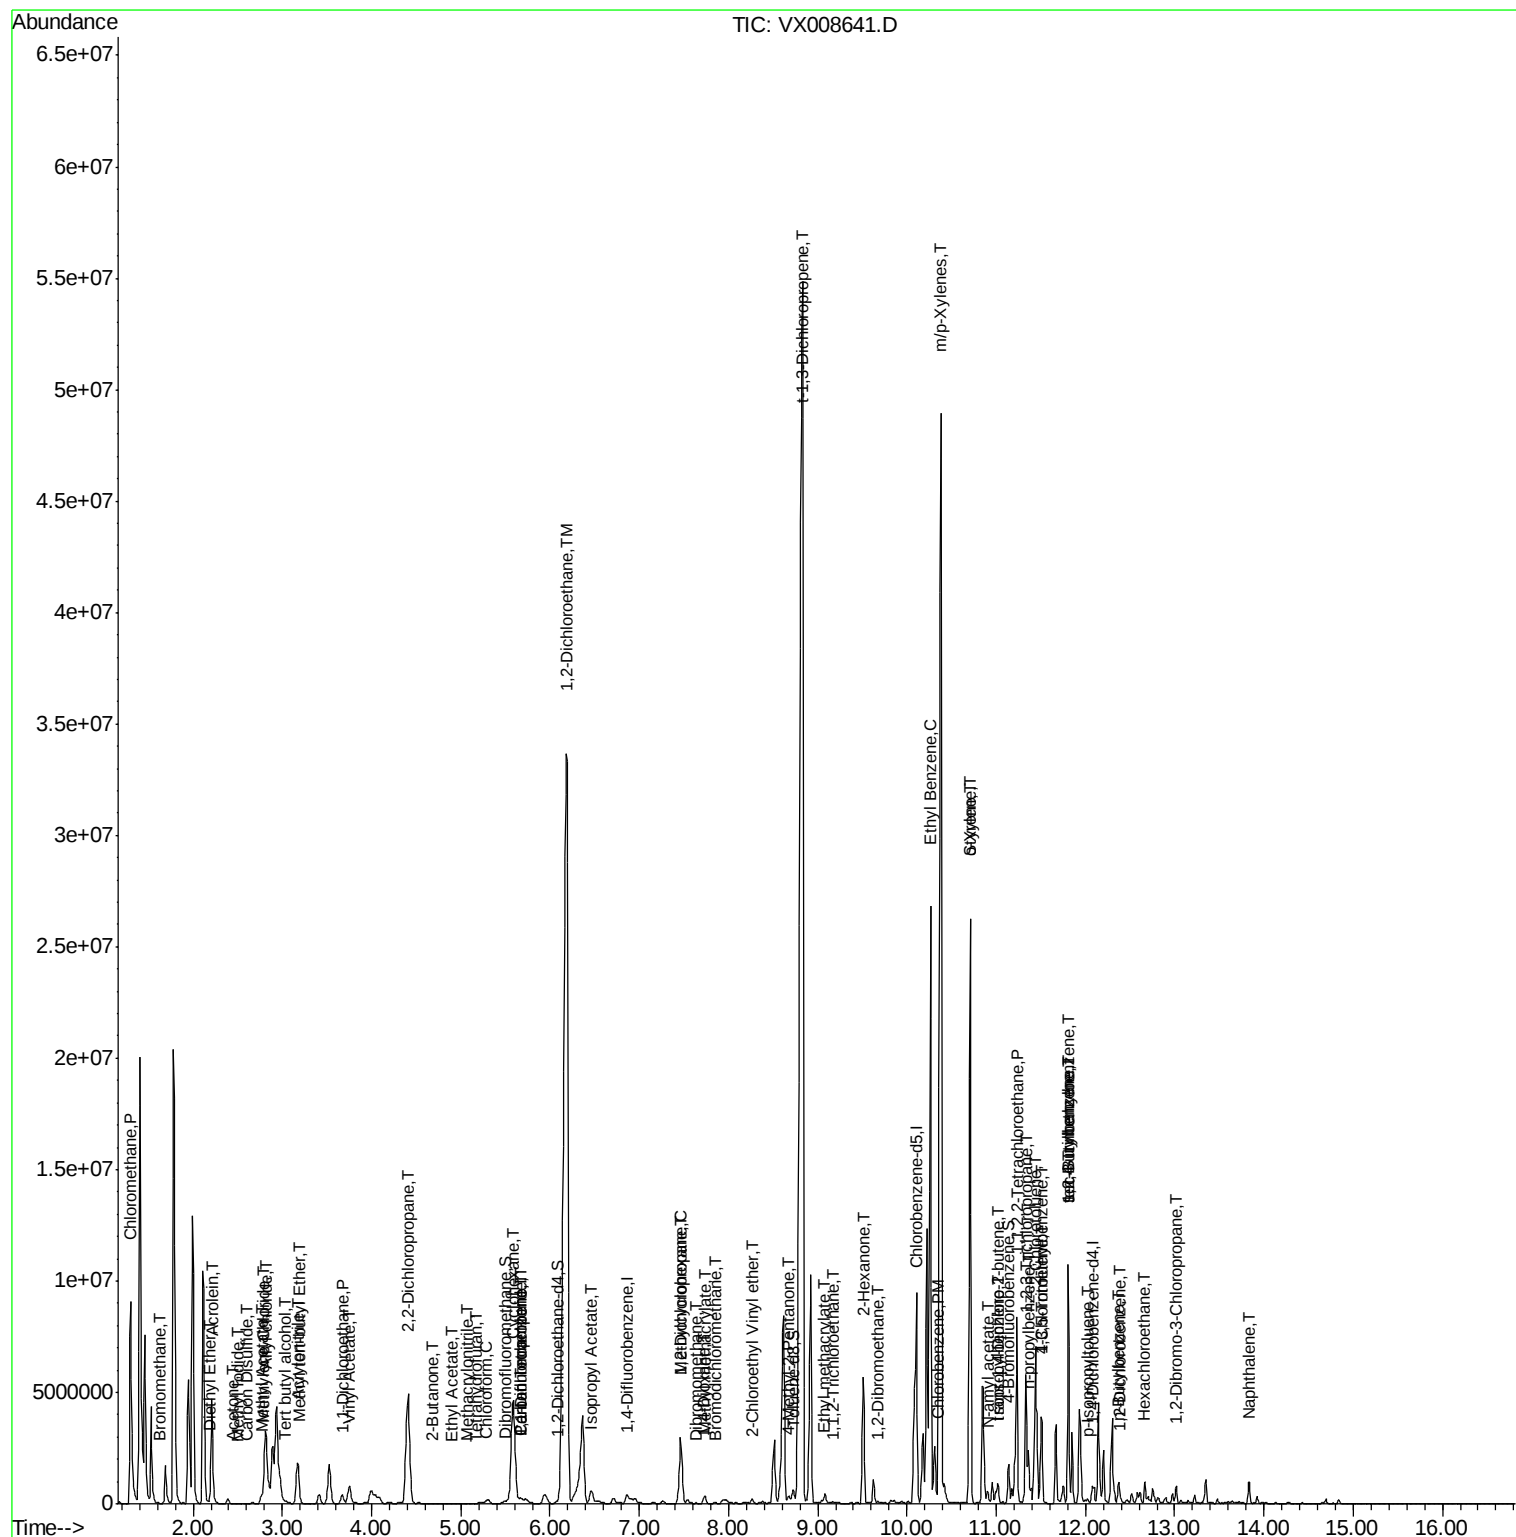



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :


MW-3

Tgt Ion:168 Resp: 224779

Ion Ratio Lower Upper




168 100

99 56.4 46.7 70.1



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

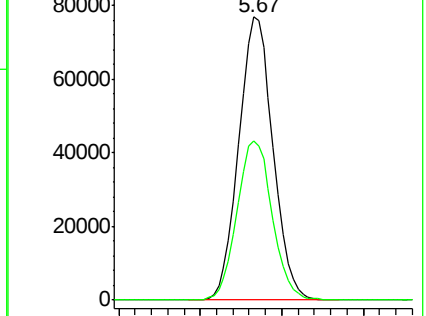

#3

Chloromethane

Concen: 22.292 ug/l

RT: 1.30 min Scan# 24

Delta R.T. -0.02 min

Lab File: VX008641.D


Acq: 04 Apr 2019 17:17

Tgt Ion: 50 Resp: 73654

Ion Ratio Lower Upper



50 100


52 15.0 25.8 38.8#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

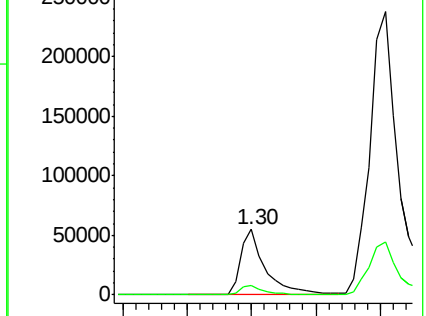

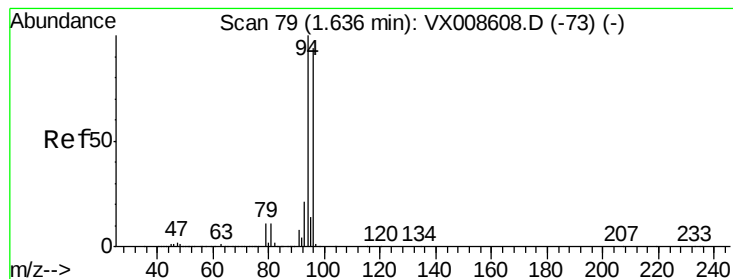

#5

Bromomethane

Concen: 2.076 ug/l

RT: 1.64 min Scan# 79

Delta R.T. 0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion: 94 Resp: 342

Ion Ratio Lower Upper

94 100

96 57.4 75.2 112.8#

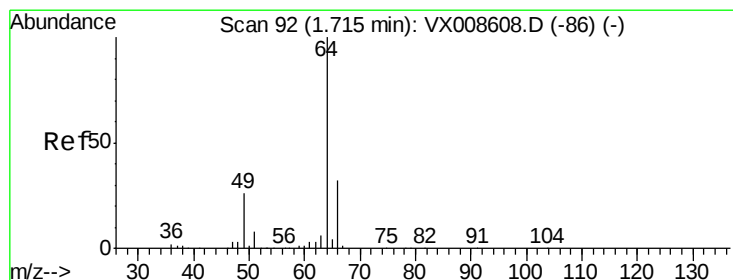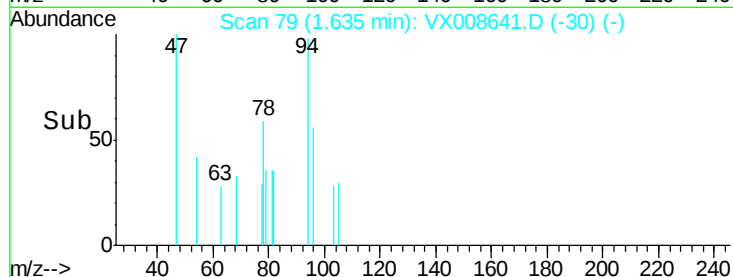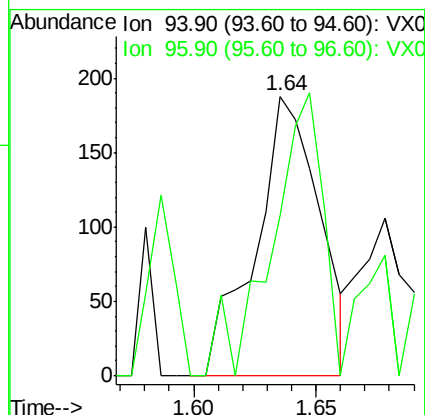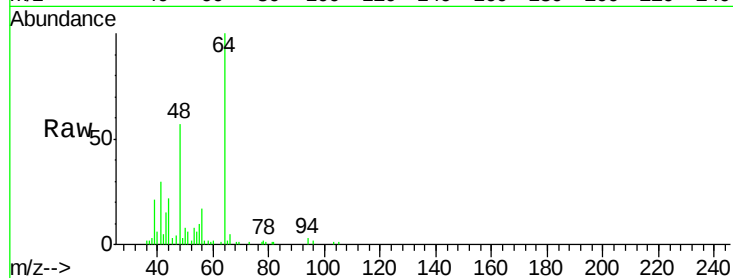

#6

Chloroethane

Concen: Below Cal

RT: 1.95 min Scan# 130

Delta R.T. 0.23 min

Lab File: VX008641.D




Acq: 04 Apr 2019 17:17


Tgt Ion: 64 Resp: 3103

Ion Ratio Lower Upper

64 100

66 189.1 25.4 38.0#

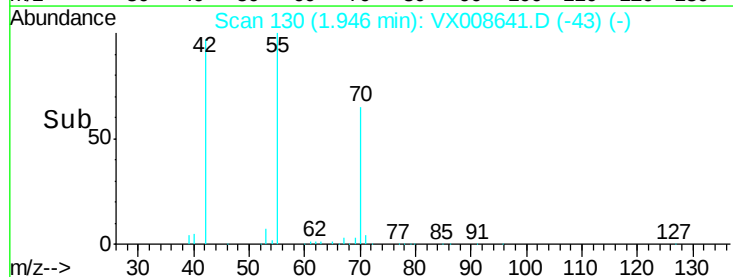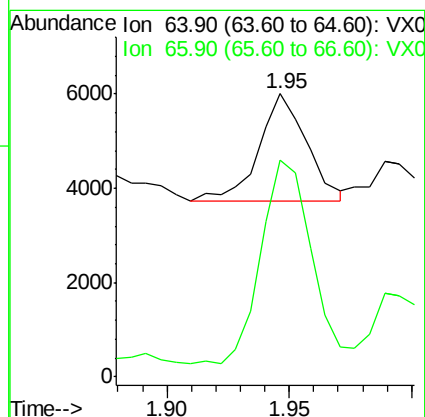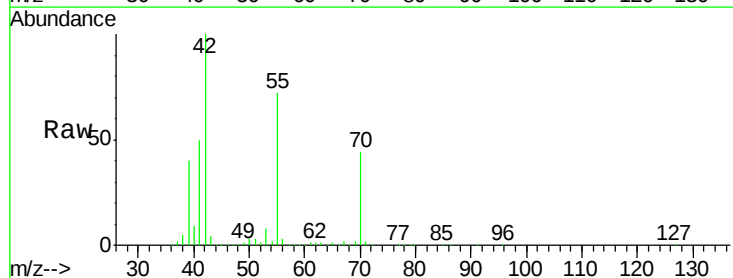



#8

Diethyl Ether

Concen: 0.791 ug/l

RT: 2.18 min Scan# 169

Delta R.T. -0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion: 74 Resp: 1450

Ion Ratio Lower Upper

74 100

45 105.6 56.5 169.5

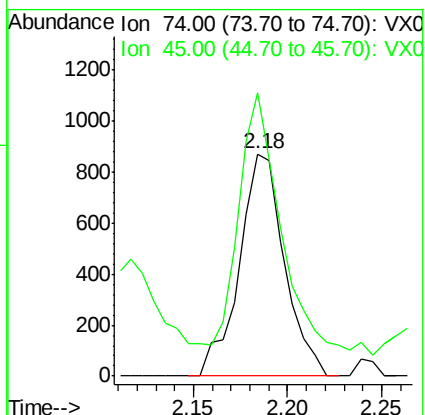

#10

Methyl Iodide

Concen: 4.079 ug/l

RT: 2.51 min Scan# 223

Delta R.T. 0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17




Tgt Ion: 142 Resp: 186


Ion Ratio Lower Upper

142 100

127 41.9 33.0 49.6

141 0.0 11.4 17.2#

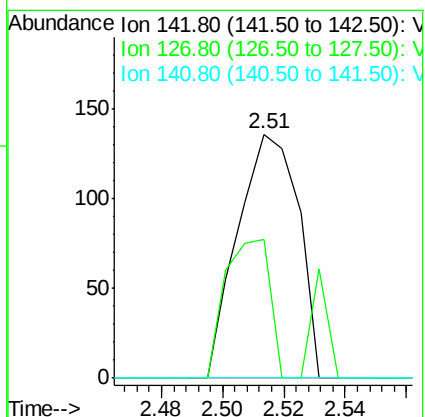




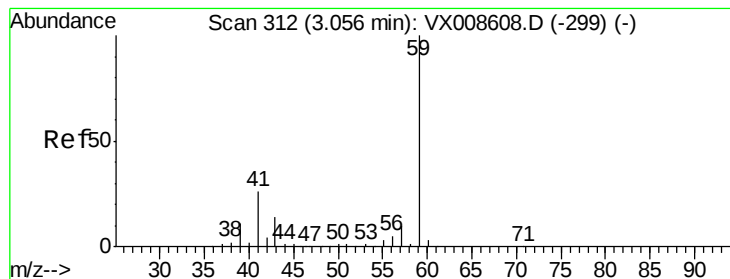


#11

Tert butyl alcohol
 Concen: 22.853 ug/l
 RT: 3.04 min Scan# 310
 Delta R.T. -0.01 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Instrument :
 MSVOA_X
 ClientSampled :
 MW-3




Tgt Ion: 59 Resp: 17541
 Ion Ratio Lower Upper
 59 100
 57 0.0 8.3 12.5#

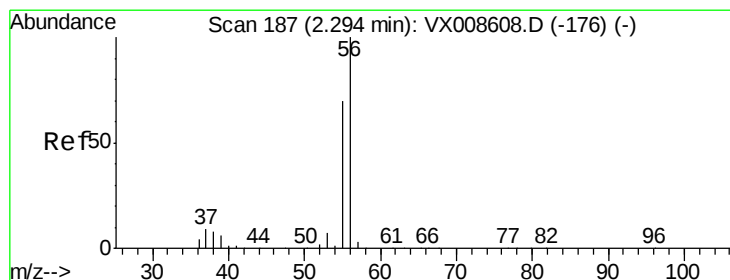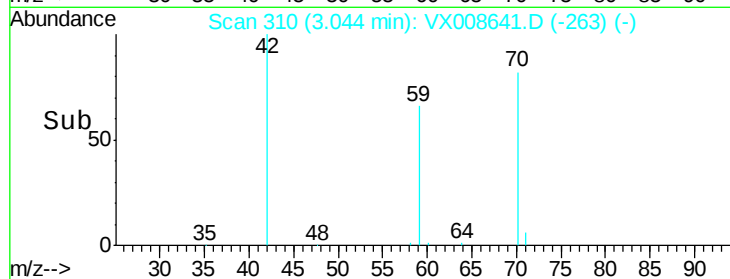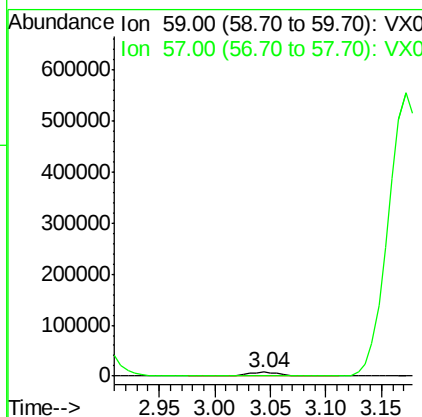


#13

Acrolein
 Concen: 318.177 ug/l
 RT: 2.21 min Scan# 173
 Delta R.T. -0.09 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Tgt Ion: 56 Resp: 121095
 Ion Ratio Lower Upper
 56 100
 55 2196.2 58.0 87.0#

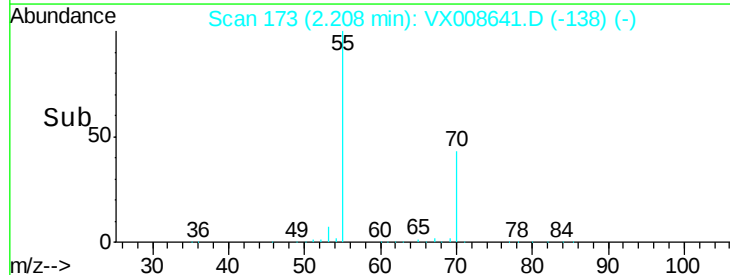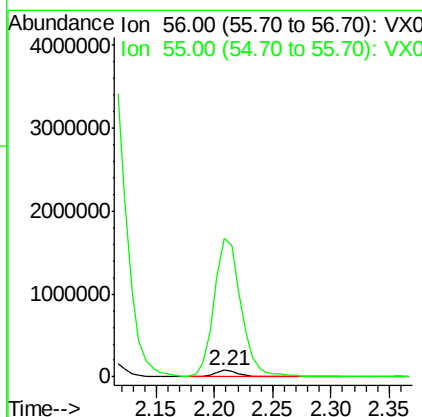



#14

Allyl chloride

Concen: 128.272 ug/l

RT: 2.81 min Scan# 272

Delta R.T. 0.09 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3





Tgt Ion: 41 Resp: 763084

Ion Ratio Lower Upper

41 100

39 107.9 48.0 72.0#

76 0.0 22.0 33.0#

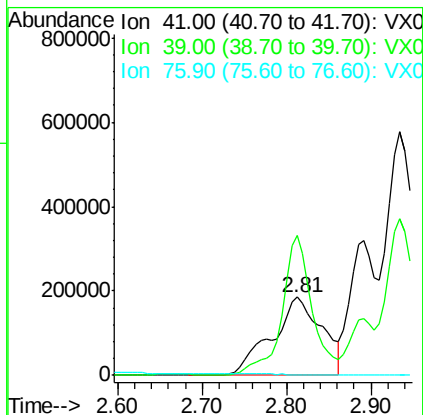

#15

Acrylonitrile

Concen: 19.262 ug/l

RT: 3.17 min Scan# 331

Delta R.T. 0.02 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17




Tgt Ion: 53 Resp: 39167


Ion Ratio Lower Upper

53 100

52 20.4 66.5 99.7#

51 58.3 28.6 42.8#

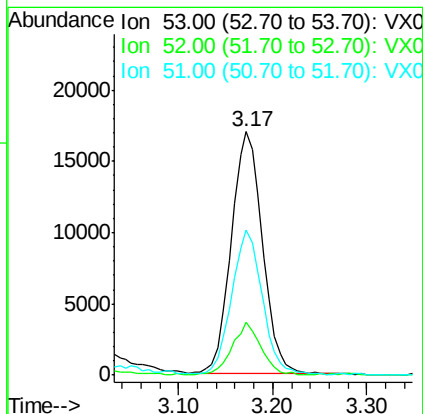



#16

Acetone

Concen: 14.027 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion: 43 Resp: 26487

Ion Ratio Lower Upper

43 100

58 28.4 24.8 37.2

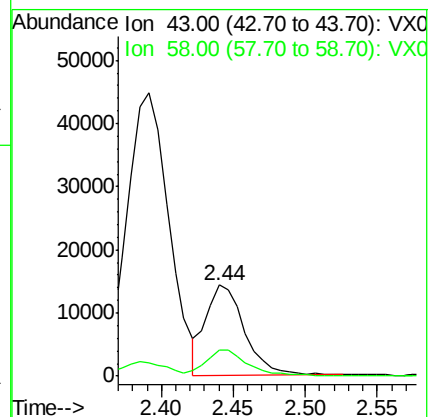

#17

Carbon Disulfide

Concen: 5.674 ug/l

RT: 2.59 min Scan# 236

Delta R.T. 0.02 min

Lab File: VX008641.D




Acq: 04 Apr 2019 17:17


Tgt Ion: 76 Resp: 47503

Ion Ratio Lower Upper

76 100

78 10.0 7.1 10.7



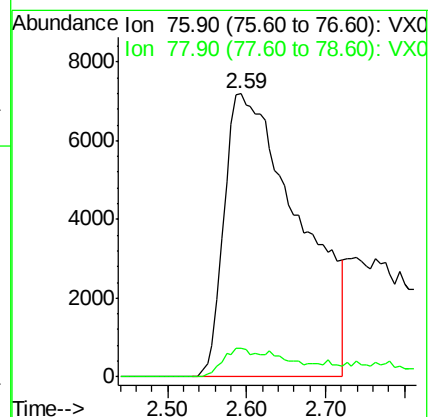





#18
Methyl Acetate
Concen: 33.623 ug/l
RT: 2.76 min Scan# 264
Delta R.T. -0.01 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17




Instrument :
MSVOA_X
ClientSampleId :
MW-3


Tgt Ion: 43 Resp: 153986
Ion Ratio Lower Upper
43 100
74 0.3 16.5 24.7#

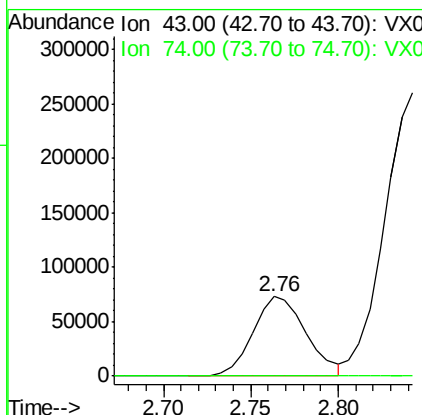

#19
Methyl tert-butyl Ether
Concen: 0.324 ug/l
RT: 3.20 min Scan# 335
Delta R.T. -0.00 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion: 73 Resp: 3008
Ion Ratio Lower Upper
73 100
57 13096.4 19.5 29.3#

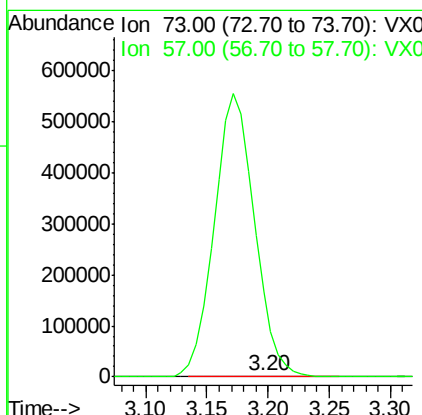



#20

Methylene Chloride

Concen: 18.889 ug/l

RT: 2.78 min Scan# 267

Delta R.T. -0.08 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3

Tgt Ion: 84 Resp: 59706





Ion Ratio Lower Upper

84 100

49 3.1 109.7 164.5#

51 28.2 33.6 50.4#

86 0.4 51.4 77.2#

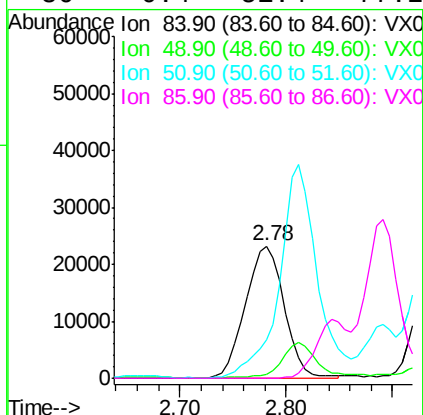

#23

Vinyl Acetate

Concen: 6.388 ug/l

RT: 3.75 min Scan# 426

Delta R.T. -0.07 min

Lab File: VX008641.D




Acq: 04 Apr 2019 17:17


Tgt Ion: 43 Resp: 63715

Ion Ratio Lower Upper

43 100

86 0.8 7.0 10.6#









#24
 1,1-Dichloroethane
 Concen: 0.580 ug/l
 RT: 3.67 min Scan# 413
 Delta R.T. -0.02 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17




Instrument :
 MSVOA_X
 ClientSampled :
 MW-3


Tgt Ion: 63 Resp: 3290
 Ion Ratio Lower Upper
 63 100
 98 0.0 2.8 8.4#
 100 0.0 1.8 5.5#

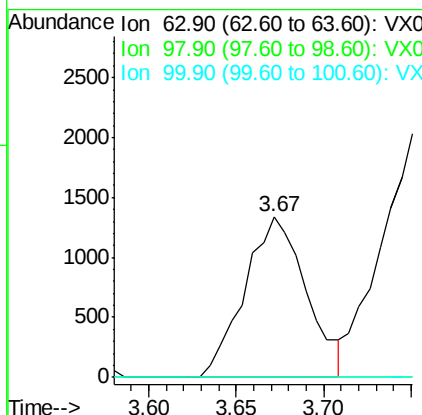

#25
 2-Butanone
 Concen: 11.011 ug/l
 RT: 4.68 min Scan# 578
 Delta R.T. -0.00 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Tgt Ion: 43 Resp: 32864
 Ion Ratio Lower Upper
 43 100
 72 23.9 18.2 27.4



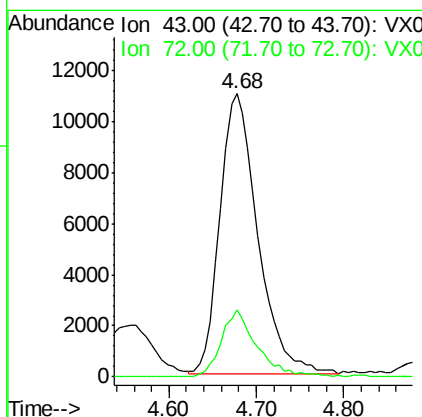





#26
 2,2-Dichloropropane
 Concen: 6.299 ug/l
 RT: 4.41 min Scan# 534
 Delta R.T. -0.18 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3


Tgt Ion: 77 Resp: 25186
 Ion Ratio Lower Upper
 77 100
 97 0.0 11.5 34.5#

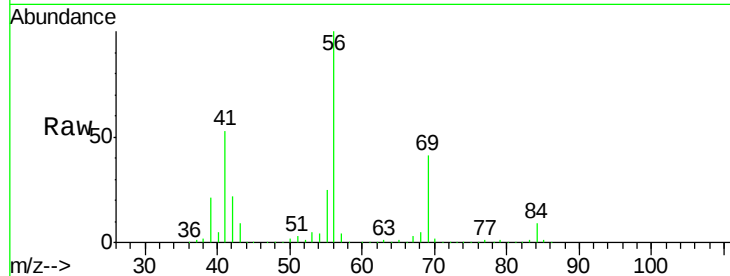

#28
 Bromochloromethane
 Concen: Below Cal
 RT: 5.03 min Scan# 636
 Delta R.T. 0.01 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Tgt Ion: 49 Resp: 97
 Ion Ratio Lower Upper
 49 100
 129 0.0 0.0 3.6
 130 0.0 49.3 73.9#









#29
Tetrahydrofuran
Concen: 0.449 ug/l
RT: 5.17 min Scan# 658
Delta R.T. 0.04 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17




Instrument :
MSVOA_X
ClientSampleId :
MW-3


Tgt Ion: 42 Resp: 890
Ion Ratio Lower Upper
42 100
72 43.6 30.5 45.7
71 0.0 28.6 43.0#



#30
Chloroform
Concen: 10.799 ug/l
RT: 5.28 min Scan# 677
Delta R.T. 0.07 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion: 83 Resp: 54754
Ion Ratio Lower Upper
83 100
85 3.3 52.1 78.1#

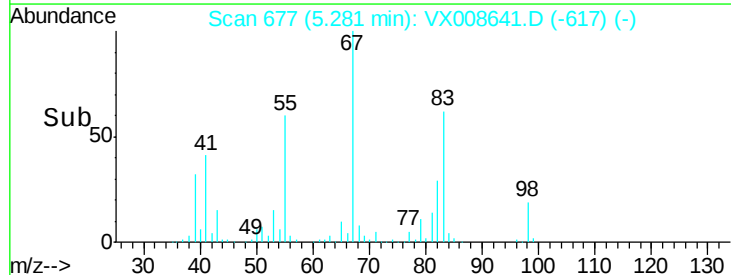

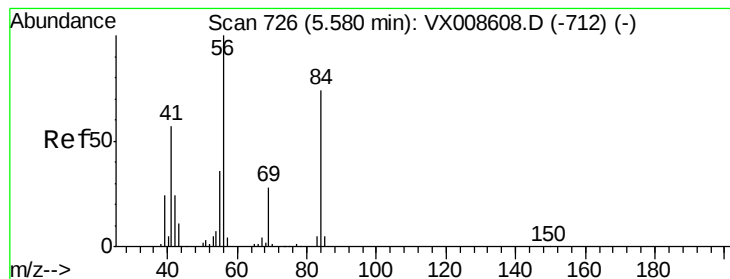

#31

Cyclohexane

Concen: 621.441 ug/l

RT: 5.59 min Scan# 727

Delta R.T. 0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :

MW-3


Tgt Ion: 56 Resp: 3520206

Ion Ratio Lower Upper




56 100

69 28.2 22.6 33.8

84 74.9 59.3 88.9



Abundance Ion 56.00 (55.70 to 56.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 84.00 (83.70 to 84.70): VX0

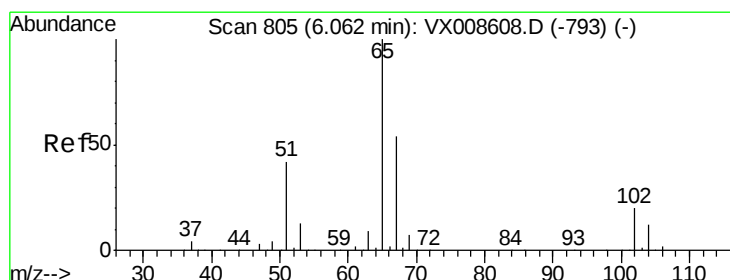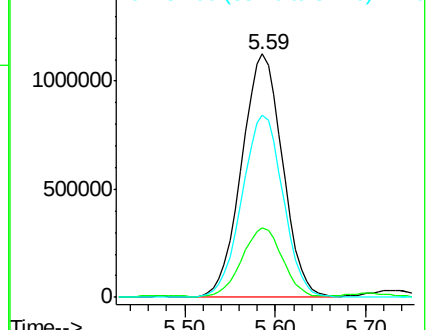

#33

1,2-Dichloroethane-d4

Concen: 45.938 ug/l

RT: 6.09 min Scan# 809

Delta R.T. 0.02 min

Lab File: VX008641.D


Acq: 04 Apr 2019 17:17

Tgt Ion: 65 Resp: 150610



Ion Ratio Lower Upper


65 100

67 53.3 0.0 107.2



Abundance Ion 64.90 (64.60 to 65.60): VX0
Ion 66.90 (66.60 to 67.60): VX0

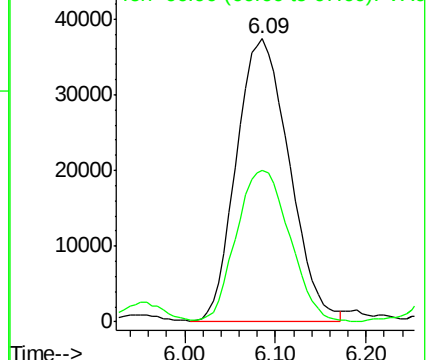







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3

Tgt Ion:114 Resp: 365875
 Ion Ratio Lower Upper
 114 100
 63 23.9 0.0 47.2
 88 17.0 0.0 34.0




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0


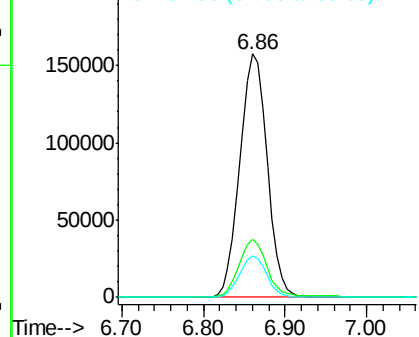



#35
 Dibromofluoromethane
 Concen: 42.108 ug/l
 RT: 5.51 min Scan# 714
 Delta R.T. 0.01 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Tgt Ion:113 Resp: 98503
 Ion Ratio Lower Upper
 113 100
 111 102.0 83.4 125.2
 192 20.7 16.1 24.1



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

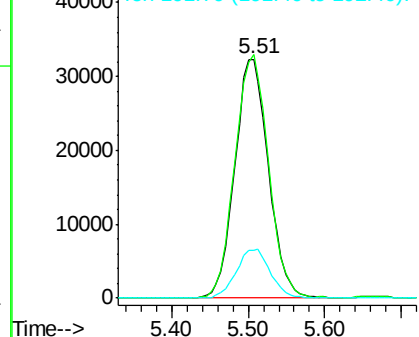

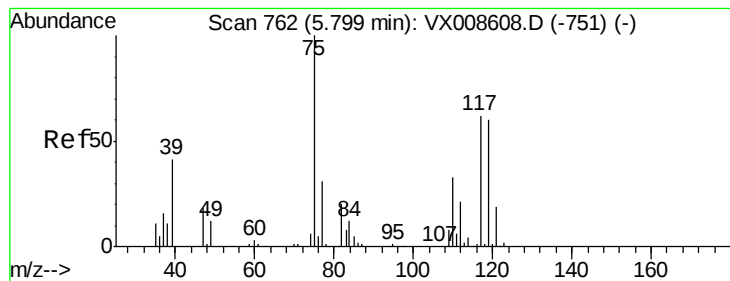

#36

1,1-Dichloropropene

Concen: 4.447 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3


Tgt Ion: 75 Resp: 17787

Ion Ratio Lower Upper

75 100

110 9.4 16.4 49.2#




77 0.0 24.7 37.1#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): VX0

Ion 76.90 (76.60 to 77.60): VX0

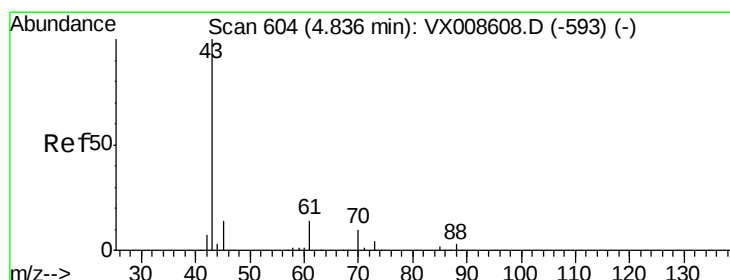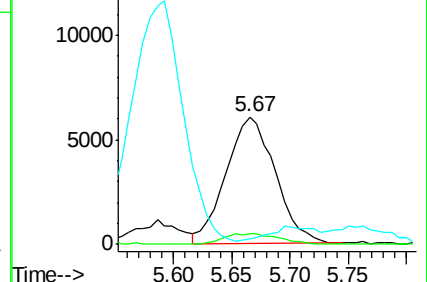

#37

Ethyl Acetate

Concen: 0.559 ug/l

RT: 4.90 min Scan# 614

Delta R.T. 0.06 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17


Tgt Ion: 43 Resp: 2985

Ion Ratio Lower Upper

43 100

61 2.6 10.3 15.5#



70 104.5 7.6 11.4#




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

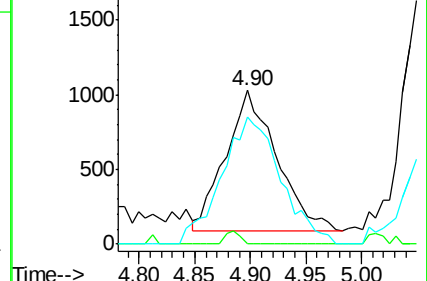

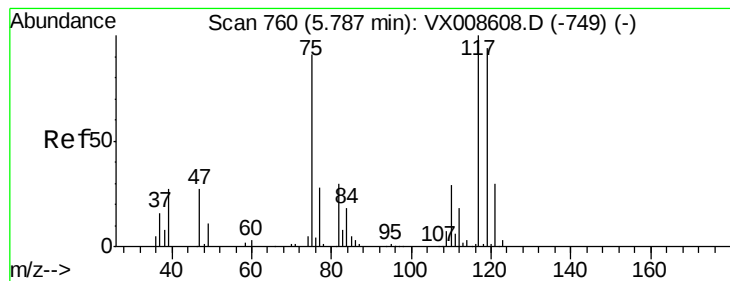

#38

Carbon Tetrachloride

Concen: 6.591 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3


Tgt Ion:117 Resp: 21818

Ion Ratio Lower Upper

117 100

119 4.0 75.0 112.6#




121 0.0 24.3 36.5#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

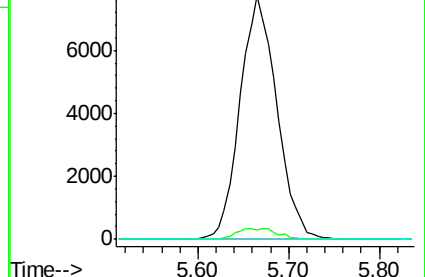

#39

Methylcyclohexane

Concen: 261.939 ug/l

RT: 7.46 min Scan# 1035

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17


Tgt Ion: 83 Resp: 1294122

Ion Ratio Lower Upper

83 100

55 87.9 69.0 103.6



98 43.9 34.4 51.6




Abundance Ion 83.00 (82.70 to 83.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 98.00 (97.70 to 98.70): VX0

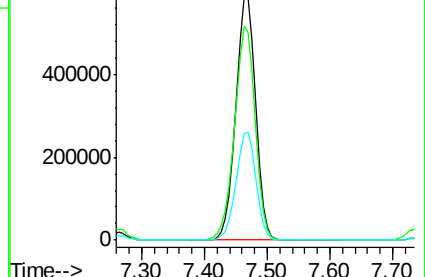



#41

Methacrylonitrile

Concen: 3.805 ug/l

RT: 5.07 min Scan# 642

Delta R.T. 0.02 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3

Tgt Ion: 41 Resp: 11677


Ion Ratio Lower Upper

41 100

39 27.8 42.1 63.1#

67 0.0 51.0 76.6#

52 0.0 21.4 32.0#



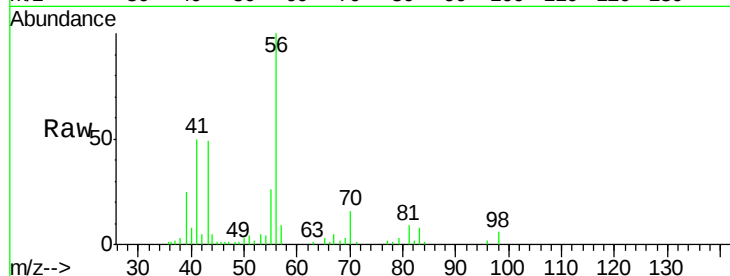


Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

Ion 67.00 (66.70 to 67.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

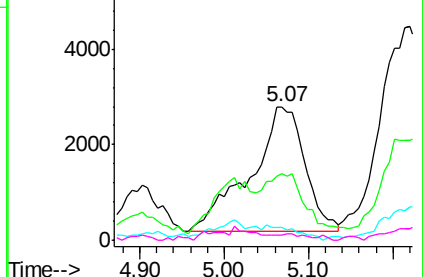

#42

1,2-Dichloroethane

Concen: 126.430 ug/l

RT: 6.18 min Scan# 825

Delta R.T. -0.01 min

Lab File: VX008641.D


Acq: 04 Apr 2019 17:17

Tgt Ion: 62 Resp: 540034

Ion Ratio Lower Upper



62 100


98 0.0 0.0 18.0



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

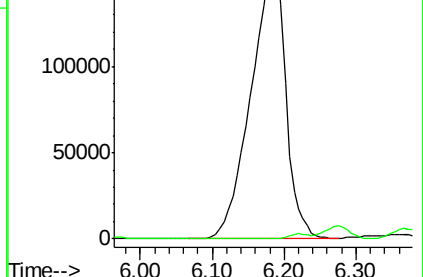



#43

Isopropyl Acetate

Concen: 3.896 ug/l

RT: 6.46 min Scan# 871

Delta R.T. 0.02 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3


Tgt Ion: 43 Resp: 32582

Ion Ratio Lower Upper

43 100

61 0.0 15.3 22.9#




87 0.1 9.0 13.6#

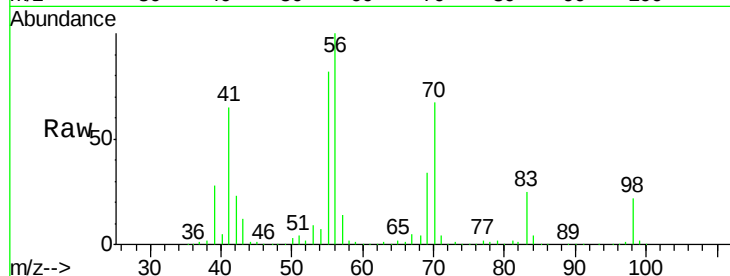

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

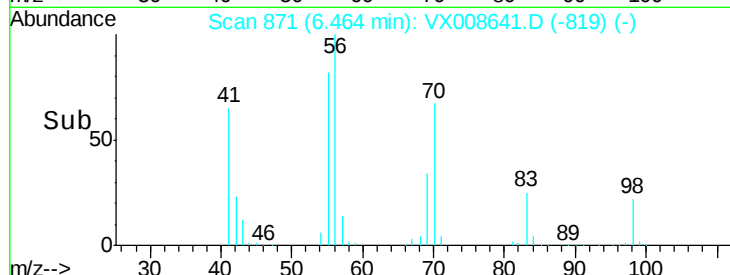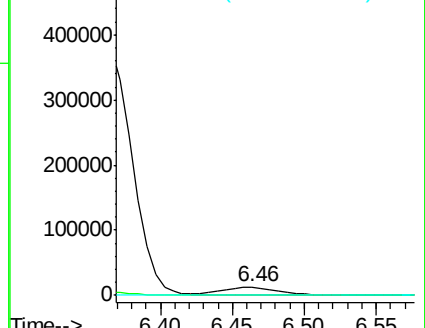

#45

1,2-Dichloropropane

Concen: 3.615 ug/l

RT: 7.47 min Scan# 1036

Delta R.T. -0.04 min

Lab File: VX008641.D


Acq: 04 Apr 2019 17:17

Tgt Ion: 63 Resp: 12294

Ion Ratio Lower Upper



63 100


65 228.9 24.2 36.4#



Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 64.90 (64.60 to 65.60): VX0




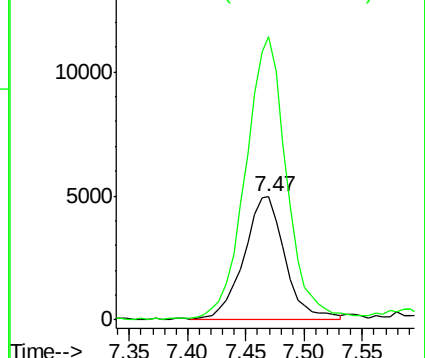


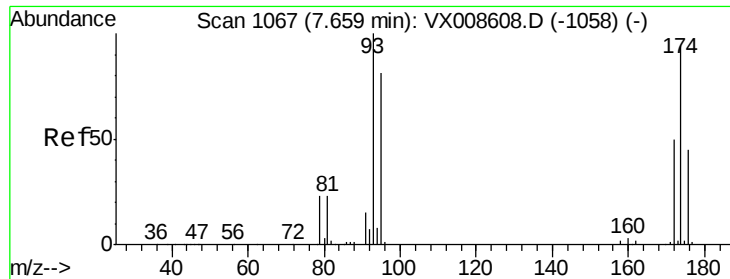

#46
 Dibromomethane
 Concen: 0.487 ug/l
 RT: 7.63 min Scan# 1063
 Delta R.T. -0.02 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17




Instrument :
 MSVOA_X
 ClientSampled :
 MW-3


Tgt Ion: 93 Resp: 961
 Ion Ratio Lower Upper
 93 100
 95 1113.8 66.6 99.8#
 174 0.0 77.7 116.5#

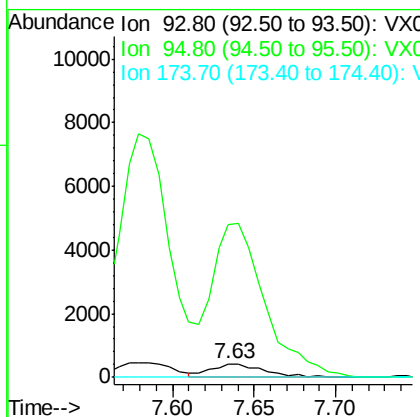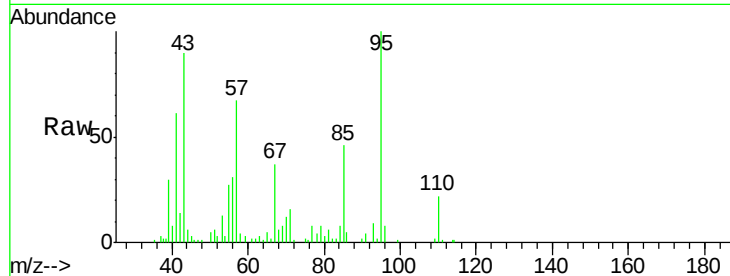

#47
 Bromodichloromethane
 Concen: 1.070 ug/l
 RT: 7.84 min Scan# 1097
 Delta R.T. -0.06 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Tgt Ion: 83 Resp: 3981
 Ion Ratio Lower Upper
 83 100
 85 43.2 51.2 76.8#
 127 0.0 6.6 10.0#

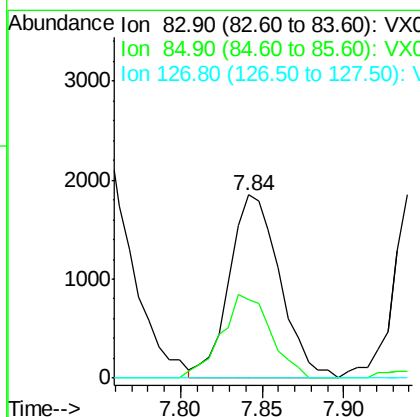



#48

Methyl methacrylate

Concen: 17.257 ug/l

RT: 7.74 min Scan# 1080

Delta R.T. -0.03 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :

MW-3





Tgt Ion: 41 Resp: 73000

Ion Ratio Lower Upper

41 100

69 132.0 59.0 88.4#

39 46.1 41.0 61.4

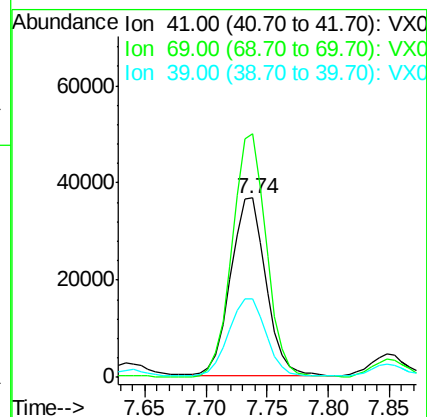

#49

1,4-Dioxane

Concen: 2.183 ug/l

RT: 7.71 min Scan# 1076

Delta R.T. -0.02 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17




Tgt Ion: 88 Resp: 173


Ion Ratio Lower Upper

88 100

43 5538.2 28.6 43.0#

58 2932.9 62.2 93.2#

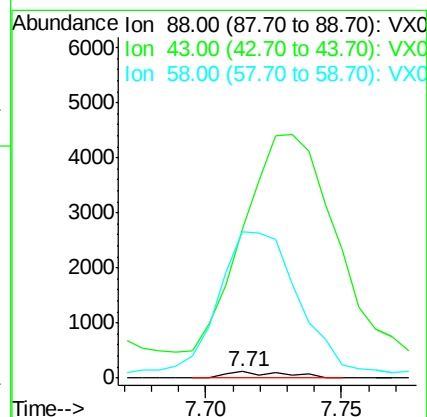



#50

Toluene-d8

Concen: 50.044 ug/l

RT: 8.73 min Scan# 1242

Delta R.T. 0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion: 98 Resp: 466127

Ion Ratio Lower Upper

98 100

100 69.9 51.4 77.0

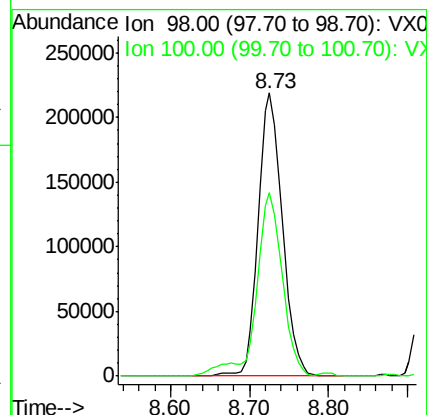

#51

4-Methyl-2-Pentanone

Concen: 39.344 ug/l

RT: 8.67 min Scan# 1233

Delta R.T. 0.03 min

Lab File: VX008641.D




Acq: 04 Apr 2019 17:17


Tgt Ion: 43 Resp: 211800

Ion Ratio Lower Upper

43 100

58 40.3 29.5 44.3

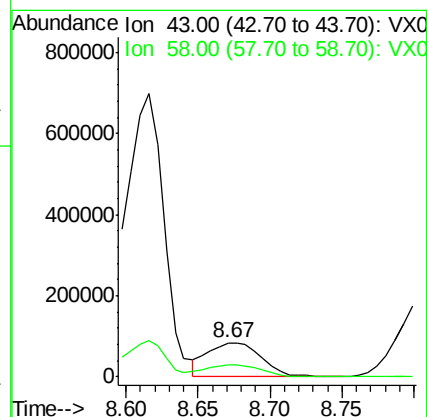



#53

t-1,3-Dichloropropene

Concen: 150.821 ug/l

RT: 8.83 min Scan# 1259

Delta R.T. -0.21 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion: 75 Resp: 628286

Ion Ratio Lower Upper

75 100

77 169.3 25.2 37.8#

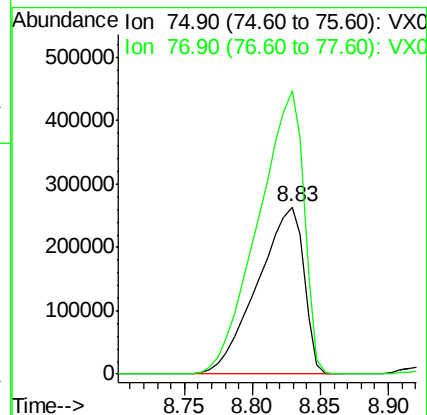

#55

1,1,2-Trichloroethane

Concen: 8.547 ug/l

RT: 9.17 min Scan# 1315

Delta R.T. -0.04 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Tgt Ion: 97 Resp: 24100




Ion Ratio Lower Upper


97 100

83 6.8 73.2 109.8#

85 1.4 46.6 69.8#

99 0.4 50.1 75.1#

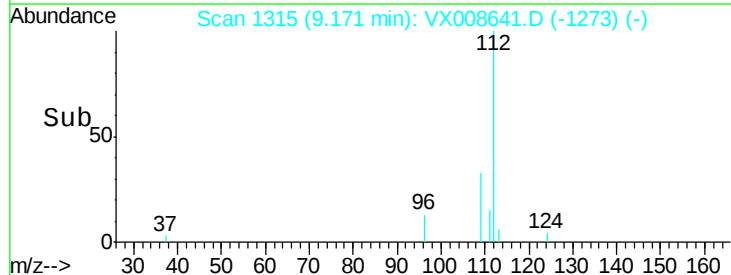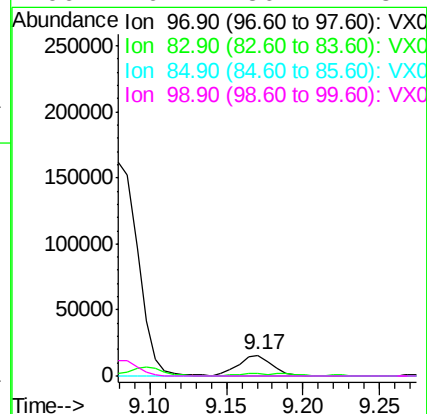

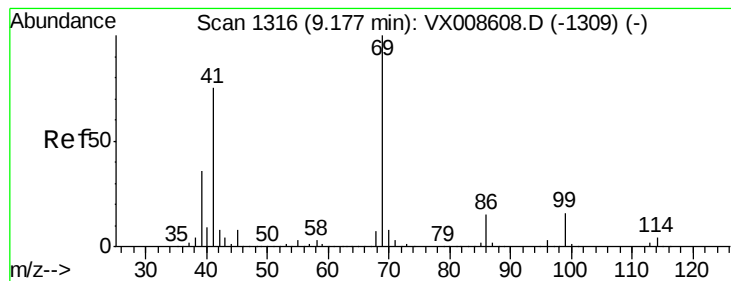

#56

Ethyl methacrylate

Concen: 11.060 ug/l

RT: 9.07 min Scan# 1298

Delta R.T. -0.11 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3





Tgt Ion: 69 Resp: 56425

Ion Ratio Lower Upper

69 100

41 0.0 60.1 90.1#

39 56.2 28.9 43.3#

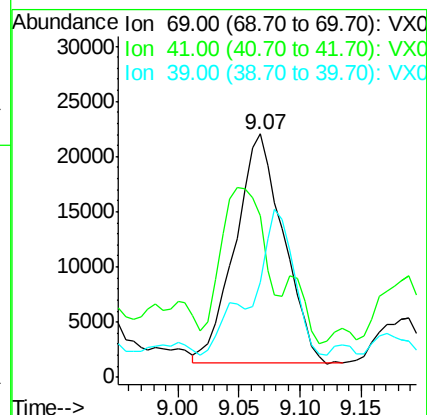

#58

2-Chloroethyl Vinyl ether

Concen: 1.526 ug/l

RT: 8.26 min Scan# 1166

Delta R.T. -0.05 min

Lab File: VX008641.D




Acq: 04 Apr 2019 17:17


Tgt Ion: 63 Resp: 3975

Ion Ratio Lower Upper

63 100

106 0.0 19.0 28.6#



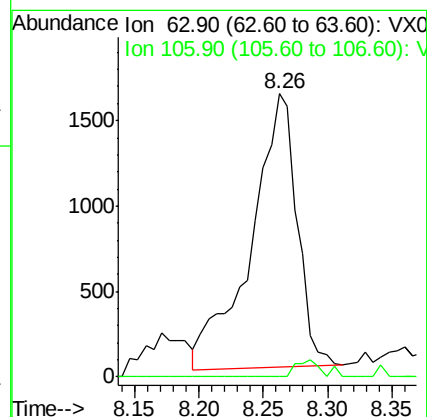





#59
2-Hexanone
Concen: 206.477 ug/l
RT: 9.51 min Scan# 1371
Delta R.T. 0.02 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17




Instrument :
MSVOA_X
ClientSampleId :
MW-3


Tgt Ion: 43 Resp: 863813
Ion Ratio Lower Upper
43 100
58 16.2 25.9 77.7#

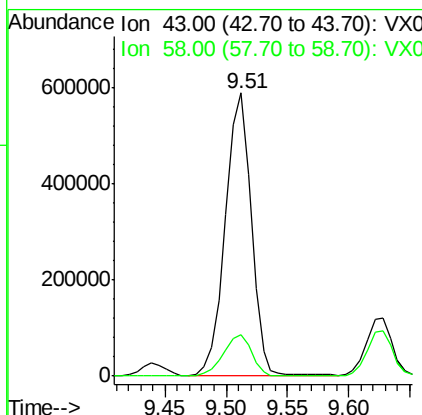

#61
1,2-Dibromoethane
Concen: 14.007 ug/l
RT: 9.67 min Scan# 1397
Delta R.T. -0.00 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion: 107 Resp: 41115
Ion Ratio Lower Upper
107 100
109 93.2 74.1 111.1



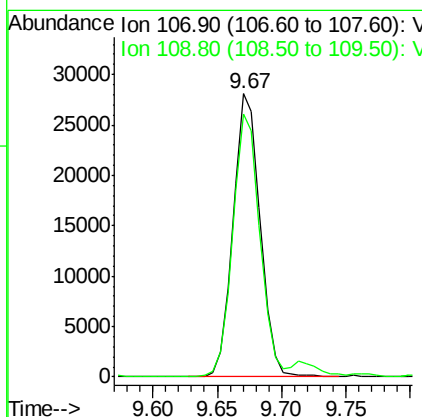





#62
4-Bromofluorobenzene
Concen: 45.136 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17




Instrument :
MSVOA_X
ClientSampleId :
MW-3


Tgt Ion	Ratio	Lower	Upper
95	100		
174	75.5	0.0	151.8
176	73.5	0.0	145.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.01 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion	Ratio	Lower	Upper
117	100		
82	57.8	49.6	74.4
119	32.3	25.0	37.4









#65
Chlorobenzene
Concen: 1.447 ug/l
RT: 10.34 min Scan# 1506
Delta R.T. 0.19 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17




Instrument :
MSVOA_X
ClientSampled :
MW-3


Tgt Ion: 112 Resp: 9900
Ion Ratio Lower Upper
112 100
114 8.6 25.8 38.8#

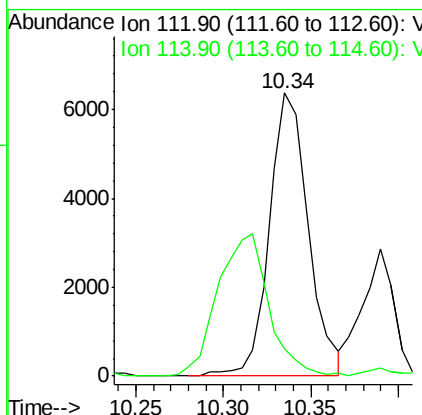

#67
Ethyl Benzene
Concen: 1130.618 ug/l
RT: 10.26 min Scan# 1494
Delta R.T. 0.01 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion: 91 Resp: 14422283
Ion Ratio Lower Upper
91 100
106 47.9 23.7 35.5#


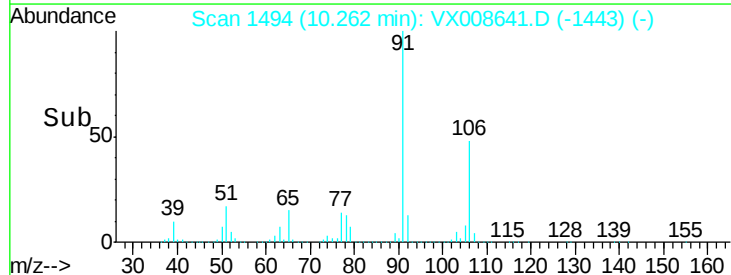
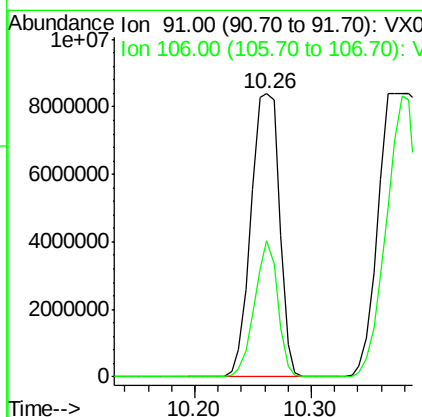





#68
m/p-Xylenes
Concen: 3207.903 ug/l
RT: 10.38 min Scan# 1513
Delta R.T. 0.02 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17




Instrument :
MSVOA_X
ClientSampled :
MW-3


Tgt Ion:106 Resp:14713025
Ion Ratio Lower Upper
106 100
91 136.2 168.5 252.7#



#69
o-Xylene
Concen: 1368.996 ug/l
RT: 10.71 min Scan# 1567
Delta R.T. 0.01 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion:106 Resp: 6084956
Ion Ratio Lower Upper
106 100
91 193.8 111.5 334.4





#70

Styrene

Concen: 47.483 ug/l

RT: 10.71 min Scan# 1568

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3





Tgt Ion:104 Resp: 363803

Ion Ratio Lower Upper

104 100

78 266.2 42.3 63.5#

103 248.7 44.4 66.6#

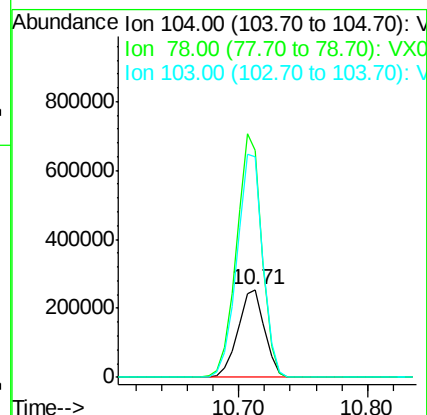

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17




Tgt Ion:152 Resp: 132496


Ion Ratio Lower Upper

152 100

115 60.3 43.5 130.5

150 156.6 0.0 348.8

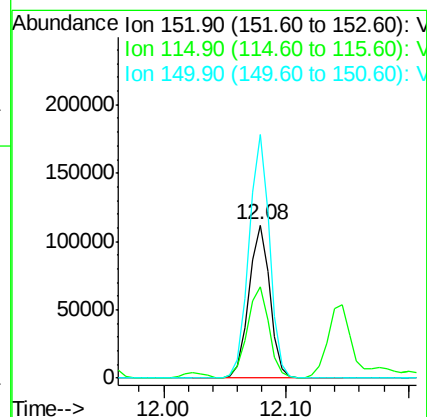



#73

Isopropylbenzene

Concen: 39.454 ug/l

RT: 11.02 min Scan# 1618

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :





MW-3

Tgt Ion:105 Resp: 433220

Ion Ratio Lower Upper

105 100

120 25.7 12.9 38.6

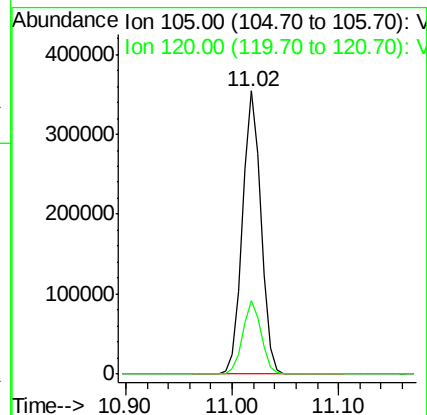

#74

N-ethyl acetate

Concen: 8.732 ug/l

RT: 10.90 min Scan# 1599

Delta R.T. 0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Tgt Ion: 43 Resp: 56413




Ion Ratio Lower Upper


43 100

70 51.0 30.2 45.4#

55 61.7 18.2 27.4#

61 0.0 18.6 28.0#

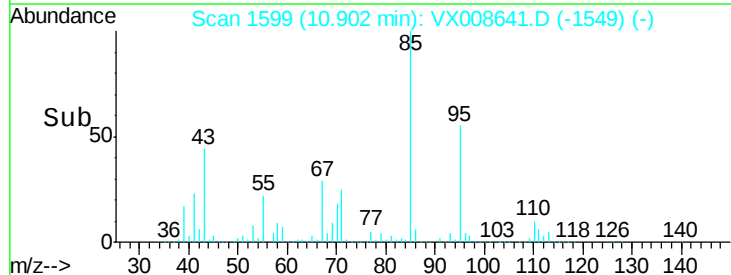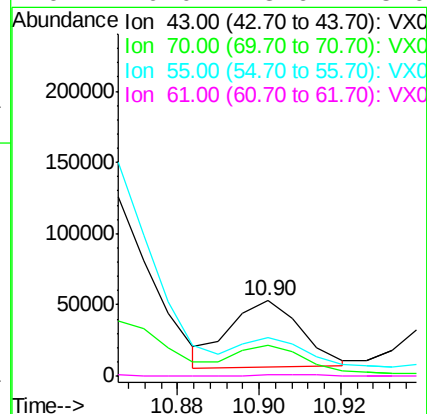



#75

1,1,2,2-Tetrachloroethane

Concen: 9.904 ug/l

RT: 11.23 min Scan# 1653

Delta R.T. -0.04 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3


Tgt Ion: 83 Resp: 41358

Ion Ratio Lower Upper

83 100

131 0.0 4.5 13.7#




85 17.7 32.0 96.2#



Abundance Ion 82.90 (82.60 to 83.60): VX0

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VX0

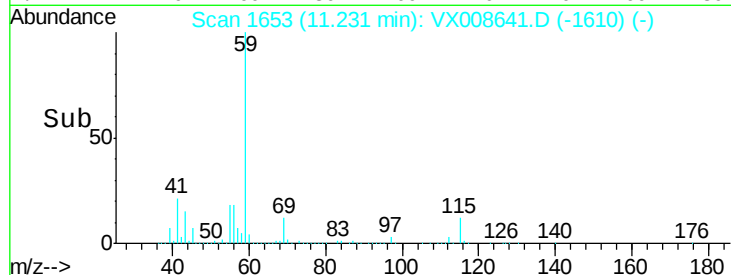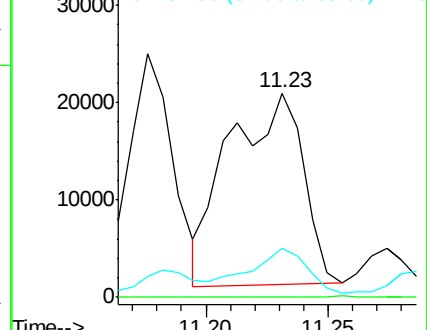

#76

1,2,3-Trichloropropane

Concen: 1.648 ug/l

RT: 11.33 min Scan# 1670

Delta R.T. 0.04 min

Lab File: VX008641.D


Acq: 04 Apr 2019 17:17

Tgt Ion: 75 Resp: 5999

Ion Ratio Lower Upper



75 100


77 0.0 22.3 66.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

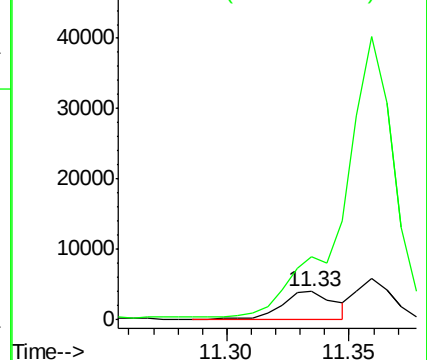



#78

n-propylbenzene

Concen: 89.939 ug/l

RT: 11.36 min Scan# 1674

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion: 91 Resp: 1149884

Ion Ratio Lower Upper

91 100

120 21.9 10.9 32.7

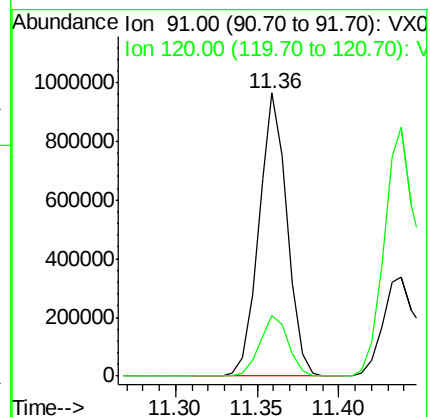

#79

2-Chlorotoluene

Concen: 74.935 ug/l

RT: 11.44 min Scan# 1687

Delta R.T. 0.02 min

Lab File: VX008641.D




Acq: 04 Apr 2019 17:17


Tgt Ion: 91 Resp: 579770

Ion Ratio Lower Upper

91 100

126 0.0 16.1 48.3#

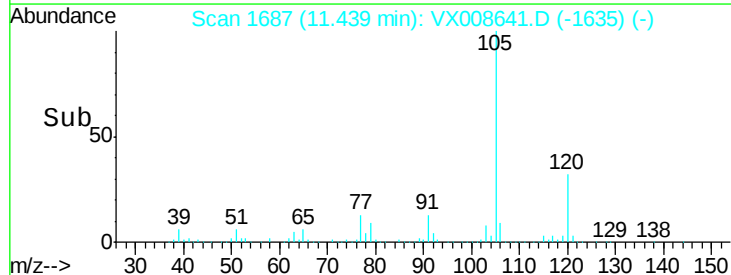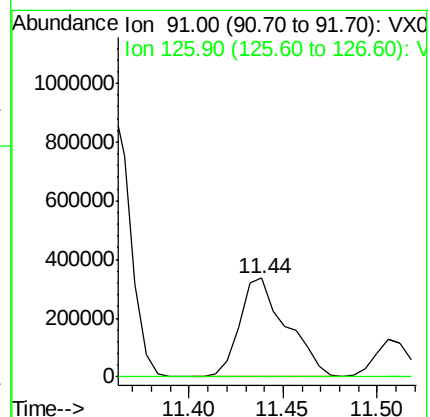



#80

1,3,5-Trimethylbenzene

Concen: 162.849 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :





MW-3

Tgt Ion:105 Resp: 1500989

Ion Ratio Lower Upper

105 100

120 48.0 23.5 70.6

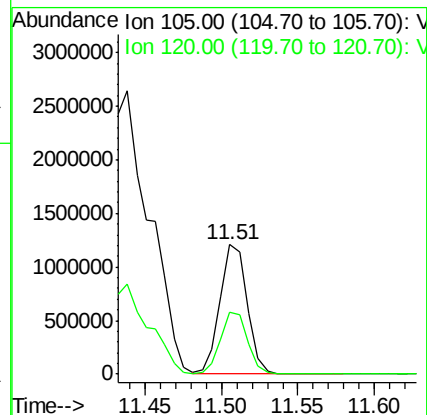

#81

trans-1,4-Dichloro-2-butene

Concen: 4.012 ug/l

RT: 11.02 min Scan# 1618

Delta R.T. -0.06 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17




Tgt Ion: 75 Resp: 5298


Ion Ratio Lower Upper

75 100

53 0.0 81.3 121.9#

89 106.9 35.6 53.4#

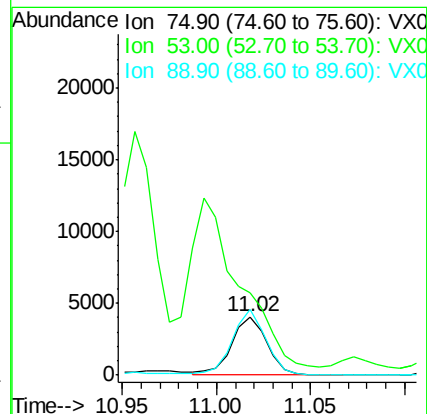



#82

4-Chlorotoluene

Concen: 18.078 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. -0.01 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :


MW-3

Tgt Ion: 91 Resp: 161903

Ion Ratio Lower Upper




91 100

126 0.0 13.9 41.6#



Abundance Ion 91.00 (90.70 to 91.70): VX008608.D (-1690) (-)

Ion 125.90 (125.60 to 126.60): VX008608.D (-1690) (-)

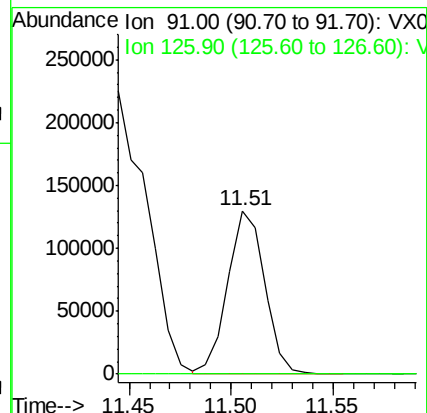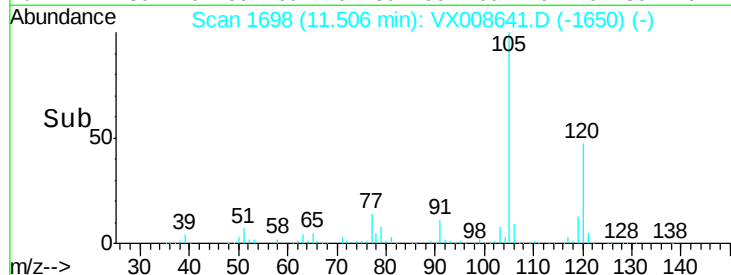

#83

tert-Butylbenzene

Concen: 61.306 ug/l

RT: 11.81 min Scan# 1748

Delta R.T. 0.04 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17


Tgt Ion: 119 Resp: 543628

Ion Ratio Lower Upper

119 100

91 84.5 30.0 90.1



134 0.0 11.1 33.3#




Abundance Ion 119.00 (118.70 to 119.70): VX008608.D (-1733) (-)

Ion 91.00 (90.70 to 91.70): VX008608.D (-1733) (-)

Ion 134.00 (133.70 to 134.70): VX008608.D (-1733) (-)



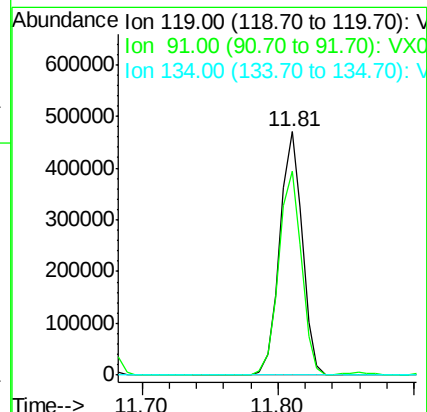





#84
 1,2,4-Trimethylbenzene
 Concen: 462.384 ug/l
 RT: 11.81 min Scan# 1748
 Delta R.T. 0.01 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17




Instrument :
 MSVOA_X
 ClientSampled :
 MW-3


Tgt Ion:105 Resp: 4315371
 Ion Ratio Lower Upper
 105 100
 120 45.9 21.8 65.3



#85
 sec-Butylbenzene
 Concen: 409.700 ug/l
 RT: 11.81 min Scan# 1748
 Delta R.T. -0.13 min
 Lab File: VX008641.D
 Acq: 04 Apr 2019 17:17

Tgt Ion:105 Resp: 4315371
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.4 28.2#









#86
p-Isopropyltoluene
Concen: 7.019 ug/l
RT: 12.02 min Scan# 1783
Delta R.T. -0.04 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Instrument :
MSVOA_X
ClientSampleId :
MW-3

Tgt Ion: 119 Resp: 66354
Ion Ratio Lower Upper
119 100
134 27.2 12.8 38.4
91 23.3 12.2 36.6




Abundance Ion 119.00 (118.70 to 119.70): V
Ion 134.00 (133.70 to 134.70): V
Ion 91.00 (90.70 to 91.70): V


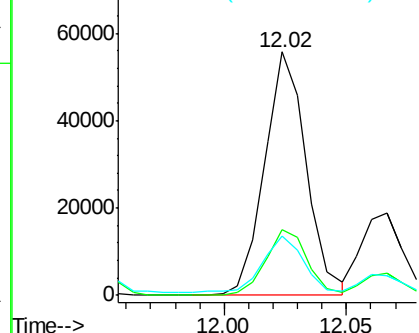



#89
n-Butylbenzene
Concen: 13.267 ug/l
RT: 12.38 min Scan# 1841
Delta R.T. -0.01 min
Lab File: VX008641.D
Acq: 04 Apr 2019 17:17

Tgt Ion: 91 Resp: 117627
Ion Ratio Lower Upper
91 100
92 27.8 26.4 79.2
134 120.1 12.0 36.0#



Abundance Ion 91.00 (90.70 to 91.70): VX0
Ion 92.00 (91.70 to 92.70): VX0
Ion 134.00 (133.70 to 134.70): V

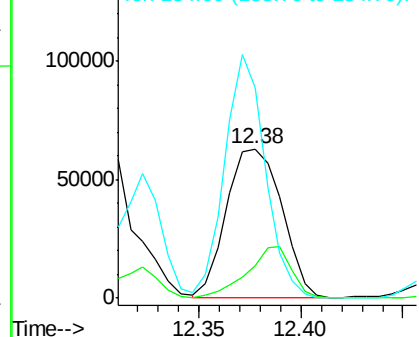



#90

Hexachloroethane

Concen: 20.903 ug/l

RT: 12.67 min Scan# 1889

Delta R.T. 0.07 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampleId :


MW-3

Tgt Ion:117 Resp: 32776

Ion Ratio Lower Upper




117 100

201 0.0 40.6 122.0#

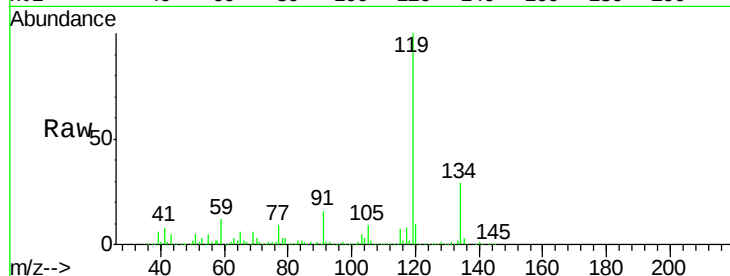

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

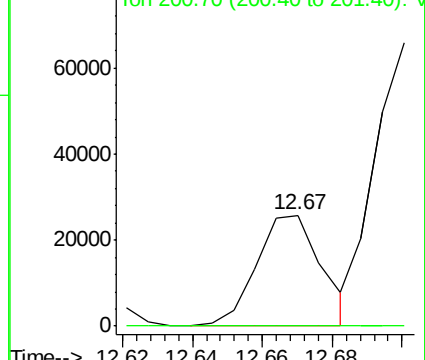

#91

1,2-Dichlorobenzene

Concen: 0.212 ug/l

RT: 12.39 min Scan# 1843

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17


Tgt Ion:146 Resp: 993

Ion Ratio Lower Upper

146 100

111 280.0 21.3 63.9#



148 67.0 31.7 95.1




Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

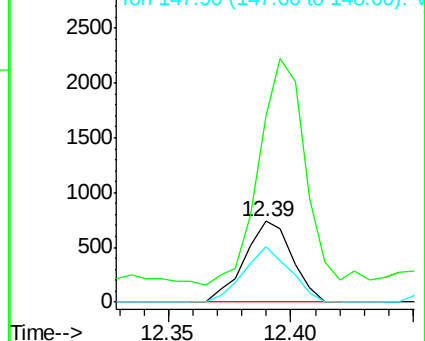



#92

1,2-Dibromo-3-Chloropropane

Concen: 2.236 ug/l

RT: 13.02 min Scan# 1946

Delta R.T. 0.02 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17

Instrument :

MSVOA_X

ClientSampled :

MW-3


Tgt Ion: 75 Resp: 2054

Ion Ratio Lower Upper

75 100

155 0.0 39.9 119.6#




157 0.0 51.5 154.7#



Abundance Ion 74.90 (74.60 to 75.60): VX008641.D (-1894) (-)

Ion 154.80 (154.50 to 155.50): VX008641.D (-1894) (-)

Ion 156.80 (156.50 to 157.50): VX008641.D (-1894) (-)

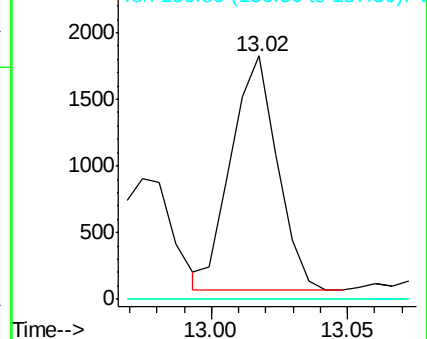

#95

Naphthalene

Concen: 55.345 ug/l

RT: 13.83 min Scan# 2080

Delta R.T. -0.00 min

Lab File: VX008641.D

Acq: 04 Apr 2019 17:17


Tgt Ion: 128 Resp: 603445

Ion Ratio Lower Upper

128 100

127 13.1 10.4 15.6

129 10.9 8.6 13.0



Abundance Ion 128.00 (127.70 to 128.70): VX008641.D (-2031) (-)

Ion 127.00 (126.70 to 127.70): VX008641.D (-2031) (-)

Ion 129.00 (128.70 to 129.70): VX008641.D (-2031) (-)

