

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
 Data File : VX008642.D
 Acq On : 04 Apr 2019 17:40
 Operator : JC/SP
 Sample : K2265-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BW-04419

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.276	16	20	23	rBV2	28477	41001	3.47%	0.608%
2	1.404	37	41	47	rVB	62591	62707	5.31%	0.930%
3	1.459	47	50	55	rVB	18617	17235	1.46%	0.256%
4	1.617	67	76	79	rVV7	6680	17693	1.50%	0.262%
5	1.782	98	103	110	rBV	27846	41592	3.52%	0.617%
6	1.946	127	130	134	rBV	9111	12565	1.06%	0.186%
7	1.995	134	138	146	rVB	24986	37479	3.18%	0.556%
8	2.117	153	158	164	rVV	19143	28594	2.42%	0.424%
9	2.215	167	174	180	rVB2	7527	13549	1.15%	0.201%
10	2.446	206	212	221	rVB	11760	20345	1.72%	0.302%
11	2.611	233	239	247	rVB2	7175	14354	1.22%	0.213%
12	4.403	525	533	547	rVB	6189	17232	1.46%	0.256%
13	5.501	699	713	723	rBV	125350	356695	30.22%	5.291%
14	5.659	729	739	758	rVB	221698	624918	52.95%	9.270%
15	6.062	795	805	813	rBV	155067	407168	34.50%	6.040%
16	6.147	813	819	828	rVB2	24378	66324	5.62%	0.984%
17	6.860	926	936	950	rBV	362534	856236	72.54%	12.702%
18	8.714	1233	1240	1247	rBV	753134	1180291	100.00%	17.509%
19	8.787	1247	1252	1262	rVB	88087	150428	12.74%	2.232%
20	10.110	1458	1469	1480	rBV	699760	980617	83.08%	14.547%
21	10.250	1487	1492	1499	rVB	26670	35599	3.02%	0.528%
22	10.354	1504	1509	1516	rBV	69553	98873	8.38%	1.467%
23	10.695	1558	1565	1572	rBV	26830	37978	3.22%	0.563%
24	11.134	1631	1637	1647	rBV	560583	726589	61.56%	10.779%
25	11.804	1743	1747	1752	rBV	11663	14931	1.27%	0.221%
26	12.079	1786	1792	1799	rBV	643867	827659	70.12%	12.278%
27	12.268	1818	1823	1835	rBV	26843	52374	4.44%	0.777%


Sum of corrected areas: 6741026

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040419\
Data File : VX008642.D
Acq On : 04 Apr 2019 17:40
Operator : JC/SP
Sample : K2265-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BW-04419

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

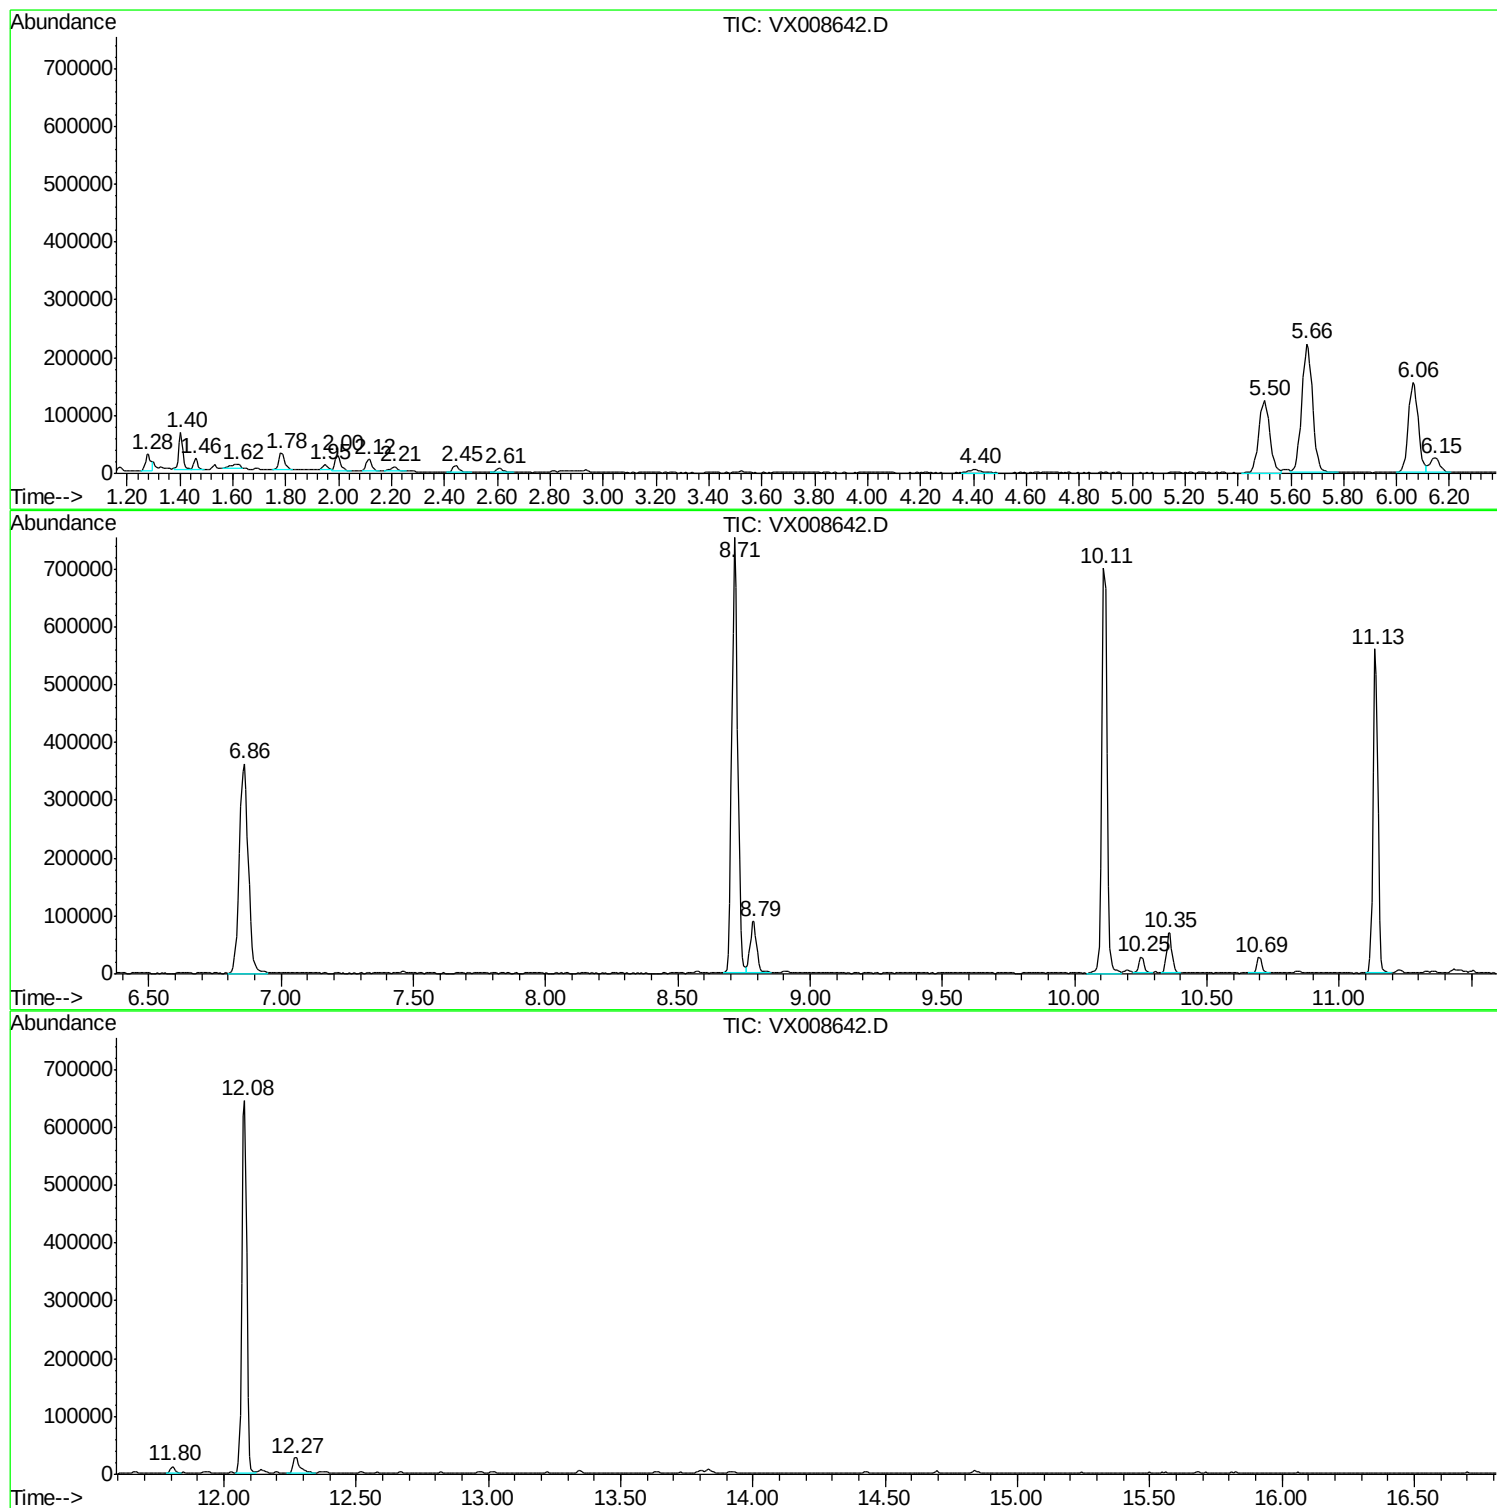

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040419\
Data File : VX008642.D
Acq On : 04 Apr 2019 17:40
Operator : JC/SP
Sample : K2265-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BW-04419










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.40	5.02 ug/l	62707	Pentafluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane	58	C4H10	000106-97-8	59
2		Isopropylsulfonyl chloride	142	C3H7ClO2S	010147-37-2	9
3		Isobutane	58	C4H10	000075-28-5	9
4		Diazene, dimethyl-	58	C2H6N2	000503-28-6	4
5		Hydrogen azide	43	HN3	007782-79-8	4

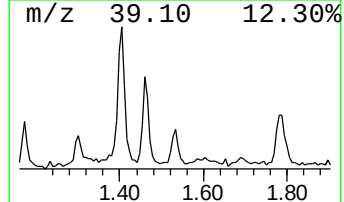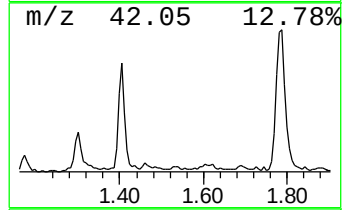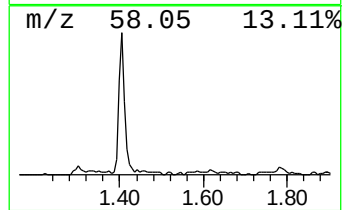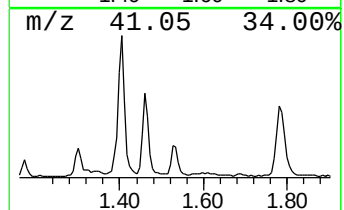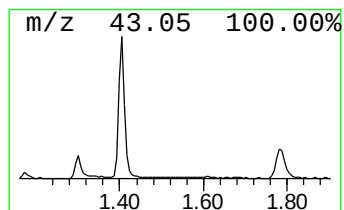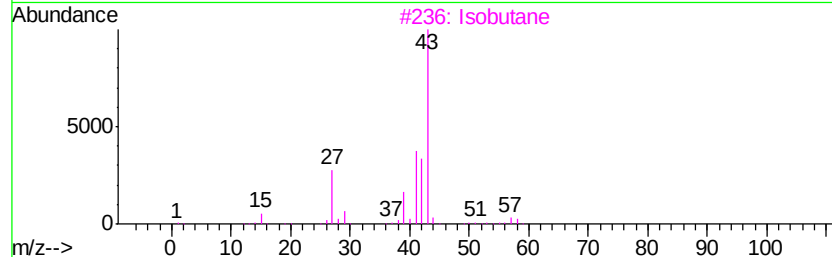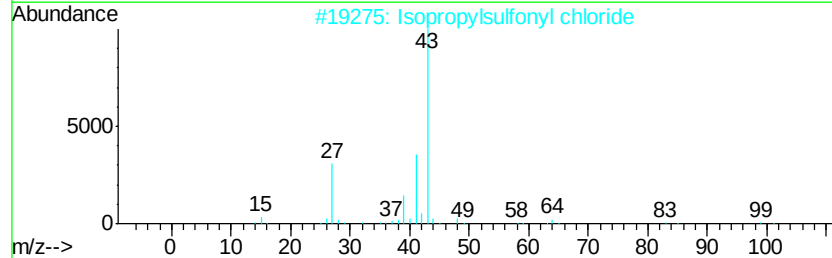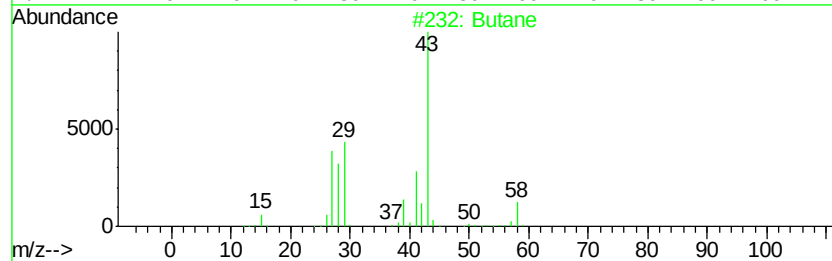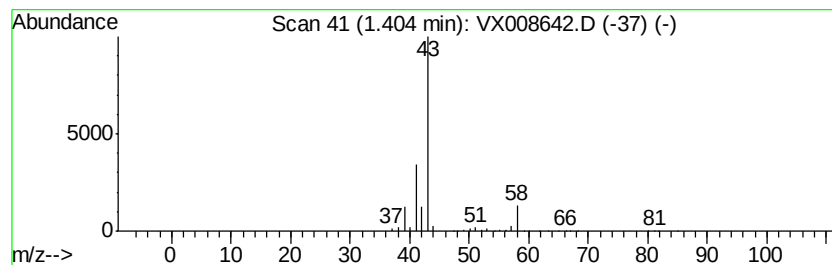

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX040419\
Data File : VX008642.D
Acq On : 04 Apr 2019 17:40
Operator : JC/SP
Sample : K2265-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BW-04419

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane	1.40	5.0	ug/l	62707	1	5.66	624918	50.0