

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
 Data File : VX008644.D
 Acq On : 04 Apr 2019 18:27
 Operator : JC/SP
 Sample : K2275-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0705

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.404	36	41	47	rBV	455516	454628	3.95%	0.625%
2	1.782	98	103	122	rVB	1593874	2359606	20.51%	3.245%
3	1.995	133	138	152	rVB	670793	989126	8.60%	1.360%
4	2.842	259	277	281	rBV	245794	562506	4.89%	0.774%
5	2.891	281	285	288	rVV	232974	473819	4.12%	0.652%
6	2.928	288	291	302	rVB	247508	490799	4.27%	0.675%
7	3.172	321	331	348	rVB	169465	389741	3.39%	0.536%
8	3.525	378	389	403	rBV	146994	338768	2.94%	0.466%
9	4.306	508	517	524	rBV2	55299	171262	1.49%	0.236%
10	4.403	524	533	549	rVB2	483289	1419623	12.34%	1.952%
11	5.500	700	713	718	rBV	122867	363447	3.16%	0.500%
12	5.580	718	726	734	rVV	599988	1940945	16.87%	2.669%
13	5.659	734	739	746	rVV	228431	689188	5.99%	0.948%
14	5.726	746	750	769	rVV2	129920	358737	3.12%	0.493%
15	5.933	771	784	796	rVV4	107289	365479	3.18%	0.503%
16	6.061	796	805	811	rVV	160724	414476	3.60%	0.570%
17	6.141	811	818	829	rVV	681848	1779399	15.46%	2.447%
18	6.256	829	837	844	rVV2	83486	258189	2.24%	0.355%
19	6.354	844	853	862	rVV3	227222	704848	6.13%	0.969%
20	6.452	862	869	883	rVB	145116	401828	3.49%	0.553%
21	6.860	925	936	947	rBV	366412	866769	7.53%	1.192%
22	7.464	1022	1035	1046	rBV	1223079	2727053	23.70%	3.750%
23	7.732	1074	1079	1091	rVB	120141	234894	2.04%	0.323%
24	8.055	1122	1132	1141	rVB	161137	369348	3.21%	0.508%
25	8.177	1144	1152	1160	rBV	215232	439464	3.82%	0.604%
26	8.500	1200	1205	1210	rBV2	77465	129509	1.13%	0.178%
27	8.665	1225	1232	1235	rBV3	180163	327328	2.84%	0.450%
28	8.713	1235	1240	1246	rVV	780991	1315708	11.43%	1.809%
29	8.786	1246	1252	1257	rVV	1850900	2849361	24.76%	3.919%
30	8.841	1257	1261	1265	rVV	88923	155397	1.35%	0.214%
31	9.043	1288	1294	1305	rVB	147080	250492	2.18%	0.344%
32	9.164	1305	1314	1319	rBV	76269	126292	1.10%	0.174%
33	9.518	1366	1372	1376	rBV	99884	147017	1.28%	0.202%
34	9.573	1376	1381	1385	rVV3	67407	118859	1.03%	0.163%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
 Data File : VX008644.D
 Acq On : 04 Apr 2019 18:27
 Operator : JC/SP
 Sample : K2275-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0705

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

35	9.622	1385	1389	1394	rVB	189521	254115	2.21%	0.349%
36	9.677	1394	1398	1403	rBV	148822	217646	1.89%	0.299%
37	10.109	1465	1469	1478	rVV2	687158	1107495	9.62%	1.523%
38	10.183	1478	1481	1486	rVV	78848	117815	1.02%	0.162%
39	10.250	1486	1492	1502	rVV	3264255	4269432	37.10%	5.872%
40	10.359	1502	1510	1516	rVV	8614652	11506582	100.00%	15.824%
41	10.640	1547	1556	1560	rBV4	53372	115886	1.01%	0.159%
42	10.695	1560	1565	1575	rVB	1723823	2325689	20.21%	3.198%
43	10.835	1579	1588	1593	rBV2	95480	156896	1.36%	0.216%
44	10.908	1593	1600	1605	rBV3	76019	146000	1.27%	0.201%
45	11.018	1613	1618	1622	rBV	381544	476460	4.14%	0.655%
46	11.134	1632	1637	1642	rBV	573727	761516	6.62%	1.047%
47	11.359	1669	1674	1681	rBV	434766	530565	4.61%	0.730%
48	11.432	1681	1686	1693	rVV	1526686	2645292	22.99%	3.638%
49	11.505	1693	1698	1708	rVB	2073654	2487983	21.62%	3.422%
50	11.664	1719	1724	1733	rVB	892671	1168885	10.16%	1.608%
51	11.804	1743	1747	1752	rVB	4172095	5028609	43.70%	6.916%
52	12.024	1776	1783	1786	rBV	279227	332288	2.89%	0.457%
53	12.079	1786	1792	1797	rVB2	669515	980265	8.52%	1.348%
54	12.140	1797	1802	1808	rBV	1995711	2420623	21.04%	3.329%
55	12.298	1823	1828	1830	rBV	471560	604001	5.25%	0.831%
56	12.322	1830	1832	1836	rVB	298583	306003	2.66%	0.421%
57	12.371	1836	1840	1848	rVB2	578043	802626	6.98%	1.104%
58	12.457	1848	1854	1859	rBV2	102728	156043	1.36%	0.215%
59	12.517	1859	1864	1870	rVB	298022	353035	3.07%	0.486%
60	12.585	1870	1875	1877	rBV	324510	433632	3.77%	0.596%
61	12.609	1877	1879	1883	rVB	388609	387826	3.37%	0.533%
62	12.664	1883	1888	1892	rBV	365380	446446	3.88%	0.614%
63	12.755	1898	1903	1910	rVB4	251377	472884	4.11%	0.650%
64	12.902	1922	1927	1931	rVB2	251482	323934	2.82%	0.445%
65	12.975	1931	1939	1942	rBV	272305	369179	3.21%	0.508%
66	13.017	1942	1946	1952	rVB	481531	588396	5.11%	0.809%
67	13.078	1952	1956	1961	rBV4	68410	139421	1.21%	0.192%
68	13.219	1972	1979	1983	rBV4	161466	282603	2.46%	0.389%
69	13.341	1995	1999	2005	rVB2	768043	1069071	9.29%	1.470%
70	13.481	2017	2022	2026	rVB	185766	247313	2.15%	0.340%
71	13.639	2044	2048	2054	rVV3	91623	170094	1.48%	0.234%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
Data File : VX008644.D
Acq On : 04 Apr 2019 18:27
Operator : JC/SP
Sample : K2275-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0705

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260

72	13.718	2058	2061	2067	rVB2	93126	165499	1.44%	0.228%
73	13.834	2073	2080	2087	rVB	871227	1242542	10.80%	1.709%
74	14.267	2148	2151	2164	rVB2	75684	180284	1.57%	0.248%
75	14.694	2216	2221	2230	rVB	687734	858498	7.46%	1.181%
76	14.834	2239	2244	2253	rVB	482433	656154	5.70%	0.902%
77	15.547	2356	2361	2366	rBV	83860	131174	1.14%	0.180%
78	15.682	2378	2383	2387	rBV	105360	173339	1.51%	0.238%
79	15.724	2387	2390	2396	rVB	82464	120399	1.05%	0.166%


Sum of corrected areas: 72714343

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040419\
Data File : VX008644.D
Acq On : 04 Apr 2019 18:27
Operator : JC/SP
Sample : K2275-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0705

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

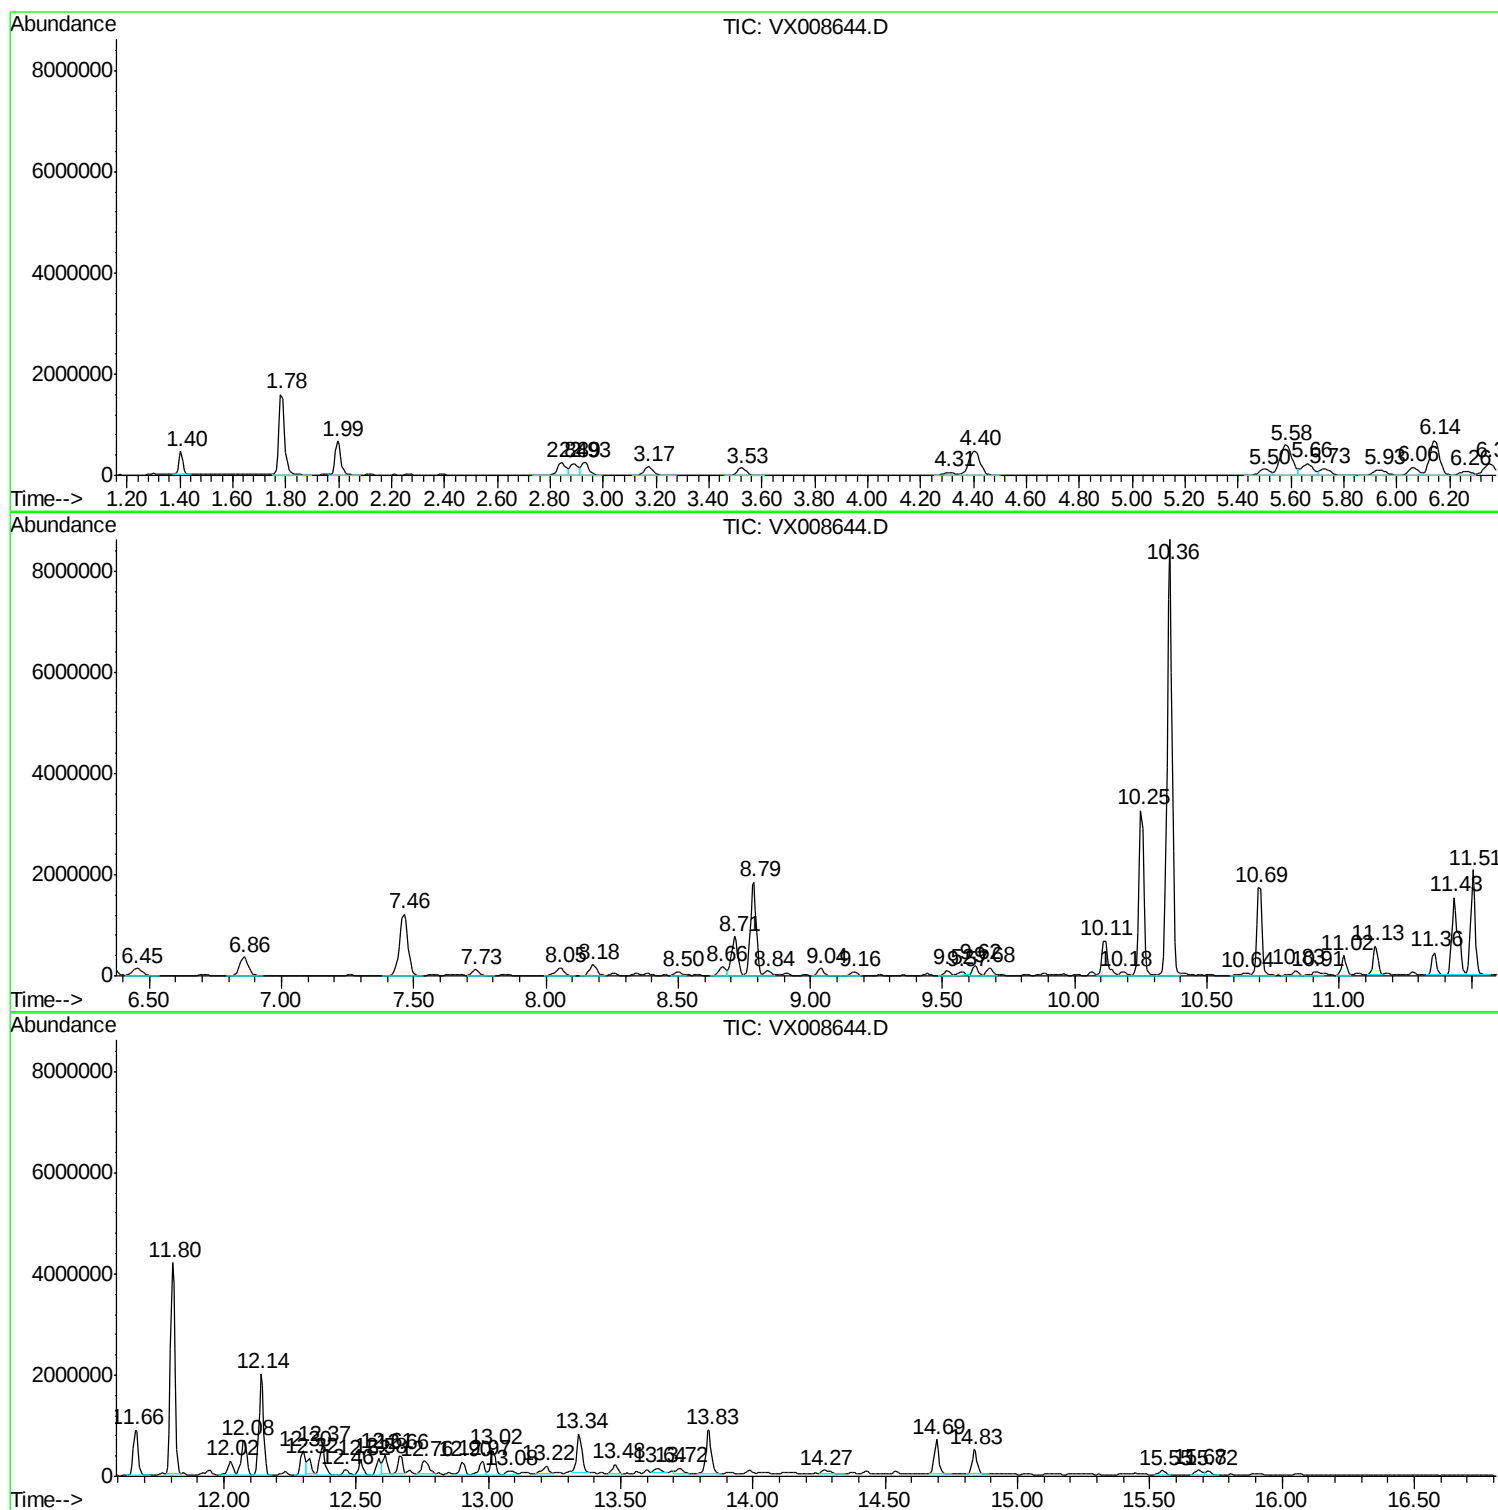

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX040419\
Data File : VX008644.D
Acq On : 04 Apr 2019 18:27
Operator : JC/SP
Sample : K2275-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0705

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX040419\
Data File : VX008644.D
Acq On : 04 Apr 2019 18:27
Operator : JC/SP
Sample : K2275-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0705

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc