

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
 Data File : VX008648.D
 Acq On : 04 Apr 2019 20:00
 Operator : JC/SP
 Sample : K2275-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0713

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	16	21	27	rBV	16751	30946	1.51%	0.160%
2	1.404	27	41	44	rBV3	13907	40937	2.00%	0.212%
3	1.782	98	103	111	rVB	21321	33078	1.62%	0.171%
4	2.611	226	239	248	rBV	22720	45539	2.23%	0.235%
5	2.843	269	277	280	rBV	12010	25533	1.25%	0.132%
6	2.891	280	285	288	rVV	17009	37289	1.82%	0.193%
7	2.928	288	291	301	rVB	18382	36742	1.80%	0.190%
8	3.172	321	331	341	rVB	17450	41631	2.03%	0.215%
9	4.403	524	533	549	rVB	34145	101923	4.98%	0.527%
10	5.501	699	713	721	rBV	122666	361785	17.68%	1.870%
11	5.580	721	726	731	rVV2	35539	99879	4.88%	0.516%
12	5.659	731	739	762	rVB	220310	676487	33.05%	3.497%
13	5.933	772	784	795	rBV5	11614	42813	2.09%	0.221%
14	6.061	795	805	814	rVV	156356	408366	19.95%	2.111%
15	6.147	814	819	827	rVV3	10039	27693	1.35%	0.143%
16	6.257	827	837	845	rVV4	11358	41120	2.01%	0.213%
17	6.354	846	853	862	rVV3	18186	55319	2.70%	0.286%
18	6.458	862	870	880	rVB2	9904	28989	1.42%	0.150%
19	6.860	926	936	954	rBV	356257	856867	41.87%	4.429%
20	7.458	1022	1034	1045	rBV2	70610	169454	8.28%	0.876%
21	8.055	1123	1132	1141	rVB3	12587	33557	1.64%	0.173%
22	8.177	1143	1152	1161	rBV	22908	50518	2.47%	0.261%
23	8.665	1224	1232	1234	rBV3	22989	39573	1.93%	0.205%
24	8.713	1234	1240	1248	rVV	747844	1196269	58.45%	6.184%
25	8.781	1248	1251	1256	rVV2	13692	22192	1.08%	0.115%
26	9.037	1288	1293	1300	rVV	24852	40824	1.99%	0.211%
27	9.165	1304	1314	1320	rBV	17628	30429	1.49%	0.157%
28	9.622	1385	1389	1394	rVB2	23441	32808	1.60%	0.170%
29	10.110	1464	1469	1477	rBV	688773	955199	46.67%	4.938%
30	10.183	1477	1481	1486	rVB	18989	29384	1.44%	0.152%
31	10.250	1486	1492	1502	rBV	1008524	1297355	63.39%	6.706%
32	10.353	1502	1509	1520	rVV	1485854	2046597	100.00%	10.580%
33	10.695	1562	1565	1575	rVB3	15276	25382	1.24%	0.131%
34	10.835	1578	1588	1596	rBV4	15561	29738	1.45%	0.154%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
 Data File : VX008648.D
 Acq On : 04 Apr 2019 20:00
 Operator : JC/SP
 Sample : K2275-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0713

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

35	11.018	1613	1618	1624	rBV	91074	120989	5.91%	0.625%
36	11.134	1631	1637	1643	rBV	581435	765732	37.41%	3.958%
37	11.183	1643	1645	1651	rVB2	18831	22021	1.08%	0.114%
38	11.359	1669	1674	1681	rVB2	137380	186477	9.11%	0.964%
39	11.432	1681	1686	1693	rVV	197853	336627	16.45%	1.740%
40	11.506	1693	1698	1708	rVB	359538	441235	21.56%	2.281%
41	11.664	1720	1724	1733	rVB	205261	269099	13.15%	1.391%
42	11.768	1733	1741	1743	rBV	18135	29247	1.43%	0.151%
43	11.804	1743	1747	1752	rVB	543794	643134	31.42%	3.325%
44	11.920	1762	1766	1768	rBV	17041	24335	1.19%	0.126%
45	11.945	1768	1770	1776	rVB	24519	28759	1.41%	0.149%
46	12.024	1776	1783	1786	rBV	66975	83167	4.06%	0.430%
47	12.079	1786	1792	1798	rVV	662480	912657	44.59%	4.718%
48	12.140	1798	1802	1807	rVB	162046	185705	9.07%	0.960%
49	12.231	1813	1817	1821	rVB	21034	24484	1.20%	0.127%
50	12.298	1821	1828	1836	rBV2	329775	514456	25.14%	2.659%
51	12.371	1836	1840	1850	rVB3	157652	276408	13.51%	1.429%
52	12.463	1850	1855	1860	rBV4	31572	52579	2.57%	0.272%
53	12.518	1860	1864	1868	rVB	53866	64822	3.17%	0.335%
54	12.585	1871	1875	1877	rBV	87132	112287	5.49%	0.580%
55	12.609	1877	1879	1884	rVV	67195	67727	3.31%	0.350%
56	12.664	1884	1888	1892	rVV	138697	168237	8.22%	0.870%
57	12.701	1892	1894	1899	rVV	32993	38081	1.86%	0.197%
58	12.755	1899	1903	1910	rVB4	87435	171096	8.36%	0.884%
59	12.847	1915	1918	1921	rBV2	16097	20795	1.02%	0.107%
60	12.902	1922	1927	1931	rVB2	74554	105530	5.16%	0.546%
61	12.975	1931	1939	1942	rBV	122098	177714	8.68%	0.919%
62	13.018	1942	1946	1951	rVB	201575	248321	12.13%	1.284%
63	13.079	1951	1956	1962	rBV4	45964	93471	4.57%	0.483%
64	13.146	1965	1967	1971	rVB	23934	26858	1.31%	0.139%
65	13.225	1976	1980	1983	rBV2	56294	68035	3.32%	0.352%
66	13.310	1989	1994	1995	rBV2	23043	31644	1.55%	0.164%
67	13.347	1995	2000	2006	rVV2	297974	465668	22.75%	2.407%
68	13.426	2010	2013	2015	rVV2	23794	30488	1.49%	0.158%
69	13.475	2016	2021	2027	rVB2	148397	218584	10.68%	1.130%
70	13.560	2031	2035	2038	rVV2	24635	32266	1.58%	0.167%
71	13.603	2038	2042	2044	rVV	38697	54010	2.64%	0.279%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040419\
 Data File : VX008648.D
 Acq On : 04 Apr 2019 20:00
 Operator : JC/SP
 Sample : K2275-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0713

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260

72	13.645	2044	2049	2053	rVV4	80232	159520	7.79%	0.825%
73	13.700	2054	2058	2059	rVV	45781	65255	3.19%	0.337%
74	13.731	2059	2063	2068	rVV4	69531	140357	6.86%	0.726%
75	13.828	2071	2079	2087	rVB	377536	588966	28.78%	3.045%
76	13.908	2087	2092	2099	rBV4	54921	97849	4.78%	0.506%
77	13.981	2099	2104	2108	rVV3	70526	104614	5.11%	0.541%
78	14.030	2108	2112	2120	rVV4	37425	74397	3.64%	0.385%
79	14.152	2121	2132	2136	rVV5	32588	102962	5.03%	0.532%
80	14.267	2147	2151	2153	rBV2	65278	92894	4.54%	0.480%
81	14.371	2163	2168	2173	rBV4	53192	100032	4.89%	0.517%
82	14.426	2173	2177	2183	rVB3	70301	96934	4.74%	0.501%
83	14.536	2191	2195	2198	rBV2	79081	106854	5.22%	0.552%
84	14.566	2198	2200	2208	rVB3	36354	47191	2.31%	0.244%
85	14.694	2214	2221	2225	rBV	124219	172105	8.41%	0.890%
86	14.786	2230	2236	2239	rBV7	18994	38182	1.87%	0.197%
87	14.834	2239	2244	2249	rBV	148311	200589	9.80%	1.037%
88	14.956	2258	2264	2272	rVB6	61797	130858	6.39%	0.676%
89	15.115	2286	2290	2294	rBV4	25338	46407	2.27%	0.240%
90	15.231	2305	2309	2313	rBV5	32017	65685	3.21%	0.340%
91	15.389	2330	2335	2342	rBV	380723	569926	27.85%	2.946%
92	15.548	2357	2361	2364	rBV	24853	41612	2.03%	0.215%
93	15.621	2370	2373	2379	rVB3	20984	35523	1.74%	0.184%
94	15.682	2379	2383	2387	rVV	24930	43769	2.14%	0.226%
95	15.718	2387	2389	2396	rVB2	26692	39862	1.95%	0.206%
96	16.047	2438	2443	2448	rBV4	37176	77535	3.79%	0.401%


Sum of corrected areas: 19344838

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040419\
Data File : VX008648.D
Acq On : 04 Apr 2019 20:00
Operator : JC/SP
Sample : K2275-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0713

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

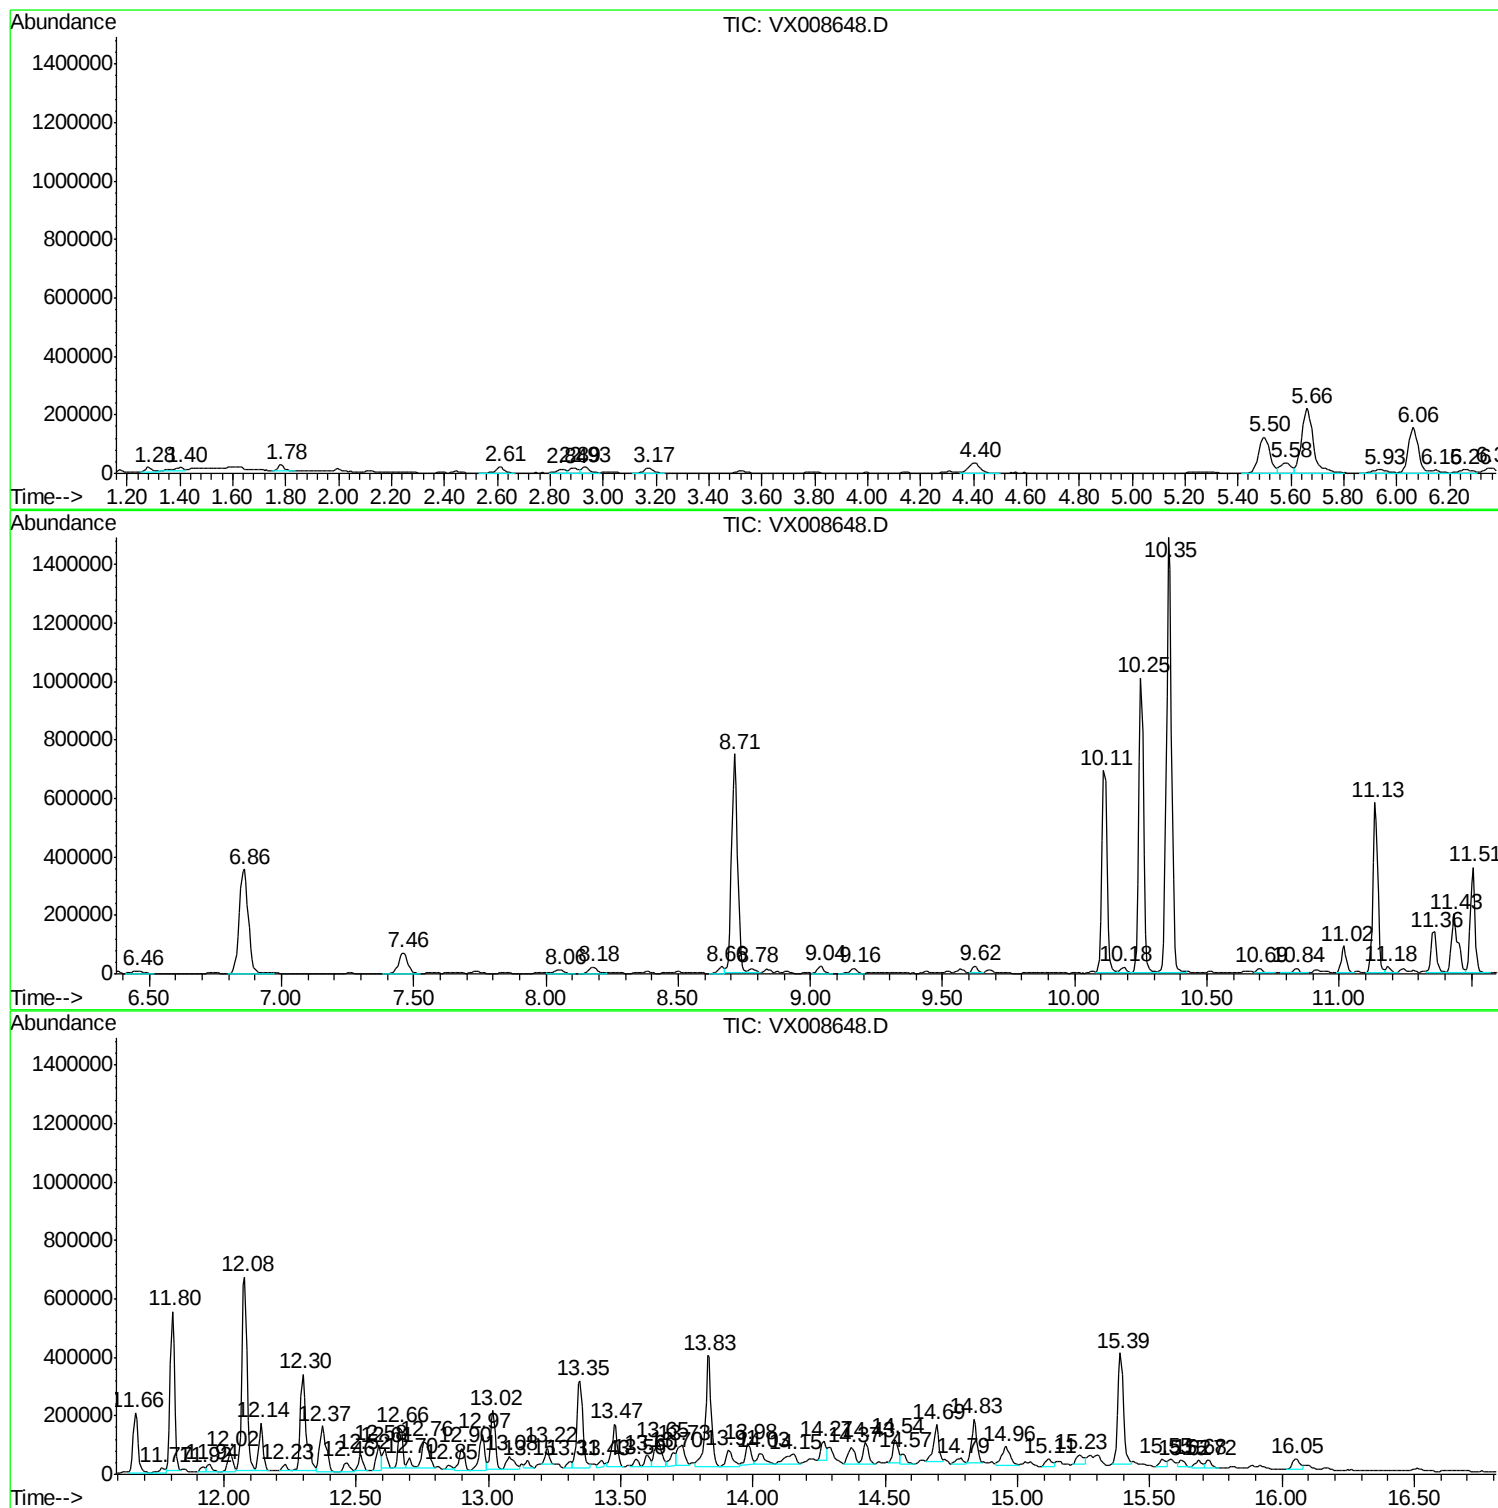

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX040419\
Data File : VX008648.D
Acq On : 04 Apr 2019 20:00
Operator : JC/SP
Sample : K2275-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0713

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX040419\
Data File : VX008648.D
Acq On : 04 Apr 2019 20:00
Operator : JC/SP
Sample : K2275-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0713

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc