


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX040419\
 Data File : VX008650.D
 Acq On : 04 Apr 2019 21:10
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260
 Last Update : Thu Apr 04 04:47:41 2019

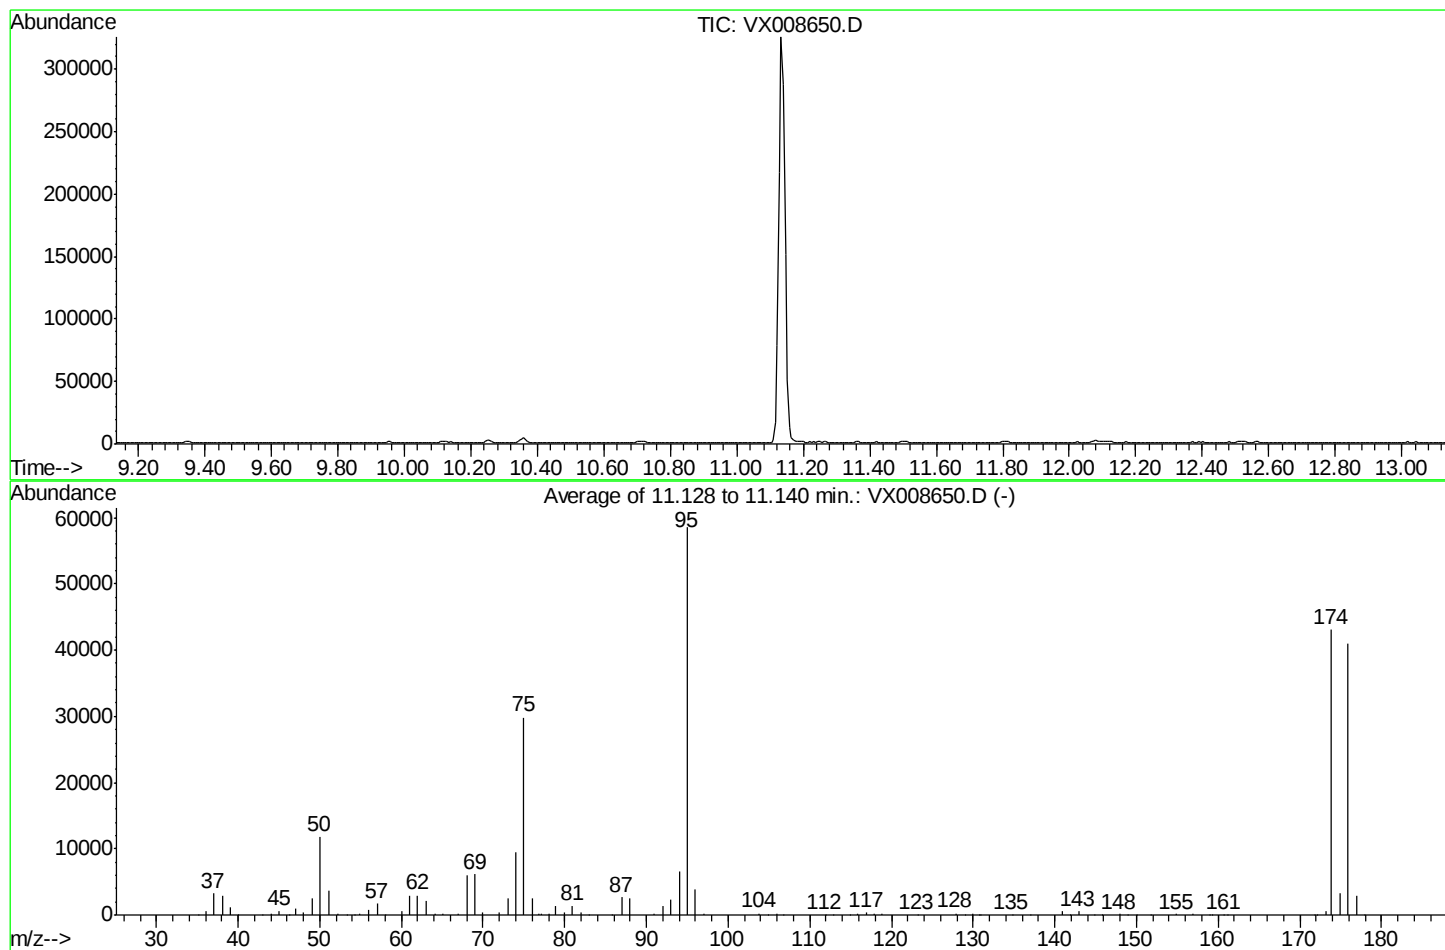

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	11792	PASS
75	95	30	60	50.9	29818	PASS
95	95	100	100	100.0	58541	PASS
96	95	5	9	6.8	3958	PASS
173	174	0.00	2	1.3	539	PASS
174	95	50	100	73.5	43040	PASS
175	174	5	9	7.8	3353	PASS
176	174	95	101	95.4	41069	PASS
177	176	5	9	7.1	2910	PASS