

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040422\
 Data File : VX027954.D
 Acq On : 04 Apr 2022 13:52
 Operator : JC/MD
 Sample : N2249-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Apr 05 05:48:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 04:39:27 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	97442	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	154840	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	132270	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	58398	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	51108	40.650	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	81.300%
35) Dibromofluoromethane	5.379	113	50538	50.566	ug/l	-0.01
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.140%
50) Toluene-d8	8.647	98	174551	49.637	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.280%
62) 4-Bromofluorobenzene	11.079	95	75348	50.420	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	100.840%
Target Compounds						
					Qvalue	
3) Chloromethane	1.270	50	338	0.433	ug/l #	42
9) 1,1,2-Trichlorotrifluo...	2.331	101	389	0.426	ug/l	92
10) Methyl Iodide	2.459	142	250	0.236	ug/l #	81
11) Tert butyl alcohol	2.952	59	3428	14.194	ug/l	97
12) 1,1-Dichloroethene	2.318	96	197	0.235	ug/l #	68
13) Acrolein	2.221	56	242	1.338	ug/l #	1
14) Allyl chloride	2.776	41	6575	4.278	ug/l #	67
15) Acrylonitrile	3.111	53	496	0.875	ug/l #	27
16) Acetone	2.337	43	2250	4.044	ug/l #	39
18) Methyl Acetate	2.782	43	14098	10.278	ug/l #	46
19) Methyl tert-butyl Ether	3.111	73	20361	6.384	ug/l #	53
22) Diisopropyl ether	3.757	45	1146	0.372	ug/l #	75
23) Vinyl Acetate	3.769	43	675	0.254	ug/l #	66
25) 2-Butanone	4.446	43	170	0.210	ug/l #	44
29) Tetrahydrofuran	5.019	42	278	0.535	ug/l #	32
30) Chloroform	5.092	83	661	0.343	ug/l	84
31) Cyclohexane	5.476	56	800	0.576	ug/l #	64
36) 1,1-Dichloropropene	5.550	75	7677	6.099	ug/l #	48
38) Carbon Tetrachloride	5.550	117	10630	7.643	ug/l #	15
40) Benzene	6.037	78	21123	5.537	ug/l	100
43) Isopropyl Acetate	6.232	43	6081	2.433	ug/l #	56
44) Trichloroethene	7.129	130	1677	1.618	ug/l	83
51) 4-Methyl-2-Pentanone	8.647	43	870	0.502	ug/l #	1
56) Ethyl methacrylate	8.836	69	818	0.485	ug/l #	8
59) 2-Hexanone	9.555	43	342	0.256	ug/l	70
60) Dibromochloromethane	9.281	129	305	0.276	ug/l #	9
64) Tetrachloroethene	9.268	164	240	0.268	ug/l #	73
67) Ethyl Benzene	10.195	91	2457	0.520	ug/l #	82
68) m/p-Xylenes	10.299	106	1371	0.789	ug/l	90
69) o-Xylene	10.646	106	519	0.306	ug/l	99
76) 1,2,3-Trichloropropane	11.079	75	41619	30.381	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	41619	88.448	ug/l #	15
84) 1,2,4-Trimethylbenzene	11.756	105	1159	0.308	ug/l	88
90) Hexachloroethane	12.640	117	706	1.174	ug/l #	10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040422\
Data File : VX027954.D
Acq On : 04 Apr 2022 13:52
Operator : JC/MD
Sample : N2249-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 05 05:48:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040422\
Data File : VX027954.D
Acq On : 04 Apr 2022 13:52
Operator : JC/MD
Sample : N2249-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Apr 05 05:48:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032922W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 04:39:27 2022
Response via : Initial Calibration

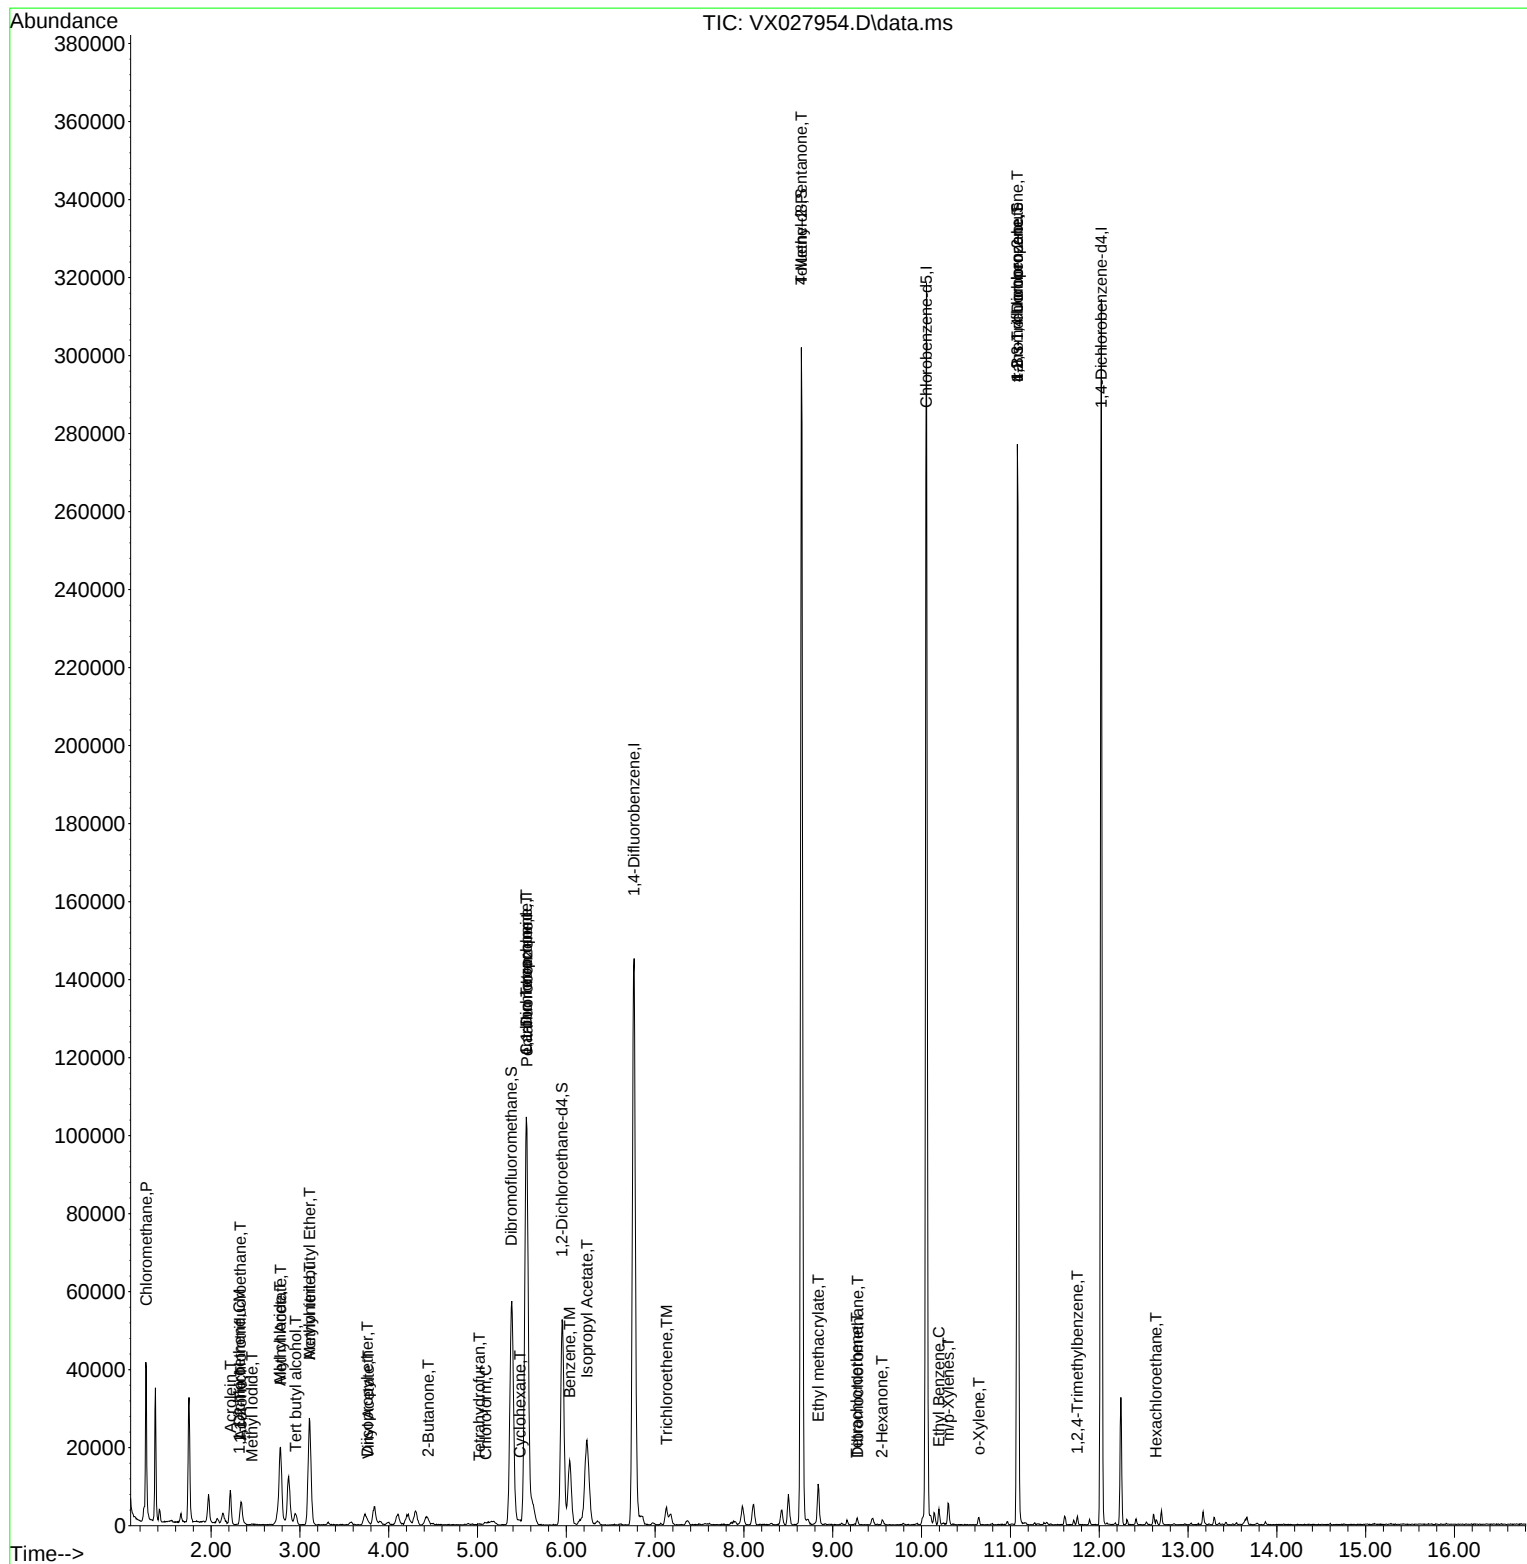




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :

MSVOA_X

ClientSampleId :







Tgt Ion:168 Resp: 97442
Ion Ratio Lower Upper
168 100
99 58.7 41.7 62.5

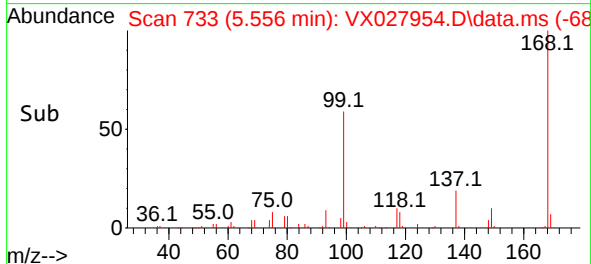

#3
Chloromethane
Concen: 0.433 ug/l
RT: 1.270 min Scan# 30
Delta R.T. -0.024 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 50 Resp: 338
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#


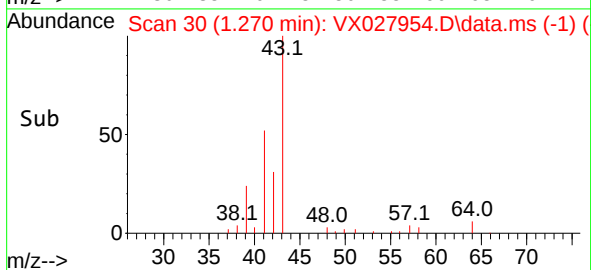

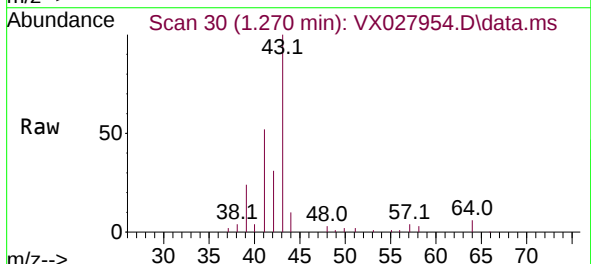




#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.426 ug/l
RT: 2.331 min Scan# 204
Delta R.T. -0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:101	Resp:	389
Ion	Ratio	Lower Upper
101	100	
85	50.1	33.5 50.3
151	73.3	61.8 92.6

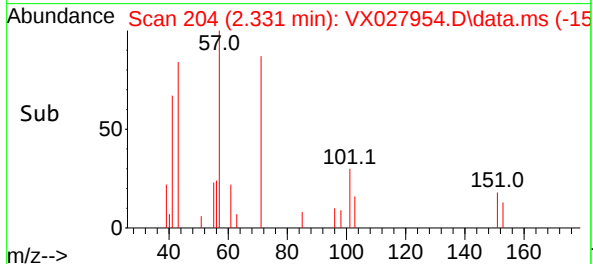

#10
Methyl Iodide
Concen: 0.236 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion:142	Resp:	250
Ion	Ratio	Lower Upper
142	100	
127	34.0	33.9 50.9
141	0.0	11.4 17.2#


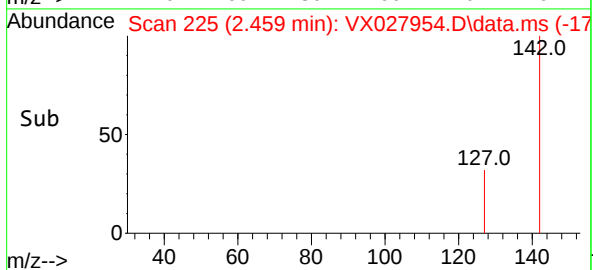

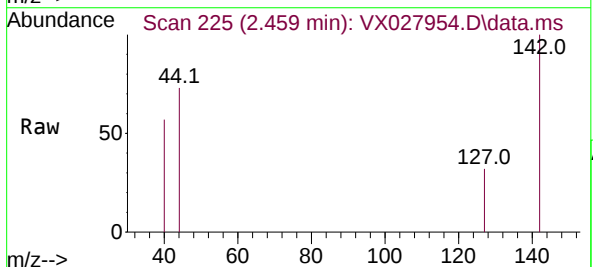




#11
Tert butyl alcohol
Concen: 14.194 ug/l
RT: 2.952 min Scan# 308
Delta R.T. -0.013 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 59 Resp: 3428
Ion Ratio Lower Upper
59 100
57 9.3 8.3 12.5

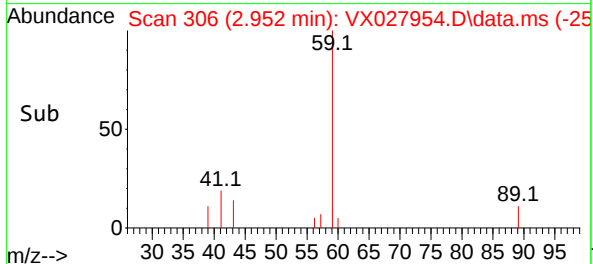

#12
1,1-Dichloroethene
Concen: 0.235 ug/l
RT: 2.318 min Scan# 202
Delta R.T. -0.001 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 96 Resp: 197
Ion Ratio Lower Upper
96 100
61 201.4 124.6 187.0#
98 81.8 51.0 76.4#

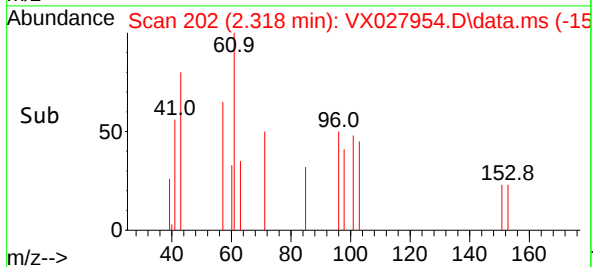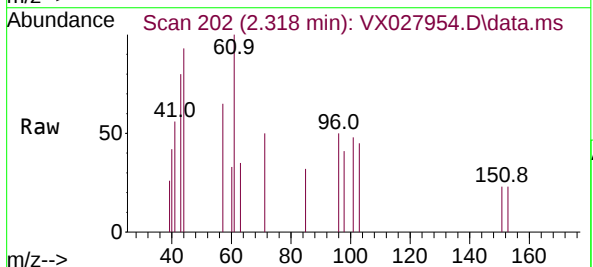



#13

Acrolein

Concen: 1.338 ug/l

RT: 2.221 min Scan# 186

Delta R.T. -0.012 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 242

Ion Ratio Lower Upper

56 100

55 1858.7 55.0 82.6#

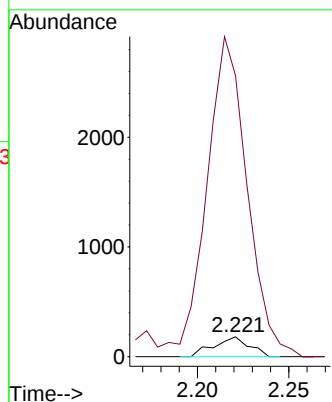

#14

Allyl chloride

Concen: 4.278 ug/l

RT: 2.776 min Scan# 277

Delta R.T. 0.110 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52




Tgt Ion: 41 Resp: 6575


Ion Ratio Lower Upper

41 100

39 54.3 50.4 75.6


76 0.0 32.7 49.1#

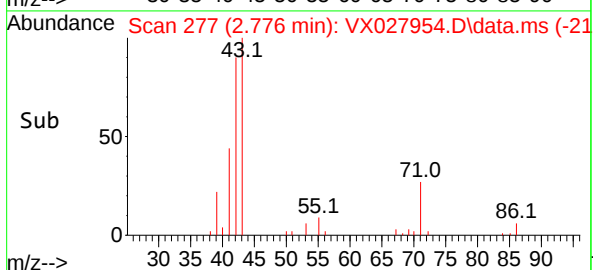






#15
Acrylonitrile
Concen: 0.875 ug/l
RT: 3.111 min Scan# 31
Delta R.T. 0.049 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 496
Ion Ratio Lower Upper
53 100
52 4.6 65.7 98.5#
51 59.5 28.4 42.6#

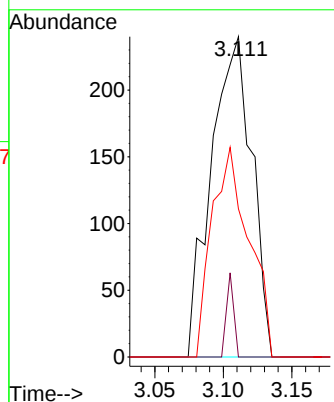

#16
Acetone
Concen: 4.044 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.043 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 43 Resp: 2250
Ion Ratio Lower Upper
43 100
58 0.0 28.8 43.2#


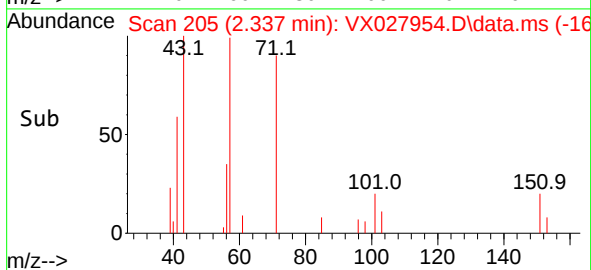
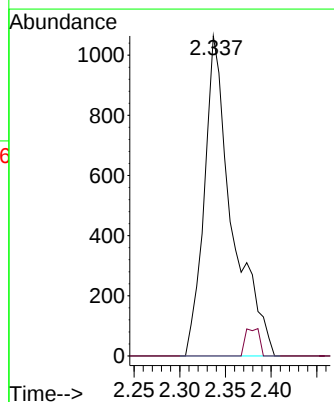
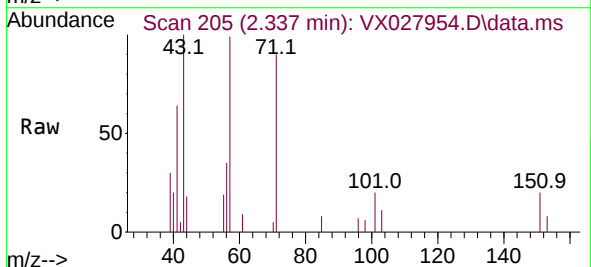




#18
Methyl Acetate
Concen: 10.278 ug/l
RT: 2.782 min Scan# 21
Delta R.T. 0.079 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 14098
Ion Ratio Lower Upper
43 100
74 0.0 22.8 34.2#

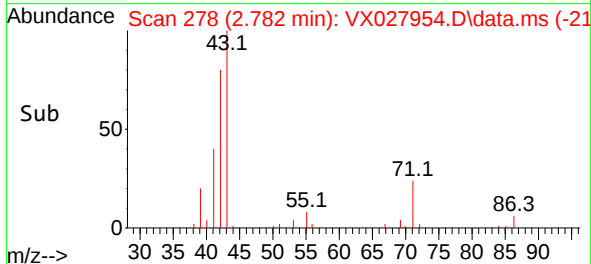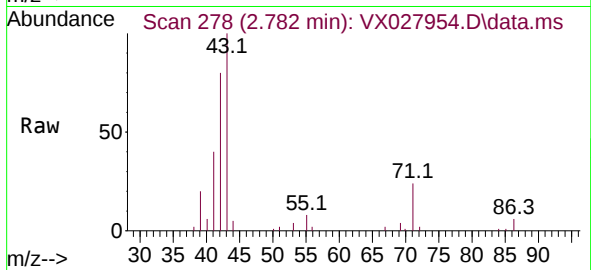

#19
Methyl tert-butyl Ether
Concen: 6.384 ug/l
RT: 3.111 min Scan# 332
Delta R.T. -0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 73 Resp: 20361
Ion Ratio Lower Upper
73 100
57 43.1 16.8 25.2#

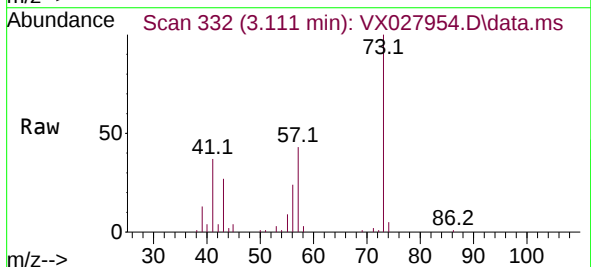



#22

Diisopropyl ether

Concen: 0.372 ug/l

RT: 3.757 min Scan# 41

Delta R.T. -0.006 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 45 Resp: 1146





Ion Ratio Lower Upper

45 100

43 41.1 50.8 76.2#

87 24.2 26.6 39.8#

59 0.0 10.5 15.7#

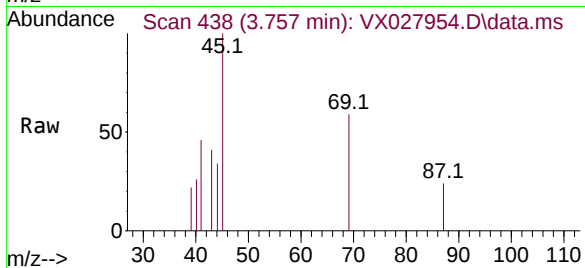

#23

Vinyl Acetate

Concen: 0.254 ug/l

RT: 3.769 min Scan# 440

Delta R.T. 0.042 min

Lab File: VX027954.D




Acq: 04 Apr 2022 13:52


Tgt Ion: 43 Resp: 675

Ion Ratio Lower Upper

43 100

86 0.0 10.8 16.2#


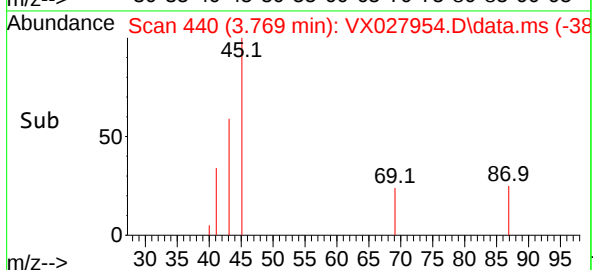

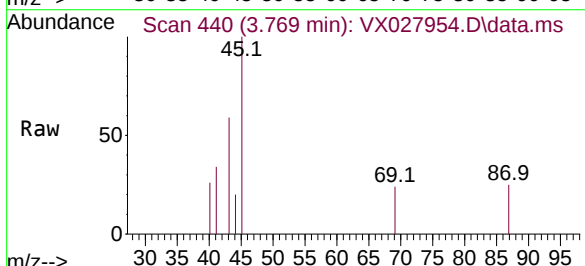




#25
2-Butanone
Concen: 0.210 ug/l
RT: 4.446 min Scan# 51
Delta R.T. -0.110 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 170
Ion Ratio Lower Upper
43 100
72 0.0 24.4 36.6#

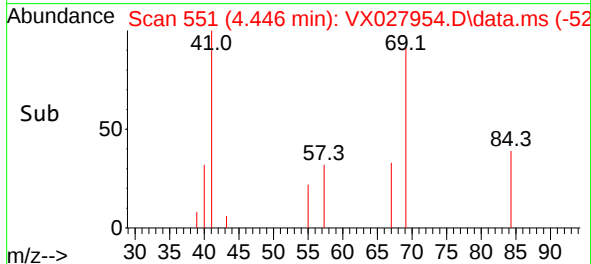

#29
Tetrahydrofuran
Concen: 0.535 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.012 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 42 Resp: 278
Ion Ratio Lower Upper
42 100
72 9.4 44.1 66.1#
71 0.0 40.5 60.7#

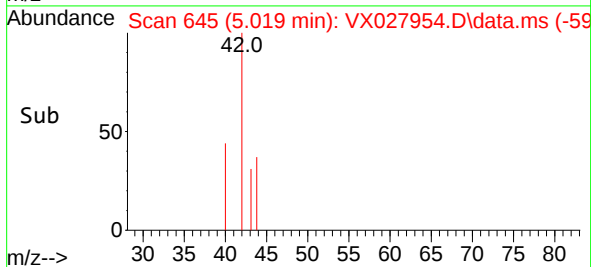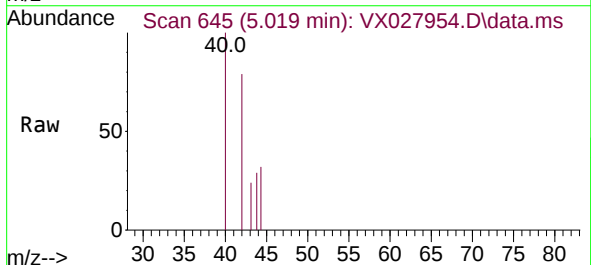



#30

Chloroform

Concen: 0.343 ug/l

RT: 5.092 min Scan# 6

Delta R.T. -0.007 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 83 Resp: 661

Ion Ratio Lower Upper

83 100

85 78.5 52.7 79.1

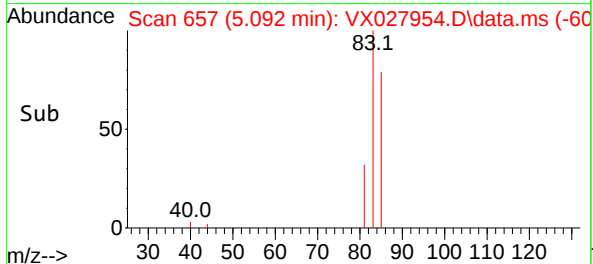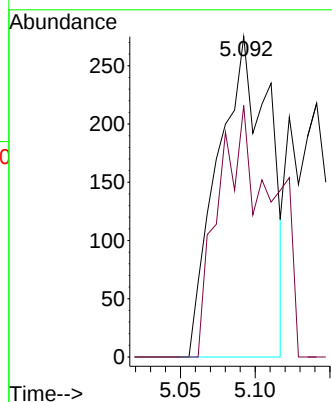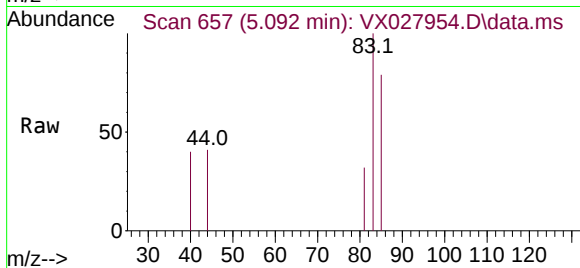

#31

Cyclohexane

Concen: 0.576 ug/l

RT: 5.476 min Scan# 720

Delta R.T. -0.001 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52




Tgt Ion: 56 Resp: 800


Ion Ratio Lower Upper

56 100

69 29.5 26.7 40.1

84 51.8 77.2 115.8#

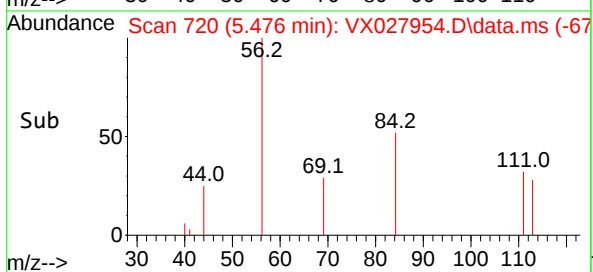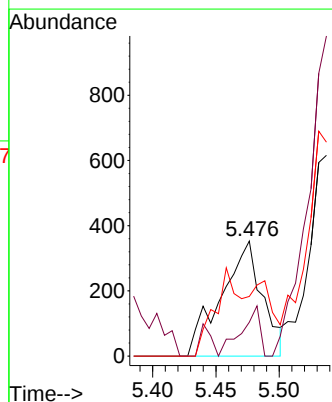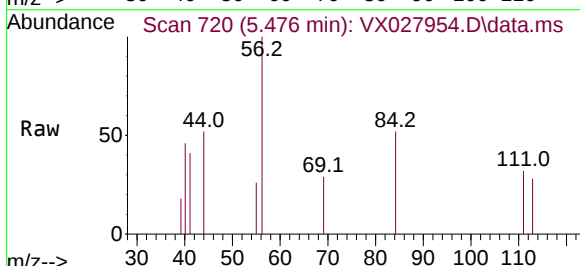



#33

1,2-Dichloroethane-d4

Concen: 40.650 ug/l

RT: 5.952 min Scan# 799

Delta R.T. -0.006 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 51108

Ion Ratio Lower Upper

65 100

67 51.8 0.0 107.4

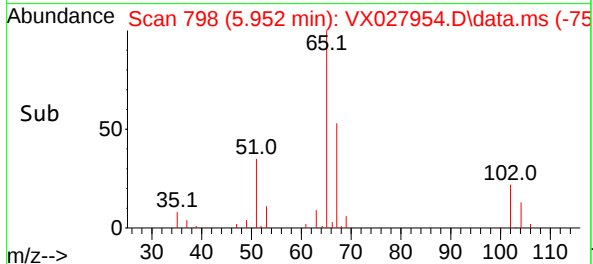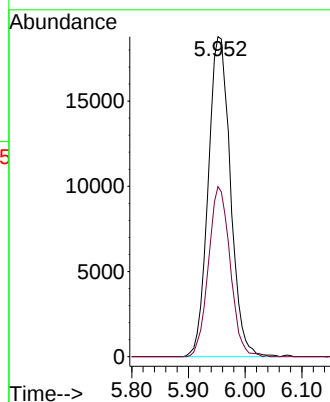

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52




Tgt Ion: 114 Resp: 154840


Ion Ratio Lower Upper

114 100

63 19.1 0.0 36.8


88 16.5 0.0 32.4

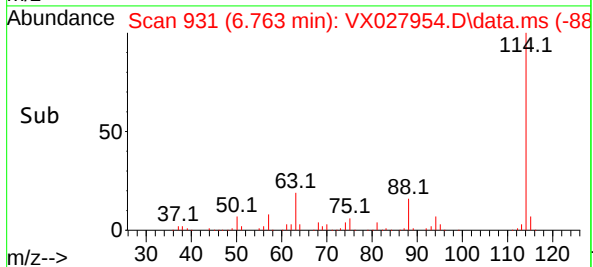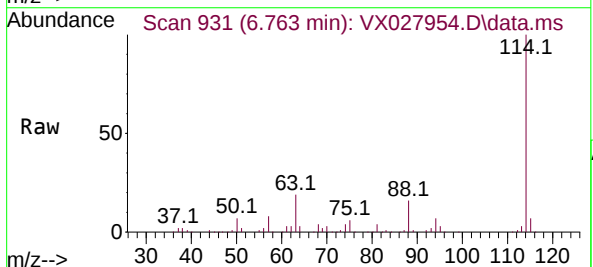






#35
Dibromofluoromethane
Concen: 50.566 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.012 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Instrument :
MSVOA_X
ClientSampleId :



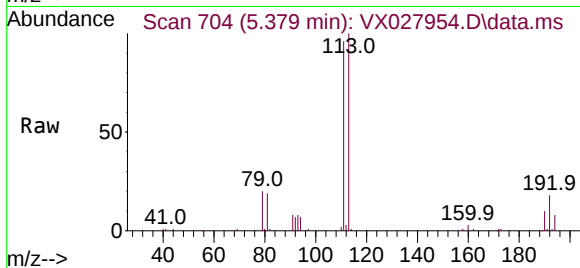



Tgt Ion:113 Resp: 50538
Ion Ratio Lower Upper
113 100
111 100.0 82.8 124.2
192 18.0 16.9 25.3

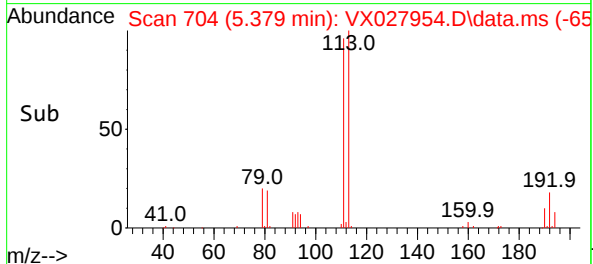

#36
1,1-Dichloropropene
Concen: 6.099 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52


Tgt Ion: 75 Resp: 7677
Ion Ratio Lower Upper
75 100
110 8.3 18.3 54.8#
77 0.0 24.8 37.2#

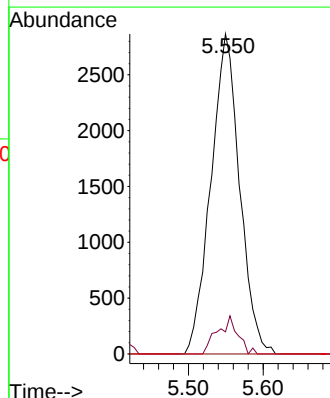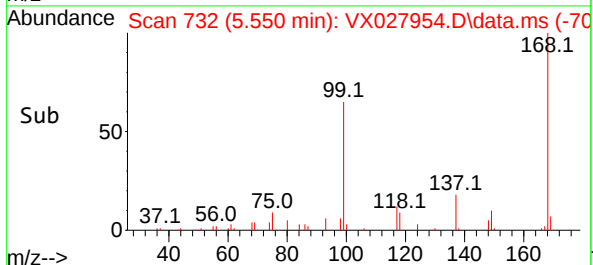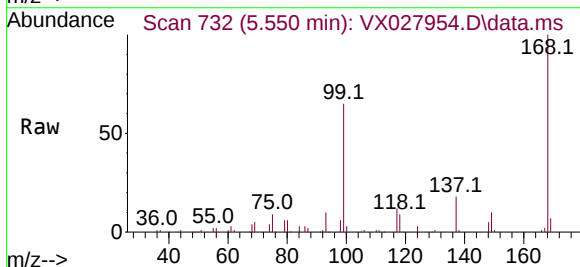






#38
Carbon Tetrachloride
Concen: 7.643 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 10630
Ion Ratio Lower Upper
117 100
119 4.1 77.3 115.9#
121 0.0 24.2 36.2#

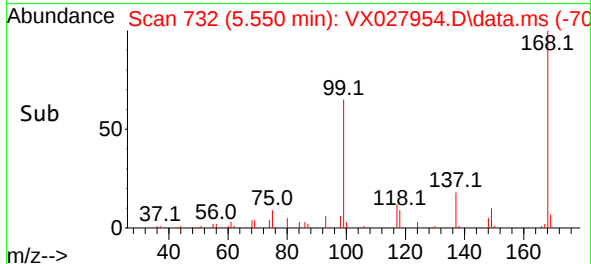

#40
Benzene
Concen: 5.537 ug/l
RT: 6.037 min Scan# 812
Delta R.T. 0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 78 Resp: 21123
Ion Ratio Lower Upper
78 100
77 23.9 19.3 28.9


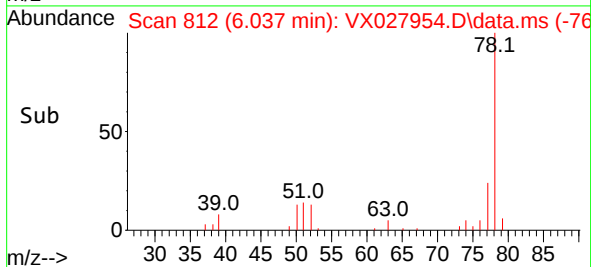

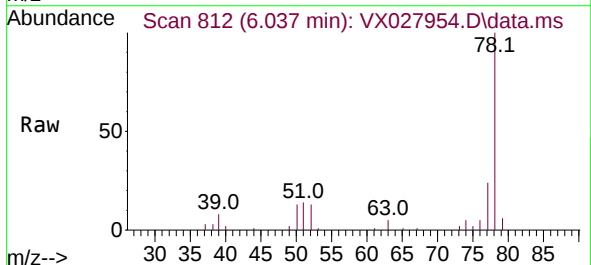




#43
Isopropyl Acetate
Concen: 2.433 ug/l
RT: 6.232 min Scan# 844
Delta R.T. -0.110 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 6081
Ion Ratio Lower Upper
43 100
61 0.0 18.5 27.7#
87 0.0 13.0 19.6#

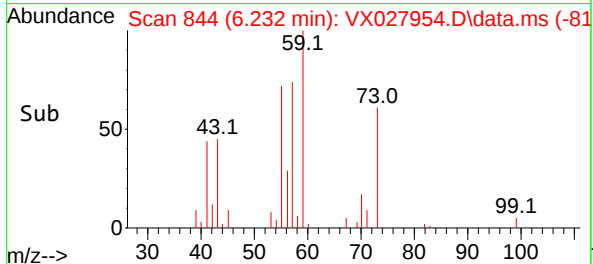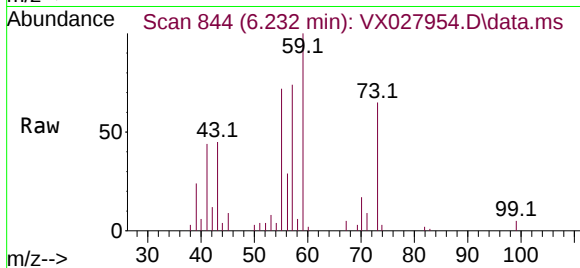

#44
Trichloroethene
Concen: 1.618 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion:130 Resp: 1677
Ion Ratio Lower Upper
130 100
95 110.6 0.0 188.8

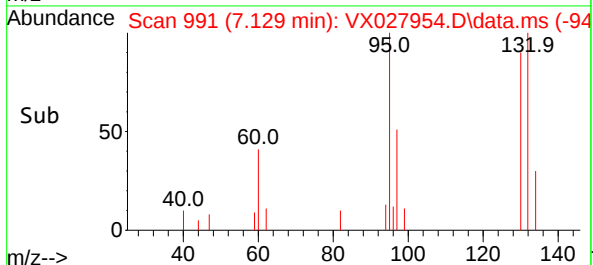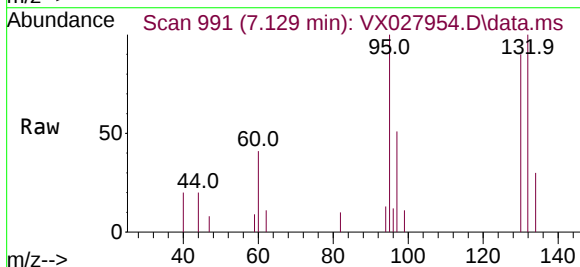



#50

Toluene-d8

Concen: 49.637 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.006 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 98 Resp: 174551

Ion Ratio Lower Upper

98 100

100 64.6 52.6 78.8



#51

4-Methyl-2-Pentanone

Concen: 0.502 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.073 min

Lab File: VX027954.D




Acq: 04 Apr 2022 13:52


Tgt Ion: 43 Resp: 870

Ion Ratio Lower Upper

43 100

58 178.3 36.1 54.1#


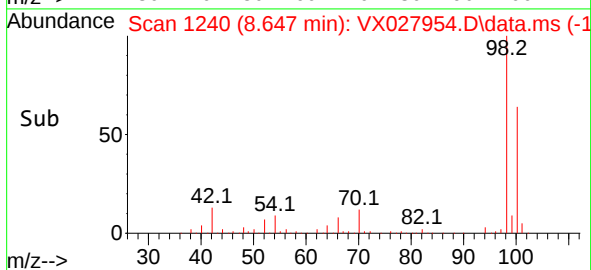

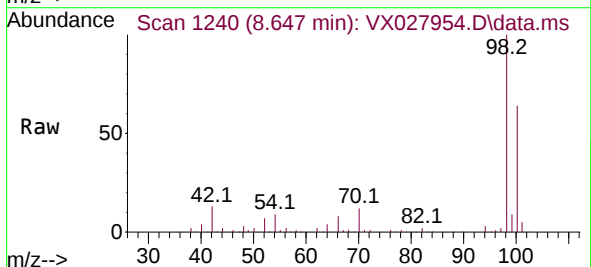




#56
Ethyl methacrylate
Concen: 0.485 ug/l
RT: 8.836 min Scan# 11
Delta R.T. -0.280 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 69 Resp: 818
Ion Ratio Lower Upper
69 100
41 134.8 43.8 65.6#
39 0.0 22.2 33.2#

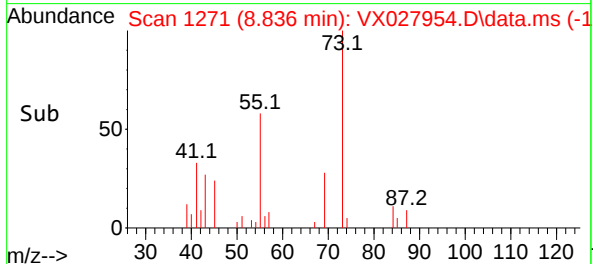

#59
2-Hexanone
Concen: 0.256 ug/l
RT: 9.555 min Scan# 1389
Delta R.T. 0.122 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52


Tgt Ion: 43 Resp: 342
Ion Ratio Lower Upper
43 100
58 40.6 31.9 95.7

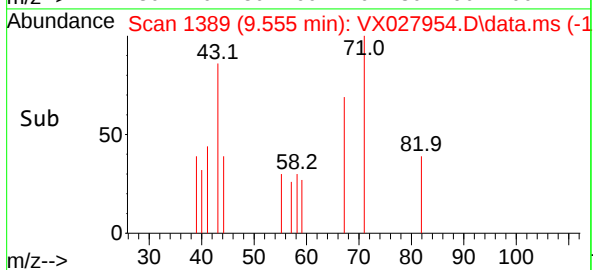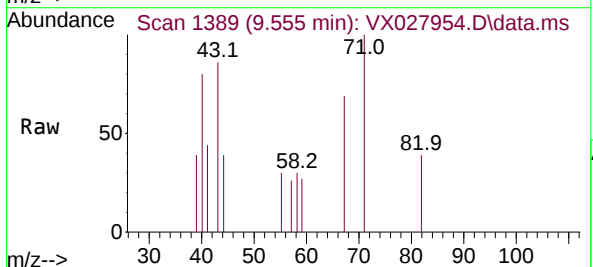






#60
Dibromochloromethane
Concen: 0.276 ug/l
RT: 9.281 min Scan# 11
Delta R.T. -0.244 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion:129 Resp: 305
Ion Ratio Lower Upper
129 100
127 0.0 40.3 120.8#

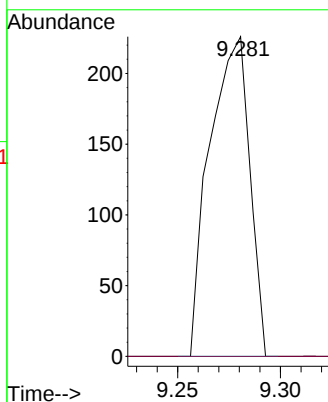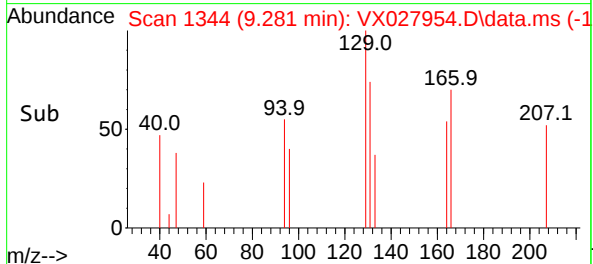


#62
4-Bromofluorobenzene
Concen: 50.420 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52



Tgt Ion: 95 Resp: 75348
Ion Ratio Lower Upper
95 100
174 70.2 0.0 163.0
176 67.0 0.0 155.0



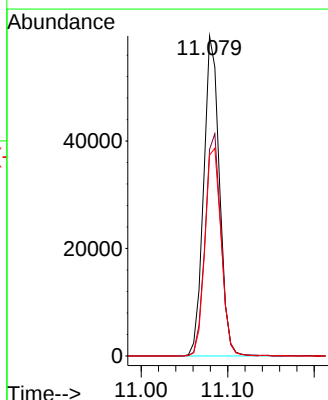
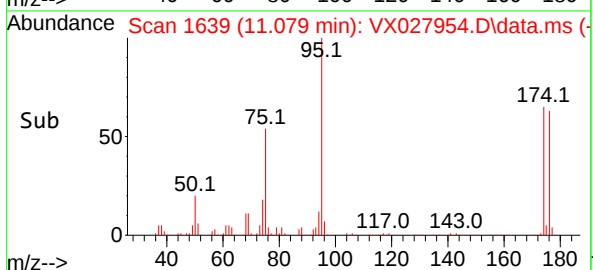




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 132270
Ion Ratio Lower Upper
117 100
82 59.6 41.8 62.8
119 32.4 24.8 37.2

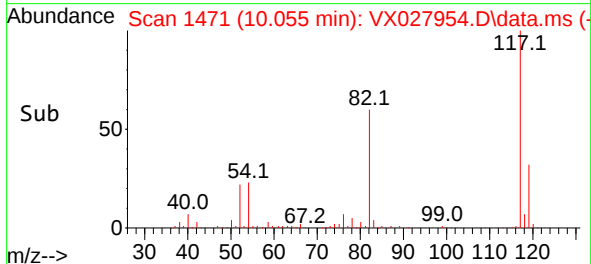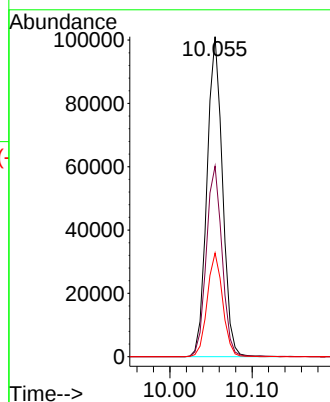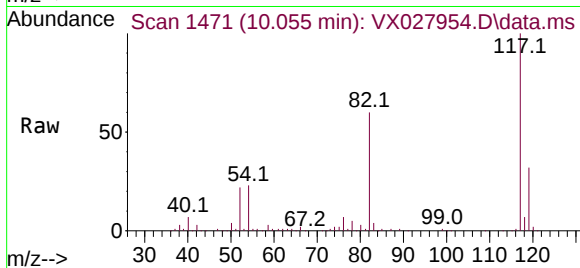

#64
Tetrachloroethene
Concen: 0.268 ug/l
RT: 9.268 min Scan# 1342
Delta R.T. -0.007 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion:164 Resp: 240
Ion Ratio Lower Upper
164 100
166 163.8 101.2 151.8#
129 130.8 73.0 109.4#
131 98.5 74.2 111.2

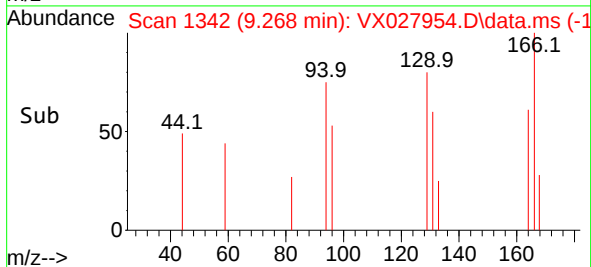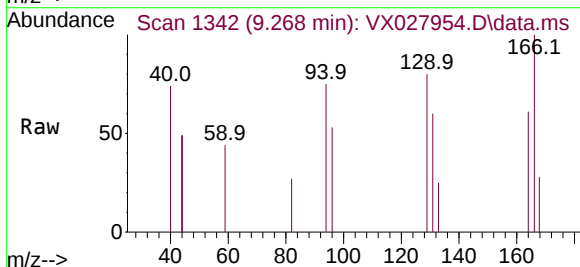



#67

Ethyl Benzene

Concen: 0.520 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 2457

Ion Ratio Lower Upper

91 100

106 21.1 24.6 36.8#



#68

m/p-Xylenes

Concen: 0.789 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.006 min

Lab File: VX027954.D




Acq: 04 Apr 2022 13:52


Tgt Ion: 106 Resp: 1371

Ion Ratio Lower Upper

106 100

91 216.2 160.4 240.6


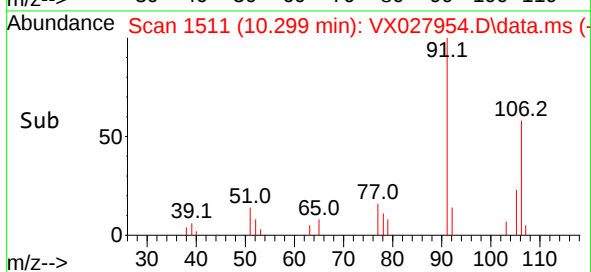






#69
o-Xylene
Concen: 0.306 ug/l
RT: 10.646 min Scan# 1567
Delta R.T. 0.006 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:106 Resp: 519
Ion Ratio Lower Upper
106 100
91 214.5 106.1 318.1

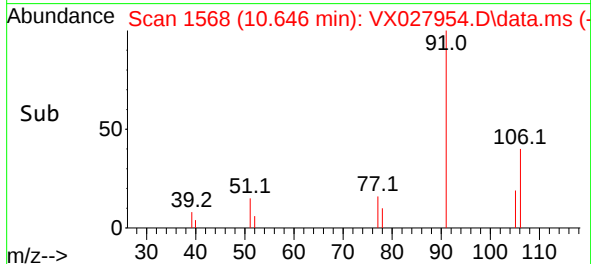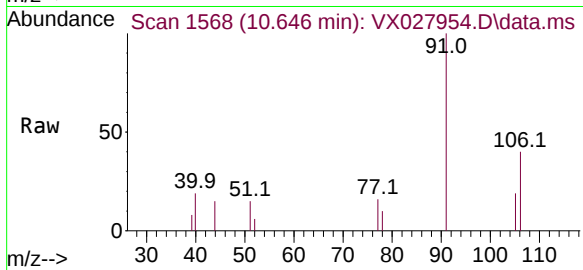

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion:152 Resp: 58398
Ion Ratio Lower Upper
152 100
115 65.0 37.5 112.7
150 159.4 0.0 338.2


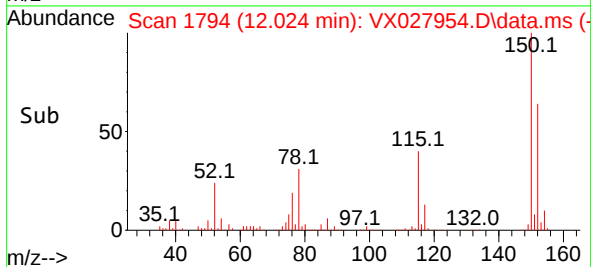

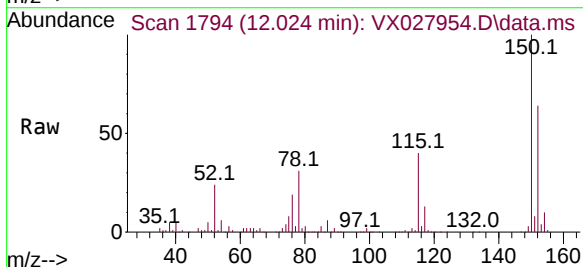




#76
1,2,3-Trichloropropane
Concen: 30.381 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 41619
Ion Ratio Lower Upper
75 100
77 1.1 19.4 58.2#

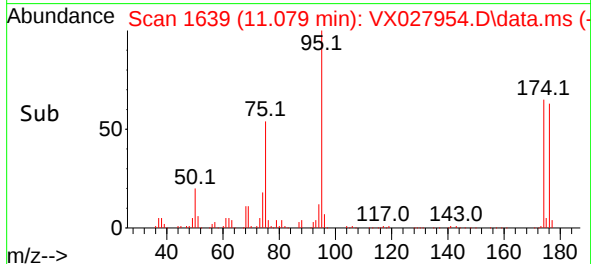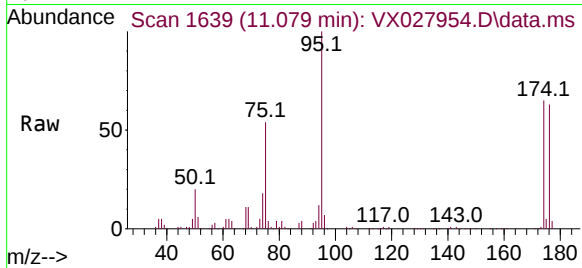

#81
trans-1,4-Dichloro-2-butene
Concen: 88.448 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX027954.D
Acq: 04 Apr 2022 13:52

Tgt Ion: 75 Resp: 41619
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#

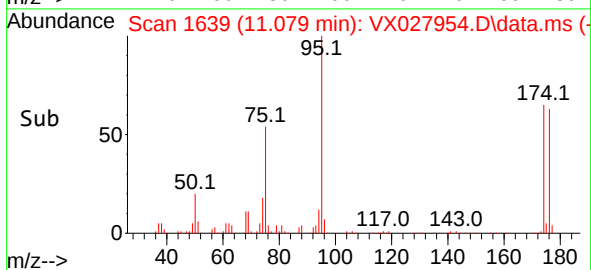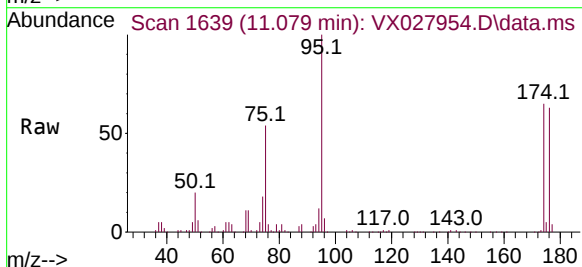



#84

1,2,4-Trimethylbenzene

Concen: 0.308 ug/l

RT: 11.756 min Scan# 1159

Delta R.T. -0.000 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 1159

Ion Ratio Lower Upper

105 100

120 37.4 22.6 67.8

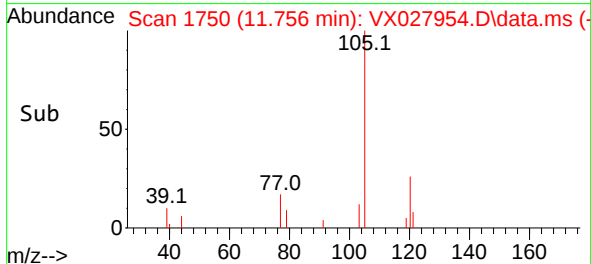

#90

Hexachloroethane

Concen: 1.174 ug/l

RT: 12.640 min Scan# 1895

Delta R.T. 0.098 min

Lab File: VX027954.D

Acq: 04 Apr 2022 13:52

Tgt Ion:117 Resp: 706

Ion Ratio Lower Upper

117 100

201 0.0 39.5 118.5#

