

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX040519\
 Data File : VX008706.D
 Acq On : 06 Apr 2019 00:45
 Operator : JC/SP
 Sample : K2296-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0702

Quant Time: Apr 06 01:31:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	209578	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	348986	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	305072	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	129377	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.06	65	143495	46.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.88%	
35) Dibromofluoromethane	5.50	113	105068	47.09	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.18%	
50) Toluene-d8	8.71	98	441234	49.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.32%	
62) 4-Bromofluorobenzene	11.13	95	149366	47.41	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.82%	

Target Compounds


					Qvalue	
3) Chloromethane	1.32	50	556	Below Cal	#	69
4) Vinyl Chloride	1.40	62	3748	1.149	ug/l	90
5) Bromomethane	1.64	94	293	2.061	ug/l #	74
6) Chloroethane	1.62	64	4218	Below Cal	#	73
11) Tert butyl alcohol	3.03	59	3245	4.534	ug/l #	94
13) Acrolein	2.31	56	127	0.358	ug/l #	13
14) Allyl chloride	2.84	41	4700	0.847	ug/l #	72
15) Acrylonitrile	3.17	53	549	0.290	ug/l #	33
16) Acetone	2.44	43	4809	2.731	ug/l	98
17) Carbon Disulfide	2.57	76	518	Below Cal	#	75
18) Methyl Acetate	2.84	43	11797	2.763	ug/l #	56
27) cis-1,2-Dichloroethene	4.60	96	97368	32.314	ug/l	89
28) Bromochloromethane	5.01	49	22	Below Cal	#	22
31) Cyclohexane	5.58	56	15854	3.002	ug/l	97
36) 1,1-Dichloropropene	5.66	75	16739	4.388	ug/l #	51
38) Carbon Tetrachloride	5.66	117	20226	6.406	ug/l #	17
39) Methylcyclohexane	7.46	83	2478	0.526	ug/l	93
40) Benzene	6.14	78	29822	2.624	ug/l	97
55) 1,1,2-Trichloroethane	9.16	97	885	0.329	ug/l #	20
65) Chlorobenzene	10.14	112	3619	0.535	ug/l	100
76) 1,2,3-Trichloropropane	11.13	75	76085	21.408	ug/l #	34
81) trans-1,4-Dichloro-2-buten	11.13	75	76085	59.011	ug/l #	9
85) sec-Butylbenzene	11.94	105	3262	0.317	ug/l	92
90) Hexachloroethane	12.75	117	1059	0.692	ug/l #	9
91) 1,2-Dichlorobenzene	12.39	146	1478	0.323	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040519\
Data File : VX008706.D
Acq On : 06 Apr 2019 00:45
Operator : JC/SP
Sample : K2296-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S8-0702

Quant Time: Apr 06 01:31:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

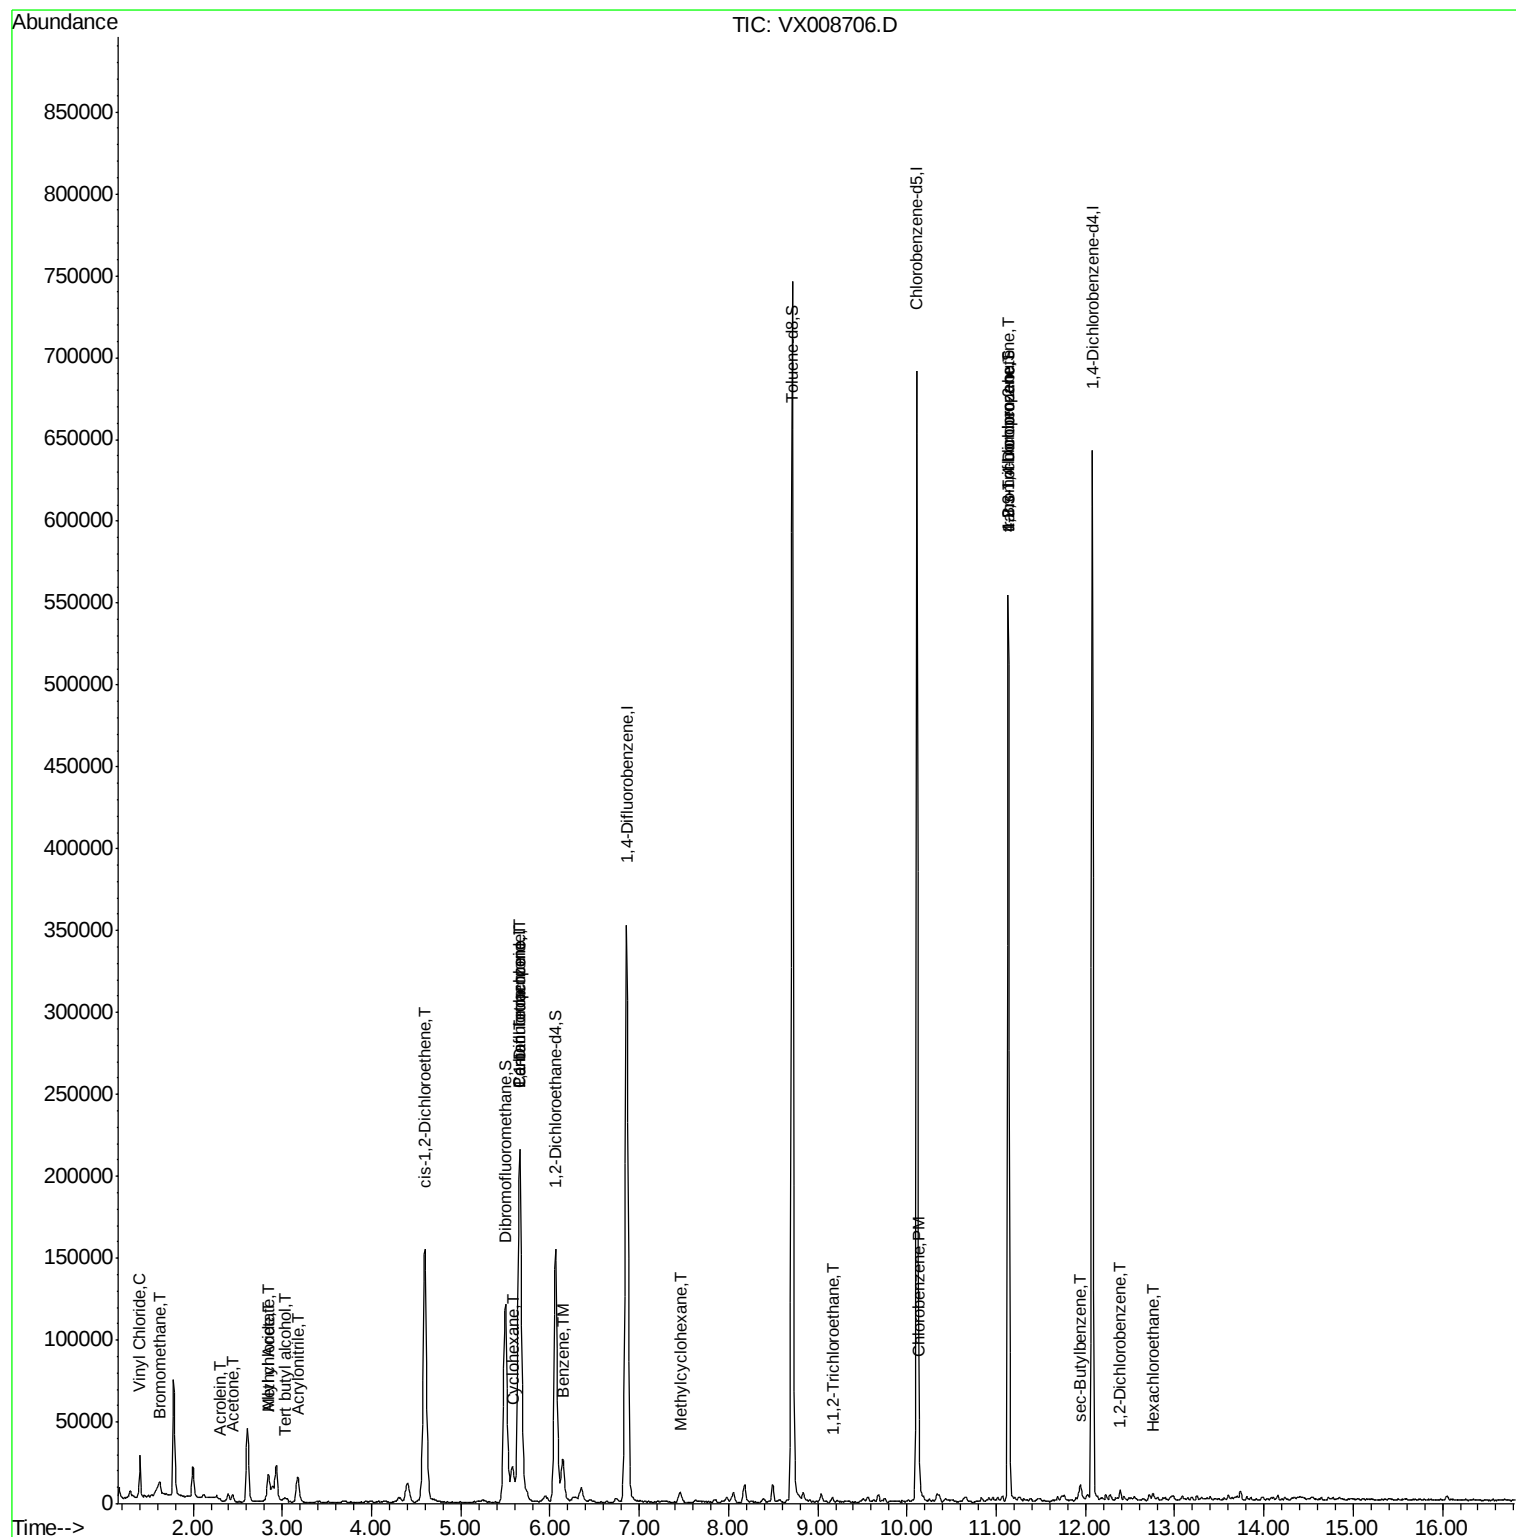



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :


S8-0702

Tot Ion:168 Resp: 209578

Ion Ratio Lower Upper

168 100

99 57.5 46.7 70.1

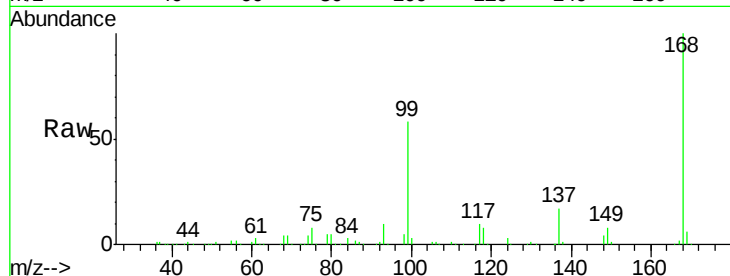

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#3

Chloromethane

Concen: Below Cal

RT: 1.32 min Scan# 28

Delta R.T. 0.00 min

Lab File: VX008706.D


Acq: 06 Apr 2019 00:45

Tgt Ion: 50 Resp: 556

Ion Ratio Lower Upper

50 100

52 49.8 25.8 38.8#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.32

500

400


300


200

100

0

Time--> 1.30 1.35



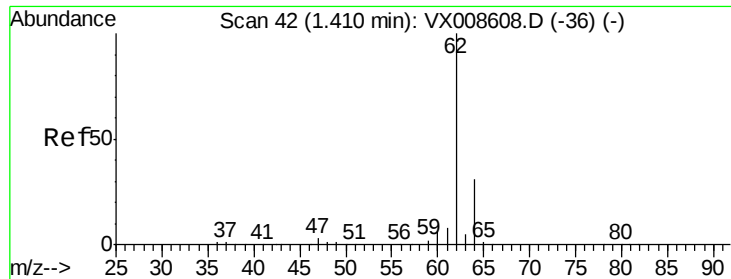

#4

Vinyl Chloride

Concen: 1.149 ug/l

RT: 1.40 min Scan# 41

Delta R.T. -0.01 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampled :


S8-0702

Tot Ion: 62 Resp: 3748

Ion Ratio Lower Upper




62 100

64 36.5 24.7 37.1

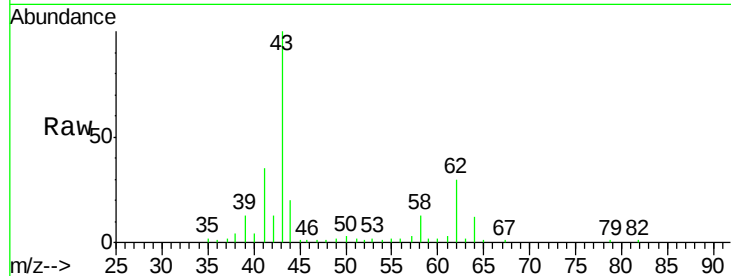

Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

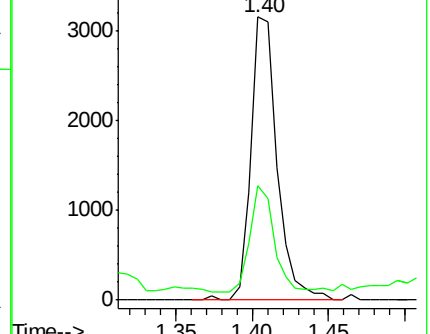

#5

Bromomethane

Concen: 2.061 ug/l

RT: 1.64 min Scan# 79

Delta R.T. 0.00 min

Lab File: VX008706.D


Acq: 06 Apr 2019 00:45

Tgt Ion: 94 Resp: 293

Ion Ratio Lower Upper



94 100


96 68.8 75.2 112.8#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

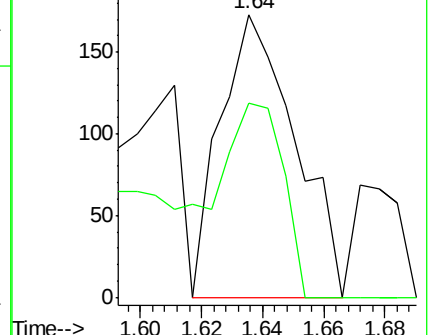

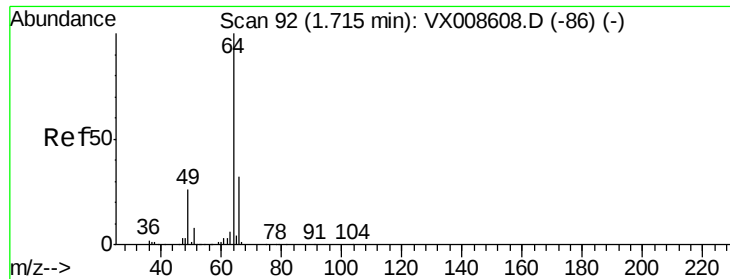

#6

Chloroethane

Concen: Below Cal

RT: 1.62 min Scan# 76

Delta R.T. -0.10 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampled :





S8-0702

Tot Ion: 64 Resp: 4218

Ion Ratio Lower Upper

64 100

66 16.5 25.4 38.0#

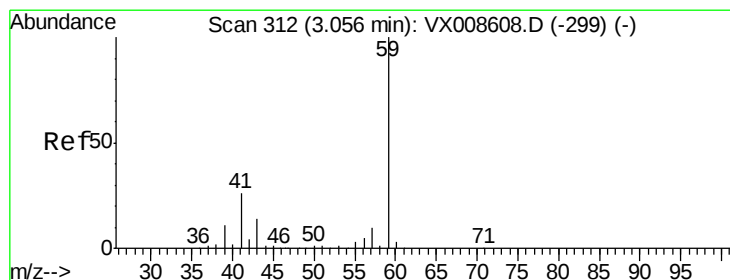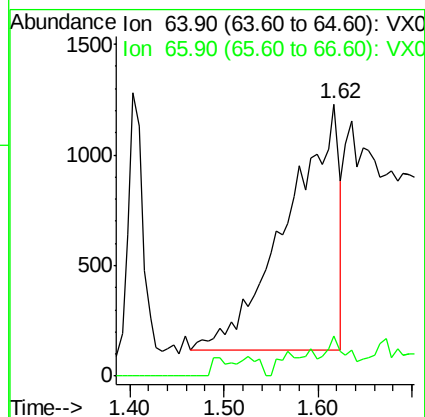

#11

Tert butyl alcohol

Concen: 4.534 ug/l

RT: 3.03 min Scan# 308

Delta R.T. -0.02 min

Lab File: VX008706.D




Acq: 06 Apr 2019 00:45


Tgt Ion: 59 Resp: 3245

Ion Ratio Lower Upper

59 100

57 12.6 8.3 12.5#

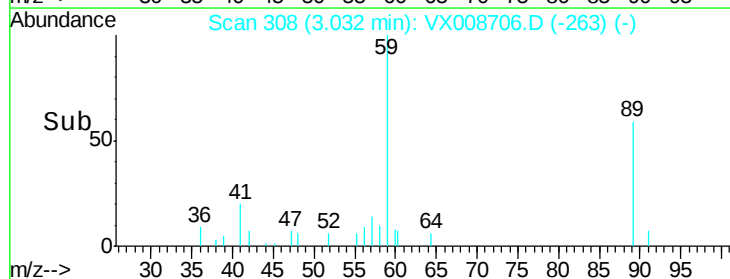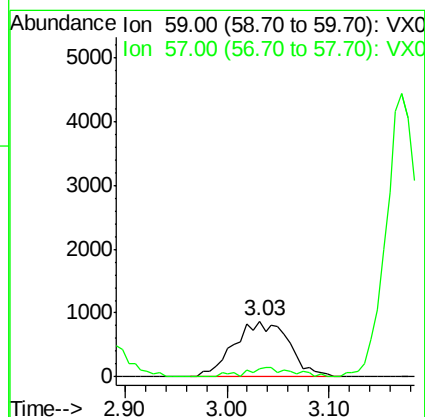

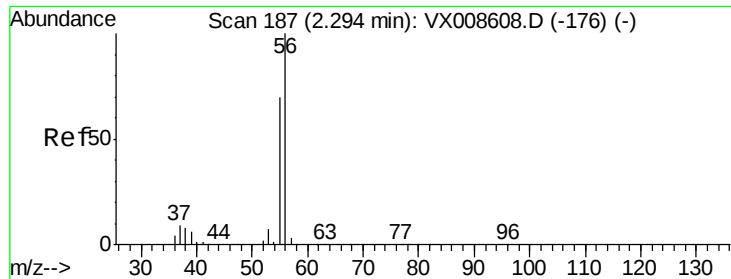

#13

Acrolein

Concen: 0.358 ug/l

RT: 2.31 min Scan# 189

Delta R.T. 0.01 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampled :


S8-0702

Tot Ion: 56 Resp: 127

Ion Ratio Lower Upper


56 100

55 0.0 58.0 87.0#


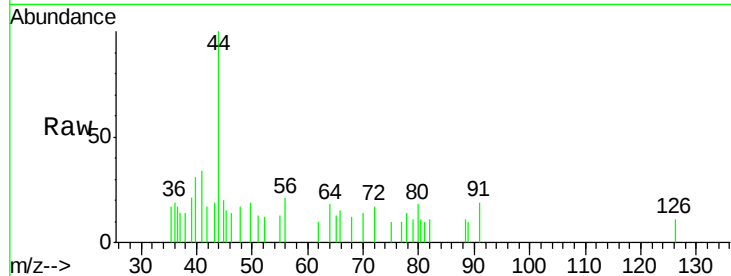


Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

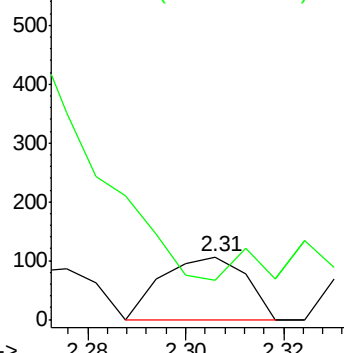

Time-->



#14

Allyl chloride

Concen: 0.847 ug/l

RT: 2.84 min Scan# 277

Delta R.T. 0.12 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45


Tgt Ion: 41 Resp: 4700

Ion Ratio Lower Upper

41 100

39 47.1 48.0 72.0#


76 0.0 22.0 33.0#




Abundance Ion 41.00 (40.70 to 41.70): VX0


Ion 39.00 (38.70 to 39.70): VX0

Ion 75.90 (75.60 to 76.60): VX0

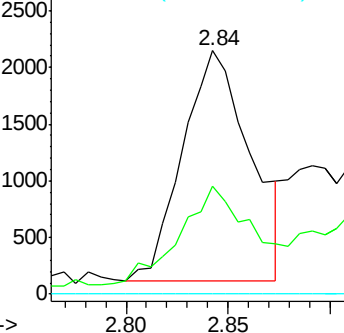

Time-->





#15

Acrylonitrile

Concen: 0.290 ug/l

RT: 3.17 min Scan# 330

Delta R.T. 0.02 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampled :

S8-0702


Tot Ion: 53 Resp: 549

Ion Ratio Lower Upper

53 100

52 0.0 66.5 99.7#




51 40.3 28.6 42.8

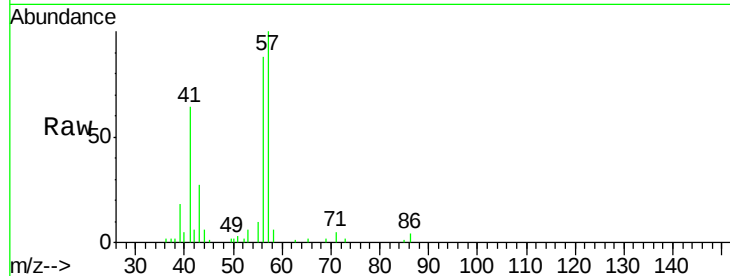

Abundance Ion 53.00 (52.70 to 53.70): VX0

Ion 52.00 (51.70 to 52.70): VX0

Ion 51.00 (50.70 to 51.70): VX0

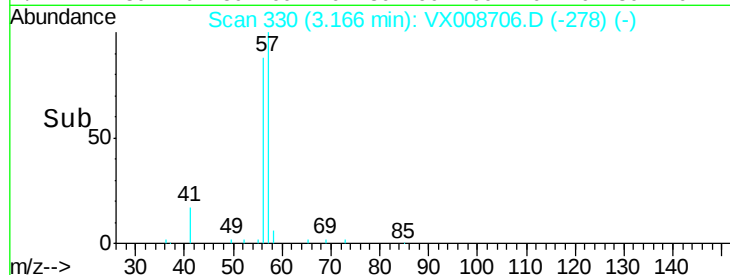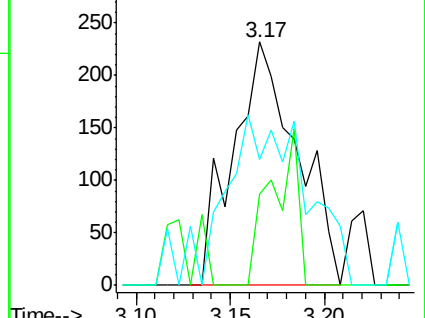

#16

Acetone

Concen: 2.731 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX008706.D


Acq: 06 Apr 2019 00:45

Tgt Ion: 43 Resp: 4809

Ion Ratio Lower Upper



43 100


58 30.0 24.8 37.2



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

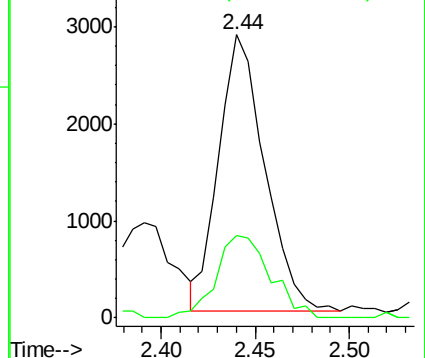

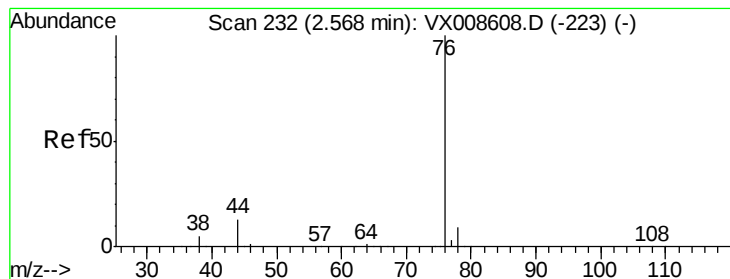

#17

Carbon Disulfide

Concen: Below Cal

RT: 2.57 min Scan# 232

Delta R.T. 0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :


S8-0702

Tot Ion: 76 Resp: 518

Ion Ratio Lower Upper




76 100

78 0.0 7.1 10.7#



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

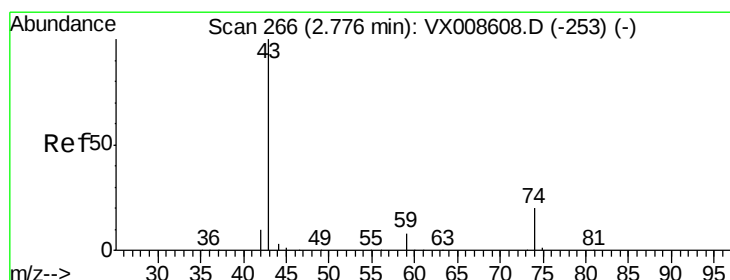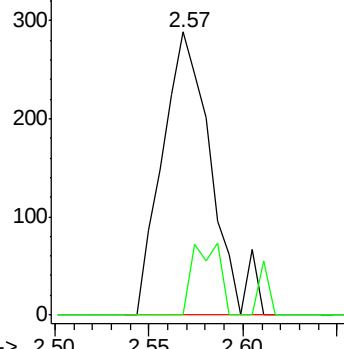

#18

Methyl Acetate

Concen: 2.763 ug/l

RT: 2.84 min Scan# 277

Delta R.T. 0.07 min

Lab File: VX008706.D


Acq: 06 Apr 2019 00:45

Tgt Ion: 43 Resp: 11797

Ion Ratio Lower Upper



43 100


74 0.2 16.5 24.7#

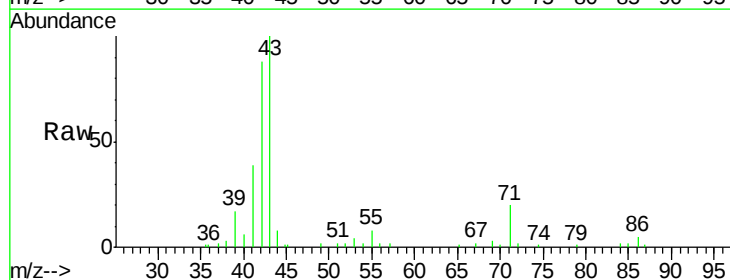

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 74.00 (73.70 to 74.70): VX0

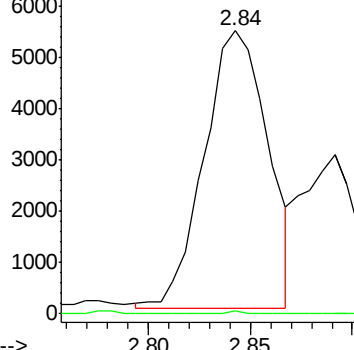

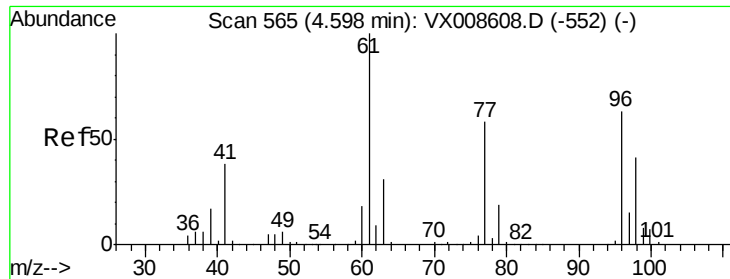


#27




cis-1,2-Dichloroethene
 Concen: 32.314 ug/l
 RT: 4.60 min Scan# 565
 Delta R.T. -0.00 min
 Lab File: VX008706.D
 Acq: 06 Apr 2019 00:45

Instrument :
 MSVOA_X
 ClientSampled :
 S8-0702

Tot Ion	96	Resp	97368
Ion	Ratio	Lower	Upper
96	100		
61	143.8	0.0	327.6
98	63.8	0.0	128.6

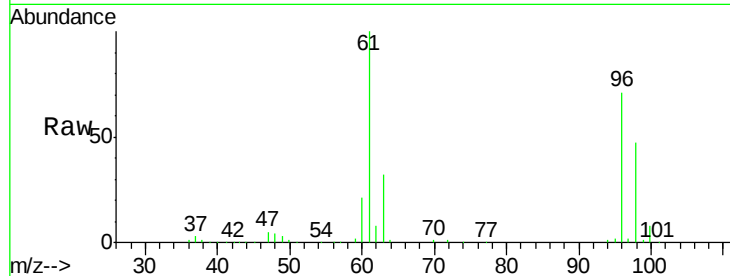


Abundance Ion 95.90 (95.60 to 96.60): VX0
 Ion 60.90 (60.60 to 61.60): VX0
 Ion 97.90 (97.60 to 98.60): VX0

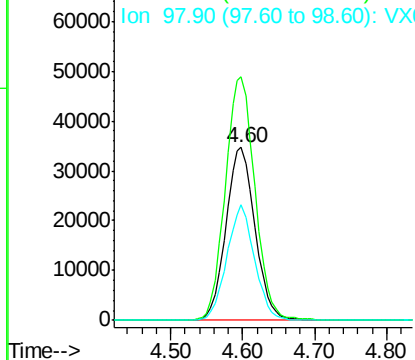



#28


Bromochloromethane
 Concen: Below Cal
 RT: 5.01 min Scan# 633
 Delta R.T. -0.01 min
 Lab File: VX008706.D
 Acq: 06 Apr 2019 00:45

Tgt Ion	49	Resp	22
Ion	Ratio	Lower	Upper
49	100		
129	0.0	0.0	3.6
130	0.0	49.3	73.9#



Abundance Ion 48.90 (48.60 to 49.60): VX0
 Ion 128.80 (128.50 to 129.50): V
 Ion 129.80 (129.50 to 130.50): V

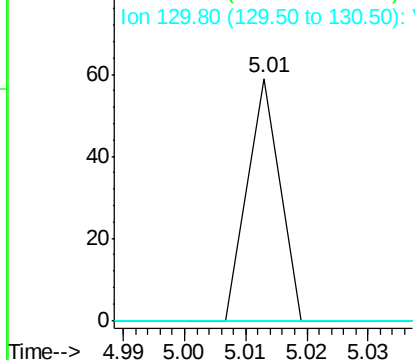

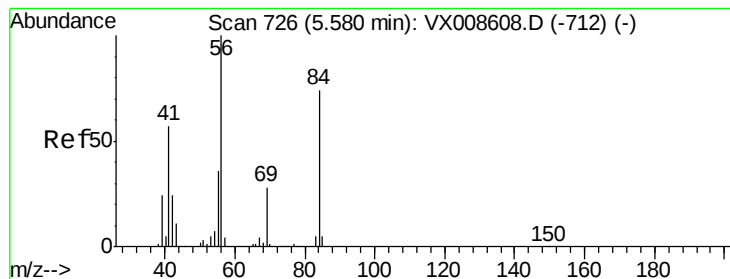

#31

Cyclohexane

Concen: 3.002 ug/l

RT: 5.58 min Scan# 726

Delta R.T. -0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :

S8-0702


Tot Ion: 56 Resp: 15854

Ion Ratio Lower Upper

56 100

69 28.2 22.6 33.8




84 70.2 59.3 88.9



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 84.00 (83.70 to 84.70): VX0

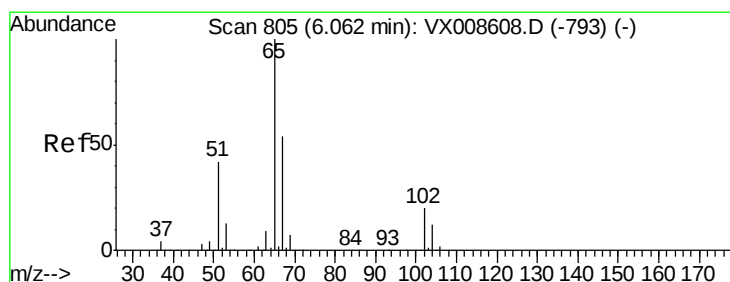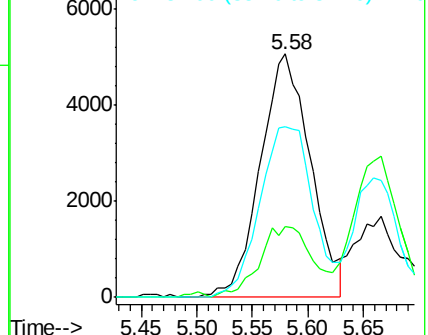

#33

1,2-Dichloroethane-d4

Concen: 46.943 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008706.D


Acq: 06 Apr 2019 00:45

Tgt Ion: 65 Resp: 143495

Ion Ratio Lower Upper



65 100


67 54.5 0.0 107.2

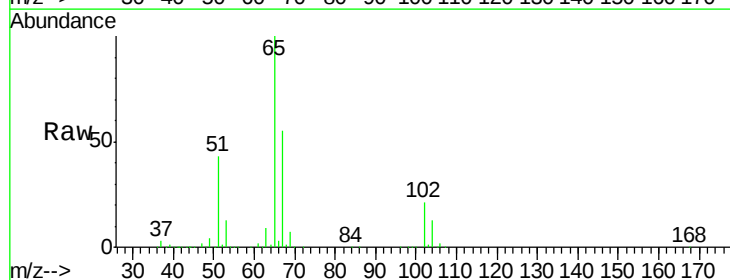

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

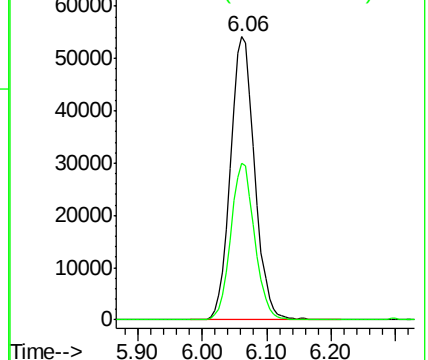


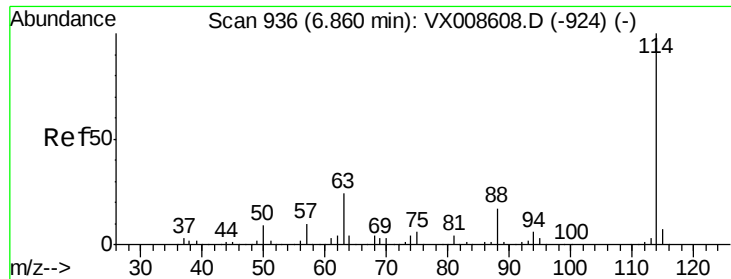


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.86 min Scan# 936
Delta R.T. -0.00 min
Lab File: VX008706.D
Acq: 06 Apr 2019 00:45

Instrument :
MSVOA_X
ClientSampleId :
S8-0702



Tot Ion:114 Resp: 348986
Ion Ratio Lower Upper
114 100
63 23.6 0.0 47.2
88 16.7 0.0 34.0

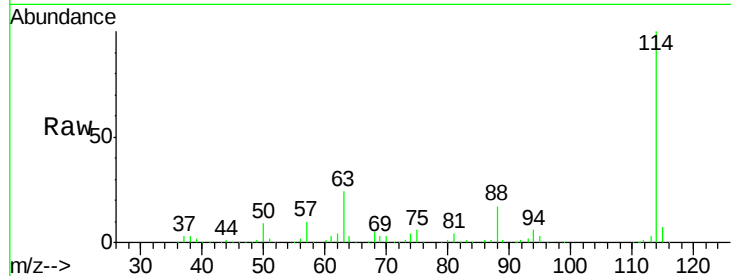

Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

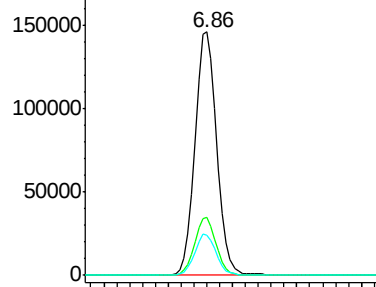


Time-->




#35
Dibromofluoromethane
Concen: 47.089 ug/l
RT: 5.50 min Scan# 713
Delta R.T. -0.00 min
Lab File: VX008706.D
Acq: 06 Apr 2019 00:45


Tgt Ion:113 Resp: 105068
Ion Ratio Lower Upper
113 100
111 103.3 83.4 125.2
192 20.3 16.1 24.1




Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

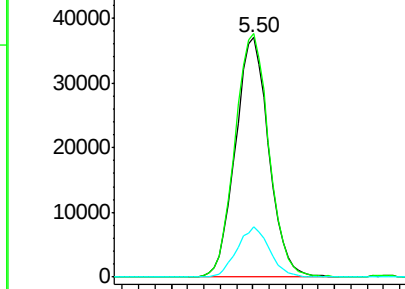

Time-->



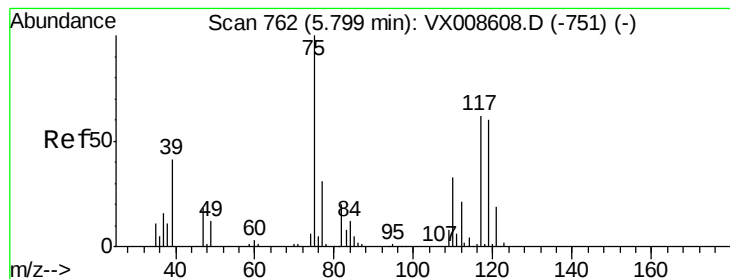

#36

1,1-Dichloropropene

Concen: 4.388 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :

S8-0702


Tot Ion: 75 Resp: 16739

Ion Ratio Lower Upper

75 100

110 8.9 16.4 49.2#




77 0.0 24.7 37.1#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

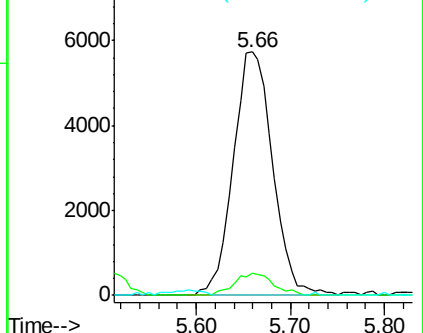

#38

Carbon Tetrachloride

Concen: 6.406 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.13 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45


Tgt Ion:117 Resp: 20226

Ion Ratio Lower Upper

117 100

119 5.0 75.0 112.6#



121 0.0 24.3 36.5#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V



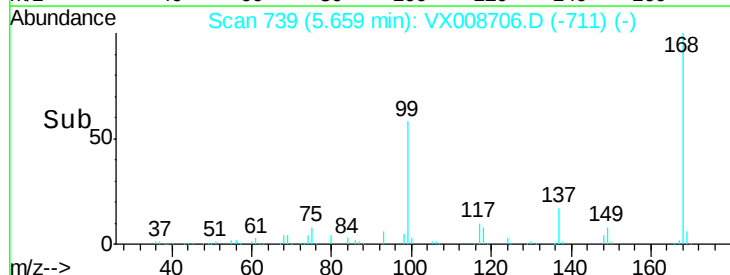
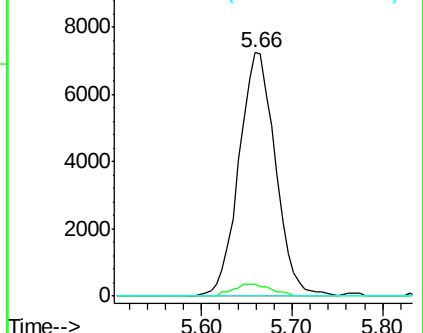


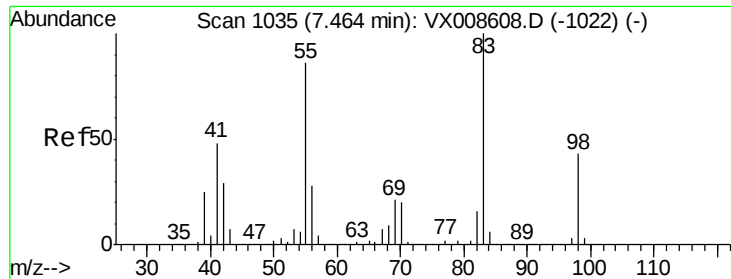

#39
Methvlcvclohexane
Concen: 0.526 ug/l
RT: 7.46 min Scan# 1034
Delta R.T. -0.01 min
Lab File: VX008706.D
Acq: 06 Apr 2019 00:45




Instrument :
MSVOA_X
ClientSampled :
S8-0702


Tot Ion: 83 Resp: 2478
Ion Ratio Lower Upper
83 100
55 95.0 69.0 103.6
98 42.2 34.4 51.6

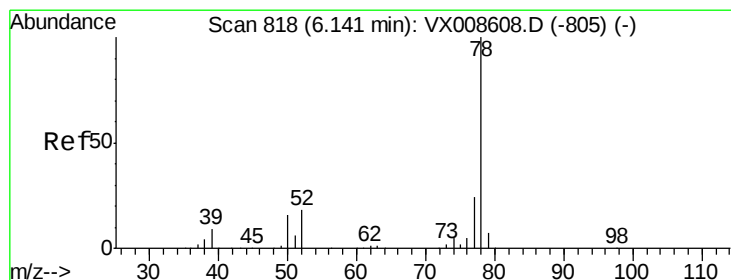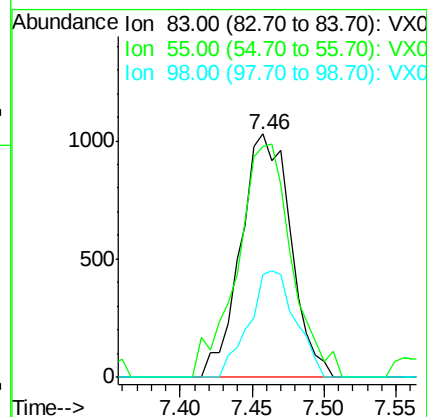

#40
Benzene
Concen: 2.624 ug/l
RT: 6.14 min Scan# 818
Delta R.T. -0.00 min
Lab File: VX008706.D
Acq: 06 Apr 2019 00:45

Tgt Ion: 78 Resp: 29822
Ion Ratio Lower Upper
78 100
77 22.6 19.1 28.7

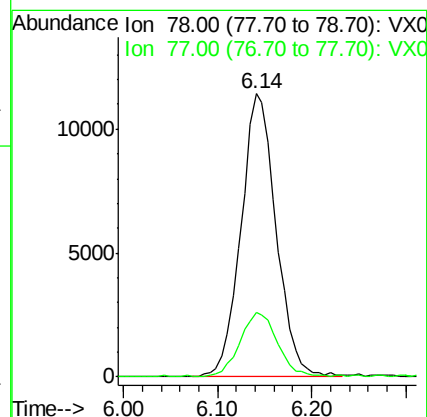

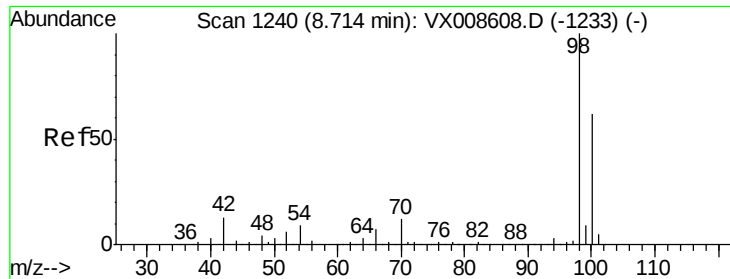

#50

Toluene-d8

Concen: 49.664 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :


S8-0702

Tot Ion: 98 Resp: 441234

Ion Ratio Lower Upper

98 100

100 64.1 51.4 77.0

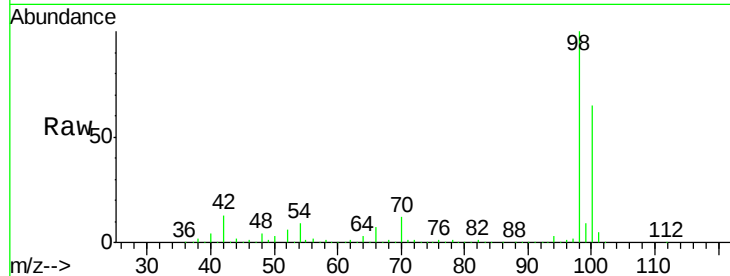

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

8.71

300000

250000

200000

150000



100000

50000

0

8.60 8.80 9.00

Time-->



#55

1,1,2-Trichloroethane

Concen: 0.329 ug/l

RT: 9.16 min Scan# 1314

Delta R.T. -0.05 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Tgt Ion: 97 Resp: 885


Ion Ratio Lower Upper

97 100

83 15.5 73.2 109.8#

85 0.0 46.6 69.8#

99 0.0 50.1 75.1#



Abundance Ion 96.90 (96.60 to 97.60): VX0

Ion 82.90 (82.60 to 83.60): VX0

Ion 84.90 (84.60 to 85.60): VX0

Ion 98.90 (98.60 to 99.60): VX0

800

600


400


200

0

9.10 9.15 9.20

Time-->



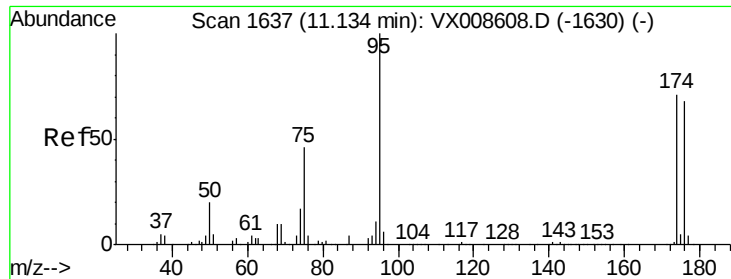

#62

4-Bromofluorobenzene

Concen: 47.410 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :

S8-0702


Tot Ion: 95 Resp: 149366

Ion Ratio Lower Upper

95 100

174 75.8 0.0 151.8




176 75.2 0.0 145.8

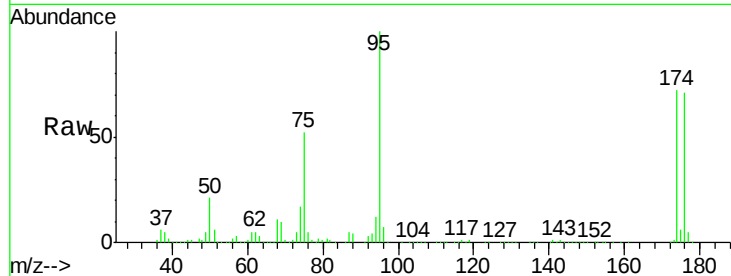

Abundance Ion 94.90 (94.60 to 95.60): VX008608.D (-1630) (-)

Ion 173.80 (173.50 to 174.50): VX008608.D (-1630) (-)

Ion 175.80 (175.50 to 176.50): VX008608.D (-1630) (-)

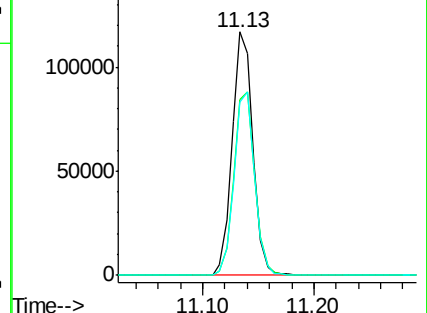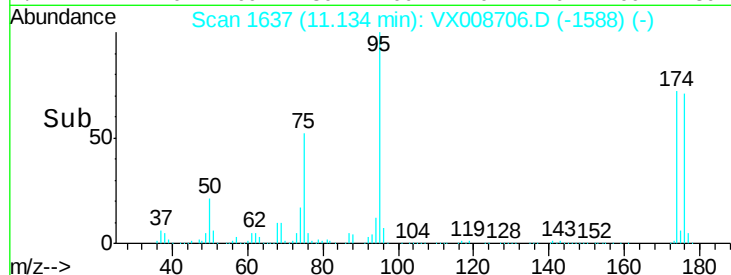

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45


Tgt Ion: 117 Resp: 305072

Ion Ratio Lower Upper

117 100

82 62.3 49.6 74.4



119 31.9 25.0 37.4




Abundance Ion 116.90 (116.60 to 117.60): VX008608.D (-1462) (-)

Ion 82.00 (81.70 to 82.70): VX008608.D (-1462) (-)

Ion 118.90 (118.60 to 119.60): VX008608.D (-1462) (-)



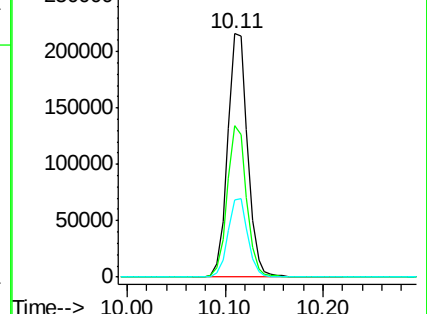



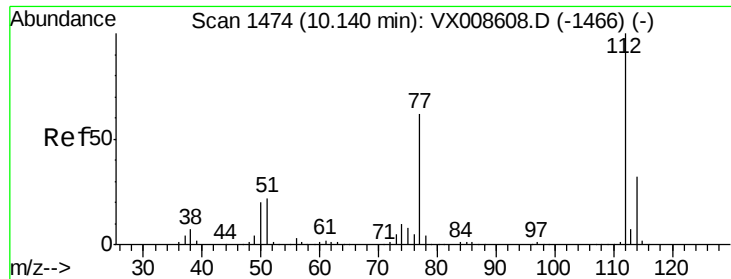

#65
Chlorobenzene
Concen: 0.535 ug/l
RT: 10.14 min Scan# 1474
Delta R.T. -0.00 min
Lab File: VX008706.D
Acq: 06 Apr 2019 00:45




Instrument :
MSVOA_X
ClientSampled :
S8-0702


Tot Ion:112 Resp: 3619
Ion Ratio Lower Upper
112 100
114 32.4 25.8 38.8

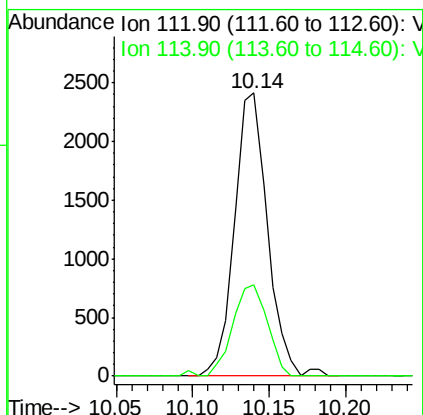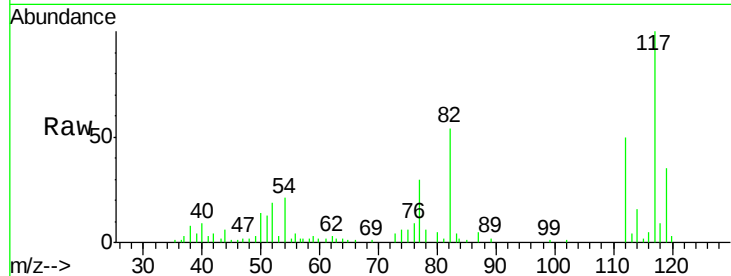

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX008706.D
Acq: 06 Apr 2019 00:45

Tgt Ion:152 Resp: 129377
Ion Ratio Lower Upper
152 100
115 59.3 43.5 130.5
150 155.8 0.0 348.8

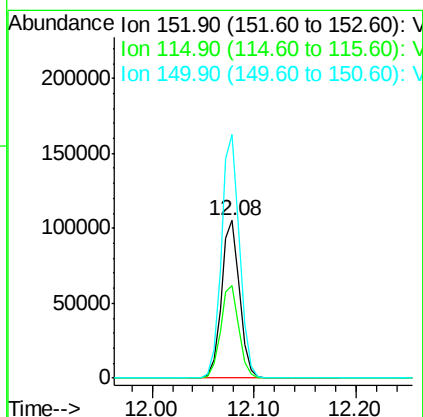

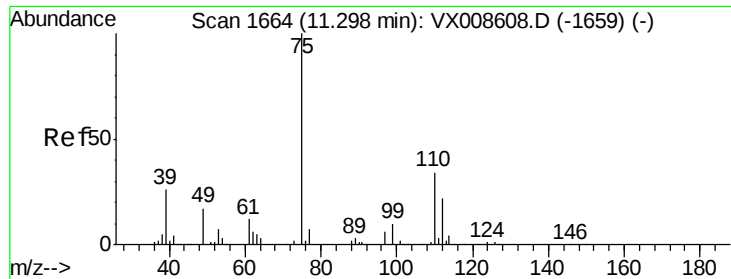

#76

1,2,3-Trichloropropane

Concen: 21.408 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :


S8-0702

Tot Ion: 75 Resp: 76085

Ion Ratio Lower Upper




75 100

77 1.3 22.3 66.8#

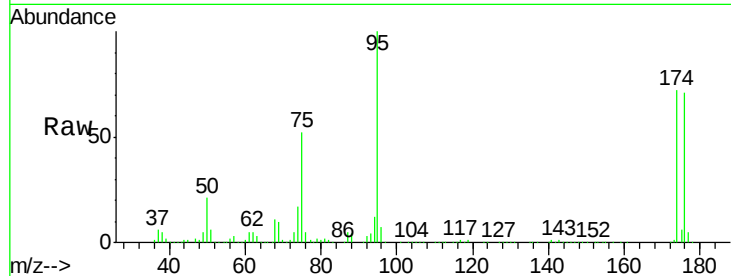

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

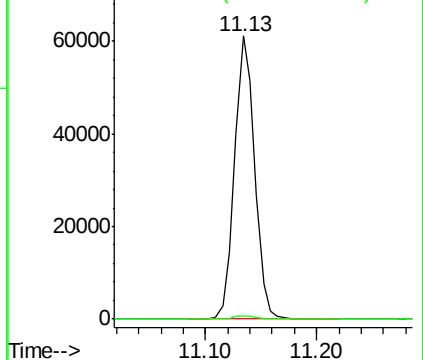

#81

trans-1,4-Dichloro-2-butene

Concen: 59.011 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45


Tgt Ion: 75 Resp: 76085

Ion Ratio Lower Upper

75 100

53 0.3 81.3 121.9#



89 0.0 35.6 53.4#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0




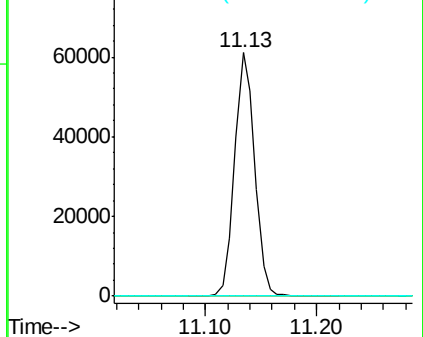


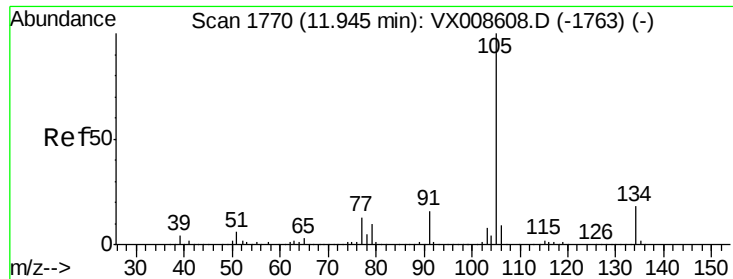

#85
 sec-Butylbenzene
 Concen: 0.317 ug/l
 RT: 11.94 min Scan# 1770
 Delta R.T. -0.00 min
 Lab File: VX008706.D
 Acq: 06 Apr 2019 00:45




Instrument :
 MSVOA_X
 ClientSampleId :
 S8-0702


Tot Ion:105 Resp: 3262
 Ion Ratio Lower Upper
 105 100
 134 22.2 9.4 28.2

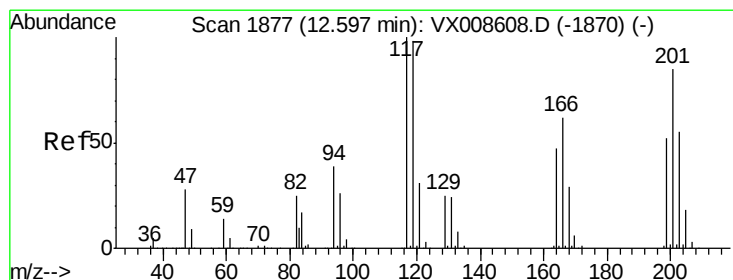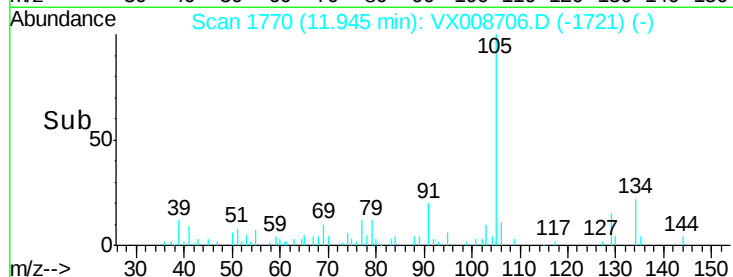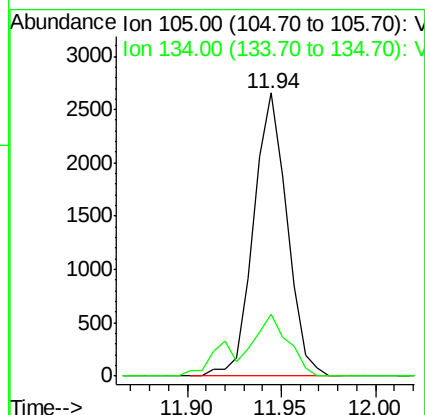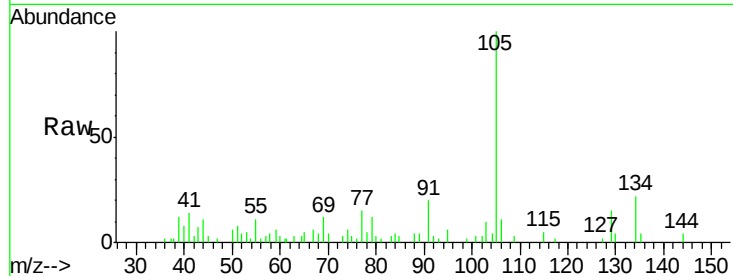

#90
 Hexachloroethane
 Concen: 0.692 ug/l
 RT: 12.75 min Scan# 1902
 Delta R.T. 0.15 min
 Lab File: VX008706.D
 Acq: 06 Apr 2019 00:45

Tgt Ion:117 Resp: 1059
 Ion Ratio Lower Upper
 117 100
 201 0.0 40.6 122.0#

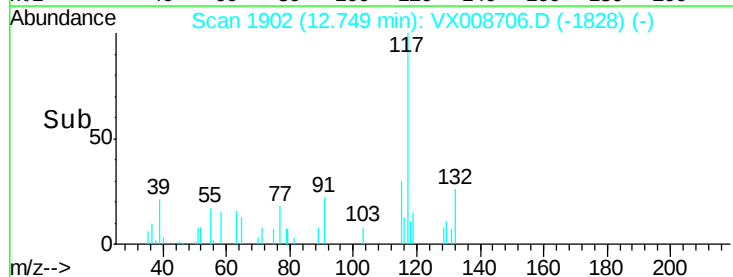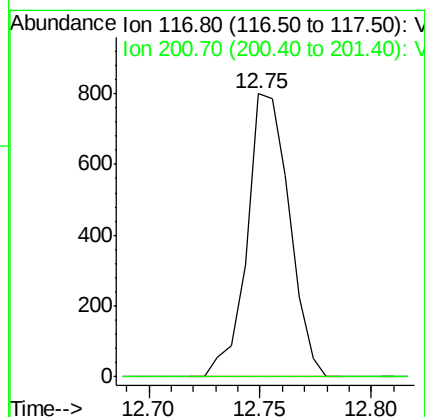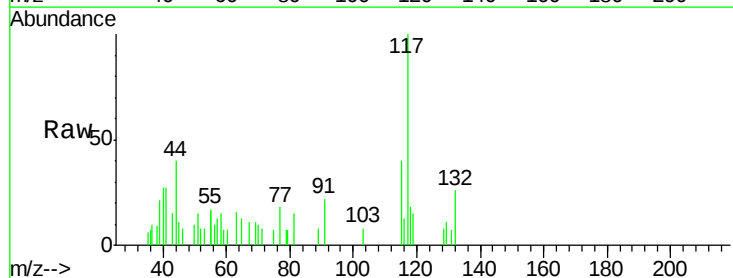

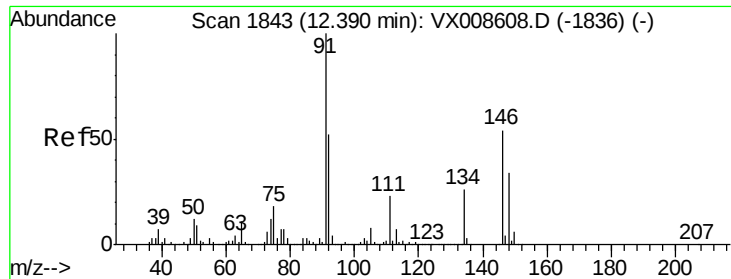

#91

1,2-Dichlorobenzene

Concen: 0.323 ug/l

RT: 12.39 min Scan# 1843

Delta R.T. -0.00 min

Lab File: VX008706.D

Acq: 06 Apr 2019 00:45

Instrument :

MSVOA_X

ClientSampleId :

S8-0702


Tot Ion:146 Resp: 1478

Ion Ratio Lower Upper

146 100

111 48.7 21.3 63.9

148 62.0 31.7 95.1



Abundance Ion 145.90 (145.60 to 146.60): V
Ion 110.90 (110.60 to 111.60): V
Ion 147.90 (147.60 to 148.60): V

