


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX040519\
 Data File : VX008672.D
 Acq On : 05 Apr 2019 09:03
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X032719W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Mar 27 12:01:15 2019

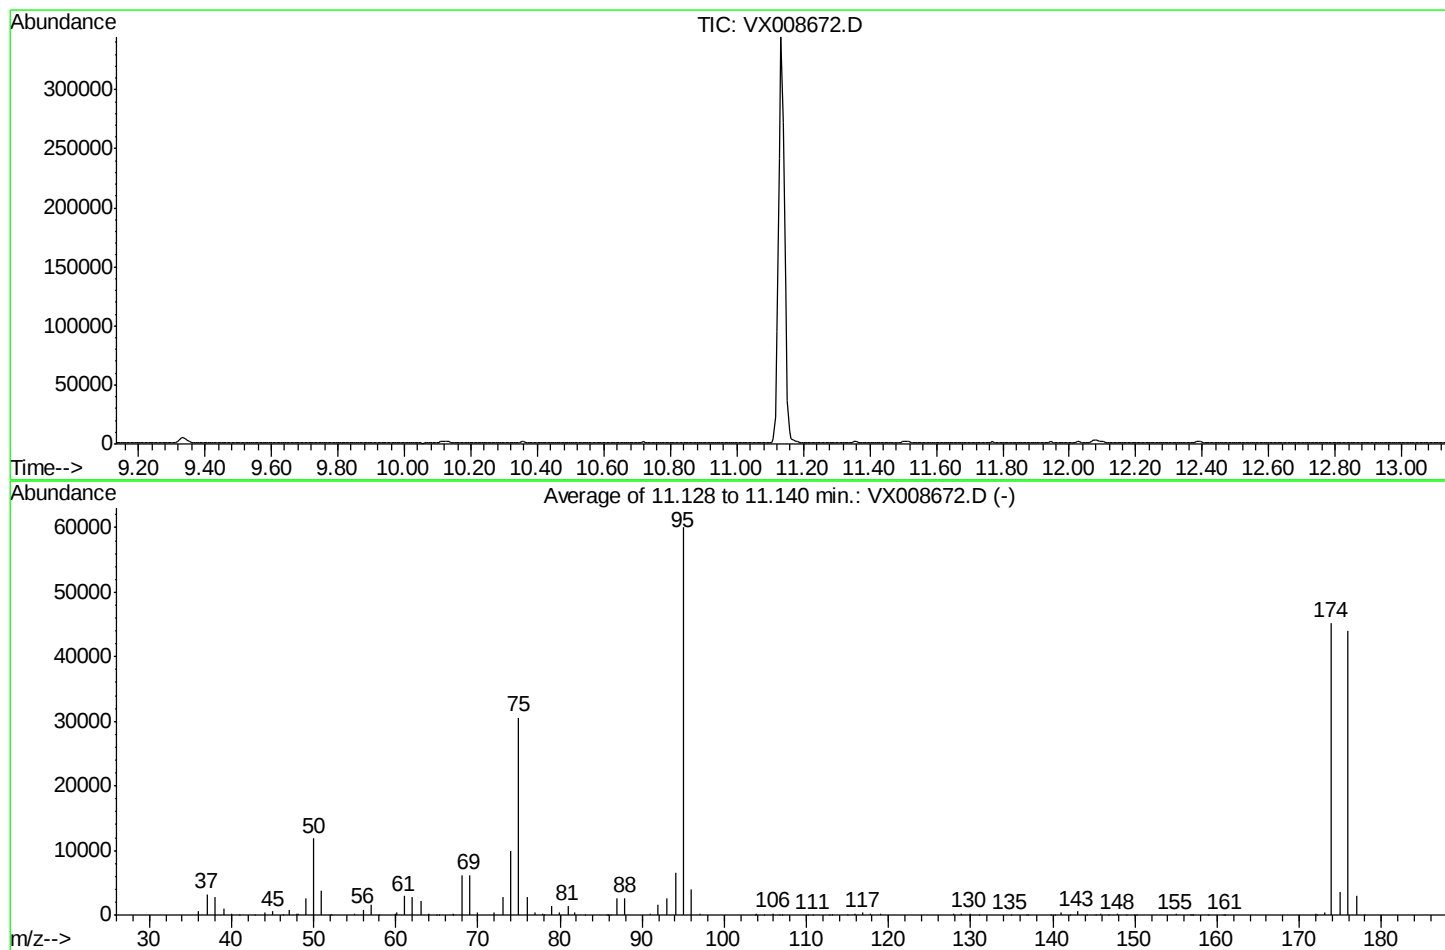

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	11868	PASS
75	95	30	60	50.9	30552	PASS
95	95	100	100	100.0	60058	PASS
96	95	5	9	6.6	3942	PASS
173	174	0.00	2	0.9	408	PASS
174	95	50	100	75.4	45304	PASS
175	174	5	9	7.8	3512	PASS
176	174	95	101	97.3	44093	PASS
177	176	5	9	6.6	2919	PASS