


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX040519\
 Data File : VX008682.D
 Acq On : 05 Apr 2019 14:08
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Title : SW846 8260
 Last Update : Thu Apr 04 04:47:41 2019

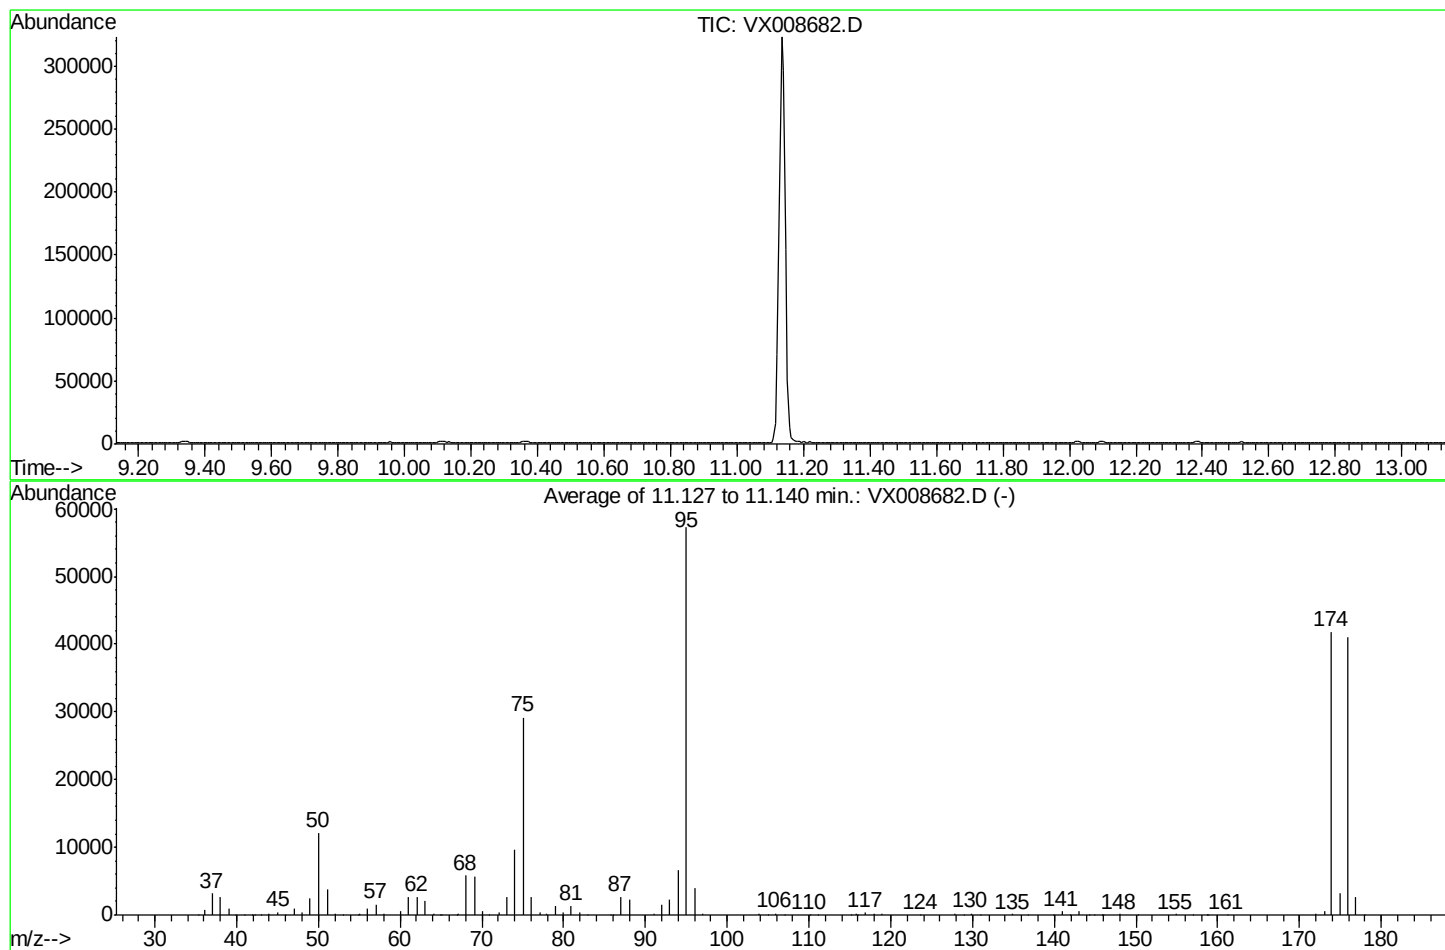

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	12139	PASS
75	95	30	60	51.0	29181	PASS
95	95	100	100	100.0	57269	PASS
96	95	5	9	7.0	3985	PASS
173	174	0.00	2	1.4	598	PASS
174	95	50	100	73.0	41797	PASS
175	174	5	9	7.8	3259	PASS
176	174	95	101	98.2	41061	PASS
177	176	5	9	6.5	2653	PASS