



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040523\
Data File : VX034939.D
Acq On : 05 Apr 2023 09:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Title : SW846 8260
Last Update : Sat Apr 01 01:50:18 2023

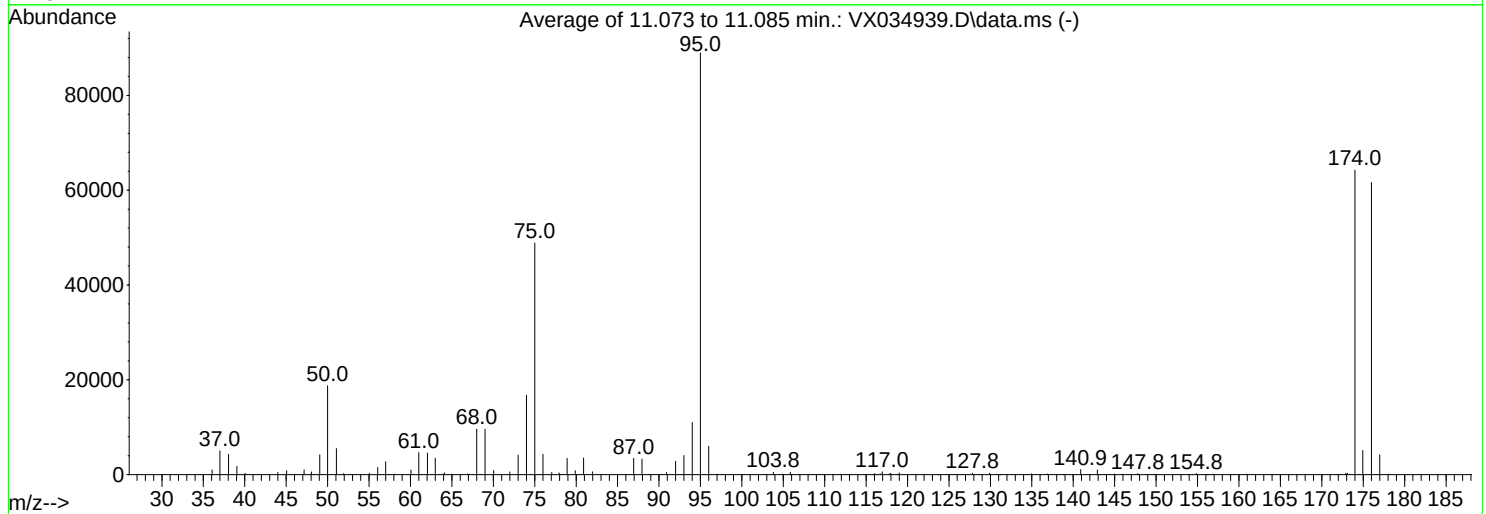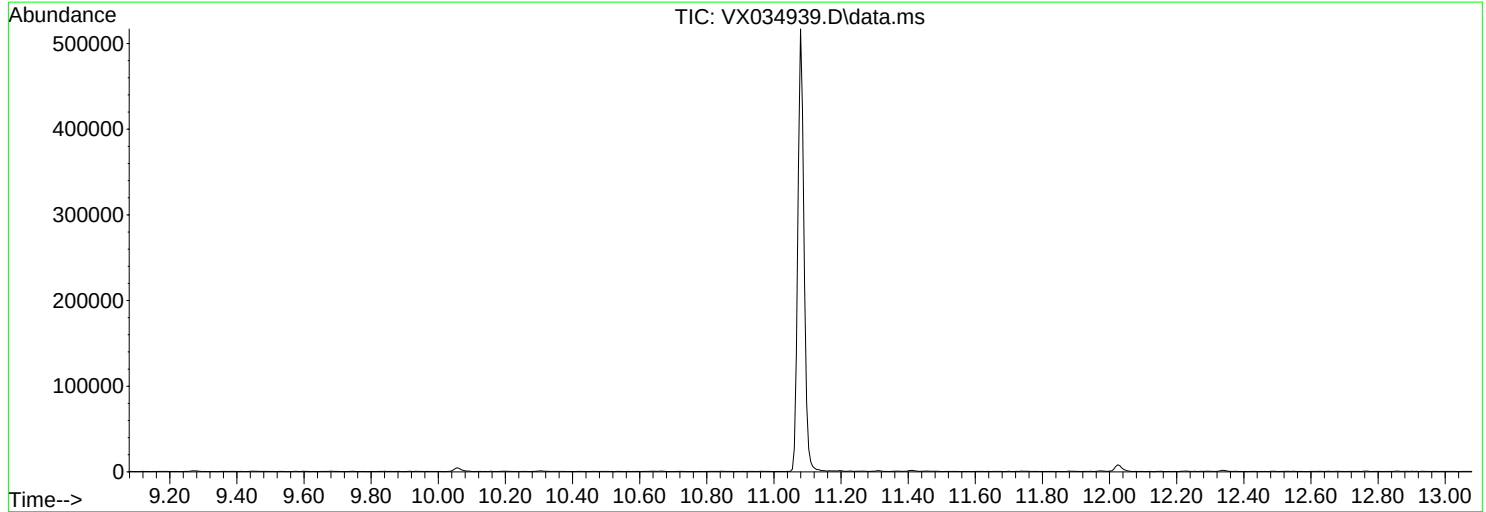

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	18768	PASS
75	95	30	60	54.9	48885	PASS
95	95	100	100	100.0	88976	PASS
96	95	5	9	6.7	5970	PASS
173	174	0.00	2	0.5	309	PASS
174	95	50	100	72.2	64227	PASS
175	174	5	9	7.9	5095	PASS
176	174	95	101	96.0	61643	PASS
177	176	5	9	6.8	4191	PASS