

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040524\
 Data File : VX040909.D
 Acq On : 05 Apr 2024 17:17
 Operator : JC/MD
 Sample : P1996-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP1

Quant Time: Apr 05 23:24:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 02 05:40:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	41288	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	78063	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	77684	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	40106	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	37839	51.077	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.160%			
35) Dibromofluoromethane	5.385	113	26324	47.609	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 95.220%			
50) Toluene-d8	8.647	98	97977	49.038	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 98.080%			
62) 4-Bromofluorobenzene	11.079	95	41072	51.477	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 102.960%			
Target Compounds						Qvalue
9) 1,1,2-Trichlorotrifluo...	2.337	101	142	0.288	ug/l #	20
11) Tert butyl alcohol	2.953	59	451	3.335	ug/l #	78
16) Acetone	2.380	43	24695	85.850	ug/l	99
17) Carbon Disulfide	2.514	76	268	0.201	ug/l #	76
18) Methyl Acetate	2.703	43	609	0.892	ug/l #	63
20) Methylene Chloride	2.794	84	2498	4.686	ug/l	97
25) 2-Butanone	4.568	43	2424	5.673	ug/l	100
29) Tetrahydrofuran	5.025	42	167	0.601	ug/l #	44
31) Cyclohexane	5.556	56	1182	1.504	ug/l #	32
36) 1,1-Dichloropropene	5.550	75	3818	4.860	ug/l #	50
37) Ethyl Acetate	4.733	43	1482	1.536	ug/l #	74
38) Carbon Tetrachloride	5.550	117	4654	5.351	ug/l #	17
43) Isopropyl Acetate	6.336	43	44644	29.965	ug/l	97
44) Trichloroethene	7.129	130	1742	3.199	ug/l	96
48) Methyl methacrylate	7.793	41	42945	58.864	ug/l #	50
51) 4-Methyl-2-Pentanone	8.549	43	35015	35.432	ug/l #	49
52) Toluene	8.720	92	2003	1.456	ug/l	100
53) t-1,3-Dichloropropene	8.945	75	222	0.994	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	12724	14.456	ug/l #	67
56) Ethyl methacrylate	9.244	69	296	0.321	ug/l #	1
57) 1,3-Dichloropropane	9.482	76	1676	1.785	ug/l #	42
59) 2-Hexanone	9.482	43	27584	34.803	ug/l #	51
67) Ethyl Benzene	10.195	91	826	0.273	ug/l #	88
68) m/p-Xylenes	10.305	106	928	0.842	ug/l	79
74) N-amyl acetate	10.774	43	675	0.476	ug/l #	44
76) 1,2,3-Trichloropropane	11.079	75	24130	28.215	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	24130	76.125	ug/l #	5
93) 1,2,4-Trichlorobenzene	13.591	180	219	0.243	ug/l	88
94) Hexachlorobutadiene	13.725	225	165	0.477	ug/l	93
95) Naphthalene	13.780	128	685	0.236	ug/l #	80
96) 1,2,3-Trichlorobenzene	13.969	180	236	0.274	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040524\
Data File : VX040909.D
Acq On : 05 Apr 2024 17:17
Operator : JC/MD
Sample : P1996-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP1

Quant Time: Apr 05 23:24:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 02 05:40:55 2024
Response via : Initial Calibration




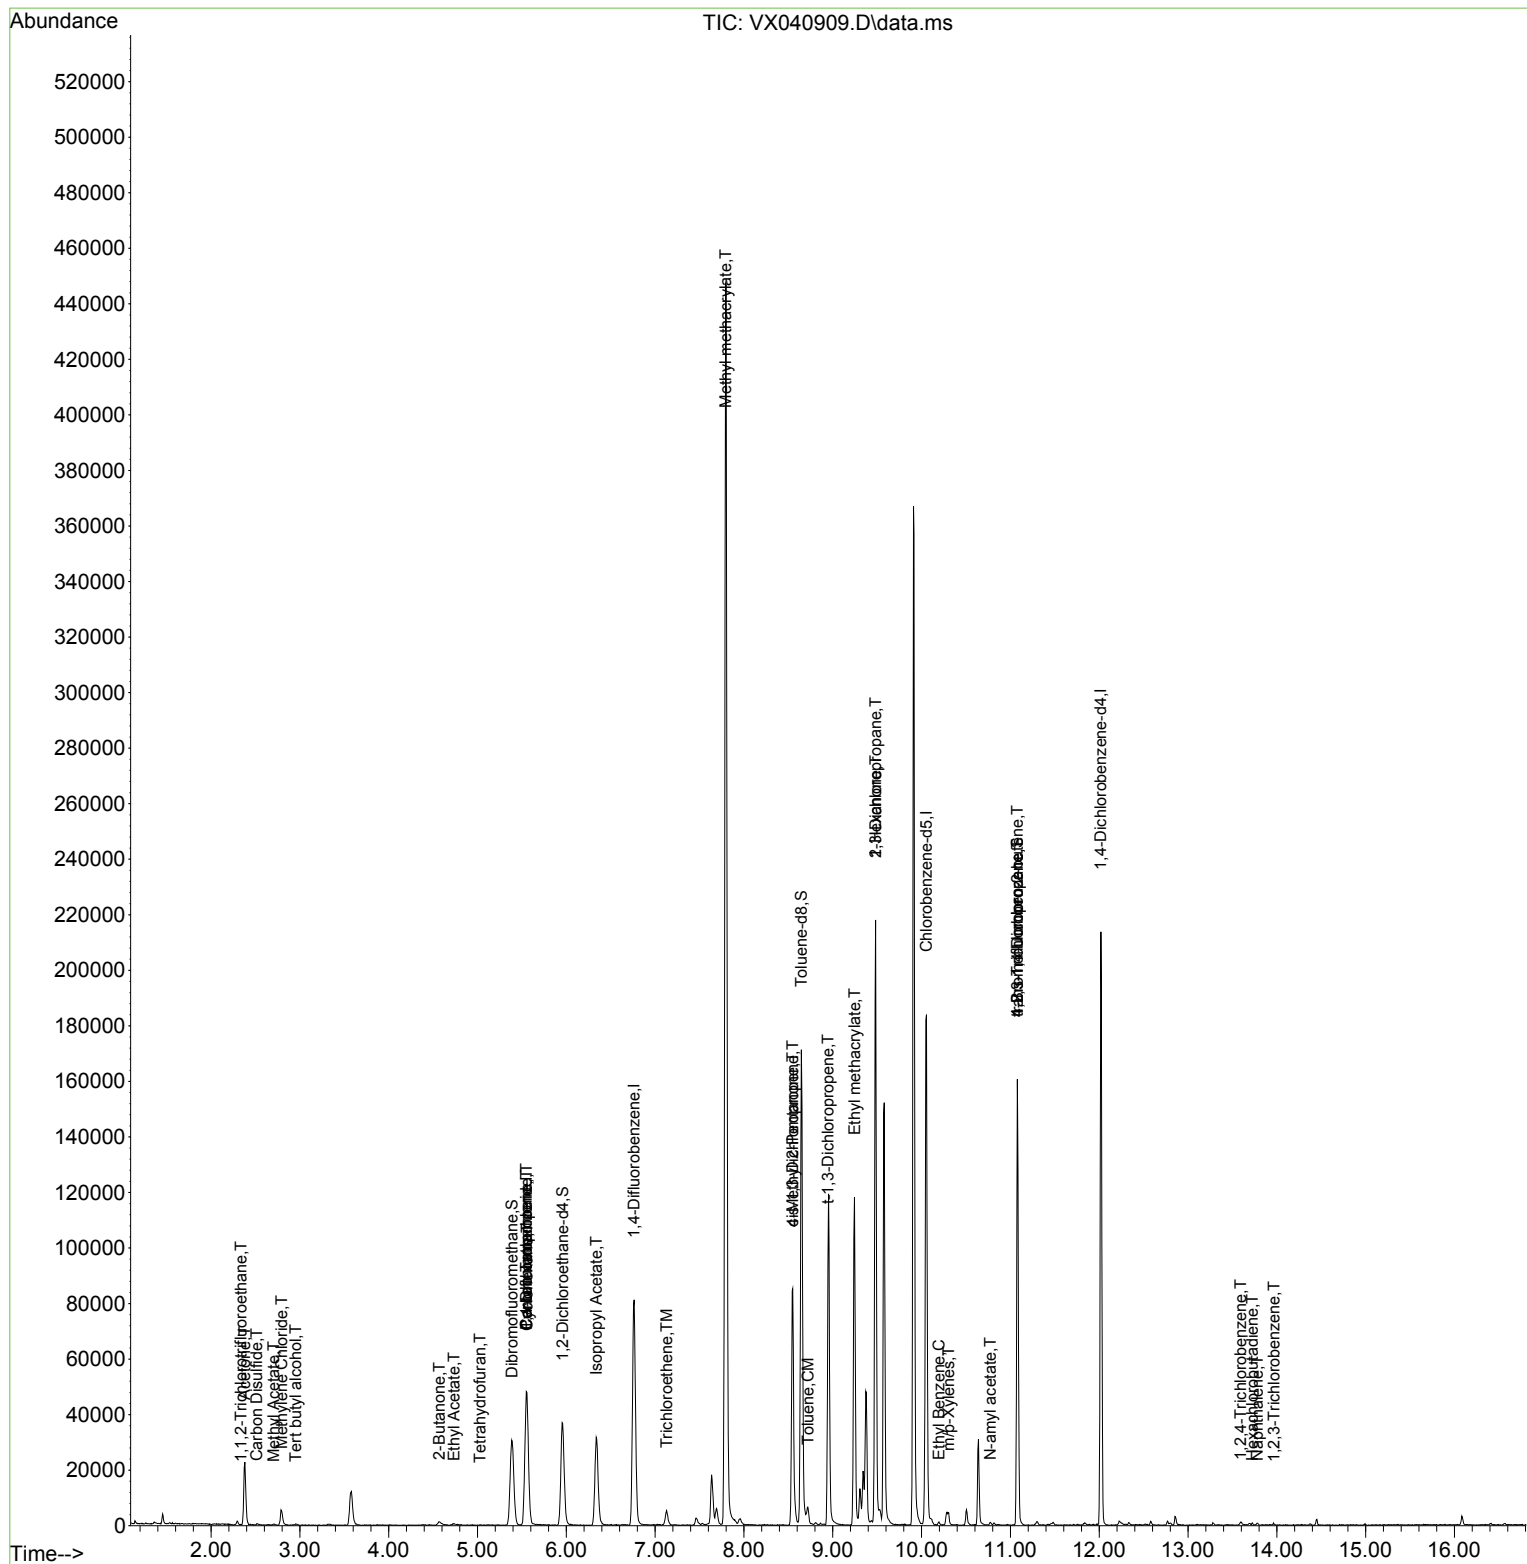


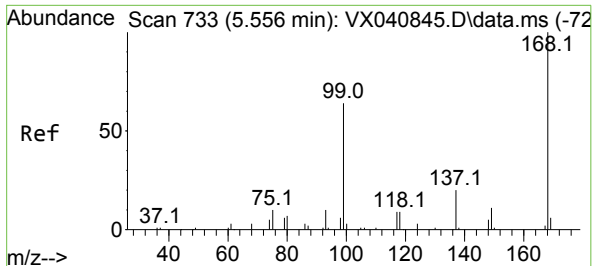

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion:168 Resp: 41288
Ion Ratio Lower Upper
168 100
99 69.6 56.6 85.0

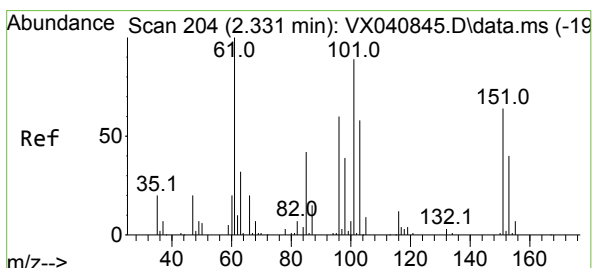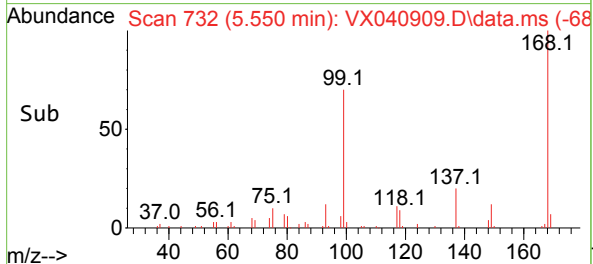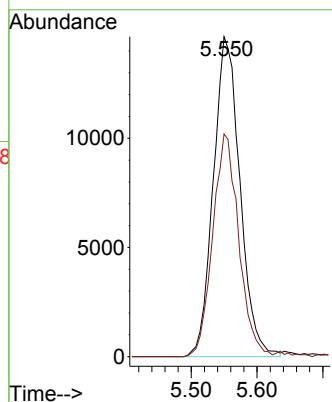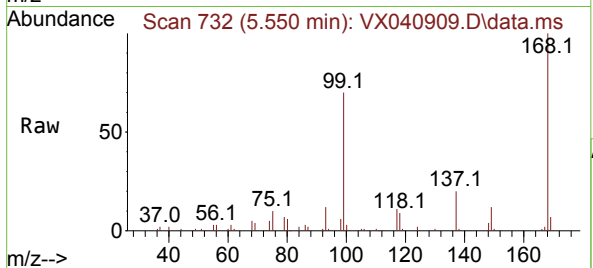

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.288 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion:101 Resp: 142
Ion Ratio Lower Upper
101 100
85 0.0 37.0 55.6#
151 0.0 58.6 87.8#

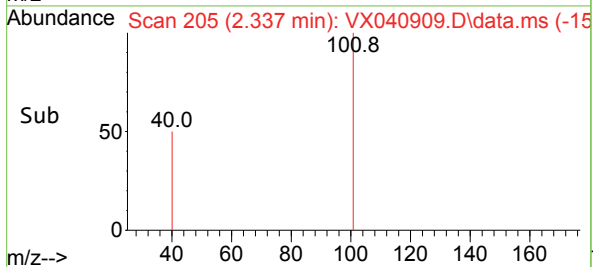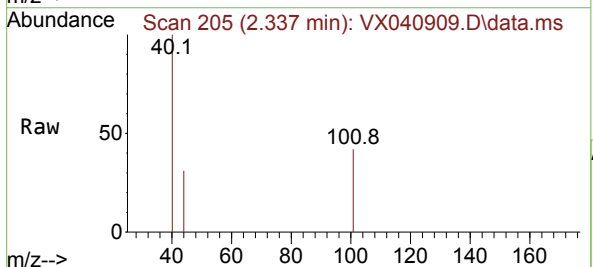



#11

Tert butyl alcohol

Concen: 3.335 ug/l

RT: 2.953 min Scan# 307

Delta R.T. -0.006 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :





TP1

Tgt Ion: 59 Resp: 451

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

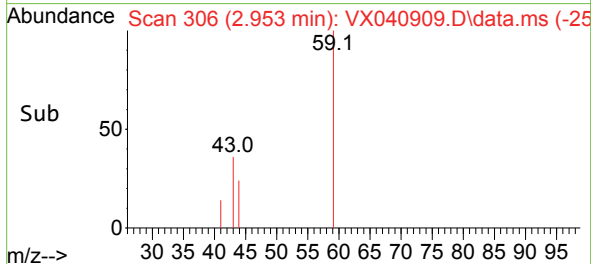

#16

Acetone

Concen: 85.850 ug/l

RT: 2.380 min Scan# 212

Delta R.T. 0.000 min

Lab File: VX040909.D




Acq: 05 Apr 2024 17:17


Tgt Ion: 43 Resp: 24695

Ion Ratio Lower Upper

43 100

58 26.8 21.9 32.9





#17

Carbon Disulfide

Concen: 0.201 ug/l

RT: 2.514 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :





TP1

Tgt Ion: 76 Resp: 268

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.6#

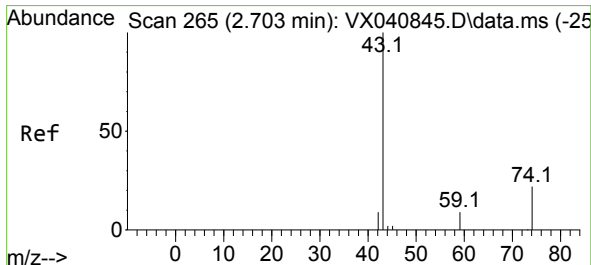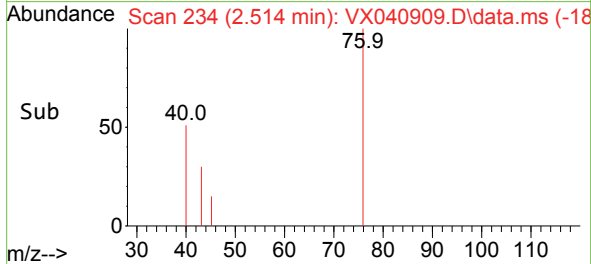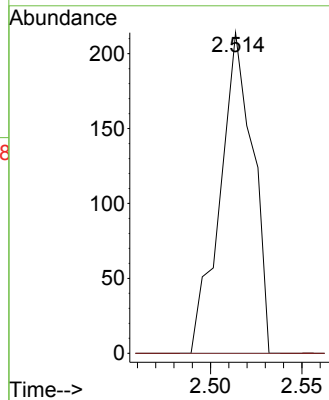

#18

Methyl Acetate

Concen: 0.892 ug/l

RT: 2.703 min Scan# 265

Delta R.T. 0.000 min

Lab File: VX040909.D




Acq: 05 Apr 2024 17:17


Tgt Ion: 43 Resp: 609

Ion Ratio Lower Upper

43 100

74 4.4 17.8 26.8#



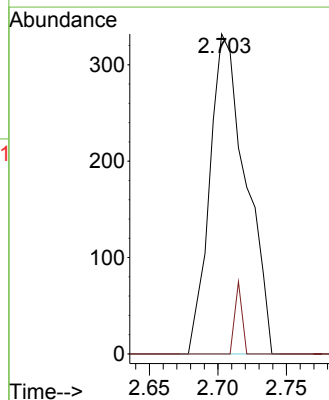
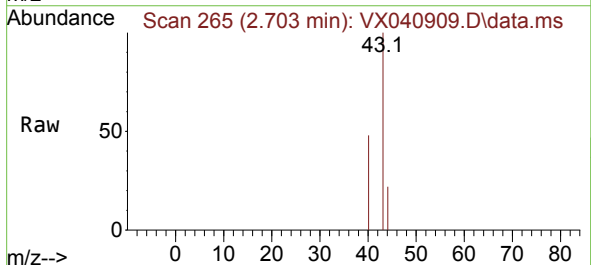




#20
Methylene Chloride
Concen: 4.686 ug/l
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 84	Resp: 2498
Ion Ratio	Lower Upper
84 100	
49 129.2	103.6 155.4
51 40.9	33.8 50.6
86 55.1	49.4 74.0

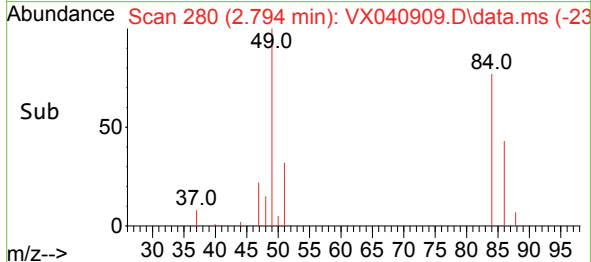

#25
2-Butanone
Concen: 5.673 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.018 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion: 43	Resp: 2424
Ion Ratio	Lower Upper
43 100	
72 24.5	19.4 29.2

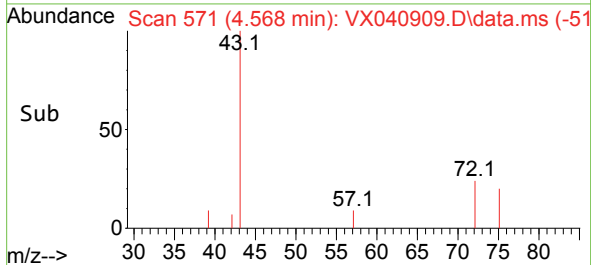

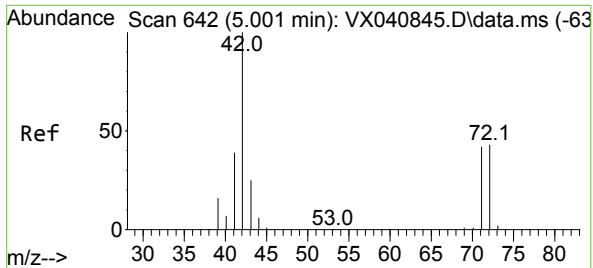

#29

Tetrahydrofuran

Concen: 0.601 ug/l

RT: 5.025 min Scan# 64

Delta R.T. 0.024 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :

TP1





Tgt Ion: 42 Resp: 167

Ion Ratio Lower Upper

42 100

72 12.0 34.2 51.4#

71 0.0 32.2 48.2#

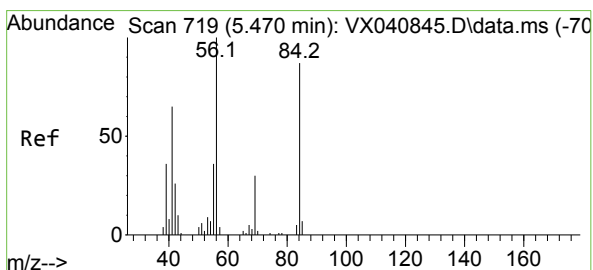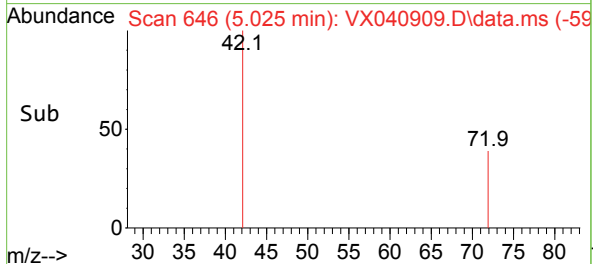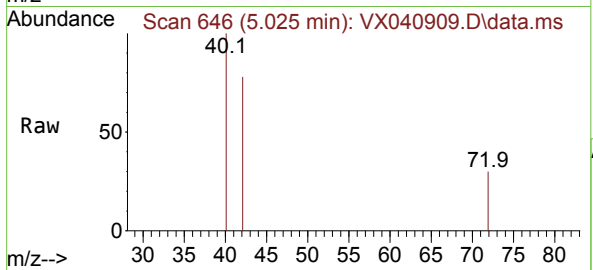

#31

Cyclohexane

Concen: 1.504 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.085 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17




Tgt Ion: 56 Resp: 1182


Ion Ratio Lower Upper

56 100

69 143.7 23.4 35.2#

84 97.4 65.9 98.9


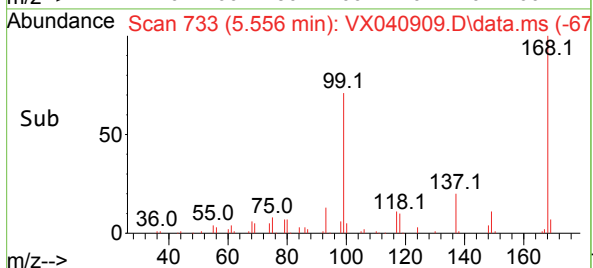

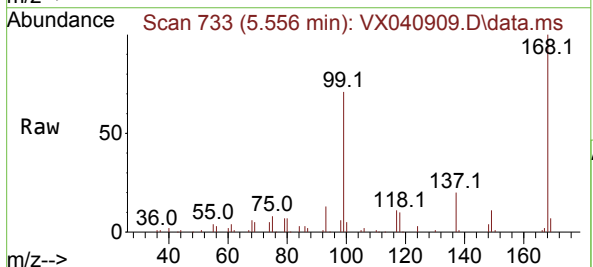




#33
1,2-Dichloroethane-d4
Concen: 51.077 ug/l
RT: 5.958 min Scan# 798
Delta R.T. 0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 65 Resp: 37839
Ion Ratio Lower Upper
65 100
67 49.0 0.0 100.2

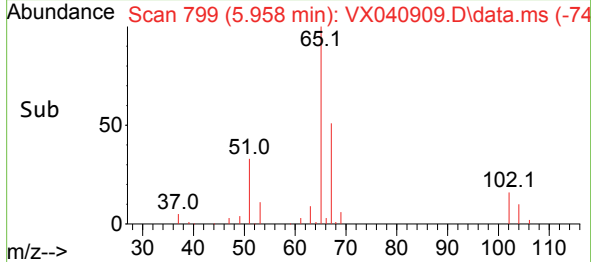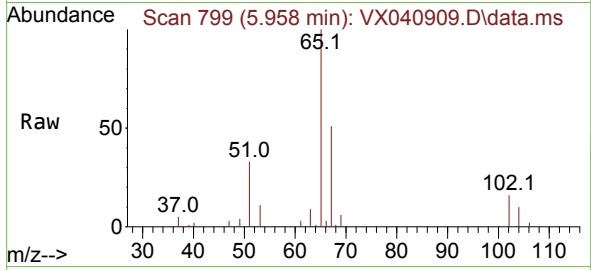

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17


Tgt Ion: 114 Resp: 78063
Ion Ratio Lower Upper
114 100
63 25.7 0.0 45.0
88 18.7 0.0 36.6





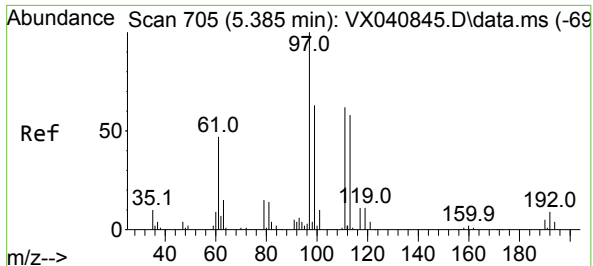


#35
Dibromofluoromethane
Concen: 47.609 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17


Instrument :
MSVOA_X
ClientSampleId :
TP1

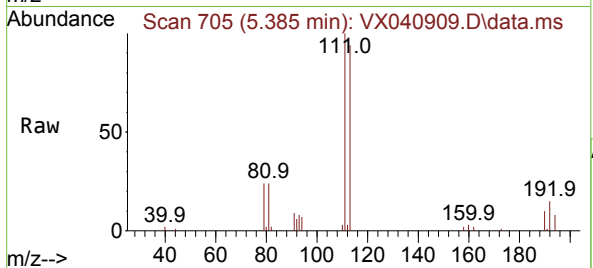



Tgt Ion:113 Resp: 26324
Ion Ratio Lower Upper
113 100
111 104.6 82.9 124.3
192 17.1 13.3 19.9

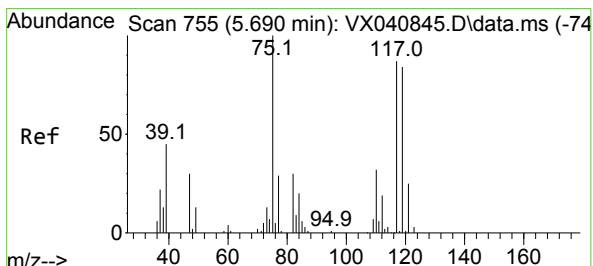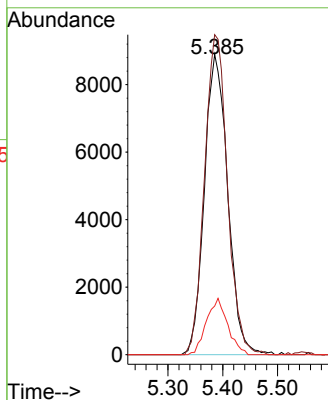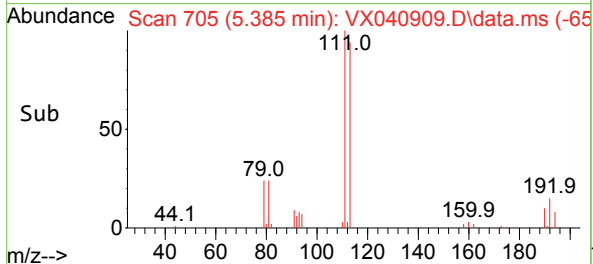


#36
1,1-Dichloropropene
Concen: 4.860 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

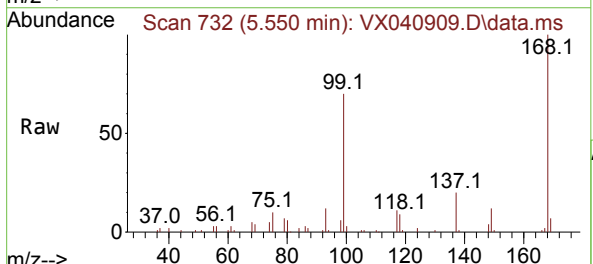

Tgt Ion: 75 Resp: 3818
Ion Ratio Lower Upper
75 100
110 8.3 17.0 50.9#
77 0.0 24.7 37.1#

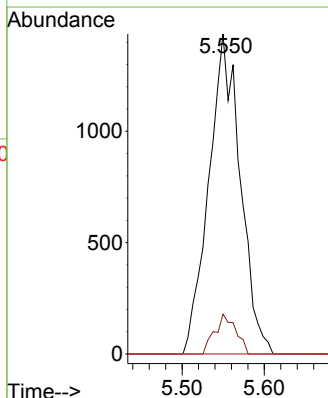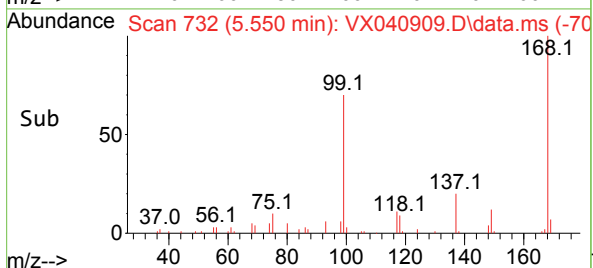



#37

Ethyl Acetate

Concen: 1.536 ug/l

RT: 4.733 min Scan# 51

Delta R.T. 0.025 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :

TP1





Tgt Ion: 43 Resp: 1482

Ion Ratio Lower Upper

43 100

61 3.6 10.6 16.0#

70 0.0 8.3 12.5#

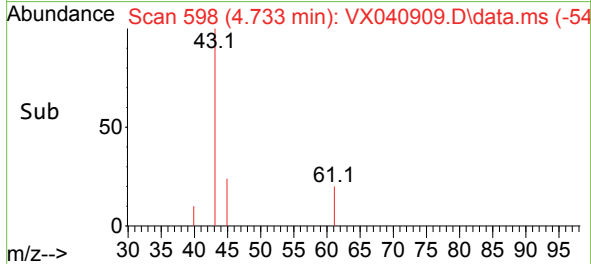

#38

Carbon Tetrachloride

Concen: 5.351 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.128 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17




Tgt Ion: 117 Resp: 4654


Ion Ratio Lower Upper

117 100

119 7.3 78.2 117.2#

121 0.0 24.4 36.6#


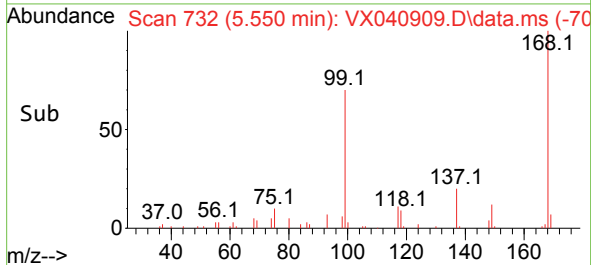






#43
Isopropyl Acetate
Concen: 29.965 ug/l
RT: 6.336 min Scan# 861
Delta R.T. -0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 43 Resp: 44644
Ion Ratio Lower Upper
43 100
61 17.4 15.2 22.8
87 11.3 9.8 14.6

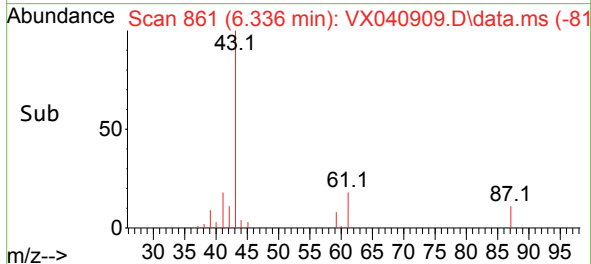

#44
Trichloroethene
Concen: 3.199 ug/l
RT: 7.129 min Scan# 991
Delta R.T. 0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion:130 Resp: 1742
Ion Ratio Lower Upper
130 100
95 106.2 0.0 204.4


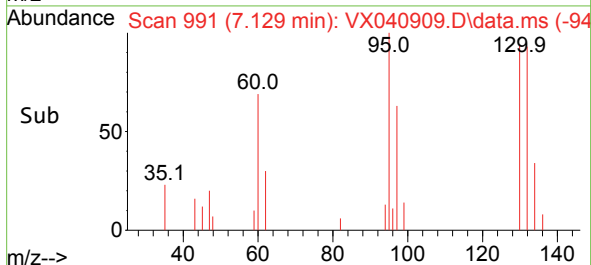






#48
Methyl methacrylate
Concen: 58.864 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.104 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 41 Resp: 42945
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 56.5 47.7 71.5

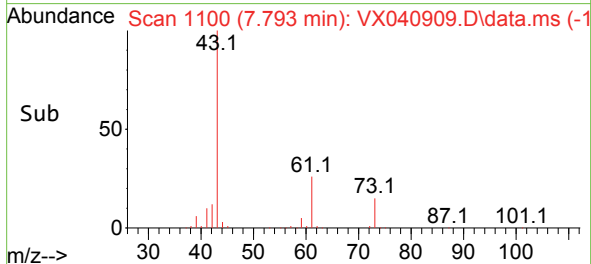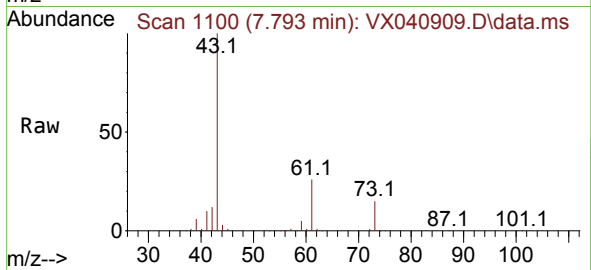

#50
Toluene-d8
Concen: 49.038 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion: 98 Resp: 97977
Ion Ratio Lower Upper
98 100
100 64.8 53.1 79.7

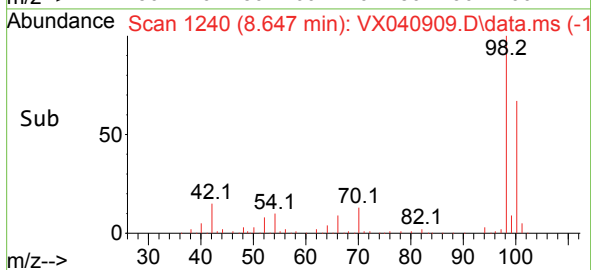



#51

4-Methyl-2-Pentanone

Concen: 35.432 ug/l

RT: 8.549 min Scan# 11

Delta R.T. -0.024 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :





TP1

Tgt Ion: 43 Resp: 35015

Ion Ratio Lower Upper

43 100

58 7.1 30.4 45.6#

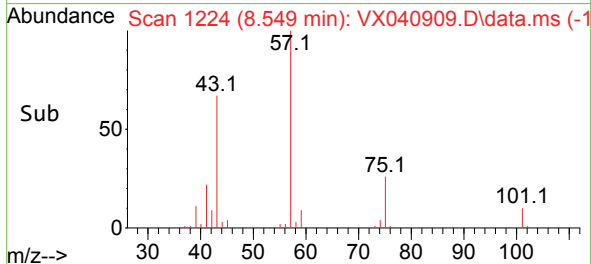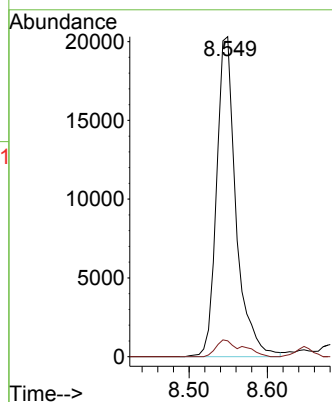

#52

Toluene

Concen: 1.456 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. 0.000 min

Lab File: VX040909.D




Acq: 05 Apr 2024 17:17


Tgt Ion: 92 Resp: 2003

Ion Ratio Lower Upper

92 100

91 167.3 134.2 201.2


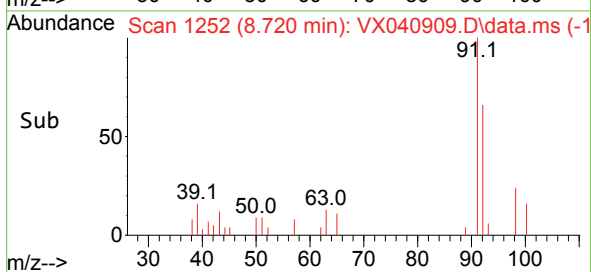
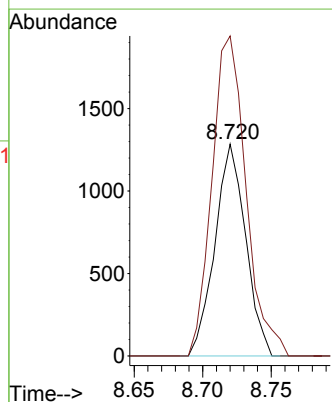





#53
t-1,3-Dichloropropene
Concen: 0.994 ug/l
RT: 8.945 min Scan# 1124
Delta R.T. -0.031 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 75 Resp: 222
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#

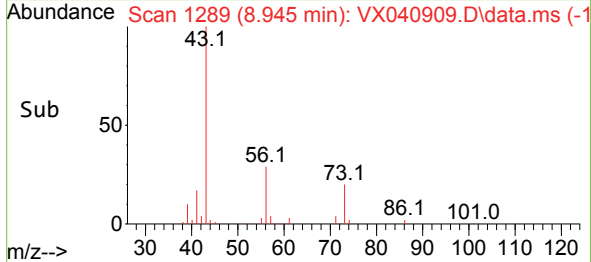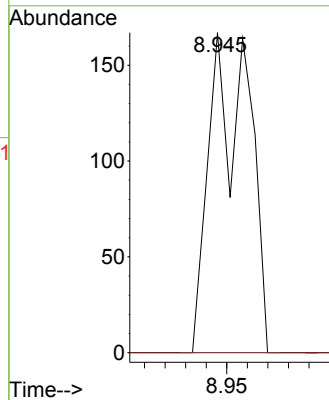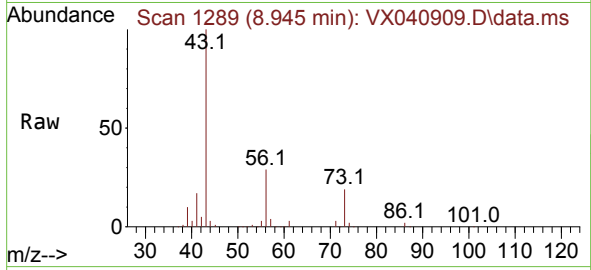

#54
cis-1,3-Dichloropropene
Concen: 14.456 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.183 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion: 75 Resp: 12724
Ion Ratio Lower Upper
75 100
77 0.0 25.3 37.9#
39 43.0 46.7 70.1#



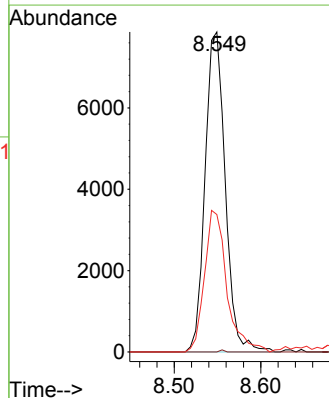





#56
Ethyl methacrylate
Concen: 0.321 ug/l
RT: 9.244 min Scan# 1338
Delta R.T. 0.128 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 69 Resp: 296
Ion Ratio Lower Upper
69 100
41 7000.3 56.8 85.2#
39 2979.1 32.0 48.0#

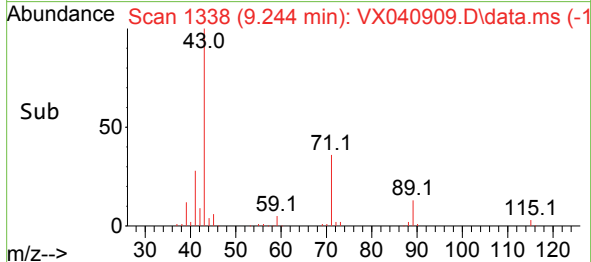

#57
1,3-Dichloropropane
Concen: 1.785 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.177 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion: 76 Resp: 1676
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#









#59
2-Hexanone
Concen: 34.803 ug/l
RT: 9.482 min Scan# 11
Delta R.T. 0.055 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 43 Resp: 27584
Ion Ratio Lower Upper
43 100
58 17.5 26.2 78.5#

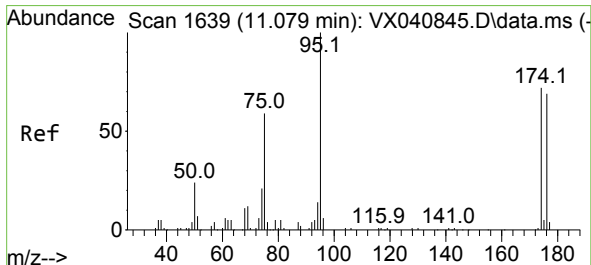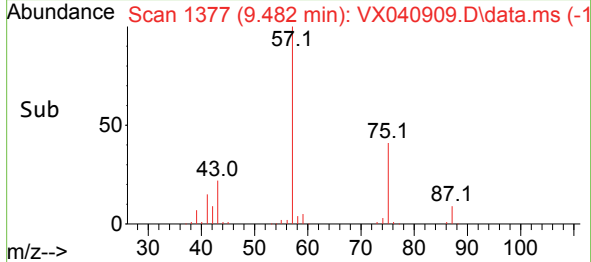

#62
4-Bromofluorobenzene
Concen: 51.477 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion: 95 Resp: 41072
Ion Ratio Lower Upper
95 100
174 70.8 0.0 135.6
176 70.2 0.0 131.0

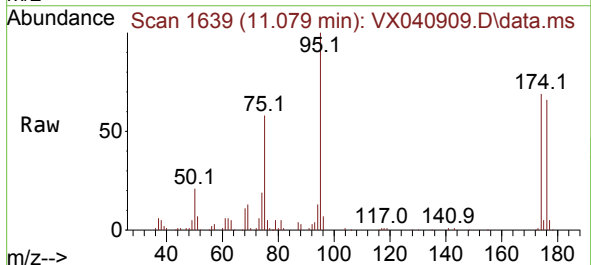



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :

TP1





Tgt Ion:117 Resp: 77684

Ion Ratio Lower Upper

117 100

82 57.9 46.2 69.4

119 33.4 25.5 38.3

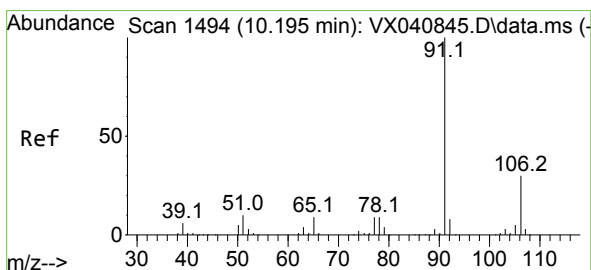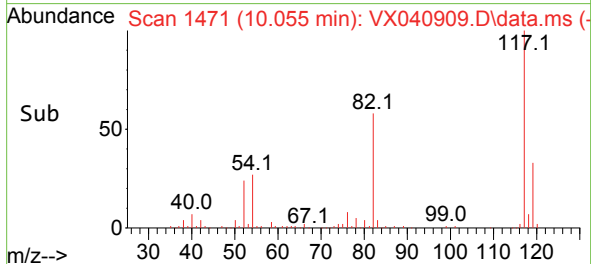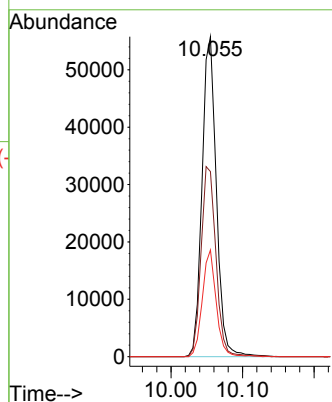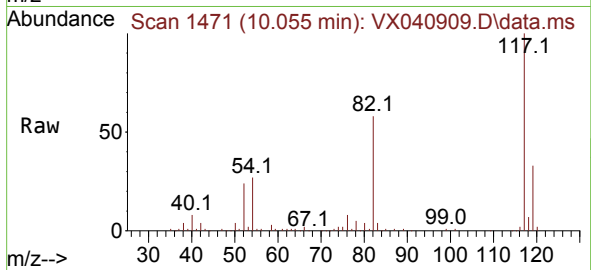

#67

Ethyl Benzene

Concen: 0.273 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX040909.D




Acq: 05 Apr 2024 17:17


Tgt Ion: 91 Resp: 826

Ion Ratio Lower Upper

91 100

106 37.8 24.9 37.3#







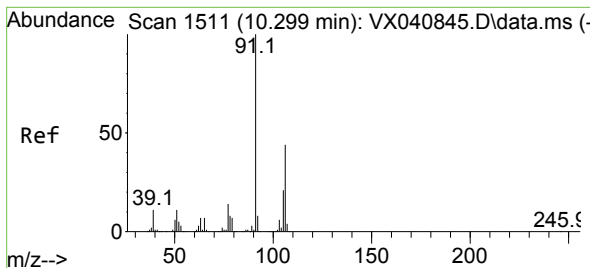

#68
m/p-Xylenes
Concen: 0.842 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion:106 Resp: 928
Ion Ratio Lower Upper
106 100
91 239.9 165.5 248.3

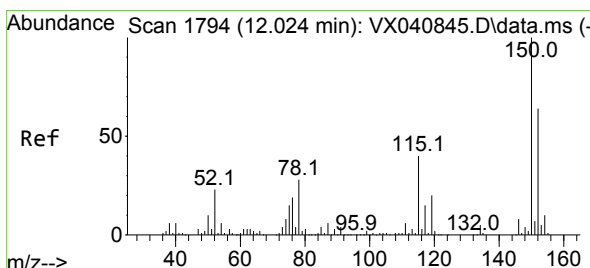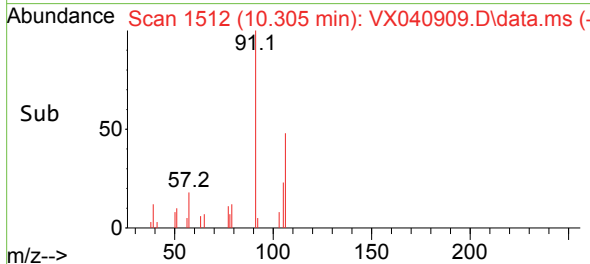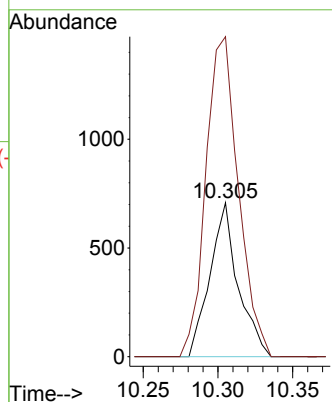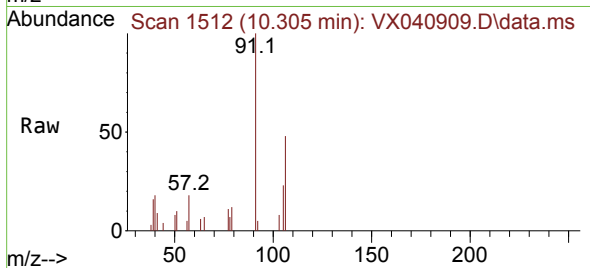

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion:152 Resp: 40106
Ion Ratio Lower Upper
152 100
115 65.4 43.3 129.9
150 156.2 0.0 345.0


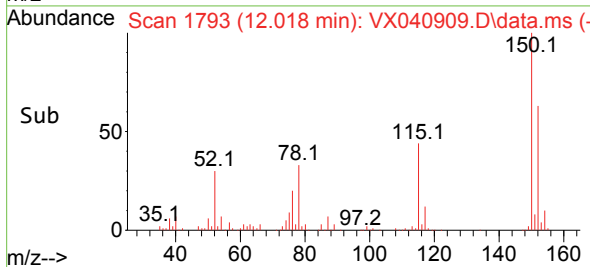
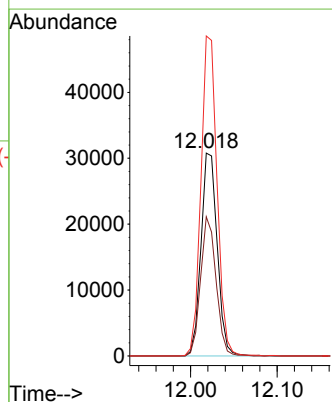
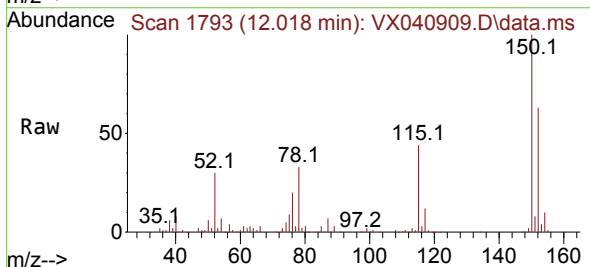




#74
N-amy1 acetate
Concen: 0.476 ug/l
RT: 10.774 min Scan# 1639
Delta R.T. -0.067 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion:	43	Resp:	675
Ion	Ratio	Lower	Upper
43	100		
70	0.0	32.9	49.3#
55	0.0	19.3	28.9#
61	0.0	18.8	28.2#

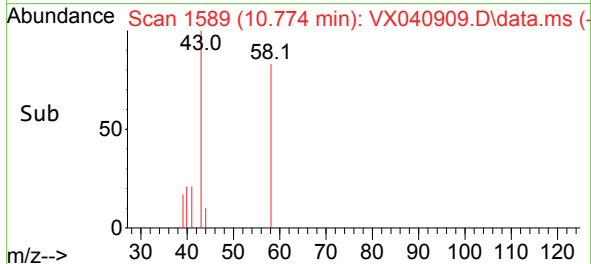

#76
1,2,3-Trichloropropane
Concen: 28.215 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion:	75	Resp:	24130
Ion	Ratio	Lower	Upper
75	100		
77	0.9	19.1	57.5#




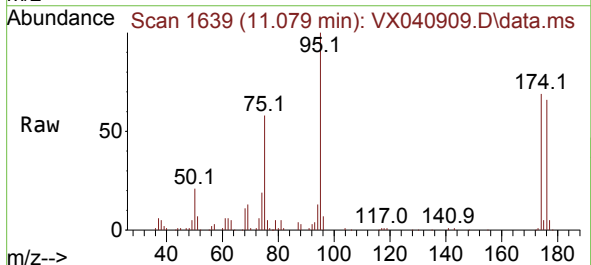




#81
trans-1,4-Dichloro-2-butene
Concen: 76.125 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17




Instrument :
MSVOA_X
ClientSampleId :
TP1


Tgt Ion: 75 Resp: 24130
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

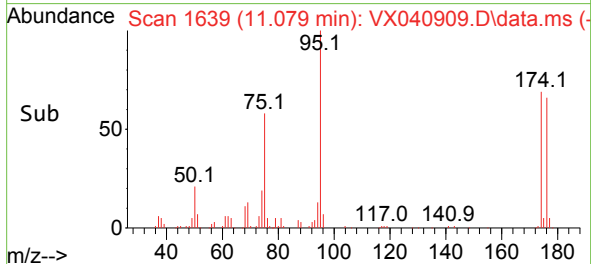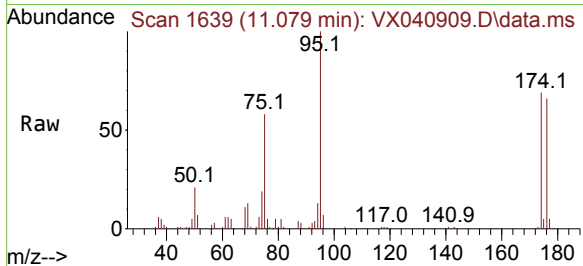

#93
1,2,4-Trichlorobenzene
Concen: 0.243 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX040909.D
Acq: 05 Apr 2024 17:17

Tgt Ion:180 Resp: 219
Ion Ratio Lower Upper
180 100
182 84.9 48.3 144.8
145 27.9 18.0 54.0

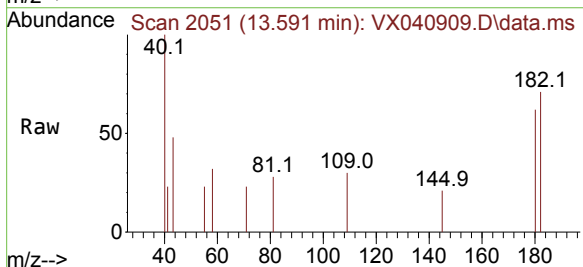



#94

Hexachlorobutadiene

Concen: 0.477 ug/l

RT: 13.725 min Scan# 2073

Delta R.T. 0.000 min

Lab File: VX040909.D


Acq: 05 Apr 2024 17:17

Instrument :




MSVOA_X

ClientSampleId :

TP1

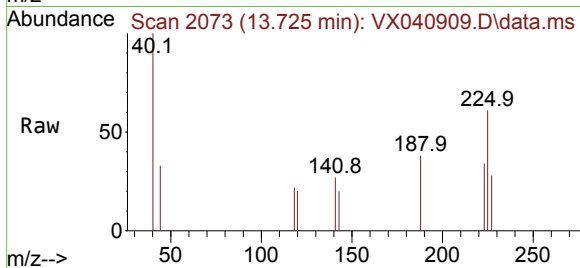

Tgt Ion:	225	Resp:	165
Ion Ratio	Lower	Upper	
225	100		
223	63.0	31.1	93.2
227	55.8	32.5	97.5

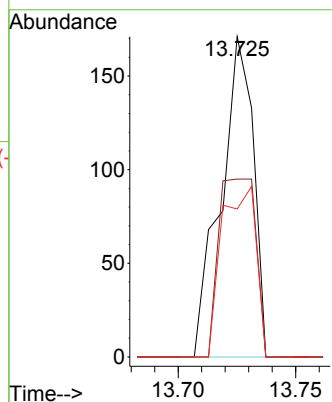

#95

Naphthalene

Concen: 0.236 ug/l




RT: 13.780 min Scan# 2082


Delta R.T. 0.006 min

Lab File: VX040909.D

Acq: 05 Apr 2024 17:17

Tgt Ion:	128	Resp:	685
Ion Ratio	Lower	Upper	
128	100		
127	7.7	10.3	15.5#
129	0.0	8.8	13.2#

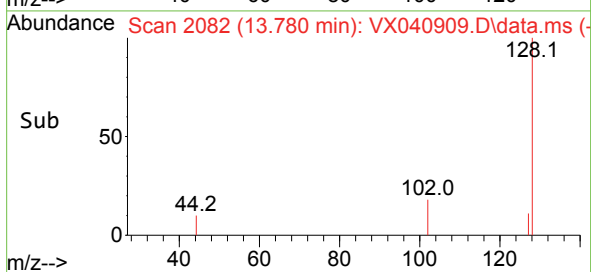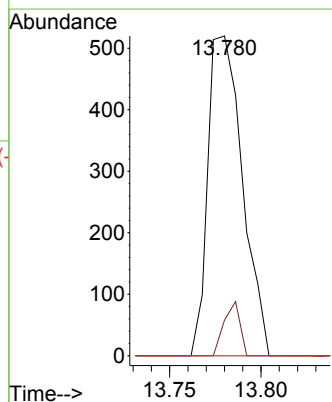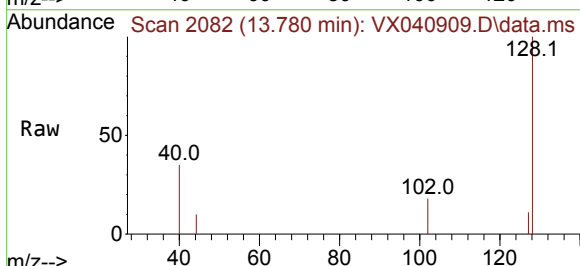



#96

1,2,3-Trichlorobenzene

Concen: 0.274 ug/l

RT: 13.969 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX040909.D


Acq: 05 Apr 2024 17:17

Instrument :

MSVOA_X

ClientSampleId :

TP1

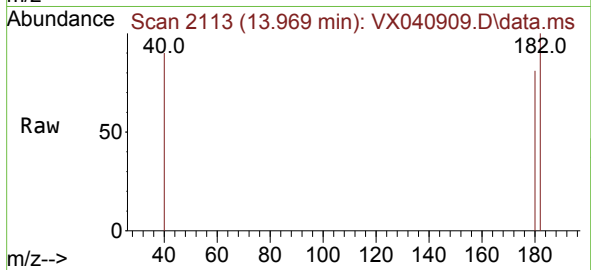

Tgt Ion:180 Resp: 236

Ion Ratio Lower Upper

180 100

182 105.1 46.9 140.6

145 24.2 17.8 53.5

