

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040619\
 Data File : VX008724.D
 Acq On : 06 Apr 2019 16:38
 Operator : JC/SP
 Sample : K2295-03 10X
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ST008MW026-190404

Quant Time: Apr 08 04:10:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	202674	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	333431	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	288381	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	120171	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	137627	46.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.12%	
35) Dibromofluoromethane	5.50	113	100199	47.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.00%	
50) Toluene-d8	8.71	98	416655	49.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.18%	
62) 4-Bromofluorobenzene	11.13	95	139260	46.26	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.52%	
Target Compounds						
27) cis-1,2-Dichloroethene	4.60	96	7725	2.651	ug/l	89
44) Trichloroethene	7.21	130	1984	0.785	ug/l	88
64) Tetrachloroethene	9.34	164	19305	9.035	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040619\
Data File : VX008724.D
Acq On : 06 Apr 2019 16:38
Operator : JC/SP
Sample : K2295-03 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ST008MW026-190404

Quant Time: Apr 08 04:10:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

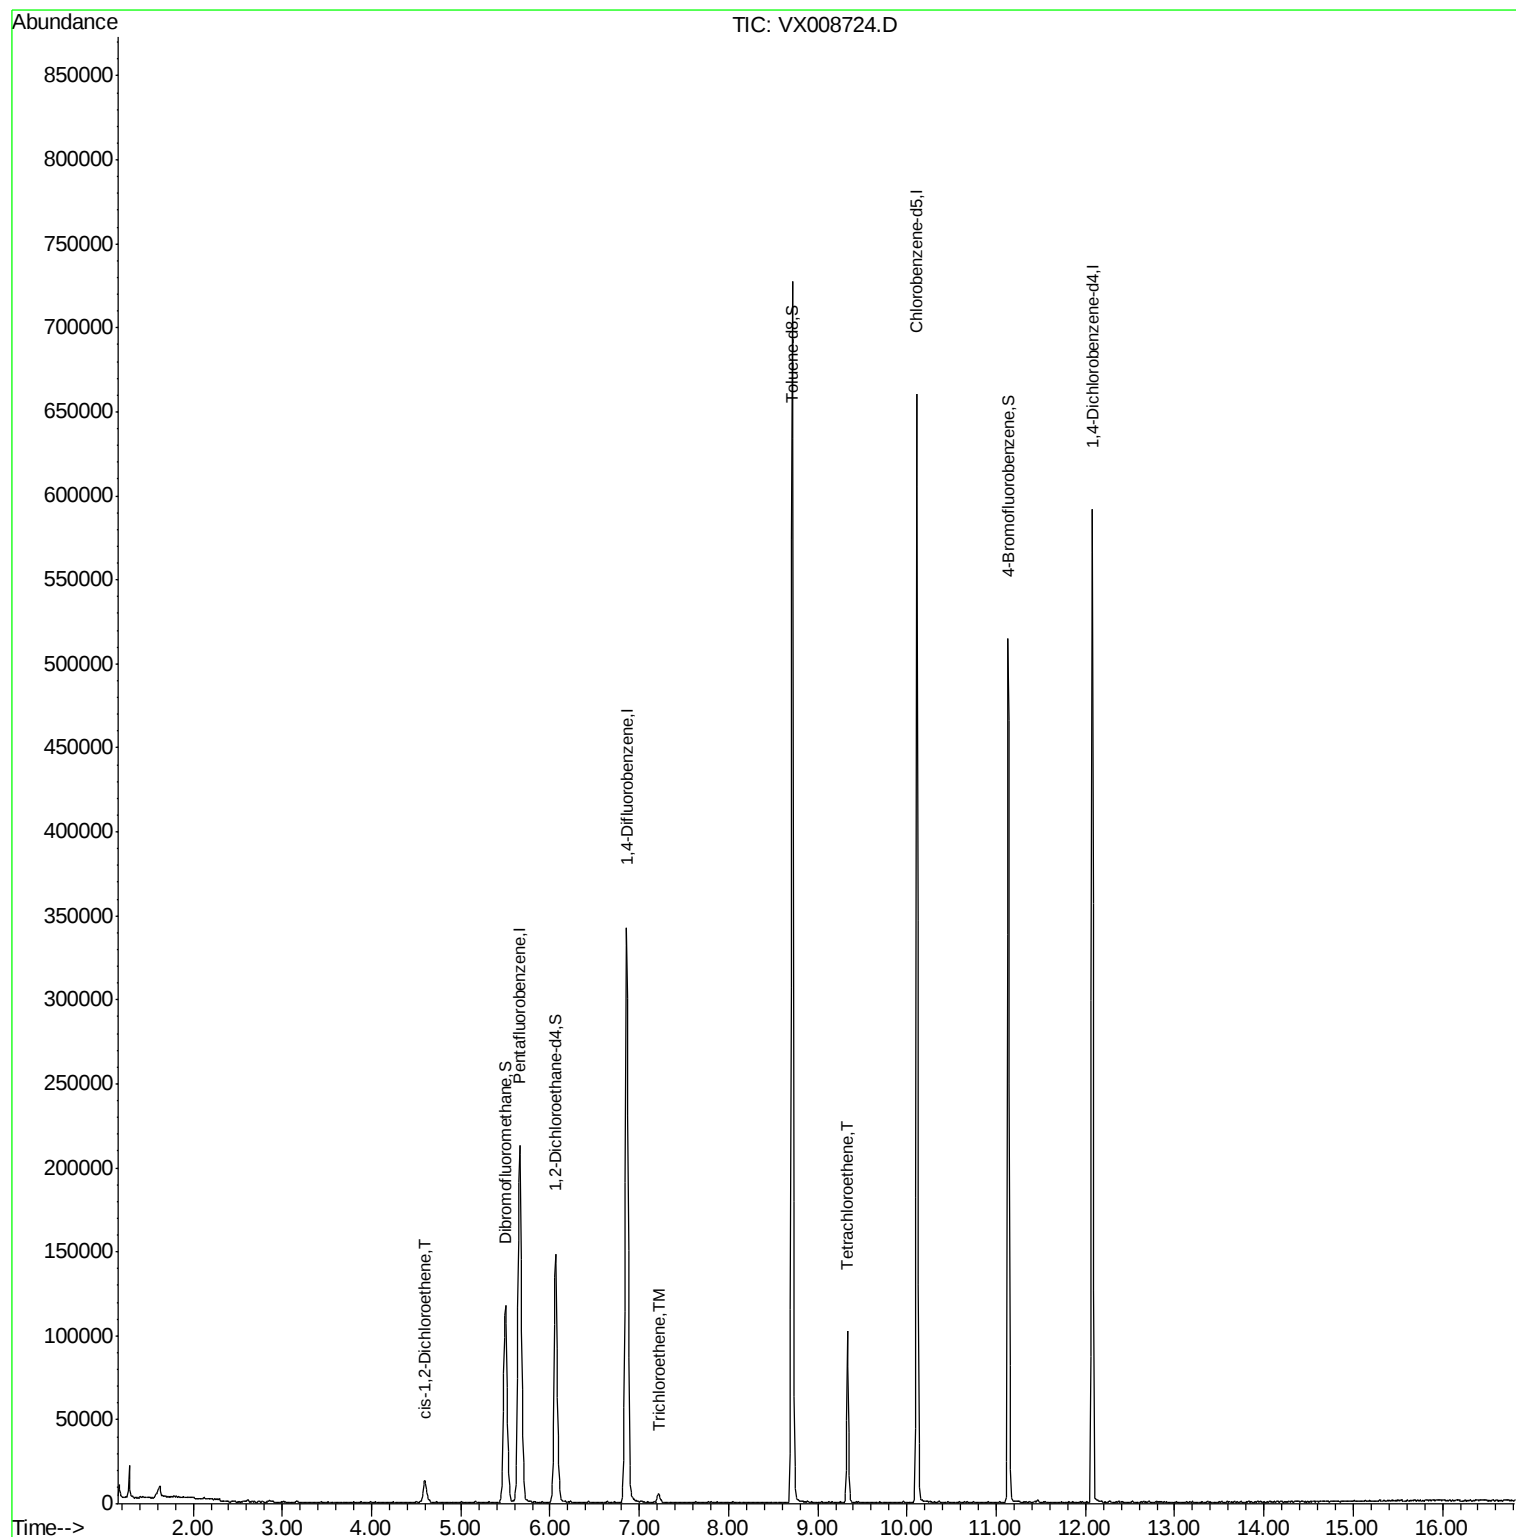

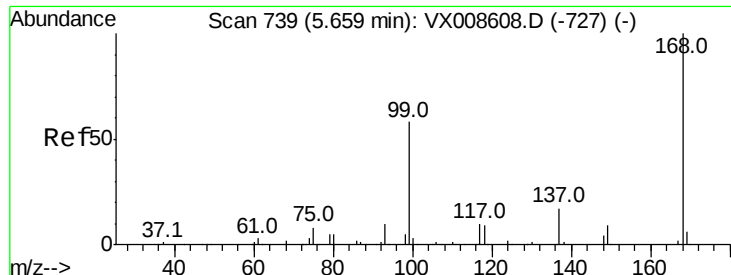

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38

Instrument :

MSVOA_X

ClientSampleId :


ST008MW026-190404

Tot Ion:168 Resp: 202674

Ion Ratio Lower Upper

168 100

99 56.4 46.7 70.1

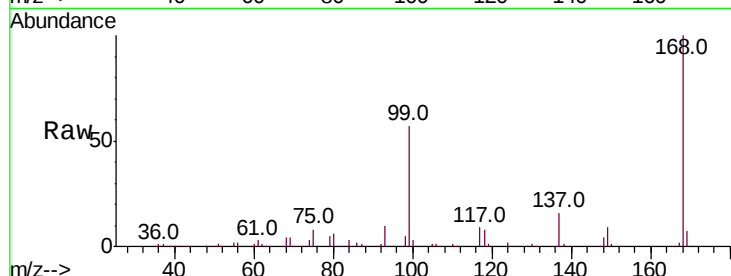

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

80000

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80 5.90

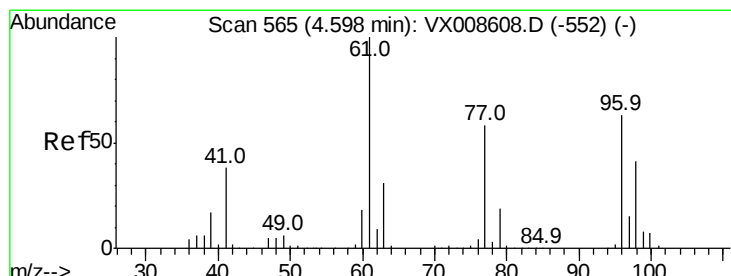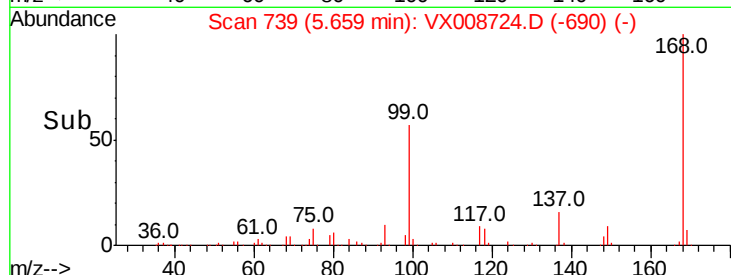

#27

cis-1,2-Dichloroethene

Concen: 2.651 ug/l

RT: 4.60 min Scan# 565

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38


Tgt Ion: 96 Resp: 7725

Ion Ratio Lower Upper

96 100

61 143.5 0.0 327.6

98 64.1 0.0 128.6

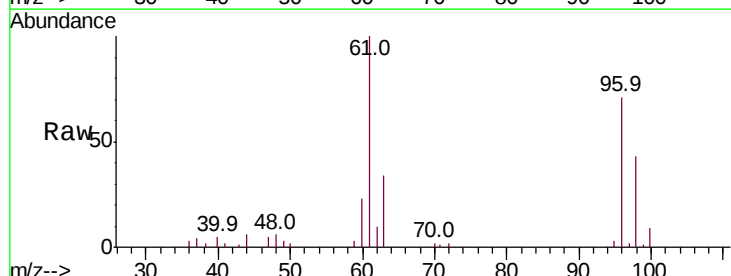

Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

5000

4000

3000


2000


1000

0

Time-->

4.50 4.60 4.70

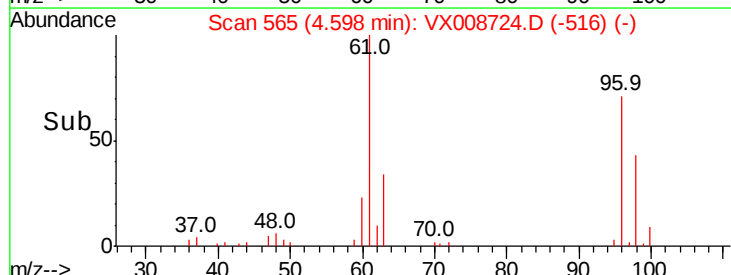

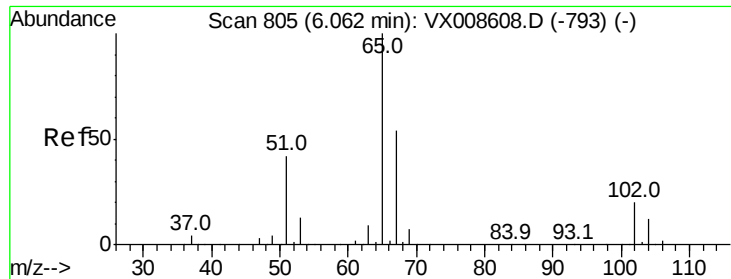

#33

1,2-Dichloroethane-d4

Concen: 46.557 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38

Instrument :

MSVOA_X

ClientSampleId :


ST008MW026-190404

Tot Ion: 65 Resp: 137627

Ion Ratio Lower Upper

65 100

67 54.3 0.0 107.2

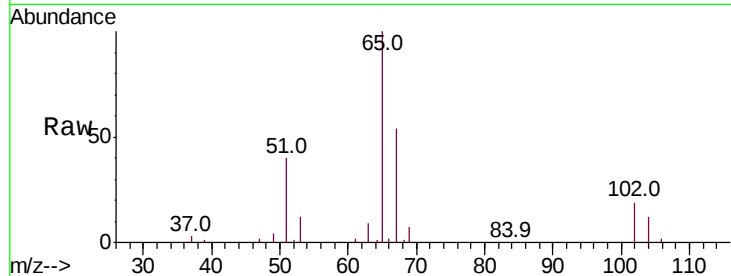

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

50000

40000



30000

20000

10000

0

Time--> 5.90 6.00 6.10 6.20

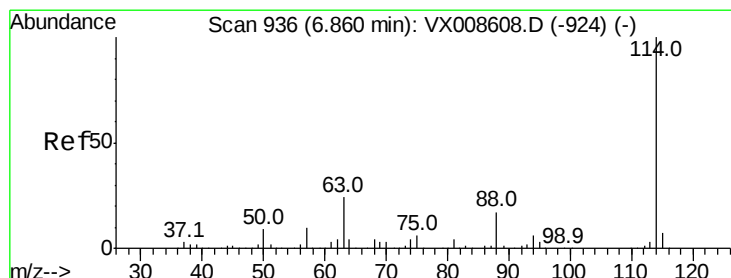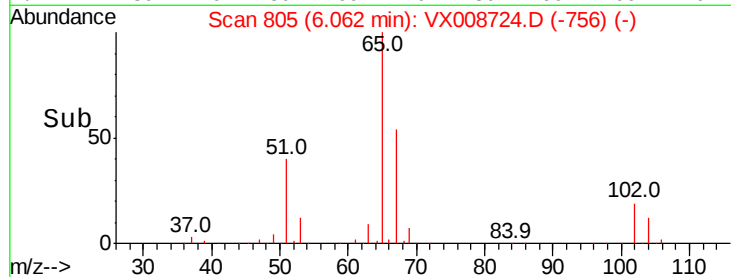

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38


Tgt Ion:114 Resp: 333431

Ion Ratio Lower Upper

114 100

63 23.7 0.0 47.2

88 16.6 0.0 34.0

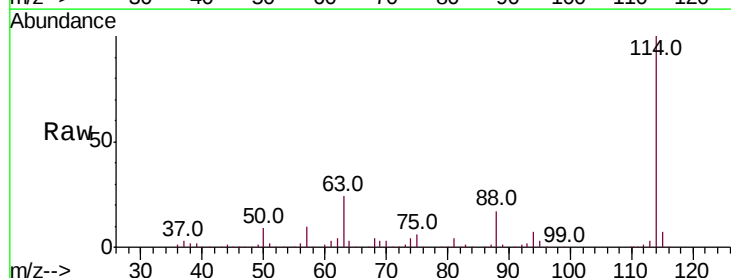

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.86


150000


100000

50000

0

Time--> 6.70 6.80 6.90 7.00

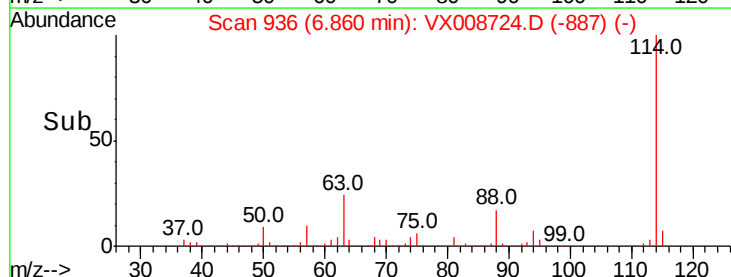

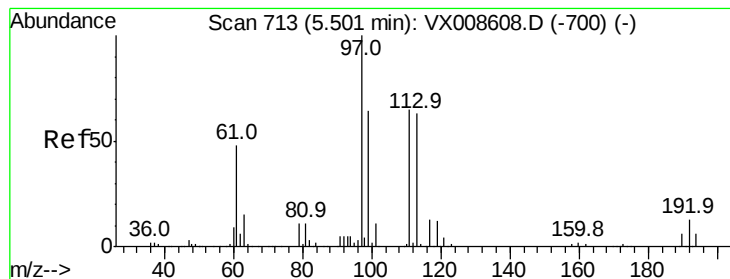

#35

Dibromofluoromethane

Concen: 47.001 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38

Instrument :

MSVOA_X

ClientSampleId :

ST008MW026-190404


Tot Ion:113 Resp: 100199

Ion Ratio Lower Upper

113 100

111 103.3 83.4 125.2




192 20.8 16.1 24.1

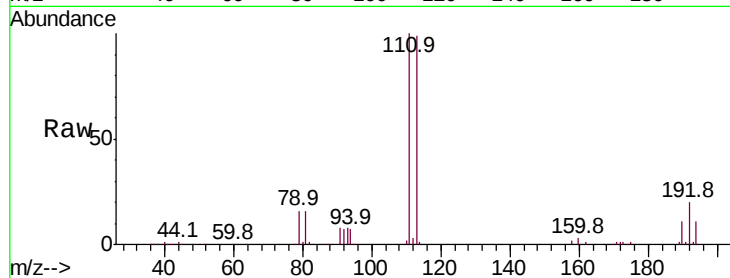

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

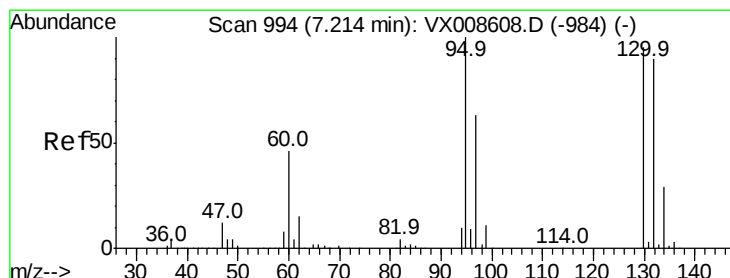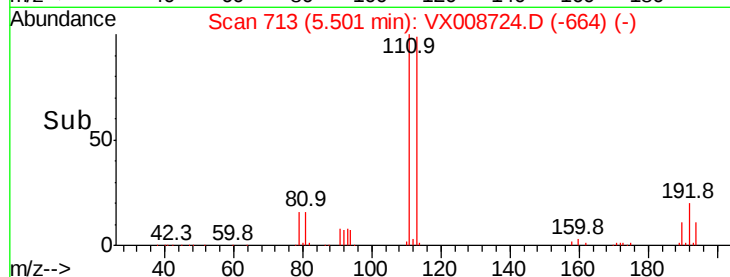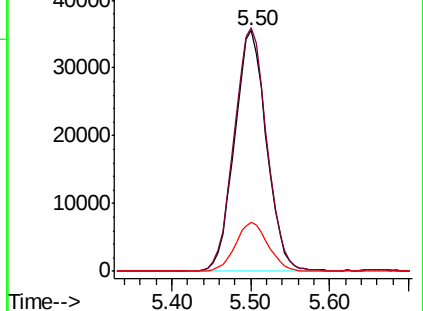

#44

Trichloroethene

Concen: 0.785 ug/l

RT: 7.21 min Scan# 994

Delta R.T. -0.00 min

Lab File: VX008724.D


Acq: 06 Apr 2019 16:38

Tgt Ion:130 Resp: 1984

Ion Ratio Lower Upper



130 100


95 92.5 0.0 209.8

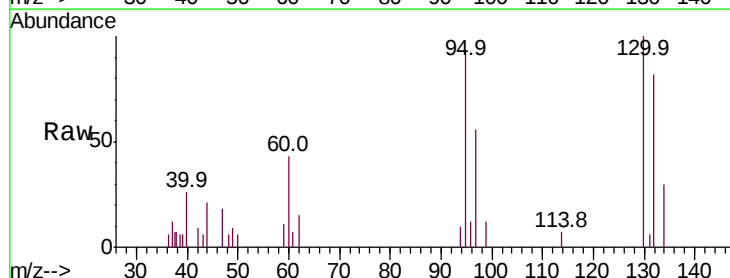

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): V

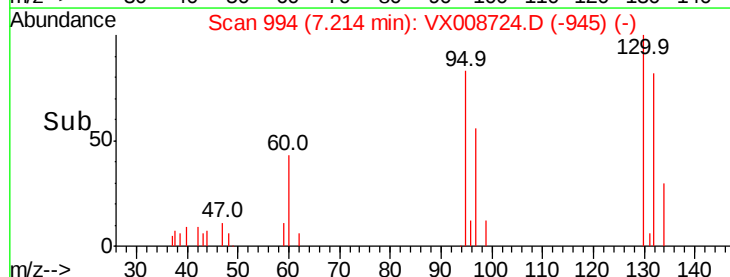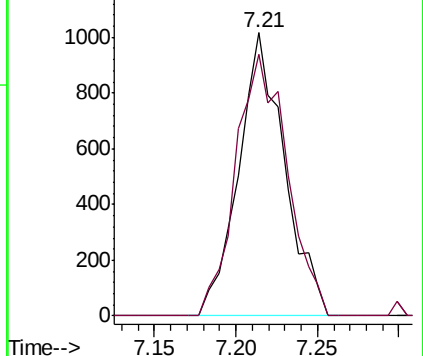

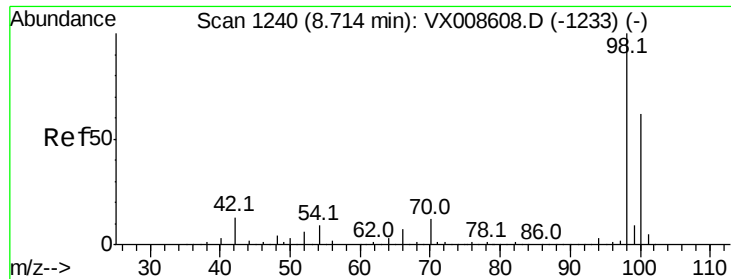

#50

Toluene-d8

Concen: 49.085 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38

Instrument :

MSVOA_X

ClientSampleId :


ST008MW026-190404

Tot Ion: 98 Resp: 416655

Ion Ratio Lower Upper

98 100

100 64.1 51.4 77.0

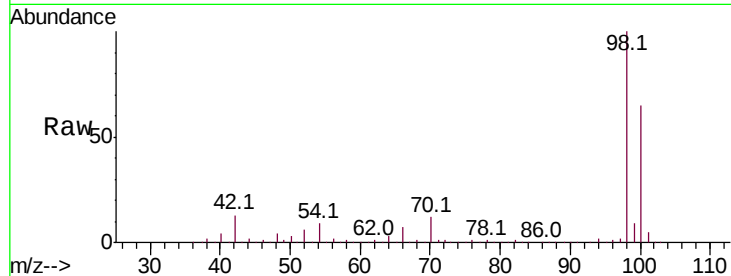

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V>

300000

250000

200000

150000

100000

50000



0

8.60

8.70

8.80

Time-->

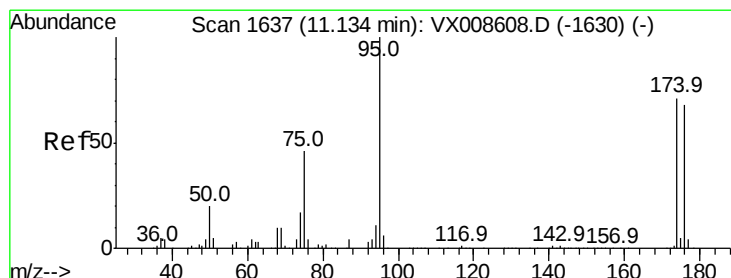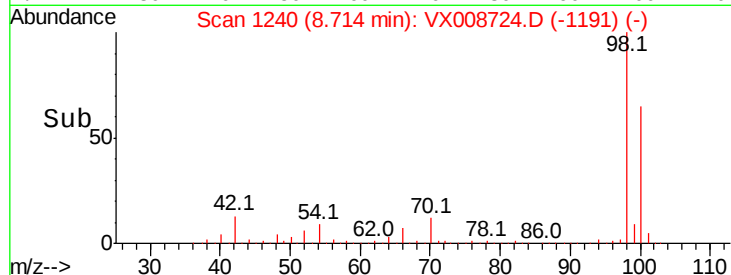

#62

4-Bromofluorobenzene

Concen: 46.264 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38


Tgt Ion: 95 Resp: 139260

Ion Ratio Lower Upper

95 100

174 77.2 0.0 151.8

176 75.7 0.0 145.8

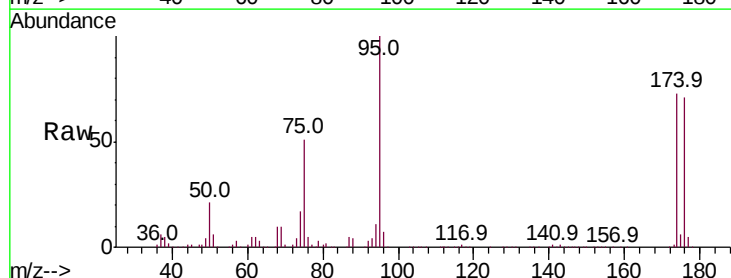

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

150000

100000


50000


0

11.10

11.20

Time-->

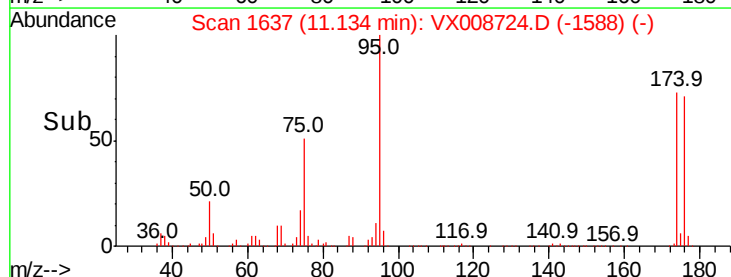


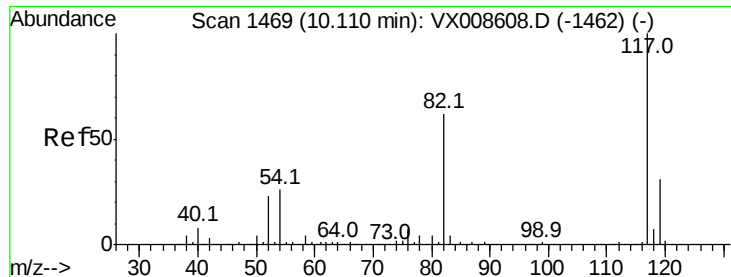




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX008724.D
Acq: 06 Apr 2019 16:38

Instrument :
MSVOA_X
ClientSampleId :
ST008MW026-190404

Tot Ion:117 Resp: 288381
Ion Ratio Lower Upper
117 100
82 61.2 49.6 74.4
119 31.4 25.0 37.4

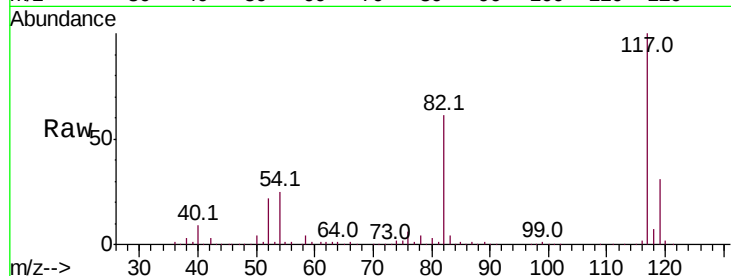


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

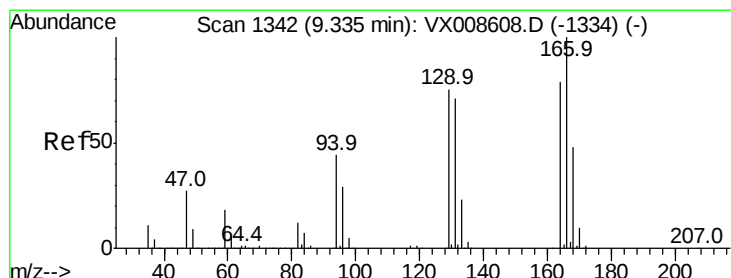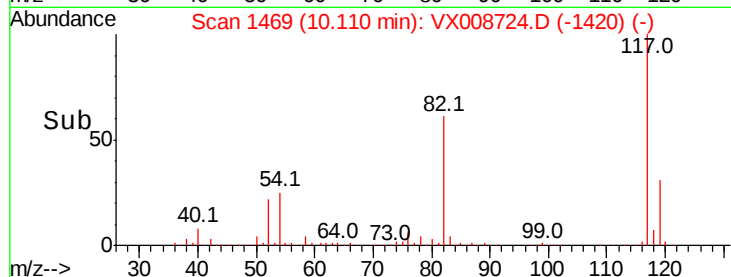
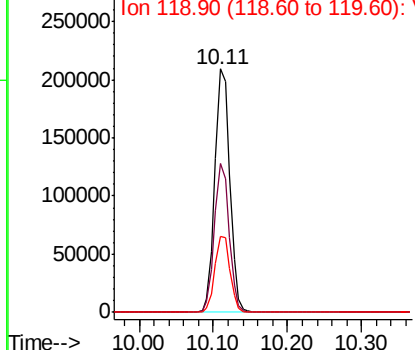



#64
Tetrachloroethene
Concen: 9.035 ug/l
RT: 9.34 min Scan# 1342
Delta R.T. -0.00 min
Lab File: VX008724.D
Acq: 06 Apr 2019 16:38

Tgt Ion:164 Resp: 19305
Ion Ratio Lower Upper
164 100
166 125.8 101.0 151.6
129 96.1 75.8 113.8
131 90.4 71.8 107.8

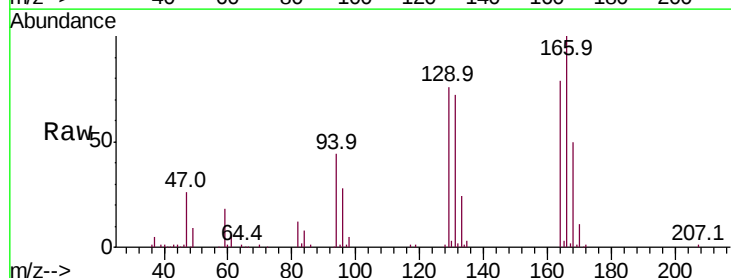

Abundance Ion 163.80 (163.50 to 164.50): V
Ion 165.80 (165.50 to 166.50): V
Ion 128.80 (128.50 to 129.50): V
Ion 130.80 (130.50 to 131.50): V

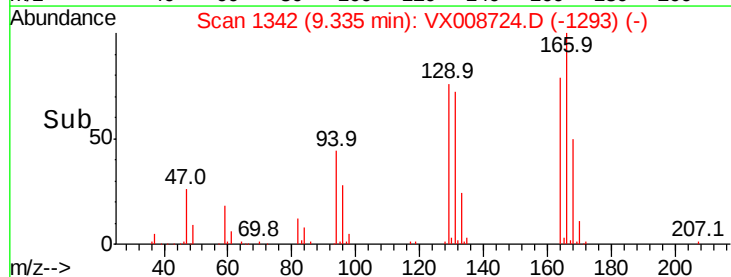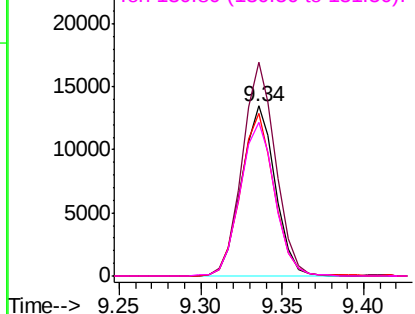

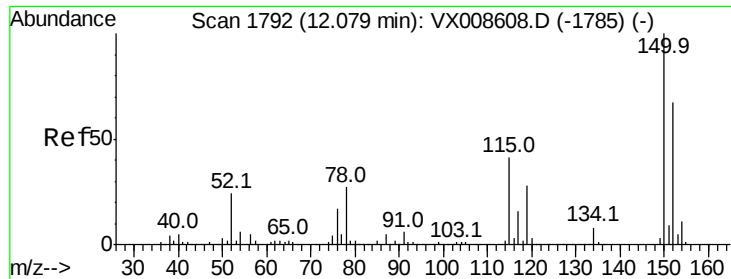

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX008724.D

Acq: 06 Apr 2019 16:38

Instrument :

MSVOA_X

ClientSampleId :

ST008MW026-190404


Tot Ion:152 Resp: 120171

Ion Ratio Lower Upper

152 100

115 59.5 43.5 130.5

150 156.1 0.0 348.8

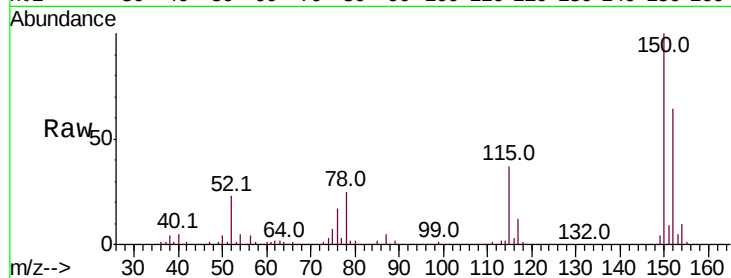

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

