

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040622\
 Data File : VX027996.D
 Acq On : 06 Apr 2022 14:27
 Operator : JC/MD
 Sample : N2253-02 200X
 Misc : 1.10g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 31292DL


Quant Time: Apr 07 08:06:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 05 15:58:31 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	109373	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	183523	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	166540	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	79164	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	71228	52.197	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 104.400%			
35) Dibromofluoromethane	5.391	113	58516	47.116	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 94.240%			
50) Toluene-d8	8.653	98	211099	46.522	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 93.040%			
62) 4-Bromofluorobenzene	11.079	95	88796	49.762	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 99.520%			
Target Compounds						
					Qvalue	
5) Bromomethane	1.617	94	147	0.330	ug/l #	74
6) Chloroethane	1.678	64	200	Below Cal	#	43
10) Methyl Iodide	2.459	142	119	3.593	ug/l #	41
16) Acetone	2.373	43	679	1.330	ug/l #	78
20) Methylene Chloride	2.788	84	323	0.282	ug/l #	83
31) Cyclohexane	5.501	56	1499	0.848	ug/l #	43
36) 1,1-Dichloropropene	5.556	75	8488	5.198	ug/l #	49
38) Carbon Tetrachloride	5.562	117	11098	6.116	ug/l #	16
39) Methylcyclohexane	7.372	83	1333	0.652	ug/l #	89
43) Isopropyl Acetate	6.184	43	760	0.294	ug/l #	56
51) 4-Methyl-2-Pentanone	8.653	43	908	0.536	ug/l #	1
52) Toluene	8.720	92	60752	19.449	ug/l	97
53) t-1,3-Dichloropropene	8.720	75	825	0.480	ug/l #	1
59) 2-Hexanone	9.384	43	414	0.316	ug/l #	18
67) Ethyl Benzene	10.195	91	1845	0.306	ug/l	95
68) m/p-Xylenes	10.305	106	2257	0.954	ug/l	94
69) o-Xylene	10.640	106	1262	0.551	ug/l	99
73) Isopropylbenzene	10.963	105	1267	0.229	ug/l	96
74) N-amyl acetate	10.854	43	537	0.279	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.213	83	898	0.494	ug/l #	25
76) 1,2,3-Trichloropropane	11.079	75	46415	28.557	ug/l #	38
78) n-propylbenzene	11.305	91	5043	0.800	ug/l	99
79) 2-Chlorotoluene	11.378	91	2033	0.513	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	5441	1.146	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.079	75	46415	90.028	ug/l #	15
82) 4-Chlorotoluene	11.457	91	939	0.207	ug/l #	45
83) tert-Butylbenzene	11.969	119	2530	0.529	ug/l	78
84) 1,2,4-Trimethylbenzene	11.756	105	20271	4.215	ug/l	97
85) sec-Butylbenzene	11.890	105	2561	0.438	ug/l	85
89) n-Butylbenzene	12.329	91	3192	0.759	ug/l #	64
90) Hexachloroethane	12.530	117	293	0.370	ug/l #	10
95) Naphthalene	13.780	128	1147	0.207	ug/l #	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 07 08:06:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 05 15:58:31 2022
Response via : Initial Calibration

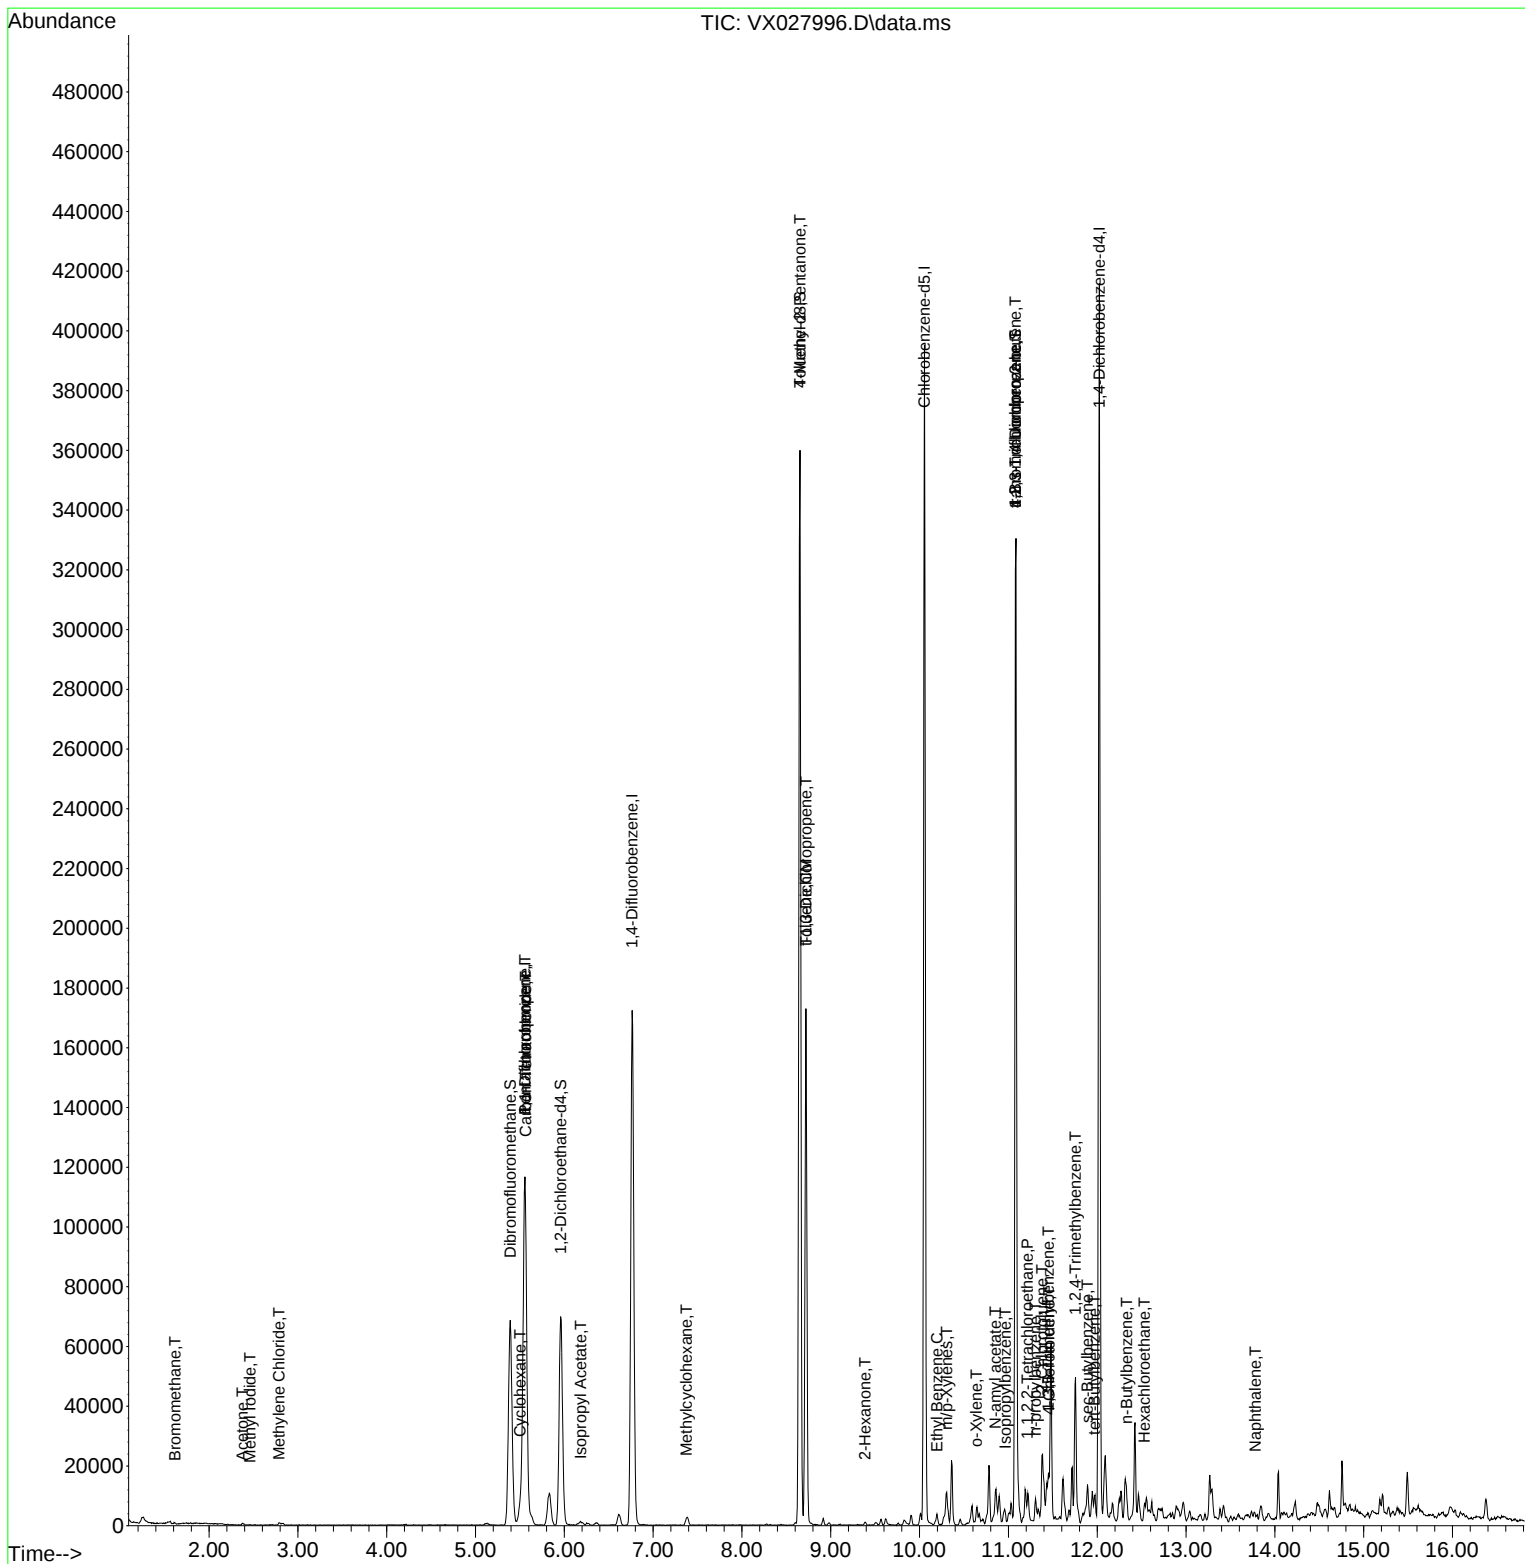




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Instrument :




MSVOA_X

ClientSampleId :

31292DL



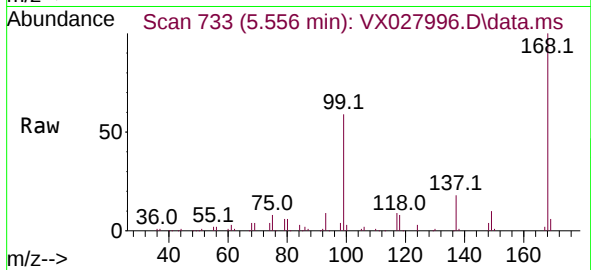



Tgt Ion:168 Resp: 109373
Ion Ratio Lower Upper
168 100
99 59.1 41.7 62.5

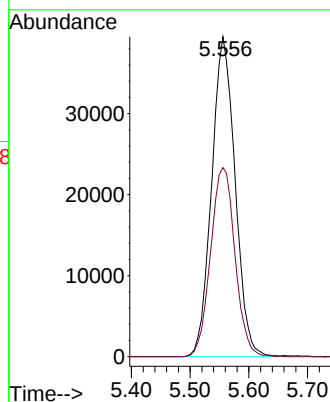

#5
Bromomethane
Concen: 0.330 ug/l
RT: 1.617 min Scan# 87
Delta R.T. 0.018 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 94 Resp: 147
Ion Ratio Lower Upper
94 100
96 68.9 75.3 112.9#




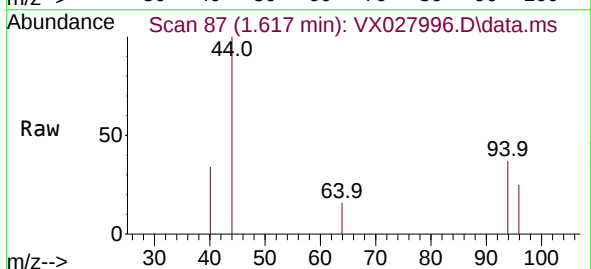


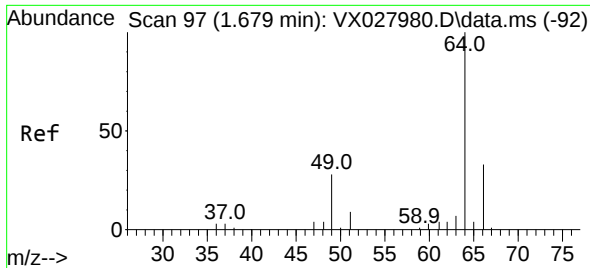

#6
Chloroethane
Concen: Below Cal
RT: 1.678 min Scan# 91
Delta R.T. -0.001 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 64 Resp: 200
Ion Ratio Lower Upper
64 100
66 0.0 25.3 37.9#

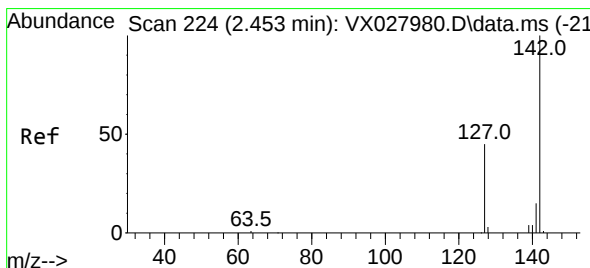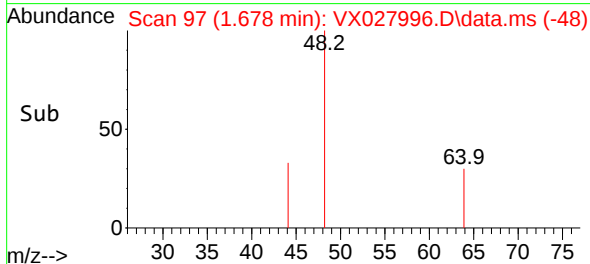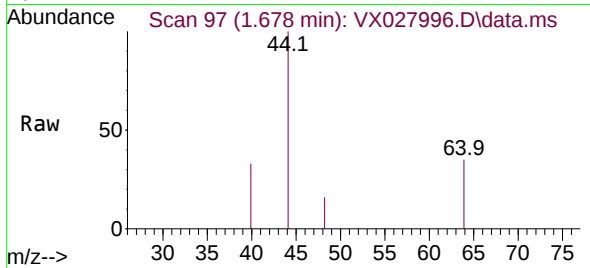

#10
Methyl Iodide
Concen: 3.593 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 142 Resp: 119
Ion Ratio Lower Upper
142 100
127 0.0 33.9 50.9#
141 0.0 11.4 17.2#

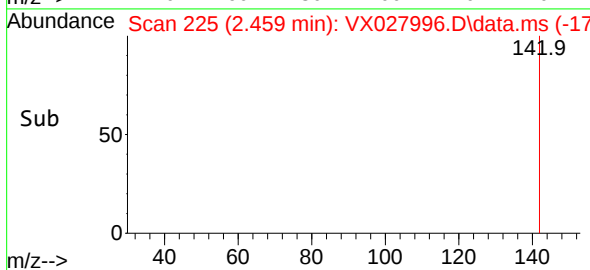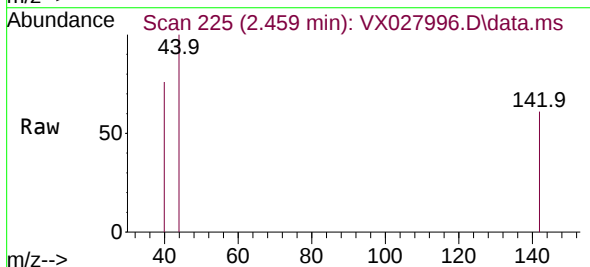



#16

Acetone

Concen: 1.330 ug/l

RT: 2.373 min Scan# 21

Delta R.T. -0.007 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Instrument :

MSVOA_X

ClientSampleId :





31292DL

Tgt Ion: 43 Resp: 679

Ion Ratio Lower Upper

43 100

58 23.1 28.8 43.2#

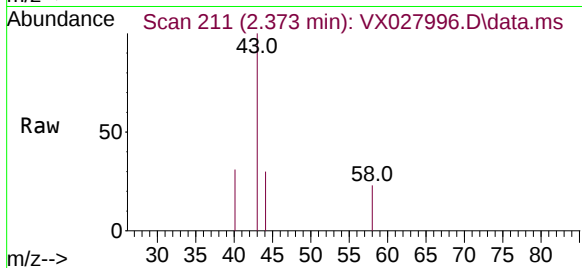

#20

Methylene Chloride

Concen: 0.282 ug/l

RT: 2.788 min Scan# 279

Delta R.T. -0.000 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Tgt Ion: 84 Resp: 323




Ion Ratio Lower Upper


84 100

49 95.1 85.5 128.3

51 0.0 26.6 39.8#

86 67.5 51.5 77.3




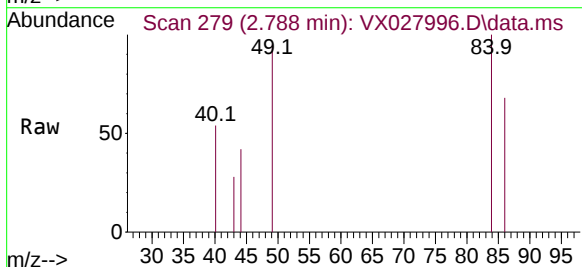




#31
Cyclohexane
Concen: 0.848 ug/l
RT: 5.501 min Scan# 719
Delta R.T. 0.030 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 56 Resp: 1499
Ion Ratio Lower Upper
56 100
69 14.8 26.7 40.1#
84 32.4 77.2 115.8#



#33
1,2-Dichloroethane-d4
Concen: 52.197 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 65 Resp: 71228
Ion Ratio Lower Upper
65 100
67 50.9 0.0 107.4


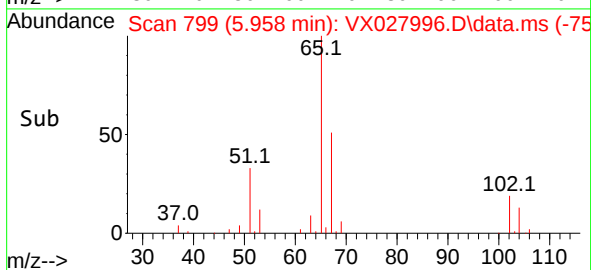






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion:114 Resp: 183523
Ion Ratio Lower Upper
114 100
63 18.9 0.0 36.8
88 16.3 0.0 32.4

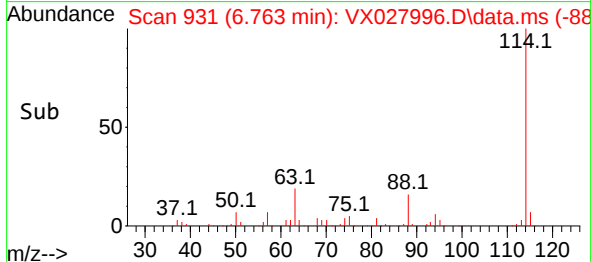

#35
Dibromofluoromethane
Concen: 47.116 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion:113 Resp: 58516
Ion Ratio Lower Upper
113 100
111 102.5 82.8 124.2
192 19.0 16.9 25.3




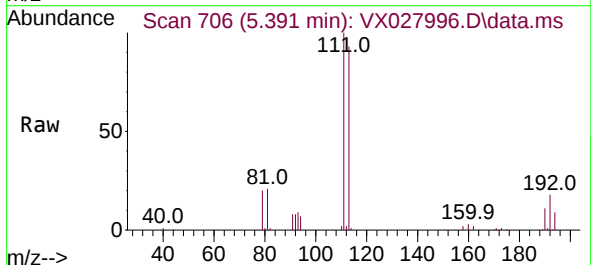




#36
1,1-Dichloropropene
Concen: 5.198 ug/l
RT: 5.556 min Scan# 714
Delta R.T. -0.140 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 75 Resp: 8488
Ion Ratio Lower Upper
75 100
110 9.4 18.3 54.8#
77 0.0 24.8 37.2#



#38
Carbon Tetrachloride
Concen: 6.116 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 117 Resp: 11098
Ion Ratio Lower Upper
117 100
119 4.9 77.3 115.9#
121 0.0 24.2 36.2#

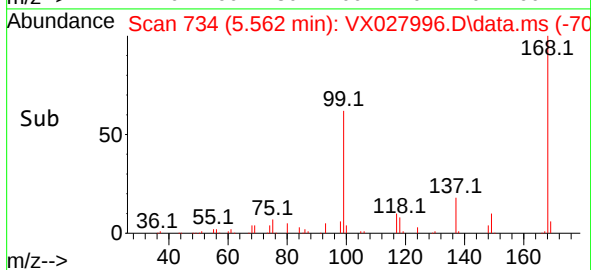

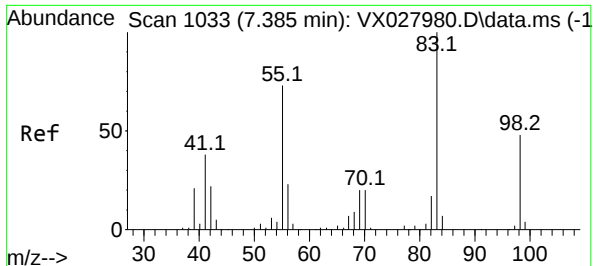

#39

Methylcyclohexane

Concen: 0.652 ug/l

RT: 7.372 min Scan# 1033

Delta R.T. -0.013 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Instrument :

MSVOA_X

ClientSampleId :

31292DL





Tgt Ion: 83 Resp: 1333

Ion Ratio Lower Upper

83 100

55 69.2 54.6 81.8

98 30.6 37.4 56.2#

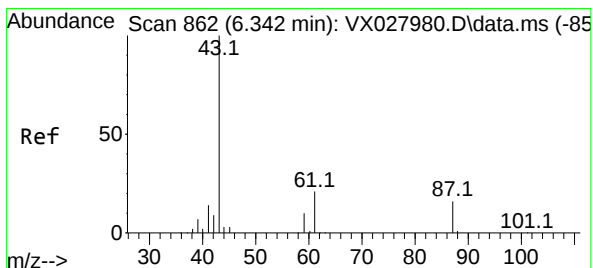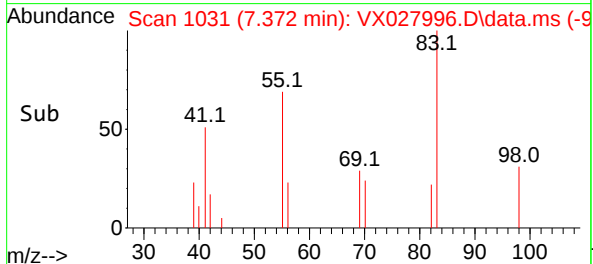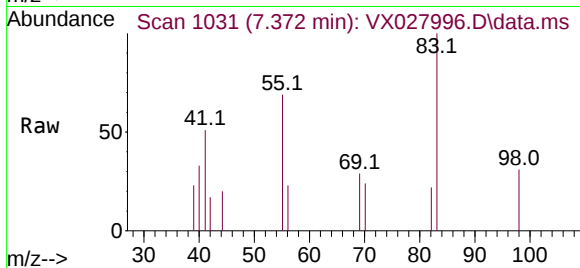

#43

Isopropyl Acetate

Concen: 0.294 ug/l

RT: 6.184 min Scan# 836

Delta R.T. -0.158 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27




Tgt Ion: 43 Resp: 760


Ion Ratio Lower Upper

43 100

61 0.0 18.5 27.7#

87 0.0 13.0 19.6#


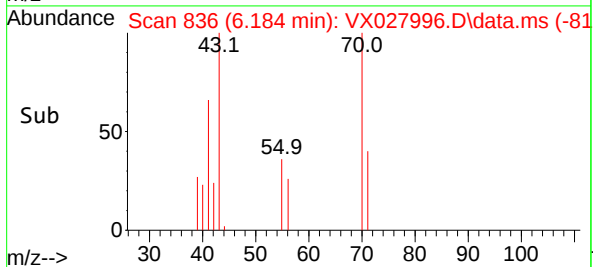

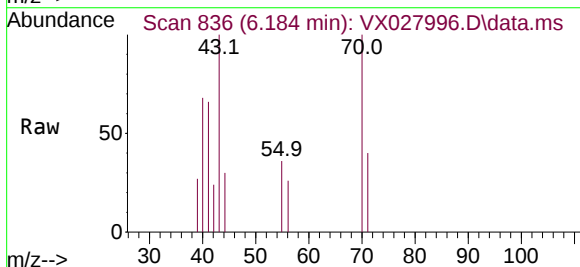


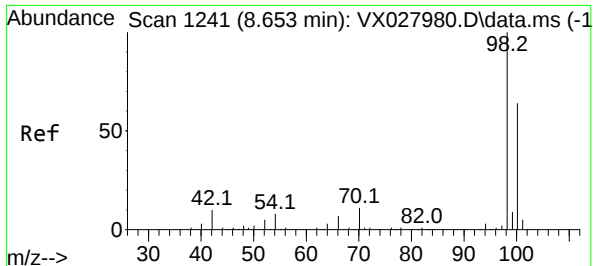

#50
Toluene-d8
Concen: 46.522 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 98 Resp: 211099
Ion Ratio Lower Upper
98 100
100 64.5 52.6 78.8

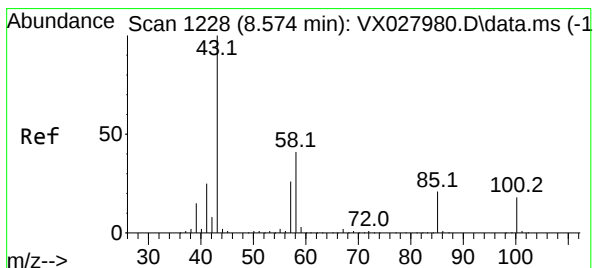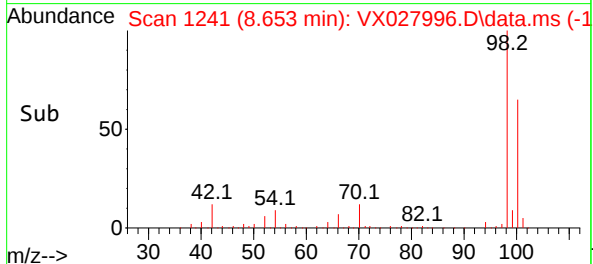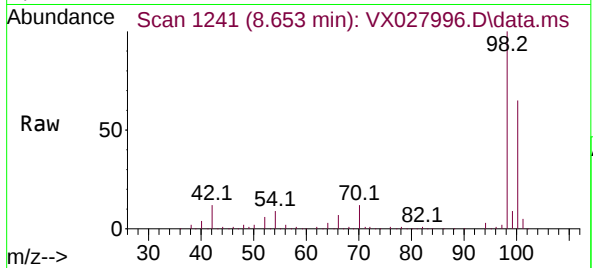

#51
4-Methyl-2-Pentanone
Concen: 0.536 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.079 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 43 Resp: 908
Ion Ratio Lower Upper
43 100
58 201.7 36.1 54.1#

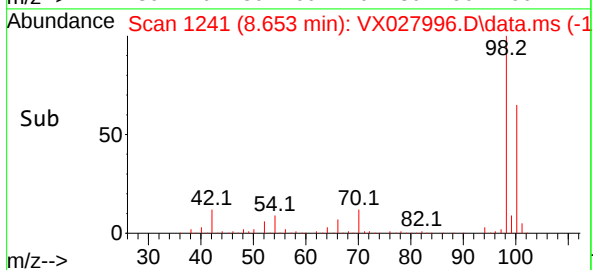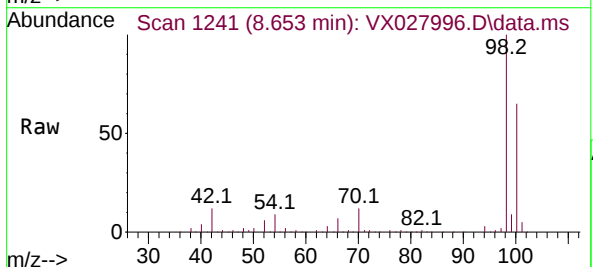



#52

Toluene

Concen: 19.449 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Instrument :

MSVOA_X

ClientSampleId :





31292DL

Tgt Ion: 92 Resp: 60752

Ion Ratio Lower Upper

92 100

91 175.4 137.5 206.3

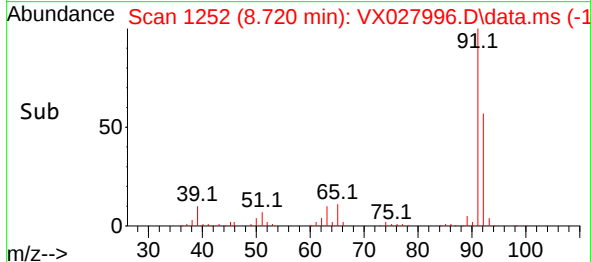

#53

t-1,3-Dichloropropene

Concen: 0.480 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.262 min

Lab File: VX027996.D




Acq: 06 Apr 2022 14:27


Tgt Ion: 75 Resp: 825

Ion Ratio Lower Upper

75 100

77 174.8 25.4 38.0#

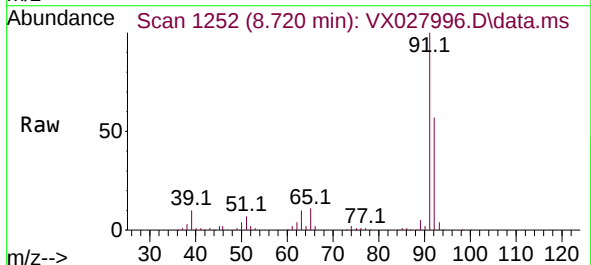

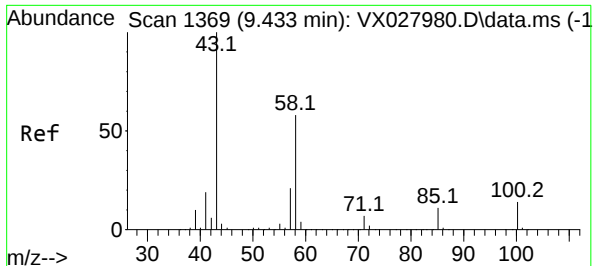

#59

2-Hexanone

Concen: 0.316 ug/l

RT: 9.384 min Scan# 11

Delta R.T. -0.049 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Instrument :

MSVOA_X

ClientSampleId :





31292DL

Tgt Ion: 43 Resp: 414

Ion Ratio Lower Upper

43 100

58 0.0 31.9 95.7#

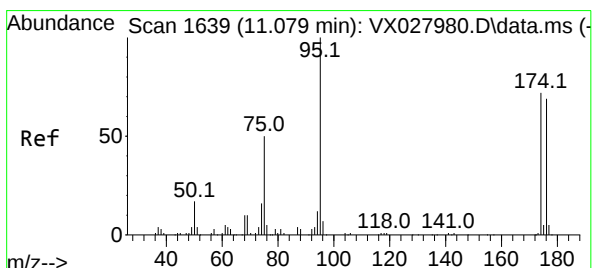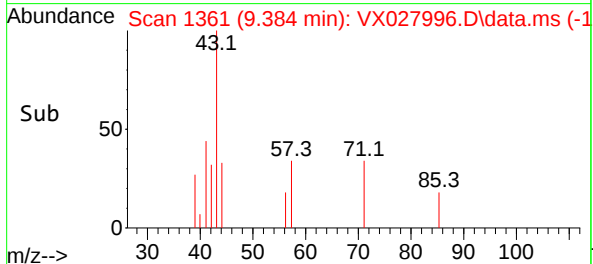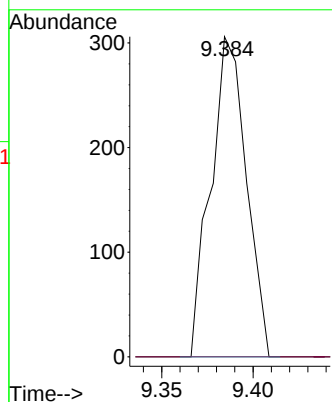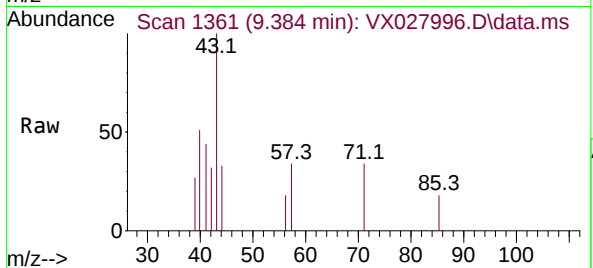

#62

4-Bromofluorobenzene

Concen: 49.762 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27




Tgt Ion: 95 Resp: 88796


Ion Ratio Lower Upper

95 100

174 71.5 0.0 163.0

176 68.5 0.0 155.0


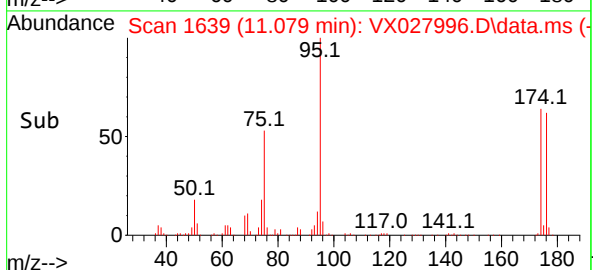

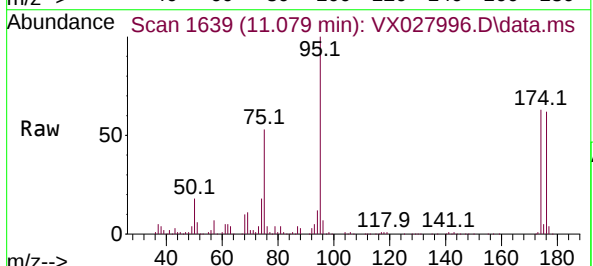




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion:117 Resp: 166540
Ion Ratio Lower Upper
117 100
82 60.6 41.8 62.8
119 33.3 24.8 37.2

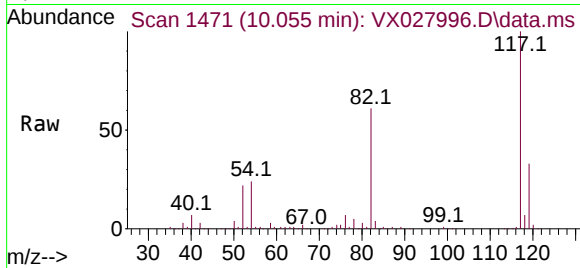

#67
Ethyl Benzene
Concen: 0.306 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 91 Resp: 1845
Ion Ratio Lower Upper
91 100
106 27.8 24.6 36.8


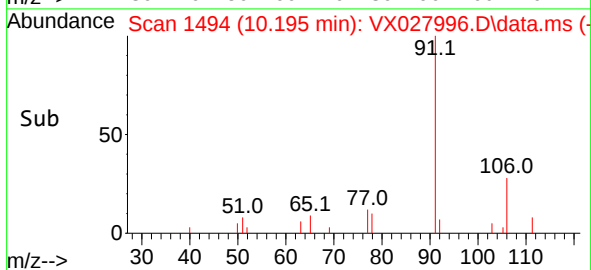

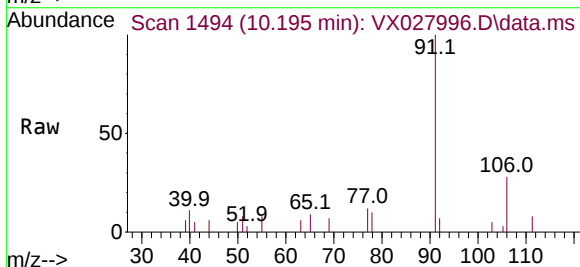




#68
m/p-Xylenes
Concen: 0.954 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion:106 Resp: 2257
Ion Ratio Lower Upper
106 100
91 209.3 160.4 240.6



#69
o-Xylene
Concen: 0.551 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion:106 Resp: 1262
Ion Ratio Lower Upper
106 100
91 213.2 106.1 318.1


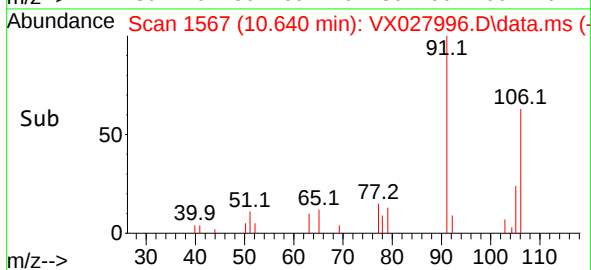






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion:152 Resp: 79164
Ion Ratio Lower Upper
152 100
115 64.4 37.5 112.7
150 157.5 0.0 338.2

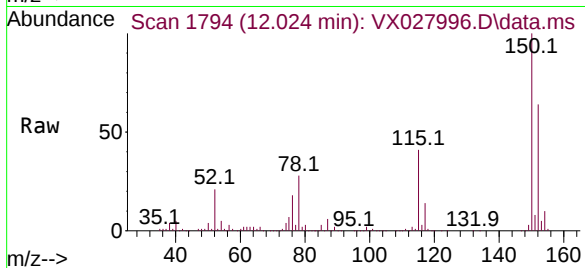

#73
Isopropylbenzene
Concen: 0.229 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion:105 Resp: 1267
Ion Ratio Lower Upper
105 100
120 29.0 13.5 40.5




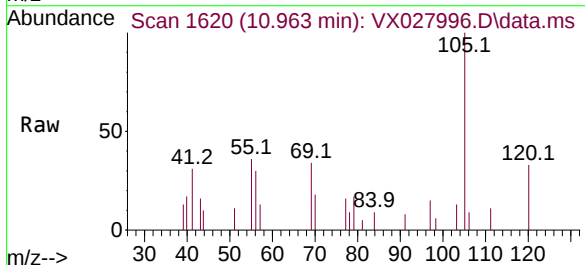




#74
N-amy1 acetate
Concen: 0.279 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.006 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 43	Resp: 537
Ion Ratio	Lower Upper
43 100	
70 94.8	42.5 63.7#
55 507.4	23.1 34.7#
61 0.0	22.8 34.2#



#75
1,1,2,2-Tetrachloroethane
Concen: 0.494 ug/l
RT: 11.213 min Scan# 1661
Delta R.T. 0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 83	Resp: 898
Ion Ratio	Lower Upper
83 100	
131 0.0	5.1 15.3#
85 0.0	32.6 97.7#


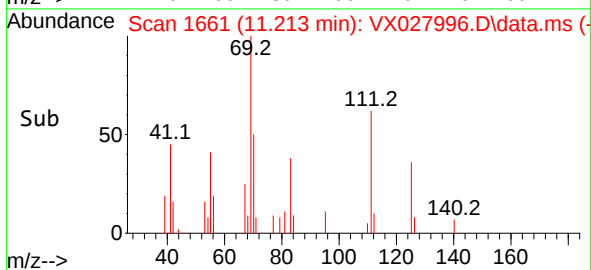






#76
1,2,3-Trichloropropane
Concen: 28.557 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 75 Resp: 46415
Ion Ratio Lower Upper
75 100
77 1.2 19.4 58.2#

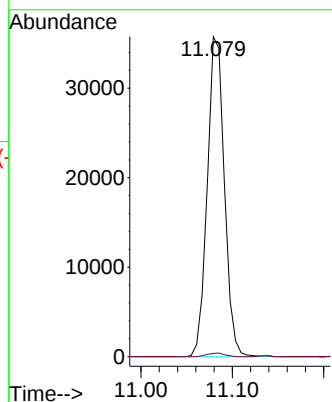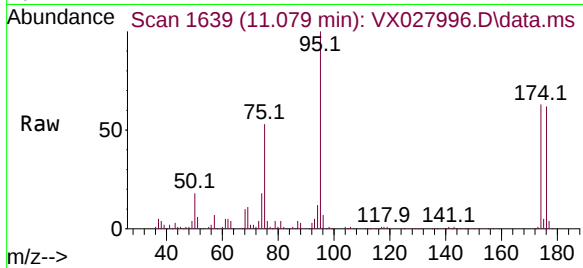

#78
n-propylbenzene
Concen: 0.800 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 91 Resp: 5043
Ion Ratio Lower Upper
91 100
120 22.5 11.6 34.8

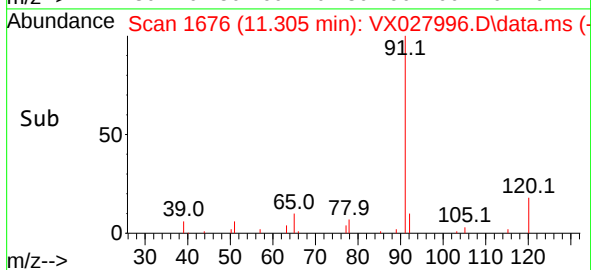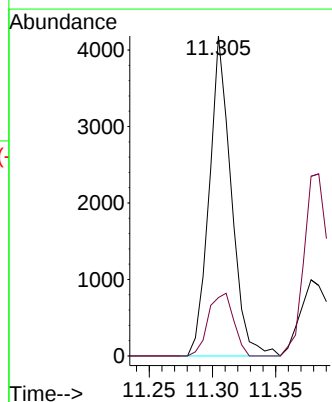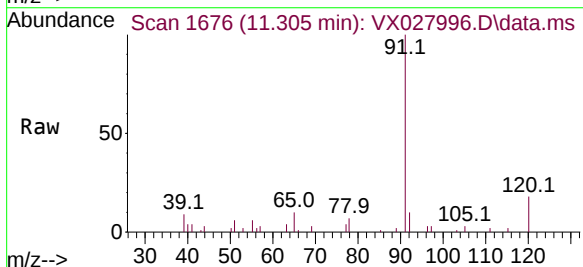



#79

2-Chlorotoluene

Concen: 0.513 ug/l

RT: 11.378 min Scan# 1

Delta R.T. 0.012 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Instrument :

MSVOA_X

ClientSampleId :





31292DL

Tgt Ion: 91 Resp: 2033

Ion Ratio Lower Upper

91 100

126 0.0 17.3 51.9#

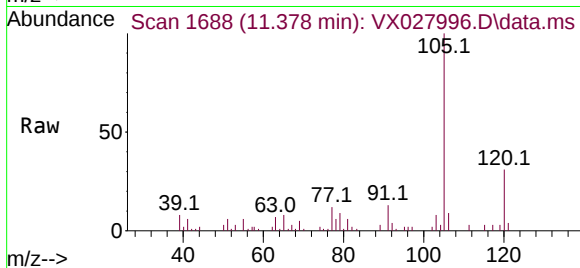

#80

1,3,5-Trimethylbenzene

Concen: 1.146 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. 0.000 min

Lab File: VX027996.D




Acq: 06 Apr 2022 14:27


Tgt Ion: 105 Resp: 5441

Ion Ratio Lower Upper

105 100

120 45.5 24.3 72.9




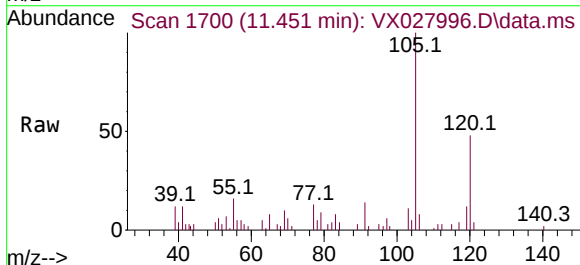




#81
trans-1,4-Dichloro-2-butene
Concen: 90.028 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27




Instrument :
MSVOA_X
ClientSampleId :
31292DL


Tgt Ion: 75 Resp: 46415
Ion Ratio Lower Upper
75 100
53 0.7 69.0 103.4#
89 0.0 37.0 55.6#

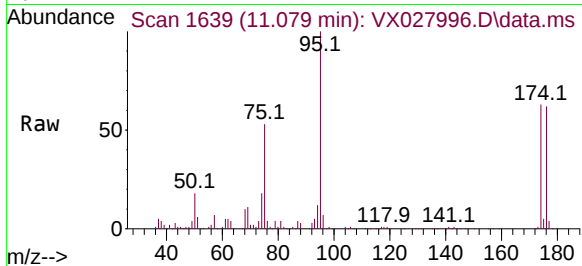

#82
4-Chlorotoluene
Concen: 0.207 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion: 91 Resp: 939
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

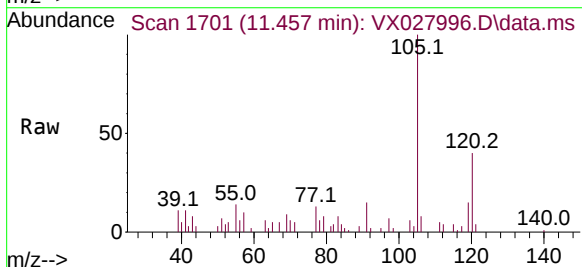



#83

tert-Butylbenzene

Concen: 0.529 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. 0.250 min

Lab File: VX027996.D

Acq: 06 Apr 2022 14:27

Instrument :

MSVOA_X

ClientSampleId :

31292DL





Tgt Ion:119 Resp: 2530

Ion Ratio Lower Upper

119 100

91 36.1 26.9 80.6

134 30.2 11.4 34.2

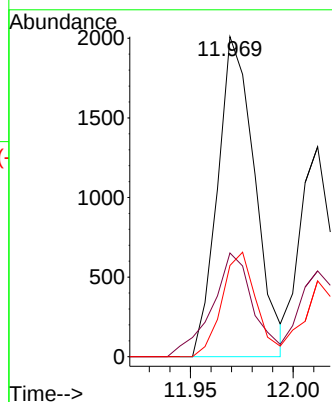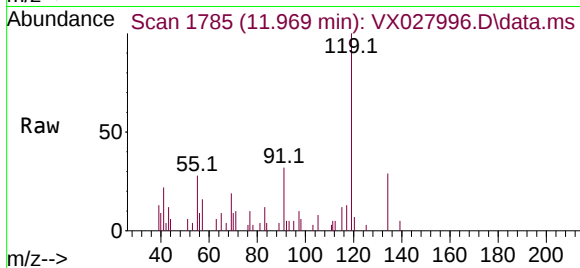

#84

1,2,4-Trimethylbenzene

Concen: 4.215 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. -0.000 min

Lab File: VX027996.D




Acq: 06 Apr 2022 14:27


Tgt Ion:105 Resp: 20271

Ion Ratio Lower Upper

105 100

120 43.4 22.6 67.8


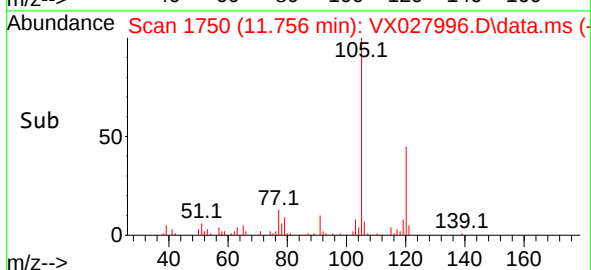

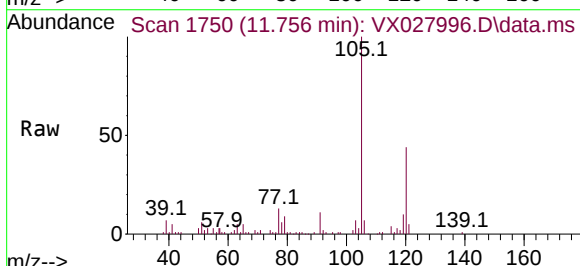




#85
 sec-Butylbenzene
 Concen: 0.438 ug/l
 RT: 11.890 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX027996.D
 Acq: 06 Apr 2022 14:27




Instrument :
 MSVOA_X
 ClientSampleId :
 31292DL


Tgt Ion:105 Resp: 2561
 Ion Ratio Lower Upper
 105 100
 134 27.3 10.2 30.4

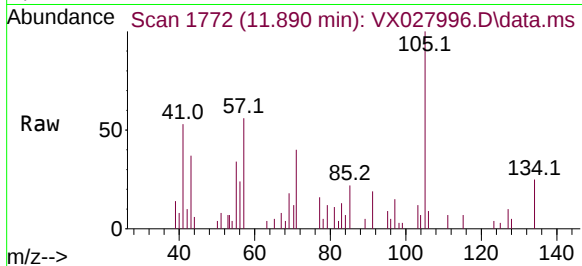

#89
 n-Butylbenzene
 Concen: 0.759 ug/l
 RT: 12.329 min Scan# 1844
 Delta R.T. -0.006 min
 Lab File: VX027996.D
 Acq: 06 Apr 2022 14:27

Tgt Ion: 91 Resp: 3192
 Ion Ratio Lower Upper
 91 100
 92 41.4 27.8 83.3
 134 62.2 13.3 39.8#




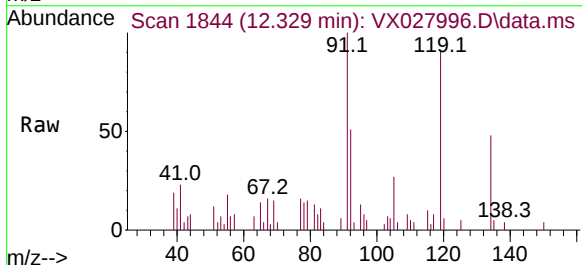




#90
Hexachloroethane
Concen: 0.370 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Instrument :
MSVOA_X
ClientSampleId :
31292DL

Tgt Ion:117 Resp: 293
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

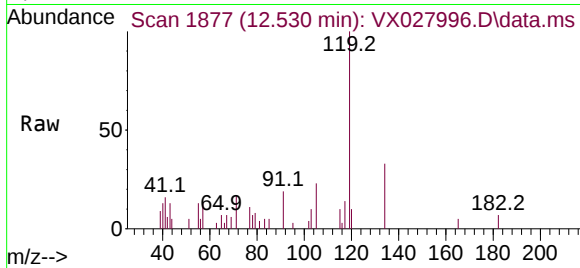

#95
Naphthalene
Concen: 0.207 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX027996.D
Acq: 06 Apr 2022 14:27

Tgt Ion:128 Resp: 1147
Ion Ratio Lower Upper
128 100
127 14.3 10.2 15.4
129 18.4 8.7 13.1#

