

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040622\
 Data File : VX027994.D
 Acq On : 06 Apr 2022 13:41
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
 Title : SW846 8260

Signal : TIC: VX027994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	695	705	719	rBV	66163	193246	34.51%	4.970%
2	5.556	719	733	750	rVB	113065	328419	58.65%	8.447%
3	5.958	788	799	815	rBV	71770	193232	34.51%	4.970%
4	6.763	922	931	947	rBV	175455	419894	74.98%	10.800%
5	8.653	1234	1241	1248	rBV	353624	560010	100.00%	14.404%
6	8.720	1248	1252	1263	rVB	33022	50696	9.05%	1.304%
7	10.055	1465	1471	1485	rVB	392560	510647	91.19%	13.134%
8	10.360	1517	1521	1525	rBV	8162	10163	1.81%	0.261%
9	10.781	1582	1590	1595	rBV	11749	16415	2.93%	0.422%
10	10.860	1595	1603	1606	rVV3	3992	7680	1.37%	0.198%
11	10.896	1606	1609	1615	rVB2	5205	7084	1.26%	0.182%
12	11.085	1634	1640	1650	rVB	337923	444108	79.30%	11.423%
13	11.195	1650	1658	1661	rBV	9139	15065	2.69%	0.387%
14	11.384	1685	1689	1693	rBV4	4330	6936	1.24%	0.178%
15	11.433	1693	1697	1700	rVV3	5629	9371	1.67%	0.241%
16	11.482	1700	1705	1711	rVB	52961	69151	12.35%	1.779%
17	11.634	1722	1730	1734	rVB6	3684	8054	1.44%	0.207%
18	11.719	1740	1744	1747	rBV	18273	21199	3.79%	0.545%
19	11.756	1747	1750	1754	rVB	8361	10504	1.88%	0.270%
20	11.890	1766	1772	1777	rVB7	7522	11777	2.10%	0.303%
21	11.945	1777	1781	1784	rBV4	4948	7604	1.36%	0.196%
22	12.024	1789	1794	1800	rVV	409785	521924	93.20%	13.424%
23	12.079	1800	1803	1805	rVV4	6952	10190	1.82%	0.262%
24	12.103	1805	1807	1812	rVB2	8329	8659	1.55%	0.223%
25	12.171	1812	1818	1826	rVB2	6827	13079	2.34%	0.336%
26	12.268	1826	1834	1838	rBV7	3142	8594	1.53%	0.221%
27	12.317	1838	1842	1848	rBV6	4727	8843	1.58%	0.227%
28	12.427	1848	1860	1864	rBV	37672	48773	8.71%	1.254%
29	12.469	1864	1867	1873	rVB6	4139	7159	1.28%	0.184%
30	12.555	1875	1881	1884	rBV6	3737	7948	1.42%	0.204%
31	12.890	1930	1936	1943	rBV6	5220	12857	2.30%	0.331%
32	12.975	1947	1950	1957	rVB8	3730	5942	1.06%	0.153%
33	13.268	1993	1998	2001	rBV	16437	19859	3.55%	0.511%
34	13.298	2001	2003	2007	rVB5	5049	6000	1.07%	0.154%
35	13.420	2020	2023	2033	rVB8	3202	6918	1.24%	0.178%
36	13.847	2088	2093	2099	rVB6	3926	7045	1.26%	0.181%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040622\
 Data File : VX027994.D
 Acq On : 06 Apr 2022 13:41
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
 Title : SW846 8260

37	14.042	2120	2125	2128	rVB	14743	16269	2.91%	0.418%
38	14.225	2151	2155	2161	rVB6	4389	7376	1.32%	0.190%
39	14.481	2193	2197	2199	rBV5	3684	5956	1.06%	0.153%
40	14.560	2207	2210	2215	rBV6	3704	7579	1.35%	0.195%
41	14.615	2215	2219	2226	rBV4	9698	16291	2.91%	0.419%
42	14.676	2226	2229	2234	rVB6	4188	6532	1.17%	0.168%
43	14.755	2234	2242	2245	rBV	18048	26406	4.72%	0.679%
44	15.054	2283	2291	2293	rBV9	3654	7307	1.30%	0.188%
45	15.188	2307	2313	2315	rBV2	13079	20348	3.63%	0.523%
46	15.280	2325	2328	2332	rVB6	4827	6530	1.17%	0.168%
47	15.377	2340	2344	2348	rBV5	5184	8743	1.56%	0.225%
48	15.487	2357	2362	2367	rBV2	16259	24789	4.43%	0.638%
49	15.615	2379	2383	2387	rBV5	7643	12824	2.29%	0.330%
50	15.847	2416	2421	2425	rBV8	4331	8961	1.60%	0.230%
51	15.981	2436	2443	2447	rBV10	6678	18022	3.22%	0.464%
52	16.091	2456	2461	2468	rBV7	11217	22836	4.08%	0.587%
53	16.200	2475	2479	2485	rVB9	3822	7789	1.39%	0.200%
54	16.292	2485	2494	2500	rBV9	4187	15477	2.76%	0.398%
55	16.377	2500	2508	2513	rVB6	9312	23899	4.27%	0.615%
56	16.560	2533	2538	2540	rBV6	5022	7413	1.32%	0.191%
57	16.590	2541	2543	2549	rVB5	6888	11406	2.04%	0.293%
58	16.658	2549	2554	2559	rVB3	5927	10163	1.81%	0.261%




Sum of corrected areas: 3887961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040622\
Data File : VX027994.D
Acq On : 06 Apr 2022 13:41
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

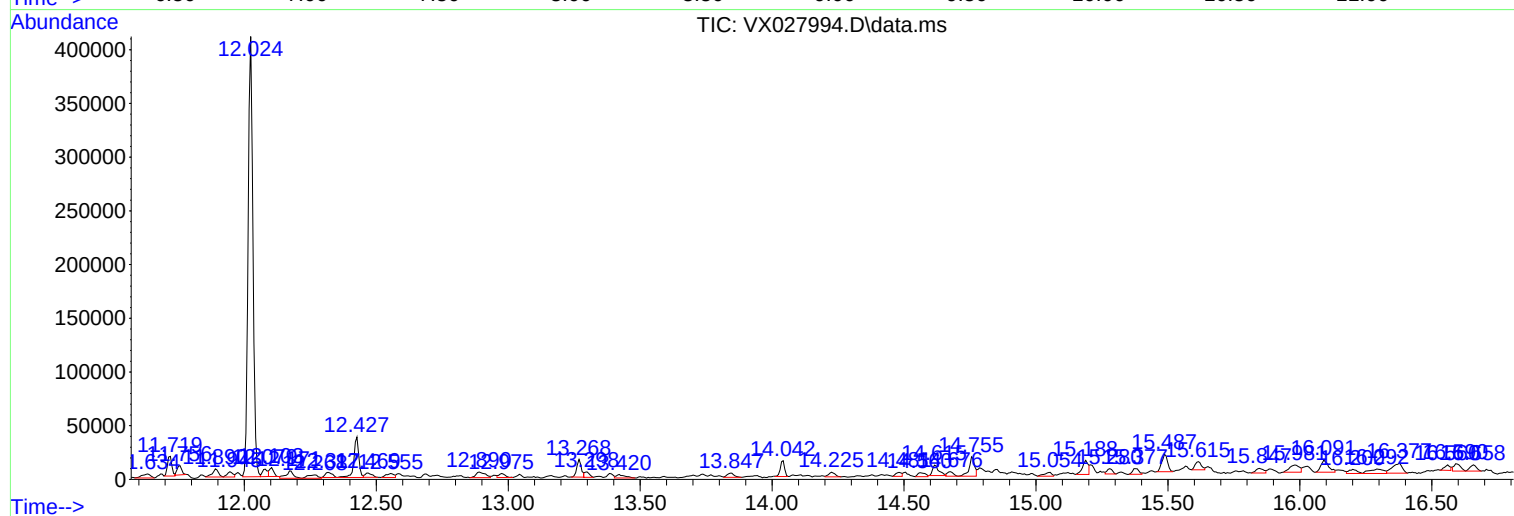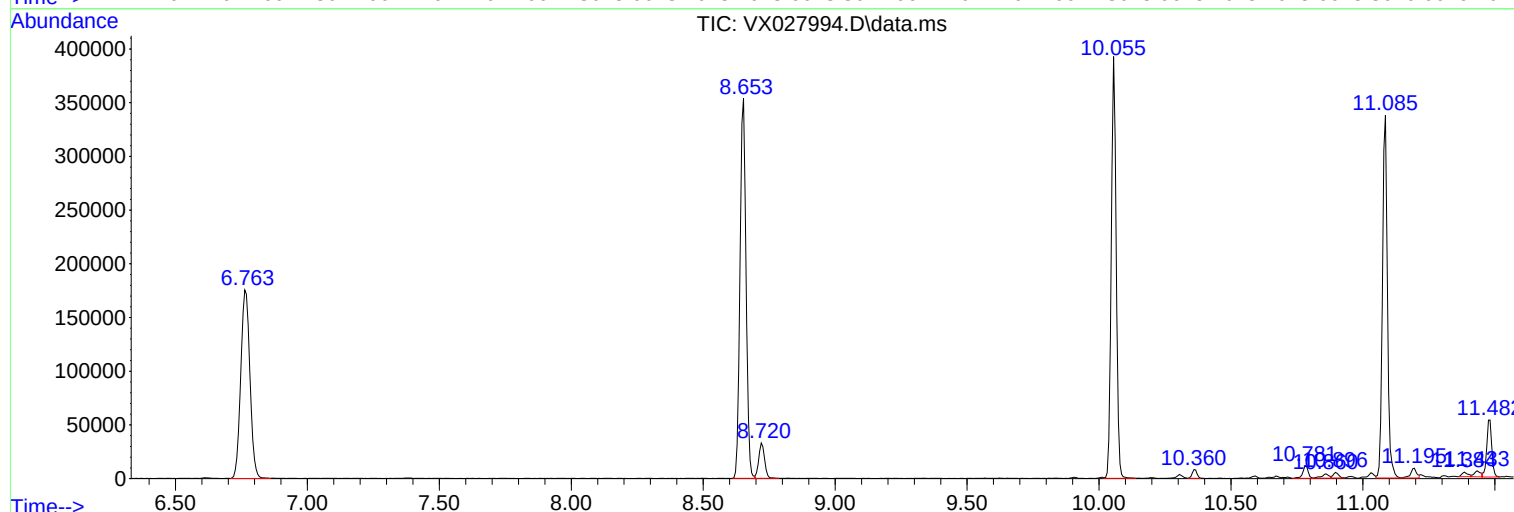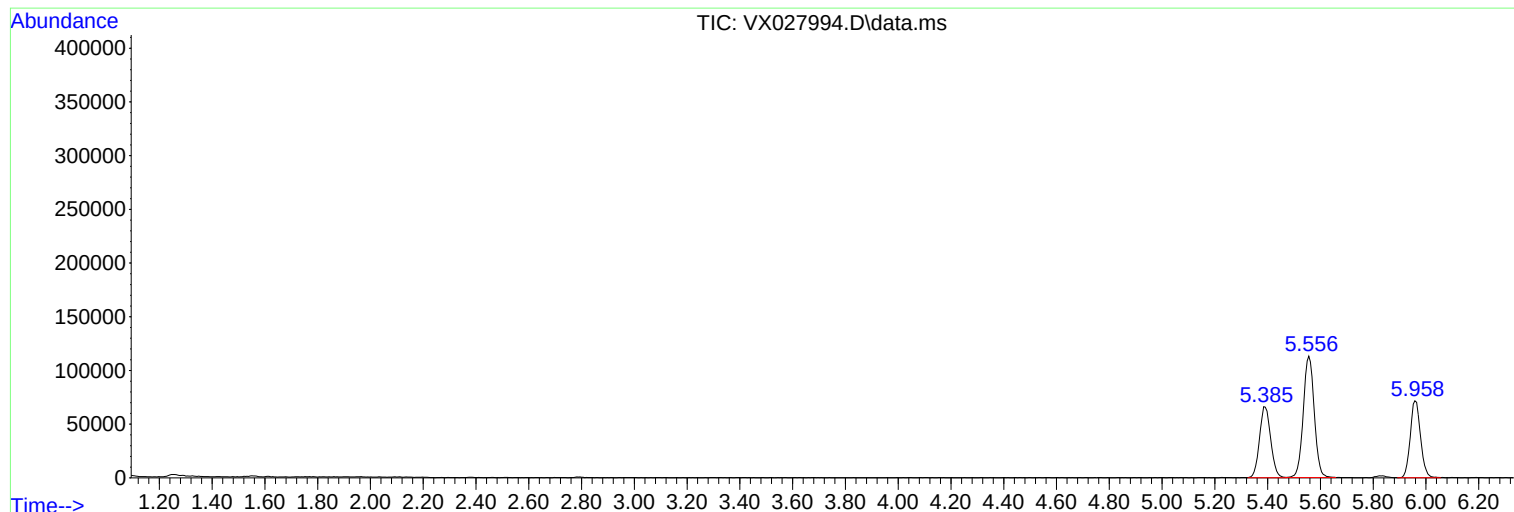

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040622\
Data File : VX027994.D
Acq On : 06 Apr 2022 13:41
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040622\
Data File : VX027994.D
Acq On : 06 Apr 2022 13:41
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------