



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040623\
Data File : VX034947.D
Acq On : 06 Apr 2023 08:29
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X032823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Mar 28 09:11:00 2023

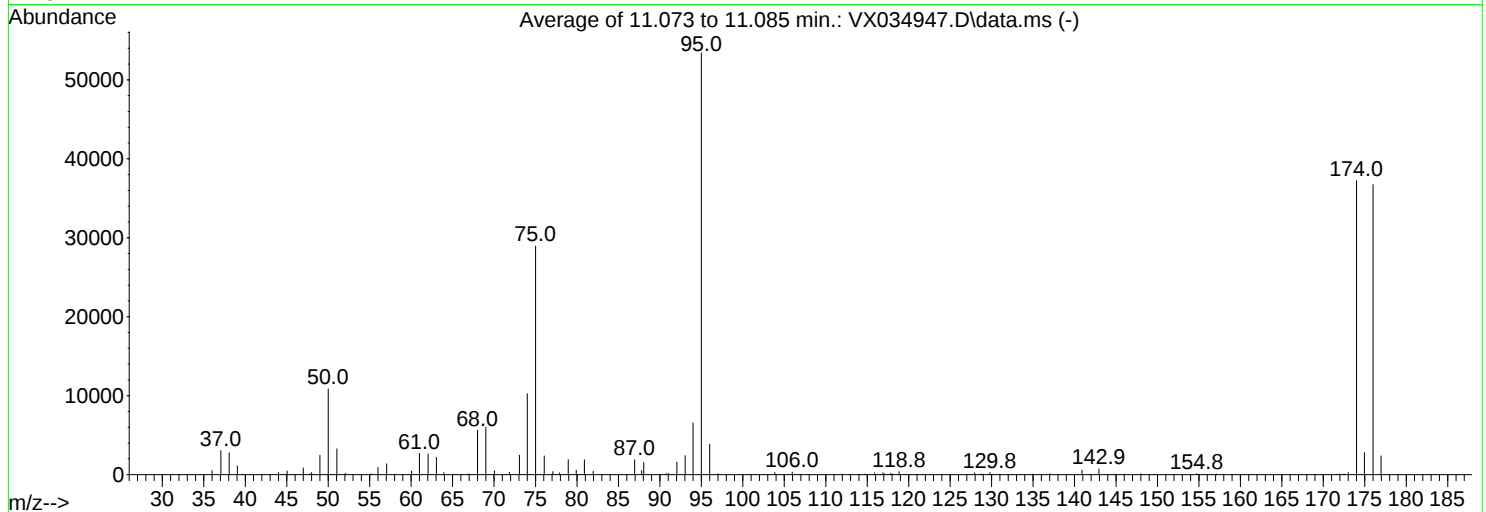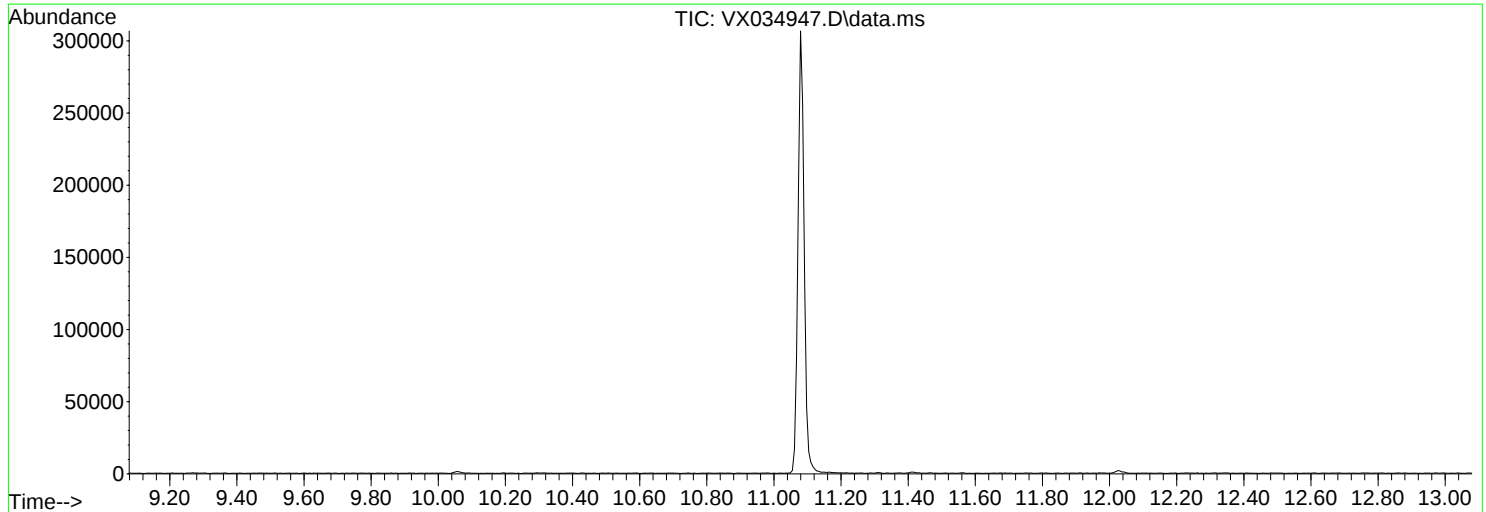

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	10841	PASS
75	95	30	60	54.2	28936	PASS
95	95	100	100	100.0	53421	PASS
96	95	5	9	7.2	3864	PASS
173	174	0.00	2	0.7	275	PASS
174	95	50	100	69.7	37224	PASS
175	174	5	9	7.5	2807	PASS
176	174	95	101	98.7	36733	PASS
177	176	5	9	6.5	2373	PASS