


Chloromethane

Response Ratio

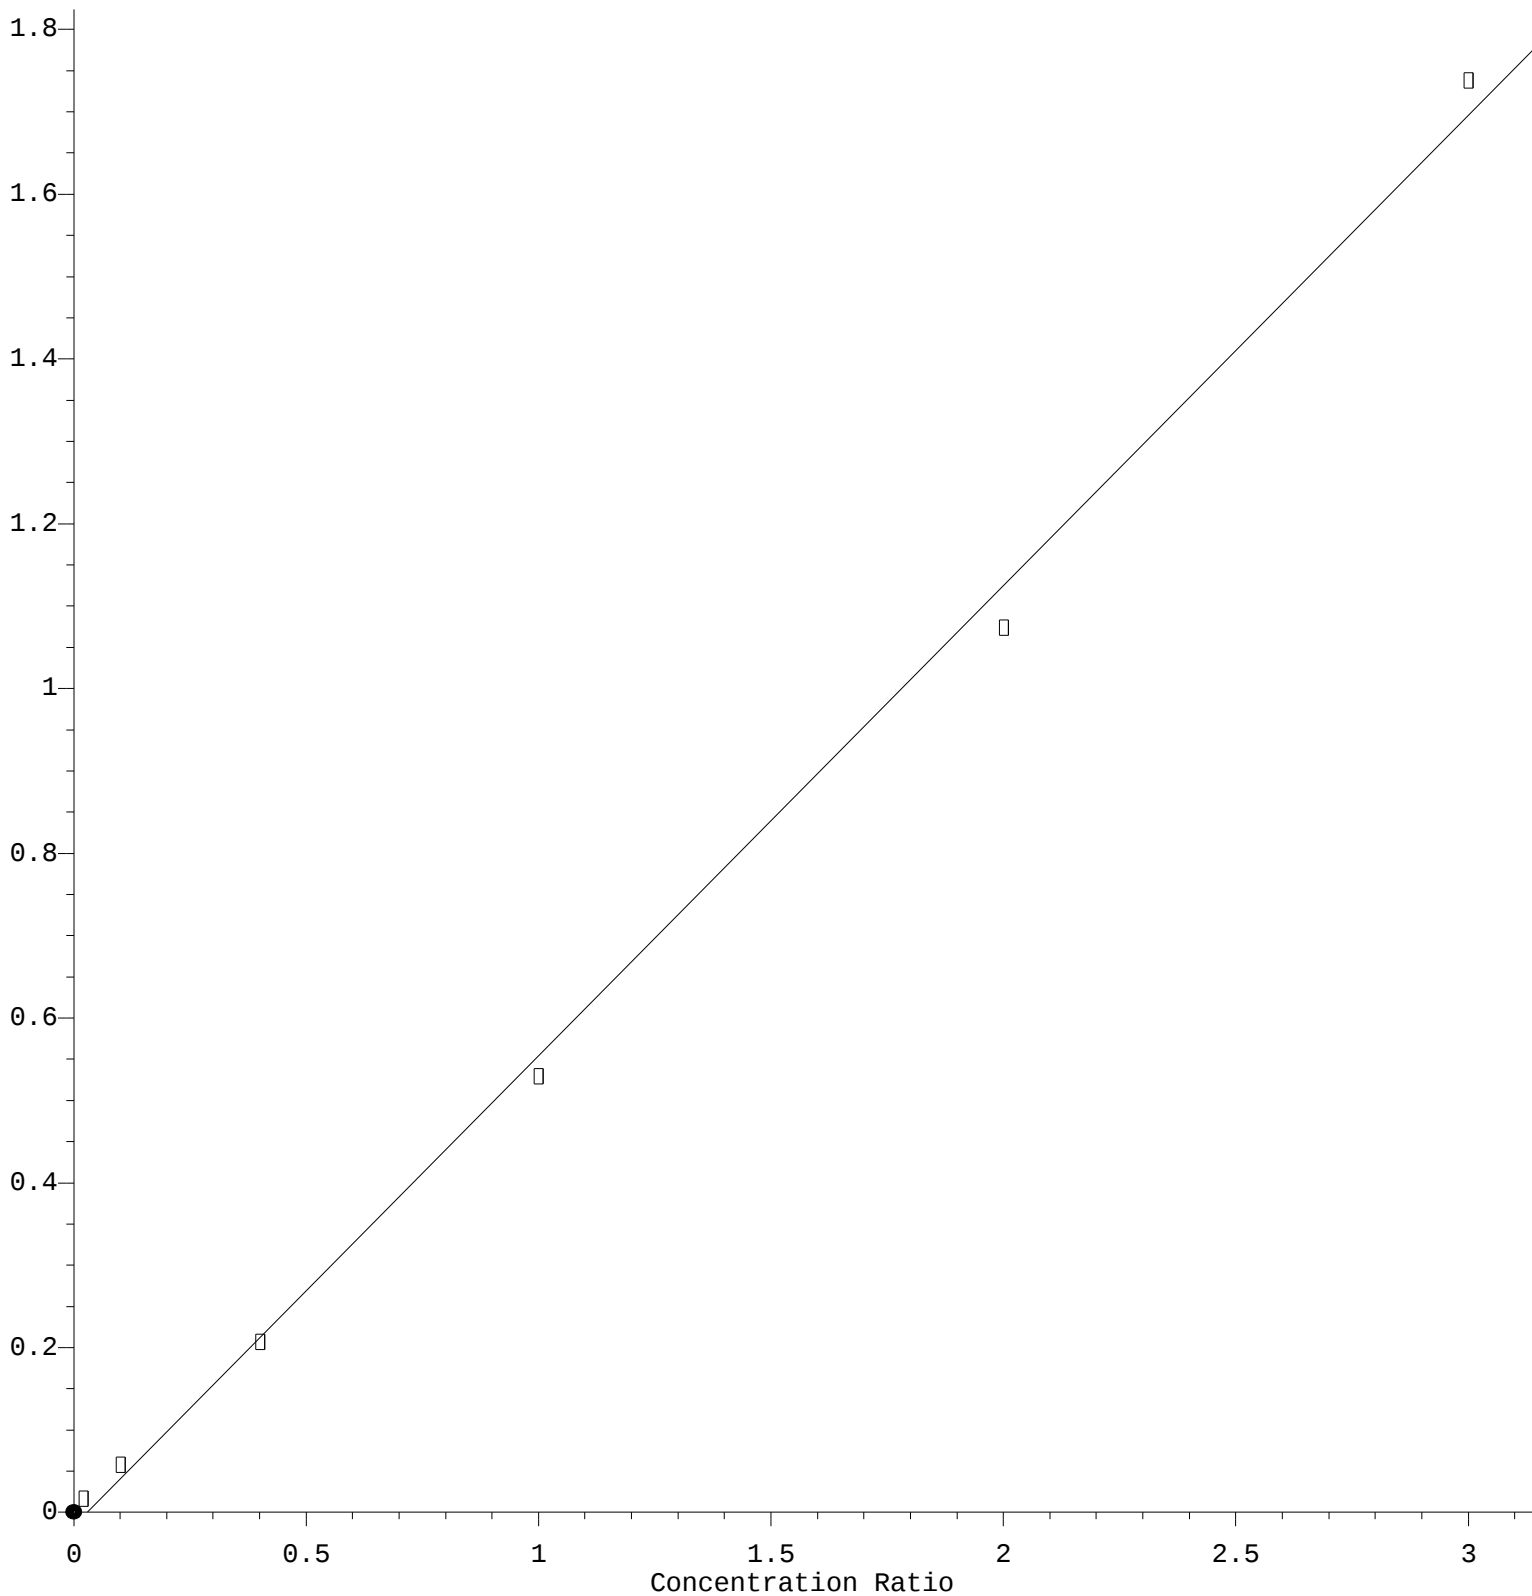


$$\text{Response} = 5.707\text{e-}001 * \text{Amt} - 1.667\text{e-}002$$

Coef of Det (r^2) = 0.997510 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022


Bromomethane

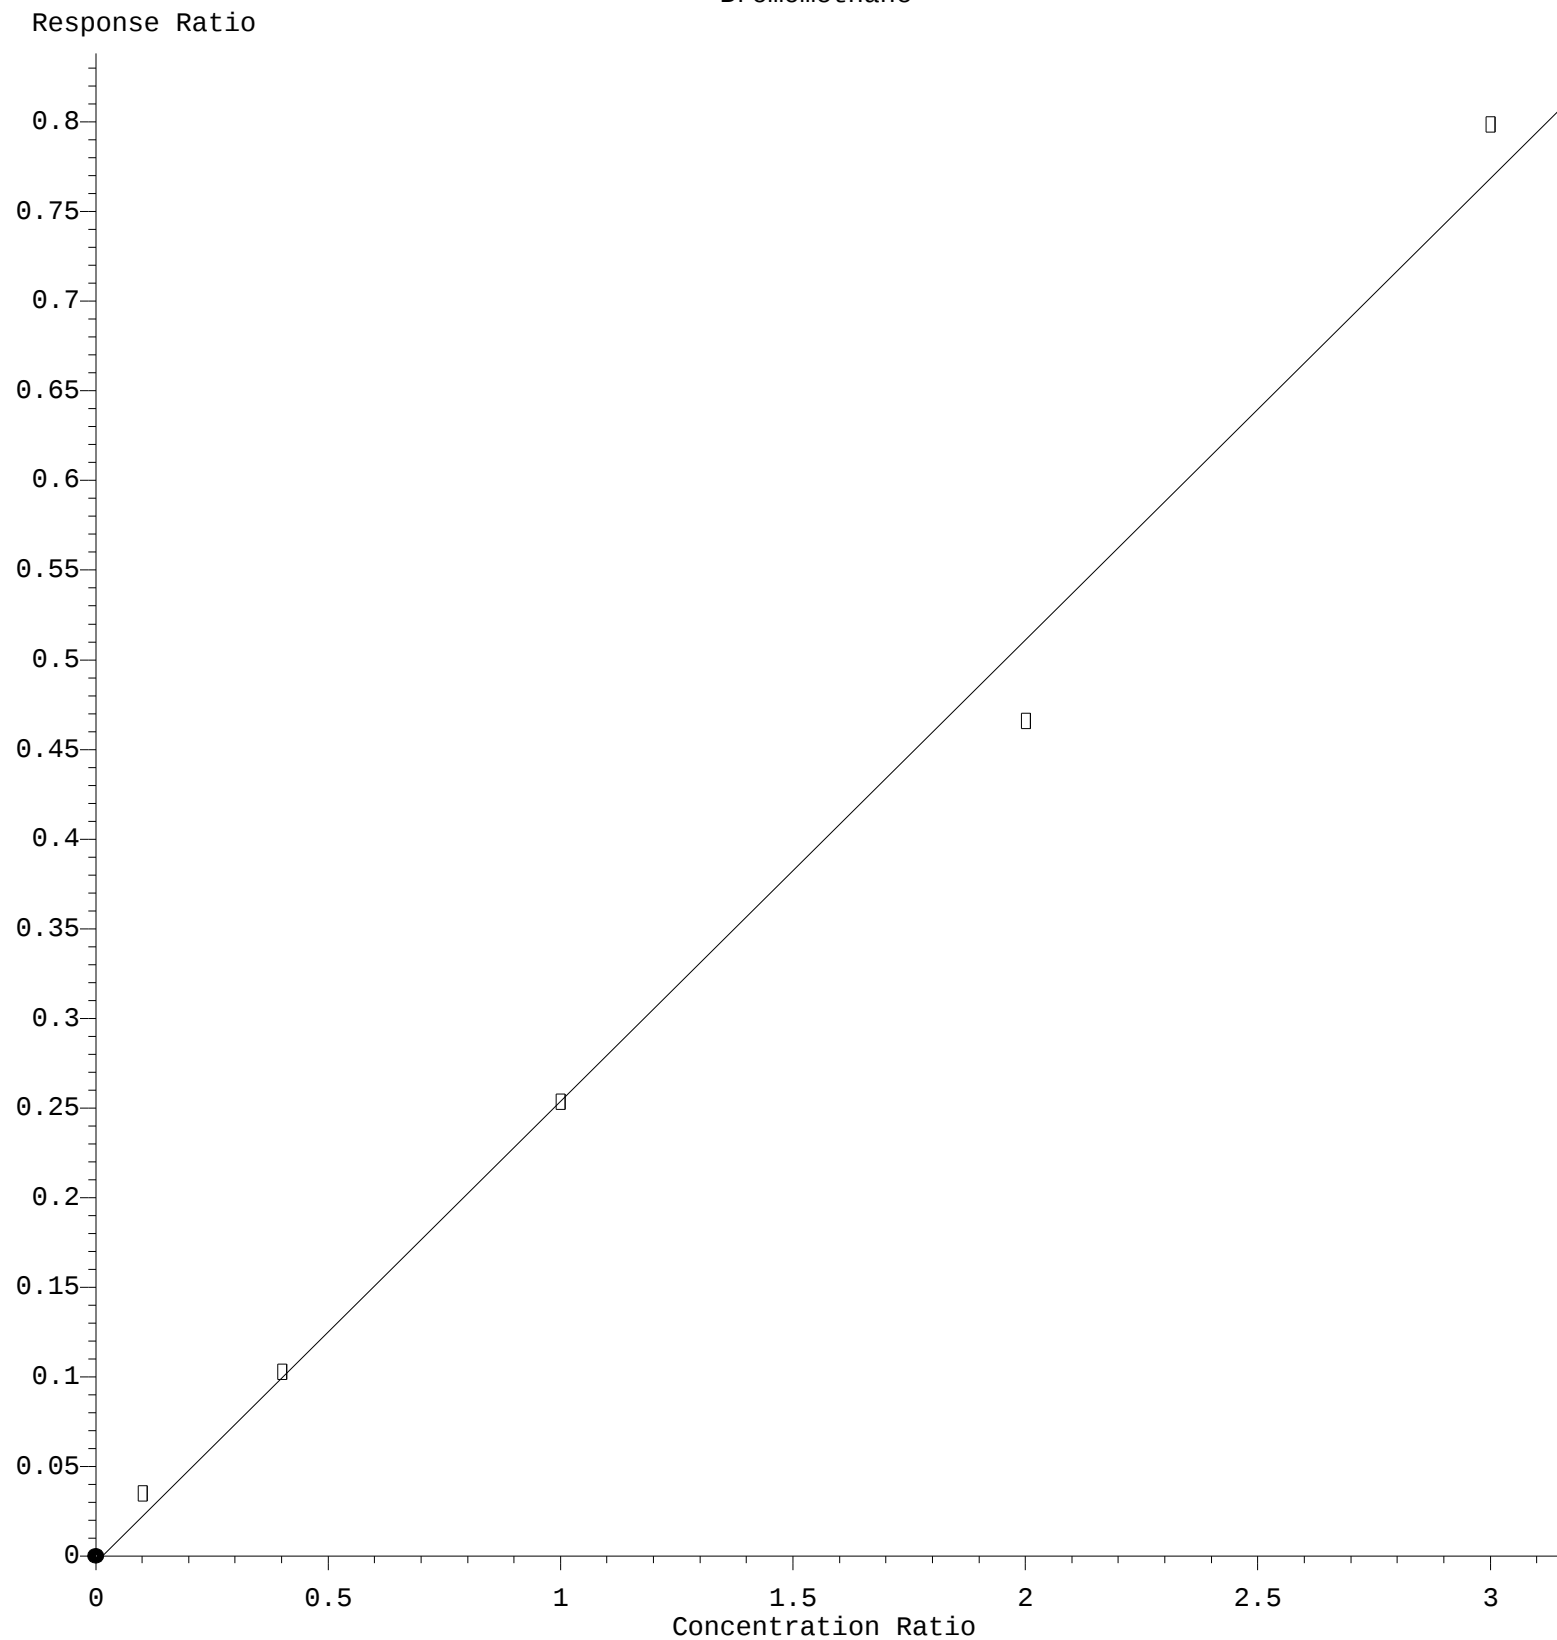

$\text{Response} = 2.574\text{e-}001 * \text{Amt} - 3.600\text{e-}003$
 Coef of Det (r^2) = 0.991823 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
 Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

Chloroethane

Response Ratio

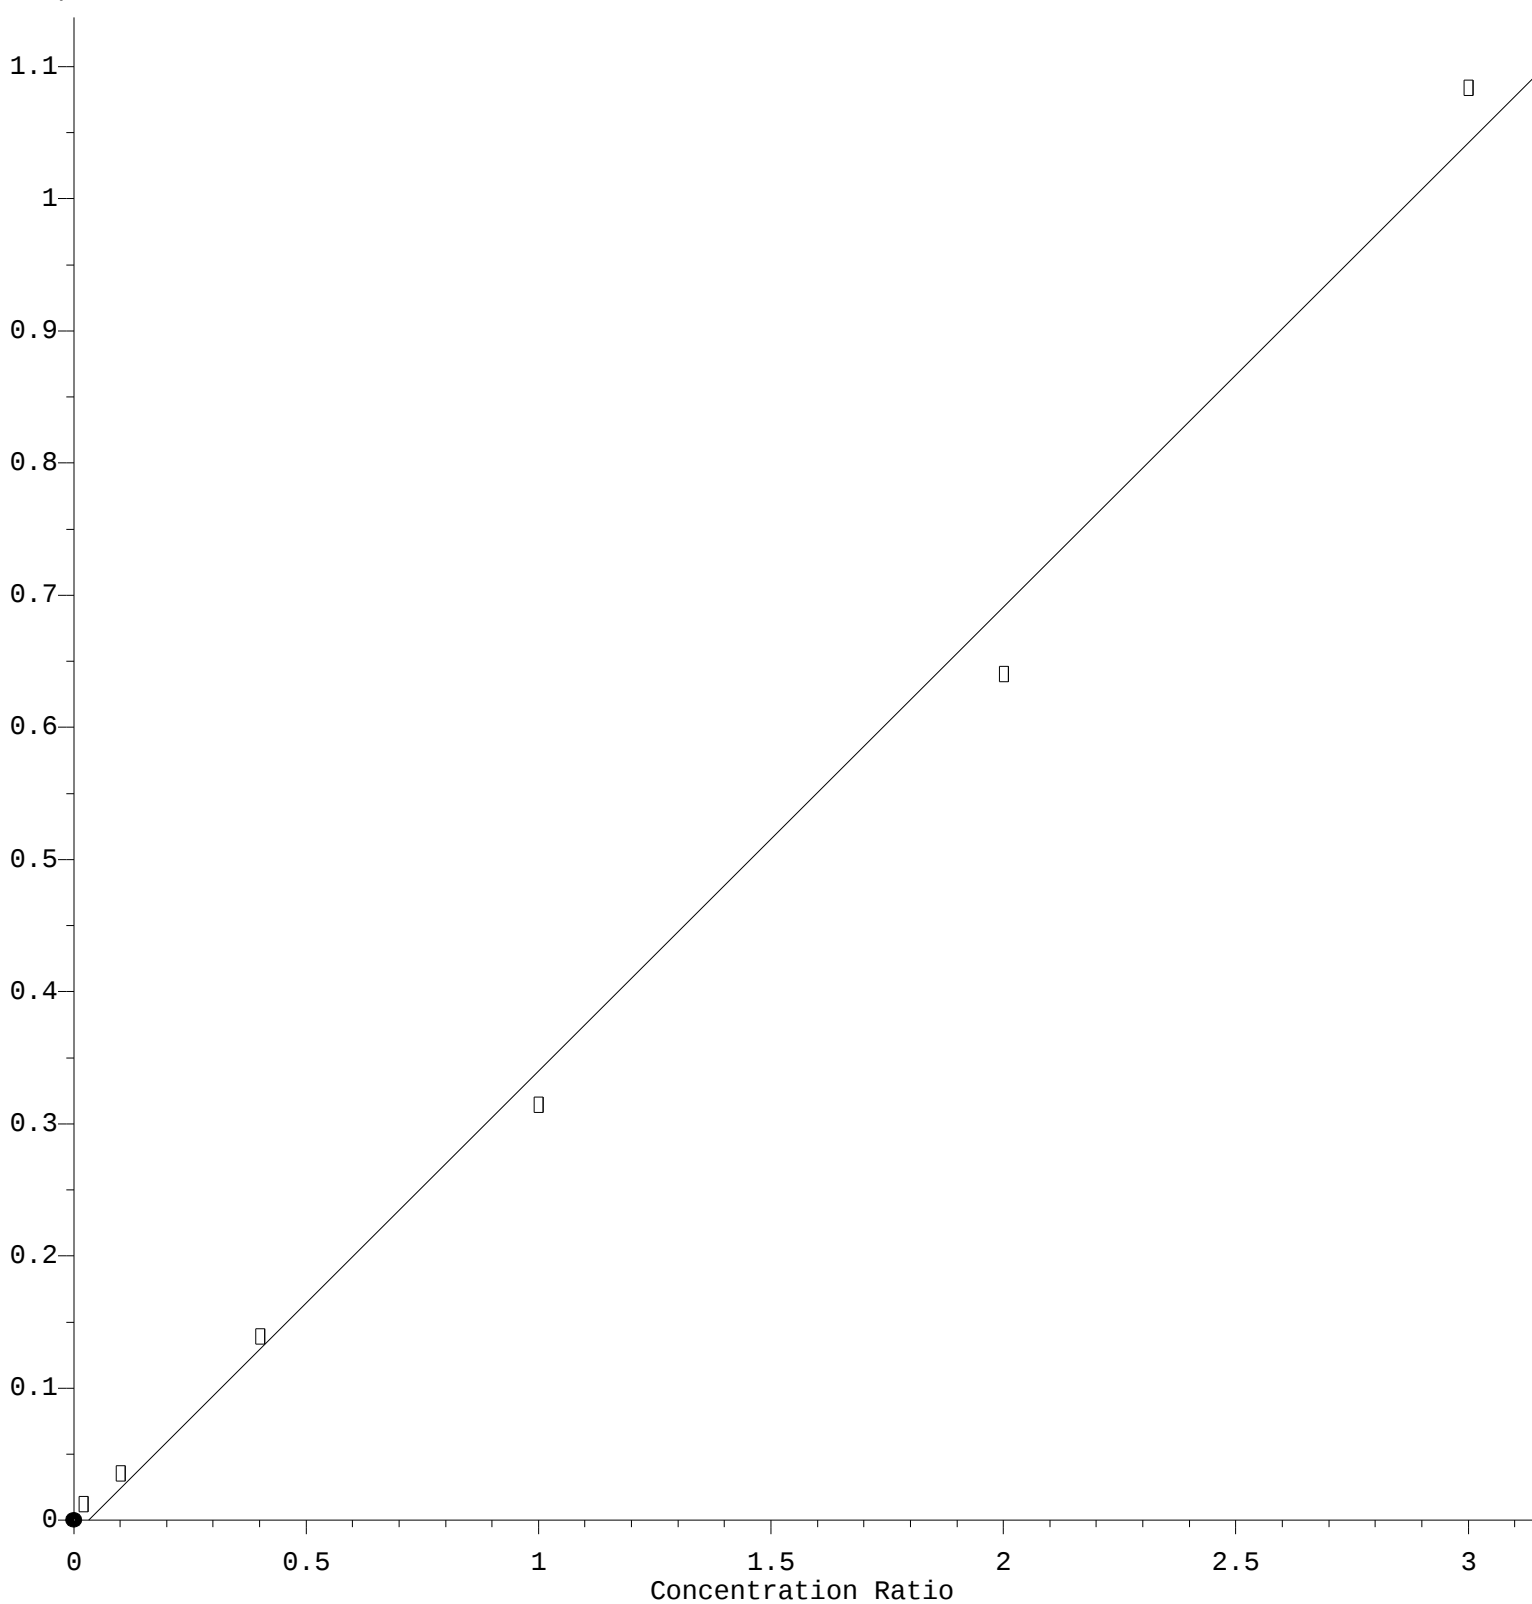

$$\text{Response} = 3.511\text{e-}001 * \text{Amt} - 1.088\text{e-}002$$


Coef of Det (r^2) = 0.993814 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

Diethyl Ether

Response Ratio

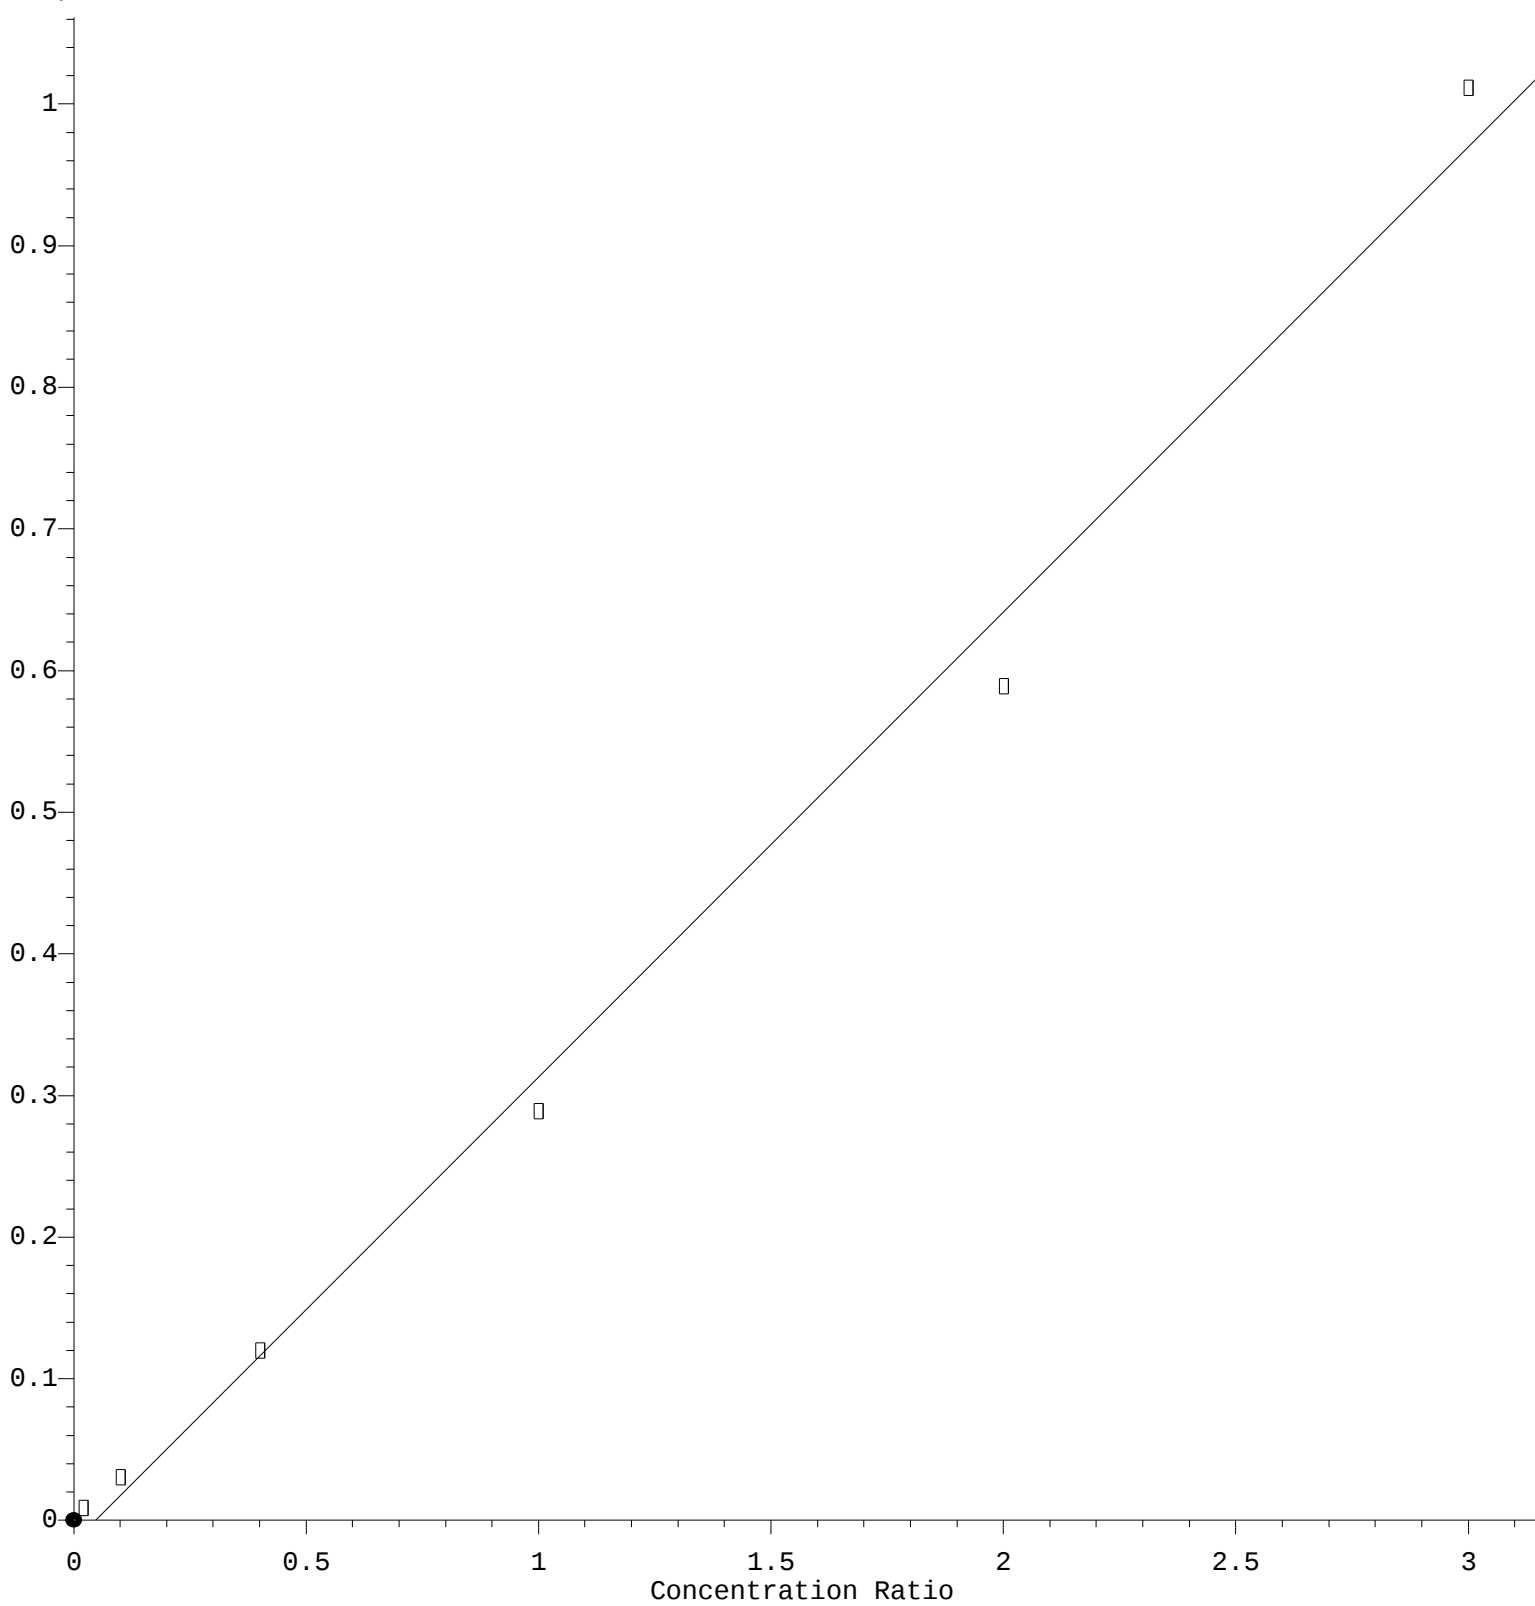

$$\text{Response} = 3.283\text{e-}001 * \text{Amt} - 1.556\text{e-}002$$


Coef of Det (r^2) = 0.992791 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

Methyl Iodide

Response Ratio

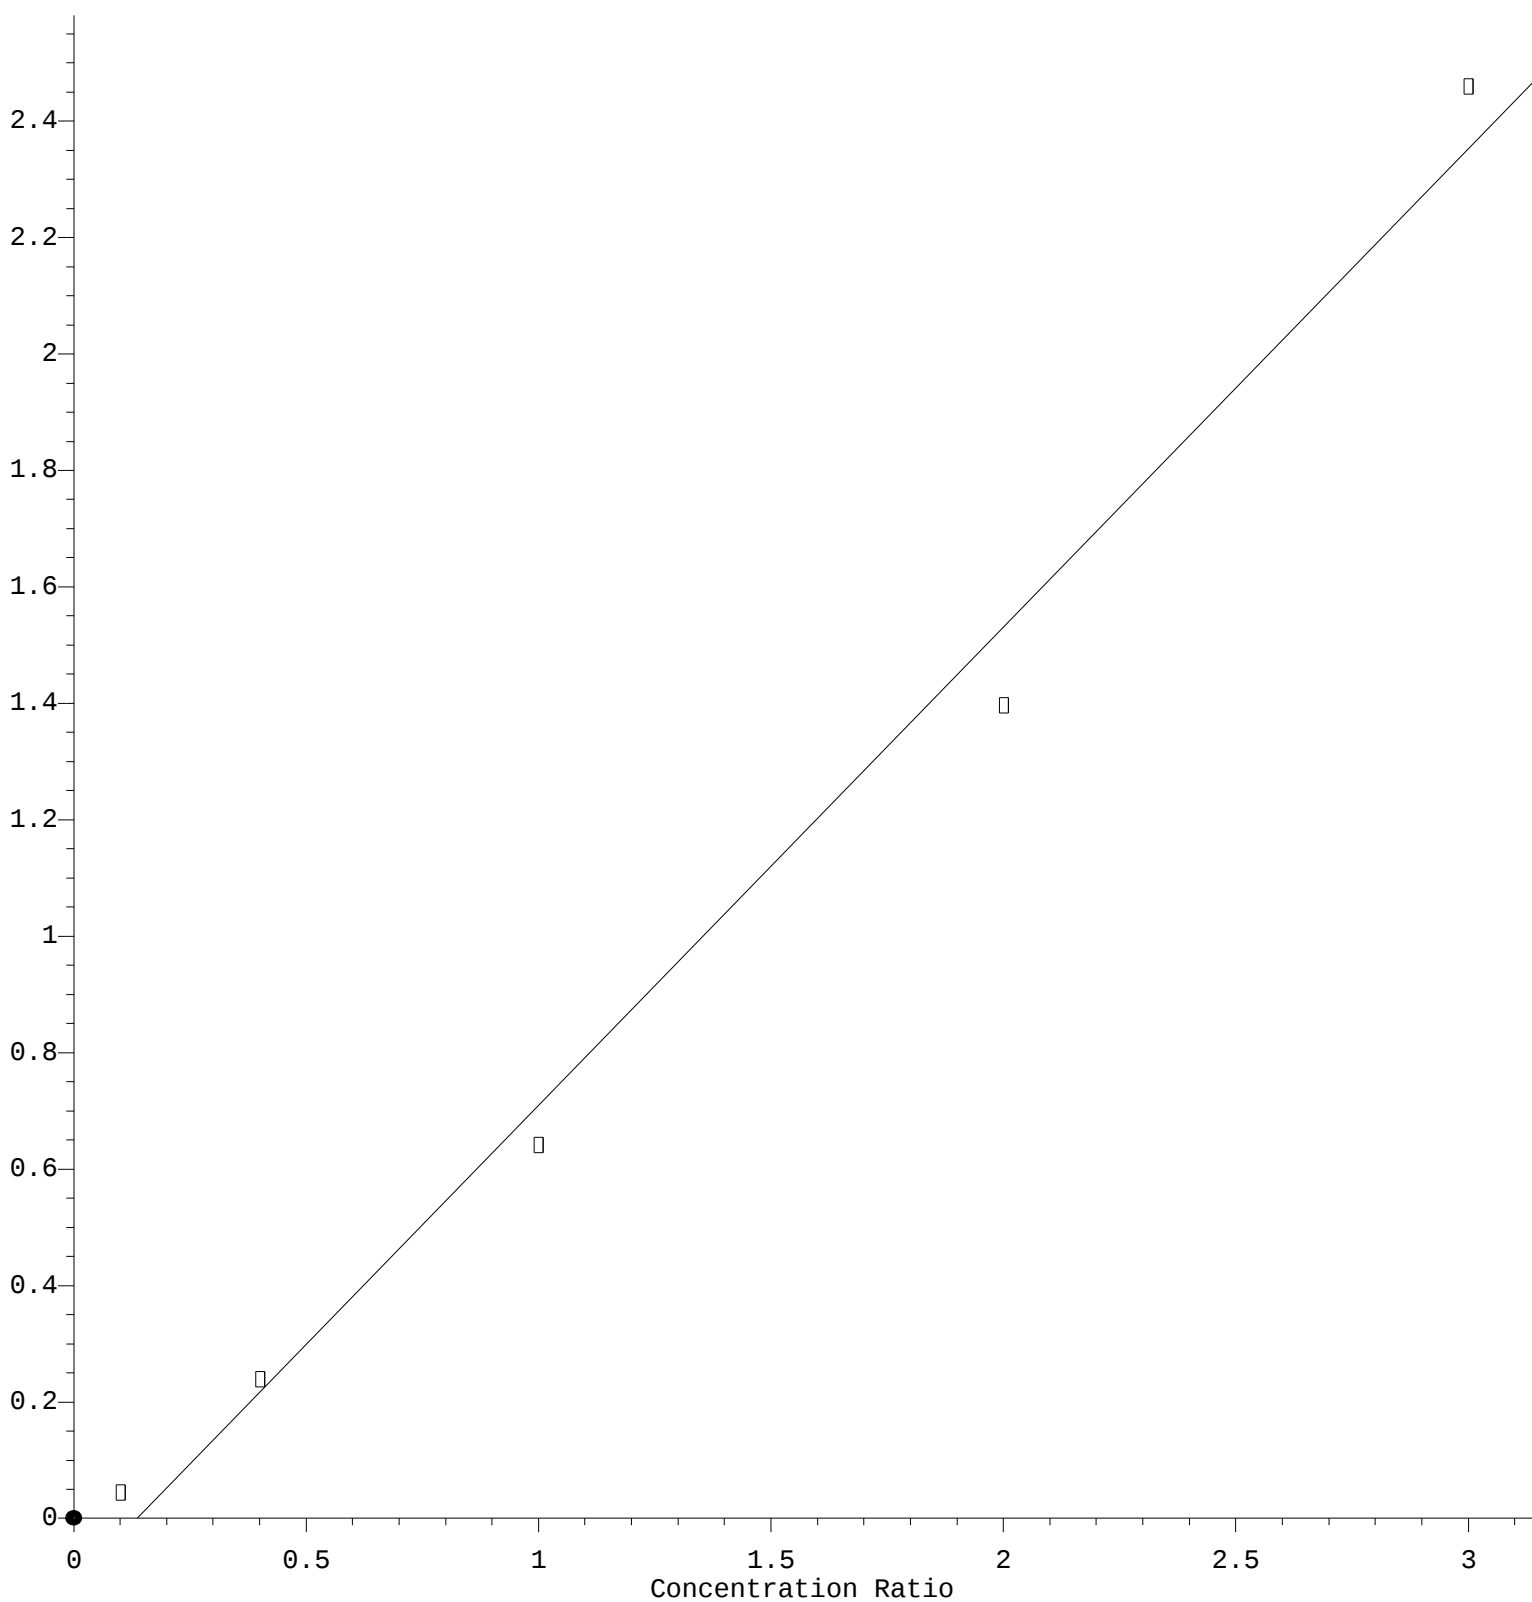

$$\text{Response} = 8.213\text{e-}001 * \text{Amt} - 1.118\text{e-}001$$


Coef of Det (r^2) = 0.989715 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

Acetone

Response Ratio

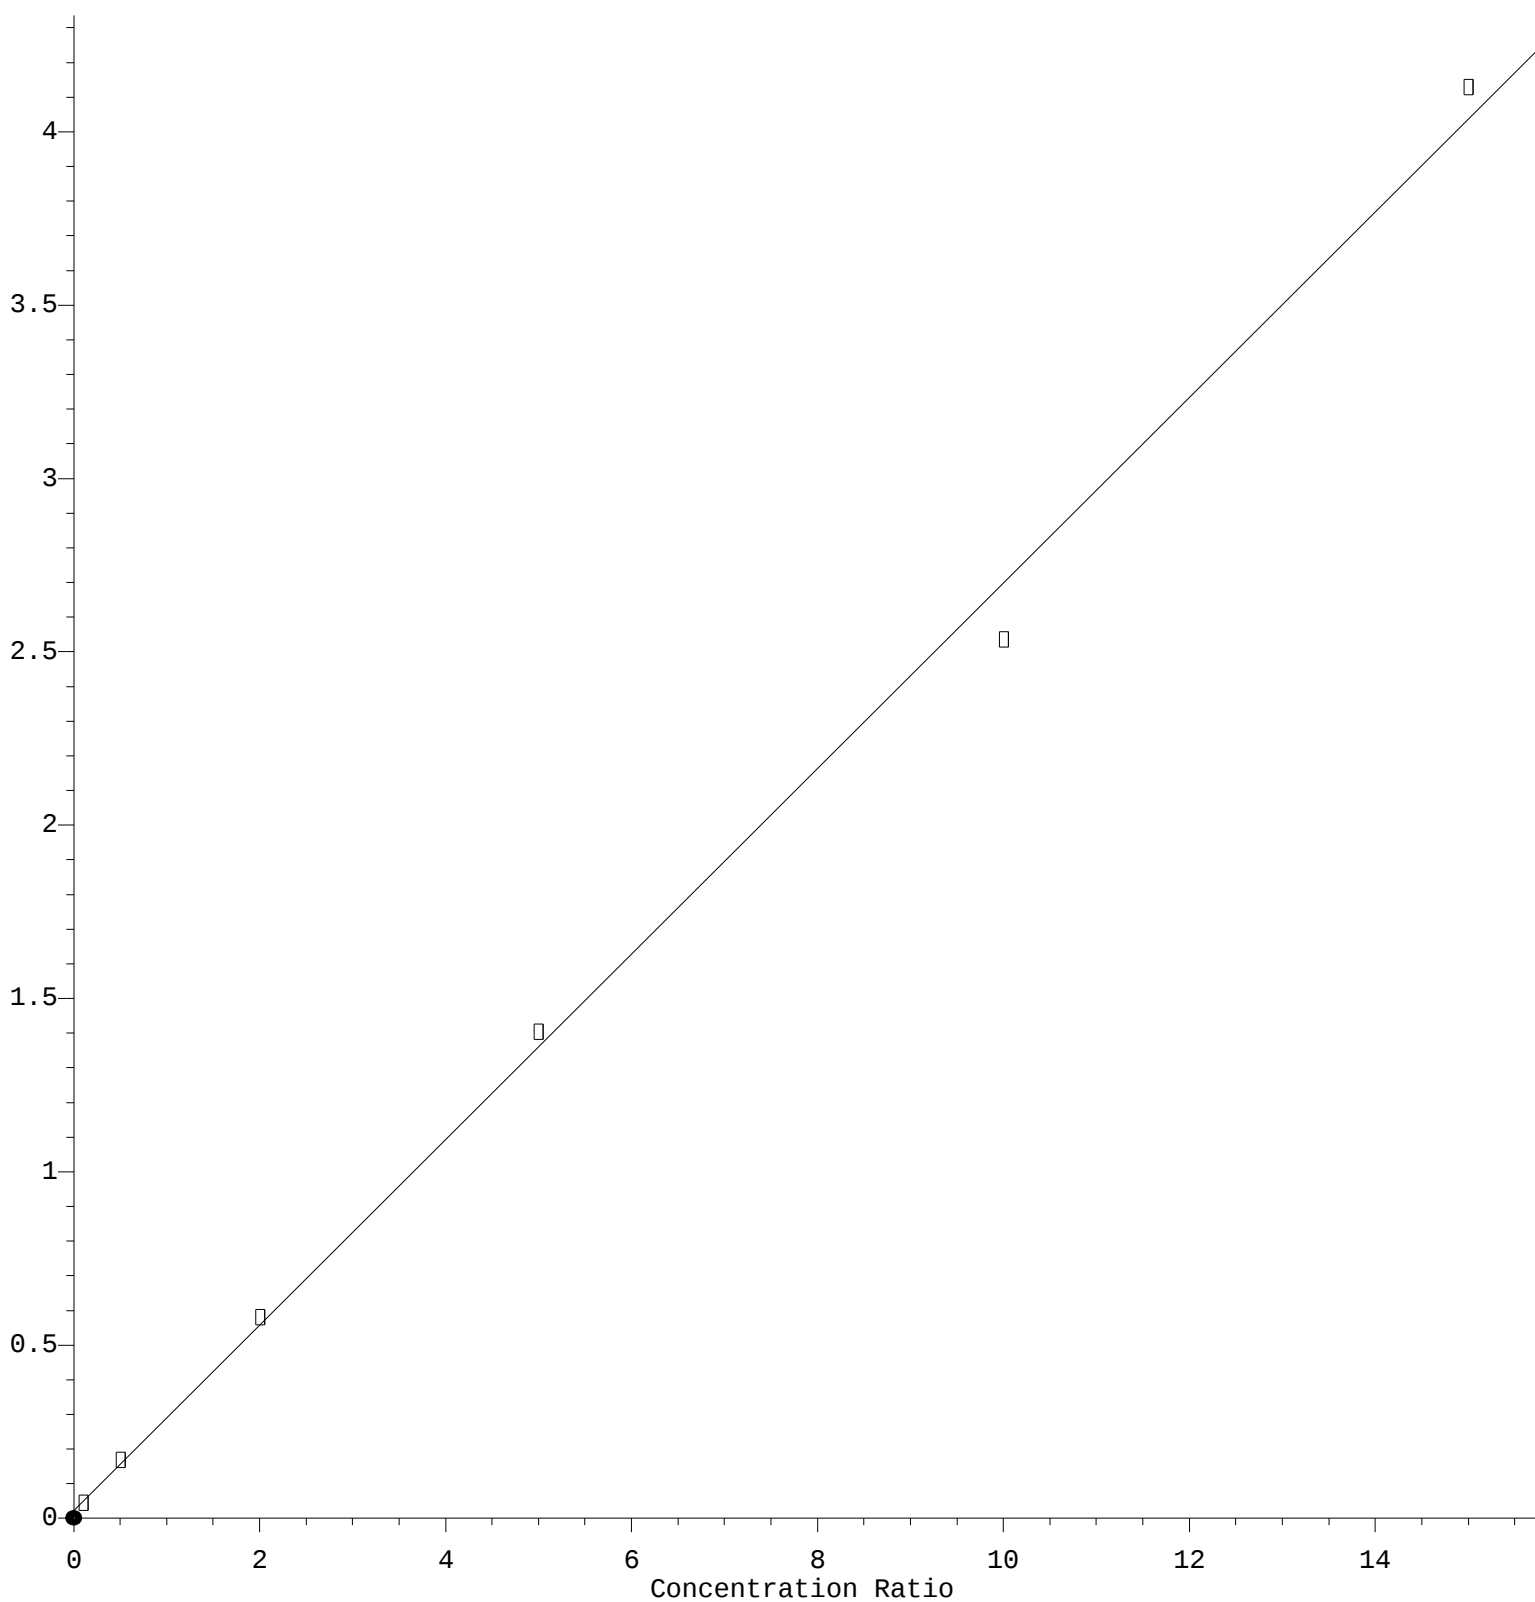

$$\text{Response} = 2.676\text{e-}001 * \text{Amt} + 2.233\text{e-}002$$


Coef of Det (r^2) = 0.997013 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

Carbon Disulfide


Response Ratio

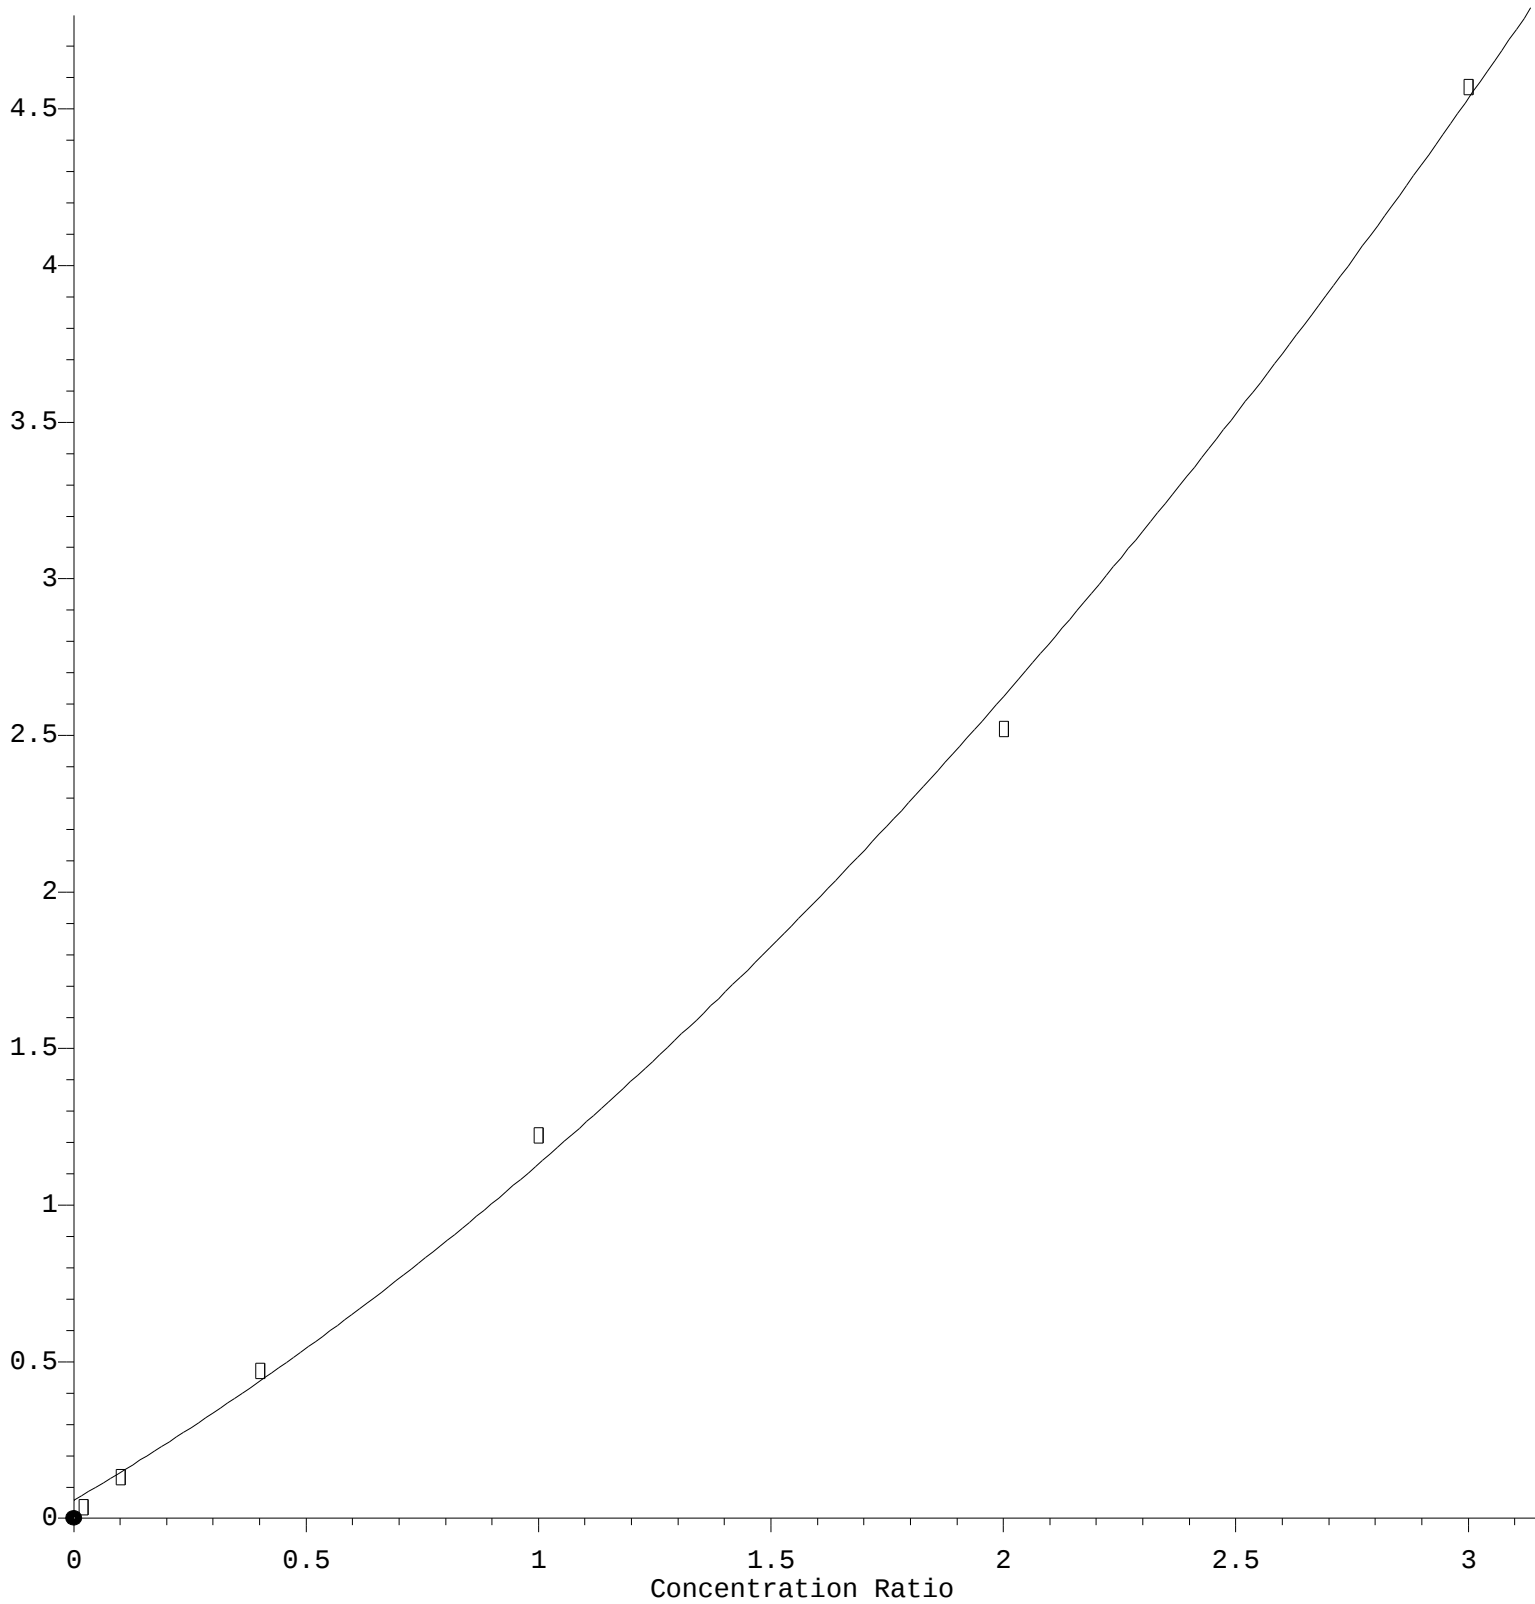

$R = 2.091e-001 A^2 + 8.649e-001 A + 5.787e-002$
Coef of Det (r^2) = 0.998507 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

Methylene Chloride

Response Ratio

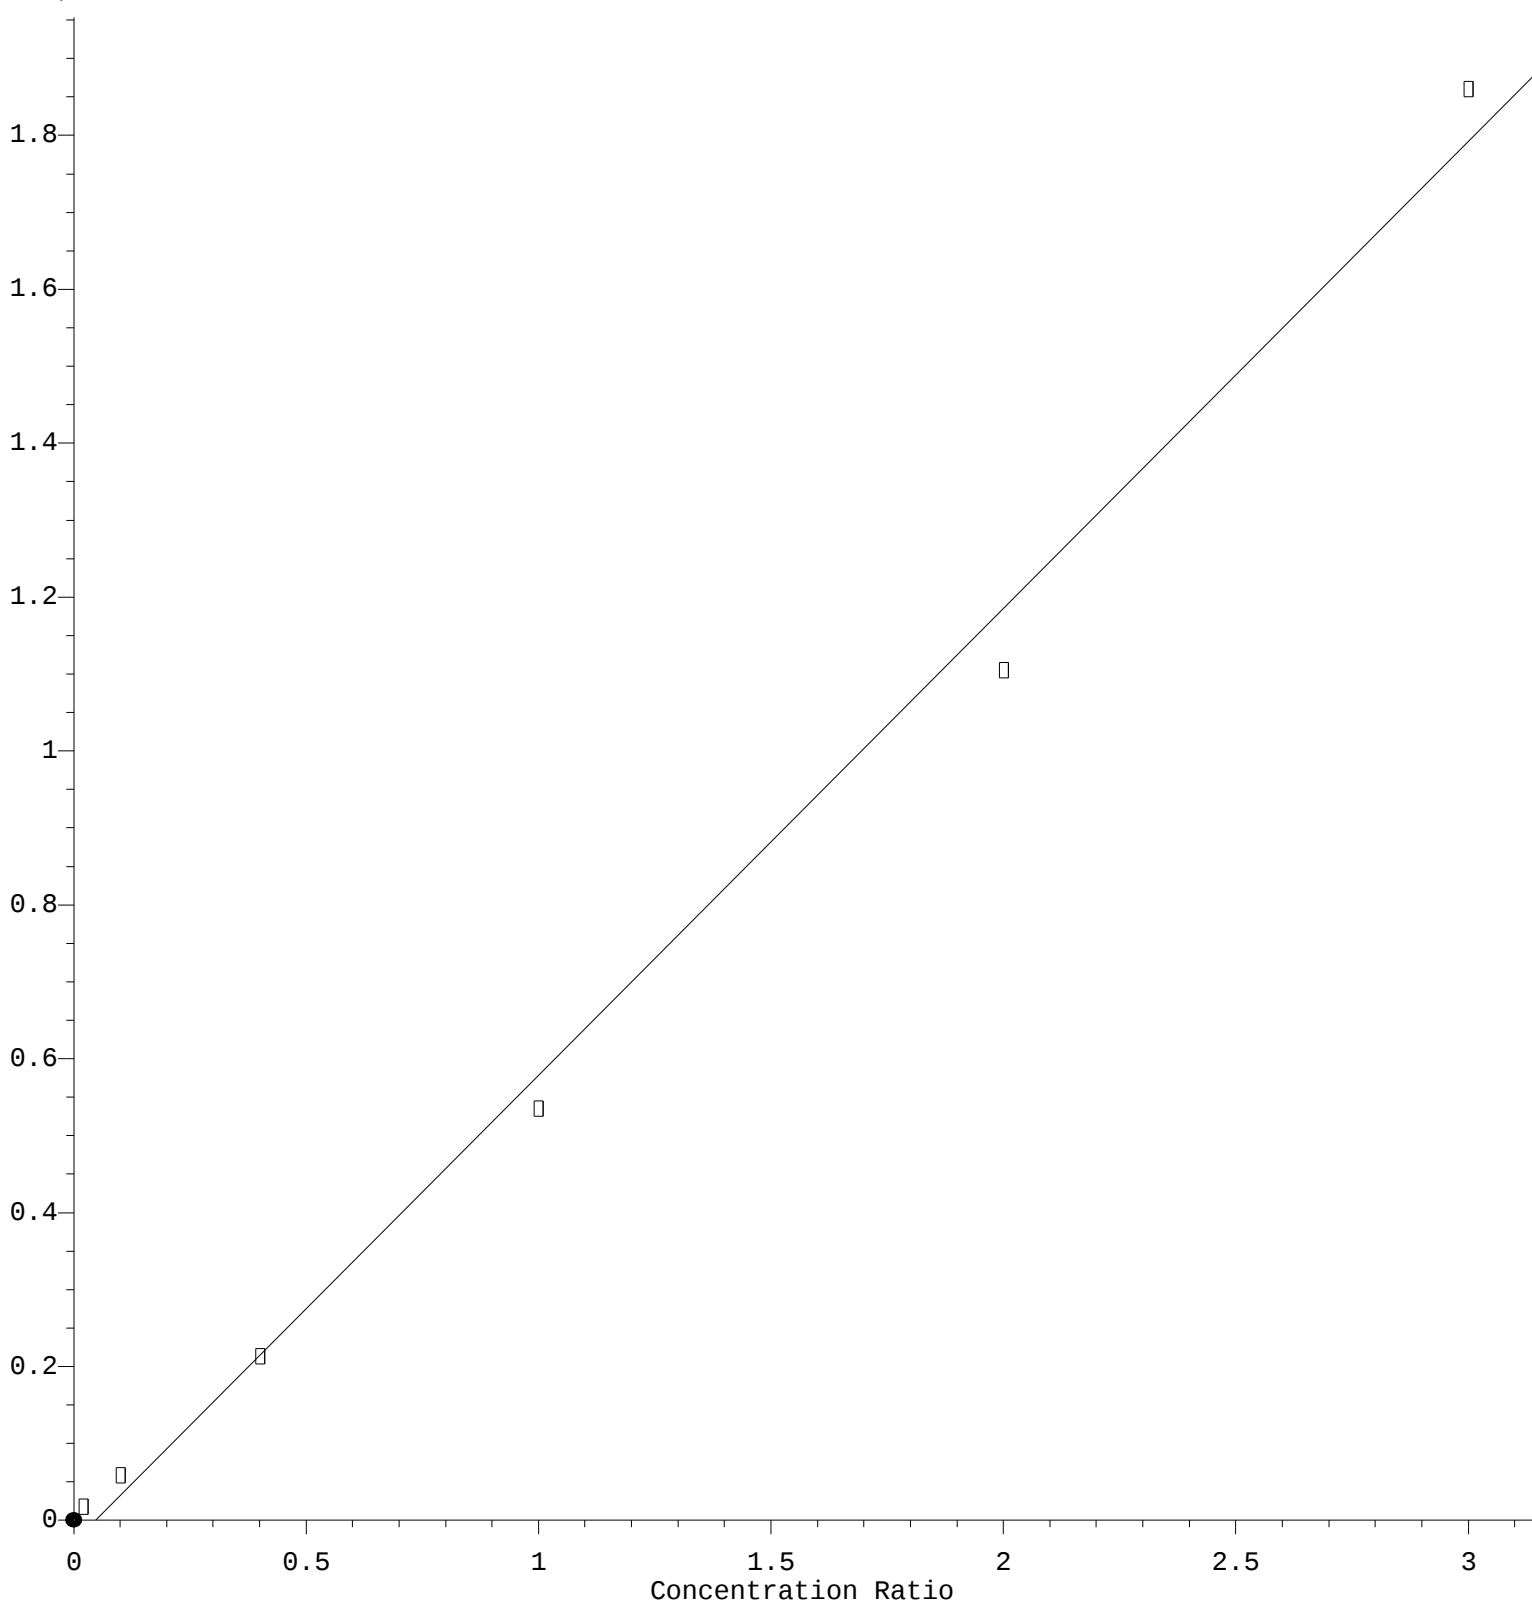

$$\text{Response} = 6.069\text{e-}001 * \text{Amt} - 2.831\text{e-}002$$


Coef of Det (r^2) = 0.994351 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022

trans-1,4-Dichloro-2-butene

Response Ratio

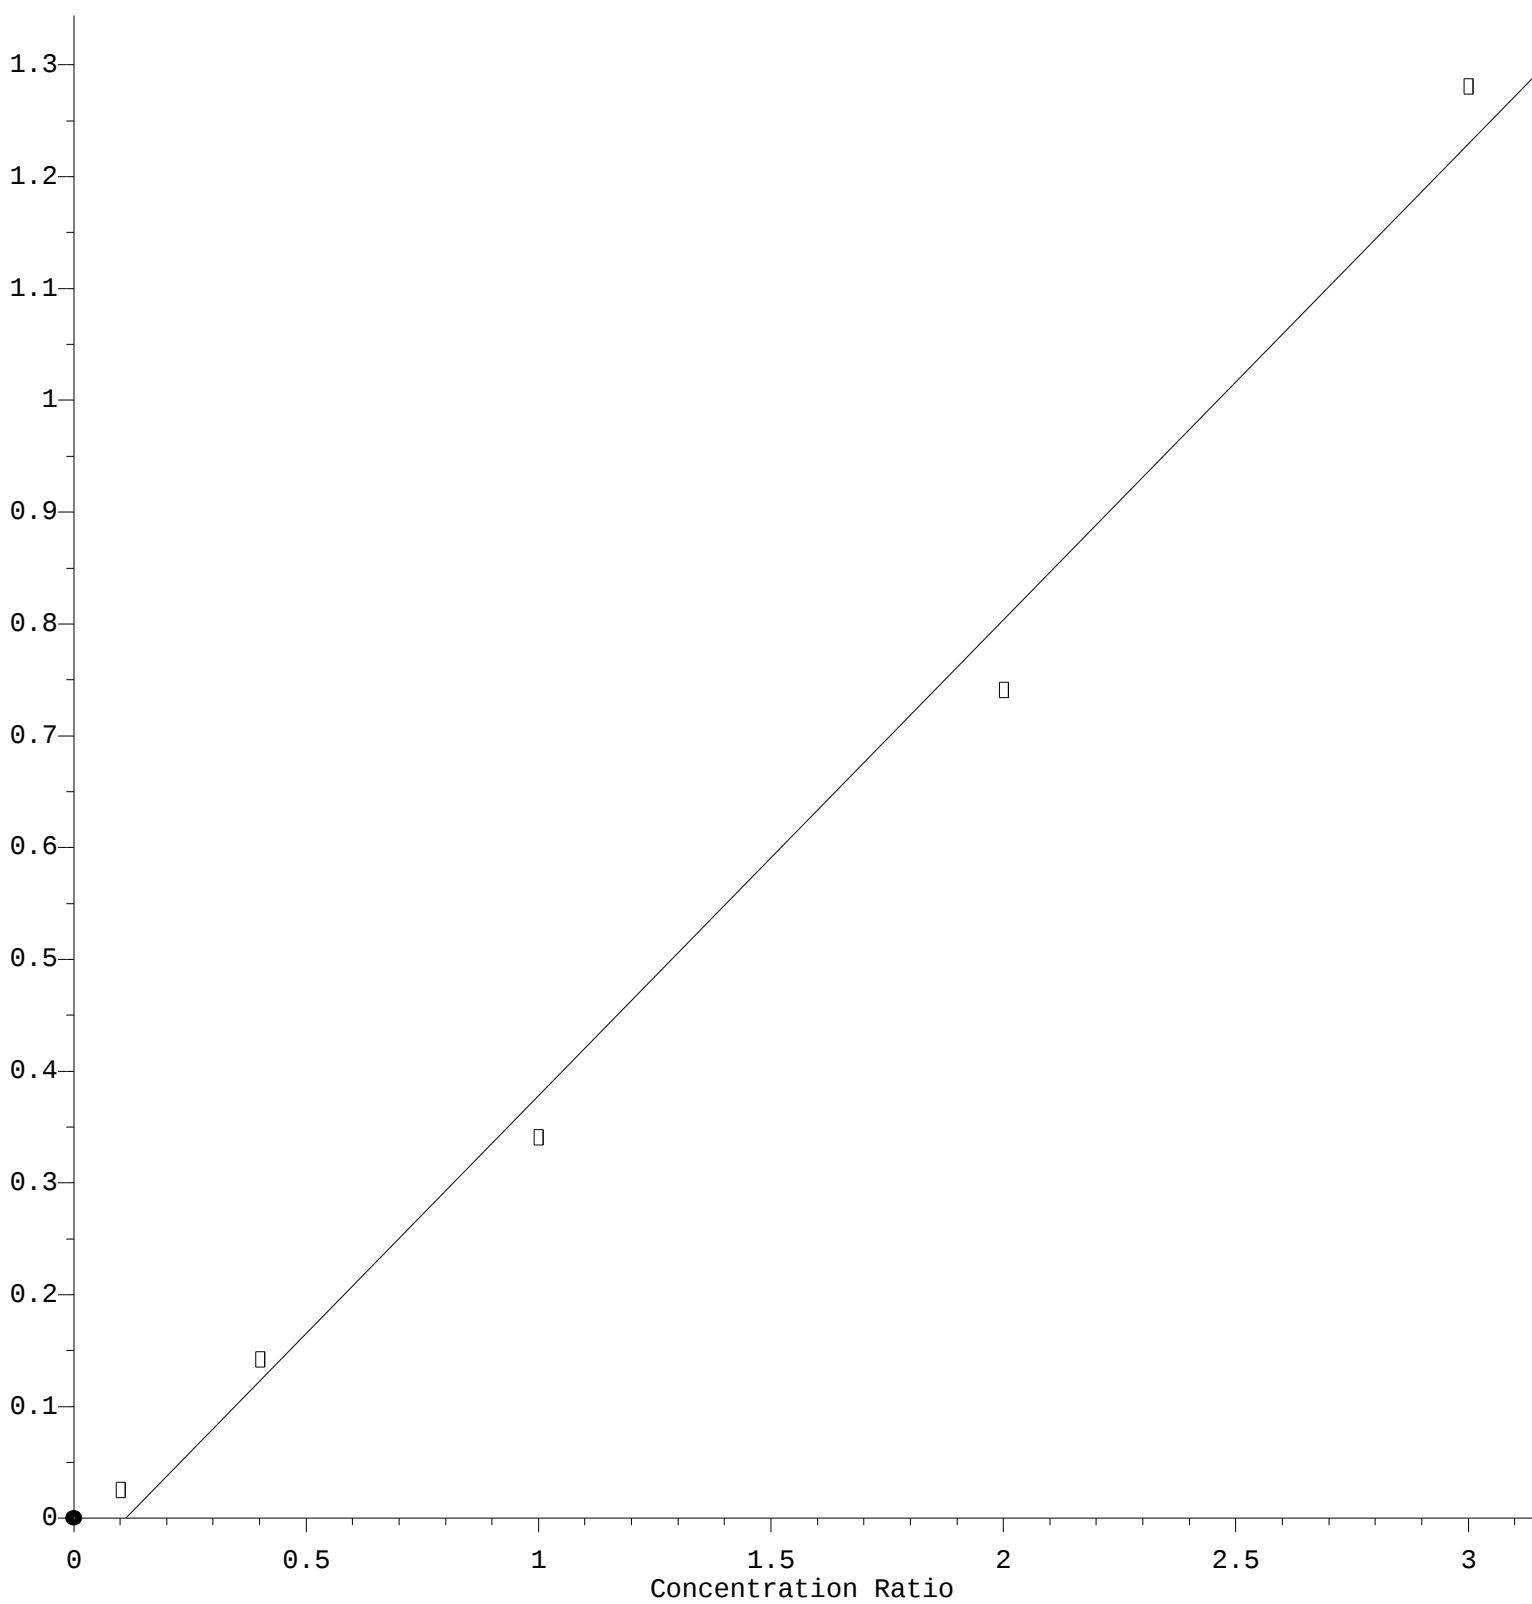

$$\text{Response} = 4.257\text{e-}001 * \text{Amt} - 4.779\text{e-}002$$

Coef of Det (r^2) = 0.991117 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Calibration Table Last Updated: Thu Apr 07 18:12:28 2022