

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040723\
 Data File : VX034975.D
 Acq On : 07 Apr 2023 17:44
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
 Title : SW846 8260

Signal : TIC: VX034975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.325	30	39	40	rBV6	7929	19086	1.29%	0.230%
2	1.624	76	88	105	rVB6	6836	36097	2.43%	0.435%
3	2.136	158	172	190	rVB	47960	256798	17.29%	3.094%
4	5.385	694	705	722	rBV	159900	472088	31.79%	5.688%
5	5.550	722	732	750	rVB2	290816	835497	56.26%	10.067%
6	5.952	786	798	814	rBV	191572	522195	35.16%	6.292%
7	6.763	920	931	948	rBV	455429	1097490	73.90%	13.224%
8	8.647	1233	1240	1250	rBV	934866	1485117	100.00%	17.895%
9	10.055	1465	1471	1484	rBV	939118	1290539	86.90%	15.550%
10	11.079	1634	1639	1651	rBV	779795	1007989	67.87%	12.146%
11	12.024	1788	1794	1804	rBV	954281	1222381	82.31%	14.729%
12	13.164	1976	1981	1987	rVB6	6703	18012	1.21%	0.217%
13	14.225	2149	2155	2160	rVB3	11962	19830	1.34%	0.239%
14	14.481	2192	2197	2202	rBV4	12551	16006	1.08%	0.193%




Sum of corrected areas: 8299125

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040723\
Data File : VX034975.D
Acq On : 07 Apr 2023 17:44
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

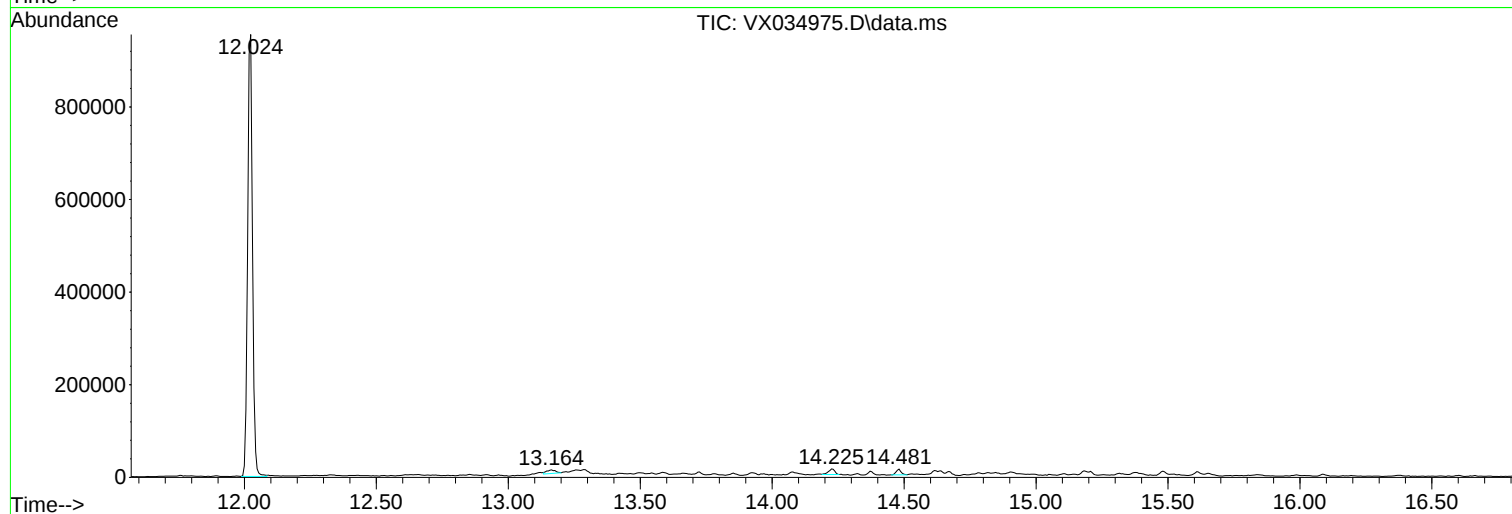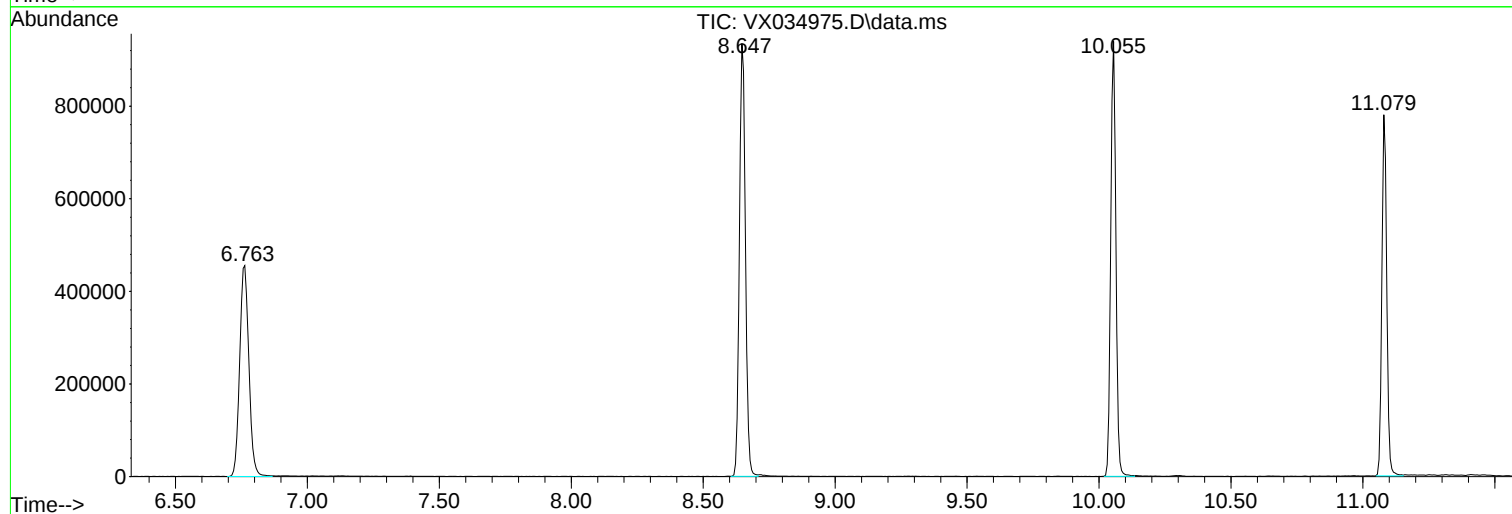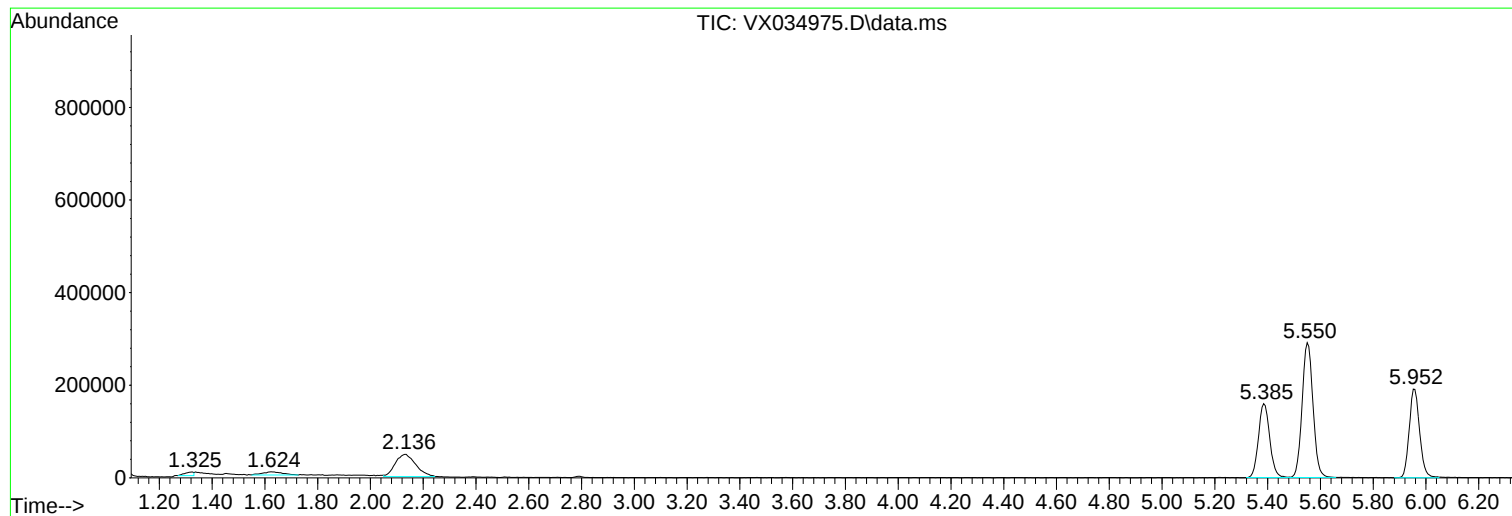

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040723\
Data File : VX034975.D
Acq On : 07 Apr 2023 17:44
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.136 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.136	15.37 ug/l	256798	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Ethanol			46	C2H6O	000064-17-5	43
2	Dimethyl ether			46	C2H6O	000115-10-6	9
3	Formic acid			46	CH2O2	000064-18-6	4
4	2,2-Dichloroethyl methyl ether			128	C3H6Cl2O	034862-07-2	4
5	Oxalic acid			90	C2H2O4	000144-62-7	4

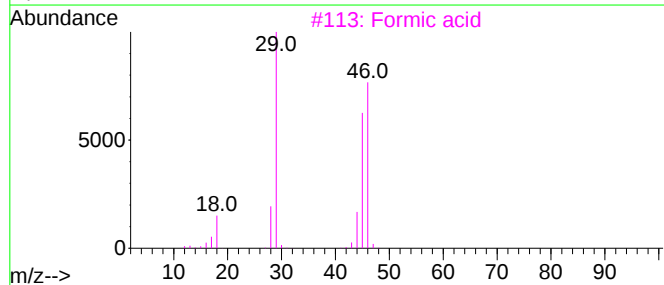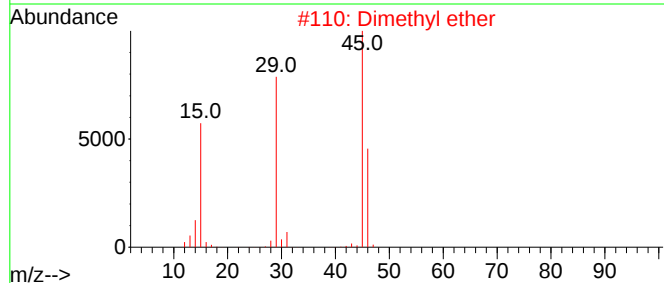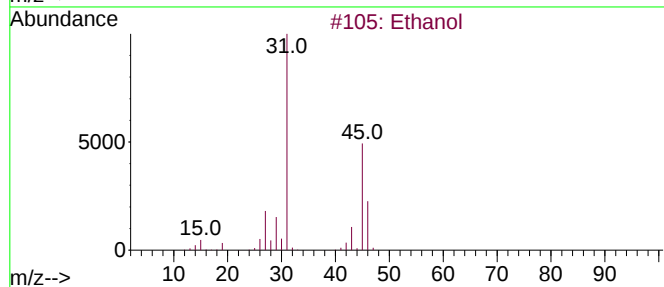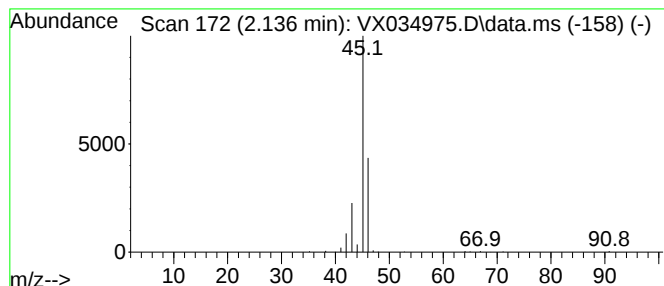

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040723\
Data File : VX034975.D
Acq On : 07 Apr 2023 17:44
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.136	2.136	15.4	ug/l	256798	1	5.556	835497	50.0