


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040723\
Data File : VX034968.D
Acq On : 07 Apr 2023 13:41
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032923W.M
Title : SW846 8260
Last Update : Sat Apr 01 01:50:18 2023

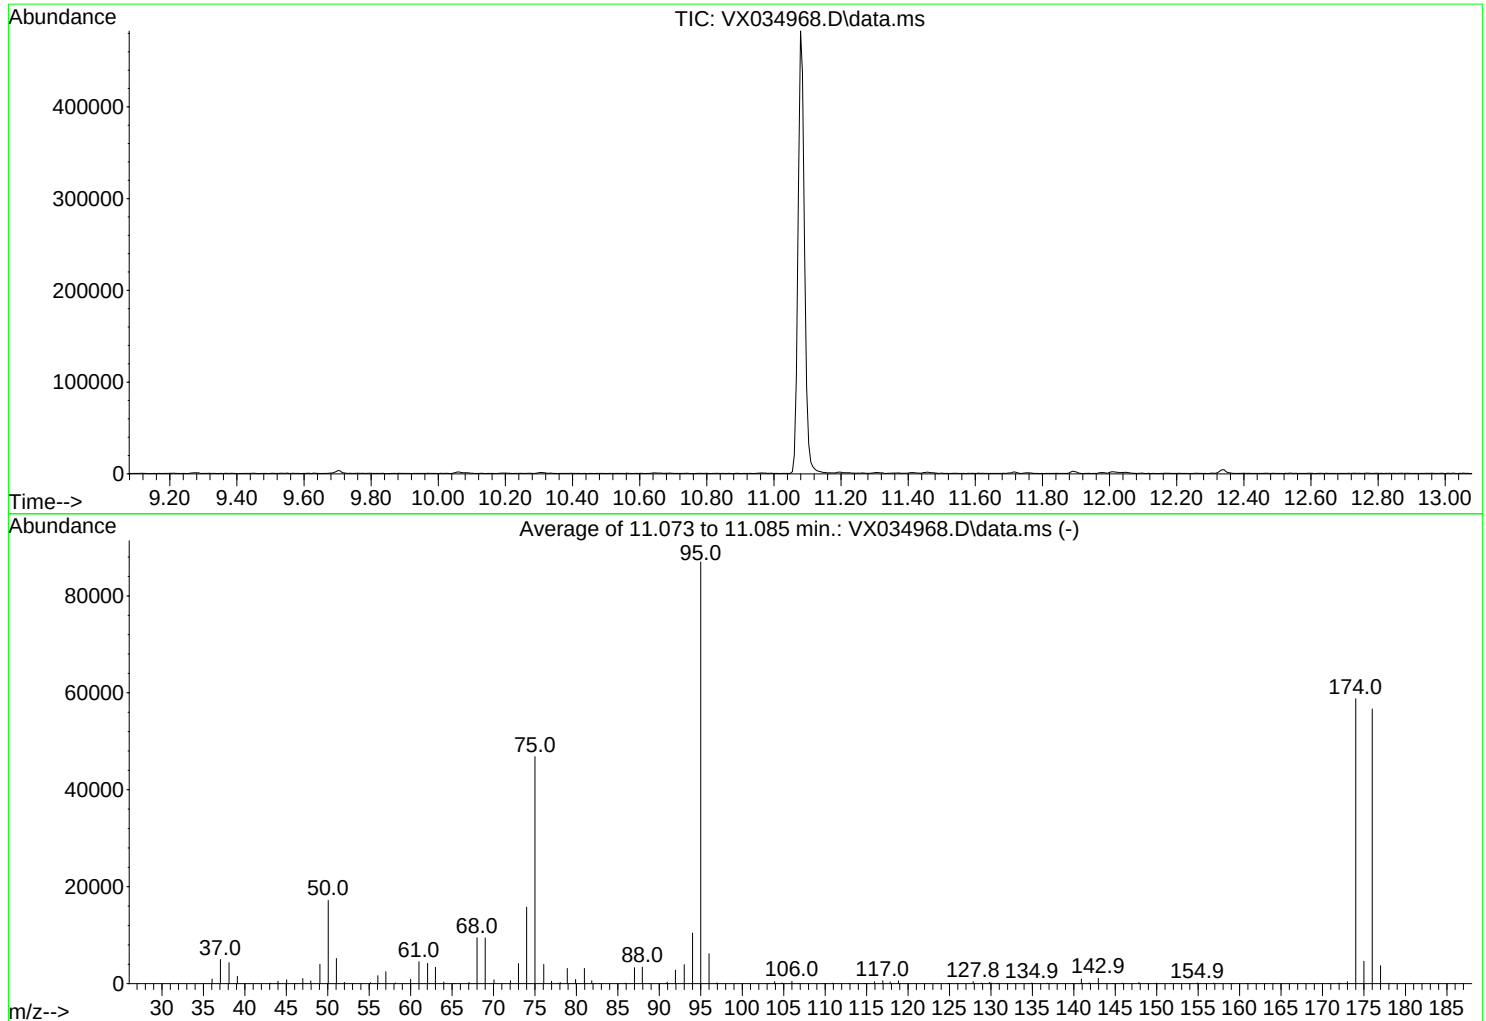

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	17173	PASS
75	95	30	60	53.8	46843	PASS
95	95	100	100	100.0	87024	PASS
96	95	5	9	7.1	6186	PASS
173	174	0.00	2	0.7	400	PASS
174	95	50	100	67.6	58792	PASS
175	174	5	9	7.8	4614	PASS
176	174	95	101	96.4	56669	PASS
177	176	5	9	6.5	3711	PASS