

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040819\  
 Data File : VX008742.D  
 Acq On : 08 Apr 2019 14:03  
 Operator : JC/SP  
 Sample : K2295-17  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 SS037MW311-190404

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.598       | 552           | 565         | 590          | rBV      | 2320465        | 6366224       | 100.00%         | 37.604%       |
| 2         | 5.500       | 699           | 713         | 728          | rBV      | 114983         | 332001        | 5.22%           | 1.961%        |
| 3         | 5.665       | 728           | 740         | 754          | rVV      | 203770         | 574932        | 9.03%           | 3.396%        |
| 4         | 6.067       | 795           | 806         | 821          | rBV      | 144921         | 386307        | 6.07%           | 2.282%        |
| 5         | 6.860       | 922           | 936         | 955          | rBV      | 339526         | 798275        | 12.54%          | 4.715%        |
| 6         | 7.214       | 984           | 994         | 1019         | rBV      | 770291         | 1636290       | 25.70%          | 9.665%        |
| 7         | 8.713       | 1233          | 1240        | 1253         | rBV      | 688238         | 1088511       | 17.10%          | 6.430%        |
| 8         | 9.335       | 1335          | 1342        | 1356         | rBV      | 2469192        | 3496920       | 54.93%          | 20.656%       |
| 9         | 10.115      | 1463          | 1470        | 1482         | rBV      | 627422         | 874665        | 13.74%          | 5.166%        |
| 10        | 11.134      | 1632          | 1637        | 1647         | rBV      | 485471         | 638425        | 10.03%          | 3.771%        |
| 11        | 12.079      | 1783          | 1792        | 1802         | rBV      | 592094         | 737027        | 11.58%          | 4.353%        |


Sum of corrected areas: 16929577

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040819\  
Data File : VX008742.D  
Acq On : 08 Apr 2019 14:03  
Operator : JC/SP  
Sample : K2295-17  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS037MW311-190404

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

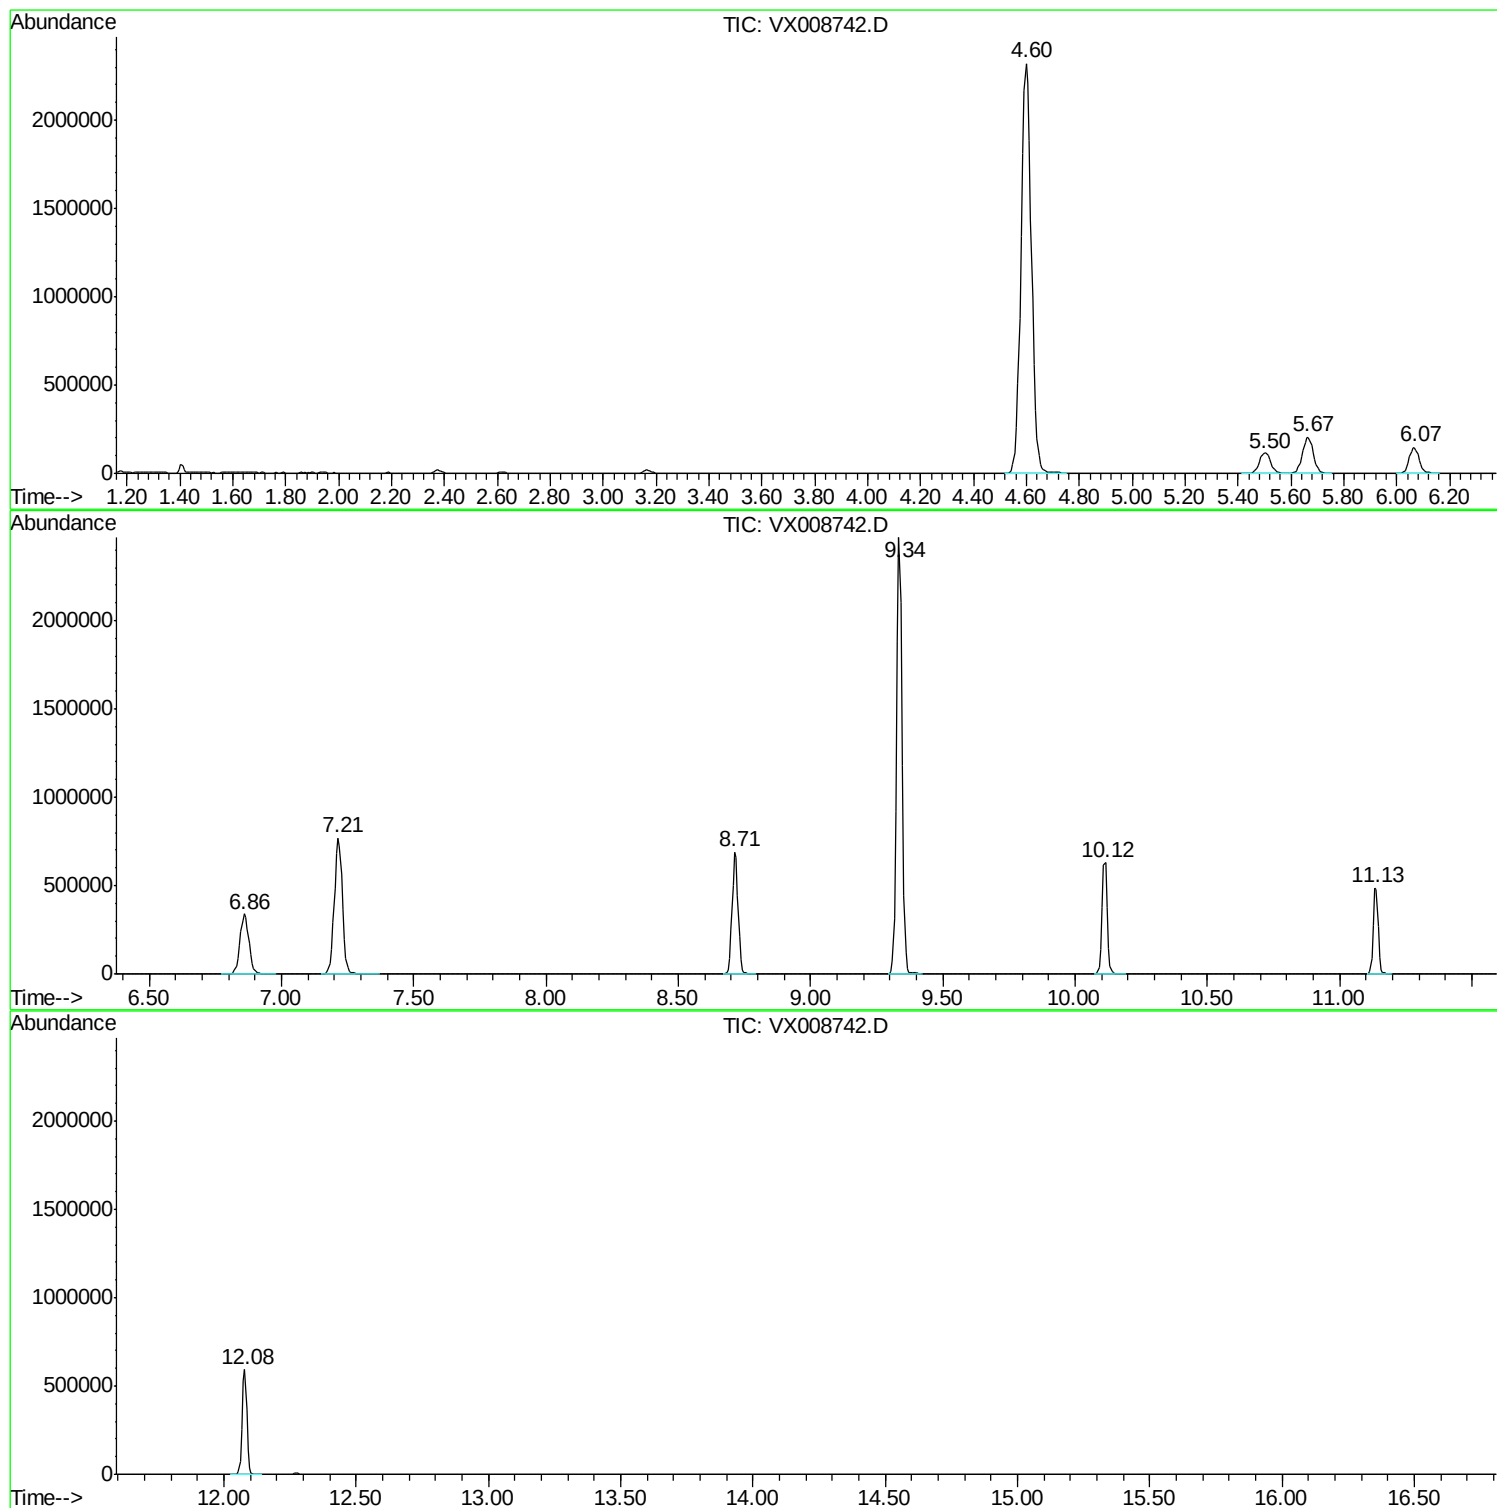

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX040819\  
Data File : VX008742.D  
Acq On : 08 Apr 2019 14:03  
Operator : JC/SP  
Sample : K2295-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS037MW311-190404

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX040819\  
Data File : VX008742.D  
Acq On : 08 Apr 2019 14:03  
Operator : JC/SP  
Sample : K2295-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
SS037MW311-190404

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X040319W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |