


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX040819\
Data File : VX008735.D
Acq On : 08 Apr 2019 09:15
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260
Last Update : Thu Apr 04 04:47:41 2019

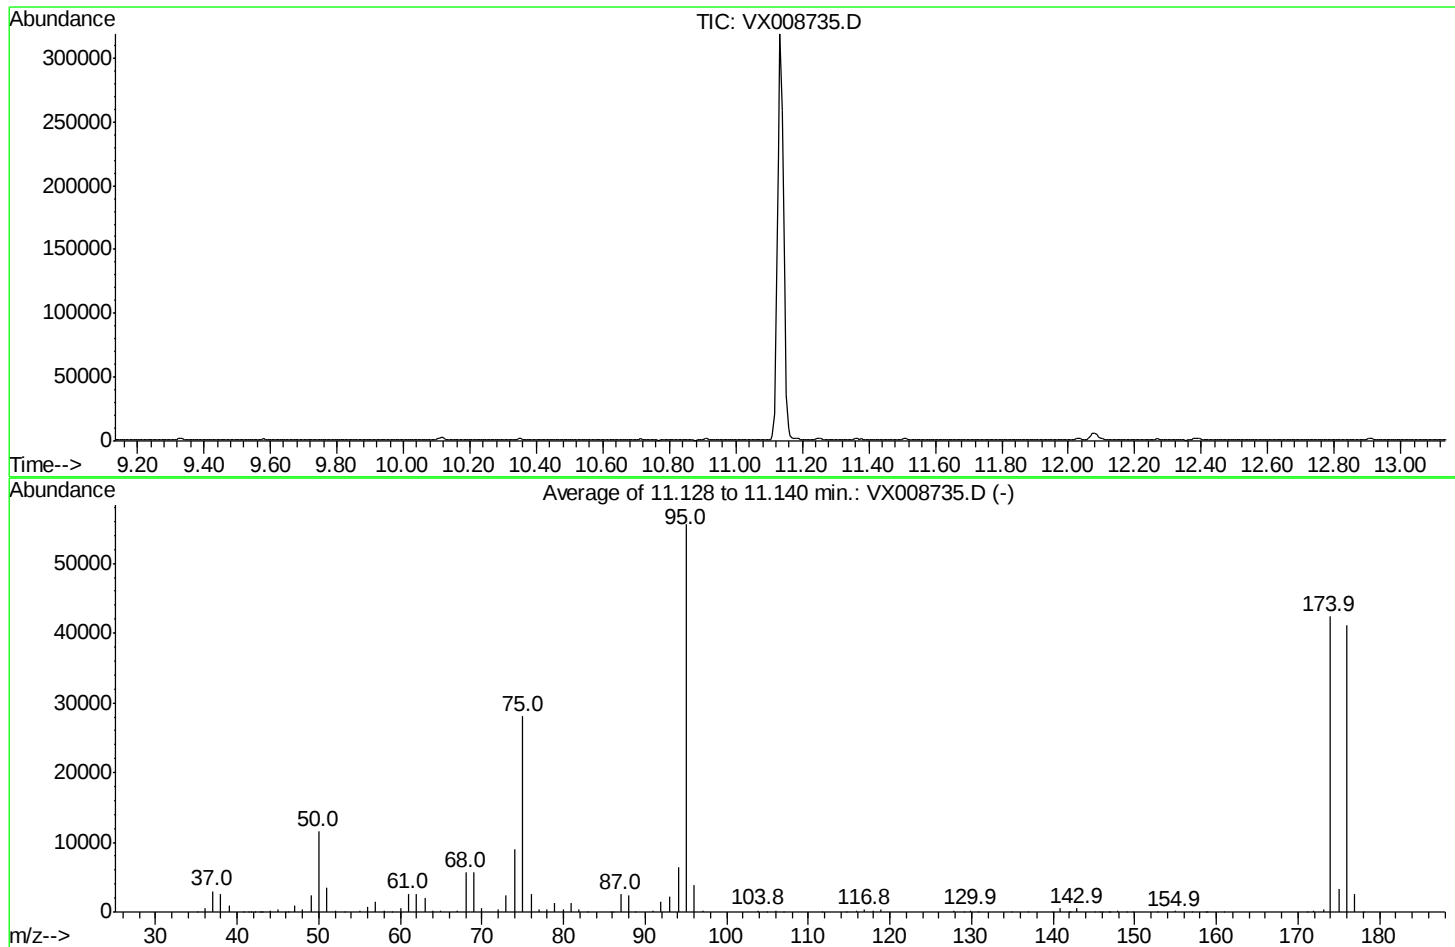

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	11512	PASS
75	95	30	60	50.5	28074	PASS
95	95	100	100	100.0	55605	PASS
96	95	5	9	6.8	3806	PASS
173	174	0.00	2	0.8	330	PASS
174	95	50	100	76.2	42378	PASS
175	174	5	9	7.8	3312	PASS
176	174	95	101	97.1	41138	PASS
177	176	5	9	6.5	2659	PASS