

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
 Data File : VX028041.D
 Acq On : 08 Apr 2022 20:37
 Operator : JC/MD
 Sample : N2334-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP040522

Quant Time: Apr 11 01:20:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 07 18:12:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	102880	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	151542	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	128723	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	57420	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	61521	39.393	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	78.780%		
35) Dibromofluoromethane	5.391	113	54409	53.488	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	106.980%		
50) Toluene-d8	8.653	98	168693	46.478	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	92.960%		
62) 4-Bromofluorobenzene	11.079	95	68635	44.484	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	88.960%		
Target Compounds						Qvalue
3) Chloromethane	1.246	50	3796	4.693	ug/l #	42
5) Bromomethane	1.618	94	109	0.905	ug/l #	3
6) Chloroethane	1.916	64	292	1.954	ug/l #	64
10) Methyl Iodide	2.459	142	23	6.820	ug/l #	41
11) Tert butyl alcohol	2.959	59	2011	7.308	ug/l #	92
13) Acrolein	2.215	56	118	0.469	ug/l #	1
14) Allyl chloride	2.782	41	5140	2.781	ug/l #	68
15) Acrylonitrile	2.861	53	473	0.716	ug/l #	39
16) Acetone	2.380	43	2717	0.762	ug/l	93
17) Carbon Disulfide	2.520	76	551	Below Cal	#	75
18) Methyl Acetate	2.782	43	11715	7.214	ug/l #	46
19) Methyl tert-butyl Ether	3.111	73	1828	0.479	ug/l #	58
20) Methylene Chloride	2.788	84	304	2.576	ug/l #	33
22) Diisopropyl ether	3.763	45	3863	1.017	ug/l #	79
23) Vinyl Acetate	3.763	43	2042	0.613	ug/l #	66
25) 2-Butanone	4.556	43	220	0.217	ug/l #	44
31) Cyclohexane	5.470	56	1711	0.904	ug/l #	79
36) 1,1-Dichloropropene	5.556	75	7107	4.752	ug/l #	50
38) Carbon Tetrachloride	5.550	117	10008	6.182	ug/l #	16
39) Methylcyclohexane	7.379	83	683	0.394	ug/l #	71
40) Benzene	6.044	78	359294	86.044	ug/l	98
41) Methacrylonitrile	5.135	41	211	0.229	ug/l #	18
42) 1,2-Dichloroethane	6.037	62	3283	1.858	ug/l #	73
48) Methyl methacrylate	7.769	41	404	0.299	ug/l #	63
52) Toluene	8.720	92	1691	0.631	ug/l	88
55) 1,1,2-Trichloroethane	9.110	97	1098	1.039	ug/l #	16
67) Ethyl Benzene	10.195	91	1223	0.249	ug/l	95
73) Isopropylbenzene	10.963	105	3000	0.674	ug/l	92
76) 1,2,3-Trichloropropane	11.079	75	40959	29.080	ug/l #	38
78) n-propylbenzene	11.305	91	4284	0.807	ug/l	95
79) 2-Chlorotoluene	11.305	91	4284	1.311	ug/l #	40
81) trans-1,4-Dichloro-2-b...	11.079	75	40959	89.385	ug/l #	15
82) 4-Chlorotoluene	11.305	91	4284	1.126	ug/l #	45
90) Hexachloroethane	12.701	117	1497	2.638	ug/l #	10

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
Data File : VX028041.D
Acq On : 08 Apr 2022 20:37
Operator : JC/MD
Sample : N2334-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP040522

Quant Time: Apr 11 01:20:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 07 18:12:28 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
Data File : VX028041.D
Acq On : 08 Apr 2022 20:37
Operator : JC/MD
Sample : N2334-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP040522

Quant Time: Apr 11 01:20:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 07 18:12:28 2022
Response via : Initial Calibration




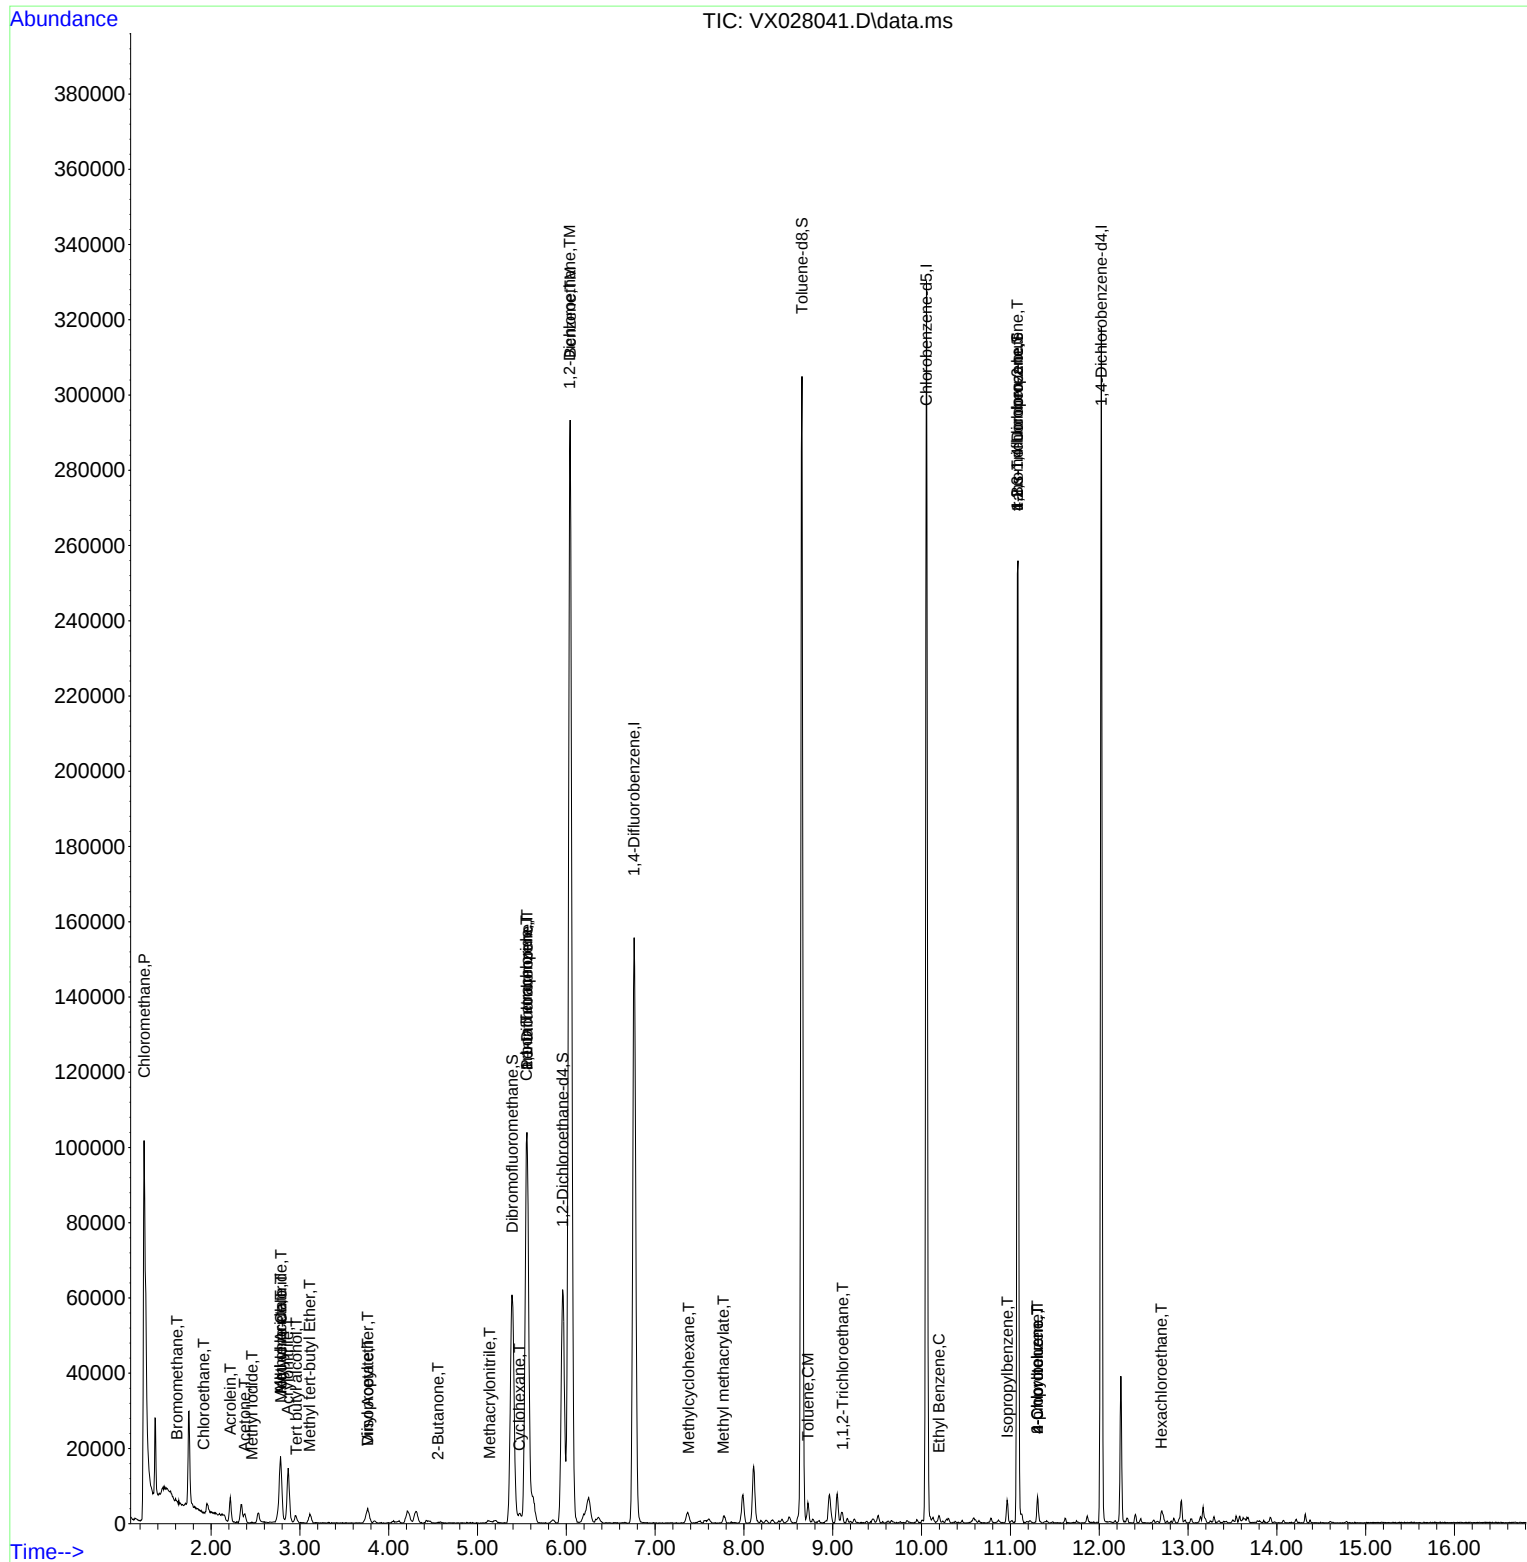




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion:168 Resp: 102880
Ion Ratio Lower Upper
168 100
99 55.2 41.7 62.5

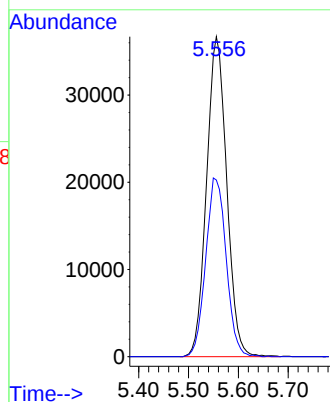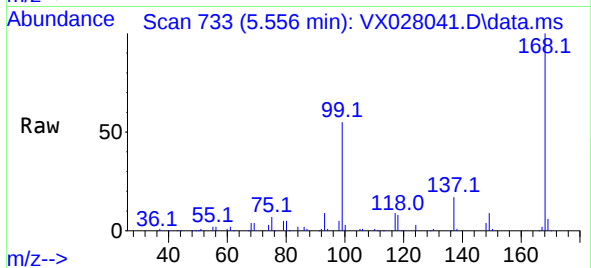

#3
Chloromethane
Concen: 4.693 ug/l
RT: 1.246 min Scan# 26
Delta R.T. -0.042 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 50 Resp: 3796
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#


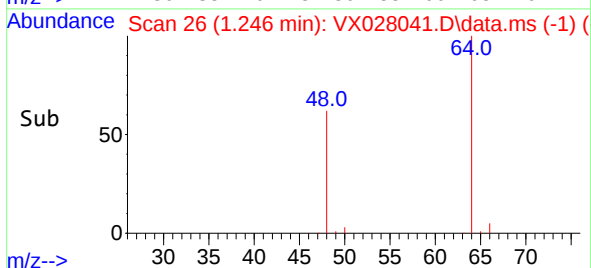




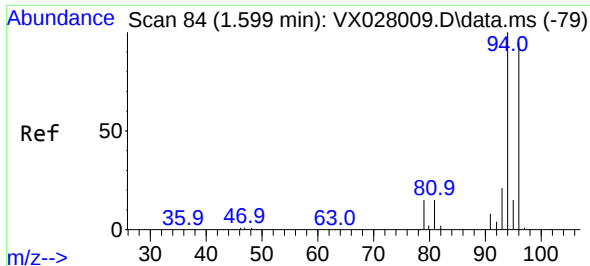

#5
Bromomethane
Concen: 0.905 ug/l
RT: 1.618 min Scan# 81
Delta R.T. 0.019 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 94 Resp: 109
Ion Ratio Lower Upper
94 100
96 0.0 75.3 112.9#

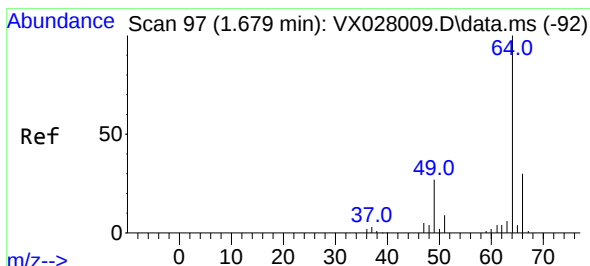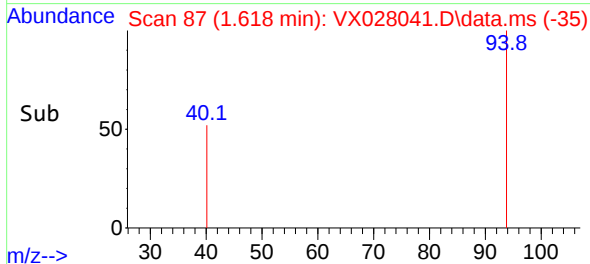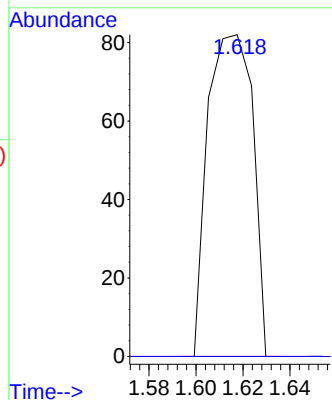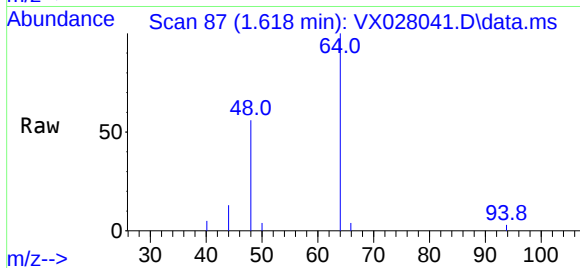

#6
Chloroethane
Concen: 1.954 ug/l
RT: 1.916 min Scan# 136
Delta R.T. 0.237 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 64 Resp: 292
Ion Ratio Lower Upper
64 100
66 11.7 25.3 37.9#


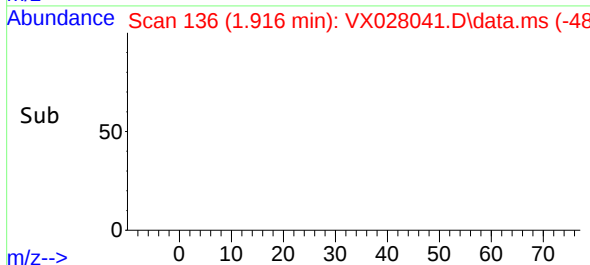
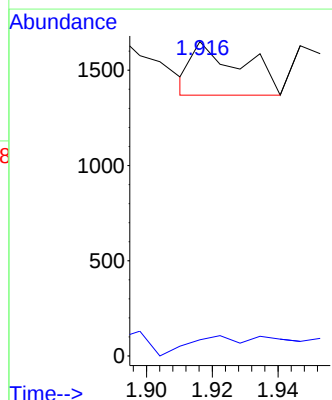
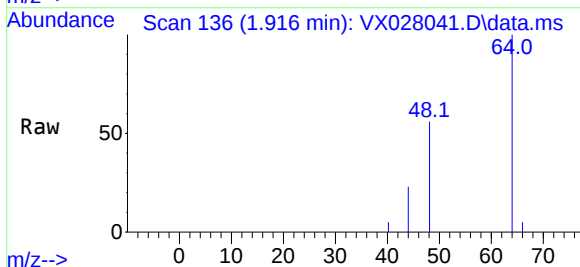




#10
Methyl Iodide
Concen: 6.820 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion:142 Resp: 23
Ion Ratio Lower Upper
142 100
127 0.0 33.9 50.9#
141 0.0 11.4 17.2#

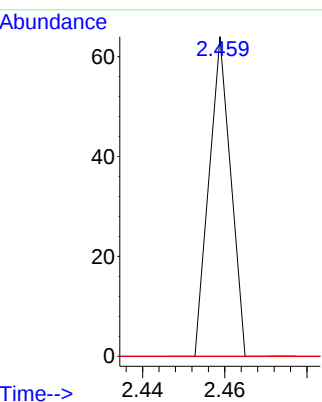

#11
Tert butyl alcohol
Concen: 7.308 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 59 Resp: 2011
Ion Ratio Lower Upper
59 100
57 7.5 8.3 12.5#


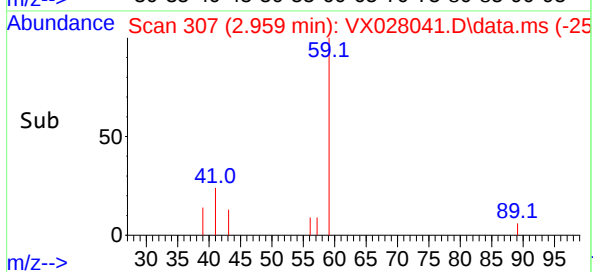
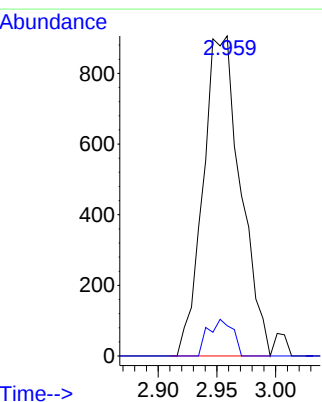





#13
Acrolein
Concen: 0.469 ug/l
RT: 2.215 min Scan# 118
Delta R.T. -0.018 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 56 Resp: 118
Ion Ratio Lower Upper
56 100
55 2839.8 55.0 82.6#



#14
Allyl chloride
Concen: 2.781 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.116 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 41 Resp: 5140
Ion Ratio Lower Upper
41 100
39 53.7 50.4 75.6
76 1.5 32.7 49.1#


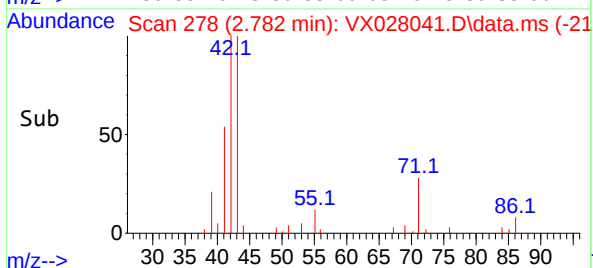
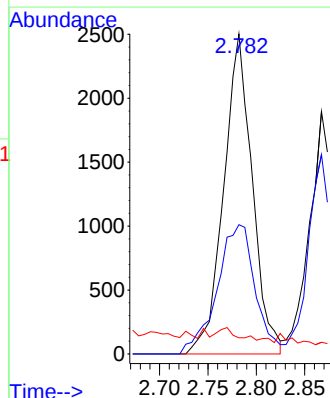





#15
Acrylonitrile
Concen: 0.716 ug/l
RT: 2.861 min Scan# 211
Delta R.T. -0.201 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 53 Resp: 473
Ion Ratio Lower Upper
53 100
52 4.7 65.7 98.5#
51 34.5 28.4 42.6



#16
Acetone
Concen: 0.762 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.007 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 43 Resp: 2717
Ion Ratio Lower Upper
43 100
58 31.6 28.8 43.2


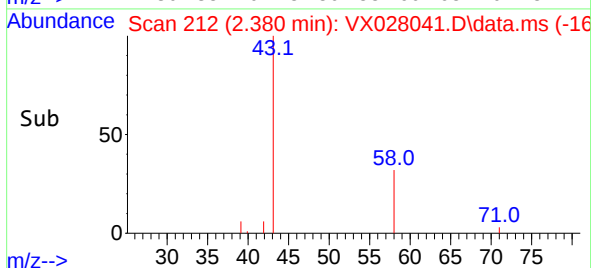






#17
Carbon Disulfide
Concen: Below Cal
RT: 2.520 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 76 Resp: 551
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

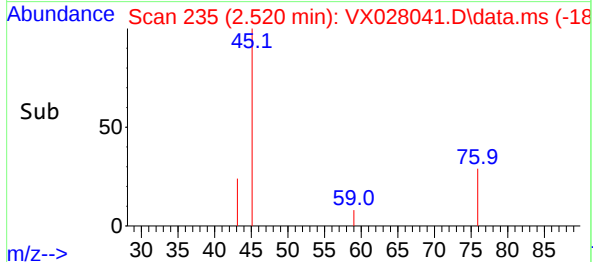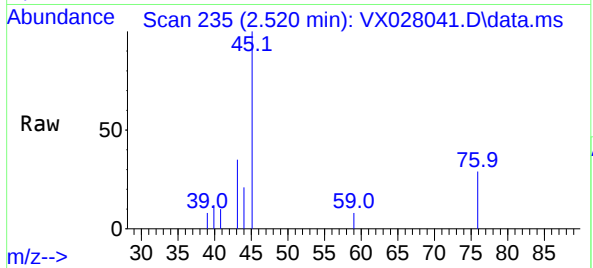

#18
Methyl Acetate
Concen: 7.214 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.079 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 43 Resp: 11715
Ion Ratio Lower Upper
43 100
74 0.0 22.8 34.2#


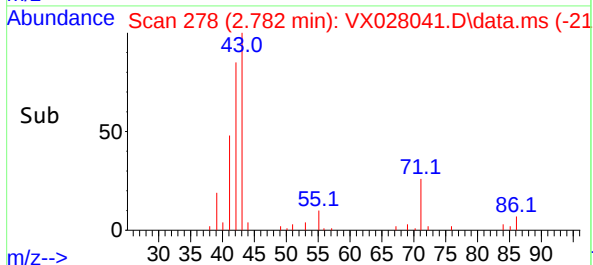
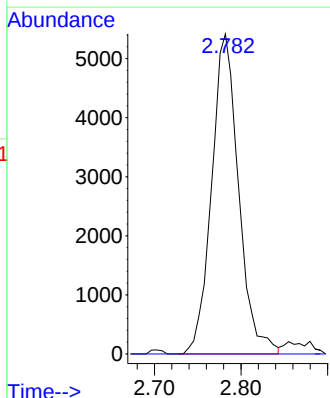
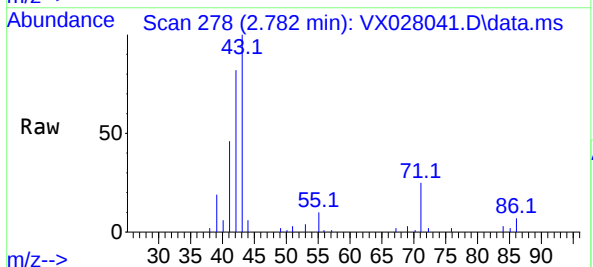




#19
Methyl tert-butyl Ether
Concen: 0.479 ug/l
RT: 3.111 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 73 Resp: 1828
Ion Ratio Lower Upper
73 100
57 40.8 16.8 25.2#

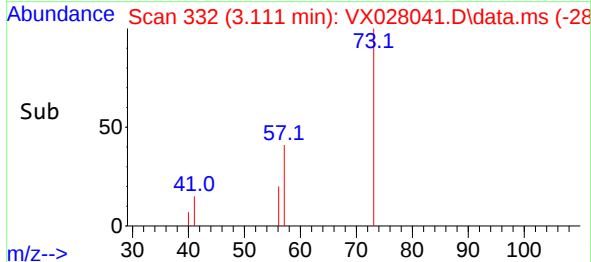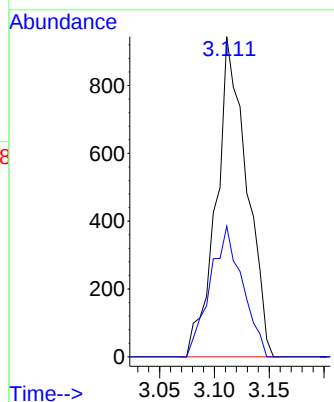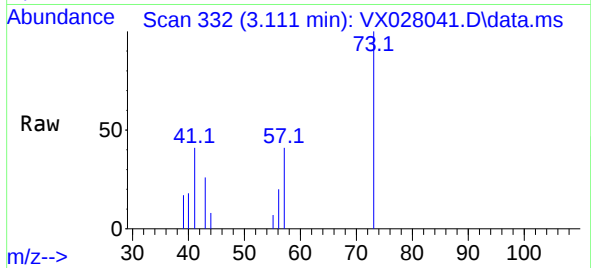

#20
Methylene Chloride
Concen: 2.576 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 84 Resp: 304
Ion Ratio Lower Upper
84 100
49 103.8 85.5 128.3
51 77.8 26.6 39.8#
86 195.6 51.5 77.3#


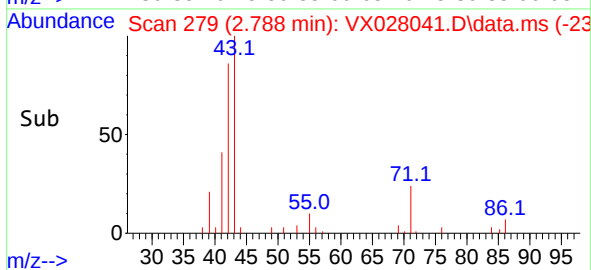
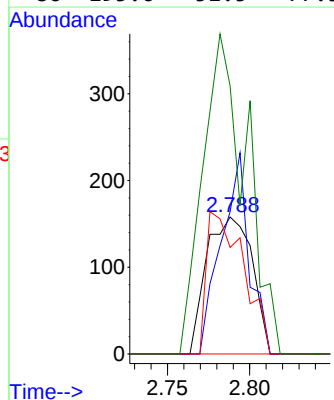





#22
Diisopropyl ether
Concen: 1.017 ug/l
RT: 3.763 min Scan# 41
Delta R.T. -0.001 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion:	45	Resp:	3863
Ion	Ratio	Lower	Upper
45	100		
43	46.6	50.8	76.2#
87	17.9	26.6	39.8#
59	10.8	10.5	15.7

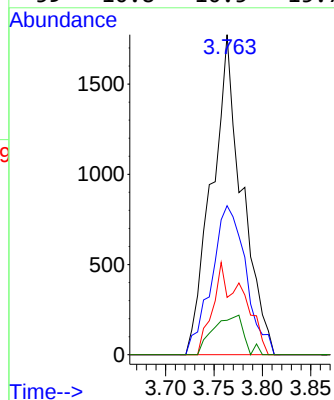

#23
Vinyl Acetate
Concen: 0.613 ug/l
RT: 3.763 min Scan# 439
Delta R.T. 0.042 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion:	43	Resp:	2042
Ion	Ratio	Lower	Upper
43	100		
86	0.0	10.8	16.2#

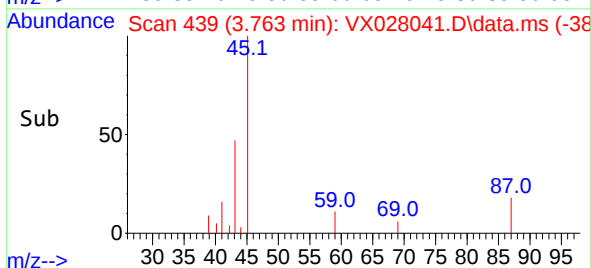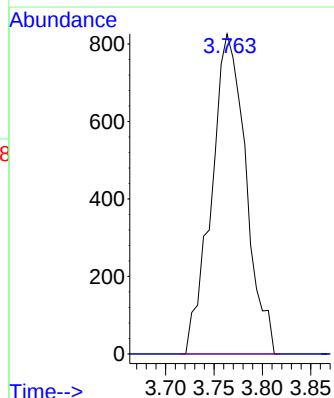



#25

2-Butanone

Concen: 0.217 ug/l

RT: 4.556 min Scan# 5

Delta R.T. 0.000 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37

Instrument :

MSVOA_X

ClientSampleId :





DUP040522

Tgt Ion: 43 Resp: 220

Ion Ratio Lower Upper

43 100

72 0.0 24.4 36.6#

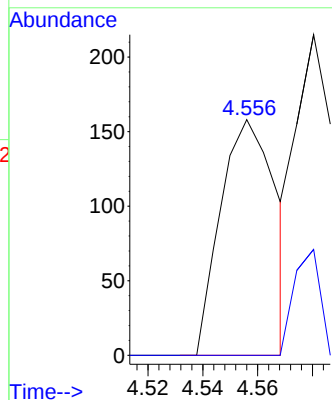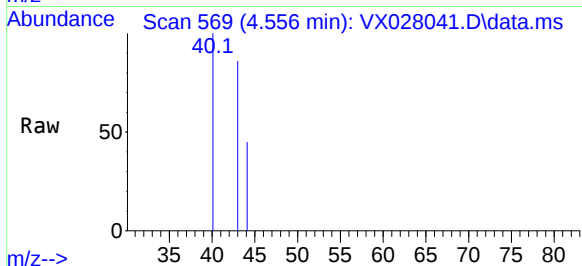

#31

Cyclohexane

Concen: 0.904 ug/l

RT: 5.470 min Scan# 719

Delta R.T. -0.001 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37




Tgt Ion: 56 Resp: 1711


Ion Ratio Lower Upper

56 100

69 48.0 26.7 40.1#

84 77.6 77.2 115.8


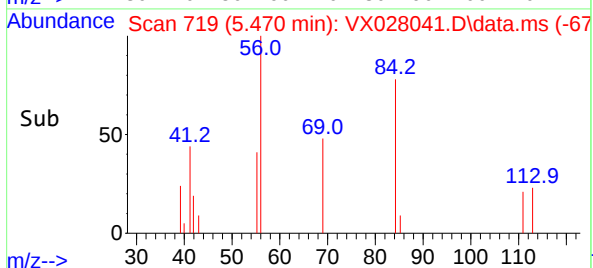
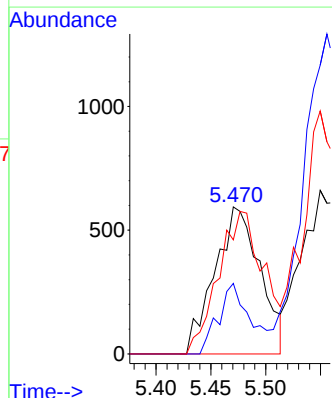
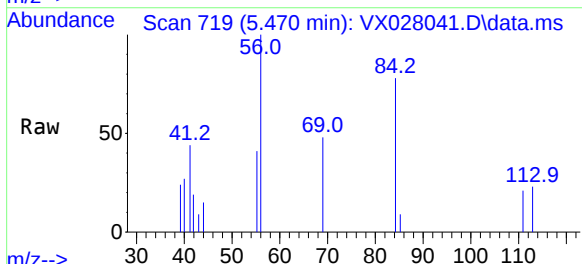




#33
1,2-Dichloroethane-d4
Concen: 39.393 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 65 Resp: 61521
Ion Ratio Lower Upper
65 100
67 51.5 0.0 107.4

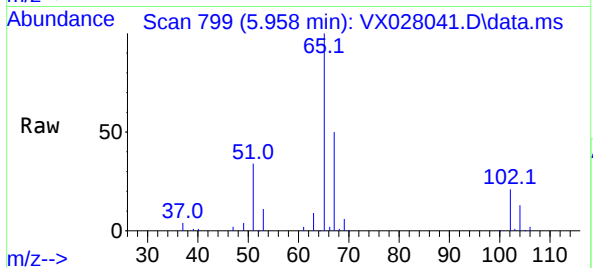

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 114 Resp: 151542
Ion Ratio Lower Upper
114 100
63 22.4 0.0 36.8
88 16.9 0.0 32.4

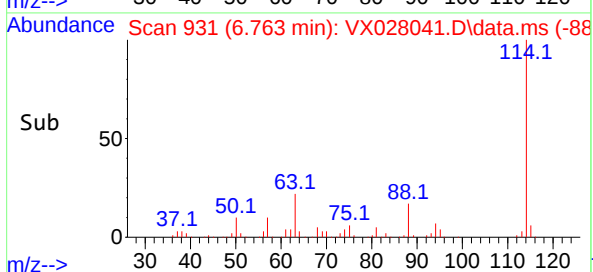

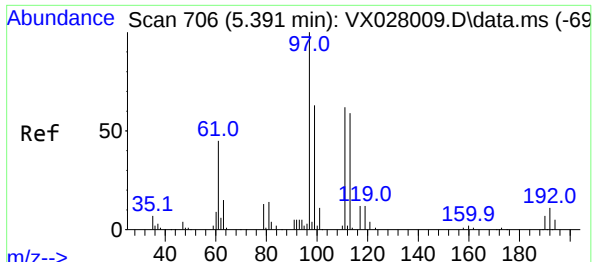

#35

Dibromofluoromethane

Concen: 53.488 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX028041.D


Acq: 08 Apr 2022 20:37

Instrument :

MSVOA_X

ClientSampleId :

DUP040522

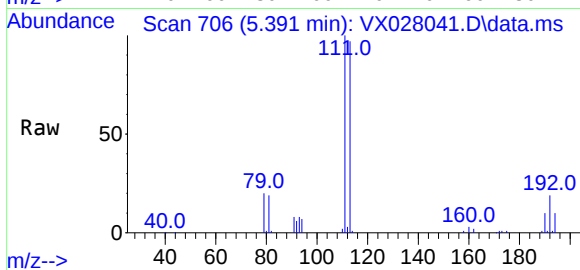




Tgt Ion:113 Resp: 54409

Ion Ratio Lower Upper

113 100

111 103.7 82.8 124.2

192 19.8 16.9 25.3

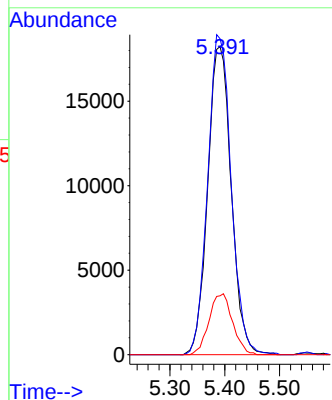

#36

1,1-Dichloropropene

Concen: 4.752 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37




Tgt Ion: 75 Resp: 7107


Ion Ratio Lower Upper

75 100

110 9.7 18.3 54.8#

77 0.0 24.8 37.2#


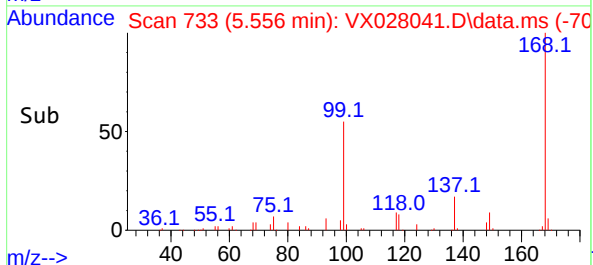
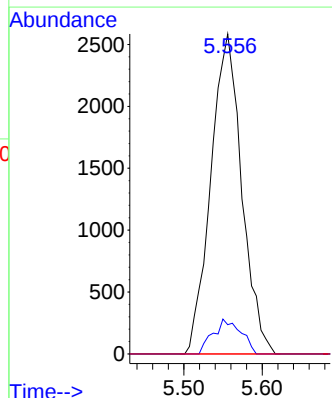
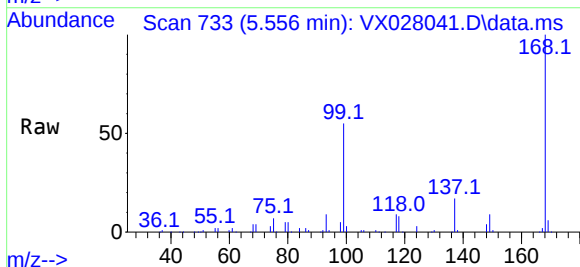




#38
Carbon Tetrachloride
Concen: 6.182 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion:117 Resp: 10008
Ion Ratio Lower Upper
117 100
119 5.0 77.3 115.9#
121 0.0 24.2 36.2#

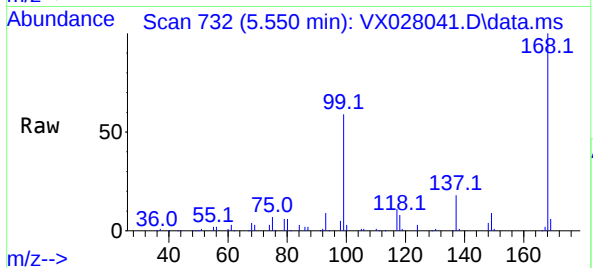

#39
Methylcyclohexane
Concen: 0.394 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 83 Resp: 683
Ion Ratio Lower Upper
83 100
55 89.5 54.6 81.8#
98 25.4 37.4 56.2#

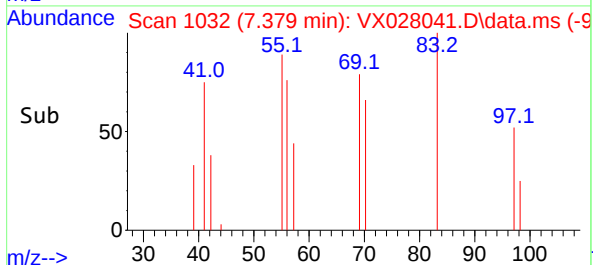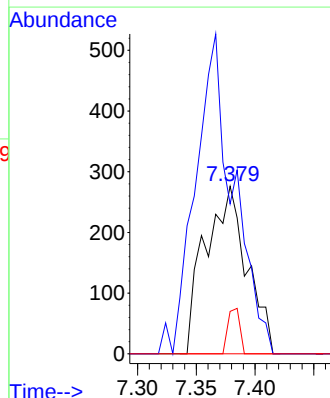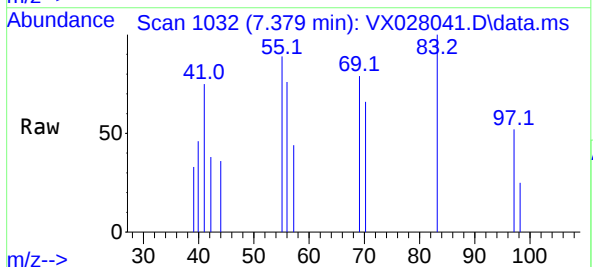



#40

Benzene

Concen: 86.044 ug/l

RT: 6.044 min Scan# 81

Delta R.T. -0.000 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37

Instrument :

MSVOA_X

ClientSampleId :





DUP040522

Tgt Ion: 78 Resp: 359294

Ion Ratio Lower Upper

78 100

77 23.3 19.3 28.9

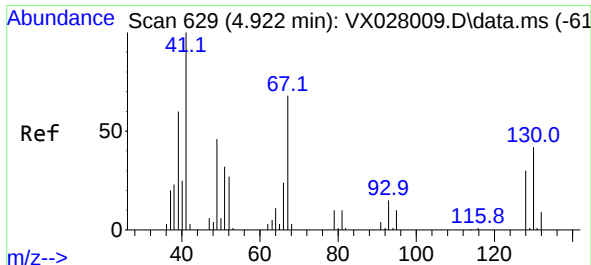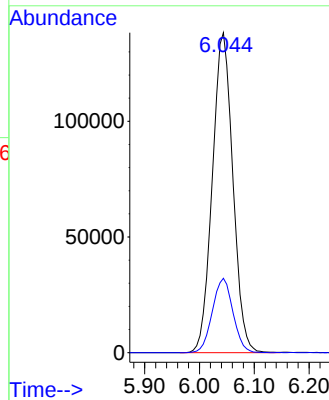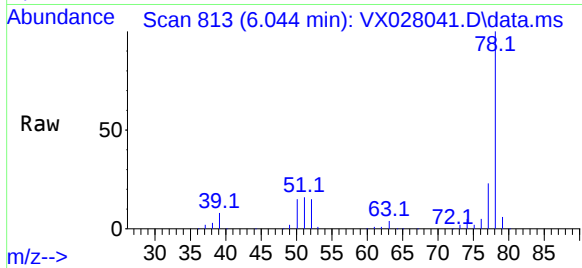

#41

Methacrylonitrile

Concen: 0.229 ug/l

RT: 5.135 min Scan# 664

Delta R.T. 0.213 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37

Tgt Ion: 41 Resp: 211




Ion Ratio Lower Upper


41 100

39 0.0 43.0 64.4#

67 0.0 70.2 105.4#

52 0.0 26.0 39.0#

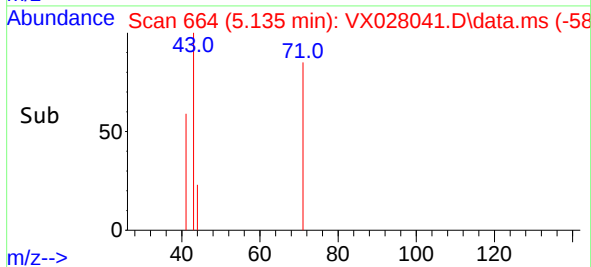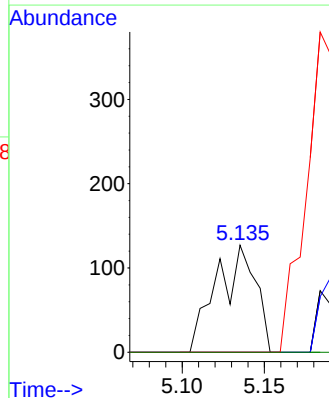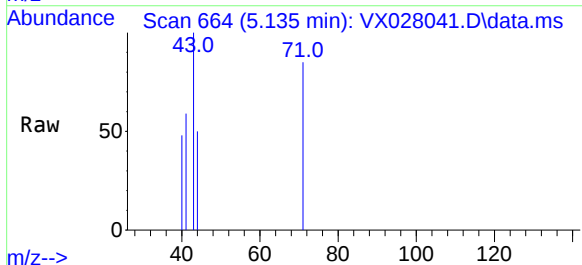



#42

1,2-Dichloroethane

Concen: 1.858 ug/l

RT: 6.037 min Scan# 81

Delta R.T. -0.049 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37

Instrument :

MSVOA_X

ClientSampleId :





DUP040522

Tgt Ion: 62 Resp: 3283

Ion Ratio Lower Upper

62 100

98 0.0 0.0 20.4

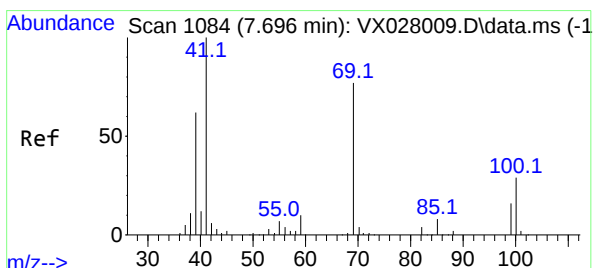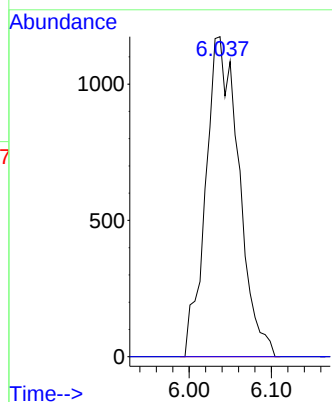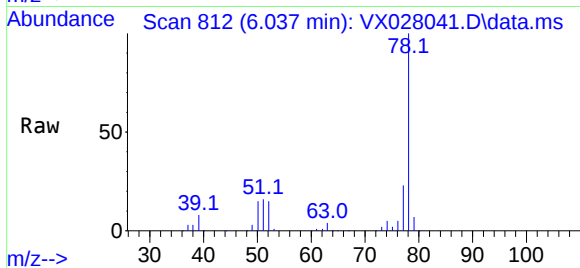

#48

Methyl methacrylate

Concen: 0.299 ug/l

RT: 7.769 min Scan# 1096

Delta R.T. 0.073 min

Lab File: VX028041.D

Acq: 08 Apr 2022 20:37




Tgt Ion: 41 Resp: 404


Ion Ratio Lower Upper

41 100

69 49.3 82.5 123.7#

39 60.6 43.8 65.8


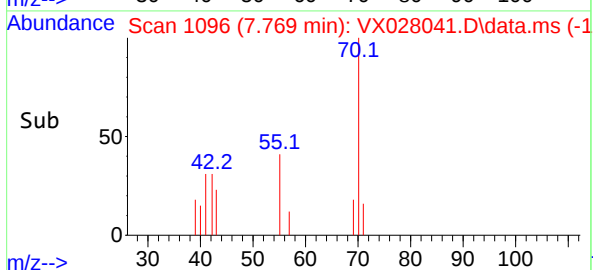
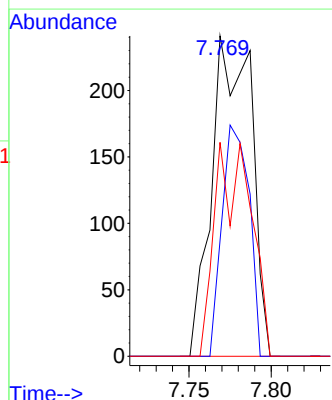
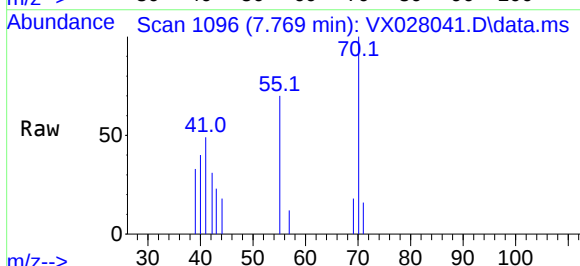




#50
Toluene-d8
Concen: 46.478 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 98 Resp: 168693
Ion Ratio Lower Upper
98 100
100 64.3 52.6 78.8

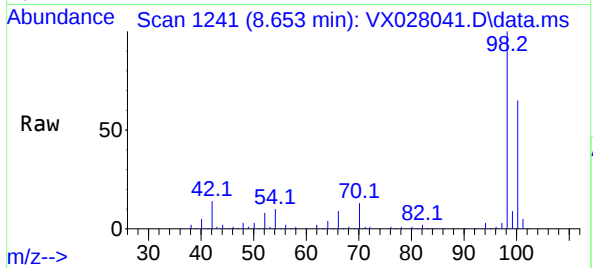

#52
Toluene
Concen: 0.631 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 92 Resp: 1691
Ion Ratio Lower Upper
92 100
91 188.2 137.5 206.3

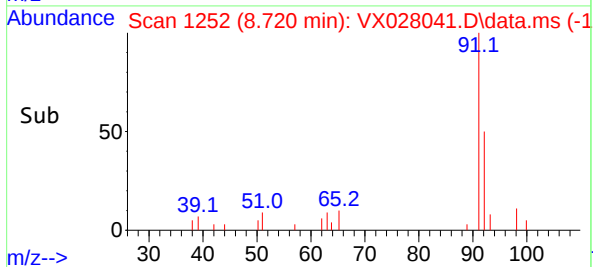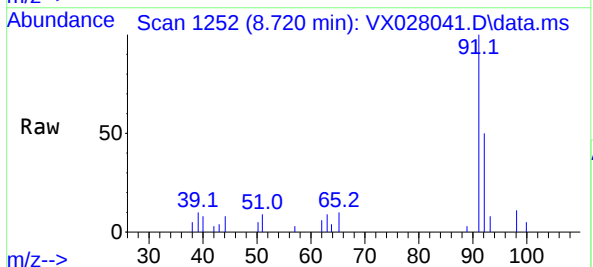







#55
1,1,2-Trichloroethane
Concen: 1.039 ug/l
RT: 9.110 min Scan# 11
Delta R.T. -0.043 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Instrument :
MSVOA_X
ClientSampleId :
DUP040522

Tgt Ion: 97 Resp: 1098




Ion	Ratio	Lower	Upper
97	100		
83	0.0	66.2	99.4#
85	0.0	42.9	64.3#
99	0.0	49.0	73.6#

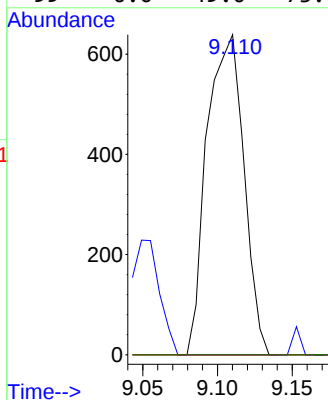


#62
4-Bromofluorobenzene
Concen: 44.484 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 95 Resp: 68635

Ion	Ratio	Lower	Upper
95	100		
174	66.5	0.0	163.0
176	64.1	0.0	155.0


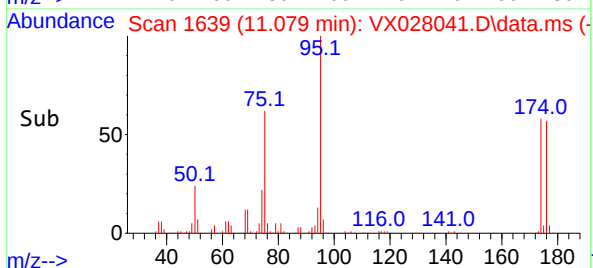
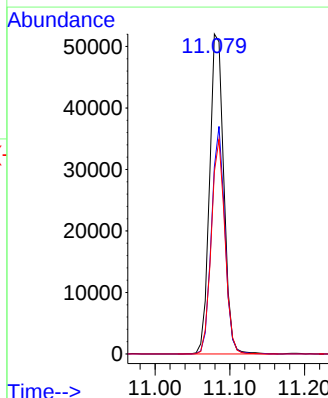





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion:117 Resp: 128723
Ion Ratio Lower Upper
117 100
82 63.0 41.8 62.8#
119 31.7 24.8 37.2

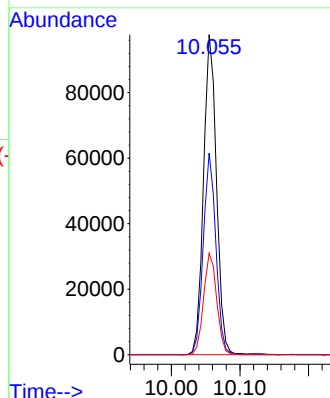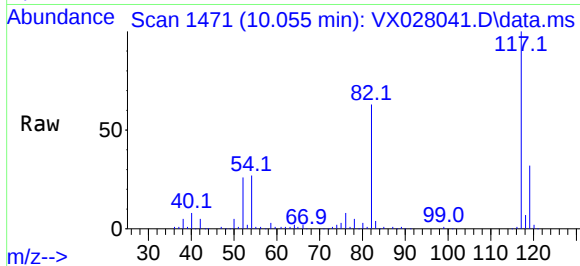

#67
Ethyl Benzene
Concen: 0.249 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 91 Resp: 1223
Ion Ratio Lower Upper
91 100
106 33.2 24.6 36.8


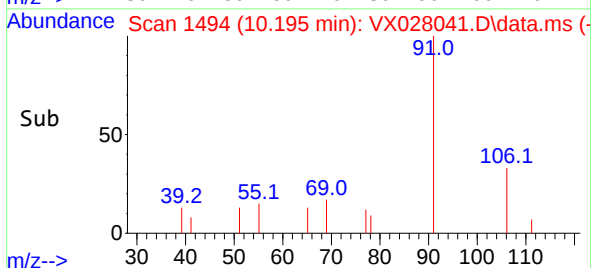
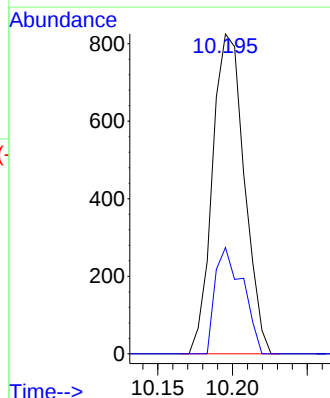
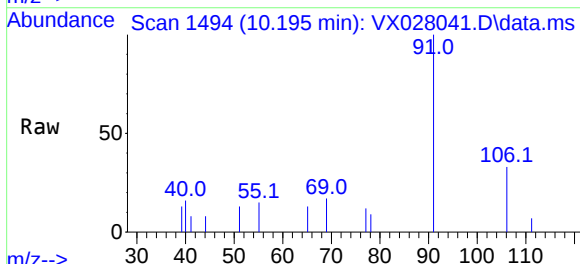




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion:152 Resp: 57420
Ion Ratio Lower Upper
152 100
115 64.2 37.5 112.7
150 156.1 0.0 338.2

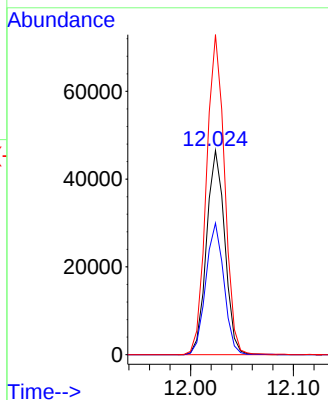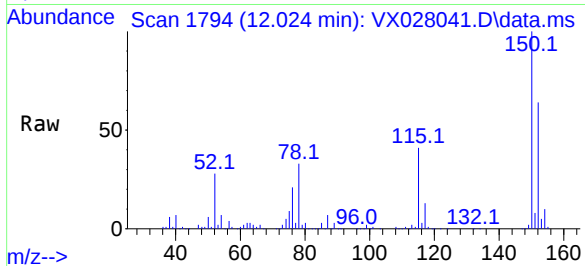

#73
Isopropylbenzene
Concen: 0.674 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion:105 Resp: 3000
Ion Ratio Lower Upper
105 100
120 23.1 13.5 40.5


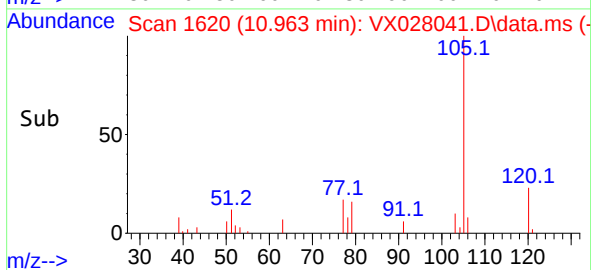
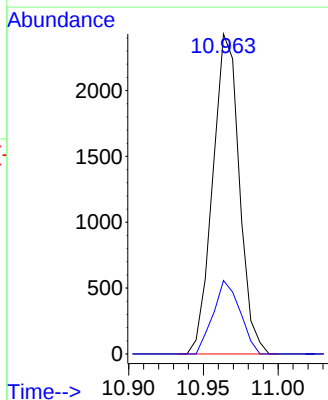
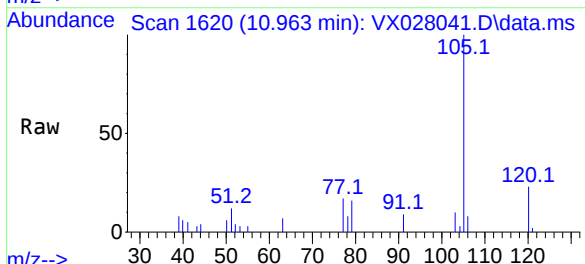




#76
1,2,3-Trichloropropane
Concen: 29.080 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 75 Resp: 40959
Ion Ratio Lower Upper
75 100
77 0.9 19.4 58.2#

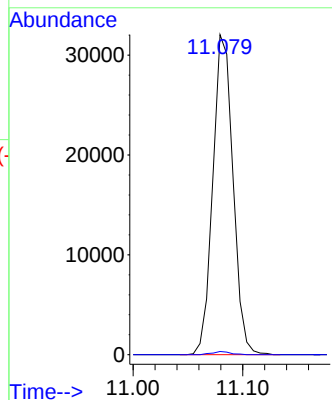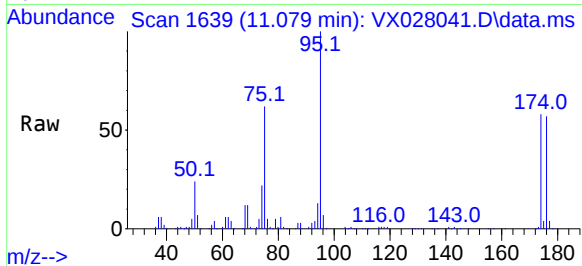

#78
n-propylbenzene
Concen: 0.807 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 91 Resp: 4284
Ion Ratio Lower Upper
91 100
120 20.7 11.6 34.8


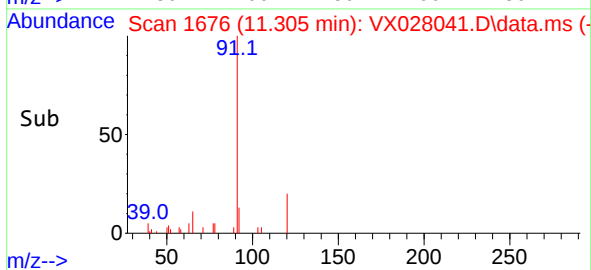
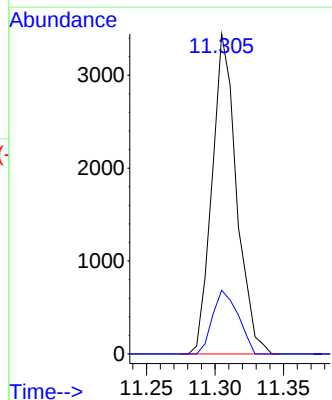
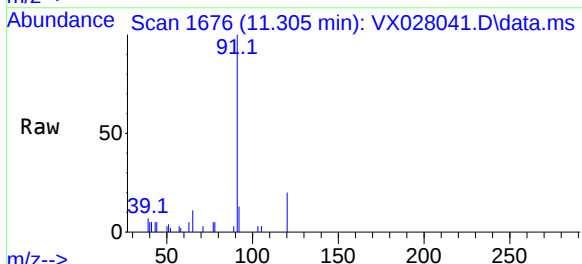




#79
2-Chlorotoluene
Concen: 1.311 ug/l
RT: 11.305 min Scan# 1639
Delta R.T. -0.061 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37




Instrument :
MSVOA_X
ClientSampleId :
DUP040522


Tgt Ion: 91 Resp: 4284
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

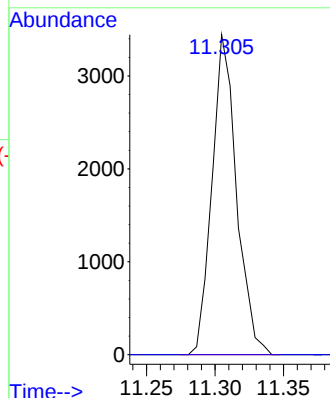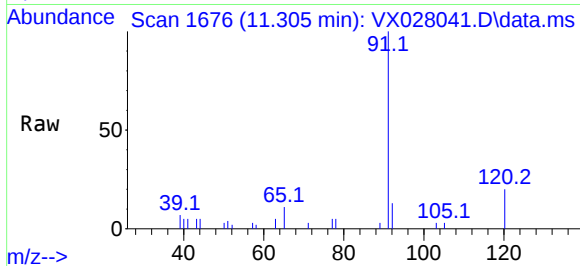

#81
trans-1,4-Dichloro-2-butene
Concen: 89.385 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 75 Resp: 40959
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#


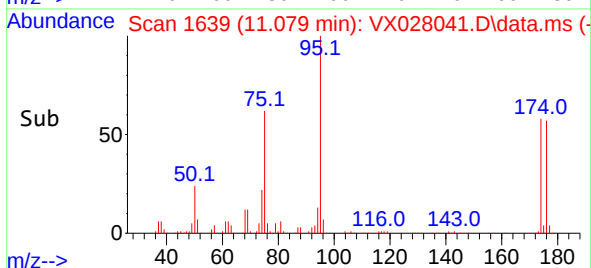

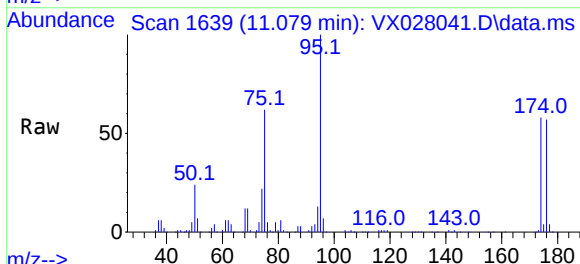




#82
4-Chlorotoluene
Concen: 1.126 ug/l
RT: 11.305 min Scan# 1105
Delta R.T. -0.152 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Instrument :
MSVOA_X
ClientSampleId :
DUP040522

Tgt Ion: 91 Resp: 4284
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

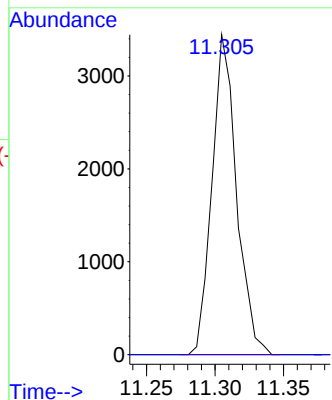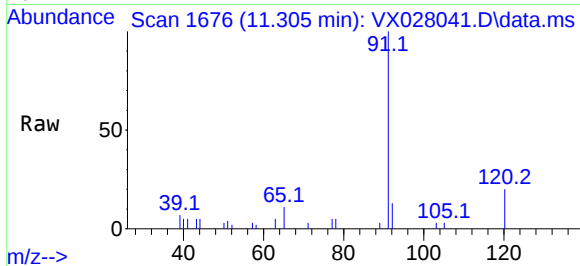

#90
Hexachloroethane
Concen: 2.638 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.159 min
Lab File: VX028041.D
Acq: 08 Apr 2022 20:37

Tgt Ion: 117 Resp: 1497
Ion Ratio Lower Upper
117 100
201 0.0 39.5 118.5#

