

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
 Data File : VX028023.D
 Acq On : 08 Apr 2022 13:38
 Operator : JC/MD
 Sample : N2333-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M

Title : SW846 8260

Signal : TIC: VX028023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	21	29	42	rBV	12950	47355	9.54%	1.672%
2	2.380	207	212	217	rBV	4653	6939	1.40%	0.245%
3	5.391	694	706	722	rBV2	63466	177612	35.78%	6.272%
4	5.556	722	733	751	rVB	99586	279783	56.37%	9.880%
5	5.958	788	799	813	rBV	69347	181673	36.60%	6.415%
6	6.251	838	847	857	rBV3	2796	7694	1.55%	0.272%
7	6.763	922	931	943	rBV	158633	372720	75.09%	13.162%
8	8.110	1145	1152	1158	rVB4	2898	5815	1.17%	0.205%
9	8.653	1234	1241	1252	rBV	317253	496343	100.00%	17.527%
10	10.055	1465	1471	1482	rBV	346199	457510	92.18%	16.156%
11	11.085	1634	1640	1650	rVB	271738	360139	72.56%	12.718%
12	12.024	1789	1794	1804	rVB	358133	438237	88.29%	15.475%




Sum of corrected areas: 2831820

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
Data File : VX028023.D
Acq On : 08 Apr 2022 13:38
Operator : JC/MD
Sample : N2333-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

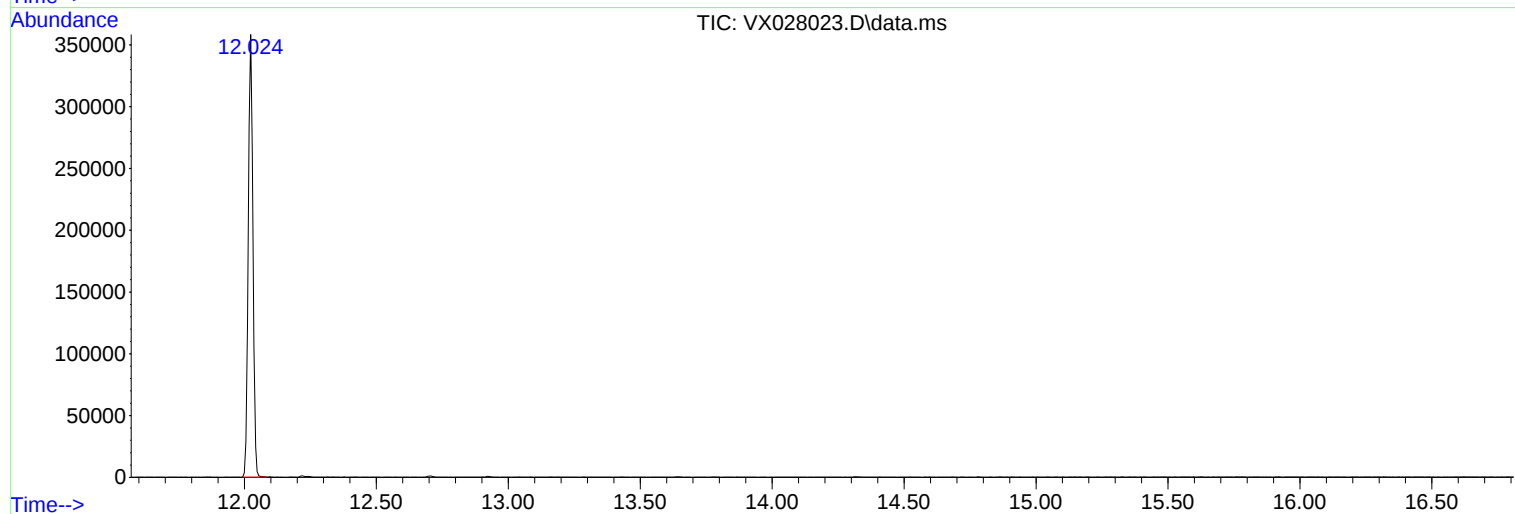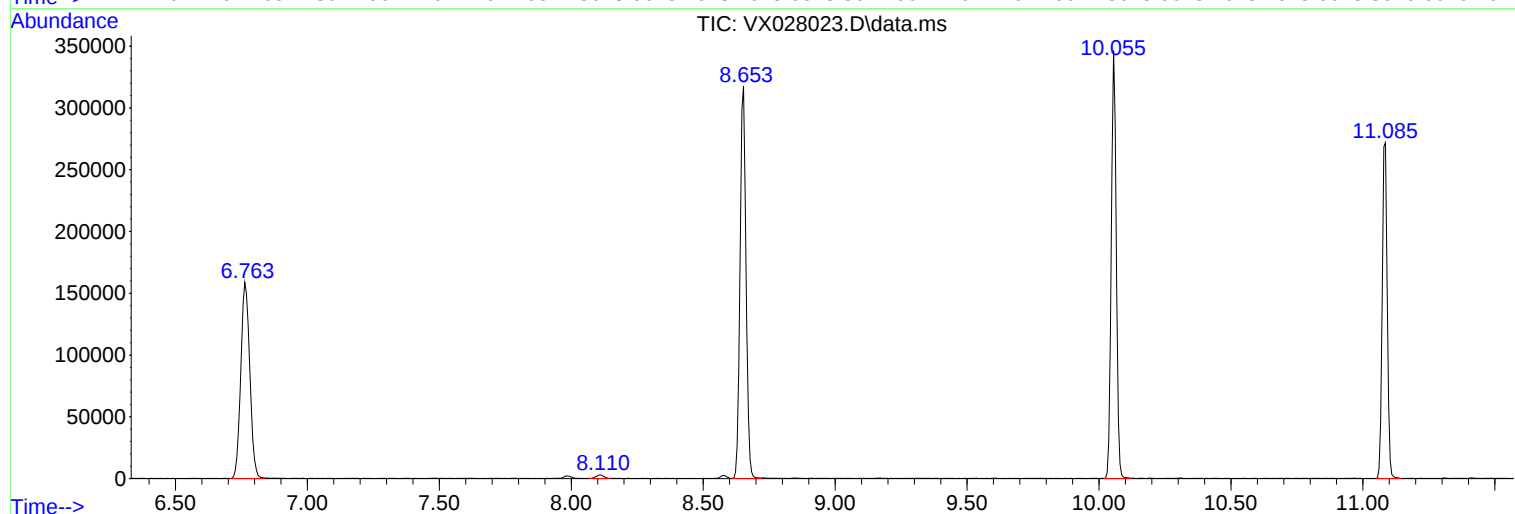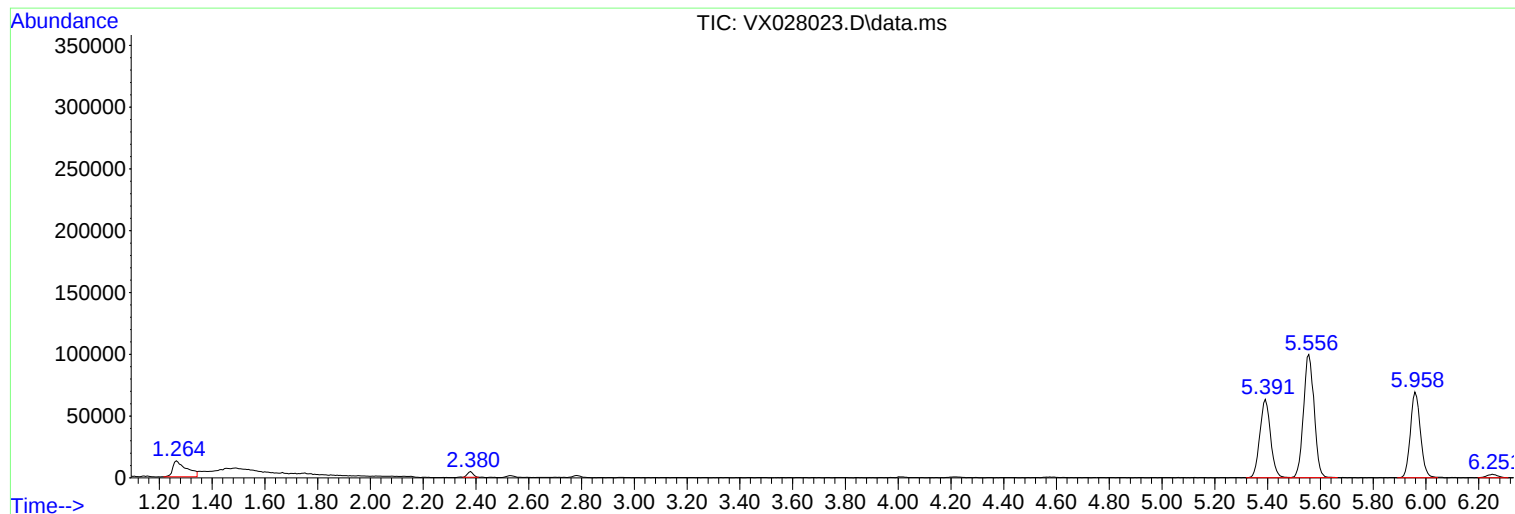

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
Data File : VX028023.D
Acq On : 08 Apr 2022 13:38
Operator : JC/MD
Sample : N2333-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Sulfur dioxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.264	8.46 ug/l	47355	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfur dioxide	64	O2S	007446-09-5	90
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	74
3			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	64
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	7
5			Ethyl Chloride	64	C2H5Cl	000075-00-3	3

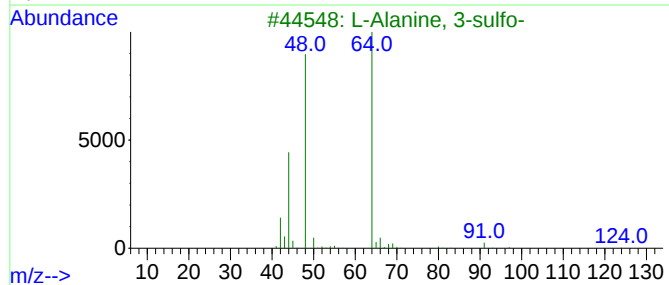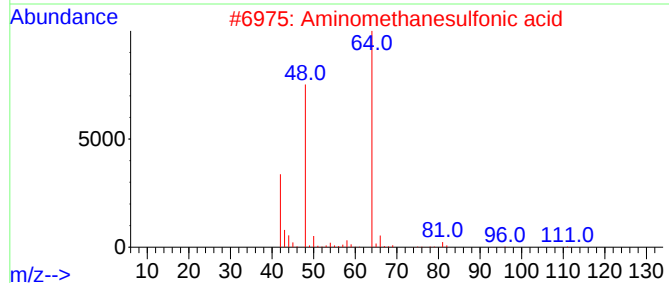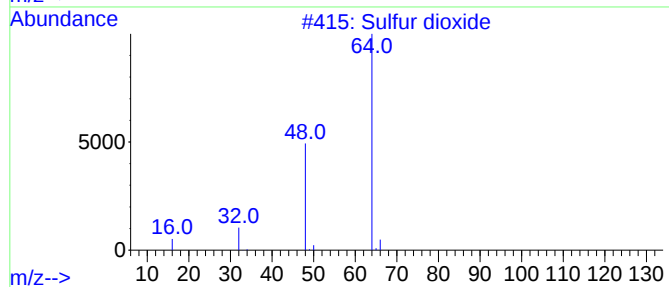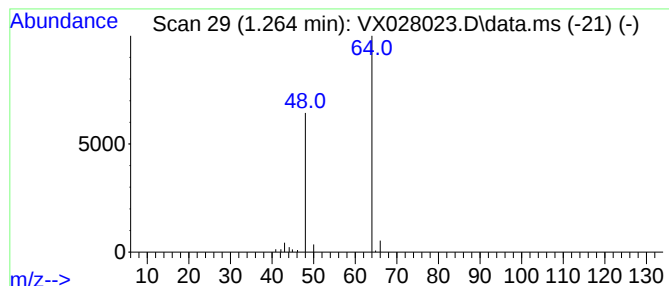

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040822\
Data File : VX028023.D
Acq On : 08 Apr 2022 13:38
Operator : JC/MD
Sample : N2333-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.264	8.5	ug/l	47355	1	5.550	279783	50.0