

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040824\
 Data File : VX040930.D
 Acq On : 08 Apr 2024 15:22
 Operator : JC/MD
 Sample : P2026-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 50306


Quant Time: Apr 09 02:49:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 02 05:40:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	36986	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	68678	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	68190	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	35861	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	33571	50.587	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 101.180%			
35) Dibromofluoromethane	5.385	113	23588	48.491	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 96.980%			
50) Toluene-d8	8.647	98	86199	49.039	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 98.080%			
62) 4-Bromofluorobenzene	11.079	95	35509	50.586	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 101.180%			
Target Compounds						Qvalue
3) Chloromethane	1.374	50	286	0.660	ug/l #	43
6) Chloroethane	1.672	64	64	0.222	ug/l #	43
13) Acrolein	2.215	56	165	2.495	ug/l #	1
14) Allyl chloride	2.751	41	229	0.309	ug/l #	1
16) Acetone	2.379	43	1746	6.776	ug/l	95
19) Methyl tert-butyl Ether	3.117	73	3333	2.288	ug/l	94
20) Methylene Chloride	2.788	84	125	0.262	ug/l #	53
22) Diisopropyl ether	3.763	45	1382	0.958	ug/l #	60
23) Vinyl Acetate	3.745	43	749	0.542	ug/l #	73
25) 2-Butanone	4.714	43	39597	103.445	ug/l #	51
31) Cyclohexane	5.476	56	412	0.585	ug/l #	85
36) 1,1-Dichloropropene	5.556	75	3719	5.381	ug/l #	49
37) Ethyl Acetate	4.714	43	39715	46.793	ug/l	98
38) Carbon Tetrachloride	5.562	117	4348	5.682	ug/l #	11
40) Benzene	6.037	78	74114	38.634	ug/l	96
41) Methacrylonitrile	4.708	41	349	0.801	ug/l #	25
42) 1,2-Dichloroethane	6.025	62	831	0.997	ug/l #	77
51) 4-Methyl-2-Pentanone	8.647	43	489	0.562	ug/l #	1
52) Toluene	8.720	92	76665	63.335	ug/l	95
53) t-1,3-Dichloropropene	8.720	75	1071	2.087	ug/l #	1
67) Ethyl Benzene	10.195	91	9818	3.692	ug/l	100
68) m/p-Xylenes	10.299	106	12065	12.468	ug/l	92
69) o-Xylene	10.640	106	5539	6.076	ug/l	94
76) 1,2,3-Trichloropropane	11.079	75	21755	28.449	ug/l #	38
78) n-propylbenzene	11.305	91	984	0.314	ug/l	88
79) 2-Chlorotoluene	11.384	91	589	0.315	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	1346	0.629	ug/l	86
81) trans-1,4-Dichloro-2-b...	11.079	75	21755	76.756	ug/l #	5
83) tert-Butylbenzene	11.756	119	580	0.273	ug/l #	38
84) 1,2,4-Trimethylbenzene	11.750	105	5140	2.385	ug/l	99
85) sec-Butylbenzene	11.750	105	5140	1.907	ug/l #	57
90) Hexachloroethane	12.695	117	210	0.533	ug/l #	17
95) Naphthalene	13.780	128	1245	0.479	ug/l	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed





Instrument :
MSVOA_X
ClientSampleId :
50306



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion:168 Resp: 36986
Ion Ratio Lower Upper
168 100
99 66.9 56.6 85.0

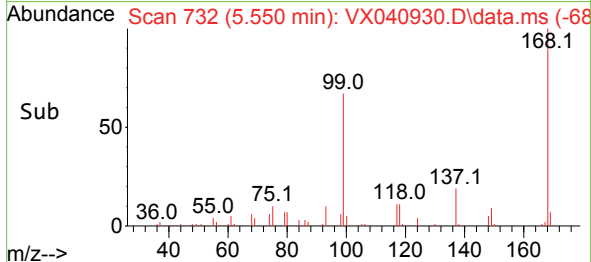

#3
Chloromethane
Concen: 0.660 ug/l
RT: 1.374 min Scan# 47
Delta R.T. 0.073 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 50 Resp: 286
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#


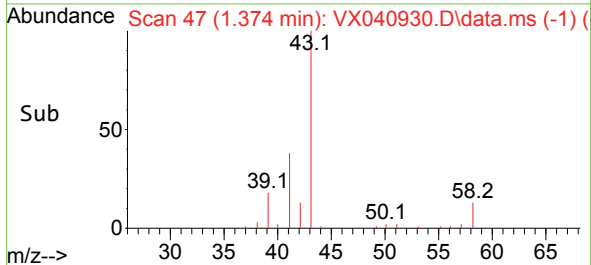




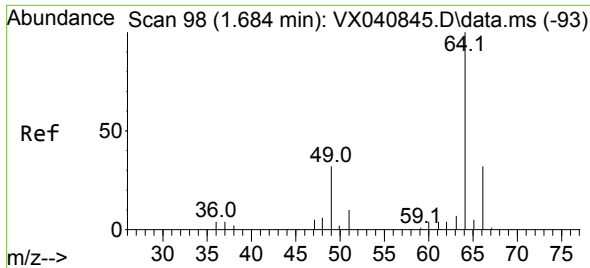

#6
Chloroethane
Concen: 0.222 ug/l
RT: 1.672 min Scan# 91
Delta R.T. -0.012 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion: 64 Resp: 64
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

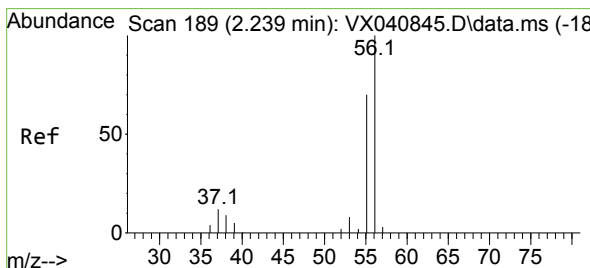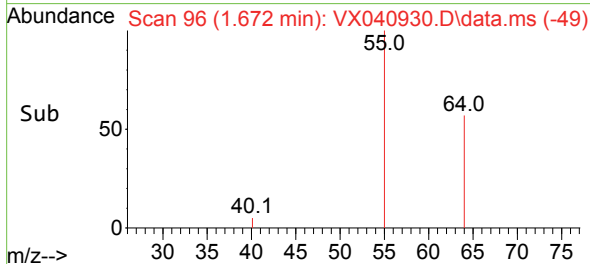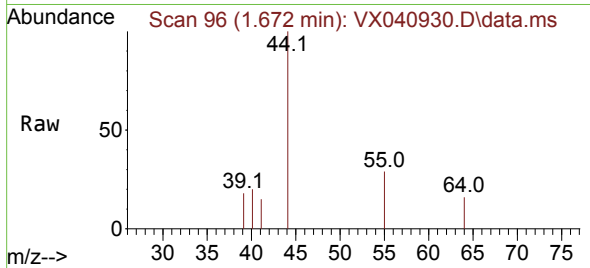

#13
Acrolein
Concen: 2.495 ug/l
RT: 2.215 min Scan# 185
Delta R.T. -0.024 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 56 Resp: 165
Ion Ratio Lower Upper
56 100
55 2853.3 57.1 85.7#


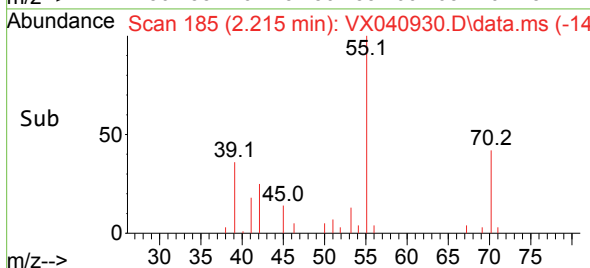

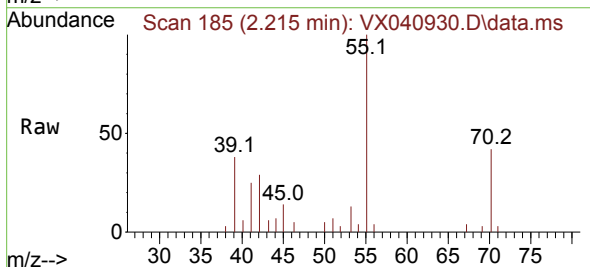




#14
 Allyl chloride
 Concen: 0.309 ug/l
 RT: 2.751 min Scan# 21
 Delta R.T. 0.085 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22




Instrument :
 MSVOA_X
 ClientSampleId :
 50306


Tgt Ion: 41 Resp: 229
 Ion Ratio Lower Upper
 41 100
 39 274.2 55.8 83.6#
 76 0.0 24.3 36.5#

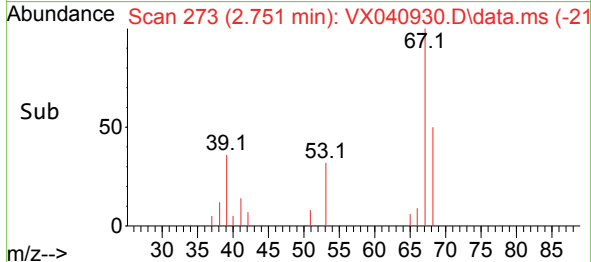

#16
 Acetone
 Concen: 6.776 ug/l
 RT: 2.379 min Scan# 212
 Delta R.T. -0.000 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22

Tgt Ion: 43 Resp: 1746
 Ion Ratio Lower Upper
 43 100
 58 25.0 21.9 32.9




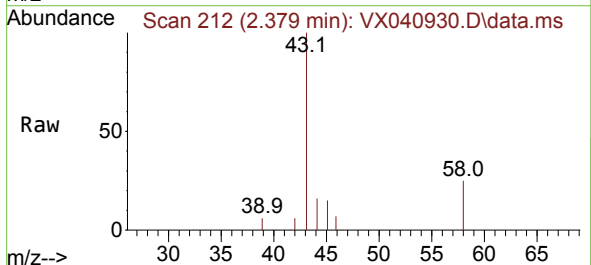




#19
Methyl tert-butyl Ether
Concen: 2.288 ug/l
RT: 3.117 min Scan# 311
Delta R.T. 0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion: 73 Resp: 3333
Ion Ratio Lower Upper
73 100
57 18.6 17.3 25.9

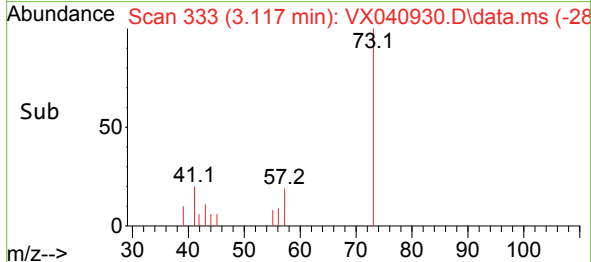

#20
Methylene Chloride
Concen: 0.262 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 84 Resp: 125
Ion Ratio Lower Upper
84 100
49 158.7 103.6 155.4#
51 0.0 33.8 50.6#
86 0.0 49.4 74.0#




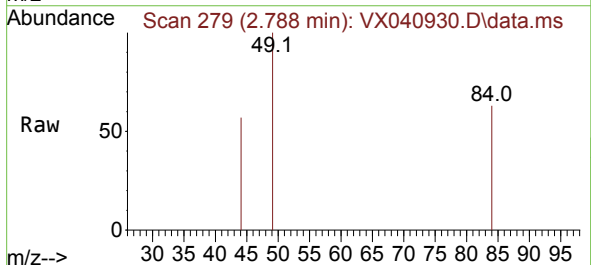




#22
Diisopropyl ether
Concen: 0.958 ug/l
RT: 3.763 min Scan# 41
Delta R.T. 0.006 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion:	45	Resp:	1382
Ion	Ratio	Lower	Upper
45	100		
43	35.6	69.7	104.5#
87	25.1	20.8	31.2
59	8.2	9.0	13.4#

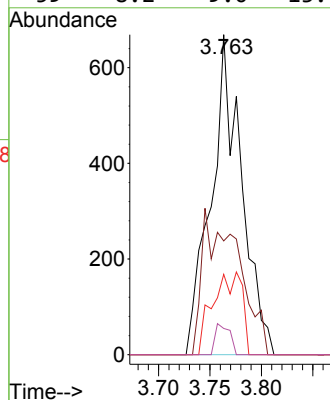

#23
Vinyl Acetate
Concen: 0.542 ug/l
RT: 3.745 min Scan# 436
Delta R.T. 0.024 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion:	43	Resp:	749
Ion	Ratio	Lower	Upper
43	100		
86	0.0	7.8	11.8#



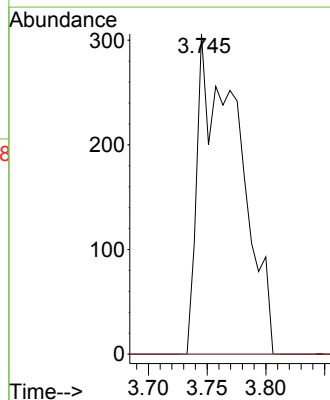





#25
2-Butanone
Concen: 103.445 ug/l
RT: 4.714 min Scan# 51
Delta R.T. 0.165 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion: 43 Resp: 39597
Ion Ratio Lower Upper
43 100
72 0.0 19.4 29.2#

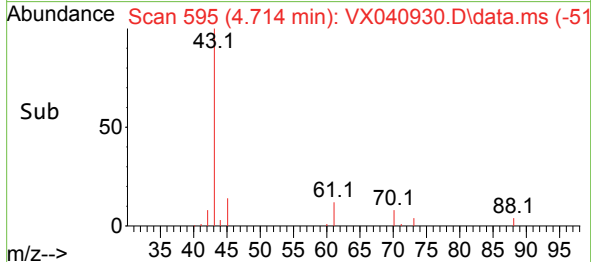

#31
Cyclohexane
Concen: 0.585 ug/l
RT: 5.476 min Scan# 720
Delta R.T. 0.006 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 56 Resp: 412
Ion Ratio Lower Upper
56 100
69 0.0 23.4 35.2#
84 81.7 65.9 98.9

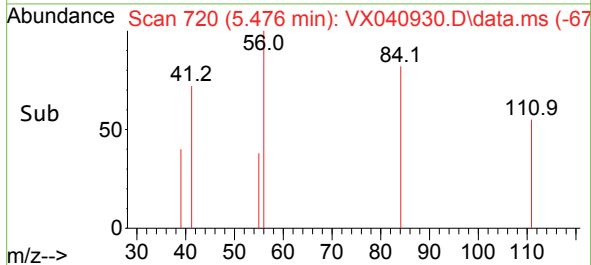



#33

1,2-Dichloroethane-d4

Concen: 50.587 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22

Instrument :

MSVOA_X

ClientSampleId :





50306

Tgt Ion: 65 Resp: 33571

Ion Ratio Lower Upper

65 100

67 49.5 0.0 100.2

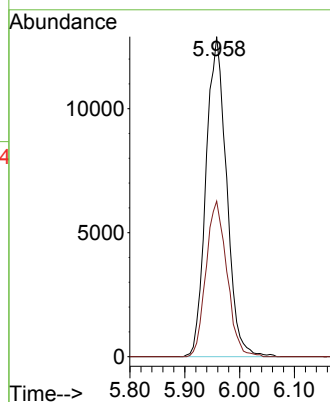

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22




Tgt Ion:114 Resp: 68678


Ion Ratio Lower Upper

114 100

63 24.0 0.0 45.0


88 17.4 0.0 36.6

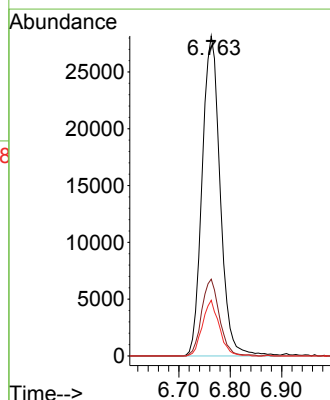



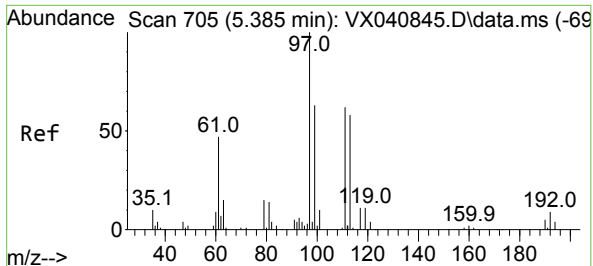


#35
 Dibromofluoromethane
 Concen: 48.491 ug/l
 RT: 5.385 min Scan# 705
 Delta R.T. -0.000 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22

Instrument :
 MSVOA_X
 ClientSampleId :
 50306



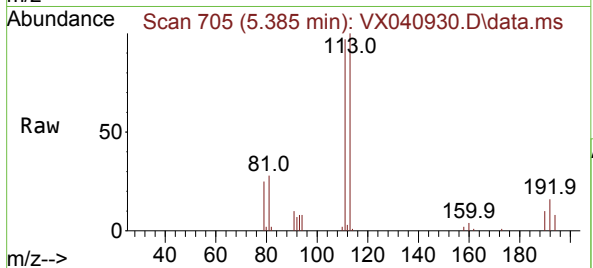



Tgt Ion:	113	Resp:	23588
Ion	Ratio	Lower	Upper
113	100		
111	102.8	82.9	124.3
192	17.2	13.3	19.9

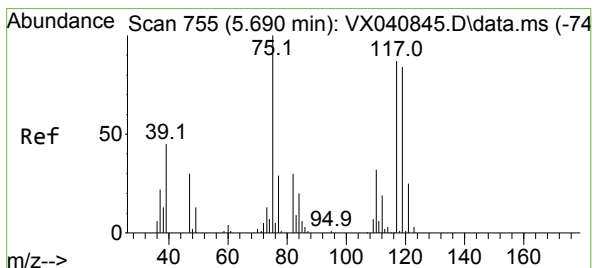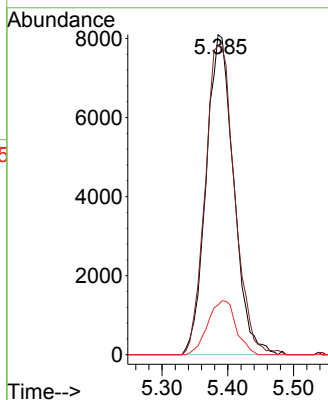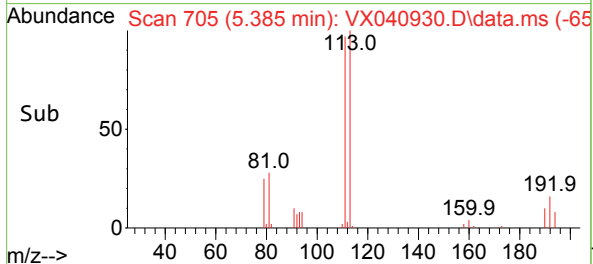

#36
 1,1-Dichloropropene
 Concen: 5.381 ug/l
 RT: 5.556 min Scan# 733
 Delta R.T. -0.134 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22

Tgt Ion:	75	Resp:	3719
Ion	Ratio	Lower	Upper
75	100		
110	7.3	17.0	50.9#
77	0.0	24.7	37.1#

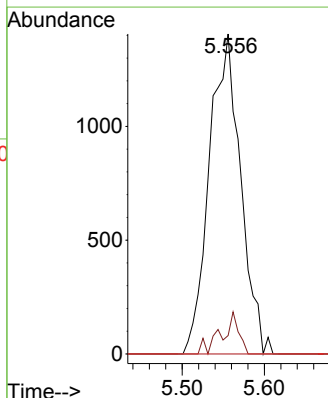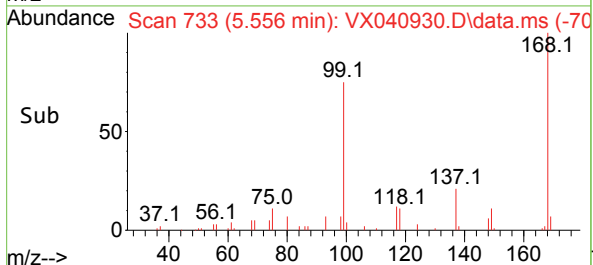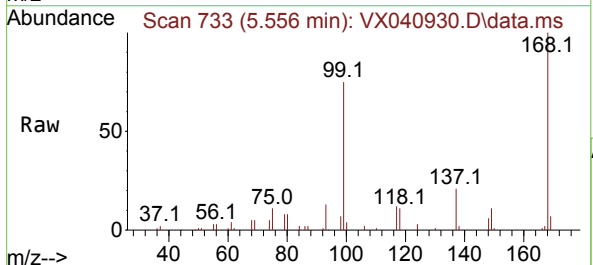



#37

Ethyl Acetate

Concen: 46.793 ug/l

RT: 4.714 min Scan# 594

Delta R.T. 0.006 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22

Instrument :

MSVOA_X

ClientSampleId :

50306





Tgt Ion: 43 Resp: 39715

Ion Ratio Lower Upper

43 100

61 12.4 10.6 16.0

70 9.5 8.3 12.5



#38

Carbon Tetrachloride

Concen: 5.682 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.116 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22




Tgt Ion: 117 Resp: 4348


Ion Ratio Lower Upper

117 100

119 0.0 78.2 117.2#

121 0.0 24.4 36.6#




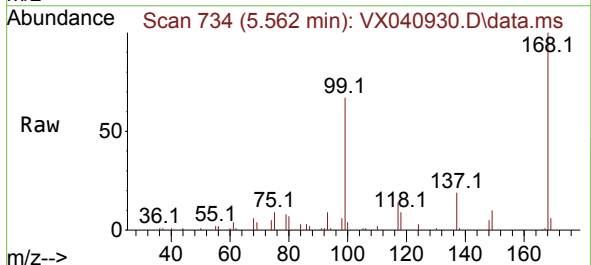




#40
Benzene
Concen: 38.634 ug/l
RT: 6.037 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion: 78 Resp: 74114
Ion Ratio Lower Upper
78 100
77 22.2 19.3 28.9



#41
Methacrylonitrile
Concen: 0.801 ug/l
RT: 4.708 min Scan# 594
Delta R.T. -0.213 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 41 Resp: 349
Ion Ratio Lower Upper
41 100
39 0.0 45.2 67.8#
67 0.0 52.6 78.8#
52 0.0 22.7 34.1#





#42

1,2-Dichloroethane

Concen: 0.997 ug/l

RT: 6.025 min Scan# 81

Delta R.T. -0.061 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22

Instrument :

MSVOA_X

ClientSampleId :





50306

Tgt Ion: 62 Resp: 831

Ion Ratio Lower Upper

62 100

98 0.0 0.0 16.0

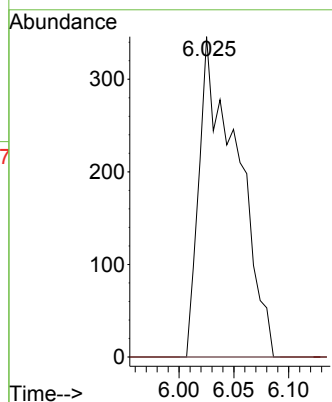

#50

Toluene-d8

Concen: 49.039 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX040930.D




Acq: 08 Apr 2024 15:22


Tgt Ion: 98 Resp: 86199

Ion Ratio Lower Upper

98 100

100 64.1 53.1 79.7



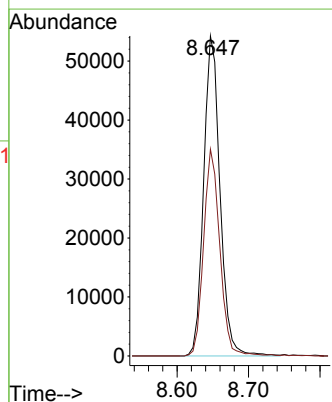





#51
4-Methyl-2-Pentanone
Concen: 0.562 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.073 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion: 43 Resp: 489
Ion Ratio Lower Upper
43 100
58 161.1 30.4 45.6#

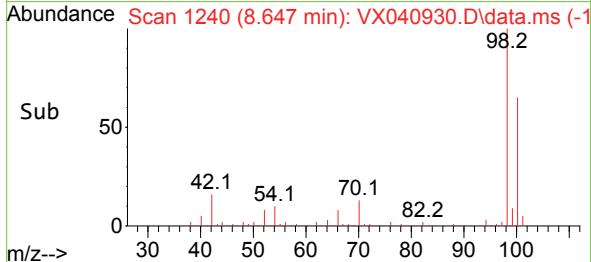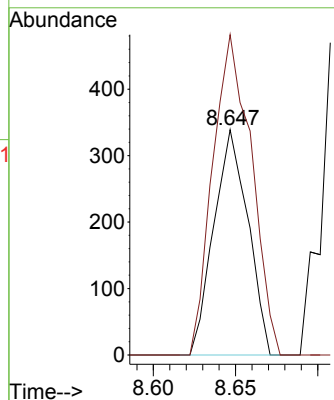

#52
Toluene
Concen: 63.335 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 92 Resp: 76665
Ion Ratio Lower Upper
92 100
91 174.7 134.2 201.2


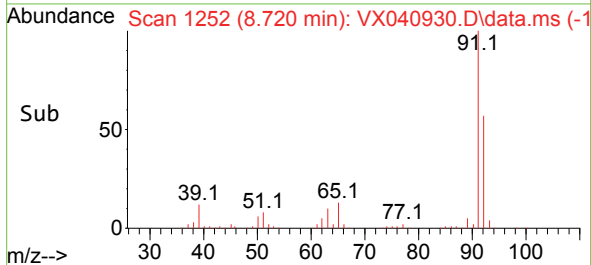
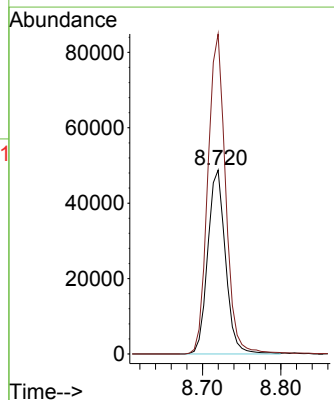





#53
t-1,3-Dichloropropene
Concen: 2.087 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.256 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion: 75 Resp: 1071
Ion Ratio Lower Upper
75 100
77 205.5 25.7 38.5#

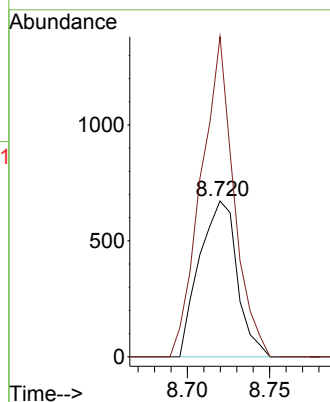

#62
4-Bromofluorobenzene
Concen: 50.586 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 95 Resp: 35509
Ion Ratio Lower Upper
95 100
174 74.2 0.0 135.6
176 70.5 0.0 131.0

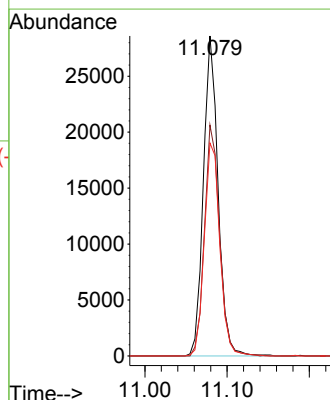



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22

Instrument :

MSVOA_X

ClientSampleId :

50306





Tgt Ion:117 Resp: 68190

Ion Ratio Lower Upper

117 100

82 59.8 46.2 69.4

119 32.3 25.5 38.3

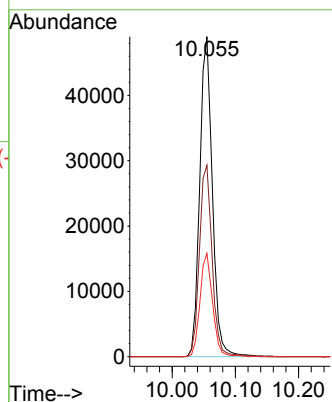

#67

Ethyl Benzene

Concen: 3.692 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX040930.D




Acq: 08 Apr 2024 15:22


Tgt Ion: 91 Resp: 9818

Ion Ratio Lower Upper

91 100

106 31.1 24.9 37.3









#68
m/p-Xylenes
Concen: 12.468 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion:106 Resp: 12065
Ion Ratio Lower Upper
106 100
91 219.7 165.5 248.3

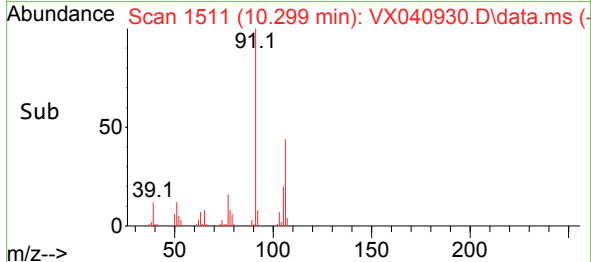

#69
o-Xylene
Concen: 6.076 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion:106 Resp: 5539
Ion Ratio Lower Upper
106 100
91 227.7 108.9 326.8


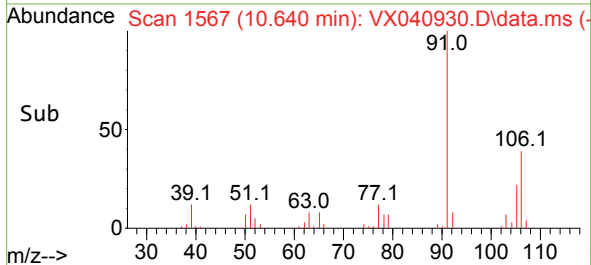






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22




Instrument :
MSVOA_X
ClientSampleId :
50306


Tgt Ion:152 Resp: 35861
Ion Ratio Lower Upper
152 100
115 62.0 43.3 129.9
150 155.5 0.0 345.0

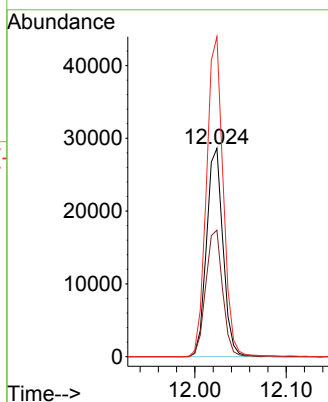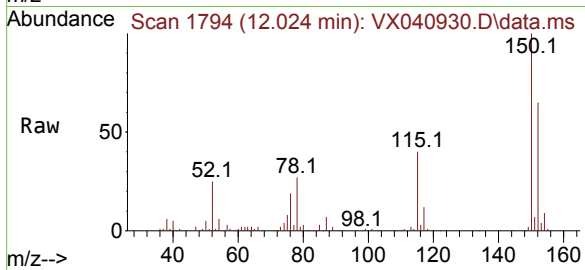

#76
1,2,3-Trichloropropane
Concen: 28.449 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Tgt Ion: 75 Resp: 21755
Ion Ratio Lower Upper
75 100
77 0.9 19.1 57.5#

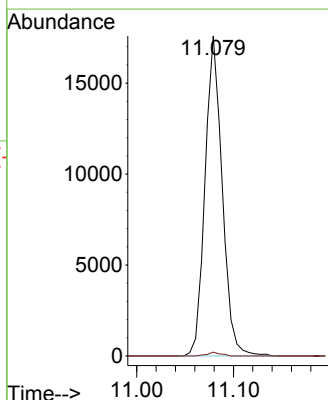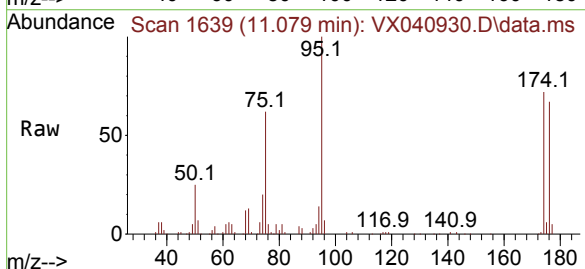



#78

n-propylbenzene

Concen: 0.314 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.000 min

Lab File: VX040930.D

Acq: 08 Apr 2024 15:22

Instrument :

MSVOA_X

ClientSampleId :





50306

Tgt Ion: 91 Resp: 984

Ion Ratio Lower Upper

91 100

120 17.2 11.5 34.4



#79

2-Chlorotoluene

Concen: 0.315 ug/l

RT: 11.384 min Scan# 1689

Delta R.T. 0.018 min

Lab File: VX040930.D




Acq: 08 Apr 2024 15:22


Tgt Ion: 91 Resp: 589

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#


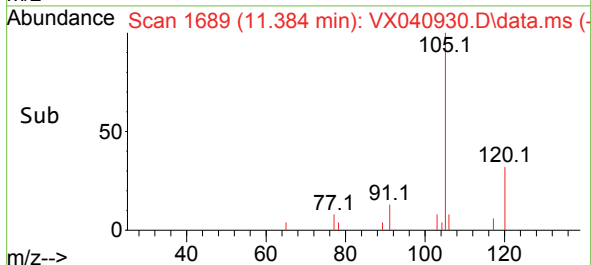






#80
 1,3,5-Trimethylbenzene
 Concen: 0.629 ug/l
 RT: 11.451 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22




Instrument :
 MSVOA_X
 ClientSampleId :
 50306


Tgt Ion:105 Resp: 1346
 Ion Ratio Lower Upper
 105 100
 120 39.0 24.1 72.3

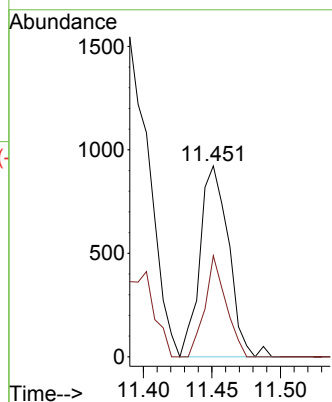

#81
 trans-1,4-Dichloro-2-butene
 Concen: 76.756 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. 0.061 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22

Tgt Ion: 75 Resp: 21755
 Ion Ratio Lower Upper
 75 100
 53 0.0 90.5 135.7#
 89 0.0 36.9 55.3#


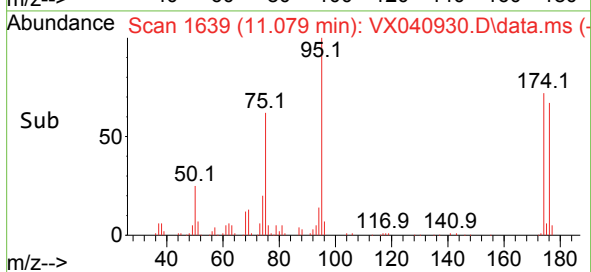
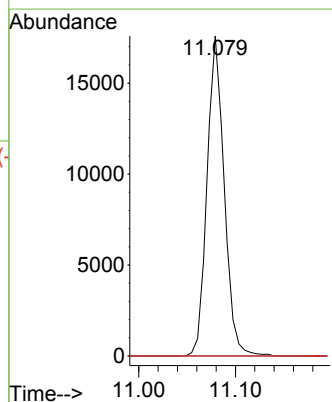
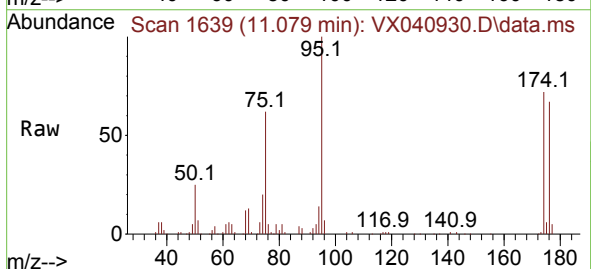




#83
 tert-Butylbenzene
 Concen: 0.273 ug/l
 RT: 11.756 min Scan# 11
 Delta R.T. 0.043 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22




Instrument :
 MSVOA_X
 ClientSampleId :
 50306


Tgt Ion:119 Resp: 580
 Ion Ratio Lower Upper
 119 100
 91 114.0 31.2 93.6#
 134 0.0 11.7 35.0#



#84
 1,2,4-Trimethylbenzene
 Concen: 2.385 ug/l
 RT: 11.750 min Scan# 1749
 Delta R.T. -0.000 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22

Tgt Ion:105 Resp: 5140
 Ion Ratio Lower Upper
 105 100
 120 43.1 21.2 63.6









#85
 sec-Butylbenzene
 Concen: 1.907 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22




Instrument :
 MSVOA_X
 ClientSampleId :
 50306


Tgt Ion:105 Resp: 5140
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.8 29.4#

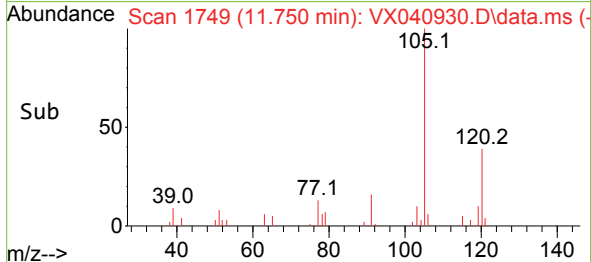

#90
 Hexachloroethane
 Concen: 0.533 ug/l
 RT: 12.695 min Scan# 1904
 Delta R.T. 0.159 min
 Lab File: VX040930.D
 Acq: 08 Apr 2024 15:22


Tgt Ion:117 Resp: 210
 Ion Ratio Lower Upper
 117 100
 201 0.0 32.9 98.6#

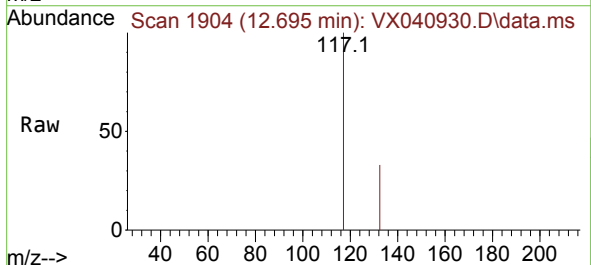



#95
Naphthalene
Concen: 0.479 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX040930.D
Acq: 08 Apr 2024 15:22

Instrument :
MSVOA_X
ClientSampleId :
50306



Tgt Ion:	128	Resp:	1245
Ion	Ratio	Lower	Upper
128	100		
127	10.8	10.3	15.5
129	13.0	8.8	13.2

