

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040824\
 Data File : VX040936.D
 Acq On : 08 Apr 2024 17:40
 Operator : JC/MD
 Sample : P2025-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TOTE-COMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M

Title : SW846 8260

Signal : TIC: VX040936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.355	42	44	50	rVB3	2854	3280	1.31%	0.234%
2	2.380	207	212	218	rBV	4444	7035	2.81%	0.502%
3	5.391	695	706	720	rBV	28258	82912	33.14%	5.914%
4	5.556	721	733	751	rBV	42309	121849	48.71%	8.692%
5	5.952	790	798	814	rBV	32244	88684	35.45%	6.326%
6	6.763	922	931	944	rBV	71897	172634	69.01%	12.314%
7	8.580	1224	1229	1234	rBV2	2929	4539	1.81%	0.324%
8	8.647	1234	1240	1258	rBV	148825	242646	96.99%	17.308%
9	10.055	1465	1471	1487	rVB	169549	231108	92.38%	16.485%
10	11.079	1634	1639	1653	rBV	149616	185002	73.95%	13.196%
11	12.018	1788	1793	1803	rBV	196206	250170	100.00%	17.845%
12	14.780	2241	2246	2252	rVB	2961	3684	1.47%	0.263%
13	16.322	2494	2499	2506	rVB2	4938	8387	3.35%	0.598%




Sum of corrected areas: 1401930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040824\
Data File : VX040936.D
Acq On : 08 Apr 2024 17:40
Operator : JC/MD
Sample : P2025-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

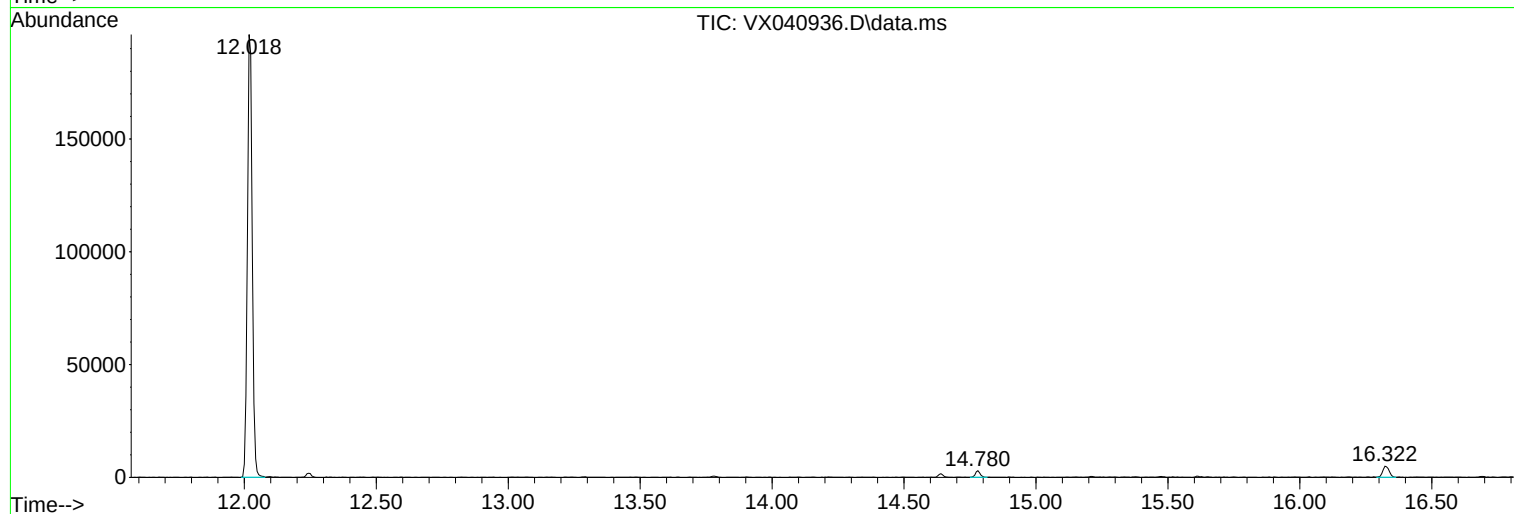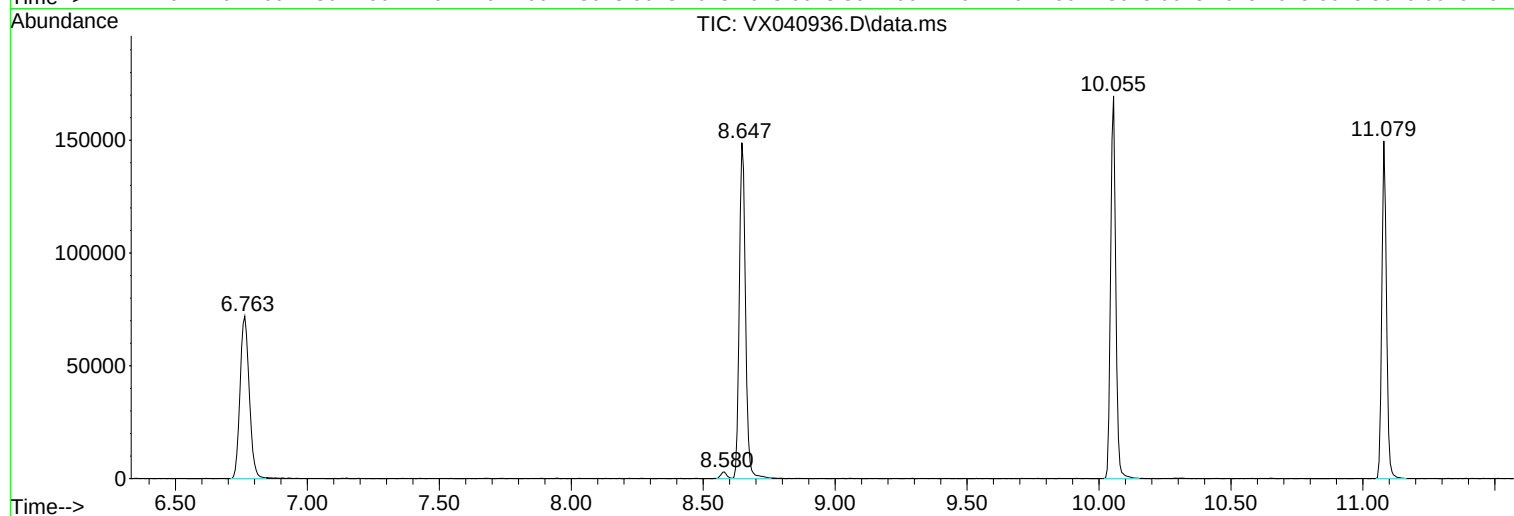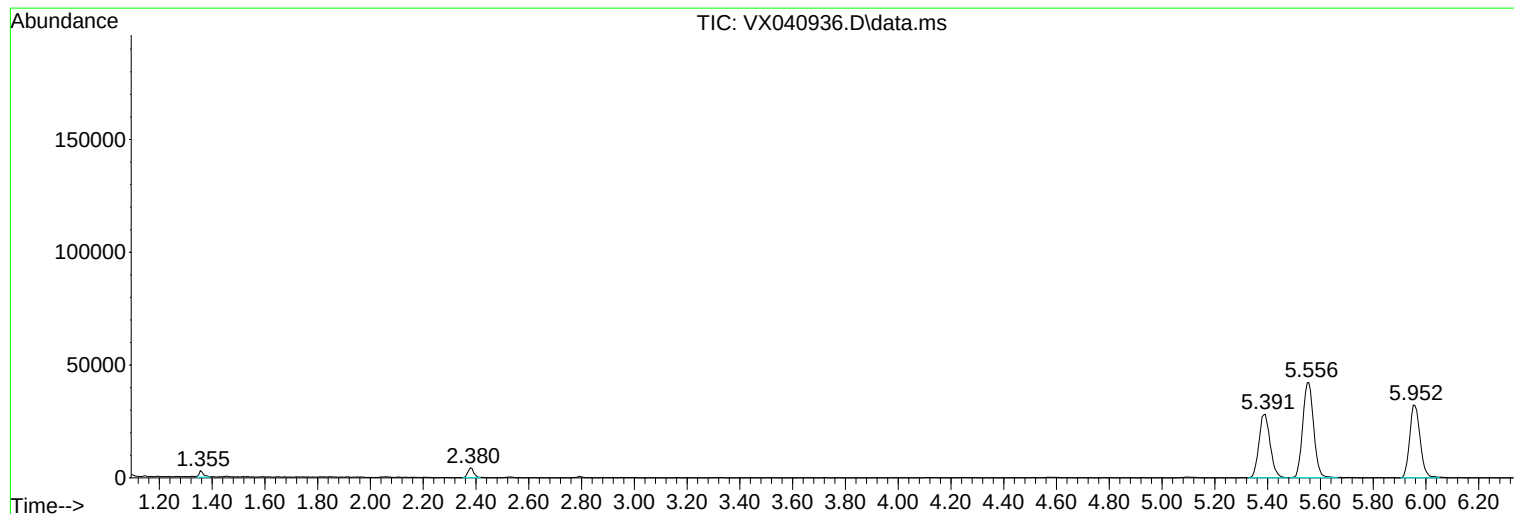

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040824\
Data File : VX040936.D
Acq On : 08 Apr 2024 17:40
Operator : JC/MD
Sample : P2025-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040824\
Data File : VX040936.D
Acq On : 08 Apr 2024 17:40
Operator : JC/MD
Sample : P2025-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TOTE-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc