

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\X040825\
 Data File : VX045645.D
 Acq On : 08 Apr 2025 12:28
 Operator : JC/MD
 Sample : Q1737-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RT3069

Quant Time: Apr 09 01:36:31 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	60517	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	117735	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	112767	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47540	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	61747	55.794	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 111.580%			
35) Dibromofluoromethane	5.379	113	43858	52.504	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 105.000%			
50) Toluene-d8	8.647	98	152623	52.346	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 104.700%			
62) 4-Bromofluorobenzene	11.079	95	56901	53.578	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 107.160%			
Target Compounds						Qvalue
6) Chloroethane	1.630	64	91	0.202	ug/l #	42
11) Tert butyl alcohol	2.983	59	973	6.542	ug/l #	79
13) Acrolein	2.227	56	196	0.957	ug/l	93
14) Allyl chloride	2.654	41	450	0.326	ug/l #	63
16) Acetone	2.386	43	104893	230.817	ug/l	96
17) Carbon Disulfide	2.495	76	454	0.253	ug/l #	76
18) Methyl Acetate	2.709	43	2032	1.942	ug/l	96
20) Methylene Chloride	2.782	84	8550	10.050	ug/l	93
25) 2-Butanone	4.568	43	21068	31.671	ug/l	99
29) Tetrahydrofuran	5.038	42	270	0.626	ug/l #	41
31) Cyclohexane	5.544	56	1709	1.259	ug/l #	17
36) 1,1-Dichloropropene	5.550	75	6067	5.379	ug/l #	50
37) Ethyl Acetate	4.568	43	21068	14.823	ug/l #	71
38) Carbon Tetrachloride	5.544	117	7185	5.894	ug/l #	16
40) Benzene	6.031	78	38671	11.227	ug/l	97
42) 1,2-Dichloroethane	6.050	62	340	0.239	ug/l #	78
43) Isopropyl Acetate	6.355	43	2870	1.332	ug/l #	77
48) Methyl methacrylate	7.616	41	735	0.661	ug/l #	24
51) 4-Methyl-2-Pentanone	8.543	43	21395	14.982	ug/l #	39
52) Toluene	8.720	92	2758	1.323	ug/l	99
54) cis-1,3-Dichloropropene	8.549	75	5246	4.237	ug/l #	75
59) 2-Hexanone	9.439	43	2304	2.179	ug/l	80
67) Ethyl Benzene	10.195	91	1549	0.359	ug/l	92
68) m/p-Xylenes	10.299	106	682	0.434	ug/l	84
73) Isopropylbenzene	10.957	105	3627	0.952	ug/l	98
74) N-amyl acetate	10.866	43	451	0.248	ug/l #	11
76) 1,2,3-Trichloropropane	11.079	75	32419	27.957	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	32419	94.882	ug/l #	1
90) Hexachloroethane	12.603	117	154	0.284	ug/l #	19
95) Naphthalene	13.780	128	1404	0.426	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040825\
Data File : VX045645.D
Acq On : 08 Apr 2025 12:28
Operator : JC/MD
Sample : Q1737-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RT3069

Quant Time: Apr 09 01:36:31 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




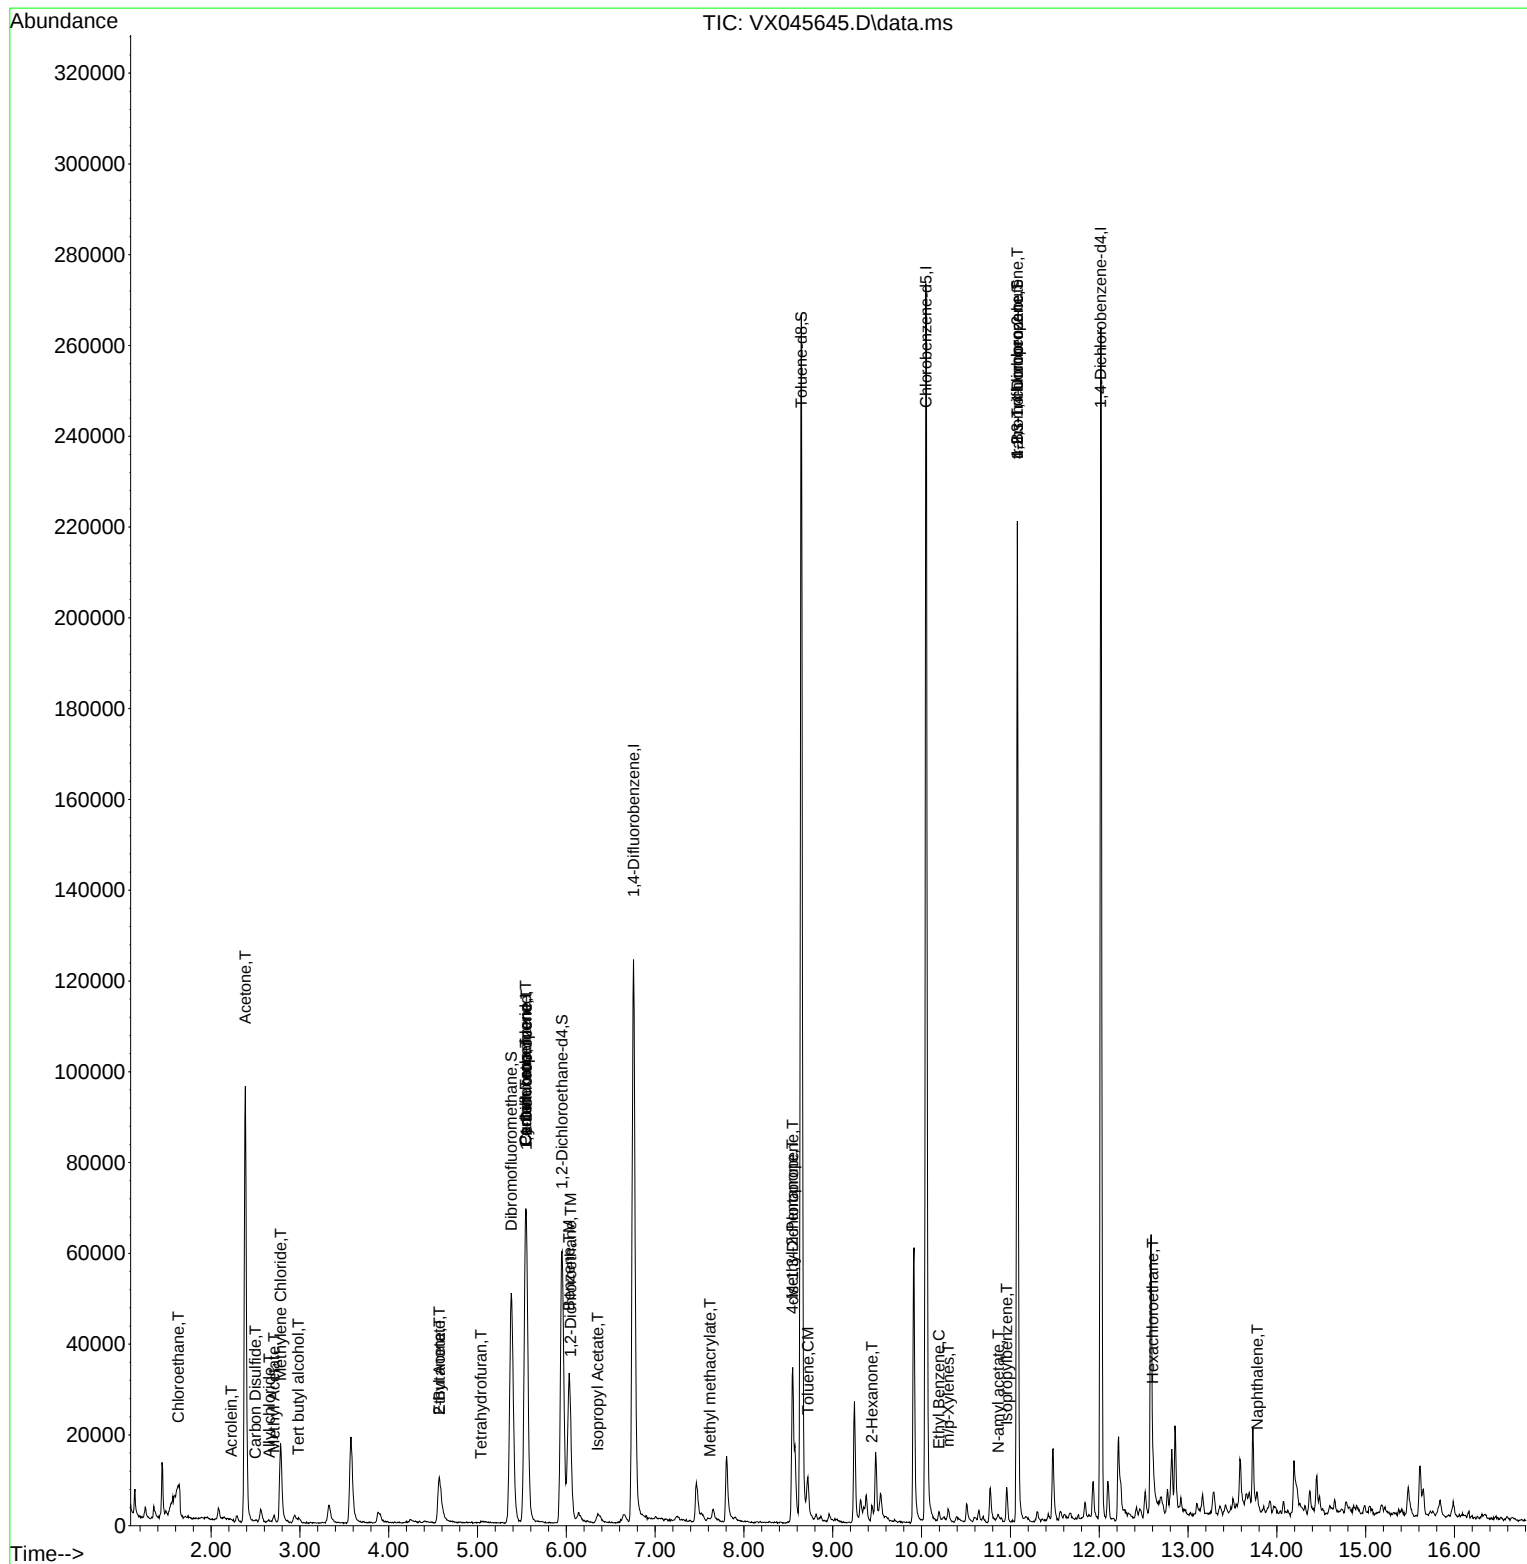




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion:168 Resp: 60517
Ion Ratio Lower Upper
168 100
99 71.1 52.3 78.5

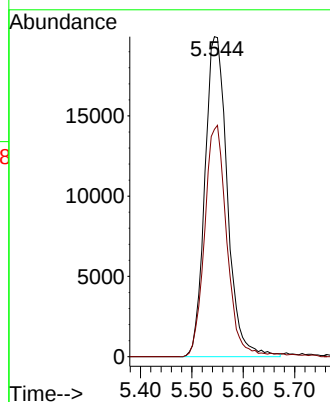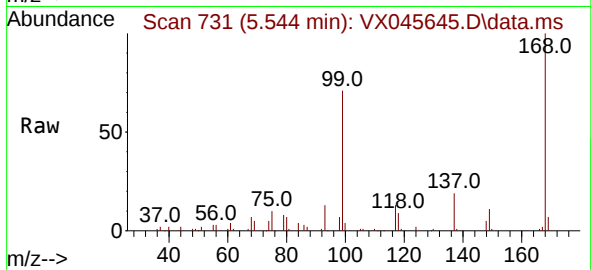

#6
Chloroethane
Concen: 0.202 ug/l
RT: 1.630 min Scan# 89
Delta R.T. -0.037 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 64 Resp: 91
Ion Ratio Lower Upper
64 100
66 0.0 26.3 39.5

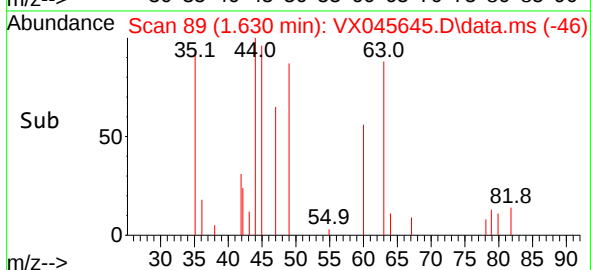



#11

Tert butyl alcohol

Concen: 6.542 ug/l

RT: 2.983 min Scan# 311

Delta R.T. 0.006 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28

Instrument :

MSVOA_X

ClientSampleId :





RT3069

Tgt Ion: 59 Resp: 973

Ion Ratio Lower Upper

59 100

57 2.7 8.6 12.8#

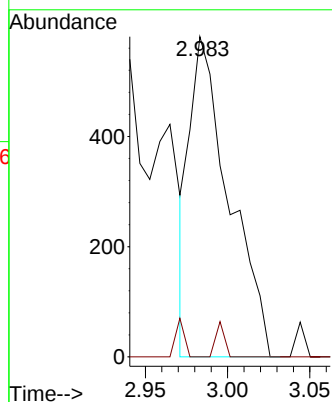

#13

Acrolein

Concen: 0.957 ug/l

RT: 2.227 min Scan# 187

Delta R.T. -0.012 min

Lab File: VX045645.D




Acq: 08 Apr 2025 12:28


Tgt Ion: 56 Resp: 196

Ion Ratio Lower Upper

56 100

55 76.0 56.2 84.2




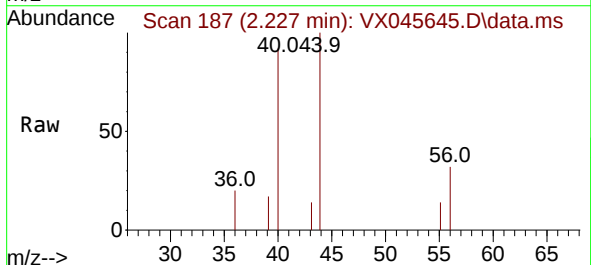




#14
 Allyl chloride
 Concen: 0.326 ug/l
 RT: 2.654 min Scan# 213
 Delta R.T. -0.006 min
 Lab File: VX045645.D
 Acq: 08 Apr 2025 12:28




Instrument :
 MSVOA_X
 ClientSampleId :
 RT3069


Tgt Ion: 41 Resp: 450
 Ion Ratio Lower Upper
 41 100
 39 50.7 60.2 90.2#
 76 0.0 24.6 36.8#

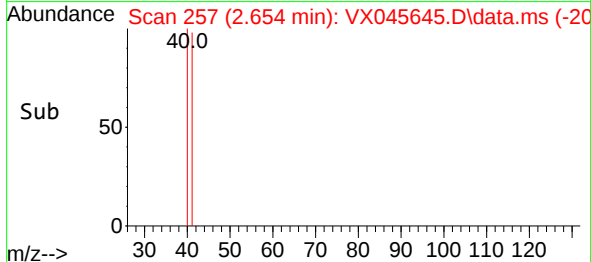

#16
 Acetone
 Concen: 230.817 ug/l
 RT: 2.386 min Scan# 213
 Delta R.T. 0.000 min
 Lab File: VX045645.D
 Acq: 08 Apr 2025 12:28

Tgt Ion: 43 Resp: 104893
 Ion Ratio Lower Upper
 43 100
 58 25.9 22.3 33.5

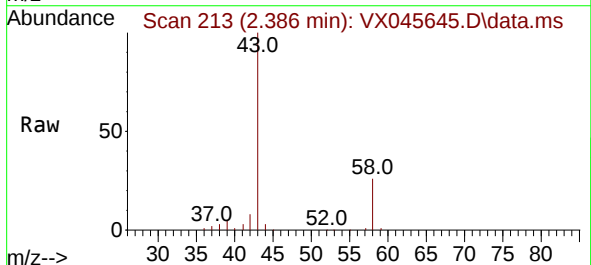



#17

Carbon Disulfide

Concen: 0.253 ug/l

RT: 2.495 min Scan# 21

Delta R.T. -0.012 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28

Instrument :

MSVOA_X

ClientSampleId :





RT3069

Tgt Ion: 76 Resp: 454

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.6#



#18

Methyl Acetate

Concen: 1.942 ug/l

RT: 2.709 min Scan# 266

Delta R.T. 0.006 min

Lab File: VX045645.D




Acq: 08 Apr 2025 12:28


Tgt Ion: 43 Resp: 2032

Ion Ratio Lower Upper

43 100

74 23.8 17.5 26.3


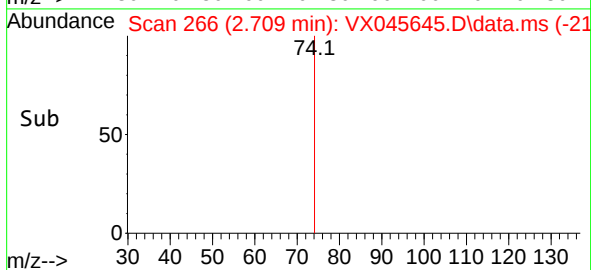






#20
Methylene Chloride
Concen: 10.050 ug/l
RT: 2.782 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion:	84	Resp:	8550
Ion	Ratio	Lower	Upper
84	100		
49	127.3	107.5	161.3
51	39.2	33.0	49.6
86	54.0	50.1	75.1



#25
2-Butanone
Concen: 31.671 ug/l
RT: 4.568 min Scan# 571
Delta R.T. 0.012 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion:	43	Resp:	21068
Ion	Ratio	Lower	Upper
43	100		
72	24.0	18.6	28.0

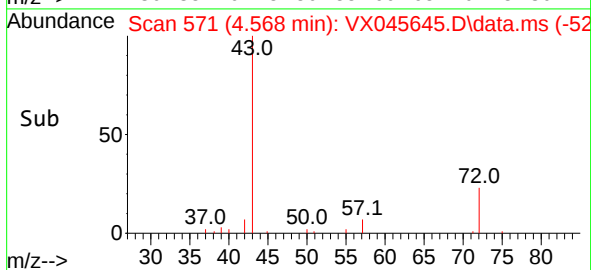

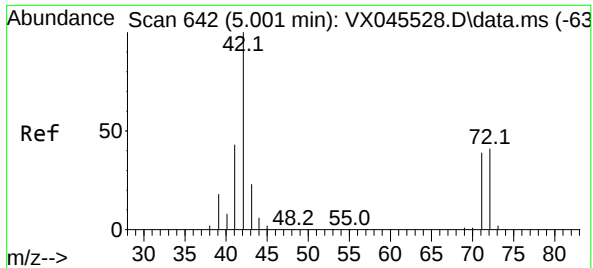

#29

Tetrahydrofuran

Concen: 0.626 ug/l

RT: 5.038 min Scan# 642

Delta R.T. 0.037 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28

Instrument :

MSVOA_X

ClientSampleId :

RT3069





Tgt Ion: 42 Resp: 270

Ion Ratio Lower Upper

42 100

72 7.0 33.4 50.0#

71 0.0 31.4 47.0#

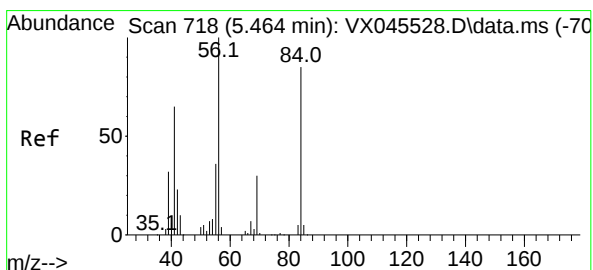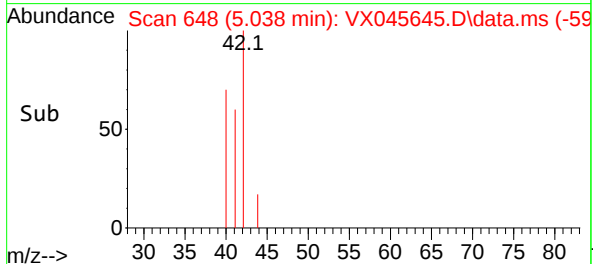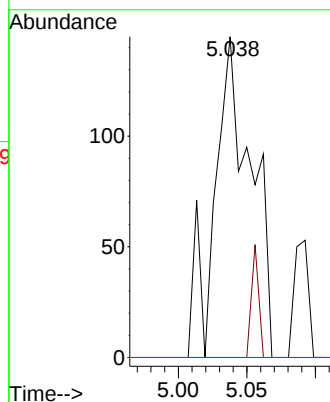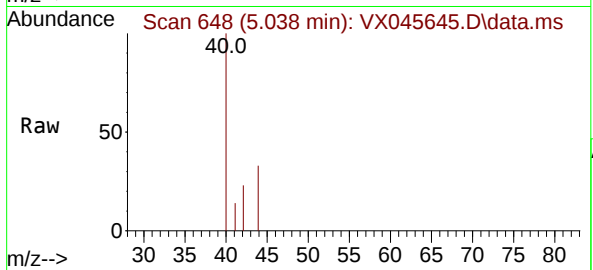

#31

Cyclohexane

Concen: 1.259 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.079 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28




Tgt Ion: 56 Resp: 1709


Ion Ratio Lower Upper

56 100

69 142.7 23.6 35.4#

84 120.1 67.7 101.5#

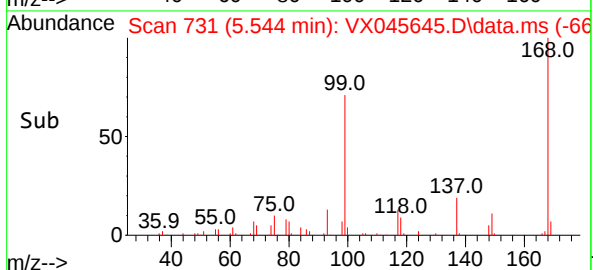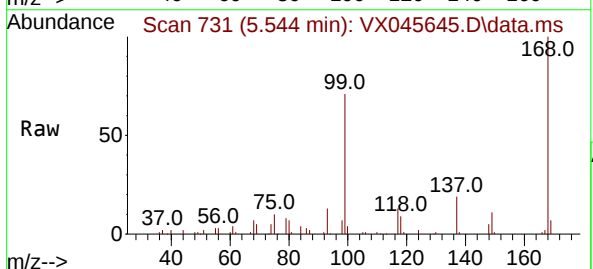



#33

1,2-Dichloroethane-d4

Concen: 55.794 ug/l

RT: 5.952 min Scan# 798

Delta R.T. 0.000 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28

Instrument :

MSVOA_X

ClientSampleId :





RT3069

Tgt Ion: 65 Resp: 61747

Ion Ratio Lower Upper

65 100

67 49.3 0.0 99.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. 0.000 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28




Tgt Ion: 114 Resp: 117735


Ion Ratio Lower Upper

114 100

63 24.2 0.0 46.8


88 17.7 0.0 35.4








#35
Dibromofluoromethane
Concen: 52.504 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Instrument :
MSVOA_X
ClientSampleId :
RT3069



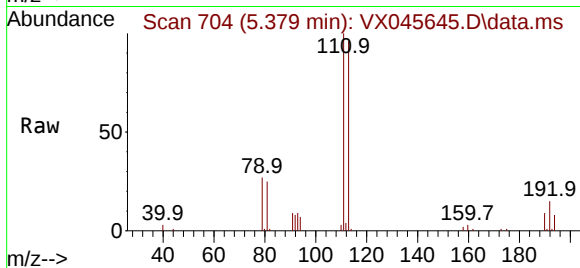



Tgt Ion:113 Resp: 43858
Ion Ratio Lower Upper
113 100
111 103.0 81.8 122.6
192 16.0 13.8 20.6



#36
1,1-Dichloropropene
Concen: 5.379 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 75 Resp: 6067
Ion Ratio Lower Upper
75 100
110 9.1 16.9 50.6#
77 0.0 25.0 37.4#

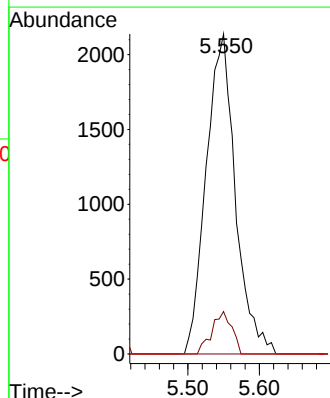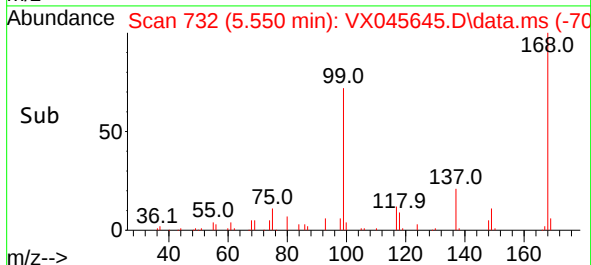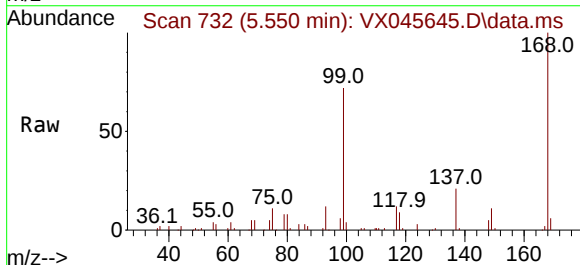



#37

Ethyl Acetate

Concen: 14.823 ug/l

RT: 4.568 min Scan# 51

Delta R.T. -0.146 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28

Instrument :

MSVOA_X

ClientSampleId :

RT3069





Tgt Ion: 43 Resp: 21068

Ion Ratio Lower Upper

43 100

61 0.0 9.9 14.9#

70 0.0 7.5 11.3#

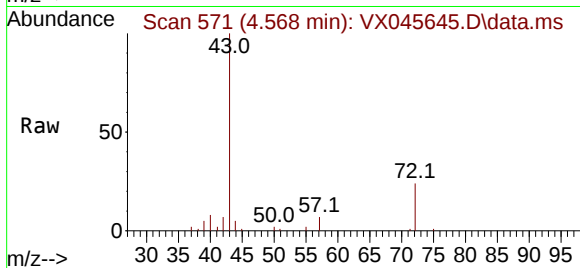

#38

Carbon Tetrachloride

Concen: 5.894 ug/l

RT: 5.544 min Scan# 731

Delta R.T. -0.128 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28




Tgt Ion: 117 Resp: 7185


Ion Ratio Lower Upper

117 100

119 5.0 76.9 115.3#

121 0.0 24.2 36.2#


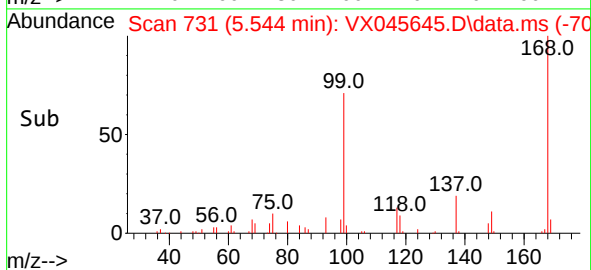

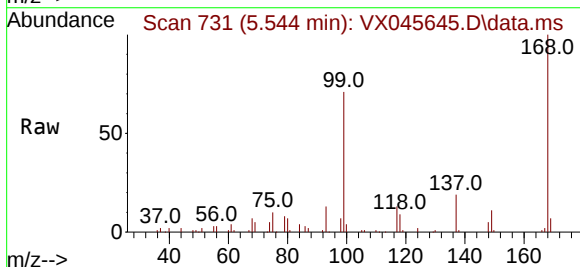


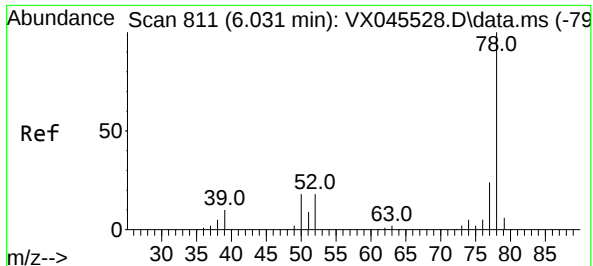

#40
Benzene
Concen: 11.227 ug/l
RT: 6.031 min Scan# 811
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion: 78 Resp: 38671
Ion Ratio Lower Upper
78 100
77 22.3 19.0 28.6

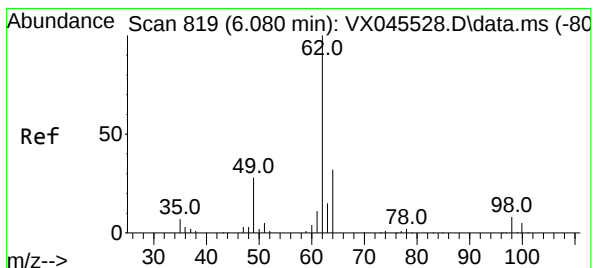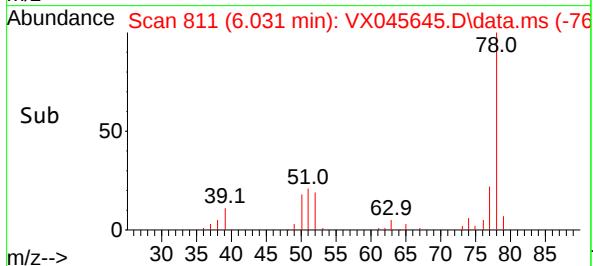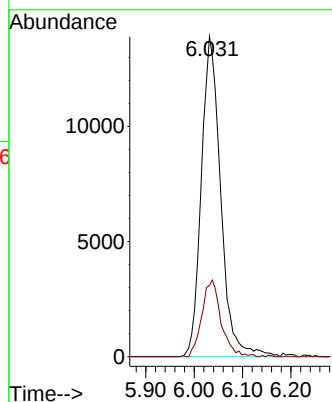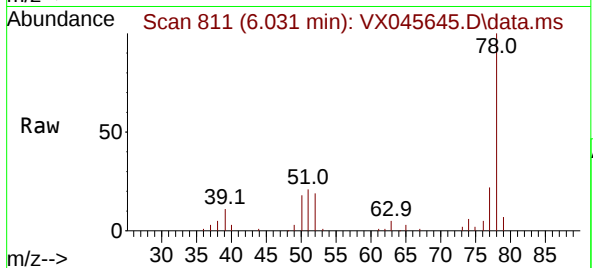

#42
1,2-Dichloroethane
Concen: 0.239 ug/l
RT: 6.050 min Scan# 814
Delta R.T. -0.030 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 62 Resp: 340
Ion Ratio Lower Upper
62 100
98 0.0 0.0 15.2


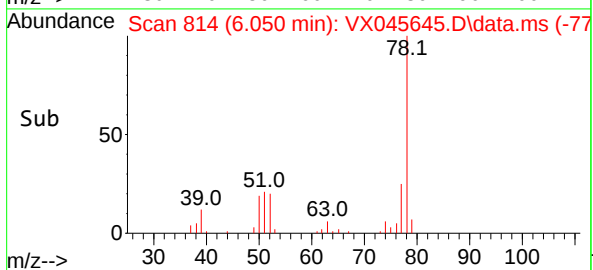
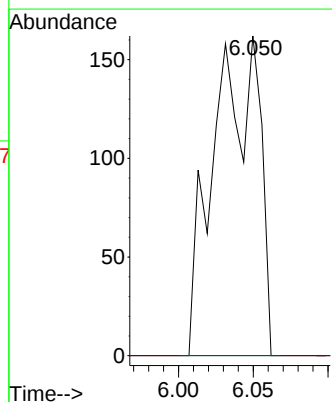
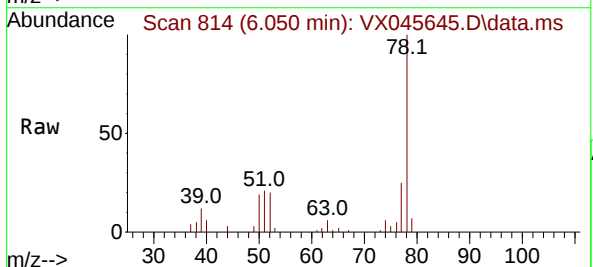




#43
Isopropyl Acetate
Concen: 1.332 ug/l
RT: 6.355 min Scan# 80
Delta R.T. 0.018 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion: 43 Resp: 2870
Ion Ratio Lower Upper
43 100
61 7.3 14.1 21.1#
87 2.5 9.2 13.8#

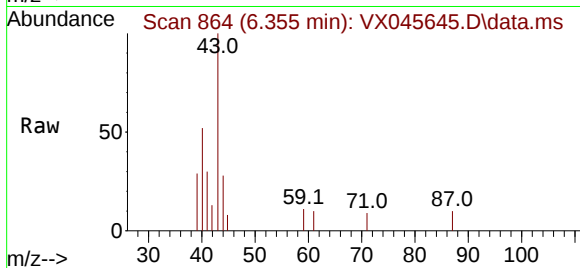

#48
Methyl methacrylate
Concen: 0.661 ug/l
RT: 7.616 min Scan# 1071
Delta R.T. -0.073 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 41 Resp: 735
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 15.4 53.6 80.4#




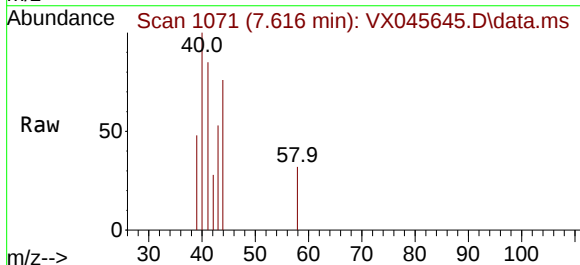


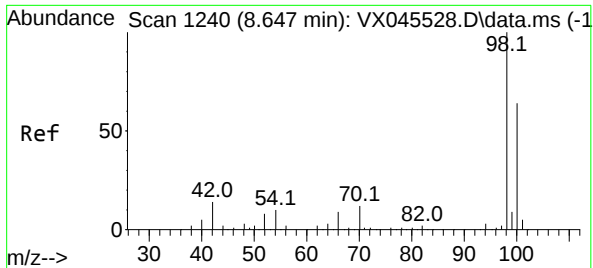

#50
Toluene-d8
Concen: 52.346 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion: 98 Resp: 152623
Ion Ratio Lower Upper
98 100
100 64.7 52.2 78.4

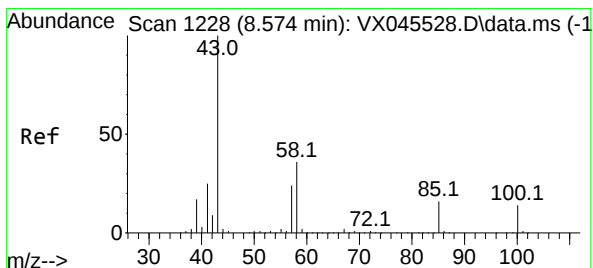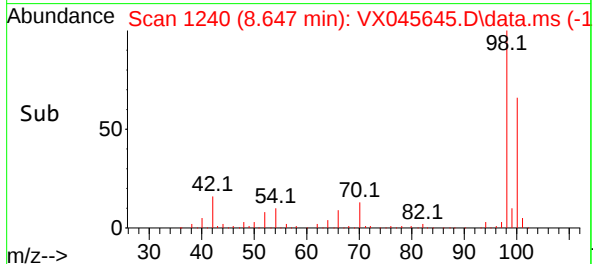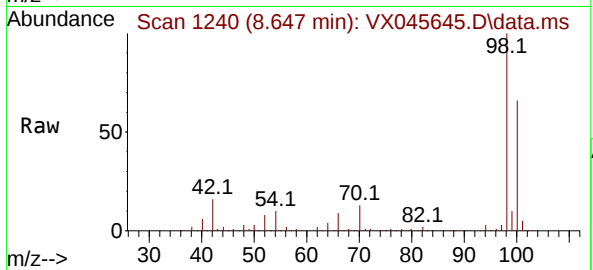

#51
4-Methyl-2-Pentanone
Concen: 14.982 ug/l
RT: 8.543 min Scan# 1223
Delta R.T. -0.030 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 43 Resp: 21395
Ion Ratio Lower Upper
43 100
58 0.0 28.5 42.7#


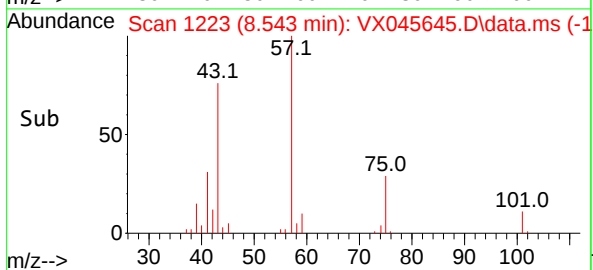

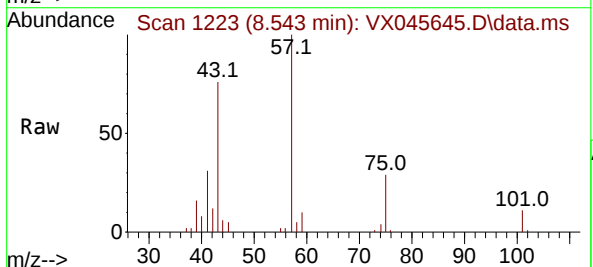




#52
Toluene
Concen: 1.323 ug/l
RT: 8.720 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion: 92 Resp: 2758
Ion Ratio Lower Upper
92 100
91 172.3 138.7 208.1



#54
cis-1,3-Dichloropropene
Concen: 4.237 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.183 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 75 Resp: 5246
Ion Ratio Lower Upper
75 100
77 0.0 24.6 36.8#
39 53.6 48.4 72.6



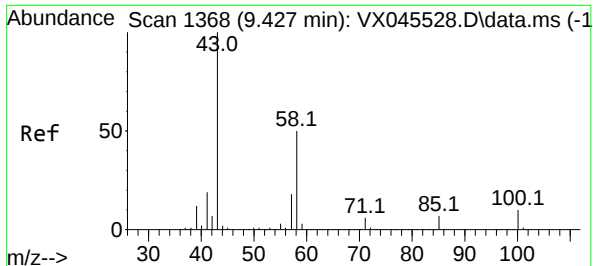

#59

2-Hexanone

Concen: 2.179 ug/l

RT: 9.439 min Scan# 11

Delta R.T. 0.012 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28

Instrument :

MSVOA_X

ClientSampleId :





RT3069

Tgt Ion: 43 Resp: 2304

Ion Ratio Lower Upper

43 100

58 36.2 24.9 74.6

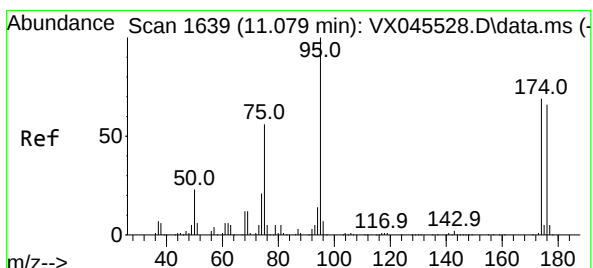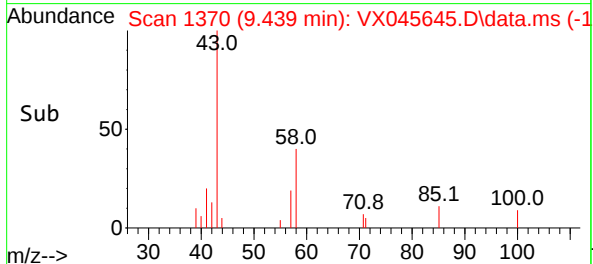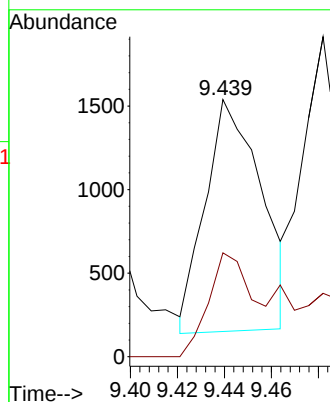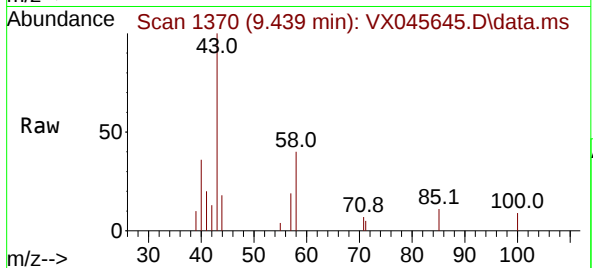

#62

4-Bromofluorobenzene

Concen: 53.578 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX045645.D

Acq: 08 Apr 2025 12:28




Tgt Ion: 95 Resp: 56901


Ion Ratio Lower Upper

95 100

174 67.7 0.0 135.8

176 64.3 0.0 131.4


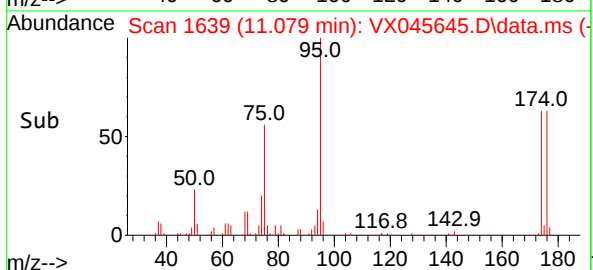

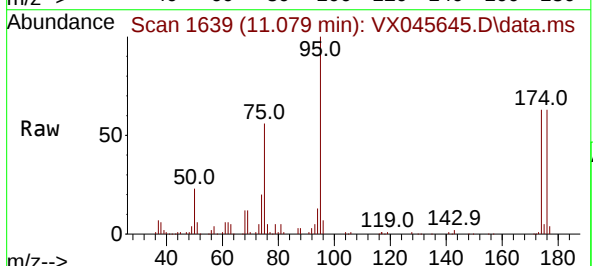




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion:117 Resp: 112767
Ion Ratio Lower Upper
117 100
82 61.9 49.2 73.8
119 32.9 25.1 37.7

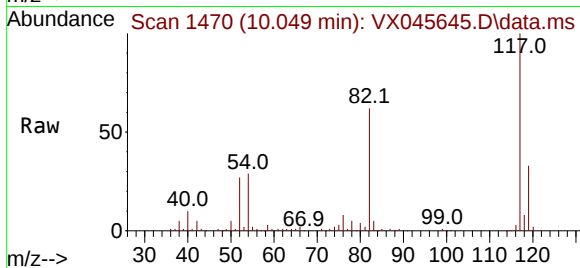

#67
Ethyl Benzene
Concen: 0.359 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 91 Resp: 1549
Ion Ratio Lower Upper
91 100
106 34.1 23.7 35.5



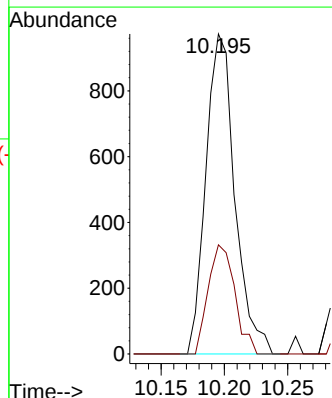
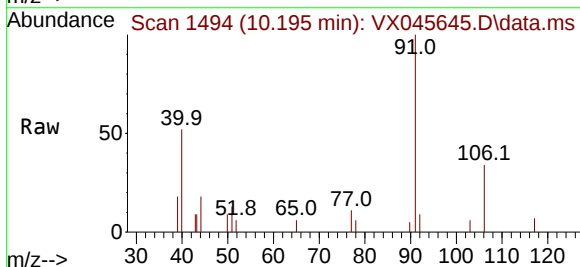




#68
m/p-Xylenes
Concen: 0.434 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion:106 Resp: 682
Ion Ratio Lower Upper
106 100
91 240.6 172.6 258.8

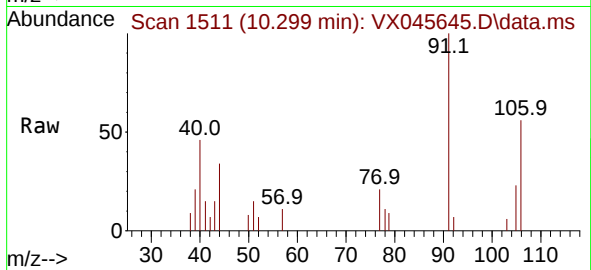

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion:152 Resp: 47540
Ion Ratio Lower Upper
152 100
115 66.4 46.9 140.7
150 160.9 0.0 349.4


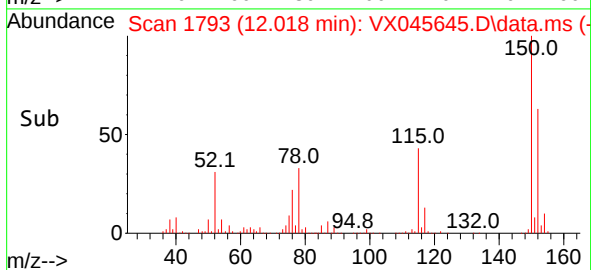






#73
Isopropylbenzene
Concen: 0.952 ug/l
RT: 10.957 min Scan# 1619
Delta R.T. 0.000 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion:105 Resp: 3627
Ion Ratio Lower Upper
105 100
120 26.4 12.7 38.0

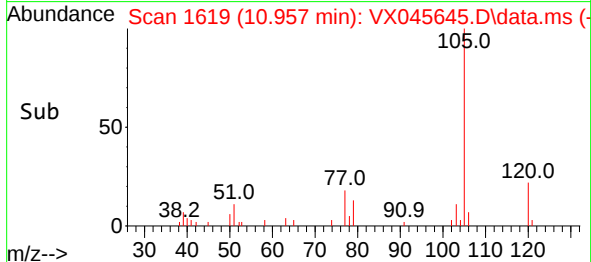

#74
N-ethyl acetate
Concen: 0.248 ug/l
RT: 10.866 min Scan# 1604
Delta R.T. 0.024 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 43 Resp: 451
Ion Ratio Lower Upper
43 100
70 65.9 30.1 45.1#
55 118.4 18.3 27.5#
61 0.0 17.5 26.3#




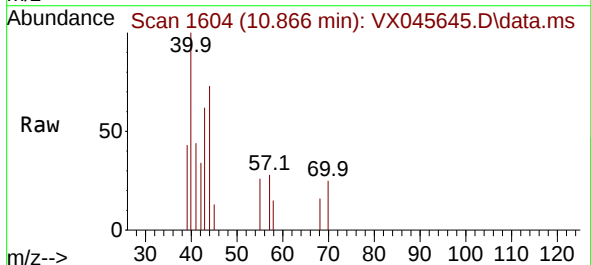




#76
1,2,3-Trichloropropane
Concen: 27.957 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28




Instrument :
MSVOA_X
ClientSampleId :
RT3069


Tgt Ion: 75 Resp: 32419
Ion Ratio Lower Upper
75 100
77 1.1 20.0 59.9#

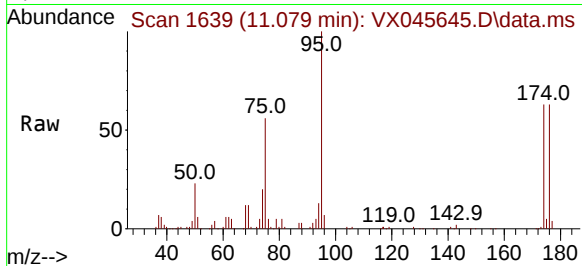

#81
trans-1,4-Dichloro-2-butene
Concen: 94.882 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion: 75 Resp: 32419
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#



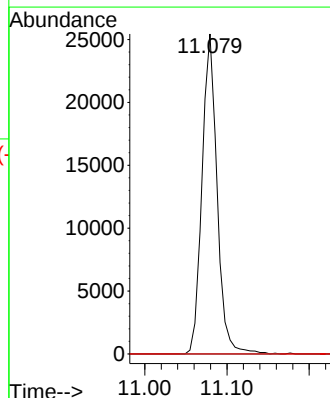
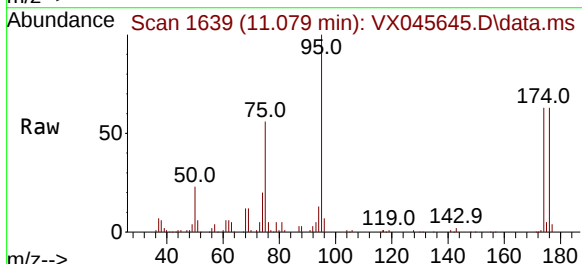




#90
Hexachloroethane
Concen: 0.284 ug/l
RT: 12.603 min Scan# 1889
Delta R.T. 0.067 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Instrument :
MSVOA_X
ClientSampleId :
RT3069

Tgt Ion:117 Resp: 154
Ion Ratio Lower Upper
117 100
201 0.0 31.2 93.6#

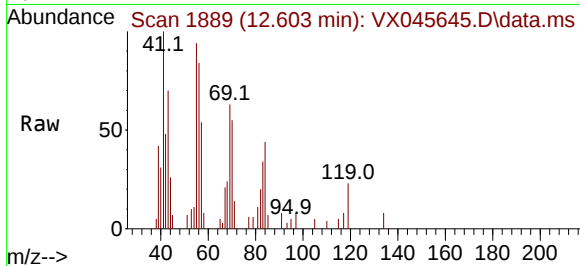

#95
Naphthalene
Concen: 0.426 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX045645.D
Acq: 08 Apr 2025 12:28

Tgt Ion:128 Resp: 1404
Ion Ratio Lower Upper
128 100
127 9.3 10.3 15.5#
129 14.0 8.6 12.8#

