

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX040919\
 Data File : VX008770.D
 Acq On : 09 Apr 2019 15:02
 Operator : JC/SP
 Sample : K2240-07
 Misc : 5.05µ/10mL/100µL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-02-COMP

Quant Time: Apr 09 16:52:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	152204	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	251820	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	221715	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	103792	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	104466	47.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.12%	
35) Dibromofluoromethane	5.50	113	72677	45.14	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.28%	
50) Toluene-d8	8.71	98	314669	49.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.16%	
62) 4-Bromofluorobenzene	11.14	95	111250	48.94	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.88%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX040919\
Data File : VX008770.D
Acq On : 09 Apr 2019 15:02
Operator : JC/SP
Sample : K2240-07
Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-02-COMP

Quant Time: Apr 09 16:52:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

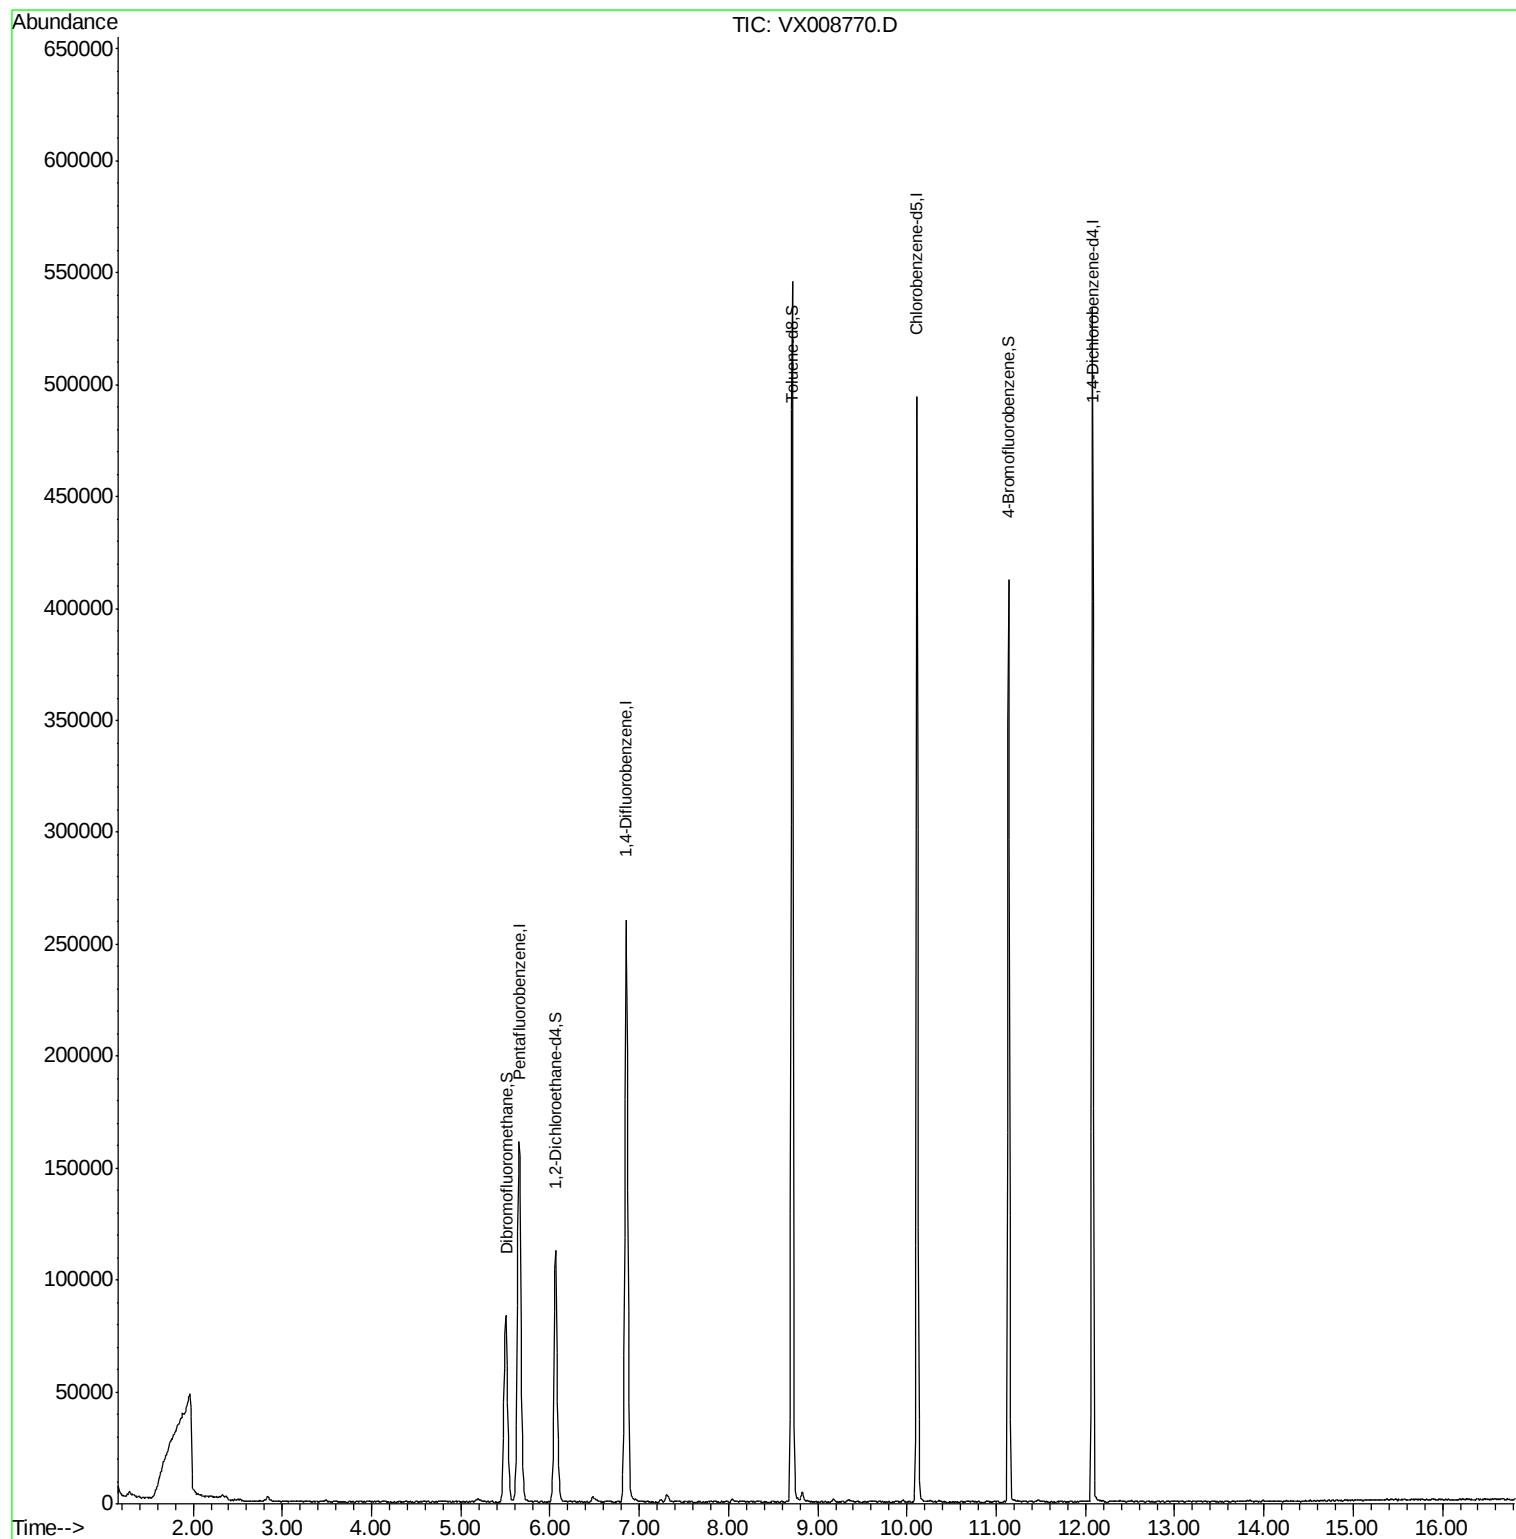

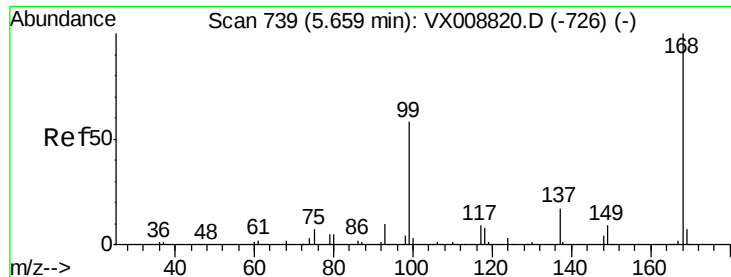

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.01 min

Lab File: VX008770.D

Acq: 09 Apr 2019 15:02

Instrument :

MSVOA_X

ClientSampleId :


SB-02-COMP

Tot Ion:168 Resp: 152204

Ion Ratio Lower Upper




168 100

99 56.7 46.7 70.1

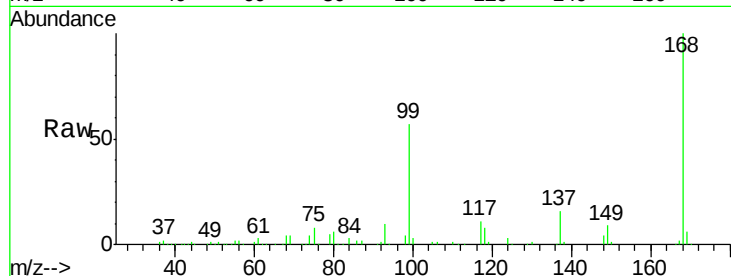

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

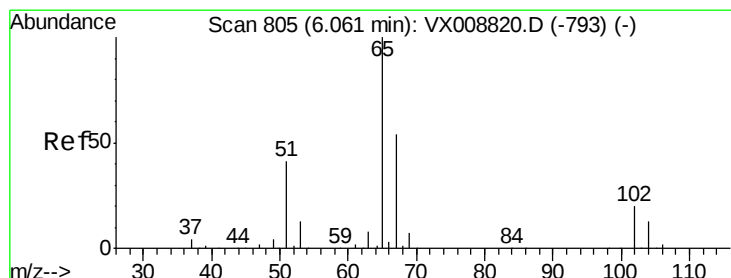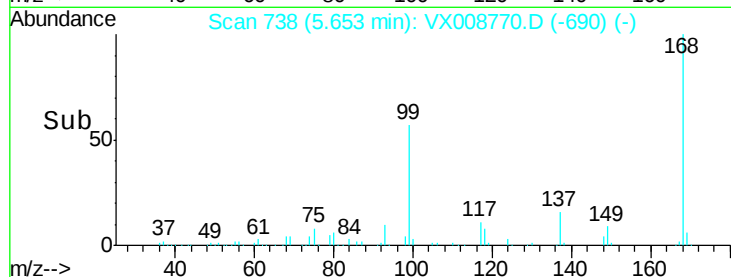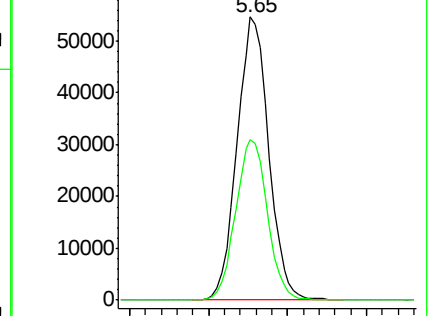

#33

1,2-Dichloroethane-d4

Concen: 47.057 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008770.D


Acq: 09 Apr 2019 15:02

Tgt Ion: 65 Resp: 104466

Ion Ratio Lower Upper



65 100


67 54.5 0.0 107.2

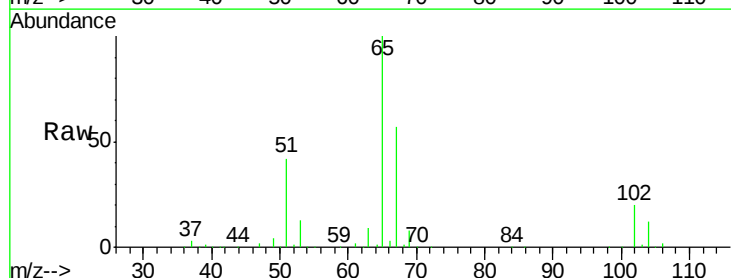

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

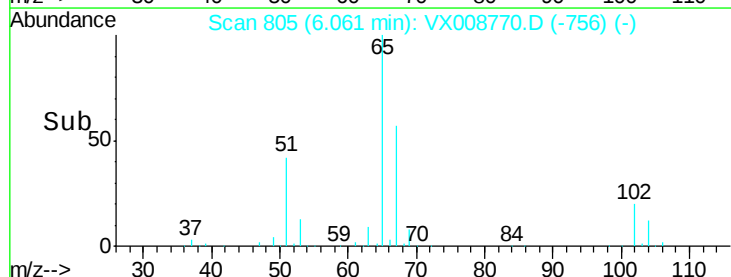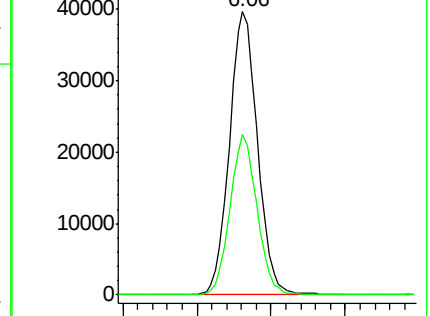


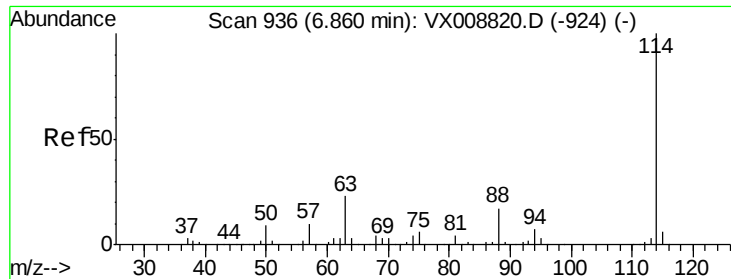




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 935
 Delta R.T. -0.01 min
 Lab File: VX008770.D
 Acq: 09 Apr 2019 15:02

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-02-COMP

Tot Ion	Ratio	Lower	Upper
114	100		
63	23.9	0.0	47.2
88	16.6	0.0	34.0

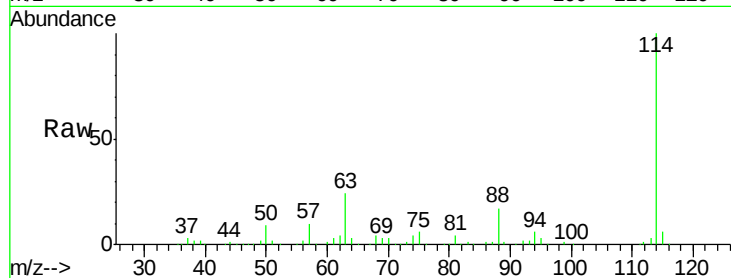


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

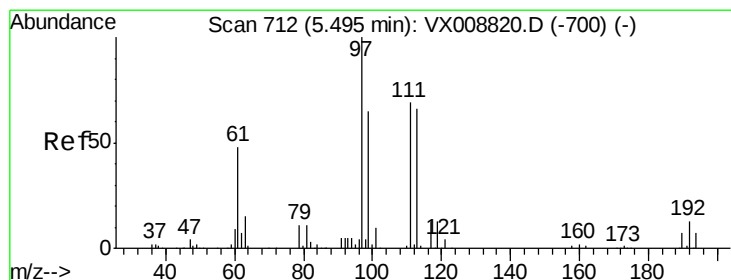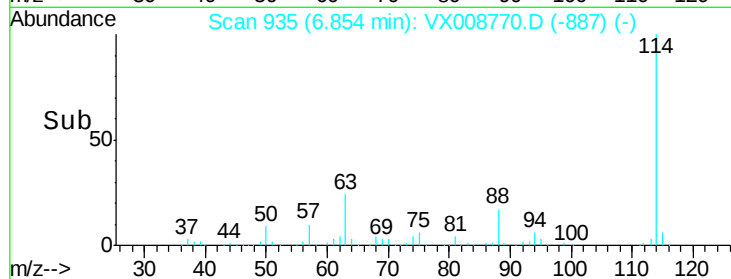
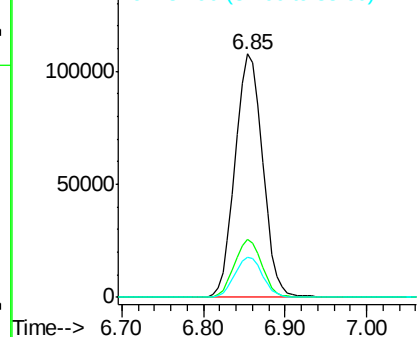



#35
 Dibromofluoromethane
 Concen: 45.140 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. -0.00 min
 Lab File: VX008770.D
 Acq: 09 Apr 2019 15:02

Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.2	83.4	125.2
192	20.6	16.1	24.1

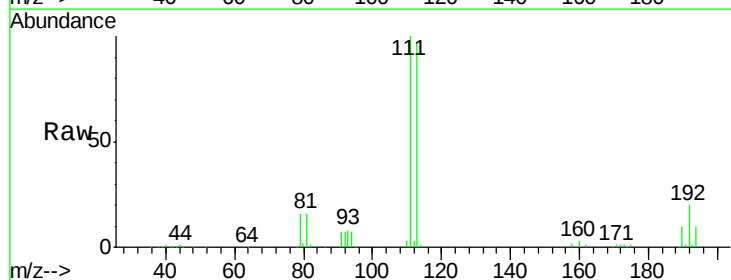

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



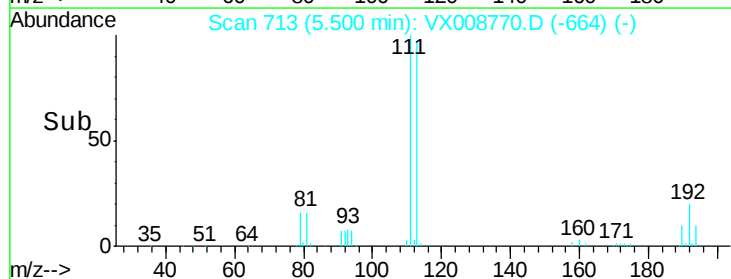
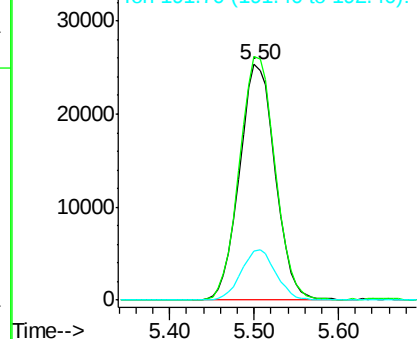


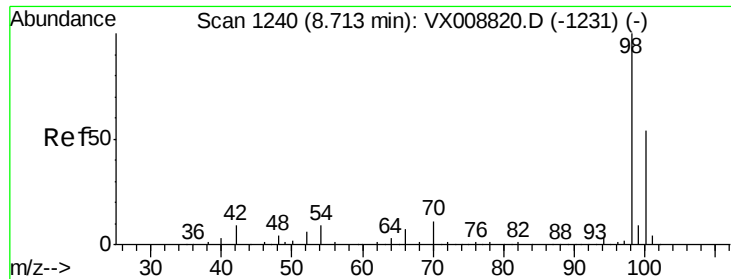

#50
Toluene-d8
Concen: 49.085 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX008770.D
Acq: 09 Apr 2019 15:02




Instrument :
MSVOA_X
ClientSampleId :
SB-02-COMP


Tot Ion: 98 Resp: 314669
Ion Ratio Lower Upper
98 100
100 64.2 51.4 77.0

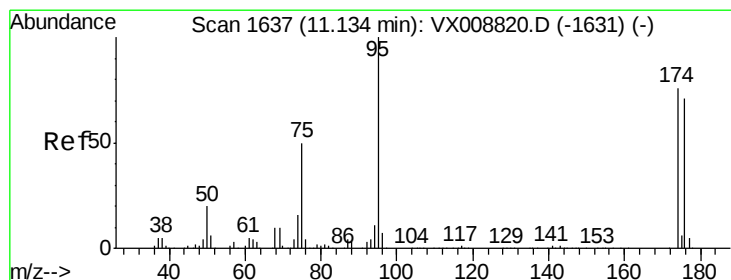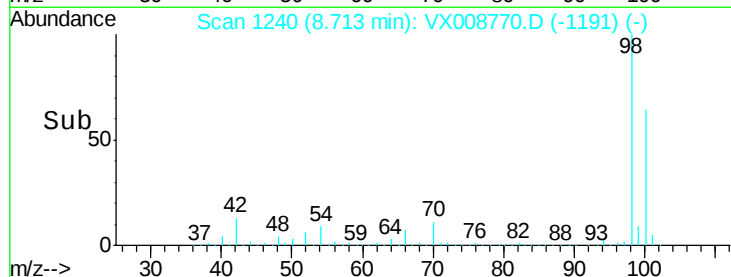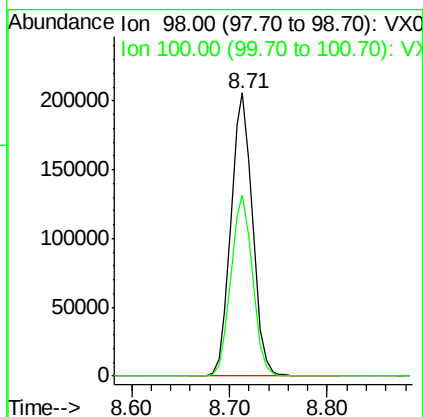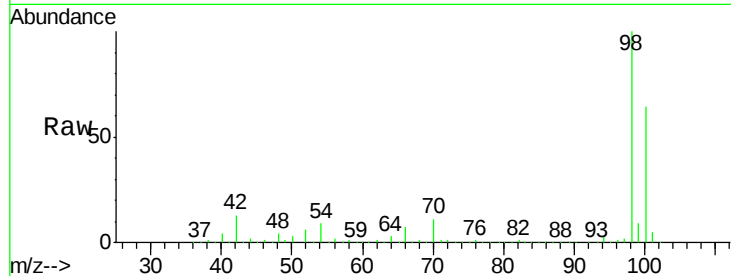

#62
4-Bromofluorobenzene
Concen: 48.936 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.01 min
Lab File: VX008770.D
Acq: 09 Apr 2019 15:02

Tgt Ion: 95 Resp: 111250
Ion Ratio Lower Upper
95 100
174 77.0 0.0 151.8
176 74.3 0.0 145.8

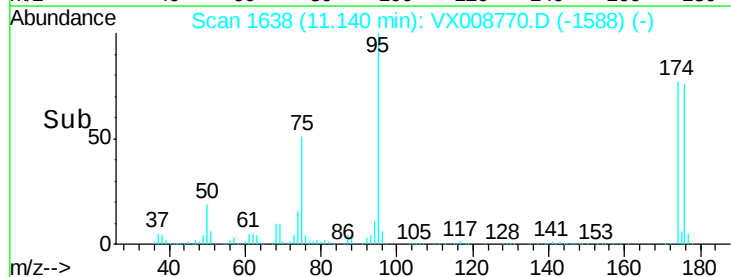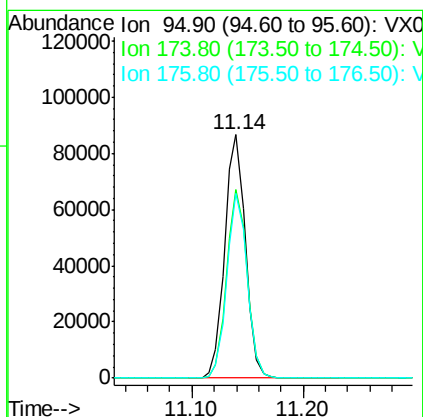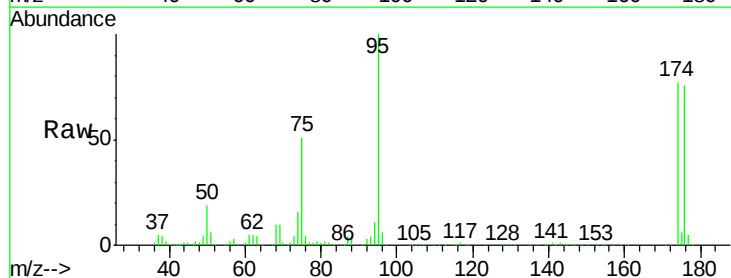


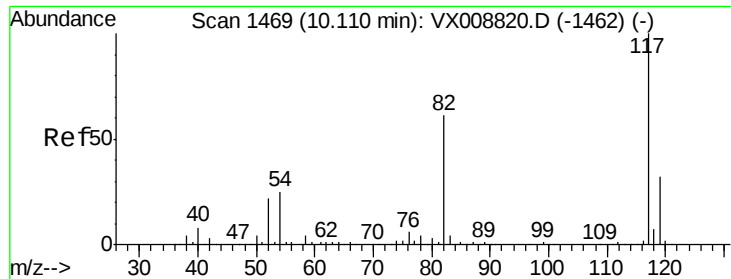




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.01 min
Lab File: VX008770.D
Acq: 09 Apr 2019 15:02

Instrument :
MSVOA_X
ClientSampleId :
SB-02-COMP

Tot Ion:117 Resp: 221715
Ion Ratio Lower Upper
117 100
82 59.2 49.6 74.4
119 32.3 25.0 37.4

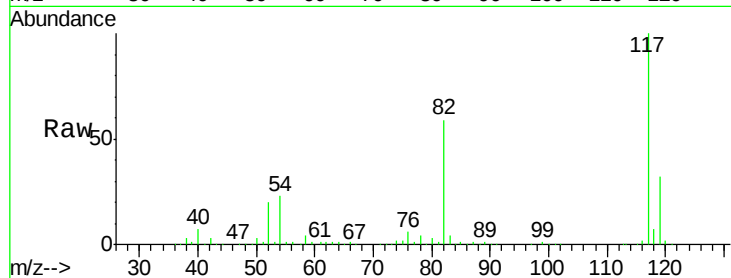


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

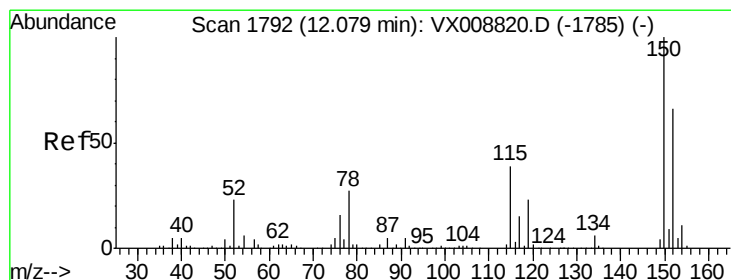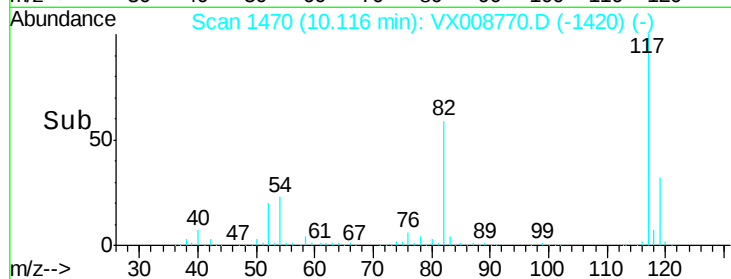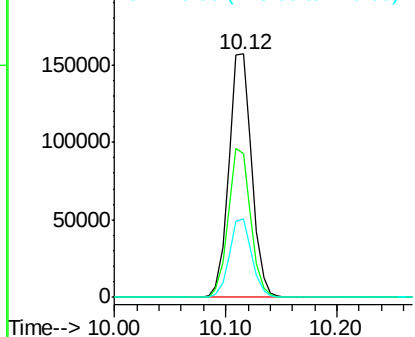

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX008770.D
Acq: 09 Apr 2019 15:02

Tgt Ion:152 Resp: 103792
Ion Ratio Lower Upper
152 100
115 58.9 43.5 130.5
150 153.6 0.0 348.8

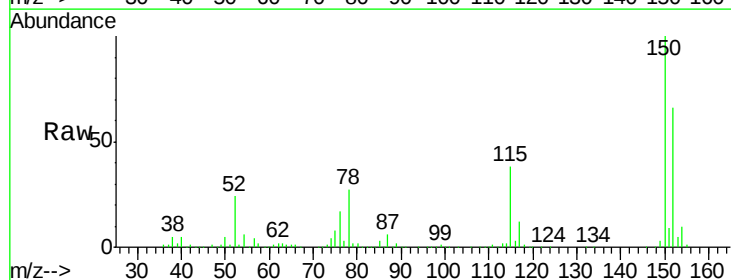

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

