

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040925\
 Data File : VX045683.D
 Acq On : 09 Apr 2025 18:02
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Title : SW846 8260

Signal : TIC: VX045683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	21	25	33	rBV	7863	13840	2.91%	0.505%
2	1.587	70	82	83	rBV4	4620	12878	2.71%	0.470%
3	5.379	694	704	720	rBV	55457	163631	34.46%	5.966%
4	5.544	722	731	747	rVB2	79941	229672	48.37%	8.374%
5	5.952	789	798	814	rBV	63649	171378	36.09%	6.249%
6	6.757	920	930	947	rBV	140501	342263	72.09%	12.480%
7	8.647	1233	1240	1253	rBV	291354	474799	100.00%	17.312%
8	10.049	1465	1470	1485	rBV	302164	429063	90.37%	15.645%
9	11.079	1634	1639	1650	rBV	248318	327787	69.04%	11.952%
10	12.018	1788	1793	1804	rBV	295193	372954	78.55%	13.599%
11	13.122	1961	1974	1975	rBV7	6823	16130	3.40%	0.588%
12	14.633	2212	2222	2233	rBV	17829	32609	6.87%	1.189%
13	14.780	2241	2246	2254	rBV	14718	21995	4.63%	0.802%
14	15.377	2338	2344	2347	rBV3	5044	8193	1.73%	0.299%
15	15.475	2354	2360	2371	rBV2	17813	32592	6.86%	1.188%
16	15.609	2375	2382	2386	rBV	20685	35408	7.46%	1.291%
17	15.645	2386	2388	2395	rVB2	12168	17818	3.75%	0.650%
18	15.841	2411	2420	2430	rVB3	7715	19738	4.16%	0.720%
19	15.987	2437	2444	2449	rBV2	4596	8115	1.71%	0.296%
20	16.597	2539	2544	2549	rVB4	3374	5419	1.14%	0.198%
21	16.657	2549	2554	2560	rBV6	3281	6287	1.32%	0.229%




Sum of corrected areas: 2742569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040925\
Data File : VX045683.D
Acq On : 09 Apr 2025 18:02
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

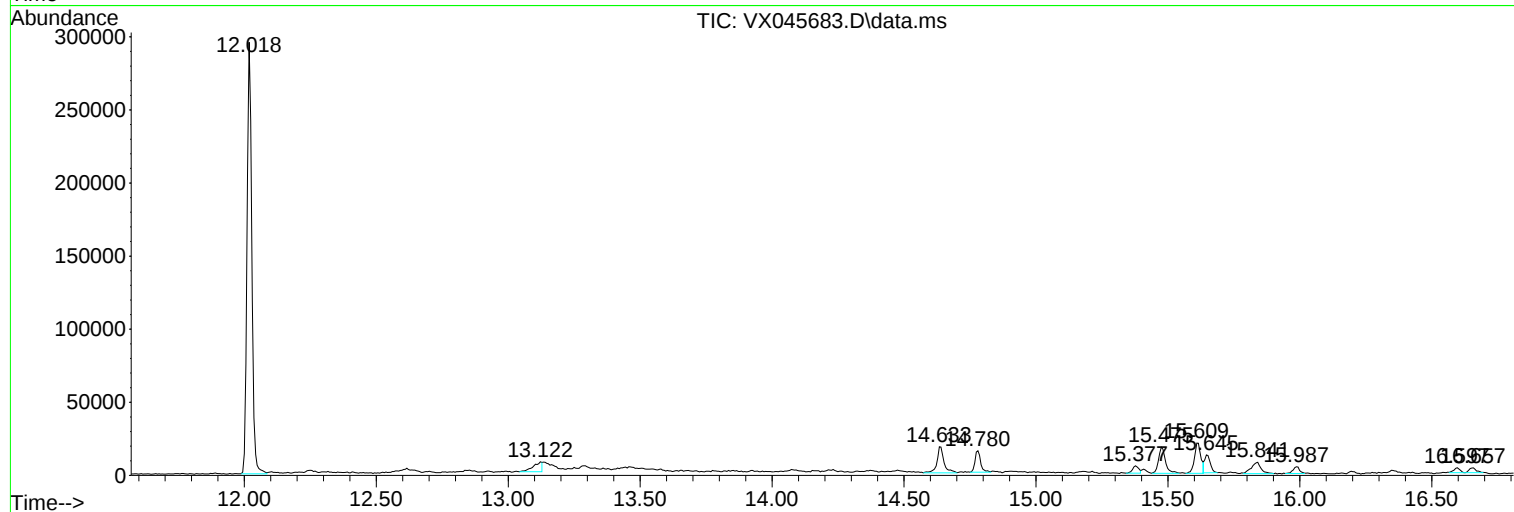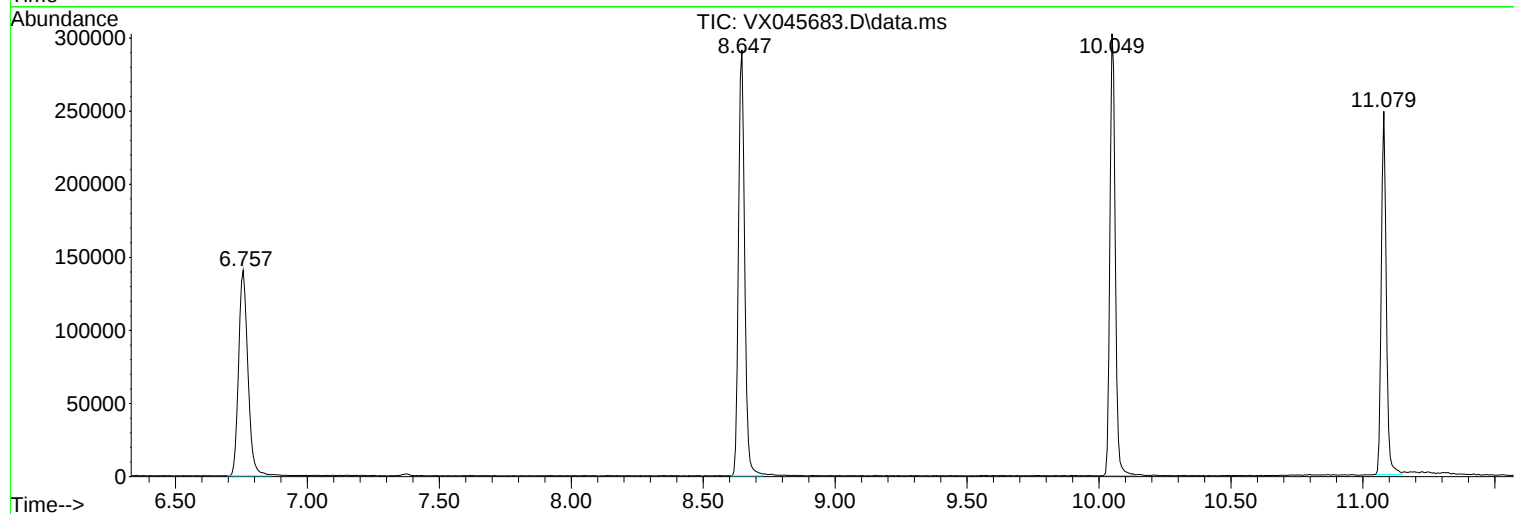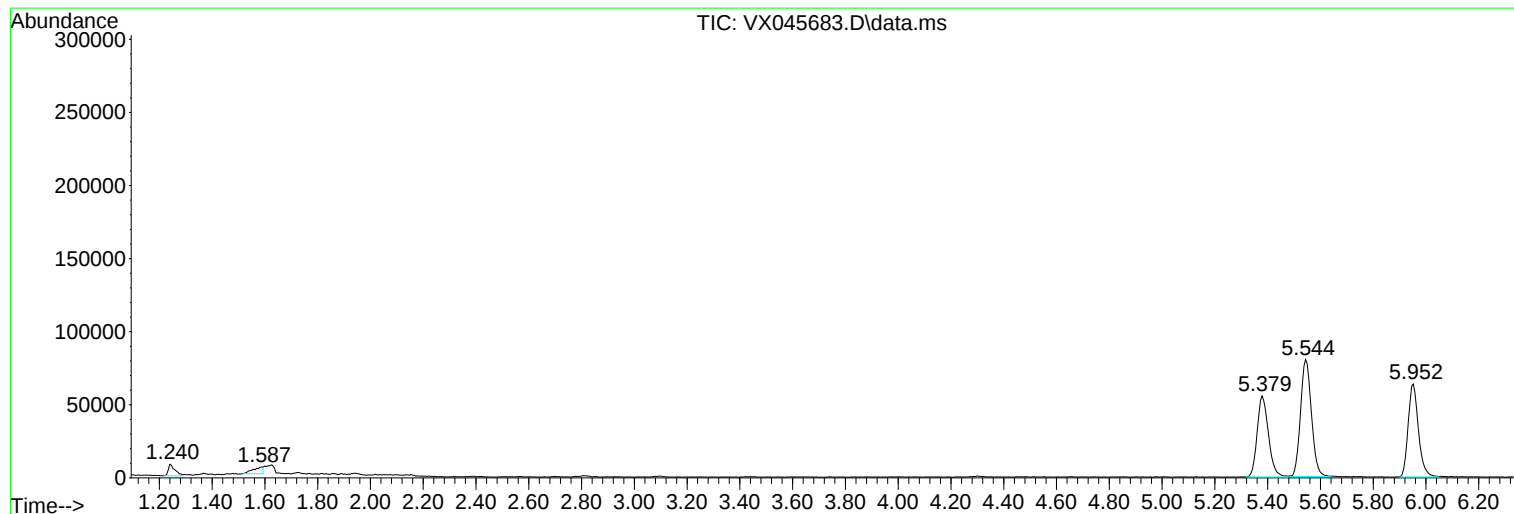

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040925\
Data File : VX045683.D
Acq On : 09 Apr 2025 18:02
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040925\
Data File : VX045683.D
Acq On : 09 Apr 2025 18:02
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc