



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX040925\
Data File : VX045663.D
Acq On : 09 Apr 2025 09:38
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Title : SW846 8260
Last Update : Wed Apr 02 03:11:43 2025

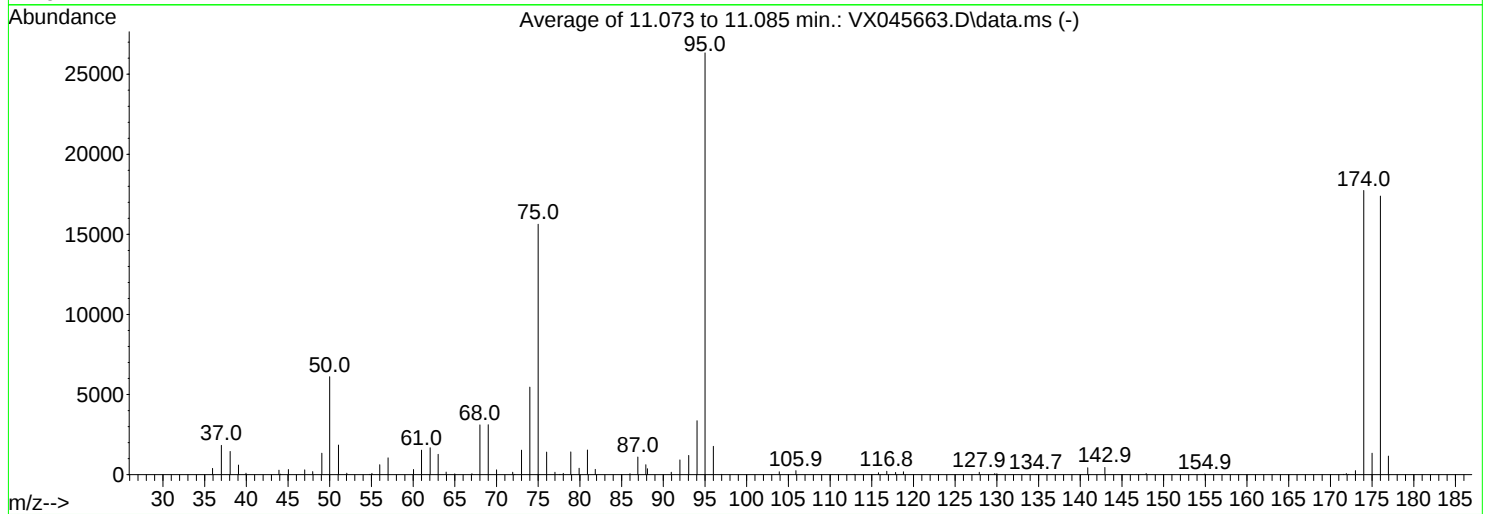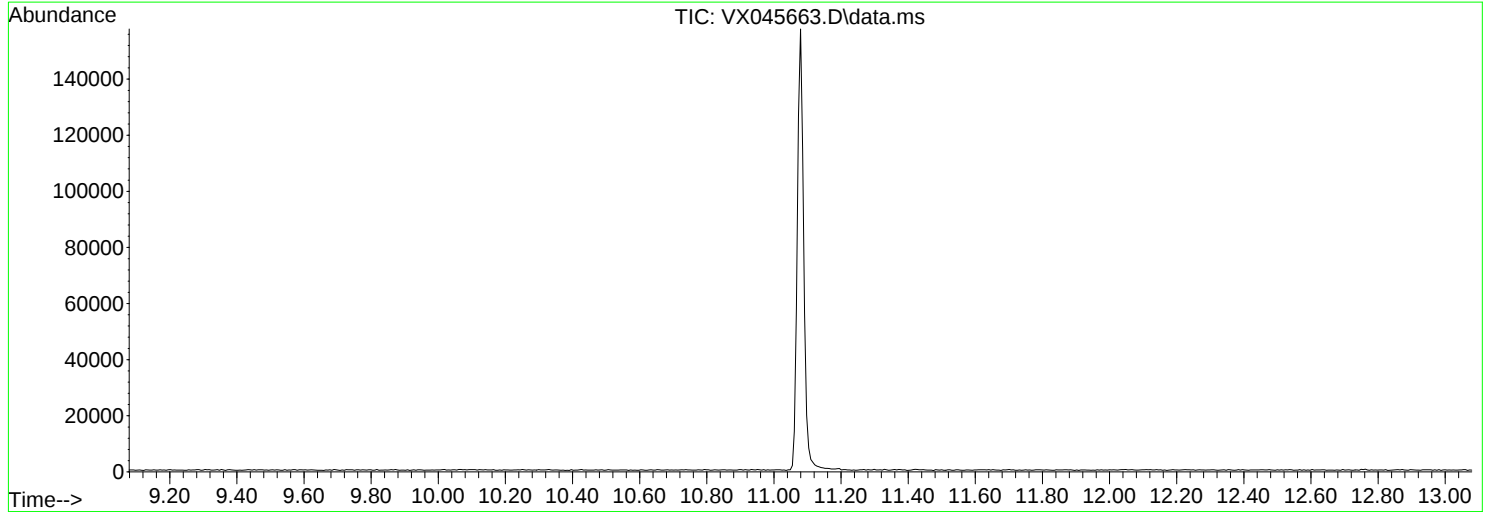

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	6109	PASS
75	95	30	60	59.4	15637	PASS
95	95	100	100	100.0	26333	PASS
96	95	5	9	6.7	1772	PASS
173	174	0.00	2	1.4	252	PASS
174	95	50	100	67.4	17742	PASS
175	174	5	9	7.5	1336	PASS
176	174	95	101	98.0	17394	PASS
177	176	5	9	6.7	1162	PASS