

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX041019\
 Data File : VX008838.D
 Acq On : 11 Apr 2019 05:01
 Operator : JC/SP
 Sample : K2342-12
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-12-S

Quant Time: Apr 11 08:55:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	193506	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	310911	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	275492	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	115057	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	127608	45.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.42%	
35) Dibromofluoromethane	5.49	113	93288	46.93	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.86%	
50) Toluene-d8	8.71	98	396431	50.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.18%	
62) 4-Bromofluorobenzene	11.13	95	133065	47.41	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.82%	
Target Compounds						
16) Acetone	2.44	43	22286	13.709	ug/l	100
20) Methylene Chloride	2.85	84	68118	25.033	ug/l	95
25) 2-Butanone	4.68	43	6604	2.570	ug/l	98
43) Isopropyl Acetate	6.45	43	10580	1.489	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX041019\
Data File : VX008838.D
Acq On : 11 Apr 2019 05:01
Operator : JC/SP
Sample : K2342-12
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-12-S

Quant Time: Apr 11 08:55:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

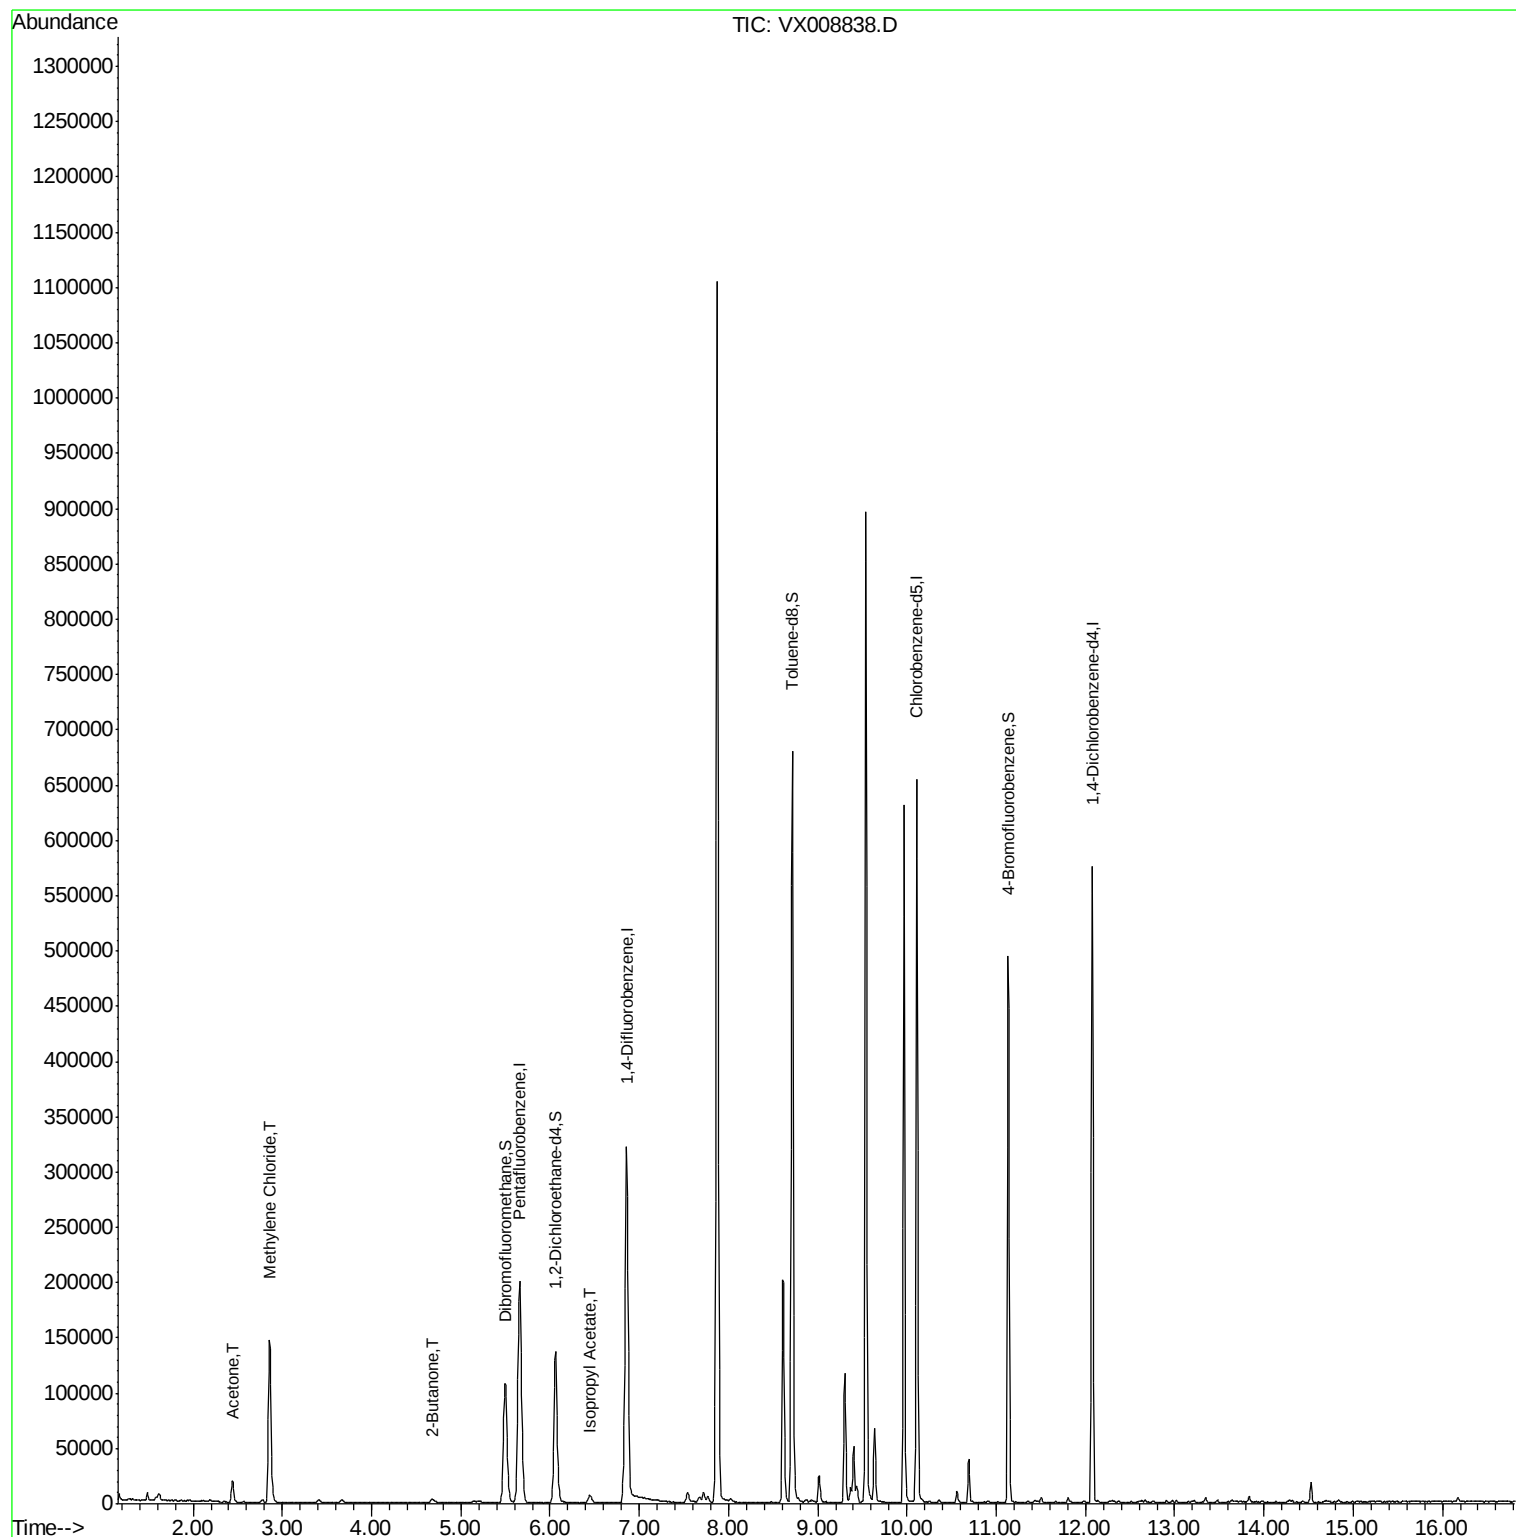

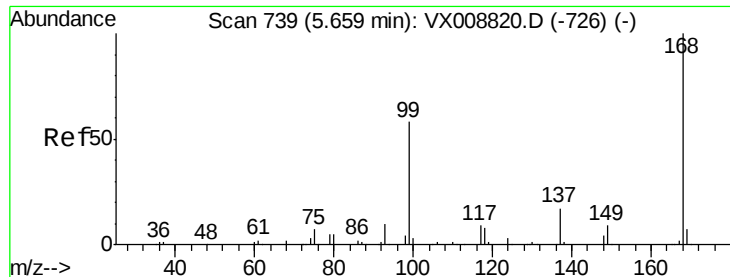

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX008838.D

Acq: 11 Apr 2019 05:01

Instrument :

MSVOA_X

ClientSampleId :


TP-12-S

Tot Ion:168 Resp: 193506

Ion Ratio Lower Upper

168 100

99 57.2 46.7 70.1

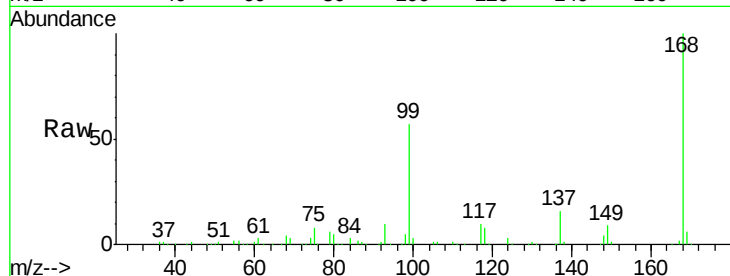

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

60000



40000

20000

0

5.50 5.60 5.70 5.80 5.90

Time-->

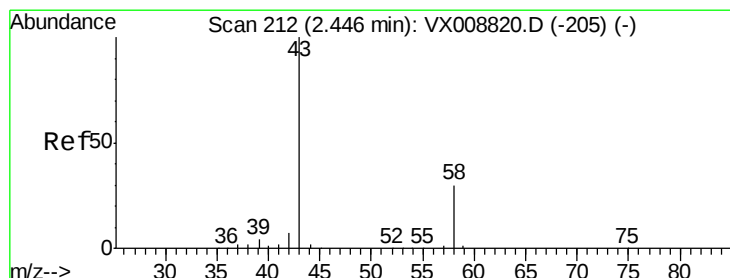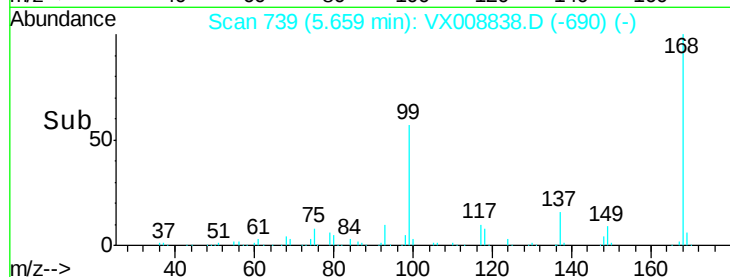

#16

Acetone

Concen: 13.709 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX008838.D


Acq: 11 Apr 2019 05:01

Tgt Ion: 43 Resp: 22286

Ion Ratio Lower Upper

43 100

58 31.1 24.8 37.2

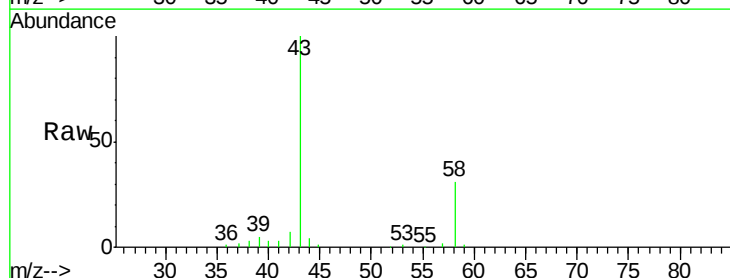

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

15000


10000


5000

0

2.40 2.44 2.48

Time-->

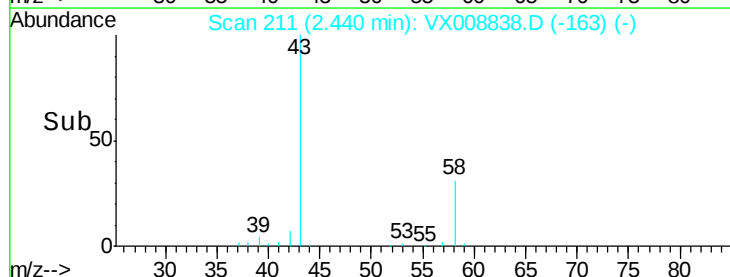


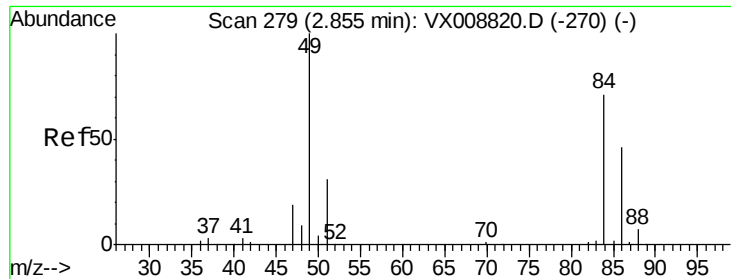




#20
Methvlene Chloride
Concen: 25.033 ug/l
RT: 2.85 min Scan# 279
Delta R.T. -0.01 min
Lab File: VX008838.D
Acq: 11 Apr 2019 05:01

Instrument :
MSVOA_X
ClientSampleId :
TP-12-S

Tot Ion: 84 Resp: 68118
Ion Ratio Lower Upper
84 100
49 145.5 109.7 164.5
51 43.6 33.6 50.4
86 63.6 51.4 77.2

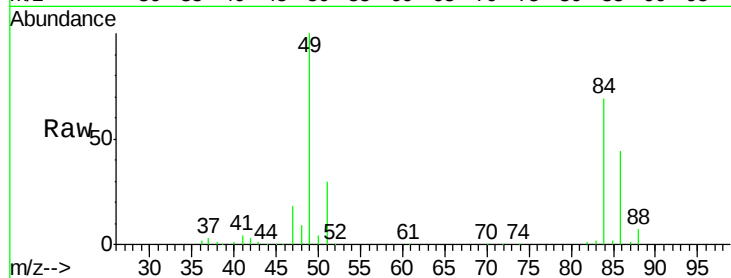


Abundance Ion 83.90 (83.60 to 84.60): VX0
Ion 48.90 (48.60 to 49.60): VX0
Ion 50.90 (50.60 to 51.60): VX0
Ion 85.90 (85.60 to 86.60): VX0

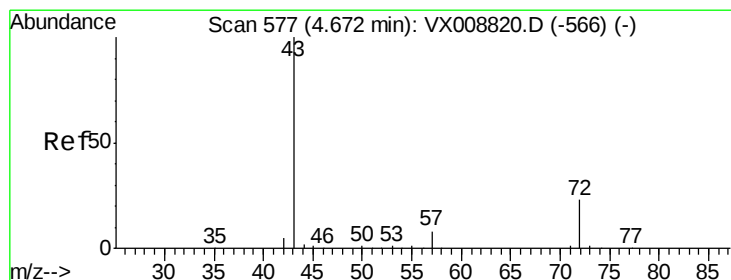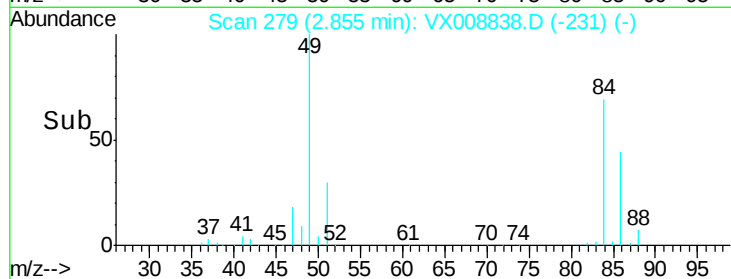
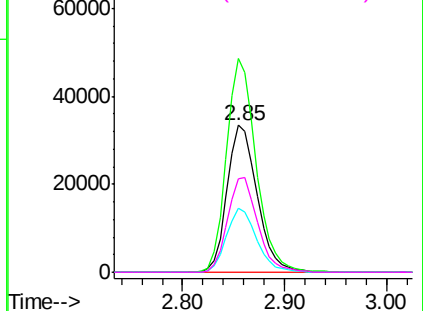



#25
2-Butanone
Concen: 2.570 ug/l
RT: 4.68 min Scan# 578
Delta R.T. -0.00 min
Lab File: VX008838.D
Acq: 11 Apr 2019 05:01

Tgt Ion: 43 Resp: 6604
Ion Ratio Lower Upper
43 100
72 21.6 18.2 27.4

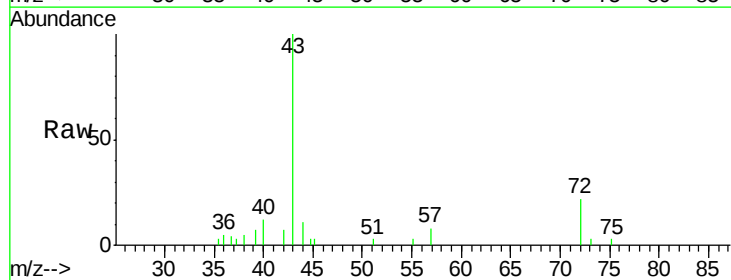

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 72.00 (71.70 to 72.70): VX0



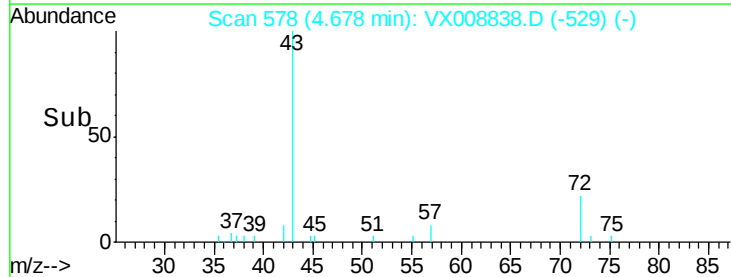
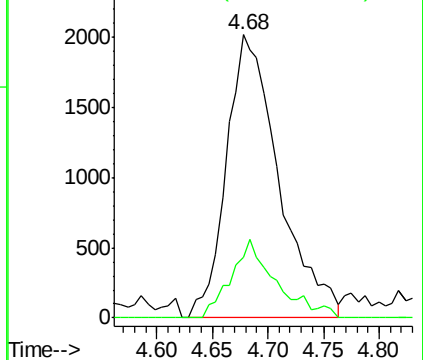


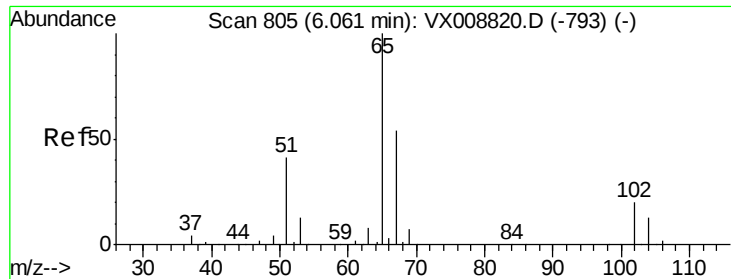

#33
 1,2-Dichloroethane-d4
 Concen: 45.213 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: VX008838.D
 Acq: 11 Apr 2019 05:01




Instrument :
 MSVOA_X
 ClientSampled :
 TP-12-S


Tot Ion: 65 Resp: 127608
 Ion Ratio Lower Upper
 65 100
 67 54.4 0.0 107.2

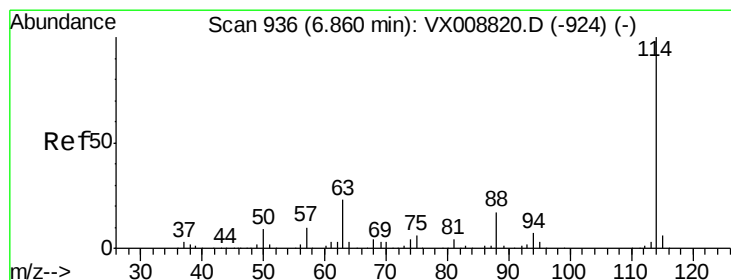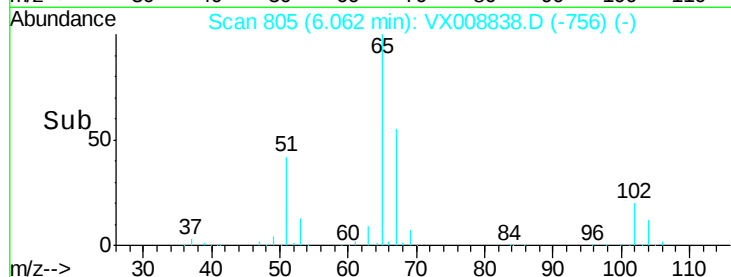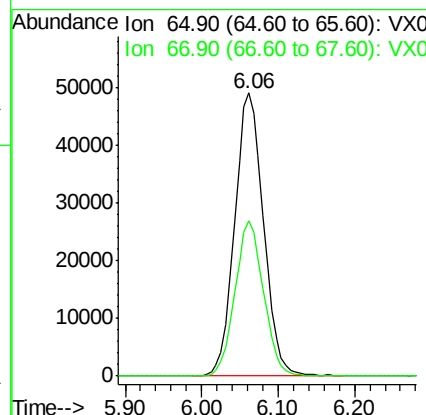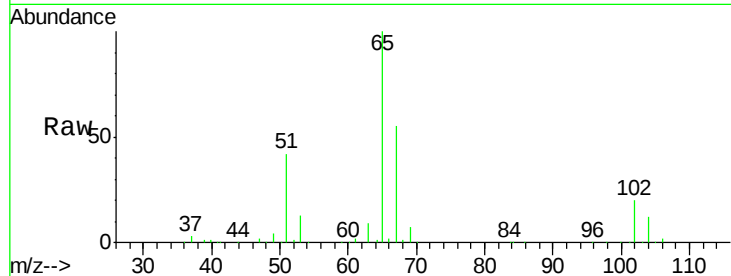

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX008838.D
 Acq: 11 Apr 2019 05:01

Tgt Ion:114 Resp: 310911
 Ion Ratio Lower Upper
 114 100
 63 23.7 0.0 47.2
 88 16.1 0.0 34.0

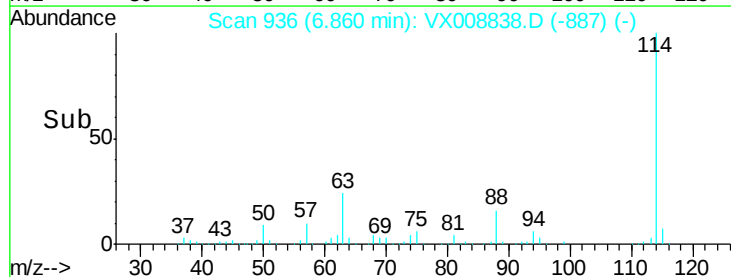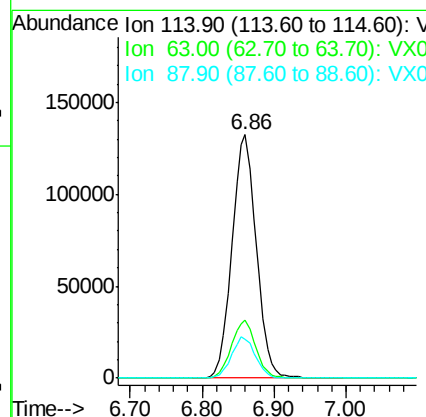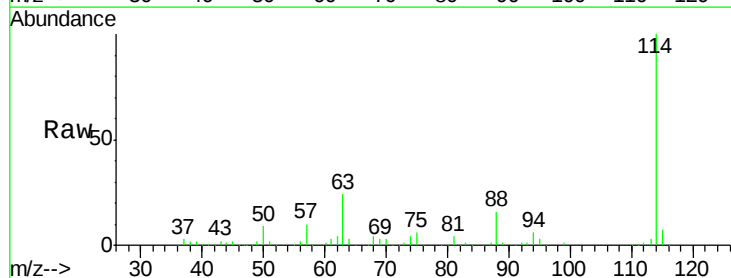

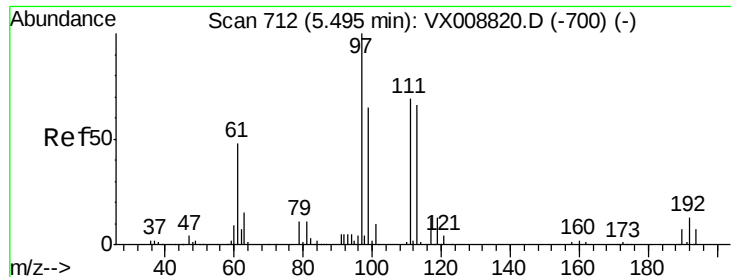

#35

Dibromofluoromethane

Concen: 46.929 ug/l

RT: 5.49 min Scan# 712

Delta R.T. -0.01 min

Lab File: VX008838.D

Acq: 11 Apr 2019 05:01

Instrument :

MSVOA_X

ClientSampled :

TP-12-S


Tot Ion:113 Resp: 93288

Ion Ratio Lower Upper

113 100

111 104.2 83.4 125.2




192 20.7 16.1 24.1

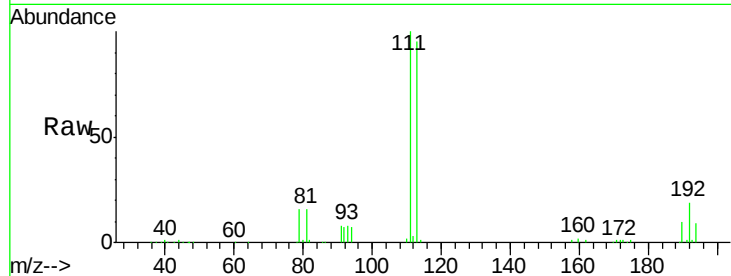

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

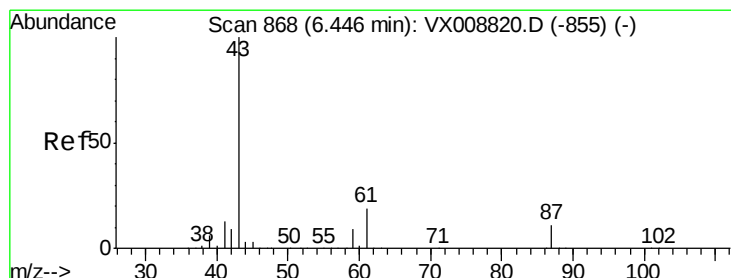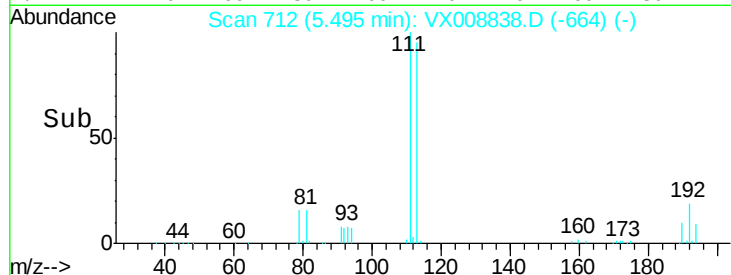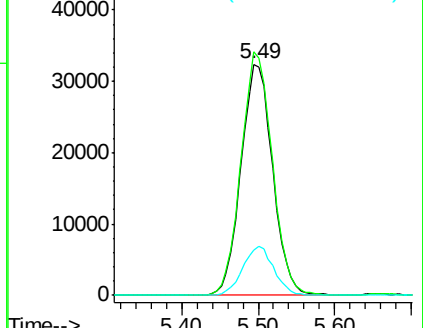

#43

Isopropyl Acetate

Concen: 1.489 ug/l

RT: 6.45 min Scan# 868

Delta R.T. -0.00 min

Lab File: VX008838.D

Acq: 11 Apr 2019 05:01


Tgt Ion: 43 Resp: 10580

Ion Ratio Lower Upper

43 100

61 19.2 15.3 22.9



87 12.1 9.0 13.6

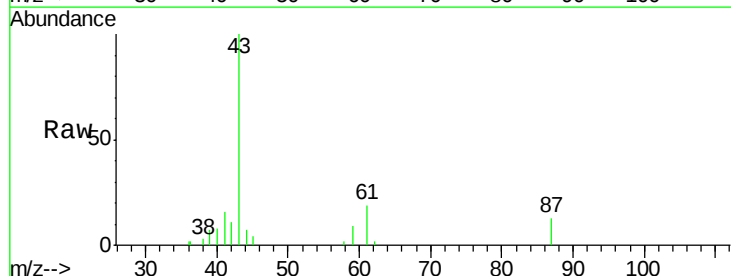


Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0



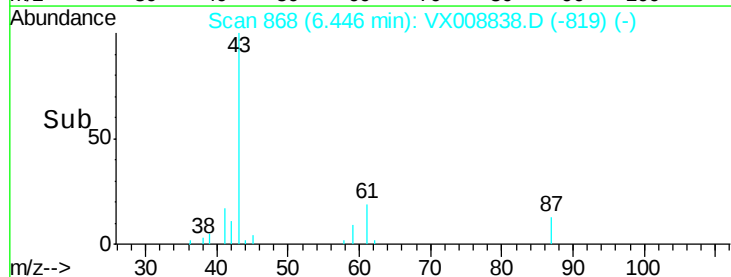
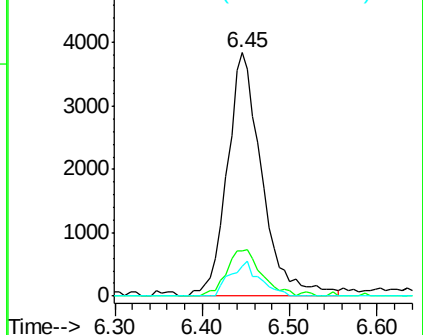


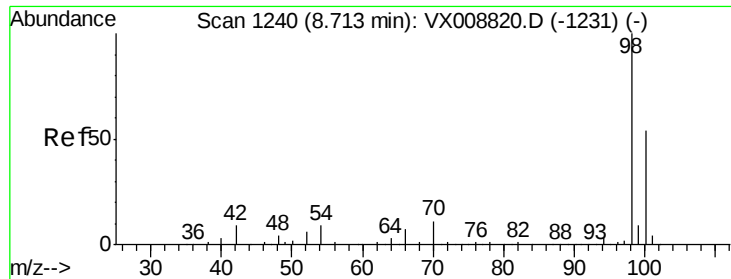

#50
Toluene-d8
Concen: 50.086 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX008838.D
Acq: 11 Apr 2019 05:01




Instrument :
MSVOA_X
ClientSampleId :
TP-12-S


Tot Ion: 98 Resp: 396431
Ion Ratio Lower Upper
98 100
100 64.4 51.4 77.0

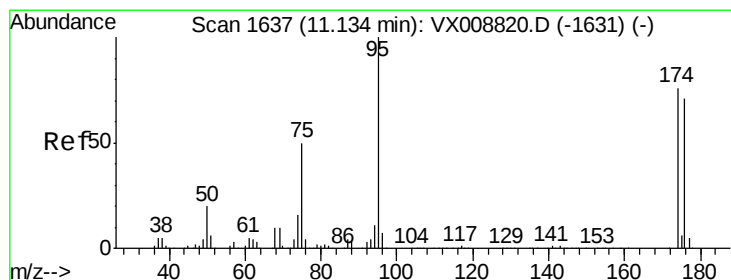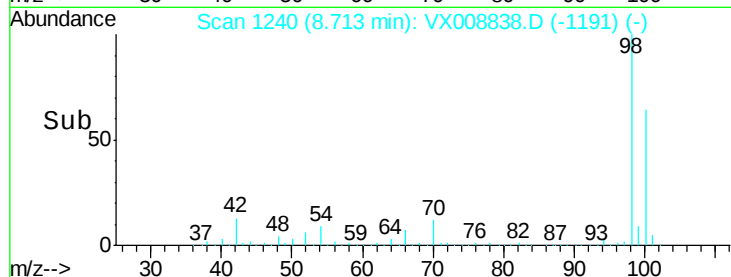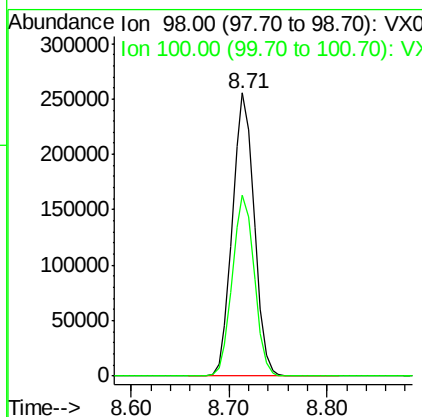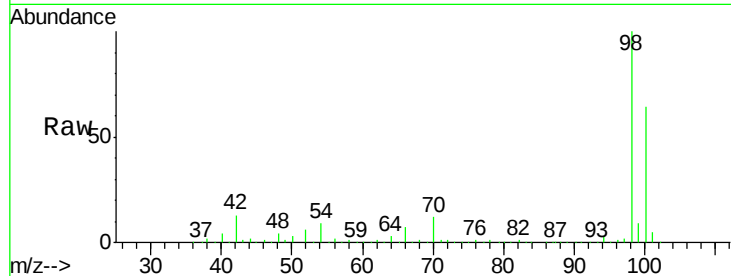

#62
4-Bromofluorobenzene
Concen: 47.408 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX008838.D
Acq: 11 Apr 2019 05:01

Tgt Ion: 95 Resp: 133065
Ion Ratio Lower Upper
95 100
174 77.9 0.0 151.8
176 76.6 0.0 145.8

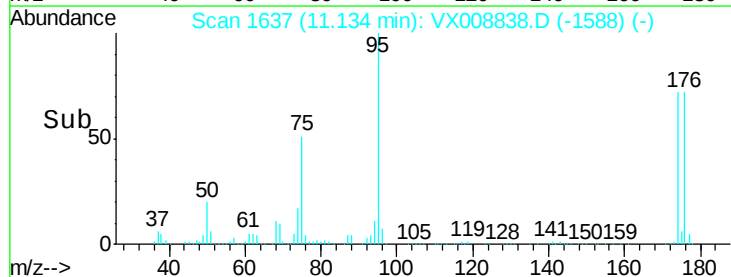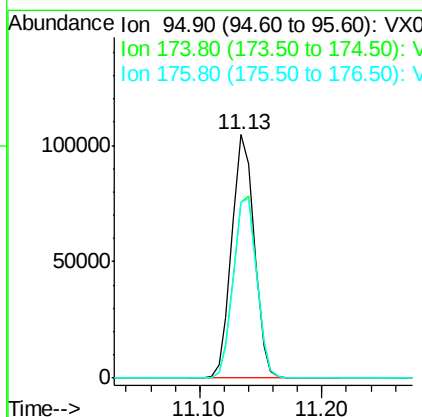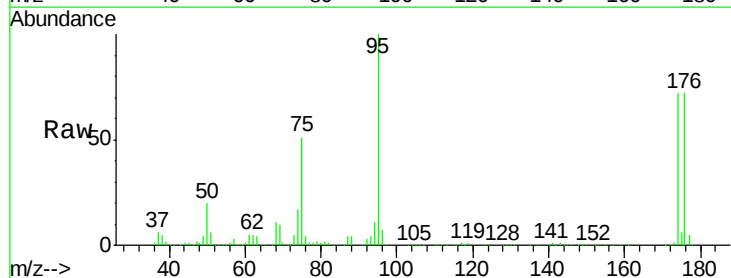


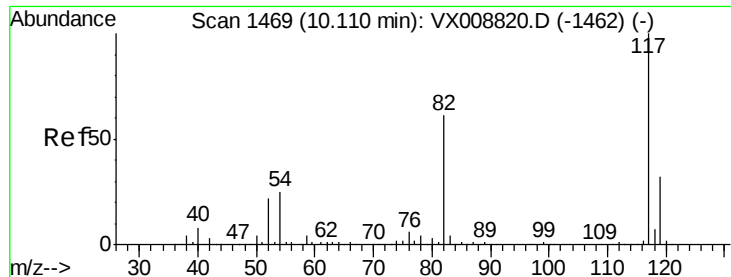




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX008838.D
Acq: 11 Apr 2019 05:01

Instrument :
MSVOA_X
ClientSampled :
TP-12-S

Tot Ion:117 Resp: 275492
Ion Ratio Lower Upper
117 100
82 61.7 49.6 74.4
119 31.6 25.0 37.4

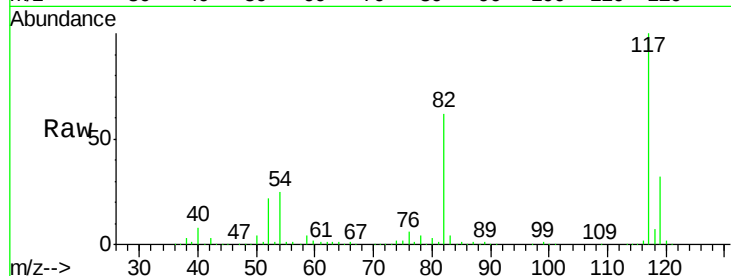


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

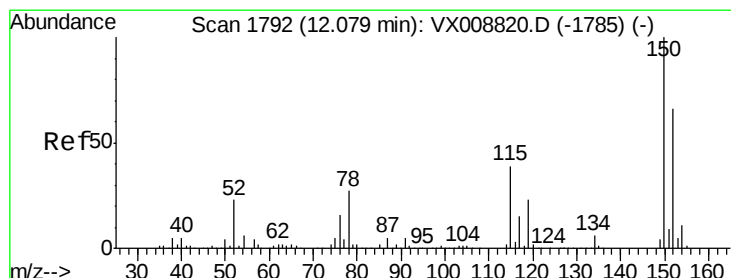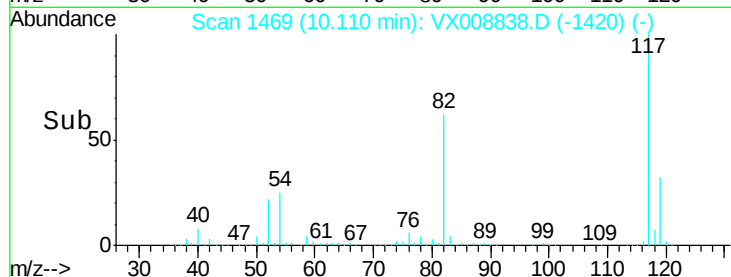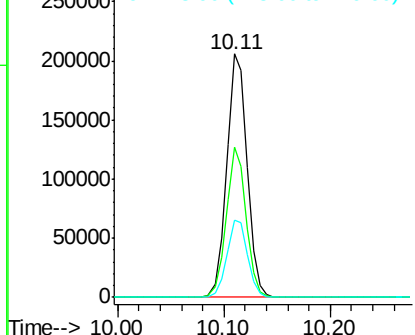

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX008838.D
Acq: 11 Apr 2019 05:01

Tgt Ion:152 Resp: 115057
Ion Ratio Lower Upper
152 100
115 60.6 43.5 130.5
150 158.3 0.0 348.8

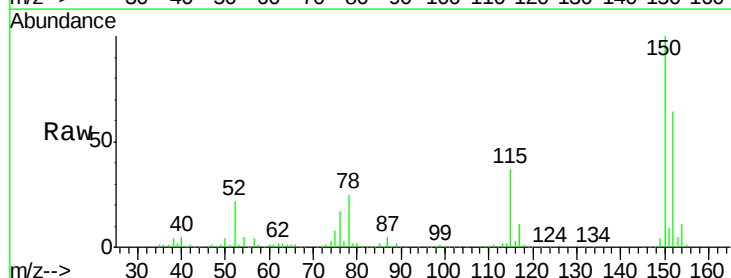

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

