


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041019\
Data File : VX008794.D
Acq On : 10 Apr 2019 09:04
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260
Last Update : Thu Apr 04 04:47:41 2019

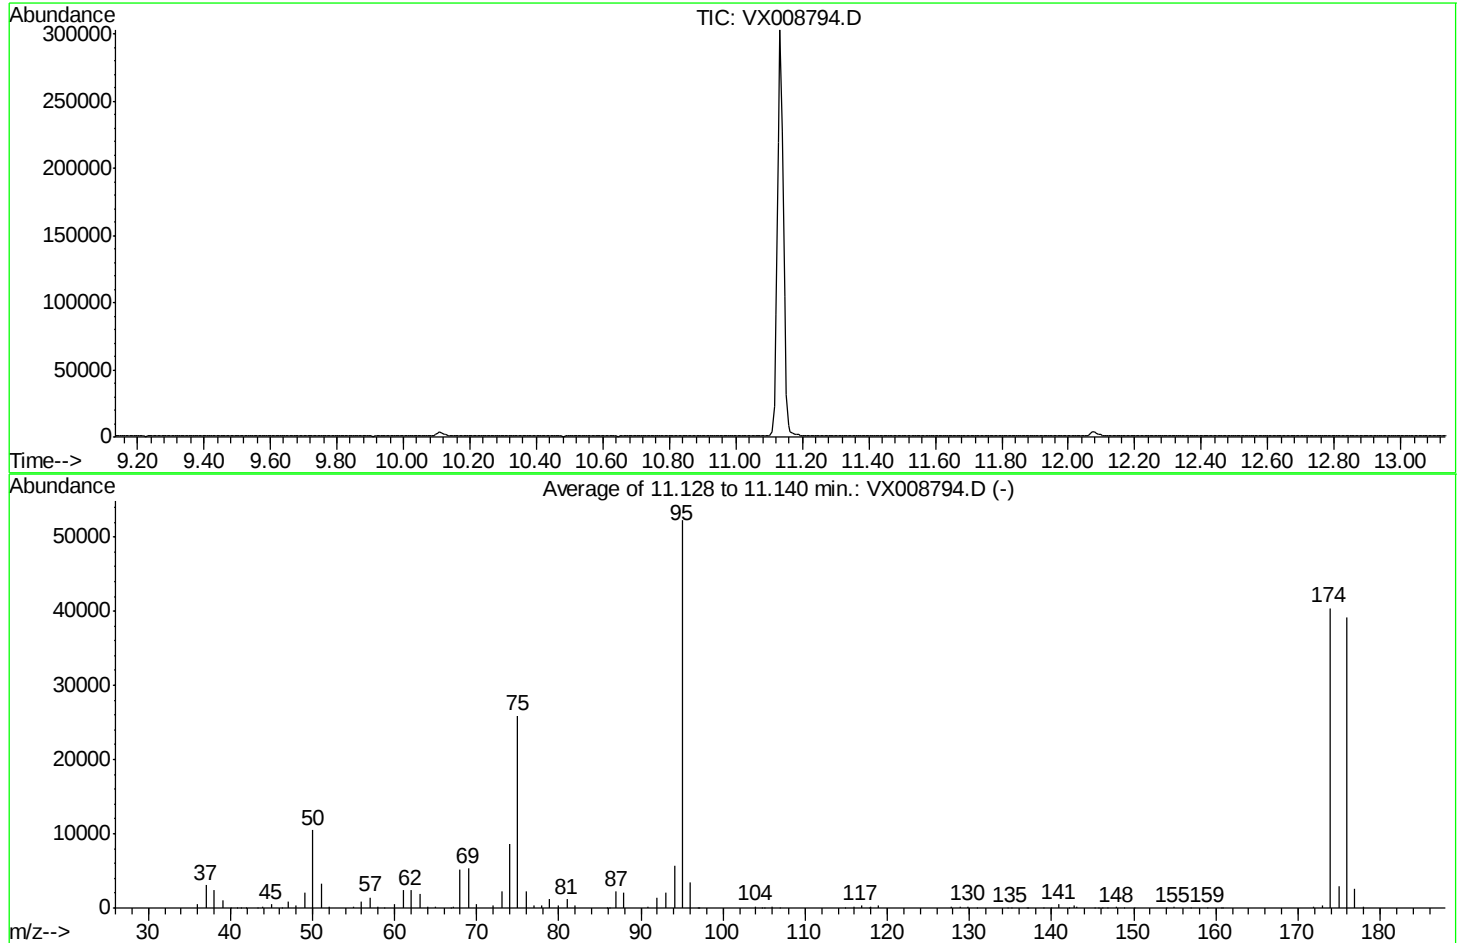

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	10462	PASS
75	95	30	60	49.7	25938	PASS
95	95	100	100	100.0	52232	PASS
96	95	5	9	6.5	3383	PASS
173	174	0.00	2	0.9	350	PASS
174	95	50	100	77.4	40445	PASS
175	174	5	9	7.2	2928	PASS
176	174	95	101	96.6	39074	PASS
177	176	5	9	6.7	2635	PASS