


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX041019\
Data File : VX008819.D
Acq On : 10 Apr 2019 20:59
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Title : SW846 8260
Last Update : Thu Apr 04 04:47:41 2019

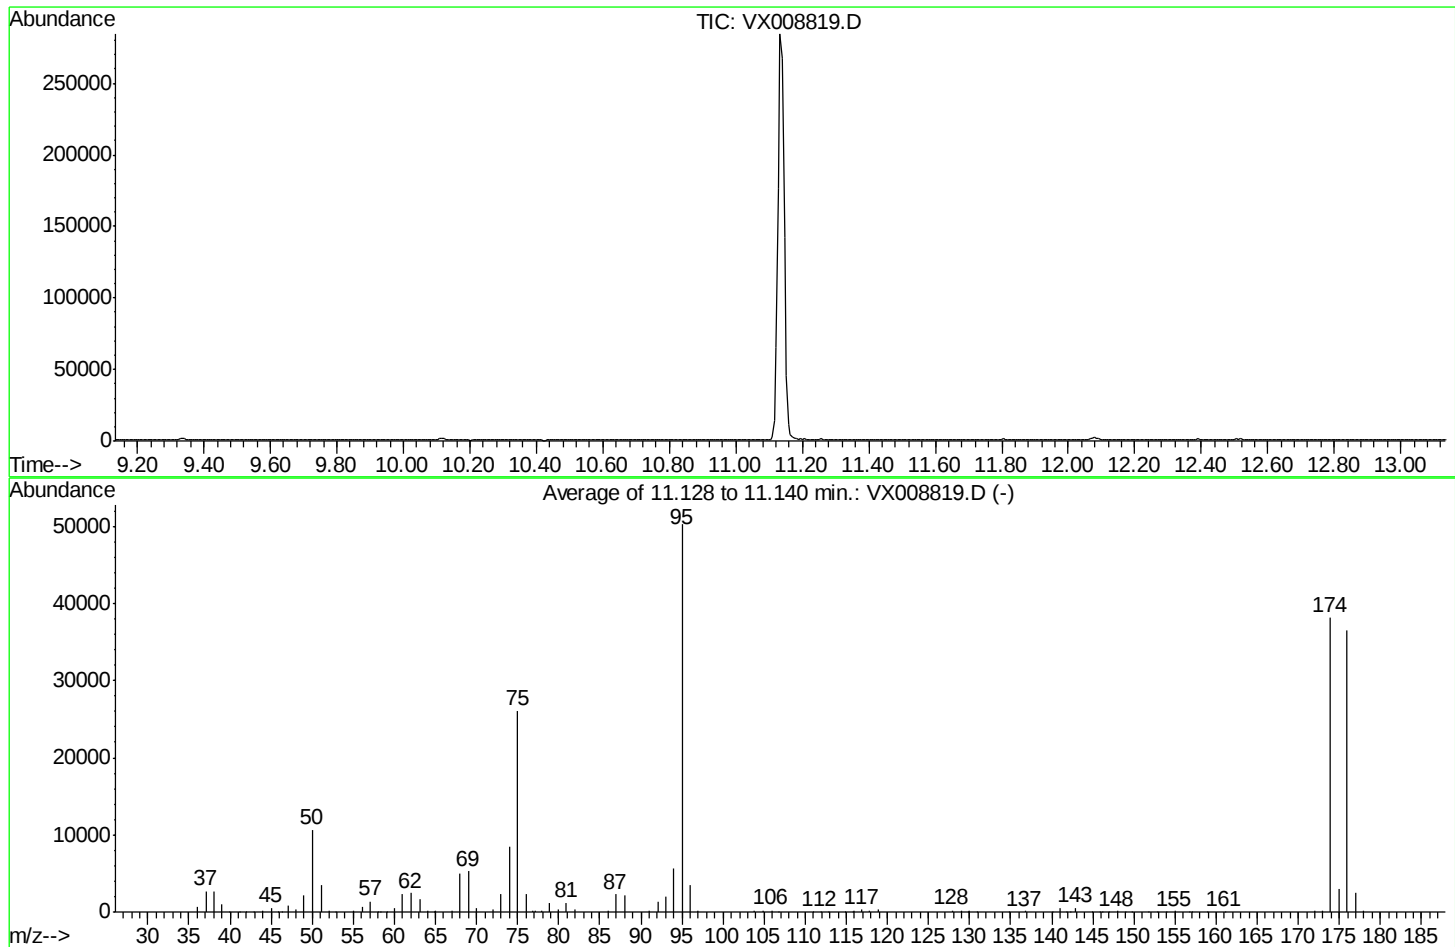

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	10696	PASS
75	95	30	60	51.8	26056	PASS
95	95	100	100	100.0	50256	PASS
96	95	5	9	6.8	3439	PASS
173	174	0.00	2	0.3	123	PASS
174	95	50	100	75.9	38125	PASS
175	174	5	9	8.0	3054	PASS
176	174	95	101	95.7	36490	PASS
177	176	5	9	6.9	2536	PASS