


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX041020\
 Data File : VX015610.D
 Acq On : 10 Apr 2020 10:51
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X032720W.M
 Title : SW846 8260
 Last Update : Fri Mar 27 09:35:51 2020

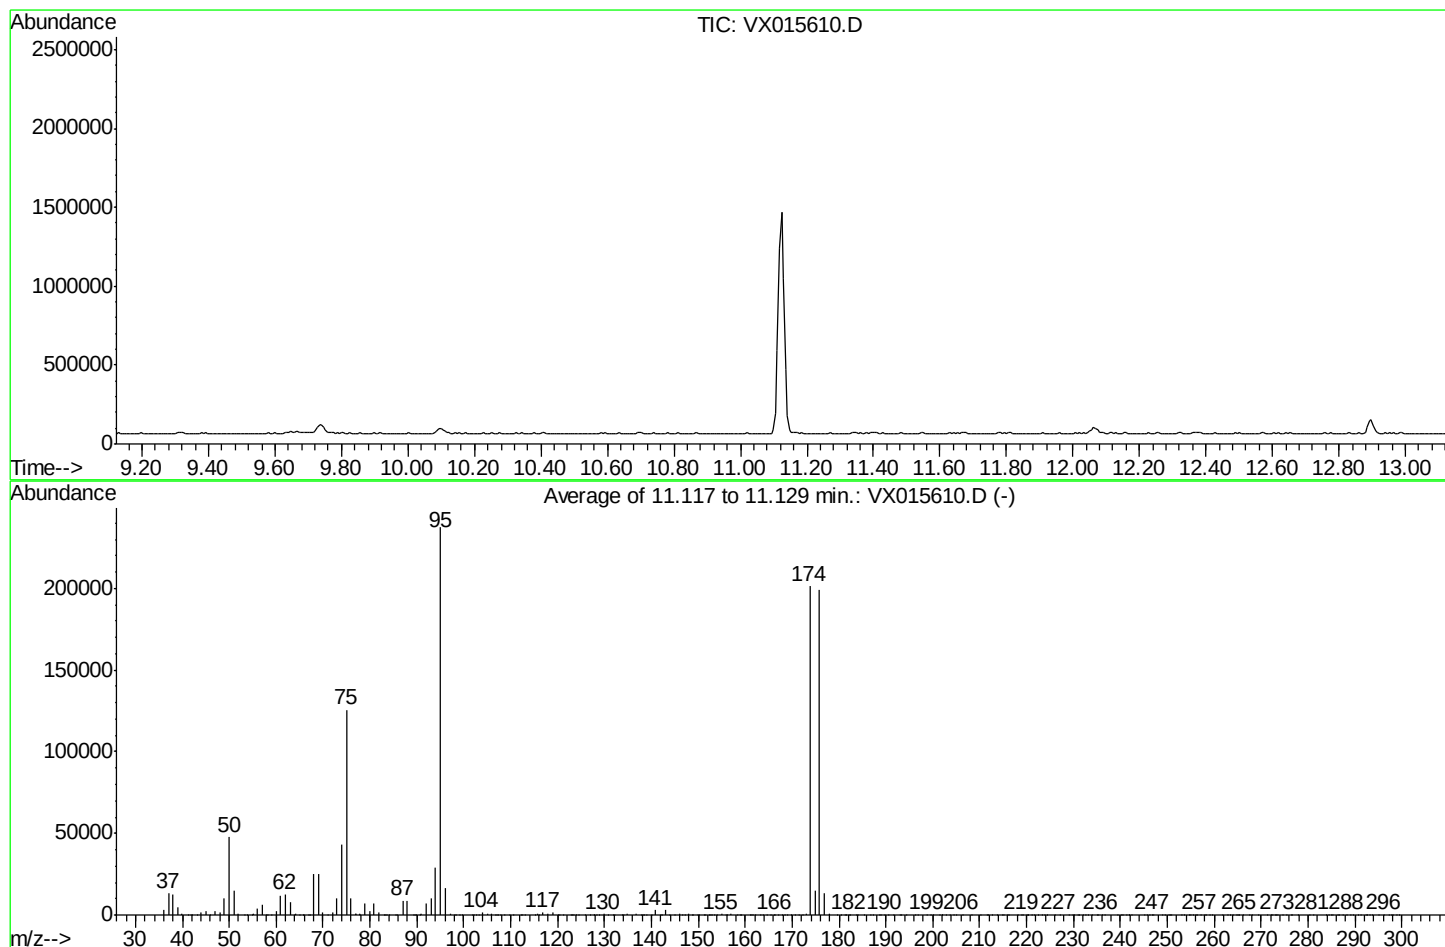

AutoFind: Scans 1678, 1679, 1680; Background Corrected with Scan 1671

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	47773	PASS
75	95	30	60	52.9	125664	PASS
95	95	100	100	100.0	237440	PASS
96	95	5	9	6.8	16112	PASS
173	174	0.00	2	0.3	654	PASS
174	95	50	100	84.7	201148	PASS
175	174	5	9	7.4	14849	PASS
176	174	95	101	98.9	198838	PASS
177	176	5	9	6.8	13583	PASS