

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
 Data File : VX034993.D
 Acq On : 10 Apr 2023 13:21
 Operator : JC/MD
 Sample : VX0410WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK618

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
 Title : VOC Analysis

Signal : TIC: VX034993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV3	2024	2537	0.15%	0.020%
2	1.368	42	46	58	rBV	216434	236626	13.65%	1.820%
3	1.672	91	96	110	rBV	161046	222732	12.85%	1.714%
4	2.306	194	200	212	rBV	389171	603869	34.83%	4.646%
5	2.514	229	234	240	rVB	3086	5363	0.31%	0.041%
6	2.605	247	249	251	rBV2	305	302	0.02%	0.002%
7	2.703	263	265	267	rBV2	429	373	0.02%	0.003%
8	2.788	274	279	287	rVB2	6762	12592	0.73%	0.097%
9	3.099	324	330	332	rBV4	2687	4931	0.28%	0.038%
10	3.312	361	365	366	rBV2	286	320	0.02%	0.002%
11	3.447	384	387	390	rVB2	357	377	0.02%	0.003%
12	3.495	390	395	396	rBV3	407	378	0.02%	0.003%
13	3.605	408	413	421	rVB4	983	2037	0.12%	0.016%
14	3.776	439	441	445	rVB	338	377	0.02%	0.003%
15	3.873	454	457	462	rBV2	182	308	0.02%	0.002%
16	3.989	473	476	477	rBV3	493	394	0.02%	0.003%
17	4.160	502	504	507	rBV2	302	309	0.02%	0.002%
18	4.282	522	524	527	rBV2	260	305	0.02%	0.002%
19	4.373	537	539	542	rBV3	312	357	0.02%	0.003%
20	4.465	545	554	570	rBV	102282	330711	19.07%	2.544%
21	4.678	587	589	591	rVB	460	409	0.02%	0.003%
22	4.897	620	625	626	rBV4	665	799	0.05%	0.006%
23	5.050	636	650	670	rBV	227271	691307	39.87%	5.318%
24	5.233	678	680	684	rVB3	490	494	0.03%	0.004%
25	5.324	692	695	697	rBV2	276	293	0.02%	0.002%
26	5.385	699	705	711	rBV4	1199	3110	0.18%	0.024%
27	5.471	714	719	726	rVB4	1556	3440	0.20%	0.026%
28	5.666	747	751	759	rVB3	957	2011	0.12%	0.015%
29	5.964	787	800	820	rBV2	572239	1733776	100.00%	13.338%
30	6.281	850	852	855	rVB2	344	375	0.02%	0.003%
31	6.464	876	882	883	rBV2	449	546	0.03%	0.004%
32	6.489	883	886	888	rVB2	347	324	0.02%	0.002%
33	6.757	919	930	953	rBV	476590	1134309	65.42%	8.727%
34	7.117	983	989	998	rVB7	6284	15499	0.89%	0.119%
35	7.306	1011	1020	1036	rBV	353219	791180	45.63%	6.087%
36	7.745	1089	1092	1093	rBV2	564	402	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
 Data File : VX034993.D
 Acq On : 10 Apr 2023 13:21
 Operator : JC/MD
 Sample : VX0410WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK618

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
 Title : VOC Analysis

37	7.824	1101	1105	1110	rVB3	713	1218	0.07%	0.009%
38	7.952	1121	1126	1130	rBV3	1293	2390	0.14%	0.018%
39	8.159	1157	1160	1162	rBV3	245	288	0.02%	0.002%
40	8.324	1180	1187	1198	rBV	224534	365315	21.07%	2.810%
41	8.574	1225	1228	1233	rBV6	1824	2708	0.16%	0.021%
42	8.647	1233	1240	1249	rBV	892839	1386378	79.96%	10.666%
43	8.842	1270	1272	1273	rBV	394	272	0.02%	0.002%
44	8.860	1273	1275	1278	rVB4	306	355	0.02%	0.003%
45	8.952	1284	1290	1301	rBV	146726	233001	13.44%	1.793%
46	9.153	1320	1323	1327	rBV4	1554	2560	0.15%	0.020%
47	9.275	1338	1343	1350	rBV4	3365	4864	0.28%	0.037%
48	9.384	1356	1361	1377	rBV	486010	708136	40.84%	5.448%
49	9.610	1394	1398	1403	rVB3	931	1723	0.10%	0.013%
50	9.756	1420	1422	1424	rVB2	388	313	0.02%	0.002%
51	9.793	1424	1428	1431	rBV2	434	563	0.03%	0.004%
52	10.055	1465	1471	1485	rBV	925776	1291201	74.47%	9.934%
53	10.195	1490	1494	1500	rVV	4382	6268	0.36%	0.048%
54	10.244	1500	1502	1507	rVB3	749	941	0.05%	0.007%
55	10.305	1507	1512	1520	rBV2	4486	7047	0.41%	0.054%
56	10.403	1526	1528	1531	rVB2	371	319	0.02%	0.002%
57	10.482	1539	1541	1543	rVB2	397	280	0.02%	0.002%
58	10.506	1543	1545	1548	rBV	262	324	0.02%	0.002%
59	10.610	1560	1562	1564	rVV2	374	292	0.02%	0.002%
60	10.646	1564	1568	1577	rVB4	4953	10404	0.60%	0.080%
61	10.756	1582	1586	1588	rBV2	186	315	0.02%	0.002%
62	10.805	1591	1594	1599	rVB3	547	667	0.04%	0.005%
63	10.896	1607	1609	1611	rBV	251	293	0.02%	0.002%
64	10.963	1615	1620	1625	rVB2	4134	5602	0.32%	0.043%
65	11.189	1652	1657	1671	rBV	556279	729754	42.09%	5.614%
66	11.396	1690	1691	1696	rVB3	370	401	0.02%	0.003%
67	11.451	1696	1700	1705	rBV	4494	5761	0.33%	0.044%
68	11.518	1709	1711	1714	rBV2	341	396	0.02%	0.003%
69	11.683	1735	1738	1740	rBV2	331	301	0.02%	0.002%
70	11.707	1740	1742	1745	rVV2	789	719	0.04%	0.006%
71	11.750	1746	1749	1754	rVV	3493	4904	0.28%	0.038%
72	11.921	1776	1777	1781	rVB2	373	421	0.02%	0.003%
73	11.975	1781	1786	1788	rBV3	4290	5630	0.32%	0.043%
74	12.018	1788	1793	1805	rVV	927578	1209242	69.75%	9.303%
75	12.317	1837	1842	1858	rBV	936964	1172793	67.64%	9.023%
76	12.530	1875	1877	1878	rBV2	417	297	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
 Data File : VX034993.D
 Acq On : 10 Apr 2023 13:21
 Operator : JC/MD
 Sample : VX0410WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK618

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
 Title : VOC Analysis

77	12.823	1924	1925	1930	rVB2	263	295	0.02%	0.002%
78	12.878	1930	1934	1936	rBV2	254	483	0.03%	0.004%
79	12.945	1942	1945	1947	rBV3	673	777	0.04%	0.006%
80	13.006	1953	1955	1958	rBV3	211	261	0.02%	0.002%
81	13.116	1968	1973	1978	rBV3	3610	4903	0.28%	0.038%
82	13.402	2018	2020	2021	rBV2	361	294	0.02%	0.002%
83	13.518	2037	2039	2041	rVV3	348	285	0.02%	0.002%
84	13.591	2047	2051	2057	rBV6	3899	5711	0.33%	0.044%
85	13.695	2064	2068	2071	rBV2	472	594	0.03%	0.005%
86	13.780	2078	2082	2087	rVB3	4477	5976	0.34%	0.046%
87	13.902	2100	2102	2104	rBV2	361	402	0.02%	0.003%
88	13.963	2108	2112	2117	rVV	4506	5255	0.30%	0.040%
89	14.128	2138	2139	2141	rBV	398	290	0.02%	0.002%
90	14.359	2173	2177	2178	rBV	281	368	0.02%	0.003%
91	14.445	2190	2191	2195	rBV2	305	285	0.02%	0.002%
92	14.579	2210	2213	2215	rVB	397	466	0.03%	0.004%
93	14.597	2215	2216	2219	rBV2	538	428	0.02%	0.003%
94	14.640	2219	2223	2224	rBV2	374	439	0.03%	0.003%
95	14.737	2237	2239	2242	rVB2	462	390	0.02%	0.003%
96	14.902	2264	2266	2268	rBV	576	330	0.02%	0.003%
97	14.957	2274	2275	2278	rBV2	570	496	0.03%	0.004%
98	15.804	2412	2414	2417	rVB3	807	489	0.03%	0.004%
99	16.005	2445	2447	2448	rBV2	721	361	0.02%	0.003%
100	16.493	2525	2527	2528	rBV2	868	583	0.03%	0.004%




Sum of corrected areas: 12998289

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
Data File : VX034993.D
Acq On : 10 Apr 2023 13:21
Operator : JC/MD
Sample : VX0410WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK618

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

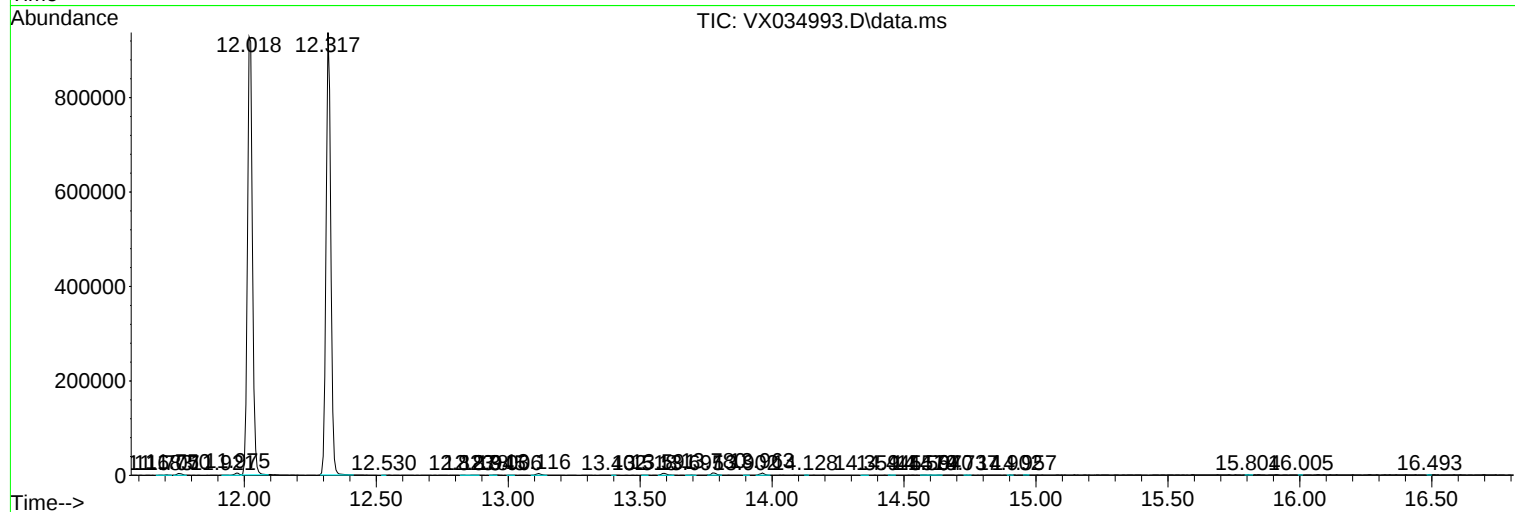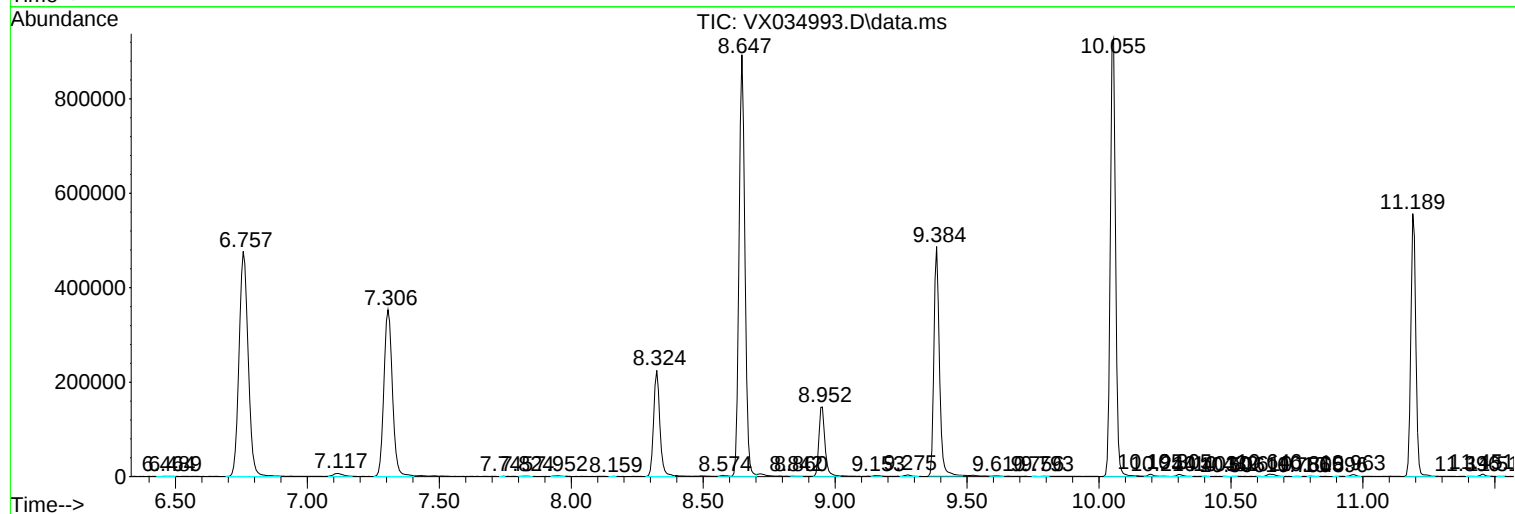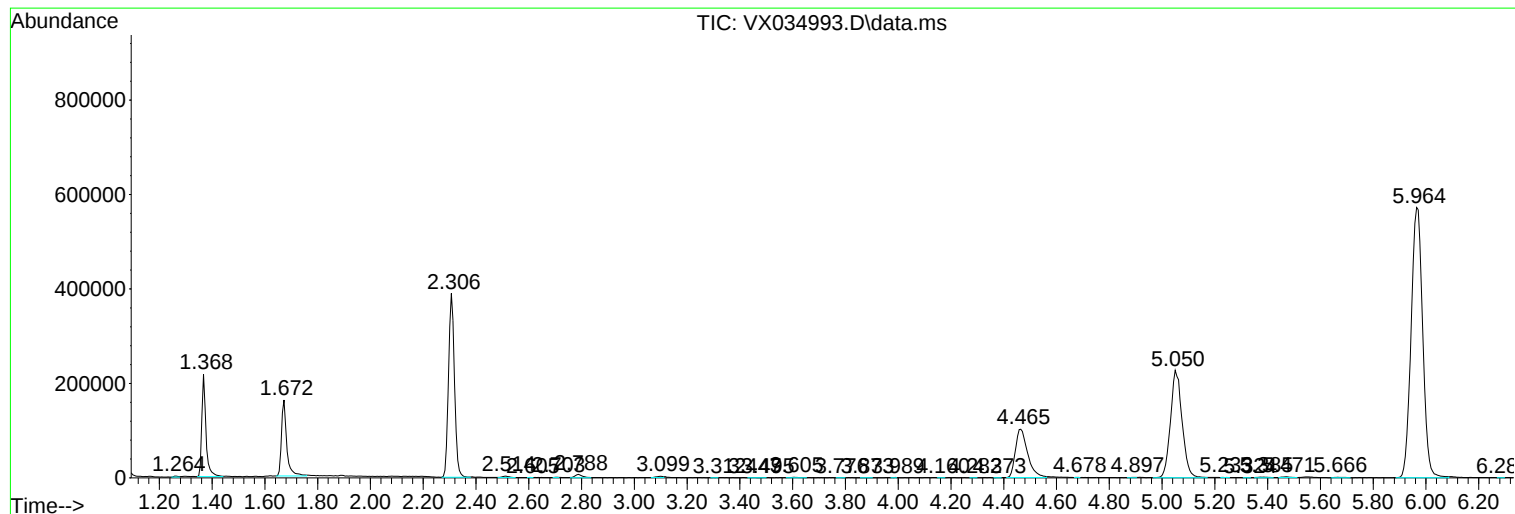

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
Data File : VX034993.D
Acq On : 10 Apr 2023 13:21
Operator : JC/MD
Sample : VX0410WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK618

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
Data File : VX034993.D
Acq On : 10 Apr 2023 13:21
Operator : JC/MD
Sample : VX0410WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK618

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------