
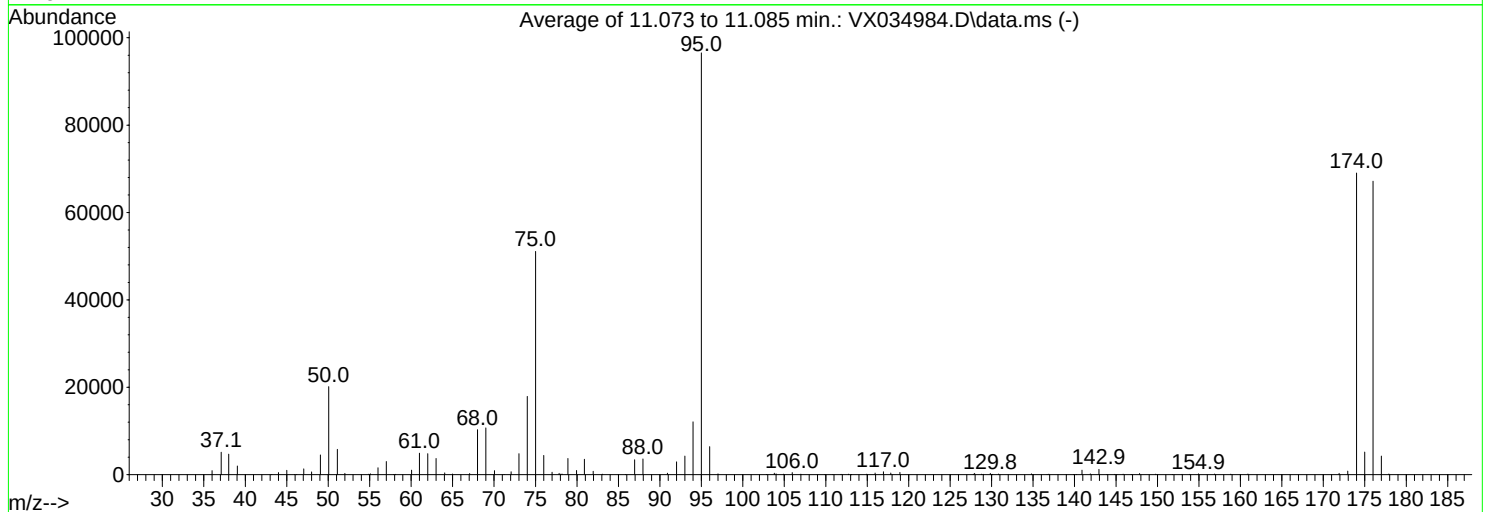


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041023\
Data File : VX034984.D
Acq On : 10 Apr 2023 08:48
Operator : JC/MD
Sample : BFB621
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB621

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041023WMA.M
Title : VOC Analysis
Last Update : Wed Apr 12 01:54:54 2023

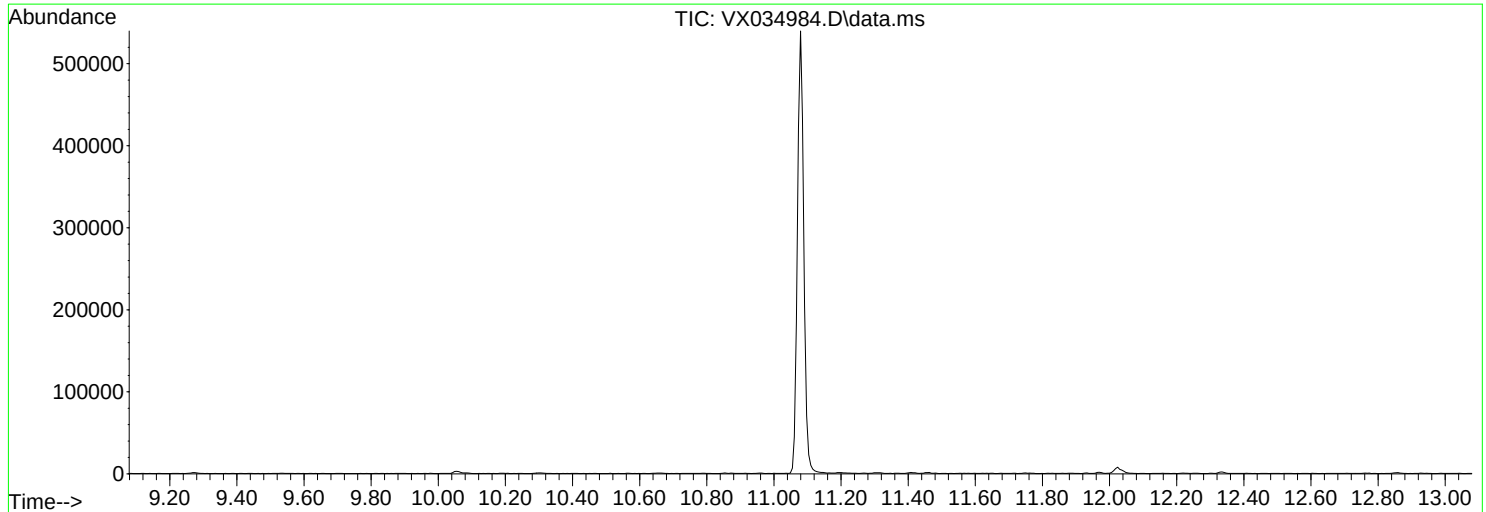

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	20157	PASS
75	95	30	80	52.9	51107	PASS
95	95	100	100	100.0	96544	PASS
96	95	5	9	6.6	6394	PASS
173	174	0.00	2	1.2	810	PASS
174	95	50	120	71.5	69045	PASS
175	174	5	9	7.5	5177	PASS
176	174	95	101	97.3	67181	PASS
177	176	5	9	6.3	4238	PASS

m/z	Abundance
35.90	114.0
38.00	77.0
40.00	243.0
43.90	320.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

m/z	Abundance
36.10	1007.0
37.10	4917.0
38.00	4986.0
39.10	1835.0
40.00	247.0
43.20	55.0
44.00	740.0
45.00	1036.0
46.20	55.0
47.10	1066.0
48.00	661.0
49.00	4279.0
50.10	20072.0
51.10	5683.0
52.10	350.0
54.90	331.0
56.10	1538.0
57.00	3341.0
57.90	105.0
60.00	959.0
61.00	4696.0
62.00	5014.0
63.00	3457.0
64.00	394.0
65.00	189.0
67.10	228.0
68.00	10714.0
69.00	10374.0
70.10	1022.0
72.00	735.0
73.00	4580.0
74.00	17576.0
75.00	48744.0
76.00	4564.0
77.10	498.0
77.90	479.0
78.20	443.0
78.90	3773.0
80.00	887.0
80.90	3506.0
81.90	768.0
83.00	74.0
85.80	97.0
86.90	2908.0
87.90	3604.0
90.90	389.0
92.00	2798.0
93.00	3690.0
94.00	11104.0
95.00	88328.0
96.00	6623.0
97.00	195.0
103.80	475.0
106.00	420.0
107.00	51.0
111.80	77.0
113.00	52.0
114.90	109.0
116.00	357.0
117.00	480.0
117.90	329.0
118.90	513.0
127.80	337.0
128.80	154.0
130.10	267.0
130.80	168.0
134.80	194.0
136.70	128.0
139.00	77.0
140.20	69.0
140.90	893.0
142.00	190.0
142.90	1082.0
143.90	92.0
144.90	148.0
145.80	111.0
147.90	198.0
149.70	56.0
151.80	50.0
152.90	50.0
153.90	64.0
155.00	196.0
157.00	130.0
158.90	104.0
160.90	79.0
172.10	215.0
172.90	663.0
174.00	56704.0
175.00	4525.0
176.00	52616.0
177.00	3648.0
177.90	218.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

m/z	Abundance
36.10	1124.0
37.10	6245.0
38.00	5079.0
39.10	2413.0
40.00	186.0
43.20	67.0
44.10	873.0
45.00	1299.0
45.90	89.0
46.20	78.0
47.10	1869.0
48.00	545.0
49.10	5352.0
50.00	23624.0
51.10	6717.0
52.00	298.0
55.10	286.0
56.00	1856.0
57.00	3470.0
58.10	173.0
60.10	1145.0
61.00	6062.0
62.00	5715.0
63.00	4273.0
64.00	488.0
65.00	213.0
66.90	313.0
68.00	11729.0
69.00	12703.0
70.00	887.0
72.10	753.0
73.00	5817.0
74.00	20704.0
75.00	59632.0
76.00	5067.0
77.00	628.0
77.80	363.0
78.90	4067.0
79.90	1137.0
80.90	4105.0
82.00	919.0
83.10	137.0
85.90	79.0
86.90	4140.0
87.90	3847.0
91.00	360.0
92.00	3402.0
93.00	4869.0
94.00	13962.0
95.00	113792.0
96.00	7425.0
97.00	232.0
102.90	87.0
104.00	596.0
104.90	148.0
105.90	713.0
107.00	100.0
109.90	130.0
110.80	55.0
111.90	74.0
112.70	147.0
115.00	114.0
115.90	389.0
117.00	781.0
117.90	504.0
119.00	557.0
128.00	436.0
129.00	229.0
129.80	397.0
130.80	151.0
134.70	176.0
134.90	171.0
136.90	183.0
139.00	61.0
139.90	106.0
140.90	1169.0
141.90	219.0
143.00	1319.0
143.90	57.0
144.80	129.0
145.90	138.0
146.80	65.0
147.90	331.0
149.80	146.0
151.80	53.0
153.00	71.0
153.80	78.0
154.90	192.0
156.90	221.0
158.90	170.0
160.90	172.0
171.90	445.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

173.00	809.0
174.00	77904.0
175.00	6159.0
176.00	77952.0
177.00	5052.0
177.90	100.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621

m/z	Abundance
36.00	977.0
37.10	4206.0
38.00	4233.0
39.00	1645.0
40.10	265.0
44.00	805.0
45.00	613.0
46.00	84.0
47.00	988.0
48.00	667.0
49.00	3874.0
50.00	16776.0
51.10	4980.0
51.90	190.0
55.10	303.0
55.90	1383.0
57.00	2257.0
58.10	93.0
60.00	1034.0
61.00	3925.0
62.00	3723.0
63.00	3376.0
64.10	344.0
64.90	96.0
67.10	231.0
68.00	8438.0
69.00	8991.0
70.00	818.0
71.20	63.0
72.00	522.0
73.00	4042.0
74.00	15488.0
75.00	44944.0
76.00	3581.0
76.90	497.0
78.00	311.0
78.90	3285.0
79.90	861.0
80.90	2971.0
81.90	593.0
83.00	143.0
87.00	3190.0
88.00	3377.0
90.80	282.0
92.00	2633.0
93.00	4165.0
94.00	11166.0
95.00	87512.0
96.00	5133.0
96.90	108.0
102.80	70.0
103.80	479.0
104.90	143.0
105.90	350.0
107.00	156.0
110.90	93.0
111.90	61.0
112.80	166.0
114.90	94.0
116.00	369.0
116.90	677.0
117.80	302.0
118.90	525.0
127.90	401.0
128.80	152.0
129.90	459.0
130.90	153.0
135.00	176.0
136.90	202.0
139.90	58.0
140.90	1064.0
141.80	102.0
142.90	1280.0
145.10	123.0
145.80	142.0
146.90	77.0
147.80	206.0
149.90	96.0
152.90	80.0
154.00	62.0
155.00	212.0
156.80	117.0
158.70	103.0
160.90	178.0
171.80	213.0
173.00	958.0
174.00	72528.0
175.00	4846.0
176.00	70976.0
177.00	4015.0
178.00	100.0

Instrument :
MSVOA_X
ClientSampleId :
BFB621