
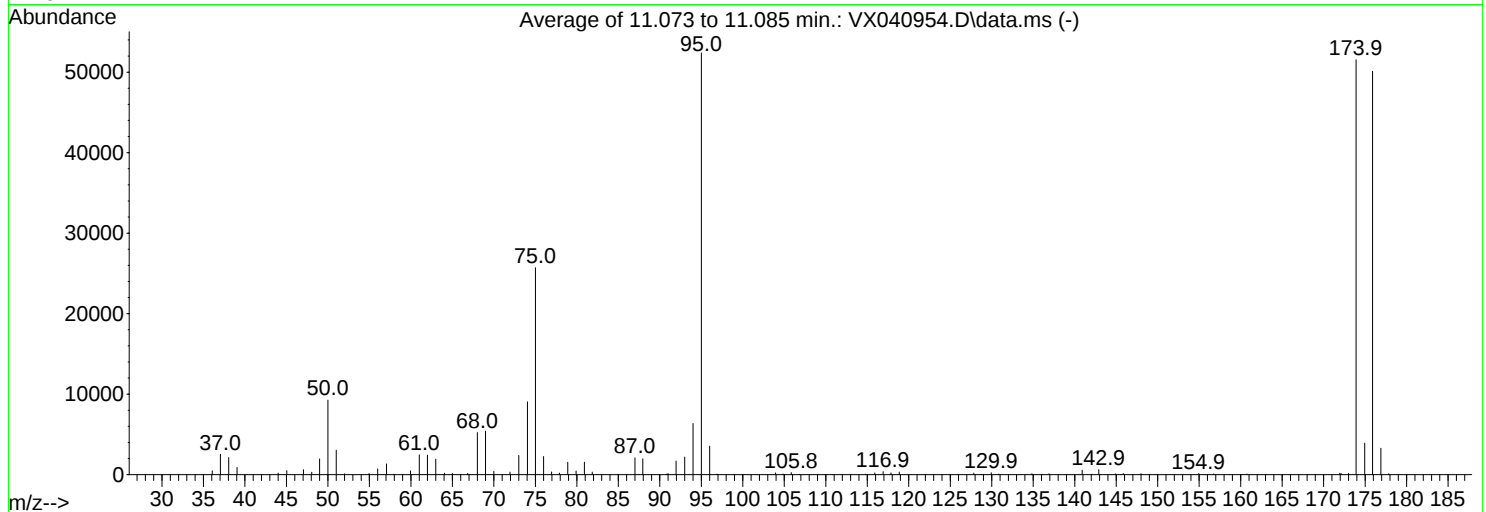


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041024\
Data File : VX040954.D
Acq On : 10 Apr 2024 14:43
Operator : JC/MD
Sample : BFB669
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB669

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041024WMA.M
Title : VOC Analysis
Last Update : Thu Apr 11 05:36:34 2024

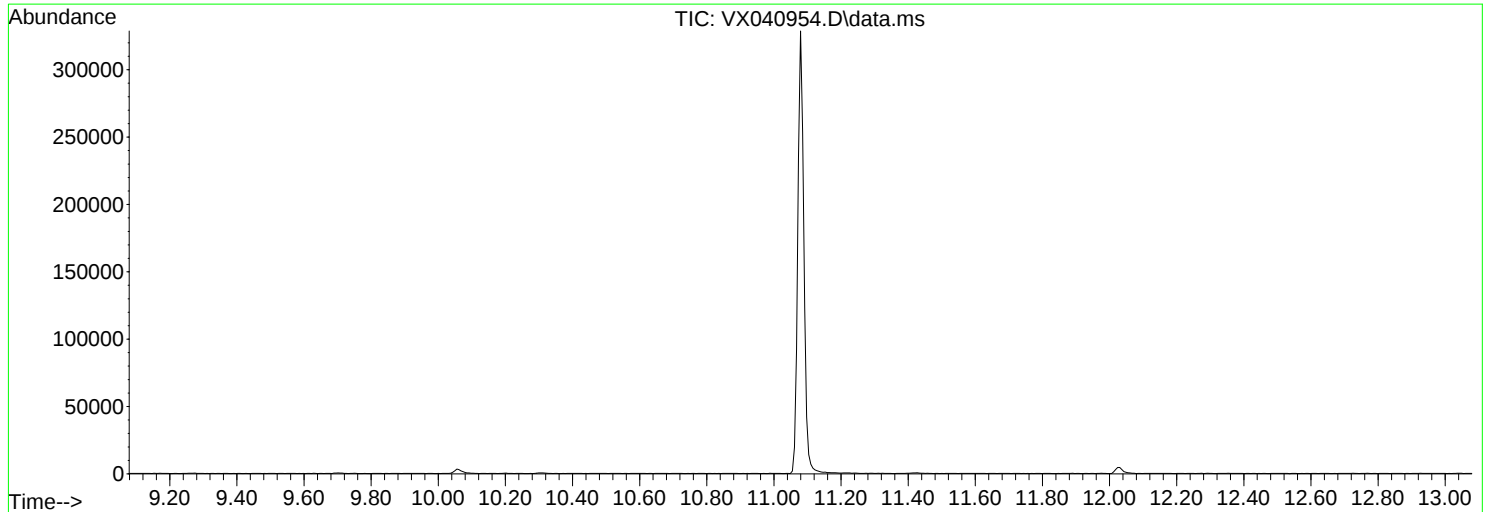

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	9257	PASS
75	95	30	80	49.0	25693	PASS
95	95	100	100	100.0	52400	PASS
96	95	5	9	6.8	3545	PASS
173	174	0.00	2	0.3	169	PASS
174	95	50	120	98.4	51541	PASS
175	174	5	9	7.6	3927	PASS
176	174	95	101	97.2	50115	PASS
177	176	5	9	6.6	3291	PASS

m/z	Abundance
40.10	245.0
44.00	180.0

Instrument :
MSVOA_X
ClientSampleId :
BFB669

m/z	Abundance
36.00	514.0
37.10	2500.0
38.10	2325.0
39.00	914.0
40.00	258.0
44.00	361.0
45.00	432.0
47.00	647.0
48.00	324.0
49.00	2027.0
50.00	8785.0
51.00	2962.0
52.10	69.0
55.00	159.0
55.90	731.0
57.00	1384.0
57.90	54.0
60.00	372.0
61.00	2608.0
62.00	2571.0
63.00	1727.0
64.10	219.0
65.00	136.0
66.90	156.0
68.00	4968.0
69.00	4769.0
70.10	448.0
71.90	415.0
73.00	2129.0
74.00	8571.0
75.00	24632.0
76.00	2077.0
76.90	281.0
78.00	199.0
78.90	1401.0
79.90	480.0
80.90	1398.0
81.90	285.0
87.00	1781.0
87.90	1802.0
90.80	202.0
92.00	1478.0
93.00	1977.0
94.00	5737.0
95.00	46968.0
96.00	3302.0
96.90	69.0
103.90	210.0
104.80	80.0
105.90	248.0
114.80	108.0
116.00	208.0
116.90	319.0
117.80	175.0
118.90	269.0
127.80	190.0
128.70	61.0
129.10	78.0
129.90	232.0
131.00	78.0
134.90	89.0
136.90	83.0
140.90	505.0
143.00	497.0
144.90	67.0
145.80	109.0
148.00	141.0
154.90	124.0
156.90	64.0
160.70	79.0
172.00	150.0
172.10	150.0
173.00	508.0
173.90	38712.0
174.90	3090.0
175.90	37632.0
176.90	2741.0
177.90	75.0

Instrument :
MSVOA_X
ClientSampleId :
BFB669

m/z	Abundance
36.10	548.0
37.00	3163.0
38.00	2442.0
39.10	1080.0
39.90	148.0
44.00	510.0
45.00	689.0
47.10	678.0
48.10	307.0
49.00	2409.0
50.00	10965.0
51.00	3759.0
52.00	145.0
54.90	130.0
56.00	894.0
57.10	1374.0
58.00	68.0
59.90	555.0
61.00	2885.0
62.00	2894.0
63.00	2471.0
64.00	162.0
65.10	194.0
66.90	207.0
68.00	6316.0
69.00	6818.0
70.00	463.0
72.00	308.0
73.00	3054.0
74.00	10868.0
75.00	30392.0
76.00	2752.0
76.90	414.0
77.90	234.0
78.90	1879.0
79.90	502.0
80.90	1876.0
81.80	395.0
87.00	2635.0
88.00	2347.0
91.00	257.0
91.90	2196.0
93.00	2677.0
94.00	7965.0
95.00	63040.0
96.00	4280.0
96.90	148.0
104.00	273.0
104.80	84.0
105.90	261.0
106.80	54.0
110.80	52.0
114.80	94.0
115.90	228.0
116.90	463.0
117.80	287.0
118.80	387.0
127.90	225.0
128.90	64.0
129.90	265.0
130.80	104.0
134.80	114.0
136.90	148.0
140.80	705.0
142.10	107.0
142.90	830.0
144.90	107.0
145.90	189.0
148.00	107.0
149.90	71.0
154.90	136.0
156.70	120.0
158.70	81.0
160.80	81.0
171.90	409.0
173.90	63568.0
174.90	4632.0
175.90	60016.0
176.90	3885.0
177.90	126.0

Instrument :
MSVOA_X
ClientSampleId :
BFB669

m/z	Abundance
36.10	394.0
37.10	1903.0
38.00	1602.0
39.00	676.0
39.90	204.0
44.10	291.0
45.10	376.0
47.00	531.0
48.00	269.0
49.00	1412.0
50.00	8022.0
51.00	2412.0
51.90	92.0
54.90	127.0
56.10	557.0
57.10	1255.0
58.00	53.0
60.00	493.0
61.00	1877.0
62.00	1798.0
63.00	1564.0
64.00	179.0
64.90	157.0
66.80	130.0
67.10	111.0
68.00	4424.0
69.00	4663.0
69.90	361.0
71.90	210.0
73.00	1959.0
74.10	7679.0
75.00	22056.0
76.00	1903.0
77.00	303.0
77.80	184.0
78.90	1341.0
79.90	372.0
80.90	1366.0
81.90	255.0
87.00	1823.0
87.90	1786.0
91.00	185.0
92.00	1378.0
93.00	1908.0
94.00	5365.0
95.00	47192.0
96.00	3054.0
96.90	54.0
103.90	174.0
104.90	69.0
105.80	247.0
106.80	59.0
109.80	61.0
115.80	205.0
116.90	351.0
117.90	187.0
118.90	325.0
127.90	202.0
128.80	75.0
130.00	216.0
130.80	85.0
134.80	143.0
136.90	101.0
141.00	486.0
142.00	69.0
142.80	533.0
145.00	110.0
145.80	117.0
148.00	137.0
149.90	56.0
155.00	184.0
156.70	112.0
160.70	65.0
172.10	335.0
173.90	52344.0
175.00	4059.0
175.90	52696.0
176.90	3248.0
177.80	89.0

Instrument :
MSVOA_X
ClientSampleId :
BFB669