

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041025\
 Data File : VX045691.D
 Acq On : 10 Apr 2025 12:17
 Operator : JC/MD
 Sample : Q1748-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IB-1.5-WC

Quant Time: Apr 11 01:54:37 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	64958	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	127970	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	120693	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	51059	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	63254	53.248	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 106.500%			
35) Dibromofluoromethane	5.385	113	46047	50.715	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.440%			
50) Toluene-d8	8.647	98	162553	51.293	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.580%			
62) 4-Bromofluorobenzene	11.079	95	60763	52.639	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 105.280%			
Target Compounds						Qvalue
5) Bromomethane	1.593	94	104	0.240	ug/l #	59
6) Chloroethane	1.685	64	483	0.997	ug/l #	42
11) Tert butyl alcohol	2.959	59	283	1.773	ug/l #	72
13) Acrolein	2.239	56	79	0.359	ug/l #	72
14) Allyl chloride	2.636	41	343	0.232	ug/l #	67
16) Acetone	2.380	43	27479	56.334	ug/l	100
17) Carbon Disulfide	2.508	76	893	0.464	ug/l #	76
18) Methyl Acetate	2.703	43	1356	1.207	ug/l	97
20) Methylene Chloride	2.788	84	5546	6.073	ug/l	92
25) 2-Butanone	4.581	43	3857	5.402	ug/l	97
29) Tetrahydrofuran	5.050	42	299	0.646	ug/l #	35
31) Cyclohexane	5.544	56	1913	1.313	ug/l #	12
36) 1,1-Dichloropropene	5.544	75	6470	5.278	ug/l #	51
37) Ethyl Acetate	4.666	43	332	0.215	ug/l #	71
38) Carbon Tetrachloride	5.550	117	8043	6.071	ug/l #	15
40) Benzene	6.044	78	3468	0.926	ug/l	99
43) Isopropyl Acetate	6.355	43	8264	3.529	ug/l	98
48) Methyl methacrylate	7.793	41	35975	29.757	ug/l #	50
51) 4-Methyl-2-Pentanone	8.549	43	30996	19.969	ug/l #	47
52) Toluene	8.720	92	903	0.399	ug/l	88
53) t-1,3-Dichloropropene	8.988	75	45	2.320	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	11563	8.592	ug/l #	73
57) 1,3-Dichloropropane	9.476	76	901	0.573	ug/l #	42
59) 2-Hexanone	9.378	43	7159	6.228	ug/l #	28
74) N-amyl acetate	10.872	43	407	0.208	ug/l #	46
76) 1,2,3-Trichloropropane	11.079	75	34903	28.024	ug/l #	37
81) trans-1,4-Dichloro-2-b...	11.079	75	34903	95.111	ug/l #	1
93) 1,2,4-Trichlorobenzene	13.591	180	349	0.367	ug/l #	77
95) Naphthalene	13.780	128	1797	0.507	ug/l	95
96) 1,2,3-Trichlorobenzene	13.963	180	301	0.302	ug/l	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041025\
Data File : VX045691.D
Acq On : 10 Apr 2025 12:17
Operator : JC/MD
Sample : Q1748-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC

Quant Time: Apr 11 01:54:37 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




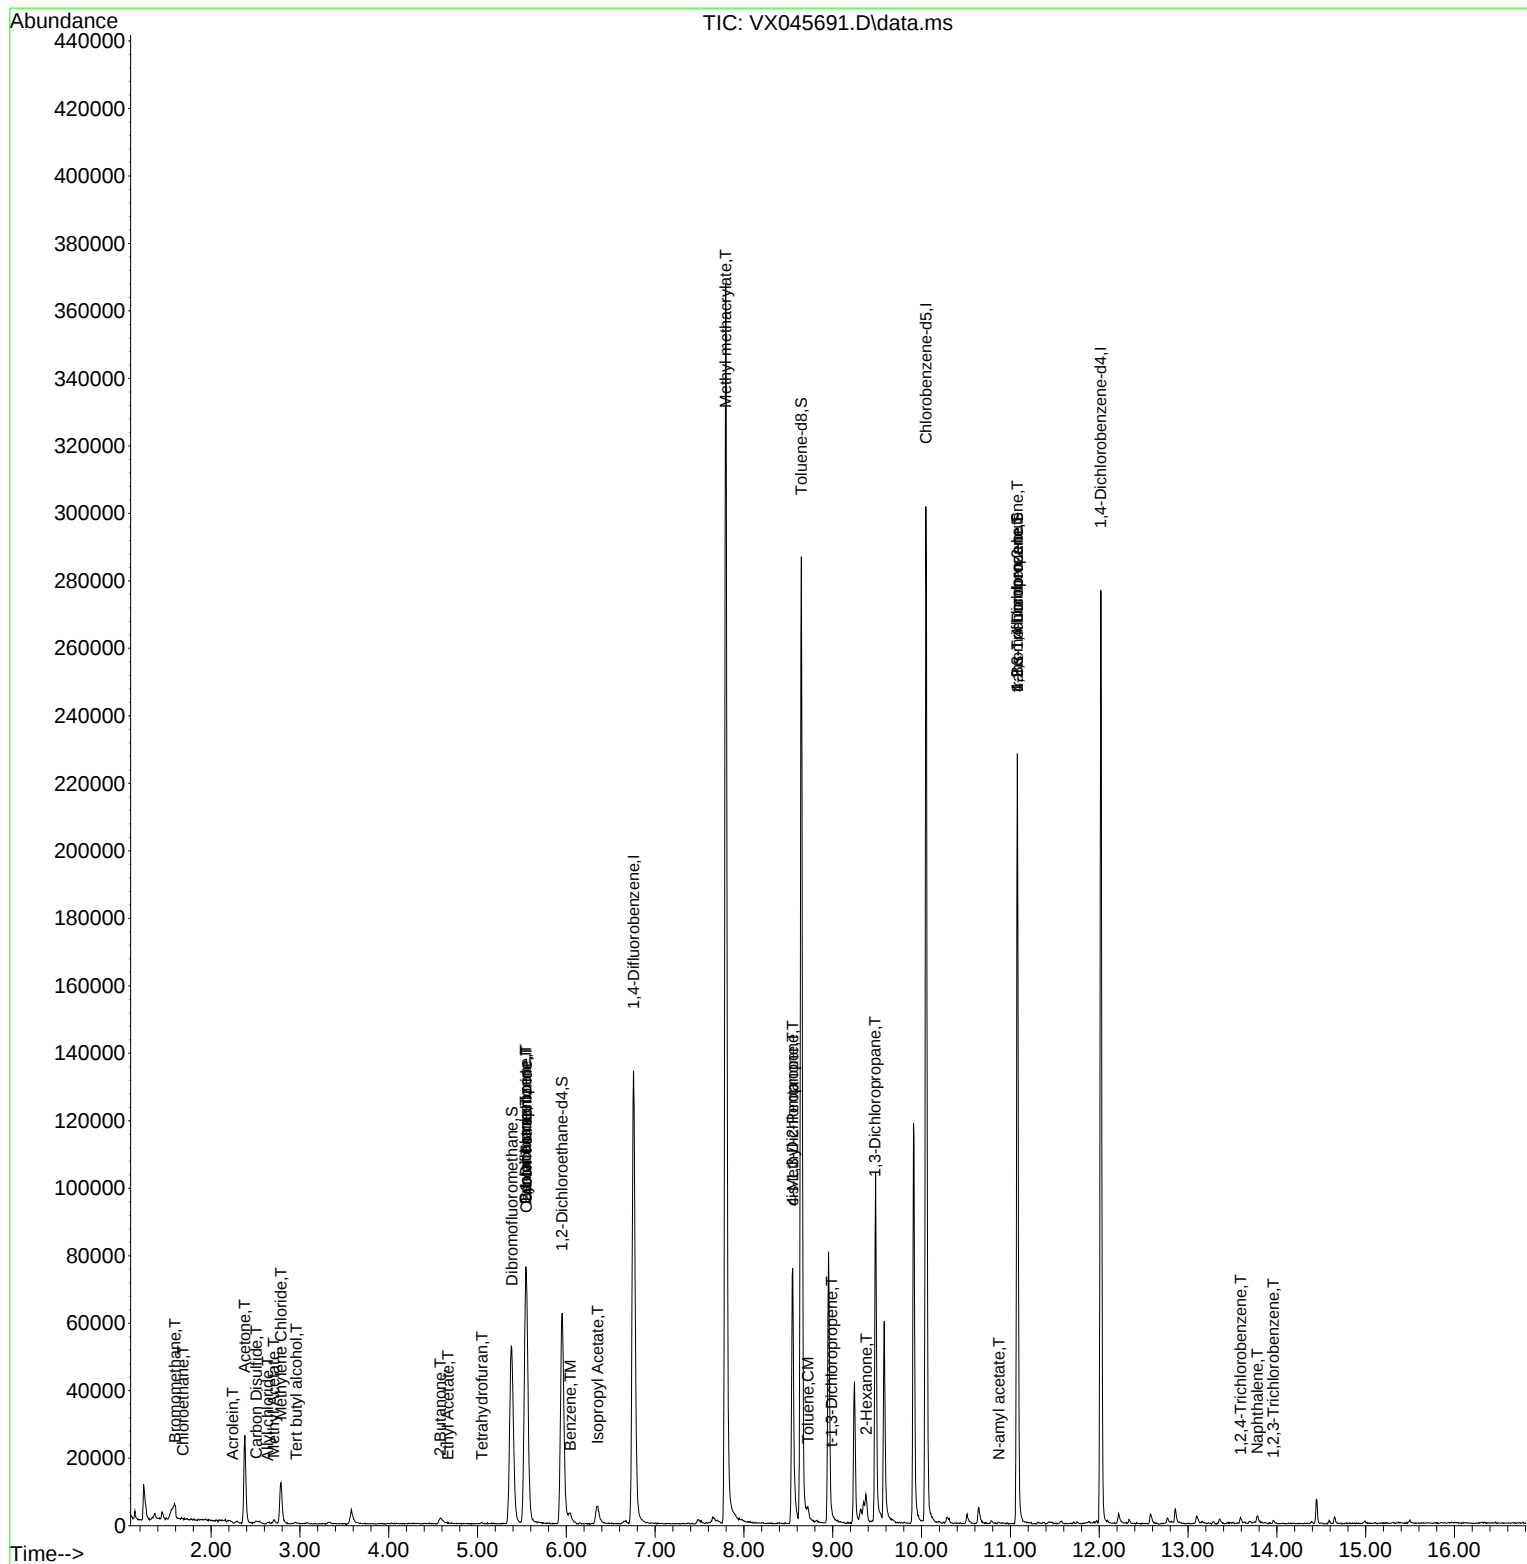




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion:168 Resp: 64958
Ion Ratio Lower Upper
168 100
99 71.6 52.3 78.5

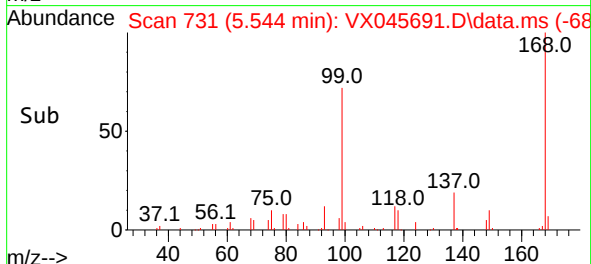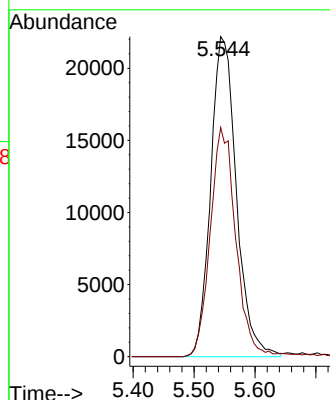

#5
Bromomethane
Concen: 0.240 ug/l
RT: 1.593 min Scan# 83
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 94 Resp: 104
Ion Ratio Lower Upper
94 100
96 53.7 74.8 112.2#


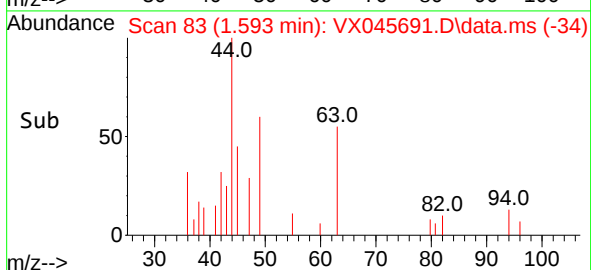
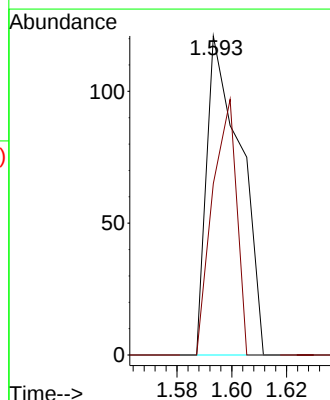



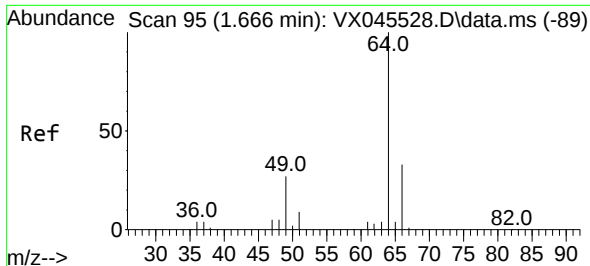

#6
Chloroethane
Concen: 0.997 ug/l
RT: 1.685 min Scan# 91
Delta R.T. 0.018 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 64 Resp: 483
Ion Ratio Lower Upper
64 100
66 0.0 26.3 39.5#

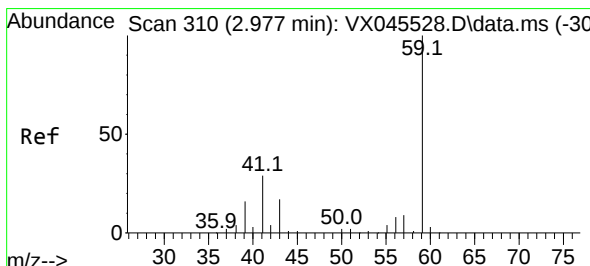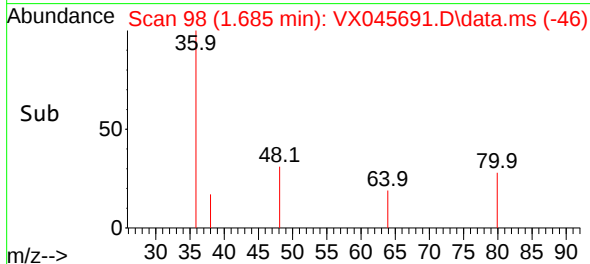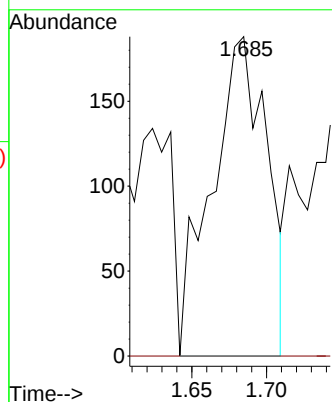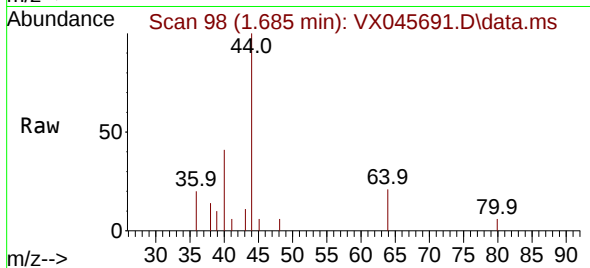

#11
Tert butyl alcohol
Concen: 1.773 ug/l
RT: 2.959 min Scan# 307
Delta R.T. -0.018 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 59 Resp: 283
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#

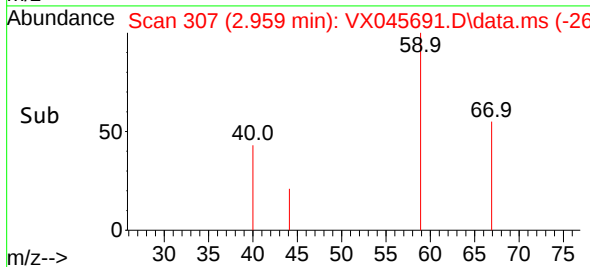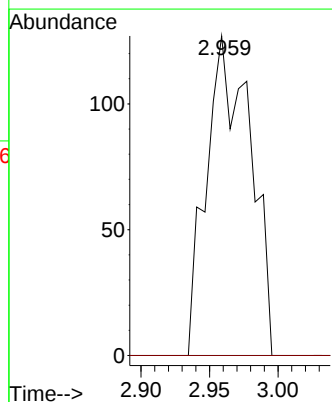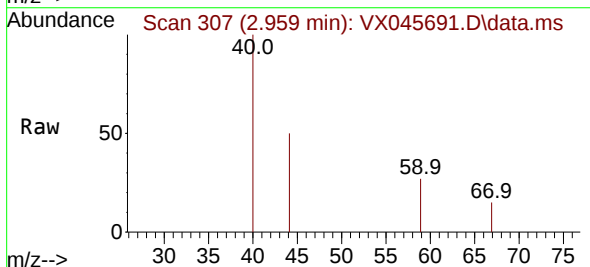

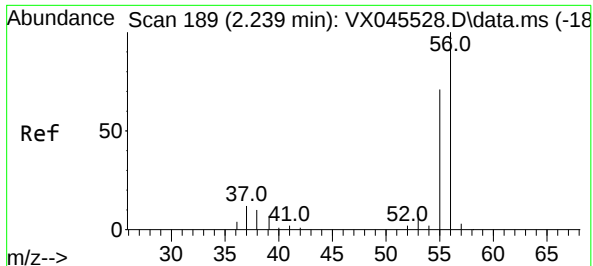

#13

Acrolein

Concen: 0.359 ug/l

RT: 2.239 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX045691.D

Acq: 10 Apr 2025 12:17

Instrument :

MSVOA_X

ClientSampleId :





IB-1.5-WC

Tgt Ion: 56 Resp: 79

Ion Ratio Lower Upper

56 100

55 46.8 56.2 84.2#

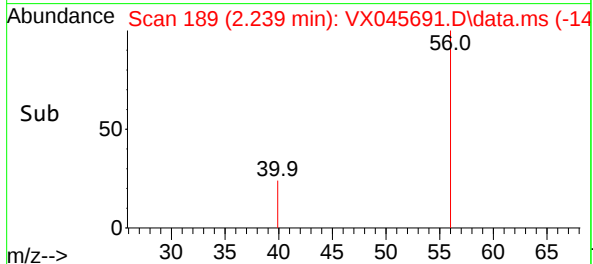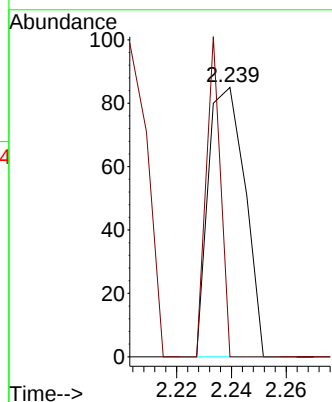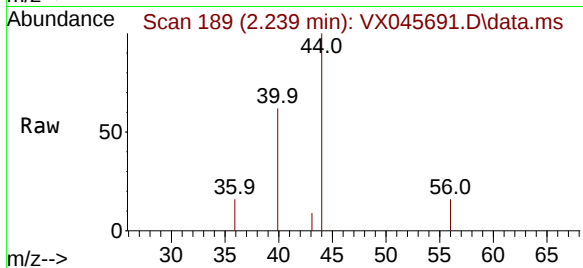

#14

Allyl chloride

Concen: 0.232 ug/l

RT: 2.636 min Scan# 254

Delta R.T. -0.024 min

Lab File: VX045691.D

Acq: 10 Apr 2025 12:17




Tgt Ion: 41 Resp: 343


Ion Ratio Lower Upper

41 100

39 95.3 60.2 90.2#

76 0.0 24.6 36.8#




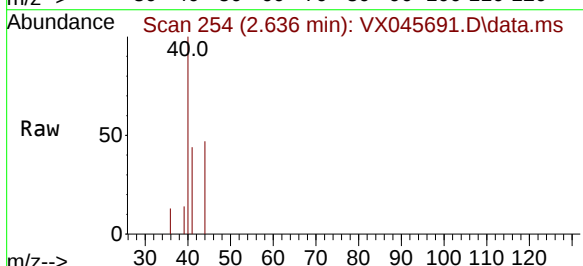




#16
Acetone
Concen: 56.334 ug/l
RT: 2.380 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 43 Resp: 27479
Ion Ratio Lower Upper
43 100
58 27.8 22.3 33.5

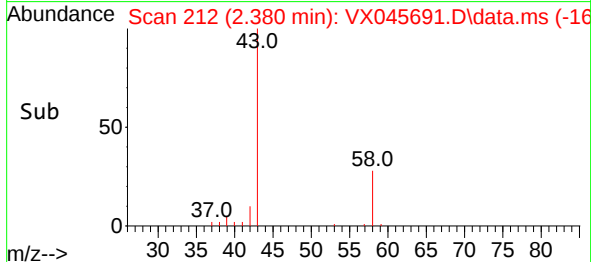

#17
Carbon Disulfide
Concen: 0.464 ug/l
RT: 2.508 min Scan# 233
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 76 Resp: 893
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#




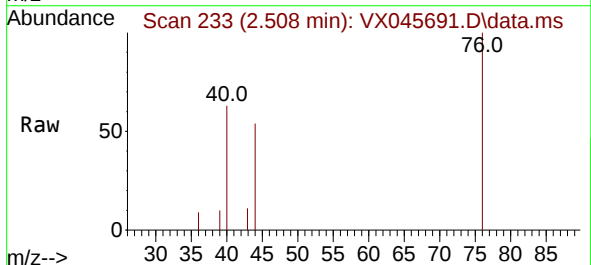




#18
Methyl Acetate
Concen: 1.207 ug/l
RT: 2.703 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 43 Resp: 1356
Ion Ratio Lower Upper
43 100
74 20.4 17.5 26.3

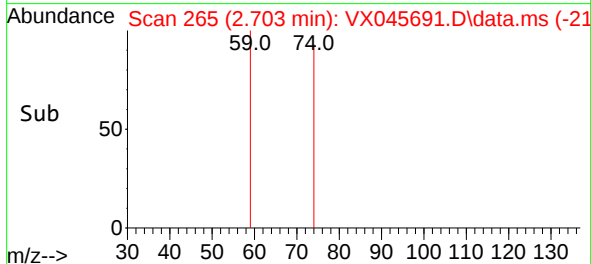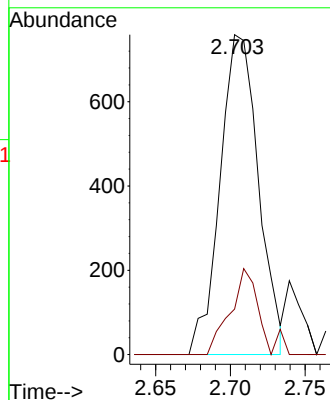

#20
Methylene Chloride
Concen: 6.073 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 84 Resp: 5546
Ion Ratio Lower Upper
84 100
49 125.6 107.5 161.3
51 35.5 33.0 49.6
86 55.2 50.1 75.1

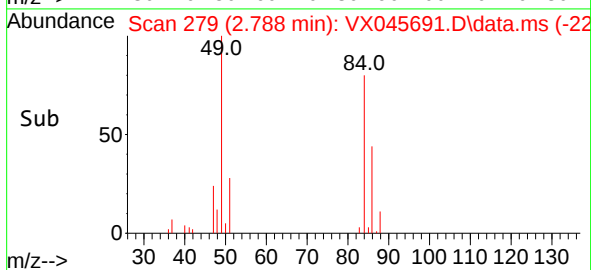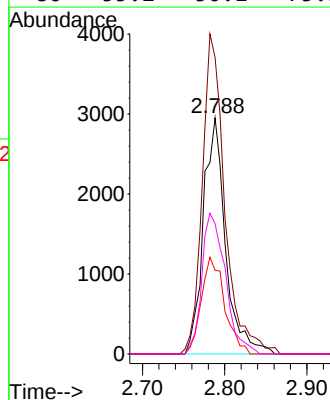



#25

2-Butanone

Concen: 5.402 ug/l

RT: 4.581 min Scan# 51

Delta R.T. 0.024 min

Lab File: VX045691.D

Acq: 10 Apr 2025 12:17

Instrument :

MSVOA_X

ClientSampleId :





IB-1.5-WC

Tgt Ion: 43 Resp: 3857

Ion Ratio Lower Upper

43 100

72 21.9 18.6 28.0

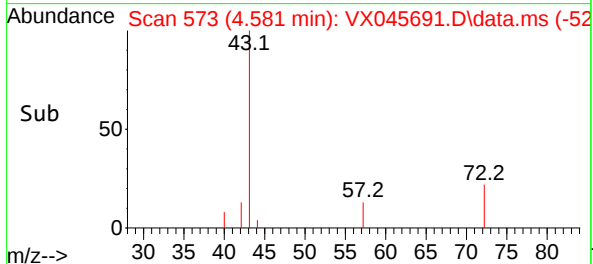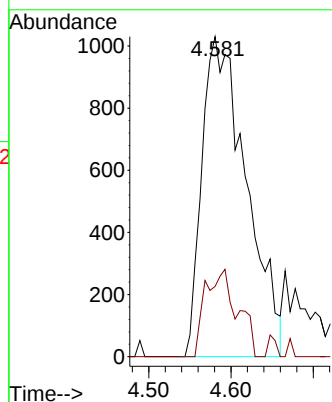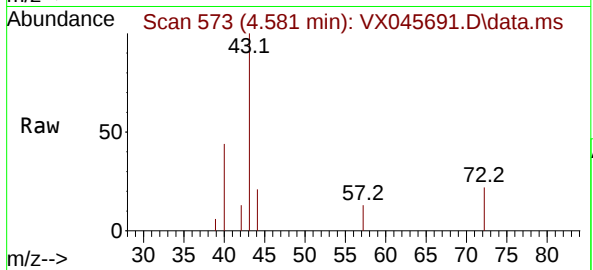

#29

Tetrahydrofuran

Concen: 0.646 ug/l

RT: 5.050 min Scan# 650

Delta R.T. 0.049 min

Lab File: VX045691.D

Acq: 10 Apr 2025 12:17




Tgt Ion: 42 Resp: 299


Ion Ratio Lower Upper

42 100

72 0.0 33.4 50.0#


71 0.0 31.4 47.0#

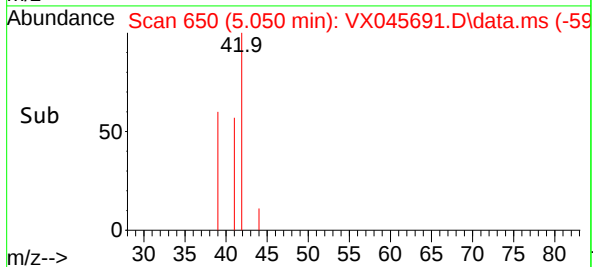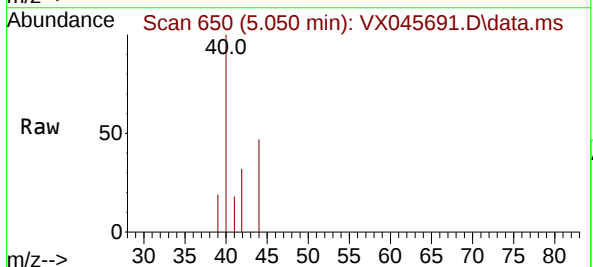






#31
Cyclohexane
Concen: 1.313 ug/l
RT: 5.544 min Scan# 718
Delta R.T. 0.079 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC



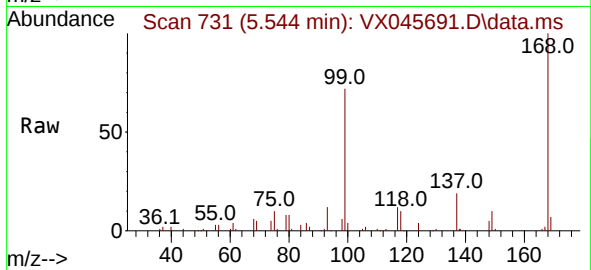



Tgt Ion: 56 Resp: 1913
Ion Ratio Lower Upper
56 100
69 167.8 23.6 35.4#
84 111.4 67.7 101.5#

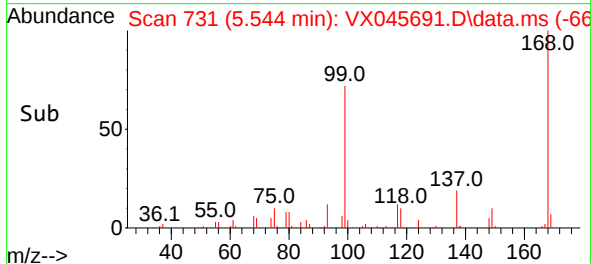

#33
1,2-Dichloroethane-d4
Concen: 53.248 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 65 Resp: 63254
Ion Ratio Lower Upper
65 100
67 48.7 0.0 99.0


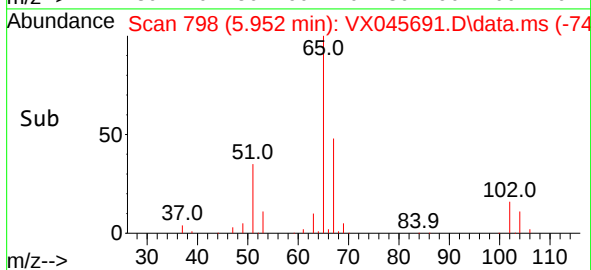






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion:114 Resp: 127970
Ion Ratio Lower Upper
114 100
63 24.2 0.0 46.8
88 16.9 0.0 35.4

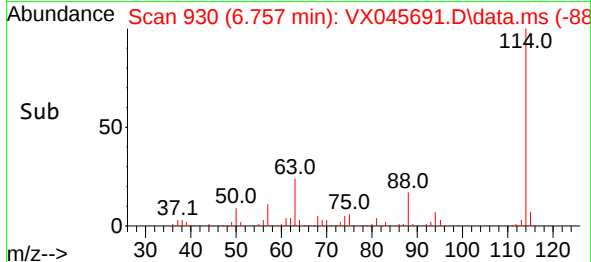

#35
Dibromofluoromethane
Concen: 50.715 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17


Tgt Ion:113 Resp: 46047
Ion Ratio Lower Upper
113 100
111 104.4 81.8 122.6
192 17.0 13.8 20.6

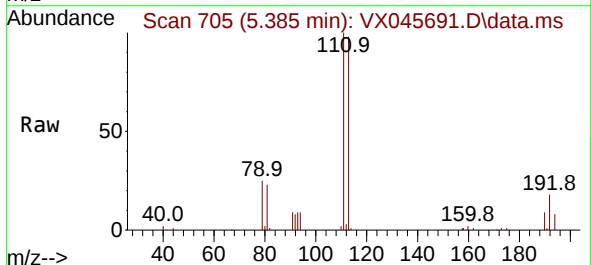






#36
1,1-Dichloropropene
Concen: 5.278 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC







Tgt Ion: 75 Resp: 6470
Ion Ratio Lower Upper
75 100
110 9.7 16.9 50.6#
77 0.0 25.0 37.4#

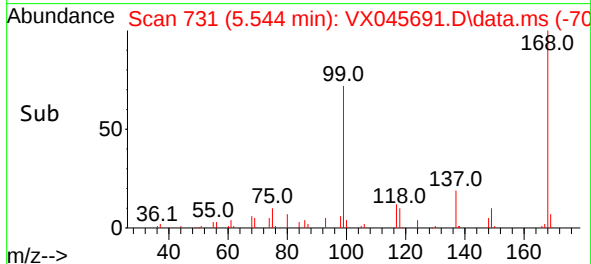

#37
Ethyl Acetate
Concen: 0.215 ug/l
RT: 4.666 min Scan# 587
Delta R.T. -0.049 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 43 Resp: 332
Ion Ratio Lower Upper
43 100
61 0.0 9.9 14.9#
70 0.0 7.5 11.3#




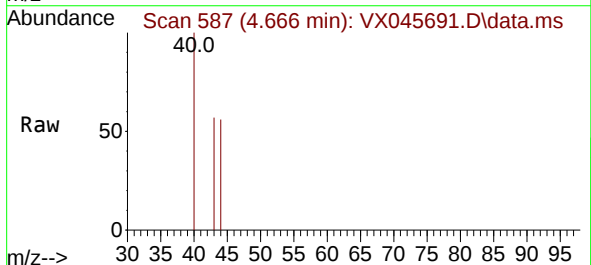




#38
Carbon Tetrachloride
Concen: 6.071 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion:117 Resp: 8043
Ion Ratio Lower Upper
117 100
119 4.2 76.9 115.3#
121 0.0 24.2 36.2#

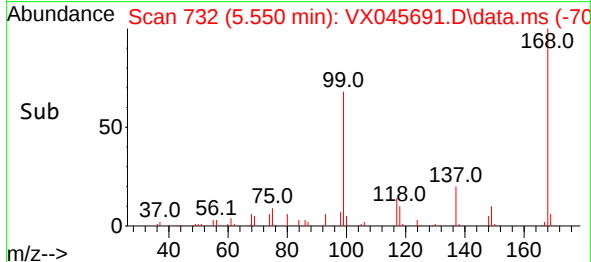

#40
Benzene
Concen: 0.926 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.012 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 78 Resp: 3468
Ion Ratio Lower Upper
78 100
77 23.4 19.0 28.6




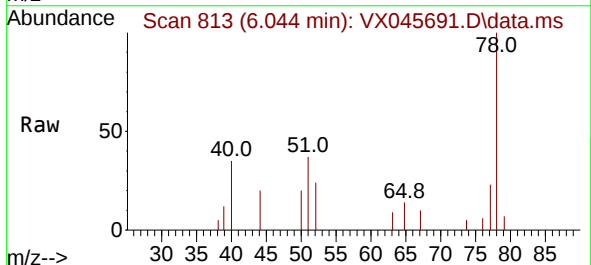




#43
Isopropyl Acetate
Concen: 3.529 ug/l
RT: 6.355 min Scan# 81
Delta R.T. 0.018 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 43 Resp: 8264
Ion Ratio Lower Upper
43 100
61 18.1 14.1 21.1
87 10.4 9.2 13.8

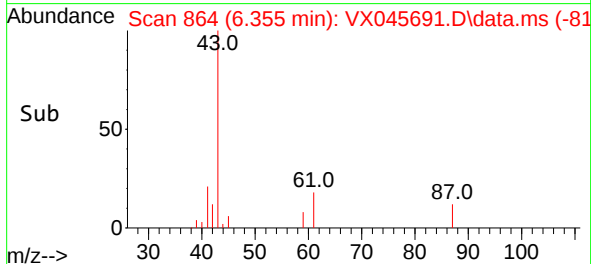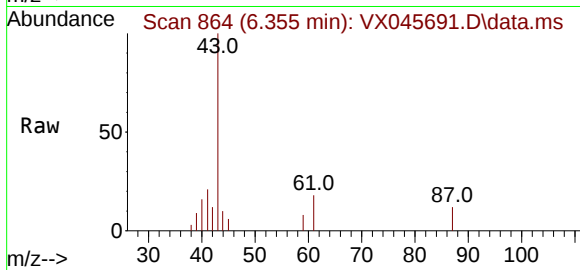

#48
Methyl methacrylate
Concen: 29.757 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.104 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 41 Resp: 35975
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 58.5 53.6 80.4


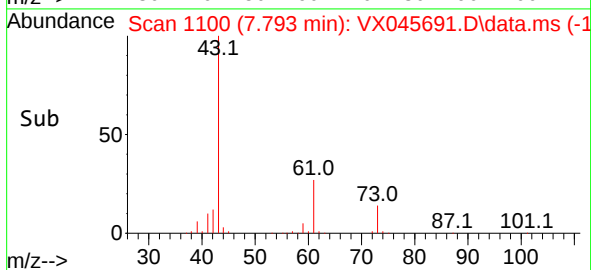

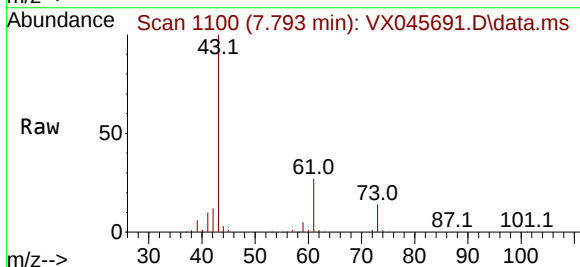


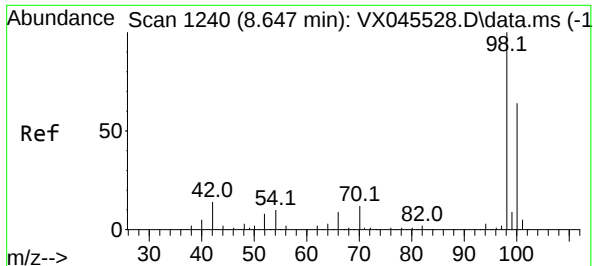

#50
Toluene-d8
Concen: 51.293 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 98 Resp: 162553
Ion Ratio Lower Upper
98 100
100 65.0 52.2 78.4

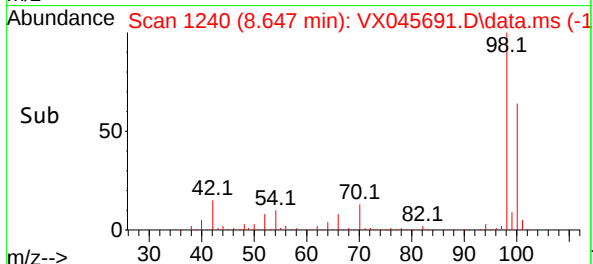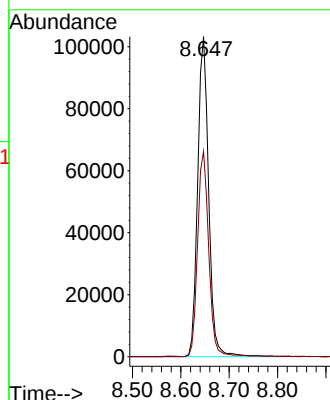

#51
4-Methyl-2-Pentanone
Concen: 19.969 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.024 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 43 Resp: 30996
Ion Ratio Lower Upper
43 100
58 4.7 28.5 42.7#


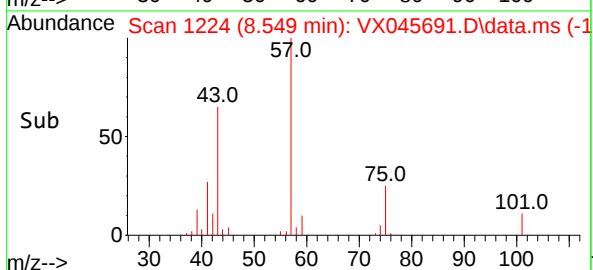
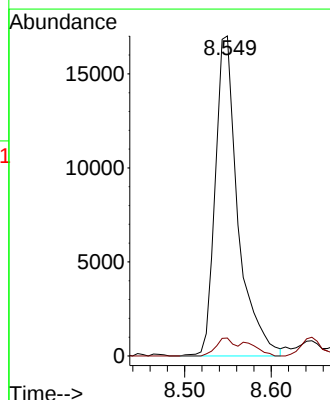
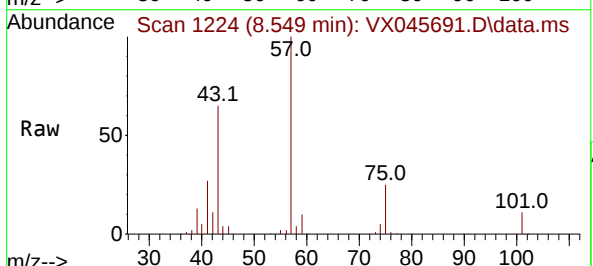


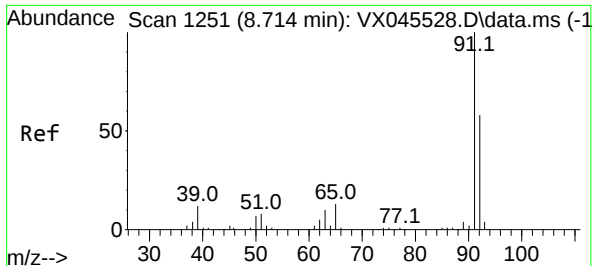

#52
Toluene
Concen: 0.399 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 92 Resp: 903
Ion Ratio Lower Upper
92 100
91 157.4 138.7 208.1

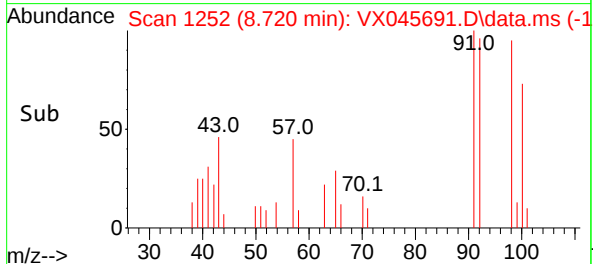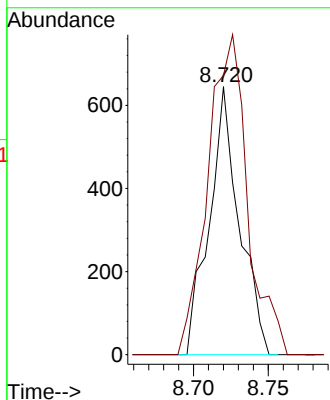

#53
t-1,3-Dichloropropene
Concen: 2.320 ug/l
RT: 8.988 min Scan# 1296
Delta R.T. 0.012 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 75 Resp: 45
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#


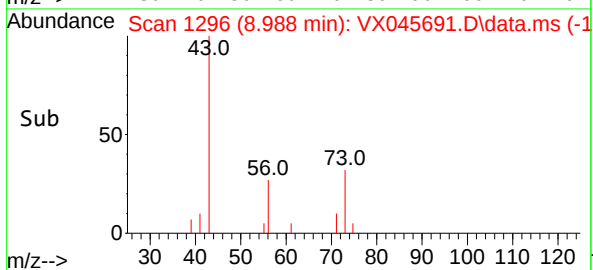
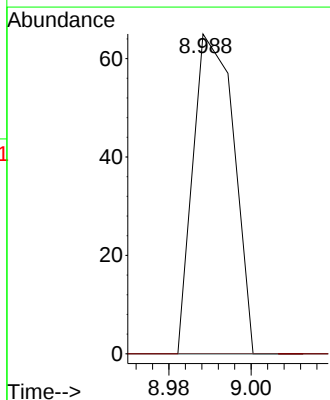
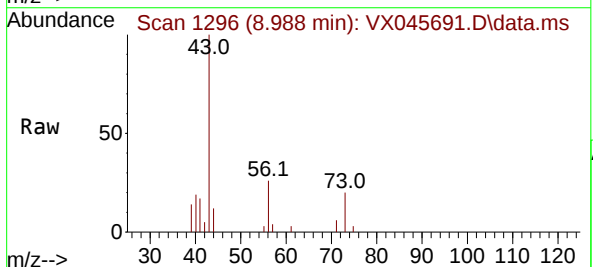




#54
 cis-1,3-Dichloropropene
 Concen: 8.592 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX045691.D
 Acq: 10 Apr 2025 12:17




Instrument :
 MSVOA_X
 ClientSampleId :
 IB-1.5-WC


Tgt Ion: 75 Resp: 11563
 Ion Ratio Lower Upper
 75 100
 77 0.8 24.6 36.8#
 39 50.7 48.4 72.6

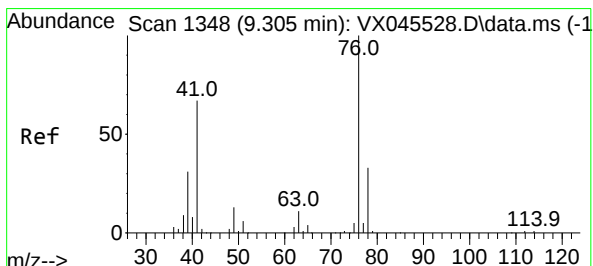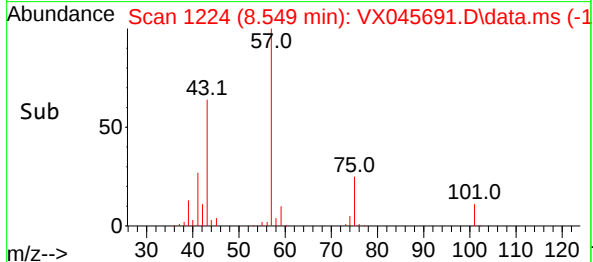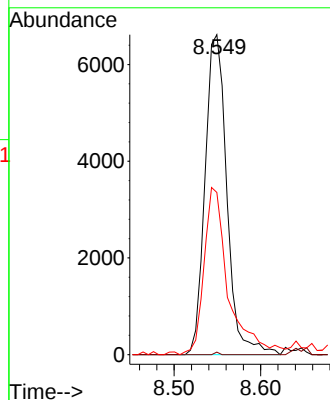

#57
 1,3-Dichloropropane
 Concen: 0.573 ug/l
 RT: 9.476 min Scan# 1376
 Delta R.T. 0.171 min
 Lab File: VX045691.D
 Acq: 10 Apr 2025 12:17

Tgt Ion: 76 Resp: 901
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.0 39.0#

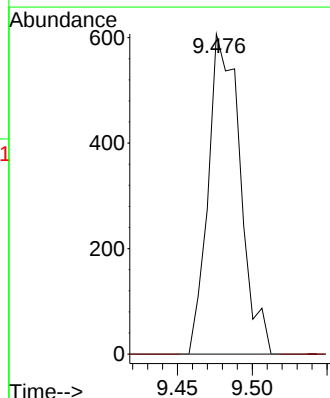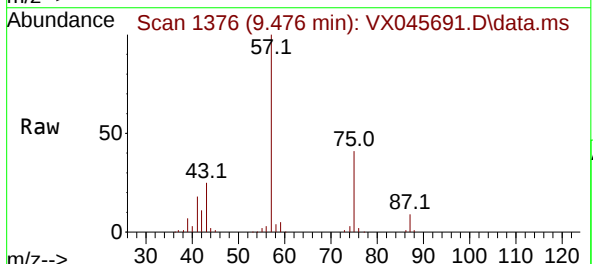



#59

2-Hexanone

Concen: 6.228 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.049 min

Lab File: VX045691.D

Acq: 10 Apr 2025 12:17

Instrument :

MSVOA_X

ClientSampleId :





IB-1.5-WC

Tgt Ion: 43 Resp: 7159

Ion Ratio Lower Upper

43 100

58 0.0 24.9 74.6#

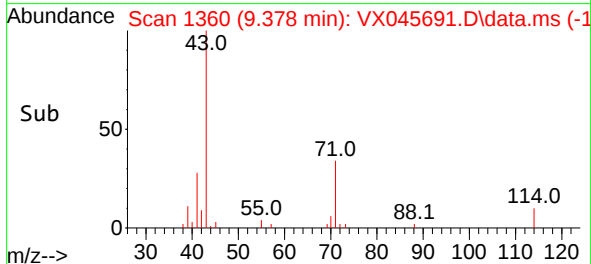

#62

4-Bromofluorobenzene

Concen: 52.639 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX045691.D

Acq: 10 Apr 2025 12:17




Tgt Ion: 95 Resp: 60763


Ion Ratio Lower Upper

95 100

174 66.4 0.0 135.8

176 65.2 0.0 131.4




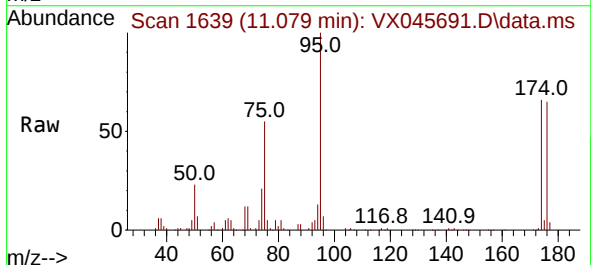




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion:117 Resp: 120693
Ion Ratio Lower Upper
117 100
82 60.5 49.2 73.8
119 31.5 25.1 37.7

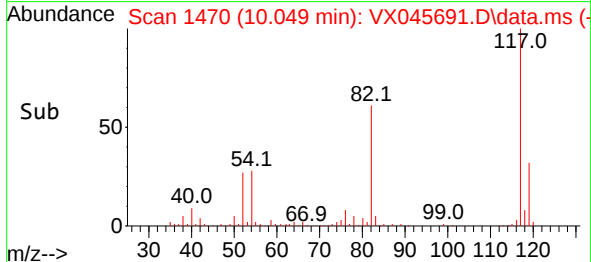

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion:152 Resp: 51059
Ion Ratio Lower Upper
152 100
115 65.8 46.9 140.7
150 156.0 0.0 349.4


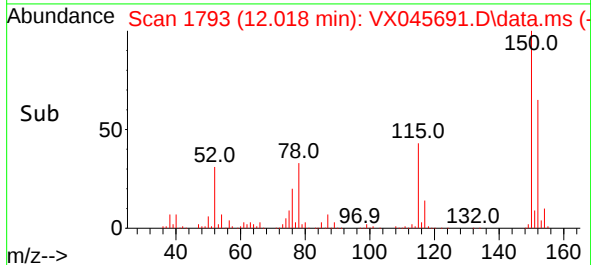






#74
N-amy1 acetate
Concen: 0.208 ug/l
RT: 10.872 min Scan# 1605
Delta R.T. 0.031 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 43 Resp: 407
Ion Ratio Lower Upper
43 100
70 0.0 30.1 45.1#
55 0.0 18.3 27.5#
61 0.0 17.5 26.3#

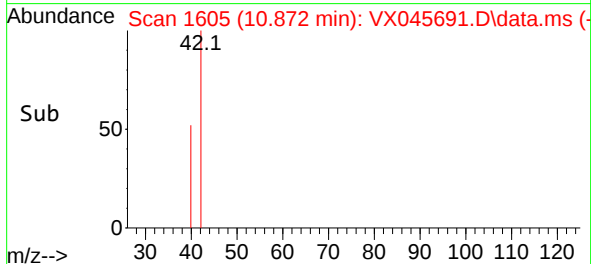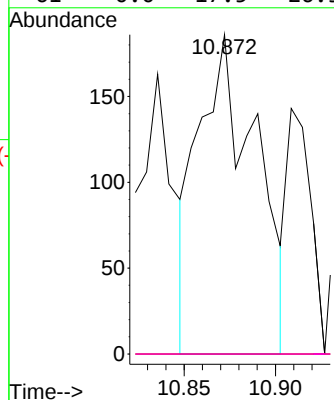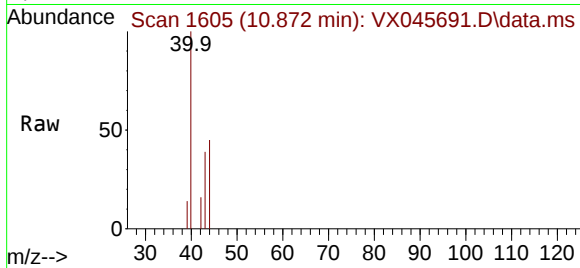

#76
1,2,3-Trichloropropane
Concen: 28.024 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.158 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion: 75 Resp: 34903
Ion Ratio Lower Upper
75 100
77 1.0 20.0 59.9#



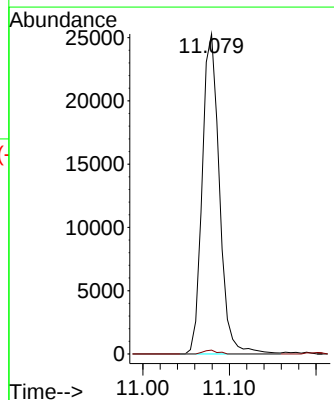
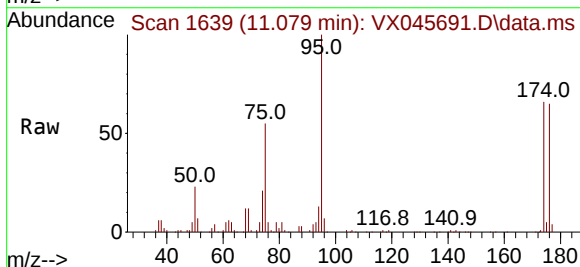




#81
trans-1,4-Dichloro-2-butene
Concen: 95.111 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17




Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC


Tgt Ion: 75 Resp: 34903
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#

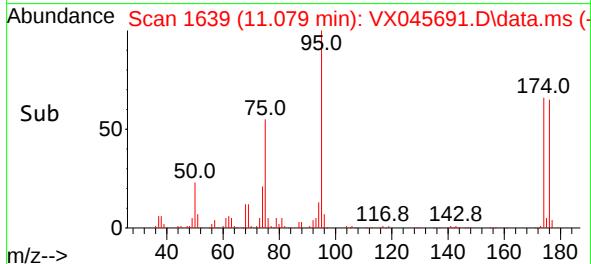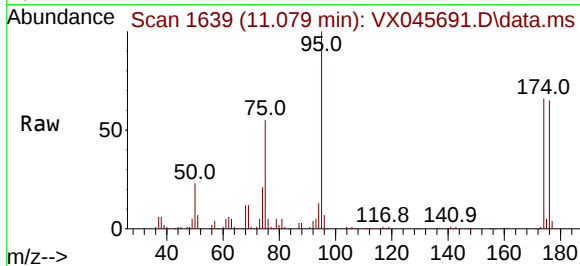

#93
1,2,4-Trichlorobenzene
Concen: 0.367 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. 0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion:180 Resp: 349
Ion Ratio Lower Upper
180 100
182 86.8 47.9 143.6
145 0.0 17.9 53.8#




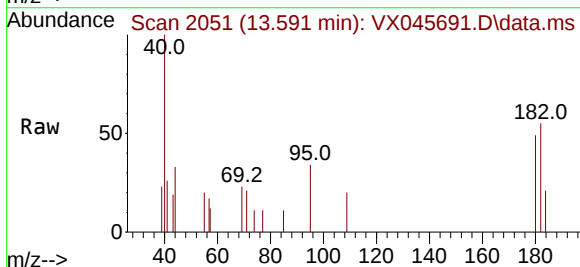




#95
Naphthalene
Concen: 0.507 ug/l
RT: 13.780 min Scan# 2081
Delta R.T. 0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Instrument :
MSVOA_X
ClientSampleId :
IB-1.5-WC

Tgt Ion:128 Resp: 1797
Ion Ratio Lower Upper
128 100
127 10.5 10.3 15.5
129 9.1 8.6 12.8

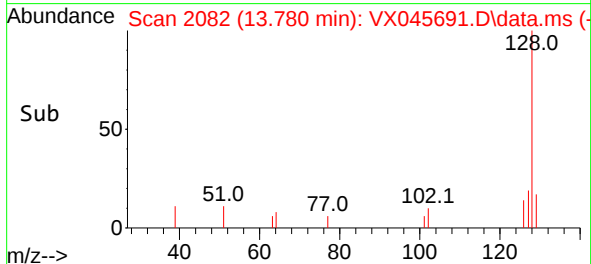

#96
1,2,3-Trichlorobenzene
Concen: 0.302 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. 0.006 min
Lab File: VX045691.D
Acq: 10 Apr 2025 12:17

Tgt Ion:180 Resp: 301
Ion Ratio Lower Upper
180 100
182 132.9 47.3 141.8
145 45.5 18.2 54.6

