

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX041119\
 Data File : VX008853.D
 Acq On : 11 Apr 2019 15:44
 Operator : JC/SP
 Sample : K2316-03
 Misc : 5.0g/10mL/100uL/10mL/MSVOA_X/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 20190171-COMP-CS-3ME

Quant Time: Apr 12 07:35:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 04 04:47:41 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	160673	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	261484	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	235032	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	115018	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	108112	46.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.26%	
35) Dibromofluoromethane	5.50	113	74521	44.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	89.14%	
50) Toluene-d8	8.71	98	331140	49.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.48%	
62) 4-Bromofluorobenzene	11.14	95	122464	51.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.76%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	1.33	50	370	Below Cal	#	87
5) Bromomethane	1.64	94	921	2.605	ug/l	87
6) Chloroethane	1.72	64	195	Below Cal	#	81
10) Methyl Iodide	2.48	142	319	4.184	ug/l #	76
16) Acetone	2.48	43	2097	1.554	ug/l	89
17) Carbon Disulfide	2.53	76	981	Below Cal	#	88
18) Methyl Acetate	2.79	43	3238	0.989	ug/l	92
20) Methylene Chloride	2.84	84	1062	0.470	ug/l #	75
28) Bromochloromethane	5.00	49	20	Below Cal	#	22
29) Tetrahydrofuran	5.17	42	649	0.458	ug/l #	71
36) 1,1-Dichloropropene	5.65	75	12930	4.524	ug/l #	52
38) Carbon Tetrachloride	5.65	117	15286	6.462	ug/l #	16
40) Benzene	6.14	78	8969	1.053	ug/l	96
52) Toluene	8.78	92	1154	0.230	ug/l	100
65) Chlorobenzene	10.14	112	1994	0.383	ug/l	99
67) Ethyl Benzene	10.25	91	2254	0.232	ug/l	94
68) m/p-Xylenes	10.36	106	1633	0.468	ug/l	98
69) o-Xylene	10.70	106	775	0.229	ug/l	87
73) Isopropylbenzene	11.02	105	5969	0.626	ug/l	98
76) 1,2,3-Trichloropropane	11.14	75	62330	19.727	ug/l #	34
79) 2-Chlorotoluene	11.43	91	2786	0.415	ug/l	92
81) trans-1,4-Dichloro-2-buten	11.14	75	62330	54.378	ug/l #	9
84) 1,2,4-Trimethylbenzene	11.81	105	1921	0.237	ug/l	87
95) Naphthalene	13.83	128	2789	0.295	ug/l #	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX041119\
Data File : VX008853.D
Acq On : 11 Apr 2019 15:44
Operator : JC/SP
Sample : K2316-03
Misc : 5.0g/10mL/100uL/10mL/MSVOA_X/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20190171-COMP-CS-3ME

Quant Time: Apr 12 07:35:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X040319W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 04 04:47:41 2019
Response via : Initial Calibration

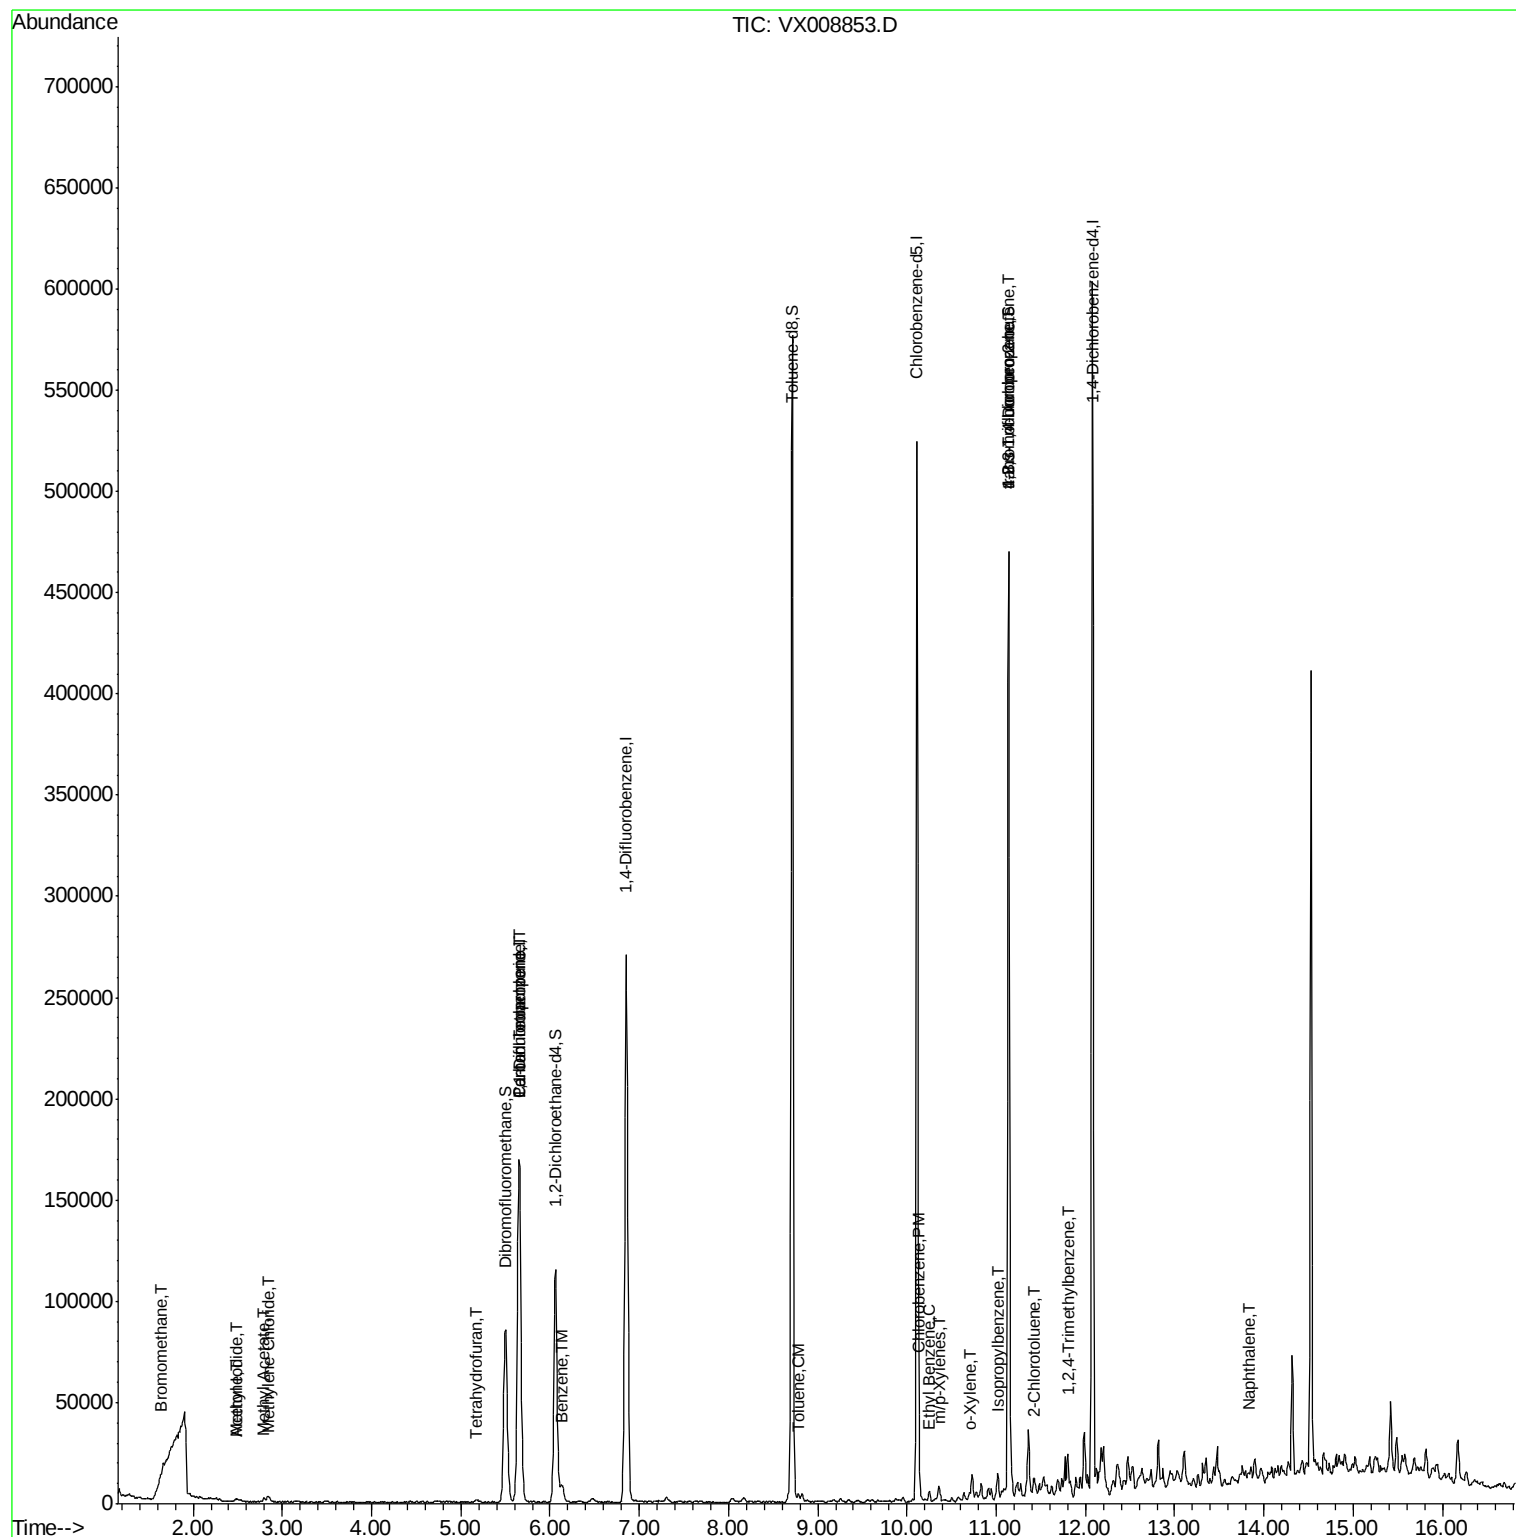



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.01 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :


20190171-COMP-CS-3ME

Tgt Ion:168 Resp: 160673

Ion Ratio Lower Upper

168 100

99 56.4 46.7 70.1

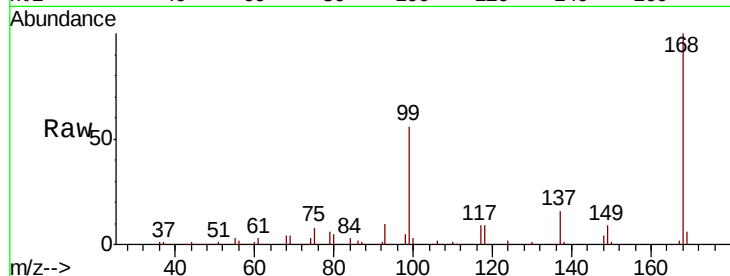

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.65

60000



40000

20000

0

Time-->

5.50 5.60 5.70 5.80

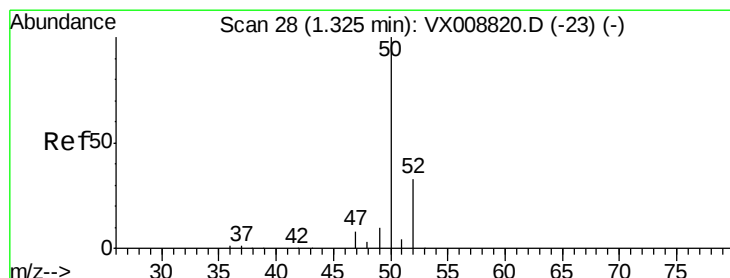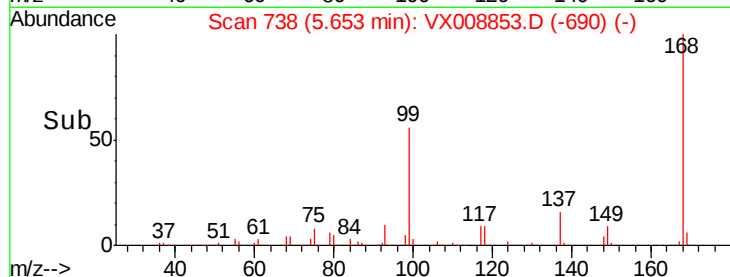

#3

Chloromethane

Concen: Below Cal

RT: 1.33 min Scan# 29

Delta R.T. 0.01 min

Lab File: VX008853.D


Acq: 11 Apr 2019 15:44

Tgt Ion: 50 Resp: 370

Ion Ratio Lower Upper

50 100

52 39.6 25.8 38.8#

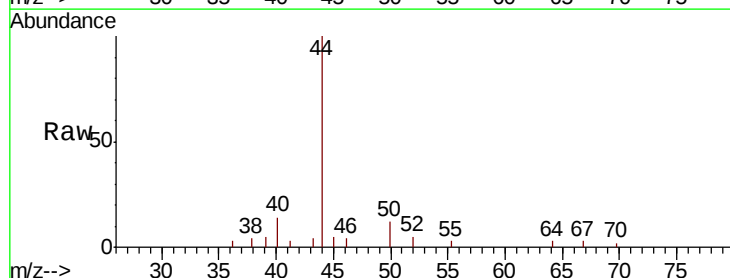

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.33

250

200

150


100

50

0

Time-->

1.30 1.35

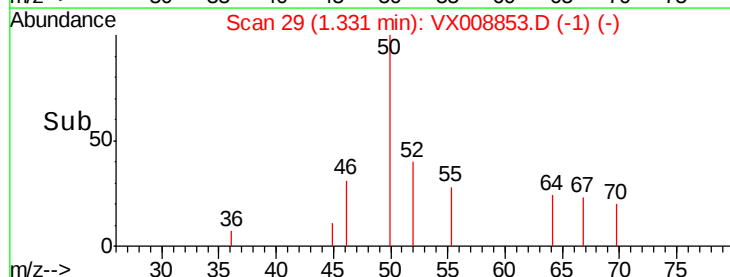



#5

Bromomethane

Concen: 2.605 ug/l

RT: 1.64 min Scan# 79

Delta R.T. 0.00 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :


20190171-COMP-CS-3ME

Tgt Ion: 94 Resp: 921

Ion Ratio Lower Upper




94 100

96 106.7 75.2 112.8

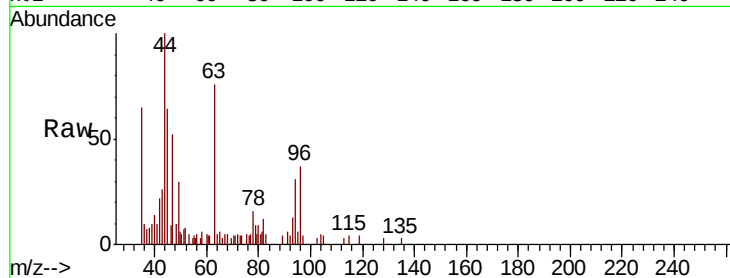

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

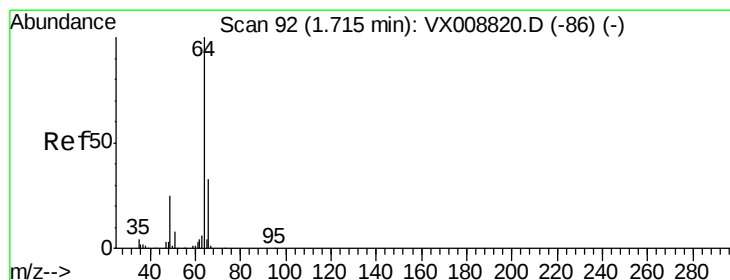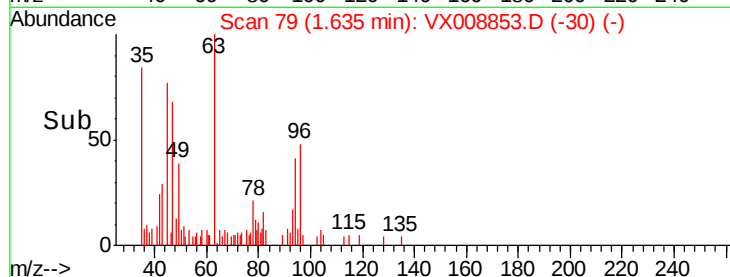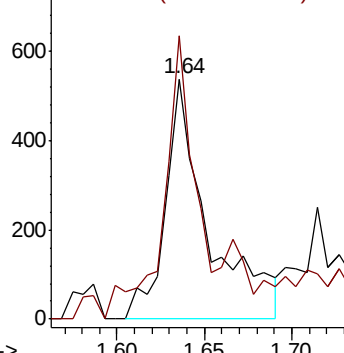

#6

Chloroethane

Concen: Below Cal

RT: 1.72 min Scan# 93

Delta R.T. 0.01 min

Lab File: VX008853.D


Acq: 11 Apr 2019 15:44

Tgt Ion: 64 Resp: 195

Ion Ratio Lower Upper



64 100


66 21.4 25.4 38.0#

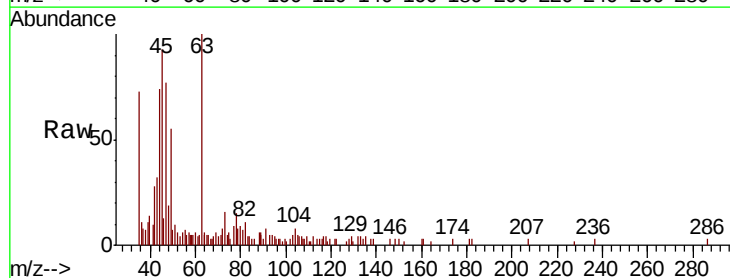

Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

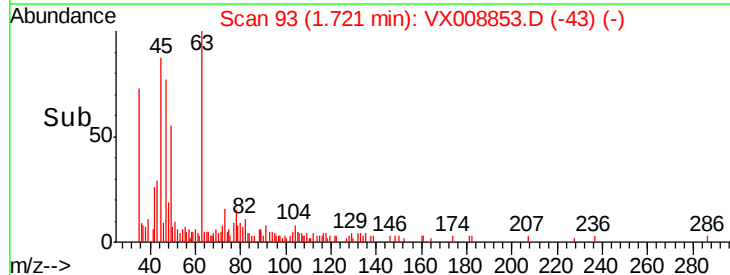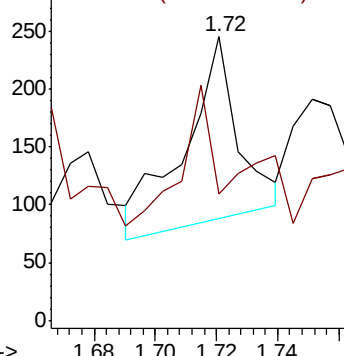


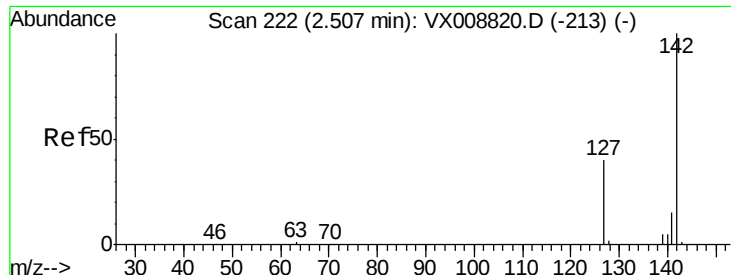




#10
Methyl Iodide
Concen: 4.184 ug/l
RT: 2.48 min Scan# 217
Delta R.T. -0.03 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44

Instrument :
MSVOA_X
ClientSampleId :
20190171-COMP-CS-3ME

Tgt Ion: 142 Resp: 319
Ion Ratio Lower Upper
142 100
127 54.2 33.0 49.6#
141 0.0 11.4 17.2#




Abundance Ion 141.80 (141.50 to 142.50): V
Ion 126.80 (126.50 to 127.50): V
Ion 140.80 (140.50 to 141.50): V


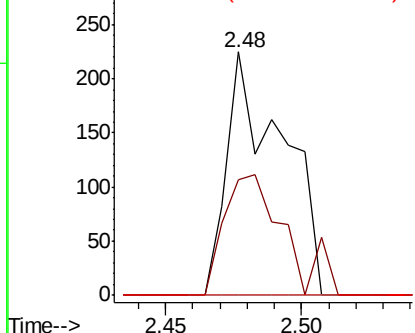



#16
Acetone
Concen: 1.554 ug/l
RT: 2.48 min Scan# 218
Delta R.T. 0.04 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44

Tgt Ion: 43 Resp: 2097
Ion Ratio Lower Upper
43 100
58 25.1 24.8 37.2



Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0




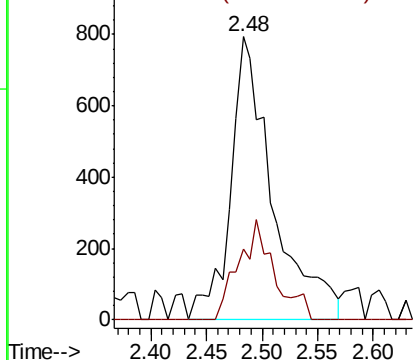




#17
Carbon Disulfide
Concen: Below Cal
RT: 2.53 min Scan# 226
Delta R.T. -0.04 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44




Instrument :
MSVOA_X
ClientSampleId :
20190171-COMP-CS-3ME


Tgt Ion: 76 Resp: 981
Ion Ratio Lower Upper
76 100
78 13.1 7.1 10.7#

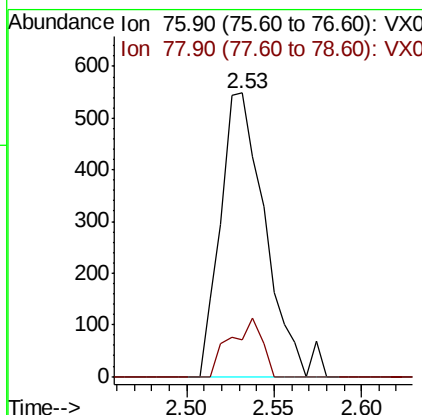

#18
Methyl Acetate
Concen: 0.989 ug/l
RT: 2.79 min Scan# 269
Delta R.T. 0.02 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44

Tgt Ion: 43 Resp: 3238
Ion Ratio Lower Upper
43 100
74 16.7 16.5 24.7

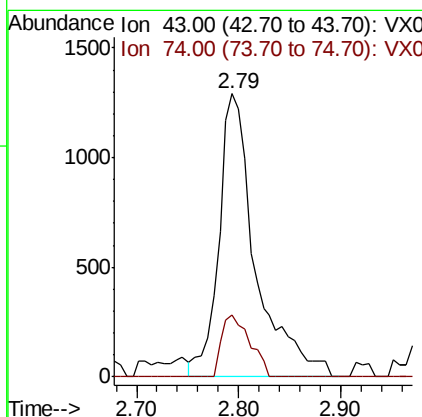

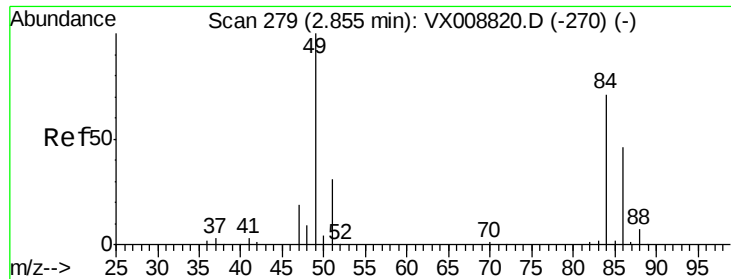

#20

Methylene Chloride

Concen: 0.470 ug/l

RT: 2.84 min Scan# 277

Delta R.T. -0.02 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :

20190171-COMP-CS-3ME

Tgt Ion: 84 Resp: 1062


Ion Ratio Lower Upper

84 100

49 173.9 109.7 164.5#

51 52.3 33.6 50.4#

86 49.1 51.4 77.2#






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

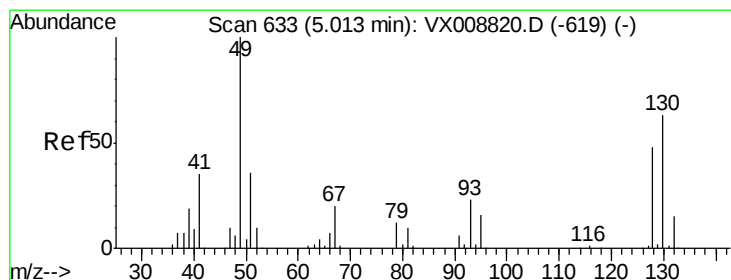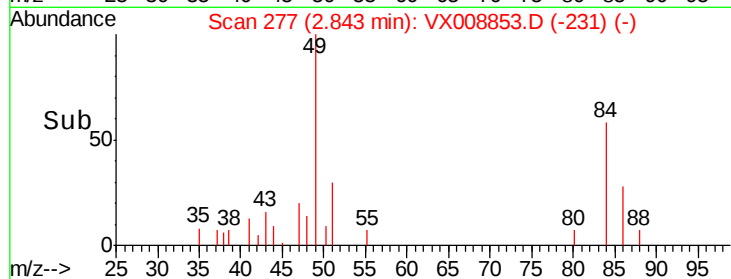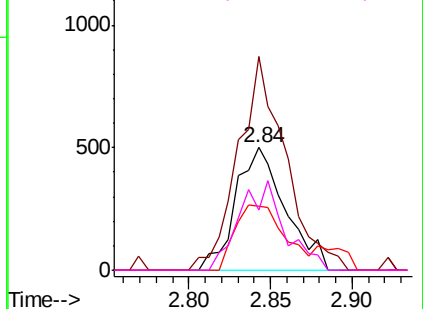

#28

Bromochloromethane

Concen: Below Cal

RT: 5.00 min Scan# 631

Delta R.T. -0.02 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44


Tgt Ion: 49 Resp: 20

Ion Ratio Lower Upper

49 100

129 0.0 0.0 3.6



130 0.0 49.3 73.9#




Abundance Ion 48.90 (48.60 to 49.60): VX0

Ion 128.80 (128.50 to 129.50): V

Ion 129.80 (129.50 to 130.50): V

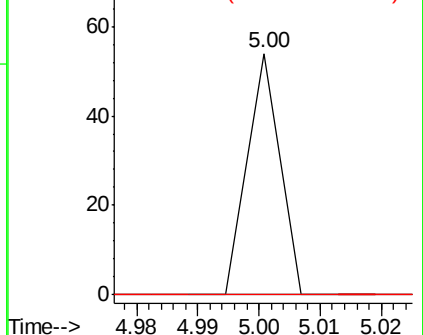



#29

Tetrahydrofuran

Concen: 0.458 ug/l

RT: 5.17 min Scan# 658

Delta R.T. 0.04 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :

20190171-COMP-CS-3ME


Tgt Ion: 42 Resp: 649

Ion Ratio Lower Upper

42 100

72 50.4 30.5 45.7#




71 12.9 28.6 43.0#



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

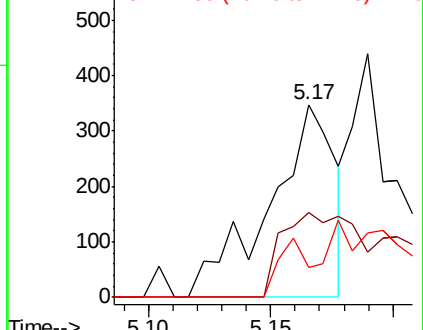

#33

1,2-Dichloroethane-d4

Concen: 46.132 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX008853.D


Acq: 11 Apr 2019 15:44

Tgt Ion: 65 Resp: 108112

Ion Ratio Lower Upper



65 100


67 53.9 0.0 107.2



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

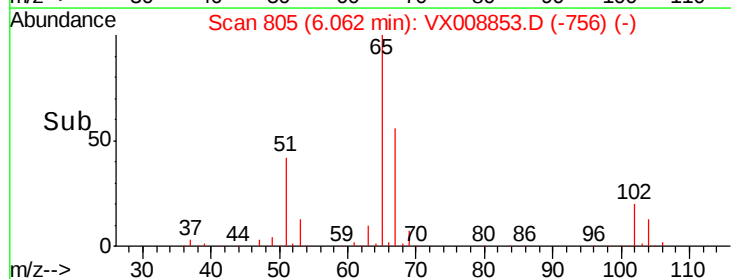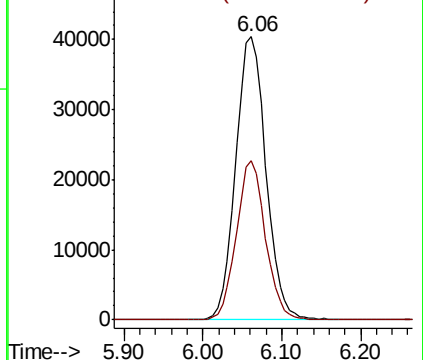

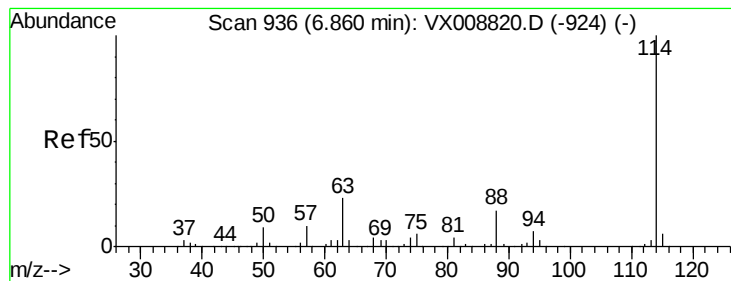

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. -0.01 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :

20190171-COMP-CS-3ME


Tgt Ion:114 Resp: 261484

Ion Ratio Lower Upper

114 100

63 23.6 0.0 47.2




88 16.4 0.0 34.0



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

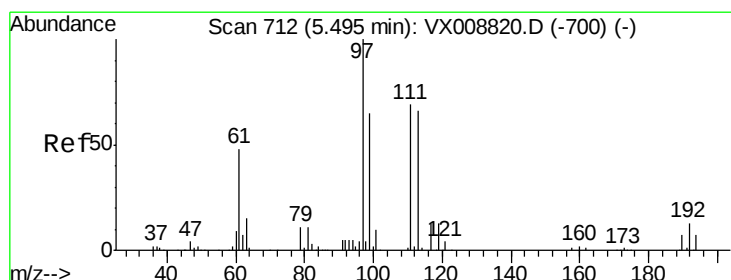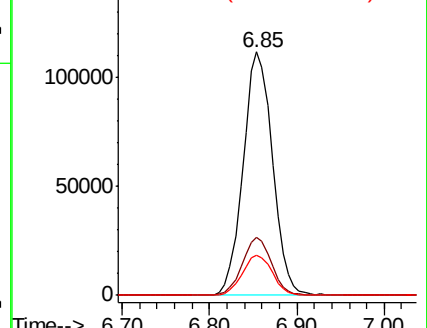

#35

Dibromofluoromethane

Concen: 44.575 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44


Tgt Ion:113 Resp: 74521

Ion Ratio Lower Upper

113 100

111 102.4 83.4 125.2



192 20.7 16.1 24.1

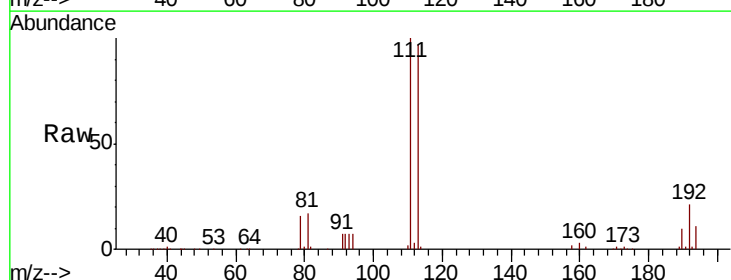


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



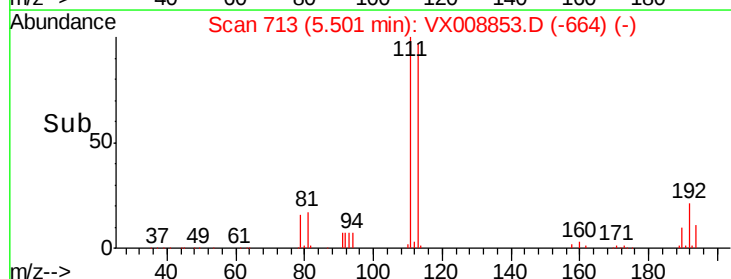
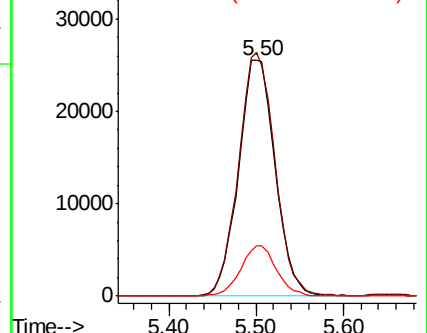


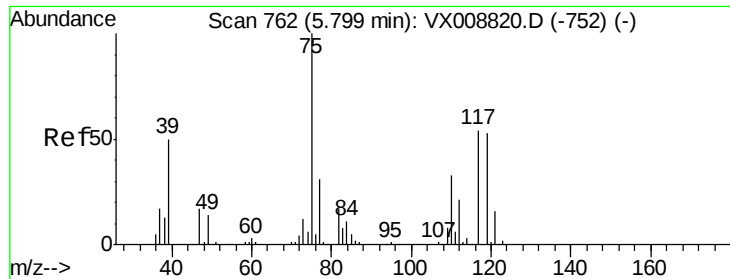

#36
 1,1-Dichloropropene
 Concen: 4.524 ug/l
 RT: 5.65 min Scan# 738
 Delta R.T. -0.15 min
 Lab File: VX008853.D
 Acq: 11 Apr 2019 15:44




Instrument :
 MSVOA_X
 ClientSampleId :
 20190171-COMP-CS-3ME


Tgt Ion: 75 Resp: 12930
 Ion Ratio Lower Upper
 75 100
 110 9.6 16.4 49.2#
 77 0.0 24.7 37.1#

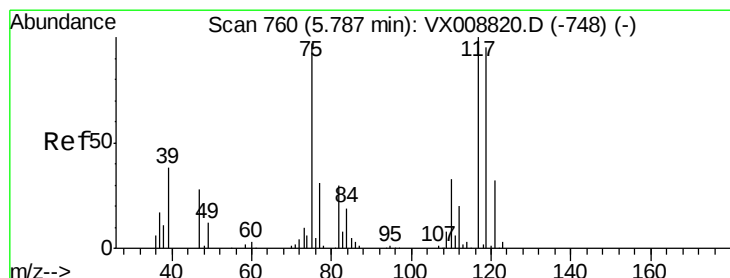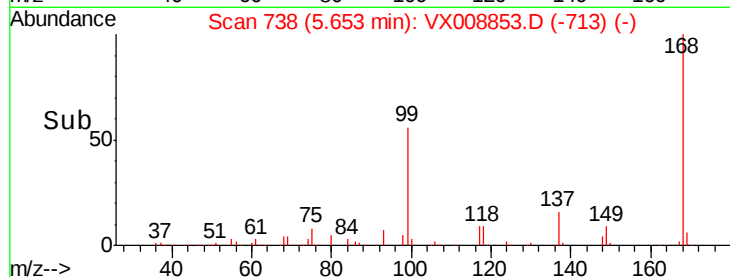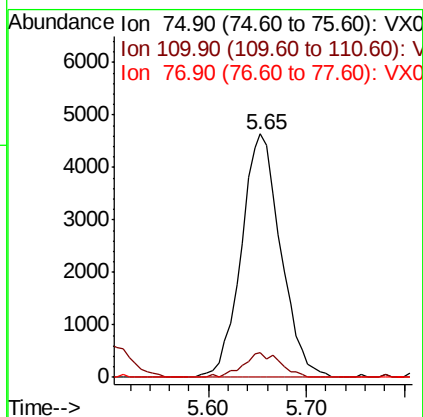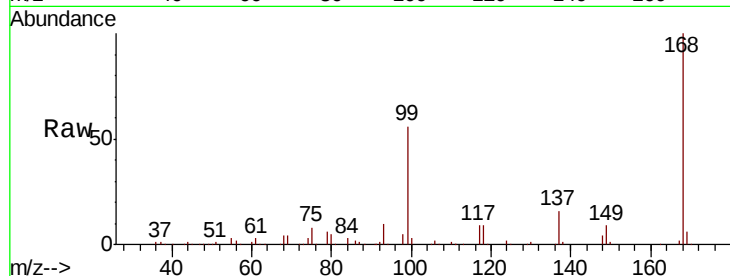

#38
 Carbon Tetrachloride
 Concen: 6.462 ug/l
 RT: 5.65 min Scan# 738
 Delta R.T. -0.13 min
 Lab File: VX008853.D
 Acq: 11 Apr 2019 15:44

Tgt Ion: 117 Resp: 15286
 Ion Ratio Lower Upper
 117 100
 119 4.5 75.0 112.6#
 121 0.0 24.3 36.5#

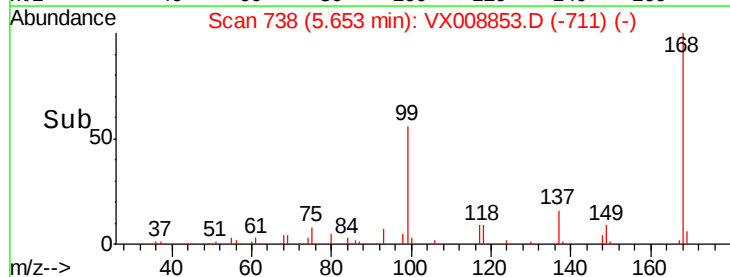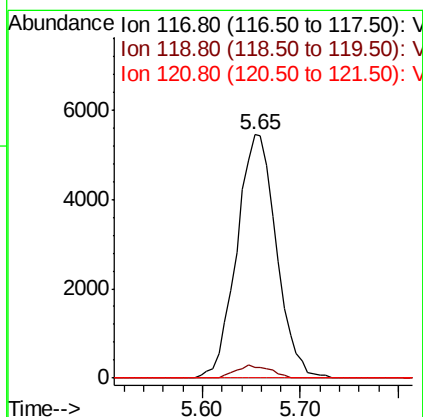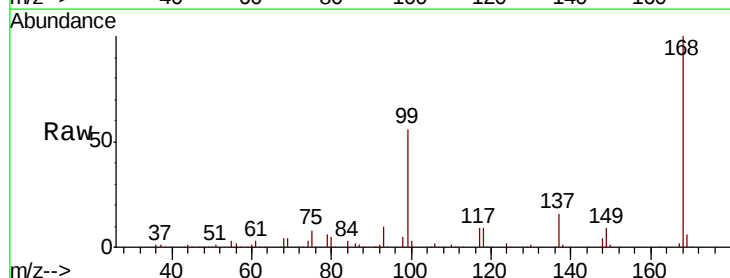

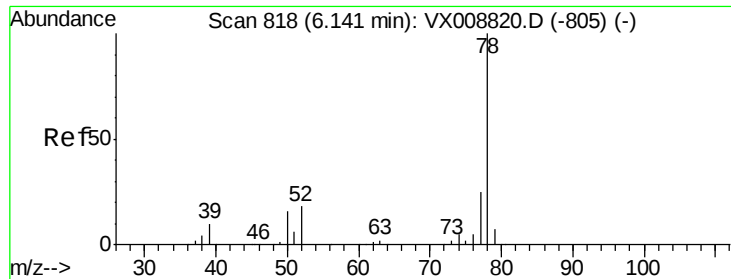

#40

Benzene

Concen: 1.053 ug/l

RT: 6.14 min Scan# 818

Delta R.T. -0.00 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :


20190171-COMP-CS-3ME

Tgt Ion: 78 Resp: 8969

Ion Ratio Lower Upper




78 100

77 21.9 19.1 28.7



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

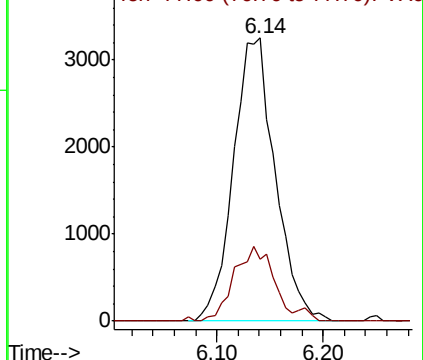

#50

Toluene-d8

Concen: 49.745 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX008853.D


Acq: 11 Apr 2019 15:44

Tgt Ion: 98 Resp: 331140

Ion Ratio Lower Upper



98 100


100 63.6 51.4 77.0



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

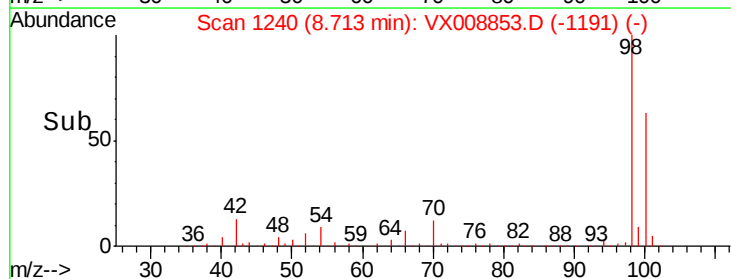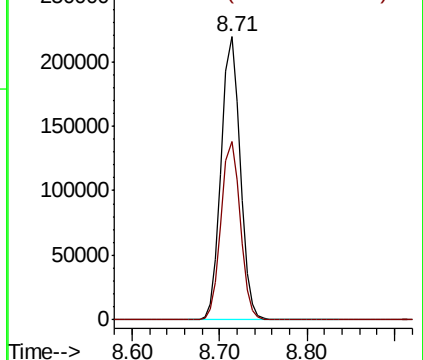

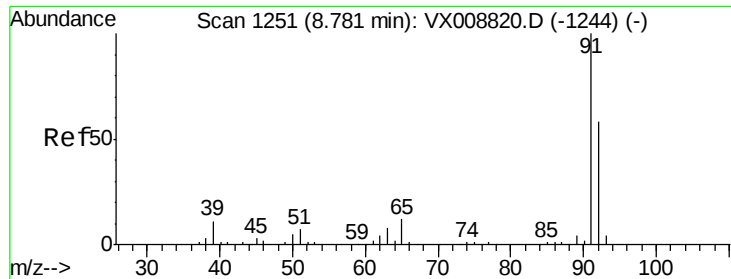

#52

Toluene

Concen: 0.230 ug/l

RT: 8.78 min Scan# 1251

Delta R.T. -0.01 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :


20190171-COMP-CS-3ME

Tgt Ion: 92 Resp: 1154

Ion Ratio Lower Upper




92 100

91 173.2 138.5 207.7



Abundance Ion 92.00 (91.70 to 92.70): VX0

Ion 91.00 (90.70 to 91.70): VX0

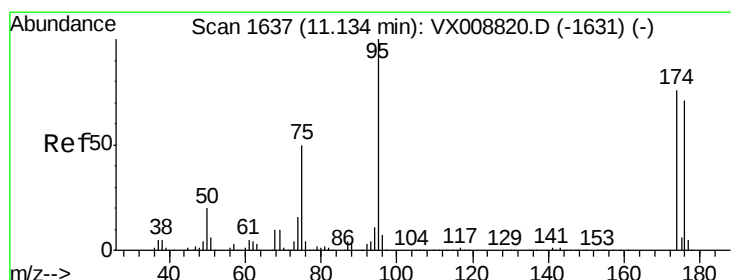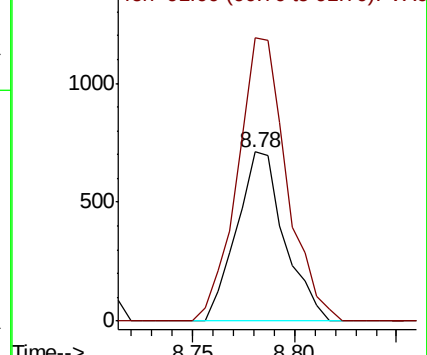

#62

4-Bromofluorobenzene

Concen: 51.878 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. 0.01 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44


Tgt Ion: 95 Resp: 122464

Ion Ratio Lower Upper

95 100

174 78.0 0.0 151.8



176 75.3 0.0 145.8




Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

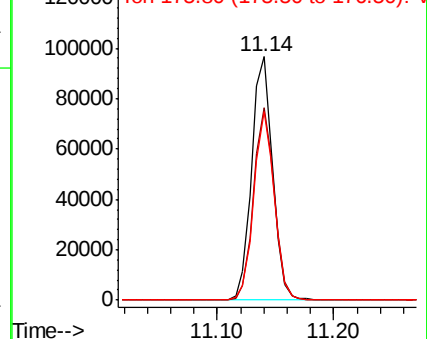



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.01 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :

20190171-COMP-CS-3ME


Tgt Ion:117 Resp: 235032

Ion Ratio Lower Upper

117 100

82 58.7 49.6 74.4




119 32.3 25.0 37.4



Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

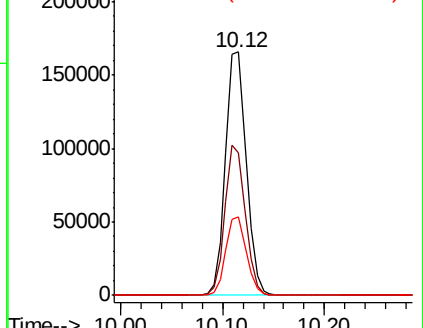

#65

Chlorobenzene

Concen: 0.383 ug/l

RT: 10.14 min Scan# 1474

Delta R.T. -0.00 min

Lab File: VX008853.D


Acq: 11 Apr 2019 15:44

Tgt Ion:112 Resp: 1994

Ion Ratio Lower Upper



112 100


114 31.8 25.8 38.8



Abundance Ion 111.90 (111.60 to 112.60): V

Ion 113.90 (113.60 to 114.60): V



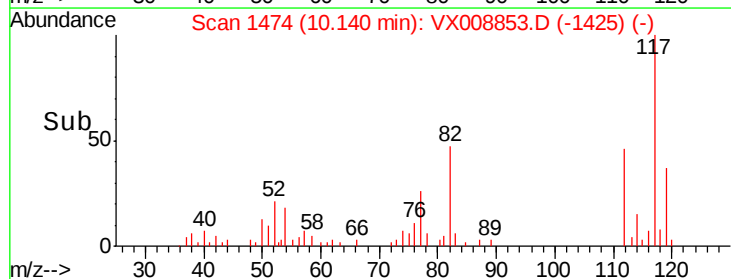
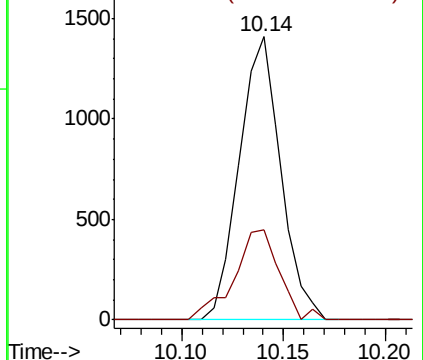


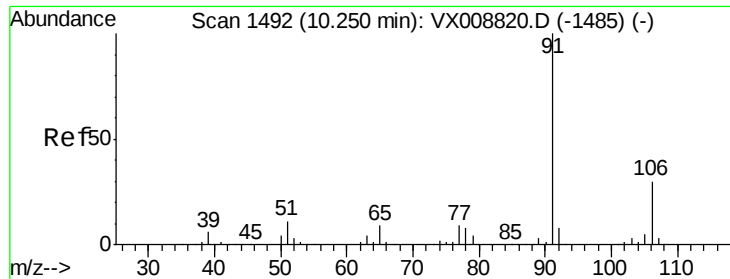

#67
Ethyl Benzene
Concen: 0.232 ug/l
RT: 10.25 min Scan# 1492
Delta R.T. -0.00 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44




Instrument :
MSVOA_X
ClientSampleId :
20190171-COMP-CS-3ME


Tgt Ion: 91 Resp: 2254
Ion Ratio Lower Upper
91 100
106 26.2 23.7 35.5

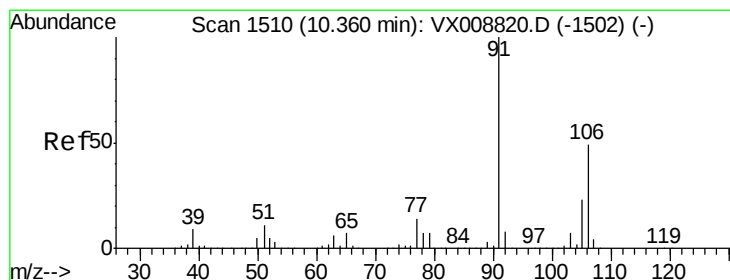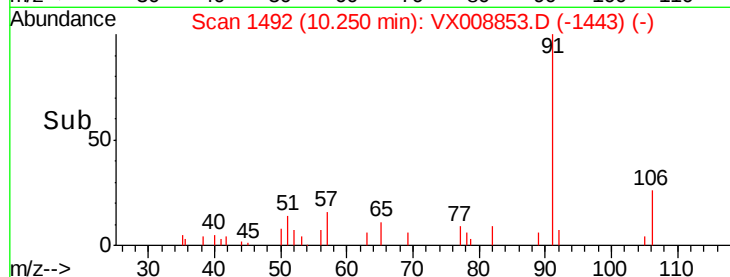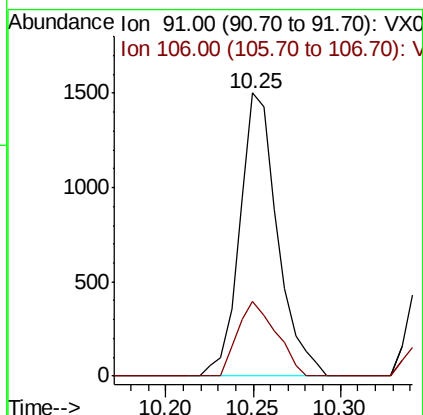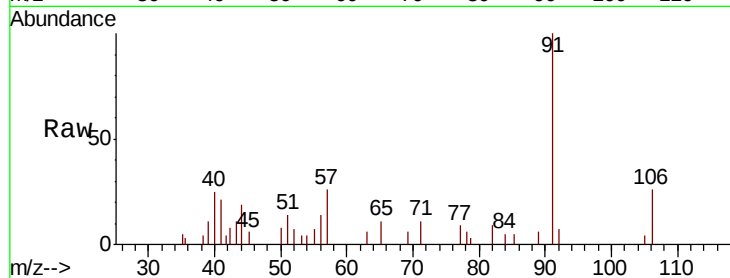

#68
m/p-Xylenes
Concen: 0.468 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. -0.00 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44

Tgt Ion: 106 Resp: 1633
Ion Ratio Lower Upper
106 100
91 208.2 168.5 252.7

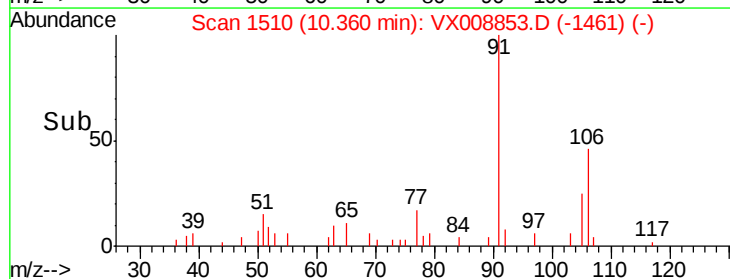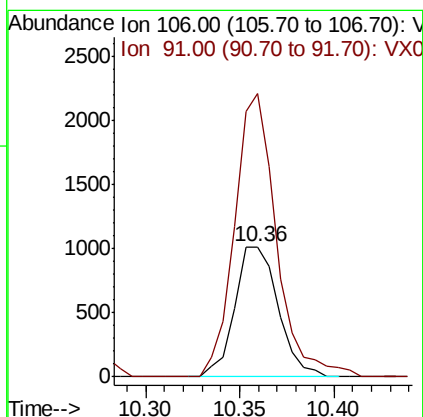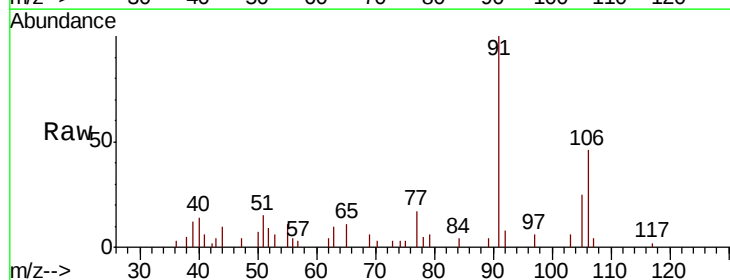


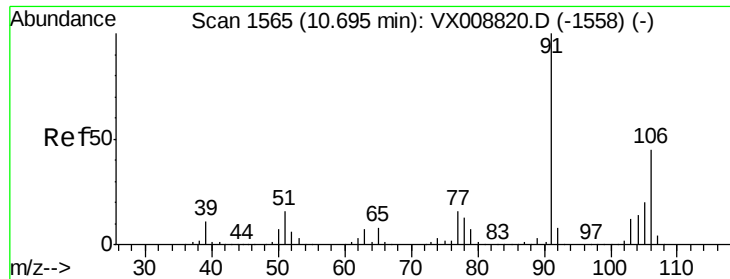




#69
o-Xylene
Concen: 0.229 ug/l
RT: 10.70 min Scan# 1566
Delta R.T. -0.00 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44

Instrument :
MSVOA_X
ClientSampleId :
20190171-COMP-CS-3ME

Tgt Ion:106 Resp: 775
Ion Ratio Lower Upper
106 100
91 202.6 111.5 334.4

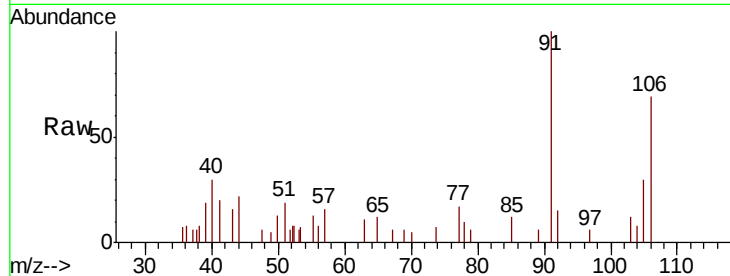


Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VX0

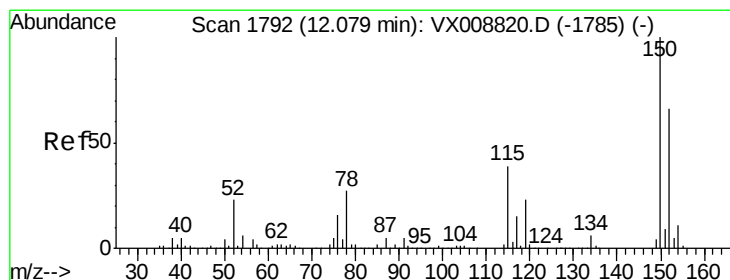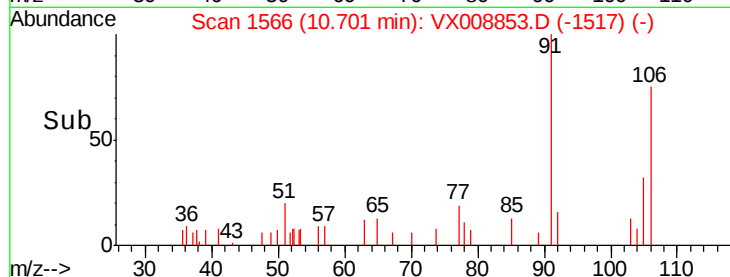
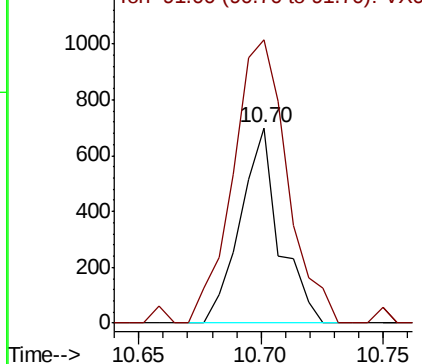



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX008853.D
Acq: 11 Apr 2019 15:44

Tgt Ion:152 Resp: 115018
Ion Ratio Lower Upper
152 100
115 60.3 43.5 130.5
150 158.0 0.0 348.8

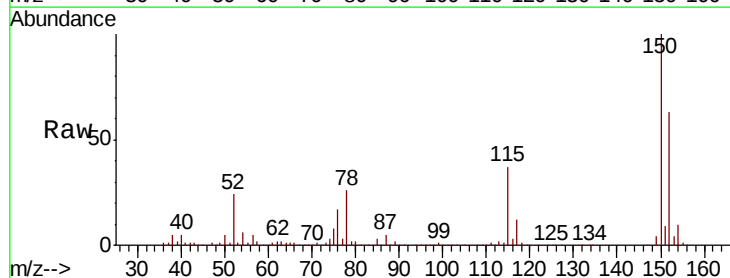

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

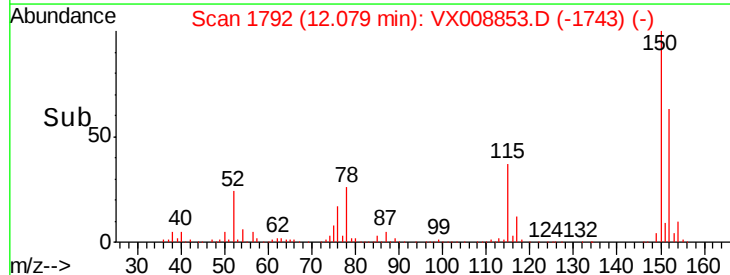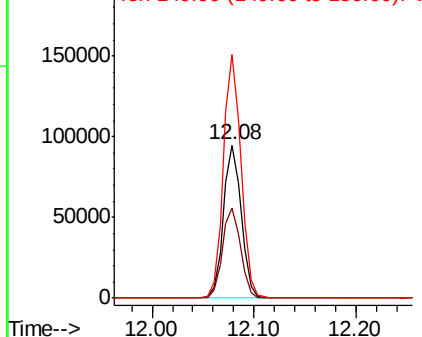

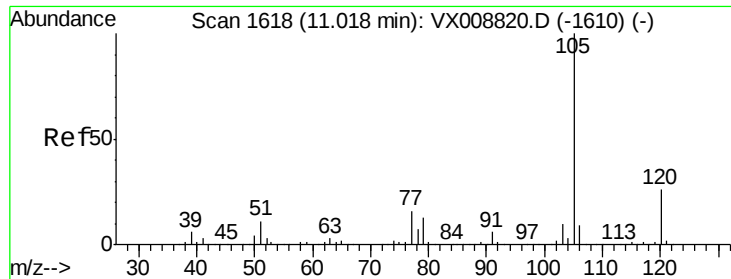

#73

Isopropylbenzene

Concen: 0.626 ug/l

RT: 11.02 min Scan# 1618

Delta R.T. -0.00 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :


20190171-COMP-CS-3ME

Tgt Ion: 105 Resp: 5969

Ion Ratio Lower Upper




105 100

120 26.9 12.9 38.6



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

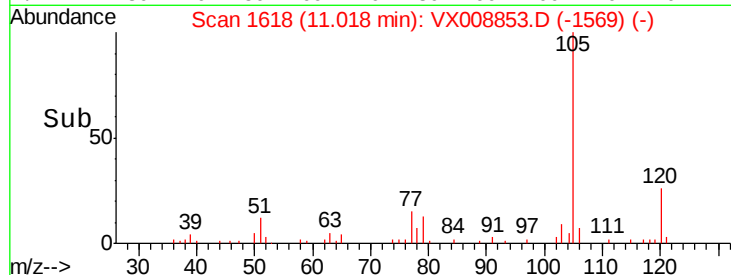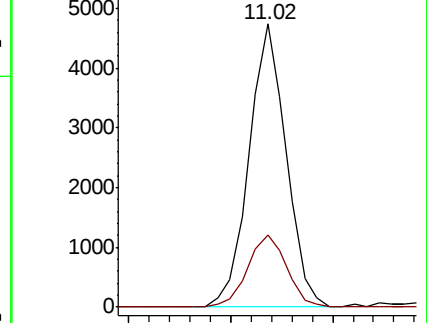

#76

1,2,3-Trichloropropane

Concen: 19.727 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. -0.16 min

Lab File: VX008853.D


Acq: 11 Apr 2019 15:44

Tgt Ion: 75 Resp: 62330

Ion Ratio Lower Upper



75 100


77 1.5 22.3 66.8#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

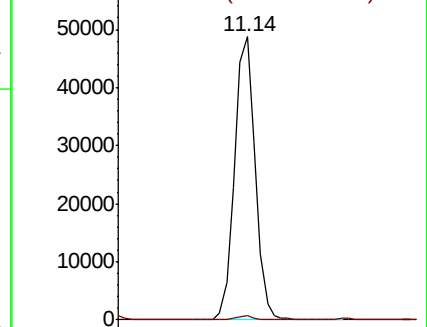



#79

2-Chlorotoluene

Concen: 0.415 ug/l

RT: 11.43 min Scan# 1685

Delta R.T. 0.01 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44

Instrument :

MSVOA_X

ClientSampleId :


20190171-COMP-CS-3ME

Tgt Ion: 91 Resp: 2786

Ion Ratio Lower Upper




91 100

126 27.7 16.1 48.3



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 125.90 (125.60 to 126.60): V

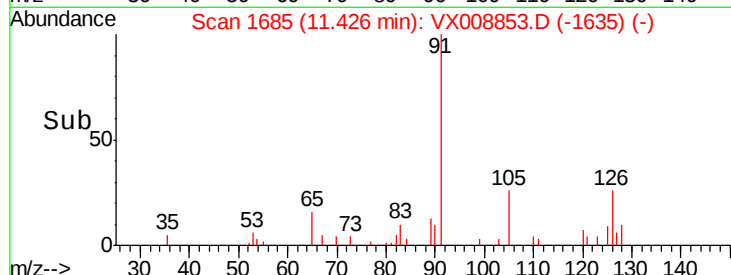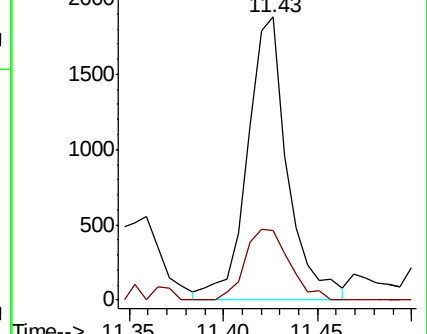

#81

trans-1,4-Dichloro-2-butene

Concen: 54.378 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. 0.07 min

Lab File: VX008853.D

Acq: 11 Apr 2019 15:44


Tgt Ion: 75 Resp: 62330

Ion Ratio Lower Upper

75 100

53 0.0 81.3 121.9#



89 0.0 35.6 53.4#




Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0




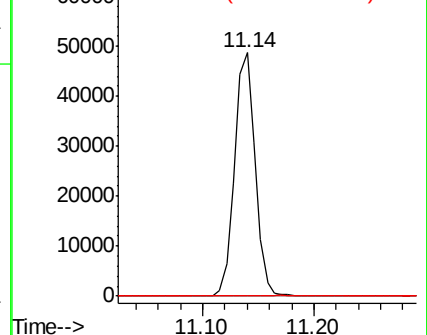




#84
 1,2,4-Trimethylbenzene
 Concen: 0.237 ug/l
 RT: 11.81 min Scan# 1748
 Delta R.T. 0.01 min
 Lab File: VX008853.D
 Acq: 11 Apr 2019 15:44

Instrument :
 MSVOA_X
 ClientSampleId :
 20190171-COMP-CS-3ME

Tgt Ion:105 Resp: 1921
 Ion Ratio Lower Upper
 105 100
 120 52.0 21.8 65.3

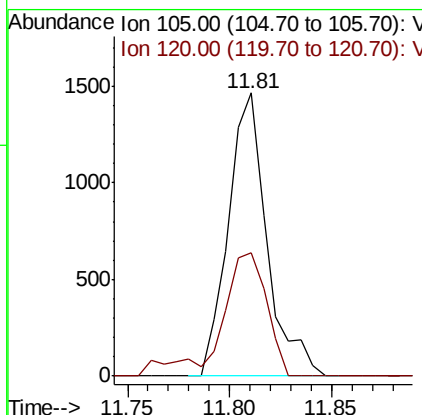

#95
 Naphthalene
 Concen: 0.295 ug/l
 RT: 13.83 min Scan# 2080
 Delta R.T. -0.00 min
 Lab File: VX008853.D
 Acq: 11 Apr 2019 15:44

Tgt Ion:128 Resp: 2789
 Ion Ratio Lower Upper
 128 100
 127 15.4 10.4 15.6
 129 14.2 8.6 13.0#

