

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
 Data File : VX035000.D
 Acq On : 11 Apr 2023 10:02
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
 Title : VOC Analysis

Signal : TIC: VX035000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	26	29	31	rBV2	2741	2498	0.14%	0.019%
2	1.368	42	46	58	rBV	211033	232649	13.19%	1.741%
3	1.672	92	96	109	rBV	166022	219684	12.45%	1.644%
4	2.307	194	200	213	rVB	380435	598334	33.92%	4.478%
5	2.398	213	215	217	rBV3	681	443	0.03%	0.003%
6	2.514	229	234	239	rVB3	1374	2433	0.14%	0.018%
7	2.672	258	260	263	rBV3	444	333	0.02%	0.002%
8	2.794	275	280	286	rVB4	1998	3454	0.20%	0.026%
9	3.001	312	314	320	rVB2	231	452	0.03%	0.003%
10	3.044	320	321	325	rBV2	265	324	0.02%	0.002%
11	3.075	325	326	328	rBV	290	294	0.02%	0.002%
12	3.105	328	331	335	rVB3	532	750	0.04%	0.006%
13	3.251	350	355	357	rBV3	242	378	0.02%	0.003%
14	3.276	357	359	360	rVV	288	223	0.01%	0.002%
15	3.300	360	363	364	rVB2	392	334	0.02%	0.002%
16	3.331	366	368	371	rBV3	413	406	0.02%	0.003%
17	3.392	377	378	381	rVV	212	239	0.01%	0.002%
18	3.489	392	394	397	rBV	329	223	0.01%	0.002%
19	3.587	407	410	413	rBV2	430	506	0.03%	0.004%
20	3.885	456	459	461	rVB2	188	222	0.01%	0.002%
21	3.953	468	470	471	rBV	338	236	0.01%	0.002%
22	3.971	471	473	474	rVV2	391	260	0.01%	0.002%
23	4.032	482	483	485	rBV	314	264	0.01%	0.002%
24	4.111	494	496	499	rVV2	291	290	0.02%	0.002%
25	4.282	522	524	528	rVV2	289	312	0.02%	0.002%
26	4.465	543	554	579	rBV	106178	356371	20.20%	2.667%
27	4.654	583	585	591	rVB4	439	575	0.03%	0.004%
28	4.965	634	636	638	rBV2	274	267	0.02%	0.002%
29	5.056	638	651	669	rBV	226462	696541	39.49%	5.213%
30	5.306	689	692	695	rBV2	239	293	0.02%	0.002%
31	5.391	699	706	712	rVV3	1636	4135	0.23%	0.031%
32	5.471	718	719	723	rVB3	450	320	0.02%	0.002%
33	5.556	724	733	743	rBV5	3865	10899	0.62%	0.082%
34	5.873	784	785	788	rVB	287	239	0.01%	0.002%
35	5.964	788	800	821	rBV2	580692	1763840	100.00%	13.200%
36	6.275	845	851	853	rBV2	380	608	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
 Data File : VX035000.D
 Acq On : 11 Apr 2023 10:02
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
 Title : VOC Analysis

37	6.452	876	880	881	rBV2	218	304	0.02%	0.002%
38	6.684	916	918	921	rVV2	381	294	0.02%	0.002%
39	6.757	921	930	953	rVV	519623	1244498	70.56%	9.314%
40	7.111	981	988	995	rBV5	5829	13591	0.77%	0.102%
41	7.208	1001	1004	1006	rBV3	383	343	0.02%	0.003%
42	7.306	1011	1020	1038	rBV	372962	811220	45.99%	6.071%
43	7.476	1044	1048	1049	rBV4	706	984	0.06%	0.007%
44	7.580	1064	1065	1067	rBV	337	239	0.01%	0.002%
45	7.793	1096	1100	1105	rBV	308	585	0.03%	0.004%
46	7.940	1119	1124	1128	rBV2	1379	2060	0.12%	0.015%
47	8.110	1149	1152	1153	rVB2	513	309	0.02%	0.002%
48	8.129	1153	1155	1159	rVB	218	309	0.02%	0.002%
49	8.324	1181	1187	1202	rBV	224735	370562	21.01%	2.773%
50	8.586	1229	1230	1232	rVB	456	220	0.01%	0.002%
51	8.647	1234	1240	1252	rBV	897795	1394801	79.08%	10.439%
52	8.952	1284	1290	1301	rBV	152845	235939	13.38%	1.766%
53	9.275	1340	1343	1346	rVB4	1185	1110	0.06%	0.008%
54	9.384	1355	1361	1383	rBV	527008	760643	43.12%	5.693%
55	9.762	1421	1423	1426	rVB3	356	305	0.02%	0.002%
56	9.860	1436	1439	1440	rBV2	304	258	0.01%	0.002%
57	9.958	1452	1455	1457	rBV2	483	484	0.03%	0.004%
58	10.055	1465	1471	1489	rBV	986937	1394322	79.05%	10.435%
59	10.250	1501	1503	1509	rVB3	335	309	0.02%	0.002%
60	10.299	1509	1511	1514	rBV2	738	1006	0.06%	0.008%
61	10.378	1523	1524	1527	rVB2	433	344	0.02%	0.003%
62	10.409	1527	1529	1533	rBV2	174	243	0.01%	0.002%
63	10.518	1546	1547	1552	rVB2	332	431	0.02%	0.003%
64	10.646	1565	1568	1569	rBV2	833	569	0.03%	0.004%
65	10.860	1598	1603	1606	rBV2	274	504	0.03%	0.004%
66	10.963	1615	1620	1625	rBV5	819	1435	0.08%	0.011%
67	11.018	1628	1629	1632	rVB	409	229	0.01%	0.002%
68	11.079	1635	1639	1640	rBV2	462	405	0.02%	0.003%
69	11.098	1640	1642	1643	rVB2	318	222	0.01%	0.002%
70	11.189	1652	1657	1667	rBV	582058	753787	42.74%	5.641%
71	11.451	1697	1700	1704	rVV3	823	1136	0.06%	0.009%
72	11.622	1726	1728	1730	rBV2	320	262	0.01%	0.002%
73	11.665	1733	1735	1737	rVV2	186	224	0.01%	0.002%
74	11.713	1740	1743	1746	rVV2	405	543	0.03%	0.004%
75	11.750	1746	1749	1753	rVB2	734	1001	0.06%	0.007%
76	11.823	1759	1761	1765	rBV3	227	251	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
 Data File : VX035000.D
 Acq On : 11 Apr 2023 10:02
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK620

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
 Title : VOC Analysis

77	11.866	1765	1768	1772	rVV3	239	359	0.02%	0.003%
78	11.975	1781	1786	1788	rBV4	832	1037	0.06%	0.008%
79	12.018	1788	1793	1810	rVV	984077	1281094	72.63%	9.588%
80	12.317	1837	1842	1859	rVB	932842	1171250	66.40%	8.765%
81	12.500	1870	1872	1873	rBV	368	253	0.01%	0.002%
82	12.573	1881	1884	1885	rBV	364	274	0.02%	0.002%
83	12.756	1913	1914	1917	rBV2	377	347	0.02%	0.003%
84	12.859	1929	1931	1933	rBV2	390	290	0.02%	0.002%
85	13.122	1970	1974	1977	rBV2	937	1057	0.06%	0.008%
86	13.274	1996	1999	2002	rBV2	388	433	0.02%	0.003%
87	13.390	2016	2018	2021	rBV2	149	221	0.01%	0.002%
88	13.445	2025	2027	2030	rBV2	276	285	0.02%	0.002%
89	13.469	2030	2031	2034	rBV2	207	219	0.01%	0.002%
90	13.591	2047	2051	2056	rVB4	1557	2030	0.12%	0.015%
91	13.652	2059	2061	2063	rBV2	315	298	0.02%	0.002%
92	13.725	2071	2073	2074	rBV	250	218	0.01%	0.002%
93	13.780	2076	2082	2088	rVV3	1098	2073	0.12%	0.016%
94	13.823	2088	2089	2094	rVB3	458	493	0.03%	0.004%
95	13.963	2109	2112	2116	rBV5	1540	1921	0.11%	0.014%
96	14.103	2134	2135	2138	rBV2	291	333	0.02%	0.002%
97	15.213	2315	2317	2318	rBV	617	358	0.02%	0.003%
98	16.347	2502	2503	2505	rBV	776	494	0.03%	0.004%
99	16.517	2529	2531	2535	rVB3	700	504	0.03%	0.004%
100	16.548	2535	2536	2538	rBV	603	301	0.02%	0.002%


Sum of corrected areas: 13362052

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
Data File : VX035000.D
Acq On : 11 Apr 2023 10:02
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

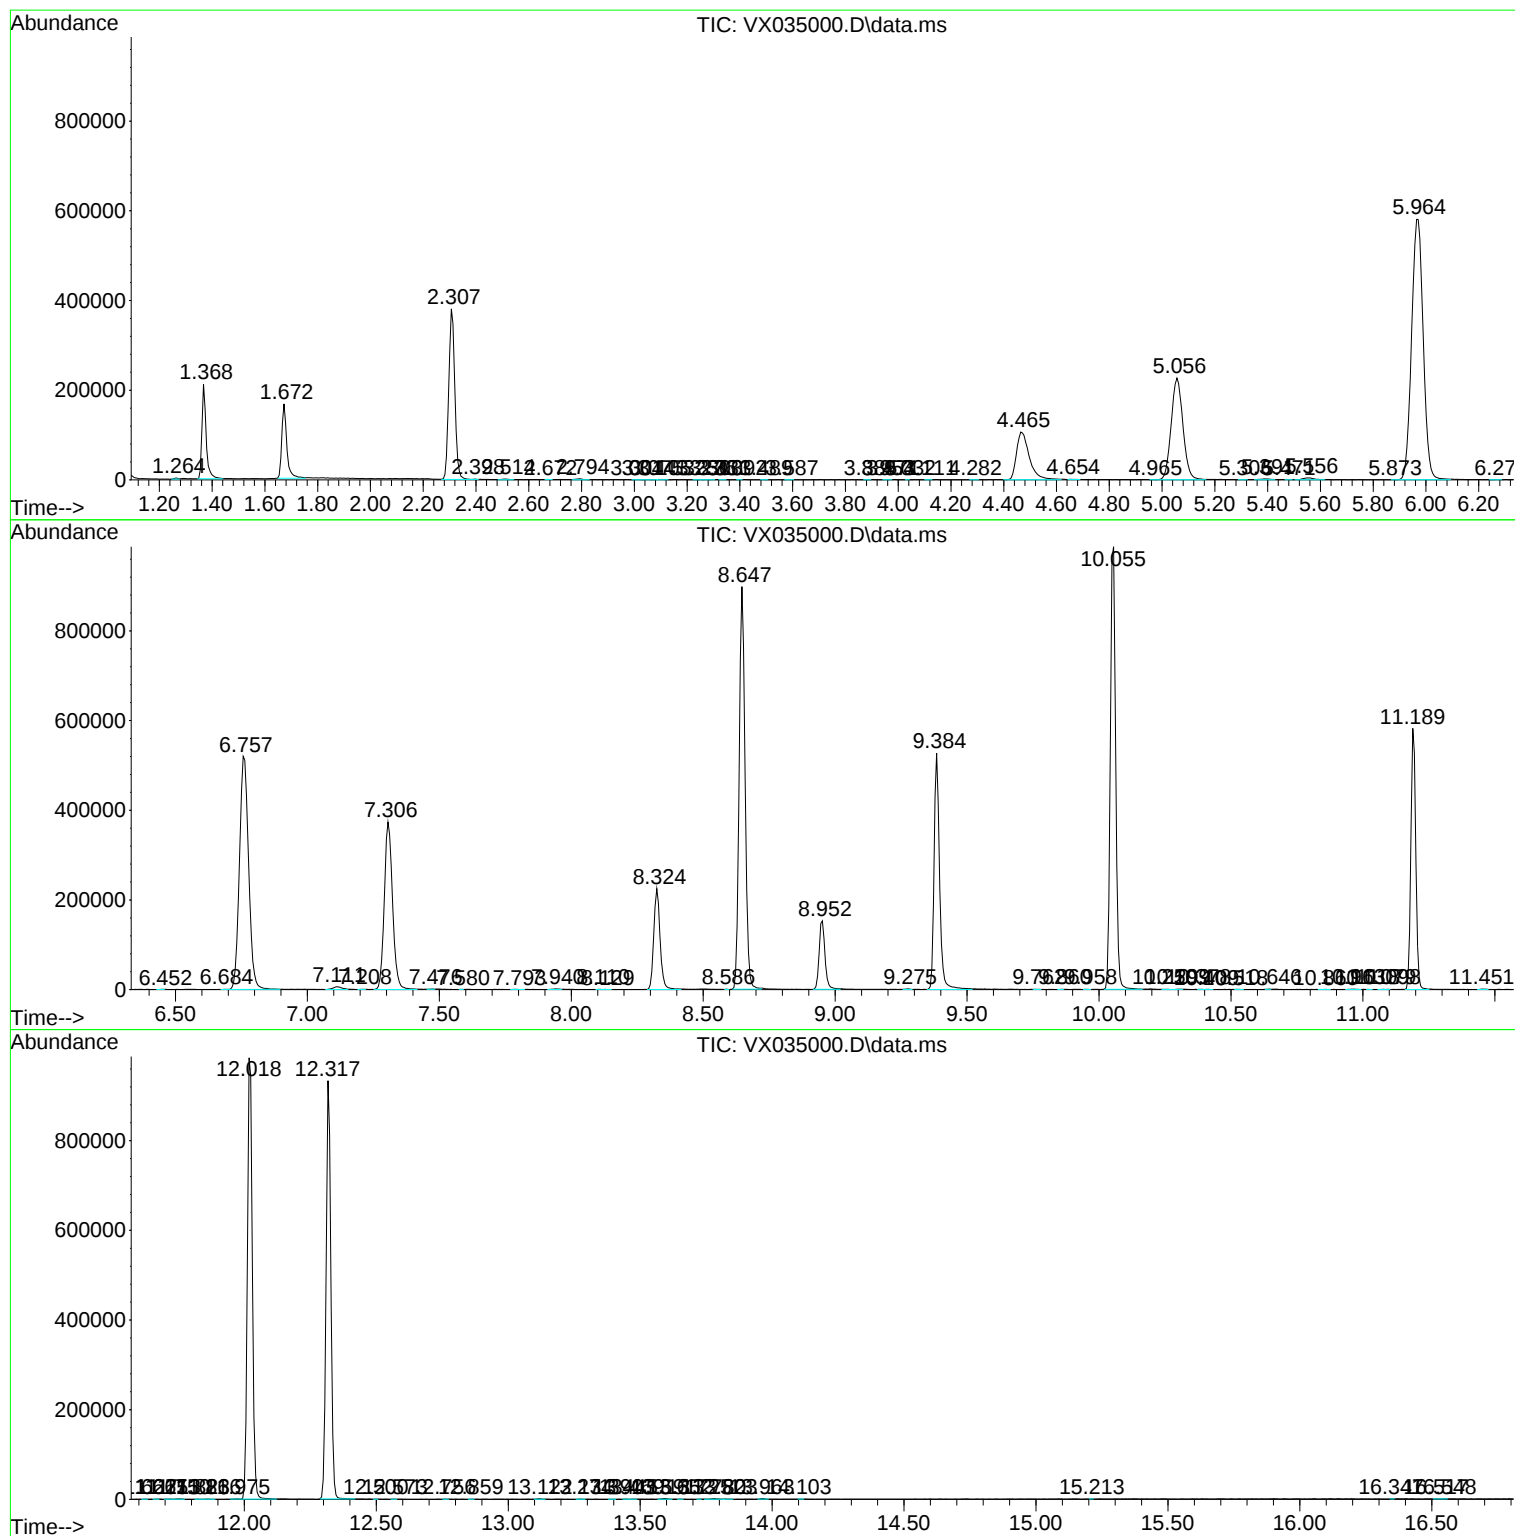

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
Data File : VX035000.D
Acq On : 11 Apr 2023 10:02
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
Data File : VX035000.D
Acq On : 11 Apr 2023 10:02
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK620

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041023WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc