
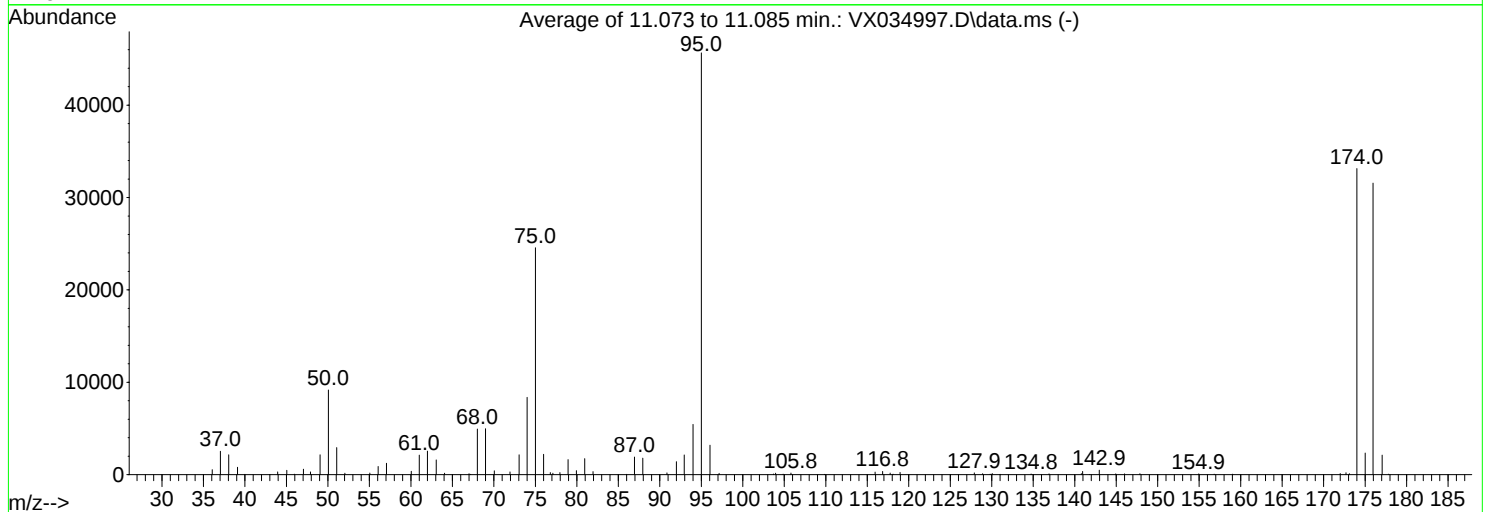


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041123\
Data File : VX034997.D
Acq On : 11 Apr 2023 08:19
Operator : JC/MD
Sample : BFB622
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB622

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM041023WMA.M
Title : VOC Analysis
Last Update : Wed Apr 12 01:54:54 2023

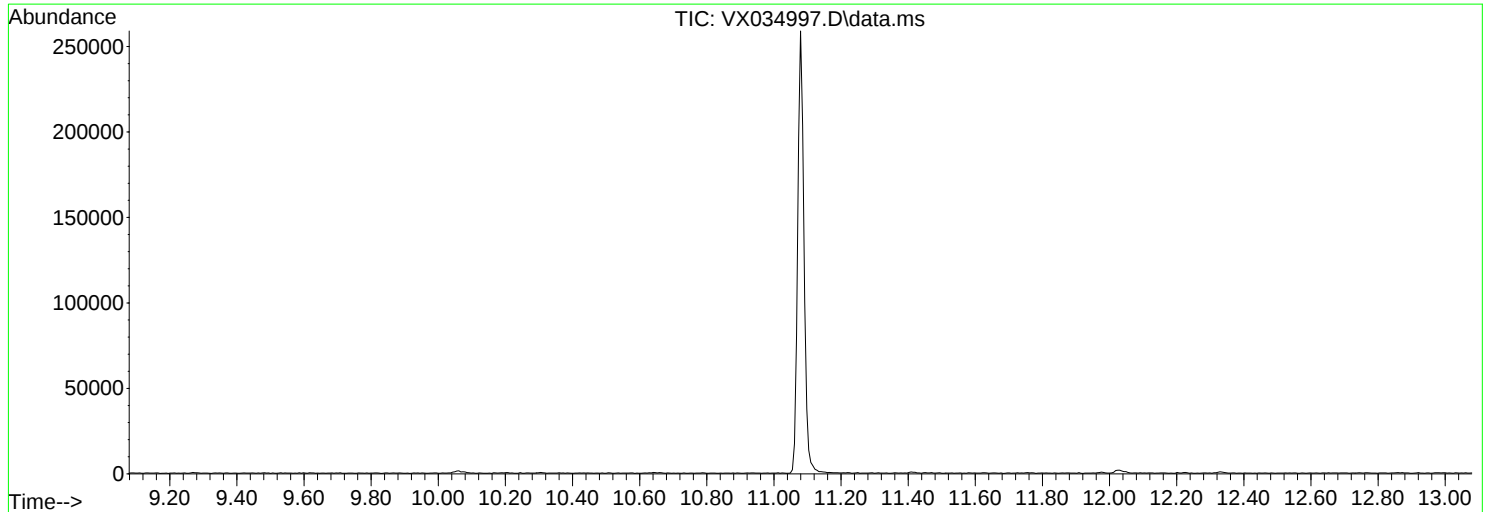

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.1	9166	PASS
75	95	30	80	53.8	24563	PASS
95	95	100	100	100.0	45664	PASS
96	95	5	9	7.0	3181	PASS
173	174	0.00	2	0.6	201	PASS
174	95	50	120	72.6	33141	PASS
175	174	5	9	7.1	2344	PASS
176	174	95	101	95.2	31563	PASS
177	176	5	9	6.7	2118	PASS

m/z	Abundance
40.10	191.0
44.00	187.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622

m/z	Abundance
36.10	591.0
37.00	2523.0
38.00	2588.0
39.10	836.0
40.00	265.0
44.00	570.0
45.00	430.0
45.90	78.0
47.10	708.0
47.90	317.0
49.00	2212.0
50.00	8880.0
51.00	2645.0
52.00	183.0
55.00	234.0
56.00	879.0
57.10	1091.0
60.00	386.0
61.00	1945.0
62.00	2322.0
63.10	1450.0
64.10	193.0
67.00	99.0
68.00	4910.0
69.00	4455.0
70.10	272.0
72.00	211.0
73.10	1895.0
74.00	7643.0
75.00	23480.0
76.00	2270.0
77.10	460.0
77.90	169.0
78.90	1494.0
80.00	329.0
80.90	1430.0
82.00	336.0
87.00	2008.0
87.90	1491.0
90.80	195.0
92.00	1316.0
92.90	1810.0
94.00	5096.0
95.00	41704.0
96.00	3308.0
97.10	161.0
104.00	193.0
105.80	111.0
115.90	224.0
116.90	325.0
117.70	195.0
118.90	288.0
127.90	160.0
128.80	96.0
129.80	156.0
134.70	82.0
136.90	80.0
140.80	302.0
143.00	395.0
146.00	56.0
147.90	114.0
159.10	53.0
172.00	69.0
173.10	318.0
174.00	26312.0
175.00	1769.0
176.00	24808.0
177.00	2113.0
177.90	68.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622

m/z	Abundance
36.00	574.0
37.00	2890.0
38.10	2125.0
39.10	994.0
39.90	224.0
43.90	470.0
45.00	566.0
46.00	55.0
47.00	697.0
47.90	410.0
49.10	2590.0
50.10	10793.0
51.10	3661.0
52.10	157.0
55.10	139.0
56.00	957.0
57.00	1380.0
60.10	420.0
61.00	2429.0
62.00	3013.0
63.00	1894.0
64.00	137.0
67.00	220.0
68.00	5853.0
69.00	5711.0
70.00	523.0
71.90	412.0
73.00	2761.0
74.00	9811.0
75.00	29544.0
76.00	2656.0
76.80	364.0
78.00	280.0
79.00	1937.0
79.90	569.0
80.90	2224.0
81.90	388.0
86.90	2135.0
87.90	2078.0
90.90	213.0
92.00	1563.0
93.00	2751.0
94.00	6674.0
95.00	53736.0
96.10	3478.0
97.10	145.0
103.70	201.0
104.90	74.0
105.80	269.0
109.90	66.0
116.00	319.0
116.80	417.0
117.70	150.0
118.10	179.0
118.90	229.0
127.90	182.0
128.90	136.0
130.00	213.0
131.00	97.0
134.80	136.0
136.80	88.0
141.00	603.0
142.90	592.0
145.00	166.0
146.00	139.0
147.80	123.0
155.00	129.0
156.90	81.0
159.00	121.0
172.00	132.0
172.80	361.0
174.00	38800.0
175.00	2939.0
176.00	37232.0
177.00	2200.0
177.80	80.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622

m/z	Abundance
36.00	425.0
37.10	2153.0
38.10	1759.0
39.00	570.0
39.90	204.0
43.00	58.0
44.00	428.0
45.10	409.0
47.00	375.0
47.90	177.0
49.00	1621.0
50.00	7826.0
51.00	2467.0
52.00	127.0
55.00	156.0
56.10	798.0
57.00	1195.0
60.00	276.0
61.00	1970.0
62.00	2310.0
63.00	1432.0
64.00	151.0
67.20	127.0
68.00	4044.0
69.00	4772.0
70.00	466.0
72.00	287.0
73.00	1794.0
74.00	7636.0
75.00	20664.0
76.00	1692.0
76.80	340.0
77.90	218.0
78.90	1440.0
79.90	401.0
81.00	1547.0
81.90	262.0
86.00	117.0
87.00	1569.0
88.00	1765.0
90.90	165.0
92.00	1324.0
93.00	1851.0
94.00	4569.0
95.00	41552.0
96.00	2758.0
97.20	130.0
103.90	277.0
104.80	80.0
105.80	157.0
109.80	55.0
115.90	312.0
116.80	315.0
117.80	201.0
119.00	216.0
127.90	227.0
129.00	73.0
130.10	149.0
135.00	76.0
137.00	74.0
140.90	458.0
141.80	60.0
143.00	495.0
144.90	91.0
145.90	60.0
147.80	77.0
154.90	132.0
156.70	64.0
172.00	163.0
172.60	241.0
174.00	34312.0
175.00	2323.0
175.90	32648.0
177.10	2041.0

Instrument :
MSVOA_X
ClientSampleId :
BFB622