




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

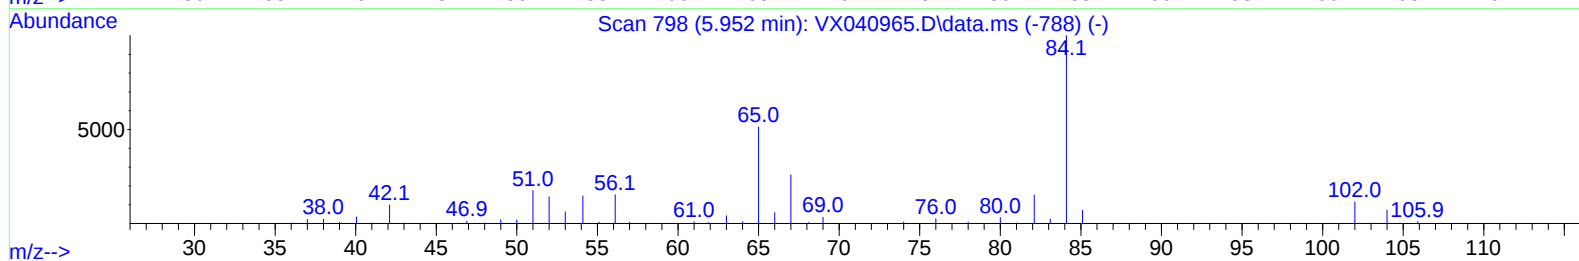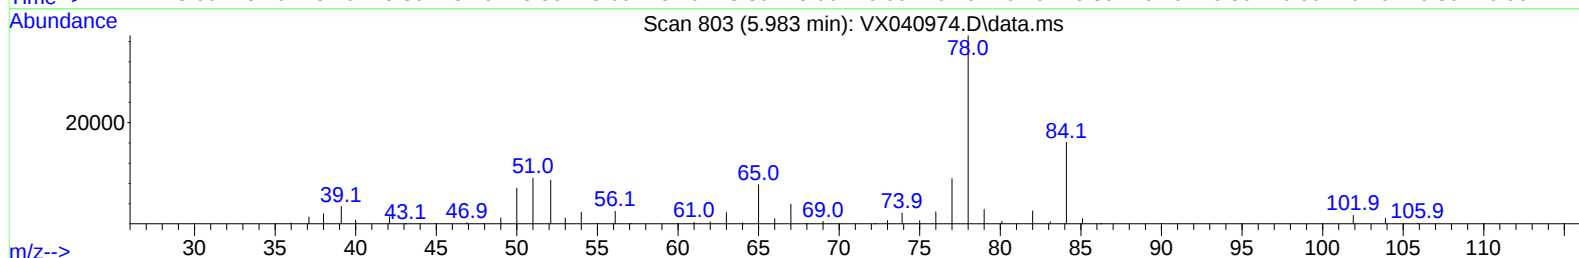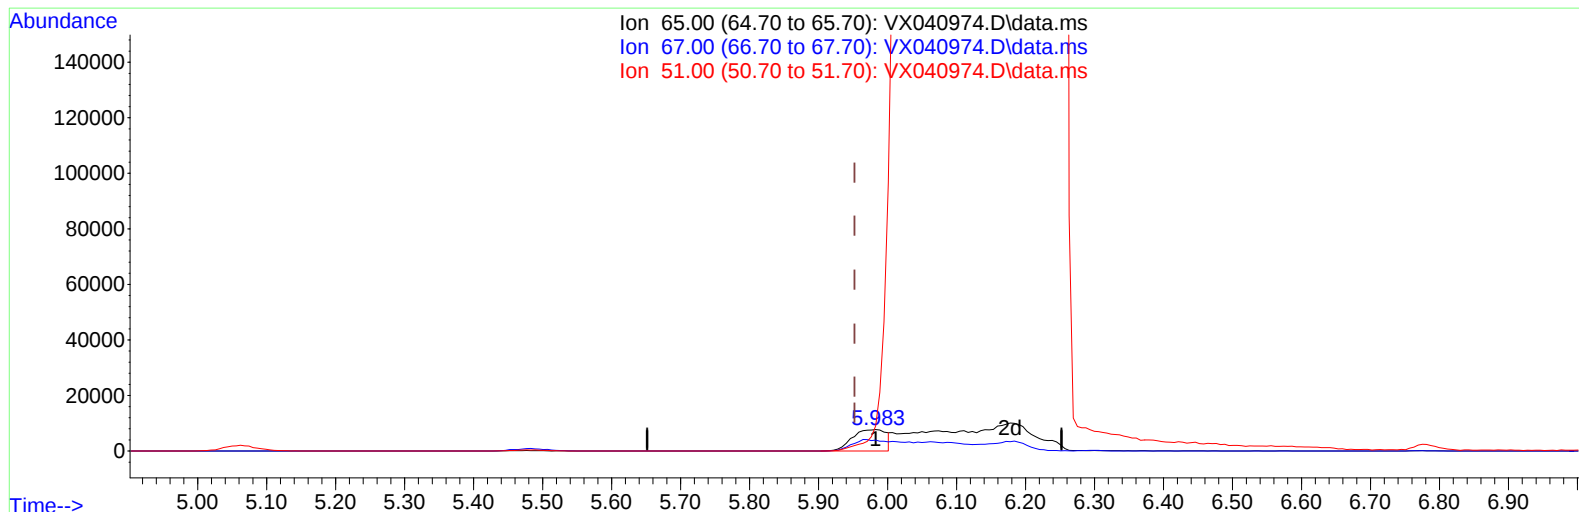

TIC: VX040974.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

5.983min (+ 0.031) 10.52 ug/L

response 26754

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	51.26
51.00	35.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

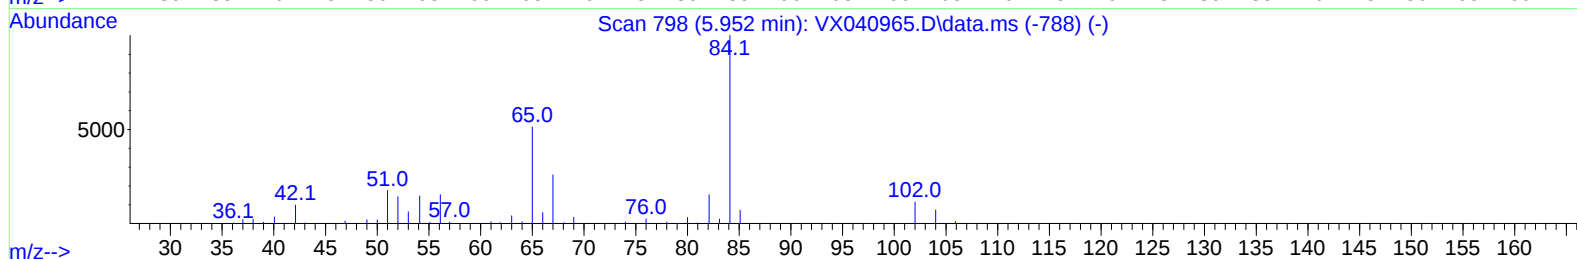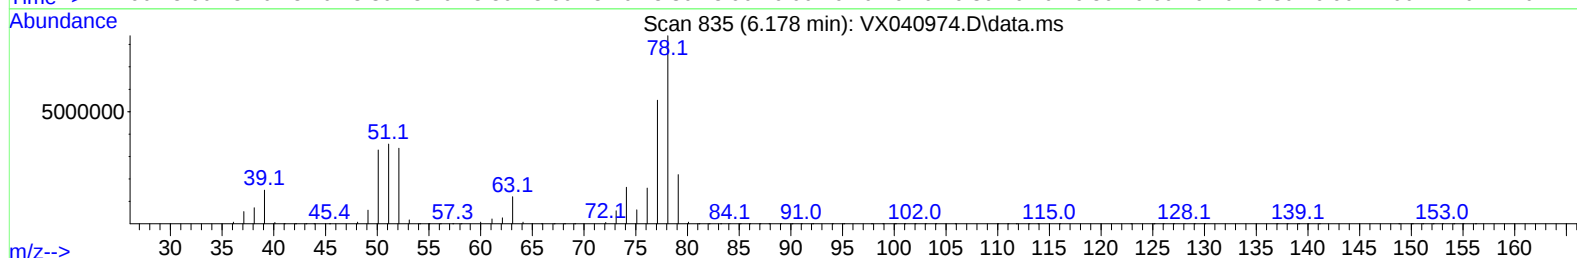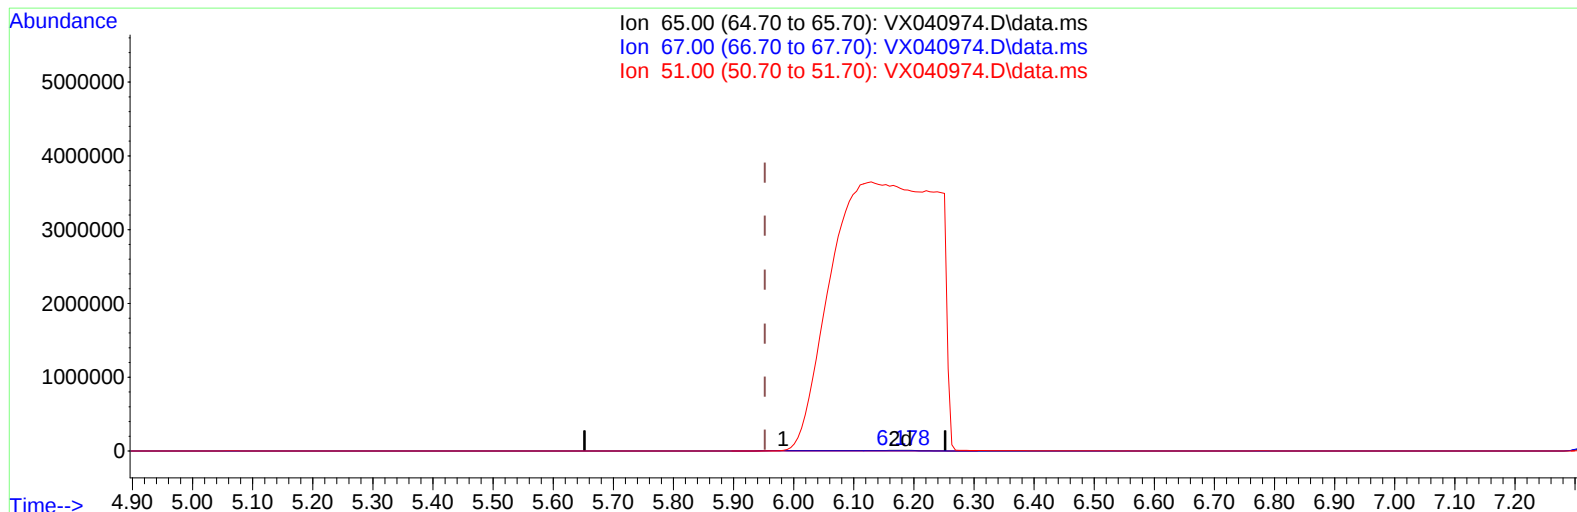

TIC: VX040974.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

6.178min (+ 0.226) 50.97 ug/L m

response 129604

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	10.58#
51.00	35.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

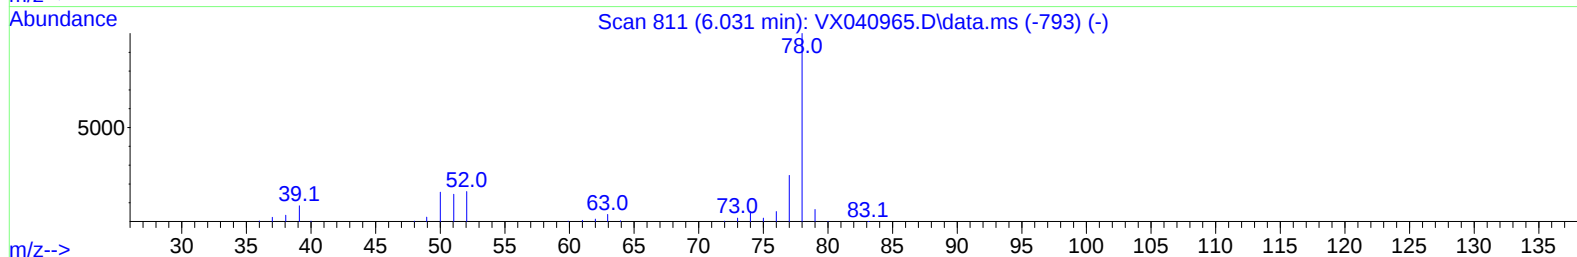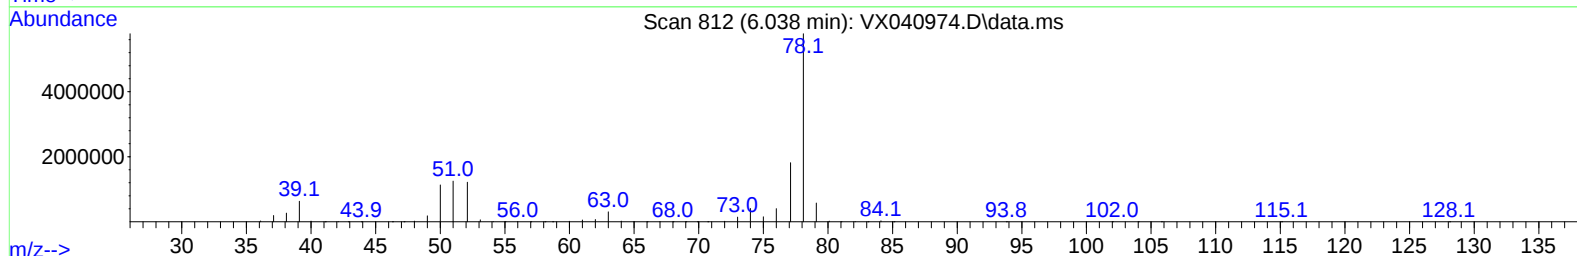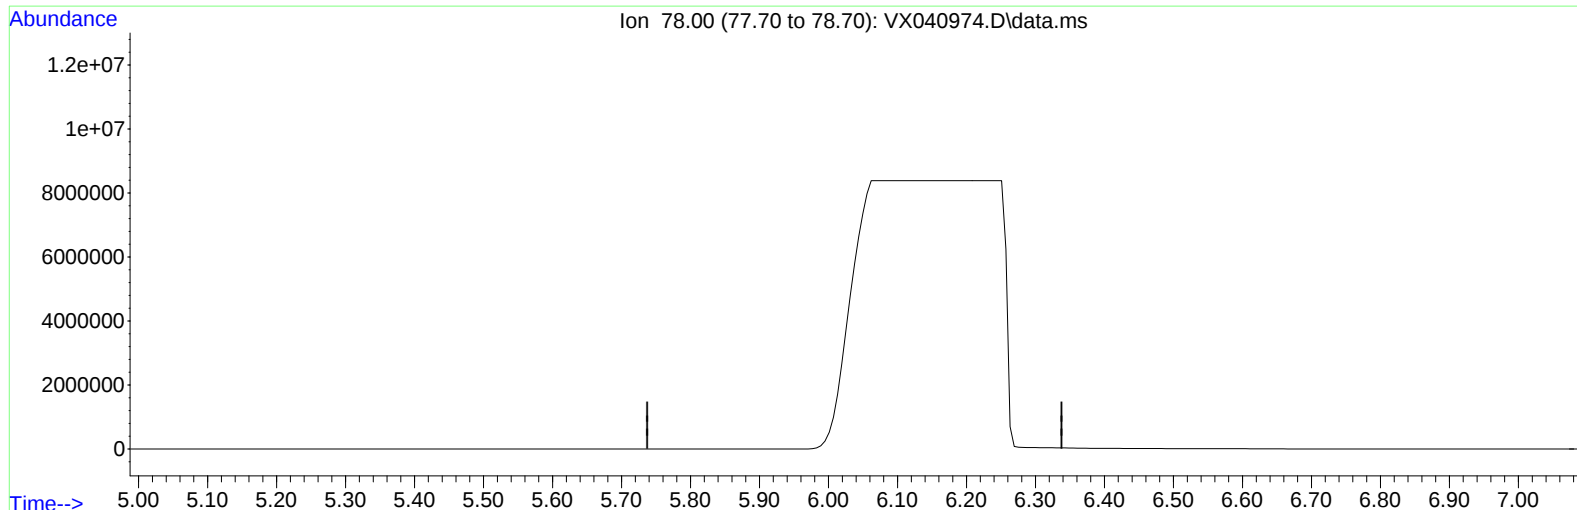

TIC: VX040974.D\data.ms

(33) Benzene (T)

6.038min (-6.038) 0.00 ug/L

response 0

Ion	Exp%	Act%
78.00	100.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

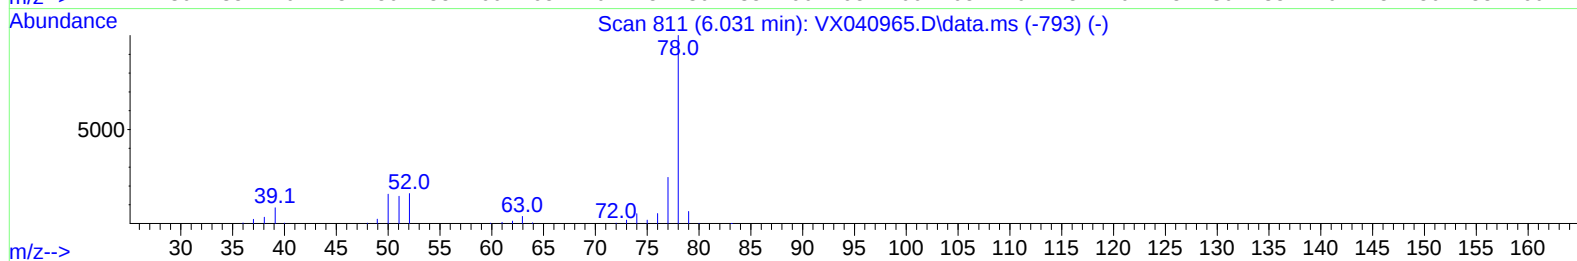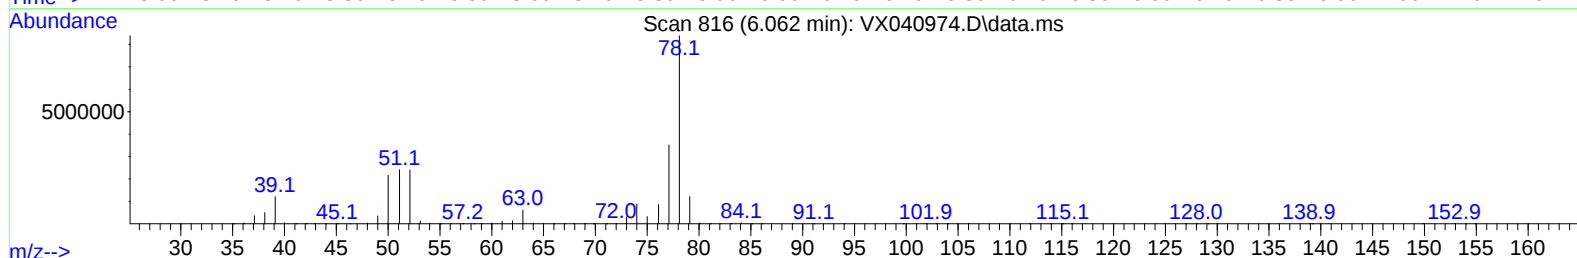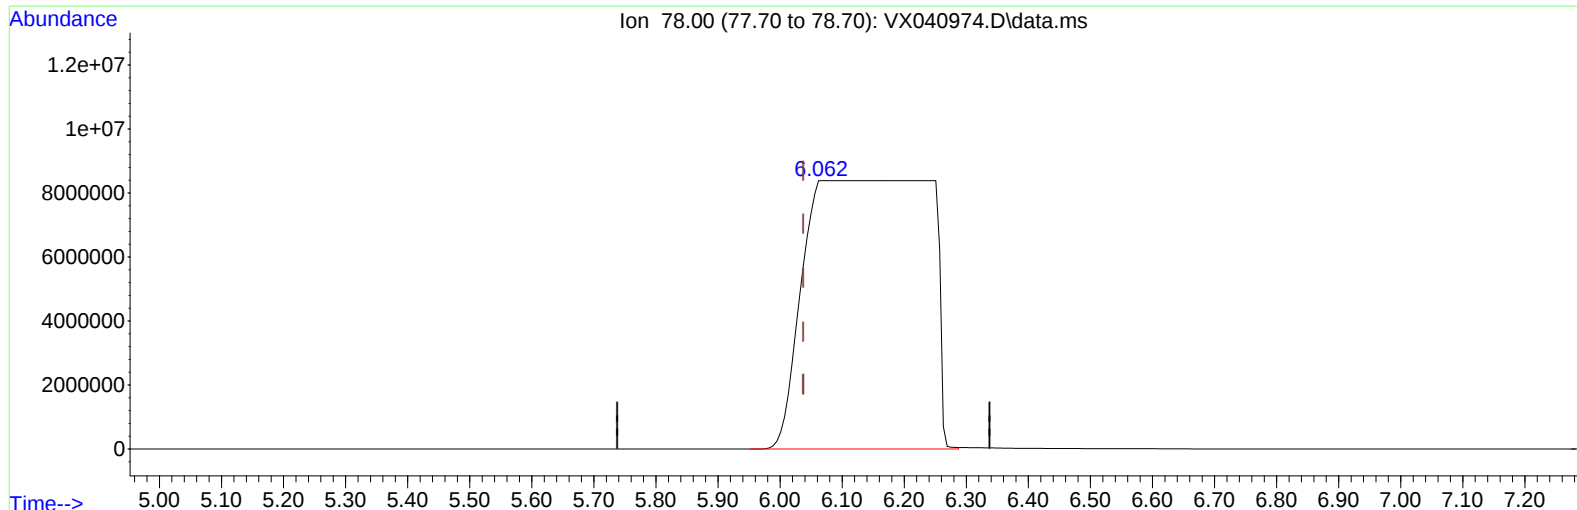

TIC: VX040974.D\data.ms

(33) Benzene (T)

6.062min (+ 0.024) 22941.42 ug/L m

response 116389574

Ion	Exp%	Act%
78.00	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

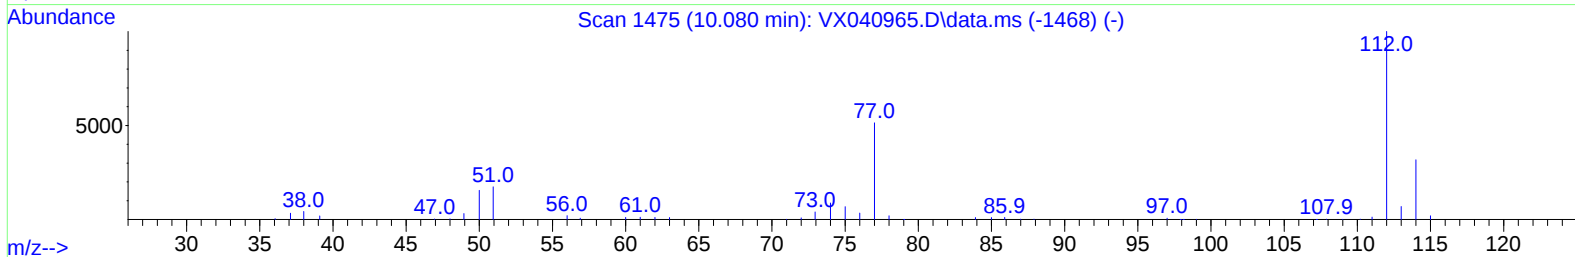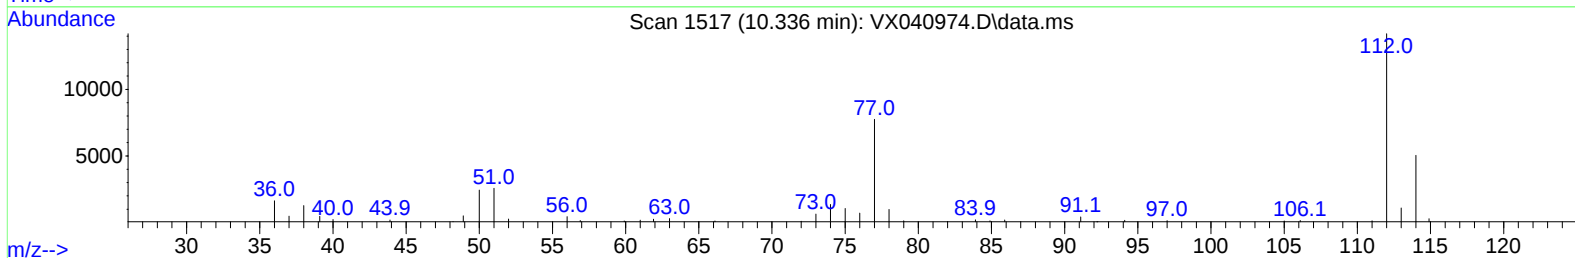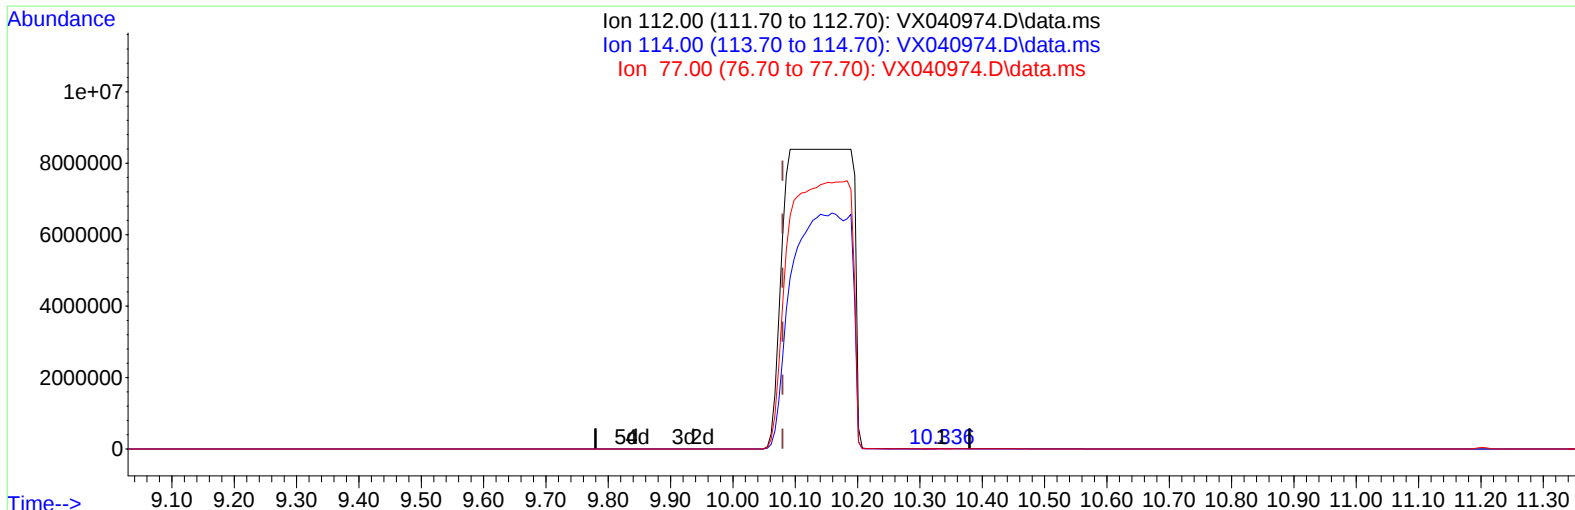

TIC: VX040974.D\data.ms

(51) Chlorobenzene (T)

10.336min (+ 0.256) 3.66 ug/L

response 14411

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	32.90	35.61
77.00	54.20	54.64
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

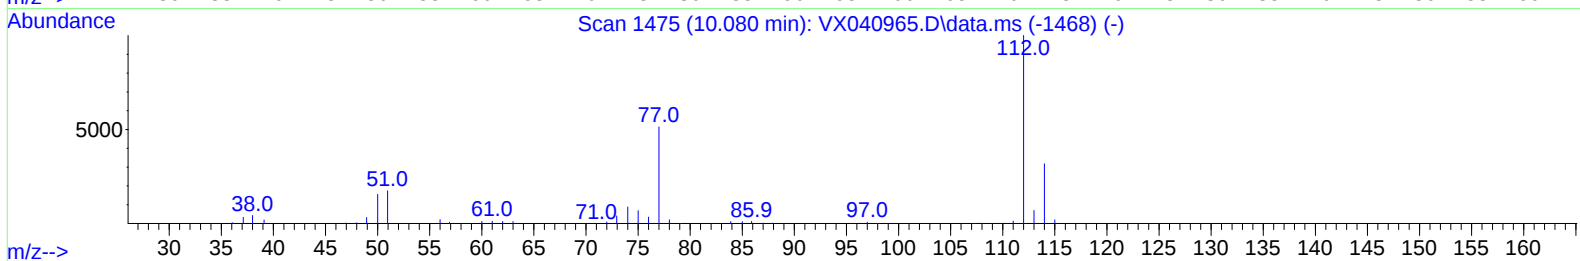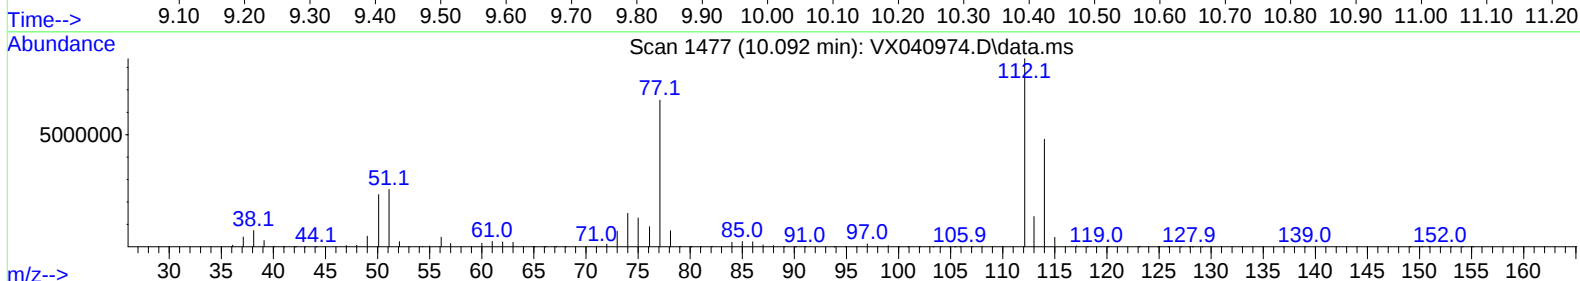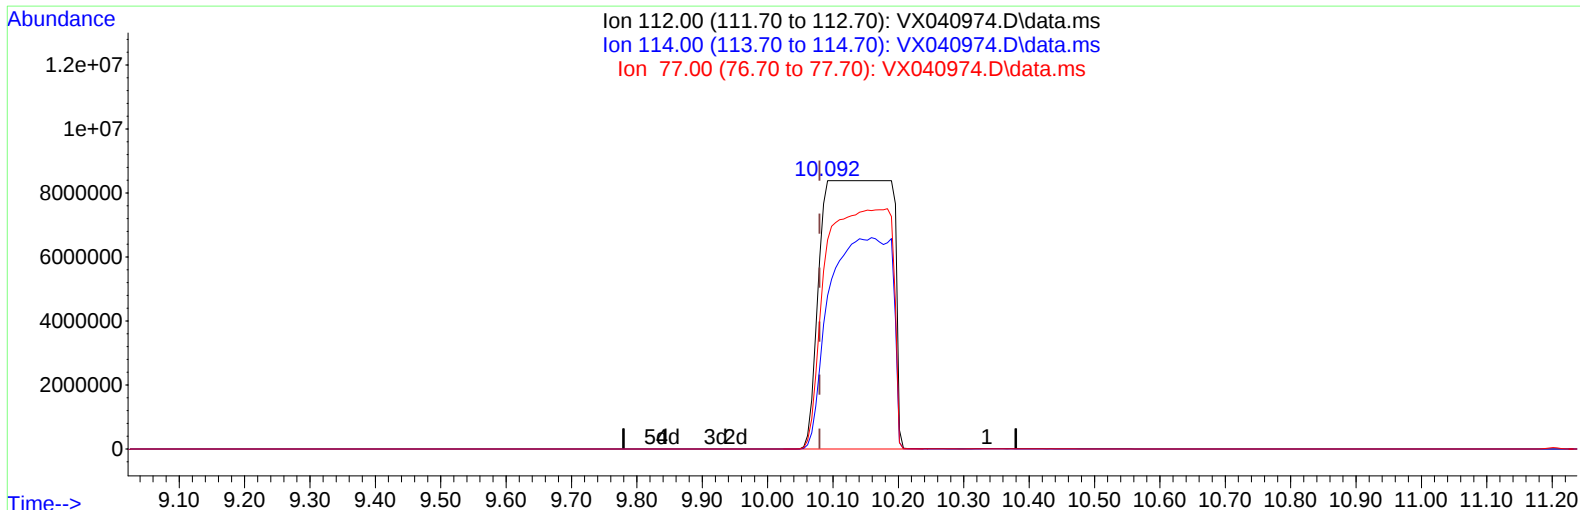

TIC: VX040974.D\data.ms

(51) Chlorobenzene (T)

10.092min (+ 0.012) 15824.40 ug/L m

response 62307047

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	32.90	57.19#
77.00	54.20	77.94#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040974.D
 Acq On : 11 Apr 2024 13:13
 Operator : JC/MD
 Sample : P2048-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:46:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 05:36:34 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 04/12/2024
 Supervised By :Semsettin Yesilyurt 04/12/2024

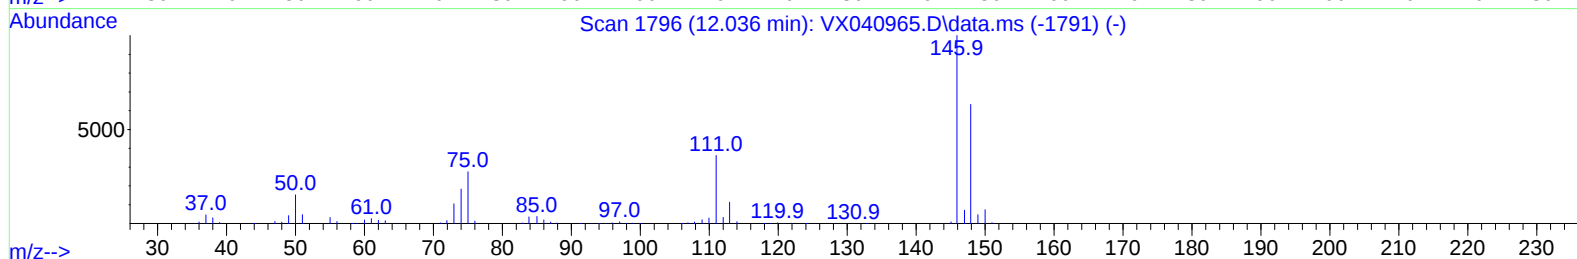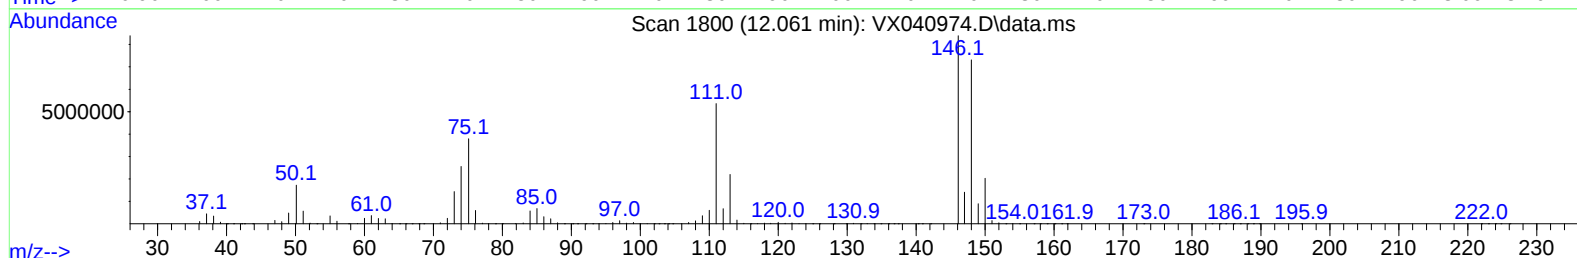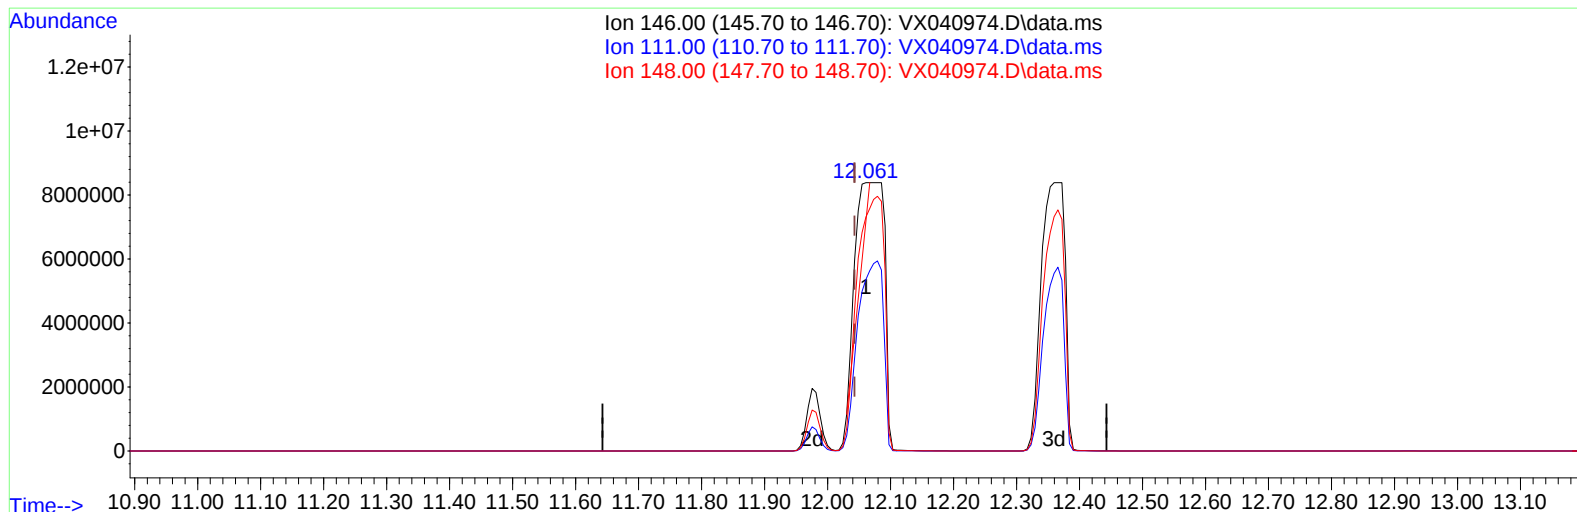

TIC: VX040974.D\data.ms

(65) 1,4-Dichlorobenzene (T)

12.061min (+ 0.018) 988.83 ug/L

response 5254128

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	33.50	63.90#
148.00	63.10	87.15#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

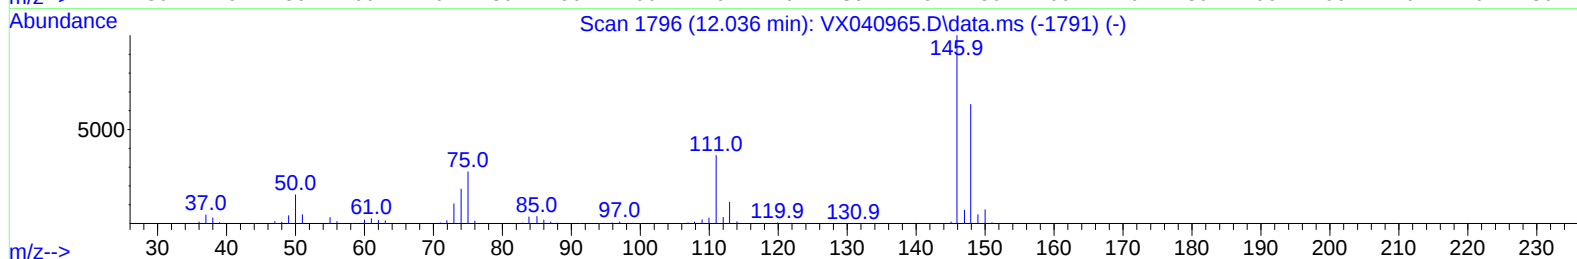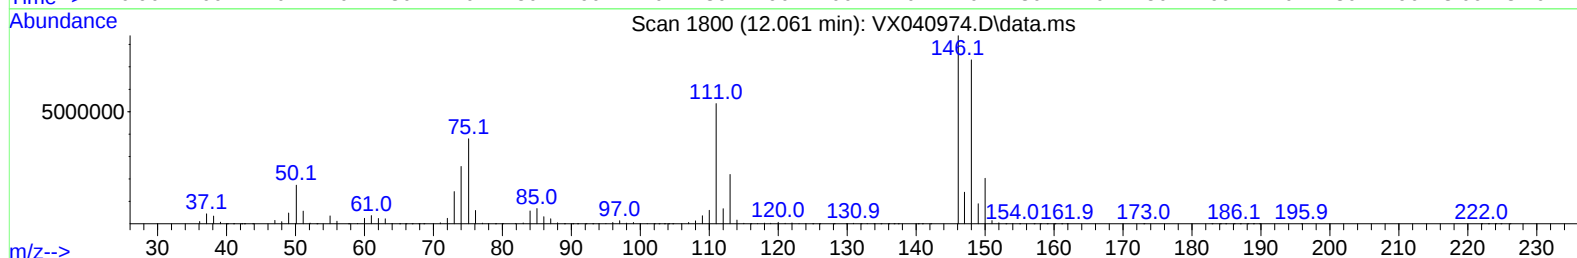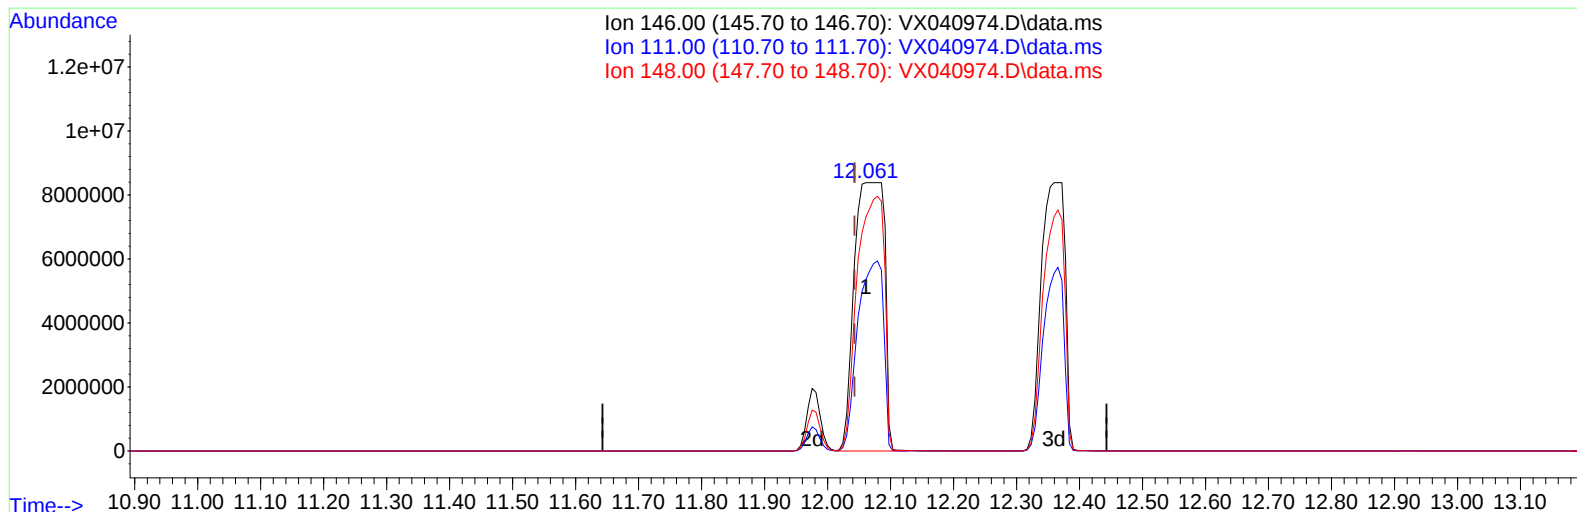

TIC: VX040974.D\data.ms

(65) 1,4-Dichlorobenzene (T)

12.061min (+ 0.018) 5262.42 ug/L m

response 27961855

Ion	Exp%	Act%
146.00	100.00	100.00
111.00	33.50	63.90#
148.00	63.10	87.15#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040974.D
 Acq On : 11 Apr 2024 13:13
 Operator : JC/MD
 Sample : P2048-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R51

Manual IntegrationsAPPROVED

Quant Time: Apr 12 01:46:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 05:36:34 2024
 Response via : Initial Calibration

Reviewed By :John Carlone 04/12/2024
 Supervised By :Semsettin Yesilyurt 04/12/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.781	114	294575	50.000	ug/L	0.02
28) Chlorobenzene-d5	10.098	117	195542	50.000	ug/L	# 0.04
58) 1,4-Dichlorobenzene-d4	12.043	152	168730	50.000	ug/L	# 0.02
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	95197	45.435	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	90.880%	
7) Chloroethane-d5	1.666	69	81655	47.785	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	95.580%	
11) 1,1-Dichloroethene-d2	2.307	65	42289	47.275	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	94.540%	
21) 2-Butanone-d5	4.459	46	116244	101.851	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	101.850%	
24) Chloroform-d	5.062	84	215118	55.026	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	110.060%	
26) 1,2-Dichloroethane-d4	6.178	65	129604m	50.966	ug/L	0.23
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.940%	
32) Benzene-d6	6.086	84	361557	68.107	ug/L	0.11
Spiked Amount 50.000	Range 70	- 125	Recovery	=	136.220%#	
36) 1,2-Dichloropropane-d6	7.318	67	107945	69.720	ug/L	0.01
Spiked Amount 50.000	Range 70	- 120	Recovery	=	139.440%#	
41) Toluene-d8	8.653	98	345653	66.647	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	133.300%#	
43) trans-1,3-Dichloroprop...	8.952	79	49392	63.393	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	126.780%#	
47) 2-Hexanone-d5	9.391	63	91363	139.962	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	139.960%#	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	150575	65.654	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	131.300%#	
66) 1,2-Dichlorobenzene-d4	12.341	152	161724	47.781	ug/L	0.02
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.560%	
Target Compounds						
					Qvalue	
12) 1,1-Dichloroethene	2.313	96	2121	1.199	ug/L #	1
13) Acetone	2.380	43	4482	3.623	ug/L	97
14) Carbon disulfide	2.514	76	32288	7.261	ug/L	100
16) Methylene chloride	2.788	84	8247	4.472	ug/L	96
25) Chloroform	5.099	83	805356	225.883	ug/L	98
29) Cyclohexane	5.483	56	28869	14.737	ug/L	99
33) Benzene	6.062	78	116389574m	22941.419	ug/L	
34) Trichloroethene	7.141	95	11598	7.969	ug/L	96
35) Methylcyclohexane	7.391	83	4689	2.272	ug/L #	68
42) Toluene	8.726	91	68630	12.215	ug/L	99
46) Tetrachloroethene	9.281	164	9742	7.107	ug/L	96
51) Chlorobenzene	10.092	112	62307047m	15824.402	ug/L	
64) 1,3-Dichlorobenzene	11.976	146	2879172	556.257	ug/L	97
65) 1,4-Dichlorobenzene	12.061	146	27961855m	5262.422	ug/L	
67) 1,2-Dichlorobenzene	12.360	146	22086786	4398.843	ug/L #	68
70) 1,2,4-trichlorobenzene	13.591	180	1151083	306.435	ug/L	100
72) 1,2,3-Trichlorobenzene	13.963	180	71528	19.416	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed							

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040974.D
Acq On : 11 Apr 2024 13:13
Operator : JC/MD
Sample : P2048-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R51

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 04/12/2024
Supervised By :Semsettin Yesilyurt 04/12/2024

Quant Time: Apr 12 01:46:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

