

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040969.D
 Acq On : 11 Apr 2024 11:18
 Operator : JC/MD
 Sample : P2048-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R84

Quant Time: Apr 12 01:46:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 05:36:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	275836	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	261258	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	141998	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	96812	49.345	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.700%	
7) Chloroethane-d5	1.672	69	81803	51.124	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	102.240%	
11) 1,1-Dichloroethene-d2	2.306	65	42224	50.409	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	100.820%	
21) 2-Butanone-d5	4.452	46	125485	117.417	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	117.420%	
24) Chloroform-d	5.056	84	180549	49.321	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	98.640%	
26) 1,2-Dichloroethane-d4	5.952	65	120470	50.592	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.180%	
32) Benzene-d6	5.970	84	366585	51.685	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	103.360%	
36) 1,2-Dichloropropane-d6	7.306	67	107191	51.818	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	103.640%	
41) Toluene-d8	8.647	98	345068	49.799	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.600%	
43) trans-1,3-Dichloroprop...	8.952	79	50761	48.762	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.520%	
47) 2-Hexanone-d5	9.384	63	87065	99.828	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	99.830%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	150894	49.244	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	98.480%	
66) 1,2-Dichlorobenzene-d4	12.317	152	148677	52.195	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.400%	
Target Compounds					Qvalue	
13) Acetone	2.380	43	11779	10.169	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040969.D
Acq On : 11 Apr 2024 11:18
Operator : JC/MD
Sample : P2048-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R84

Quant Time: Apr 12 01:46:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

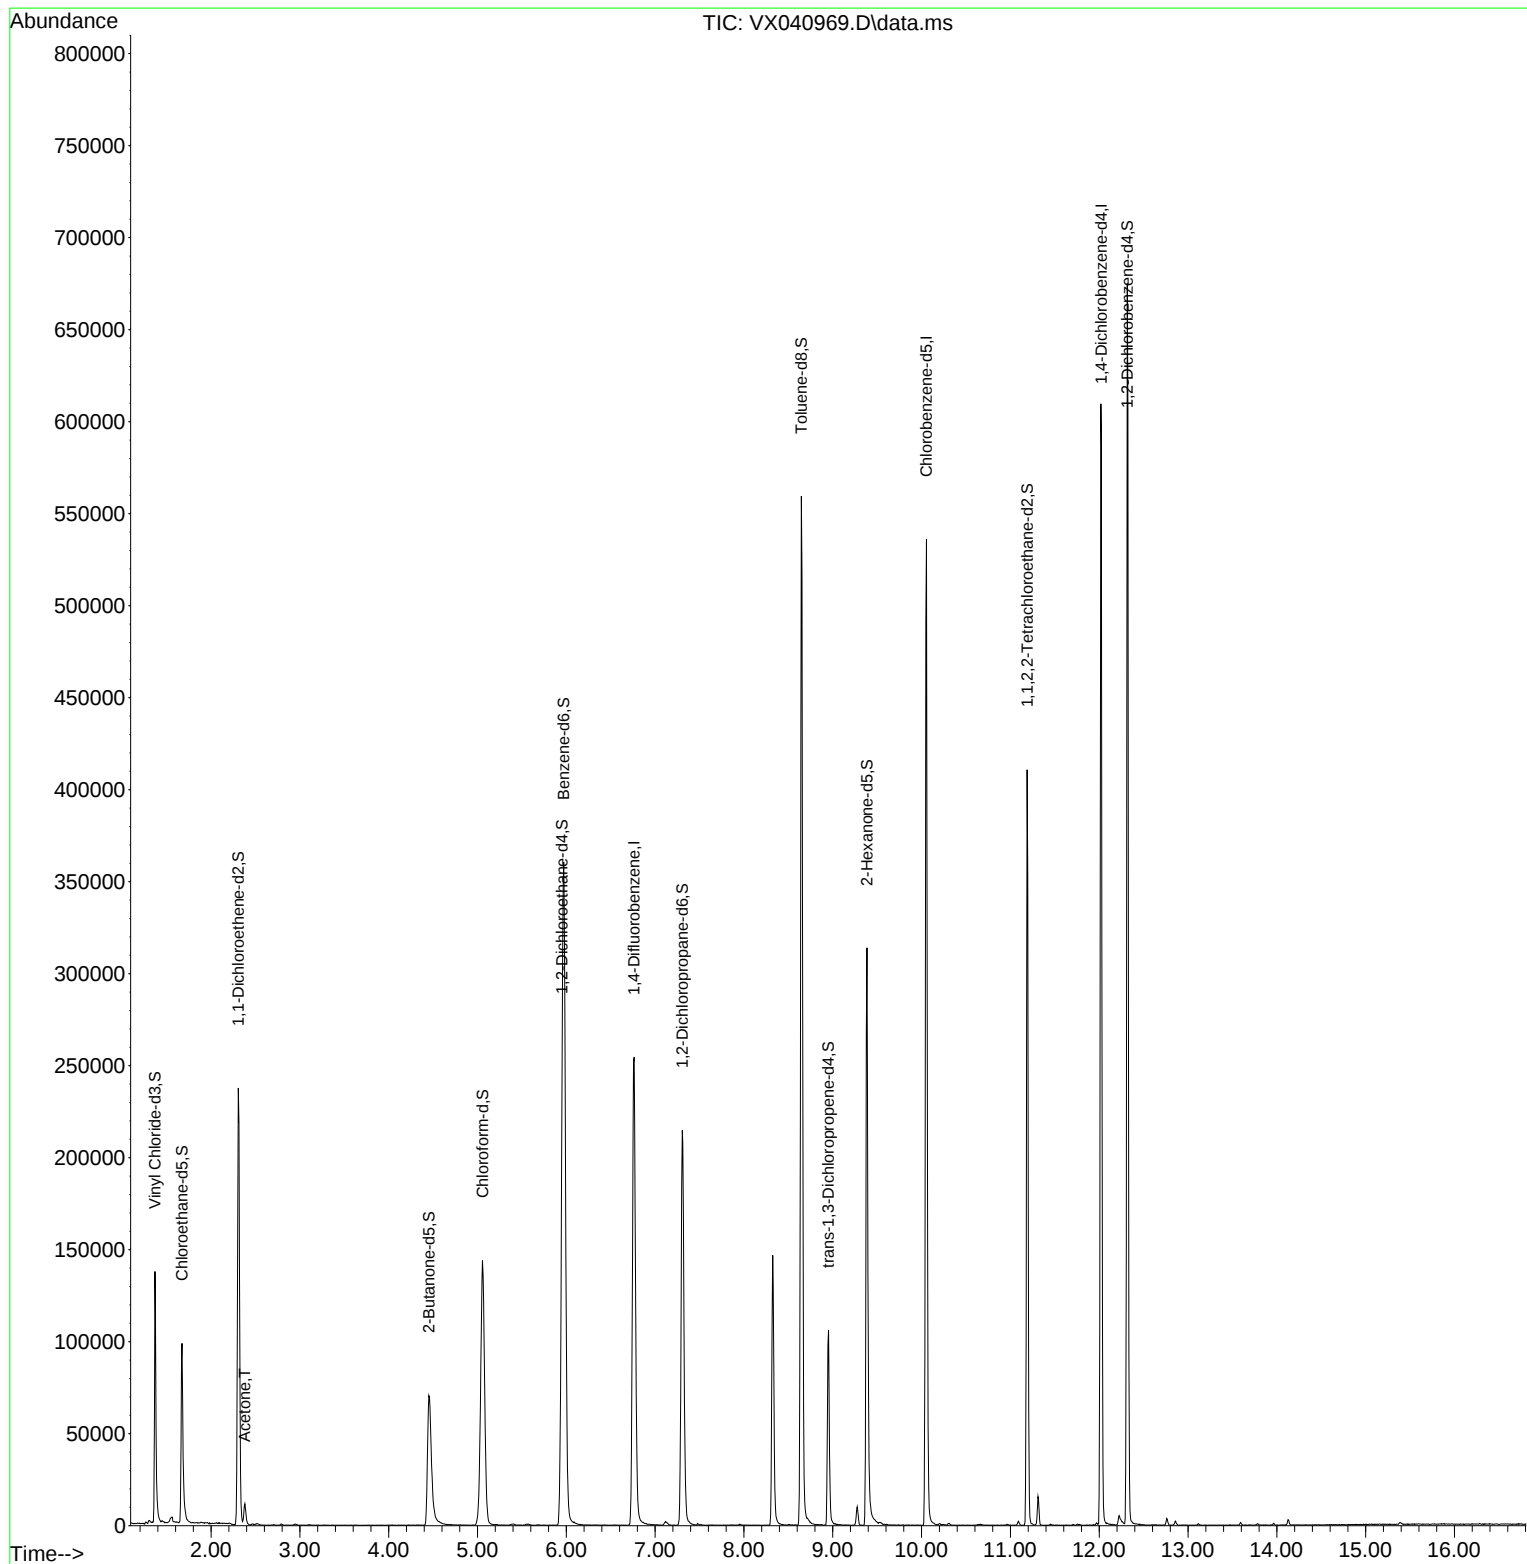

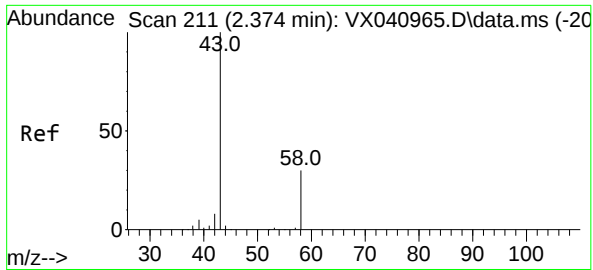

#13
 Acetone
 Concen: 10.169 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX040969.D
 Acq: 11 Apr 2024 11:18

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R84

Tgt Ion: 43 Resp: 11779
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 59.4

