

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040970.D
 Acq On : 11 Apr 2024 11:41
 Operator : JC/MD
 Sample : P2048-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R85

Quant Time: Apr 12 01:46:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 11 05:36:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	292503	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	281160	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.018	152	153689	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	98554	47.371	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.740%
7) Chloroethane-d5	1.673	69	82829	48.816	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.640%
11) 1,1-Dichloroethene-d2	2.307	65	41632	46.870	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.740%
21) 2-Butanone-d5	4.453	46	127758	112.733	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	112.730%
24) Chloroform-d	5.056	84	180501	46.498	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.000%
26) 1,2-Dichloroethane-d4	5.952	65	122421	48.482	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.960%
32) Benzene-d6	5.971	84	367509	48.147	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.300%
36) 1,2-Dichloropropane-d6	7.306	67	106384	47.788	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.580%
41) Toluene-d8	8.647	98	356640	47.825	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.660%
43) trans-1,3-Dichloroprop...	8.952	79	52472	46.838	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.680%
47) 2-Hexanone-d5	9.385	63	91130	97.093	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	97.090%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	158824	48.163	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.320%
66) 1,2-Dichlorobenzene-d4	12.317	152	153385	49.752	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.500%
Target Compounds						
					Qvalue	
13) Acetone	2.380	43	8920	7.262	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040970.D
Acq On : 11 Apr 2024 11:41
Operator : JC/MD
Sample : P2048-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R85

Quant Time: Apr 12 01:46:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 11 05:36:34 2024
Response via : Initial Calibration

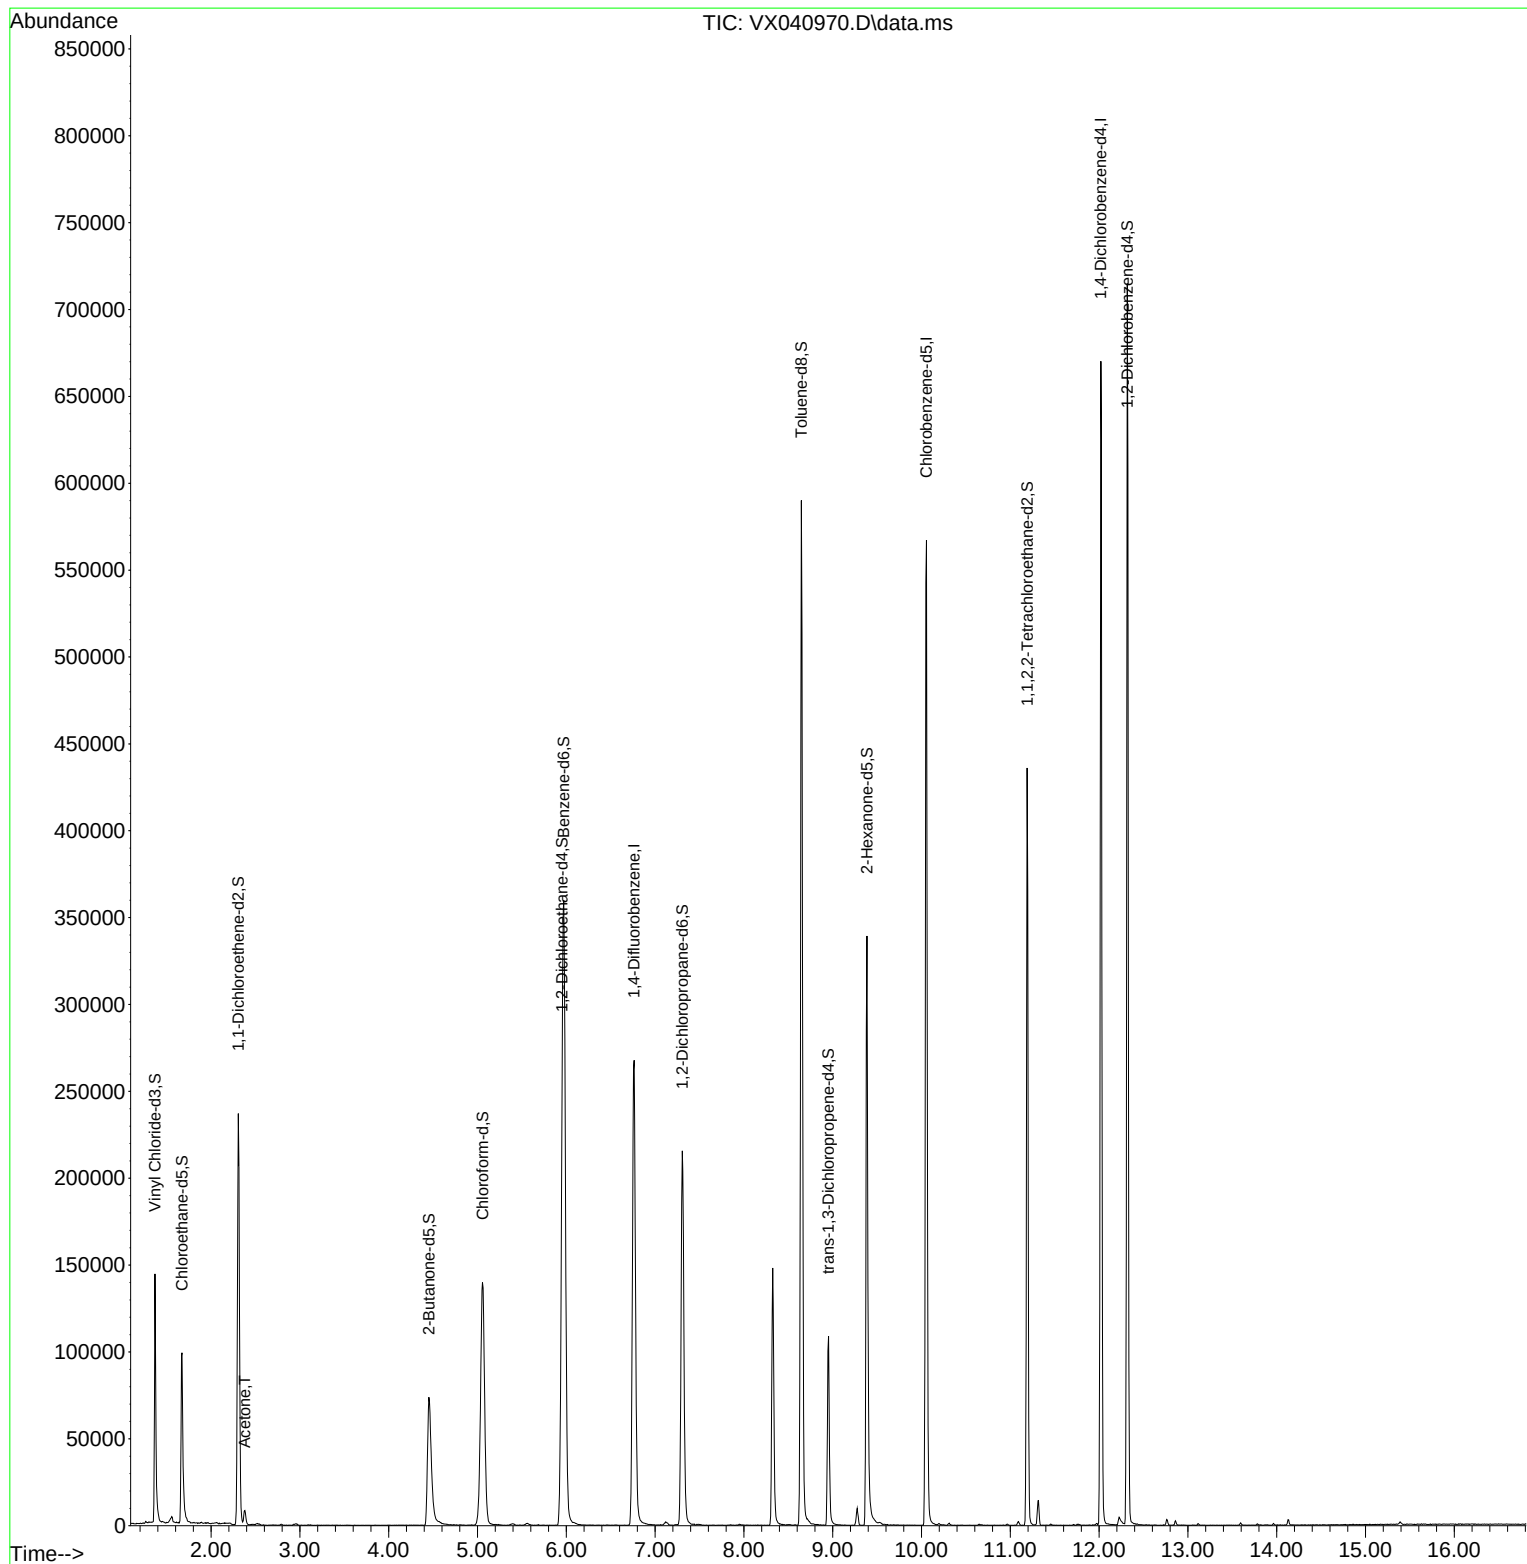

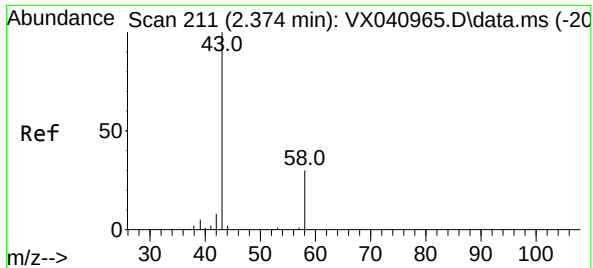

#13
 Acetone
 Concen: 7.262 ug/L
 RT: 2.380 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX040970.D
 Acq: 11 Apr 2024 11:41

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R85

Tgt Ion: 43 Resp: 8920
 Ion Ratio Lower Upper
 43 100
 58 28.8 0.0 59.4

