

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040966.D
 Acq On : 11 Apr 2024 10:00
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	145683	159479	14.94%	1.823%
2	1.666	91	95	111	rVB	101035	153348	14.37%	1.753%
3	2.307	194	200	210	rBV	237960	372909	34.93%	4.263%
4	2.575	243	244	246	rBV	131	93	0.01%	0.001%
5	2.685	261	262	263	rBV	214	98	0.01%	0.001%
6	2.703	263	265	269	rVV2	369	495	0.05%	0.006%
7	2.752	271	273	275	rVV	167	129	0.01%	0.001%
8	2.788	275	279	286	rVB4	1205	2188	0.20%	0.025%
9	2.941	300	304	311	rVB2	676	1247	0.12%	0.014%
10	3.105	324	331	334	rBV6	1091	2449	0.23%	0.028%
11	3.483	390	393	397	rVB2	211	263	0.02%	0.003%
12	3.550	402	404	407	rVV2	111	112	0.01%	0.001%
13	3.605	410	413	419	rVV2	328	625	0.06%	0.007%
14	3.703	426	429	431	rVB2	110	102	0.01%	0.001%
15	3.739	433	435	437	rBV2	145	154	0.01%	0.002%
16	3.782	437	442	445	rBV2	85	152	0.01%	0.002%
17	3.873	454	457	458	rBV	216	180	0.02%	0.002%
18	3.916	462	464	466	rBV	107	87	0.01%	0.001%
19	3.959	466	471	472	rBB2	98	88	0.01%	0.001%
20	3.971	472	473	475	rBV2	114	112	0.01%	0.001%
21	4.257	518	520	523	rBV2	168	180	0.02%	0.002%
22	4.288	523	525	527	rVB2	135	106	0.01%	0.001%
23	4.312	527	529	530	rVB	181	84	0.01%	0.001%
24	4.343	530	534	535	rBV2	87	112	0.01%	0.001%
25	4.446	543	551	577	rBV	75502	238969	22.39%	2.732%
26	4.709	592	594	596	rVB	247	161	0.02%	0.002%
27	4.958	634	635	638	rBV	155	102	0.01%	0.001%
28	5.056	638	651	666	rBV	138696	429169	40.20%	4.906%
29	5.391	700	706	713	rVB4	660	1527	0.14%	0.017%
30	5.452	714	716	717	rBV	297	202	0.02%	0.002%
31	5.544	727	731	732	rBV2	570	613	0.06%	0.007%
32	5.678	749	753	759	rVB2	482	843	0.08%	0.010%
33	5.964	788	800	819	rBV2	354886	1067463	100.00%	12.203%
34	6.294	851	854	857	rBV2	174	215	0.02%	0.002%
35	6.757	920	930	948	rBV	280514	673500	63.09%	7.699%
36	7.123	982	990	1000	rVB9	2596	6988	0.65%	0.080%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040966.D
 Acq On : 11 Apr 2024 10:00
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.220	1003	1006	1007	rBV2	181	170	0.02%	0.002%
38	7.306	1011	1020	1036	rBV	211197	470461	44.07%	5.378%
39	7.537	1056	1058	1063	rVB2	194	187	0.02%	0.002%
40	7.763	1093	1095	1096	rVB	188	105	0.01%	0.001%
41	7.818	1102	1104	1105	rBV	315	268	0.03%	0.003%
42	7.958	1122	1127	1130	rBV2	402	656	0.06%	0.007%
43	8.116	1151	1153	1156	rVB	172	162	0.02%	0.002%
44	8.159	1156	1160	1161	rBV2	129	116	0.01%	0.001%
45	8.177	1161	1163	1167	rBV2	162	165	0.02%	0.002%
46	8.324	1180	1187	1204	rBV	148531	248894	23.32%	2.845%
47	8.501	1214	1216	1225	rVB4	498	990	0.09%	0.011%
48	8.580	1225	1229	1233	rBV4	1527	1811	0.17%	0.021%
49	8.647	1233	1240	1250	rBV	587970	911042	85.35%	10.415%
50	8.946	1284	1289	1307	rBV	106236	165247	15.48%	1.889%
51	9.159	1321	1324	1327	rVB3	655	801	0.08%	0.009%
52	9.232	1333	1336	1338	rBV	228	200	0.02%	0.002%
53	9.275	1338	1343	1348	rVB2	1716	2327	0.22%	0.027%
54	9.385	1355	1361	1382	rBV	328611	518421	48.57%	5.927%
55	9.610	1396	1398	1403	rVB4	605	885	0.08%	0.010%
56	9.848	1435	1437	1440	rVB3	294	280	0.03%	0.003%
57	10.049	1465	1470	1488	rBV	594679	846373	79.29%	9.676%
58	10.195	1491	1494	1504	rVB	1851	3191	0.30%	0.036%
59	10.262	1504	1505	1508	rBV2	233	171	0.02%	0.002%
60	10.305	1508	1512	1520	rVB3	1787	2833	0.27%	0.032%
61	10.366	1520	1522	1523	rBV	139	95	0.01%	0.001%
62	10.494	1539	1543	1544	rBV2	161	213	0.02%	0.002%
63	10.579	1554	1557	1558	rBV2	71	85	0.01%	0.001%
64	10.647	1564	1568	1578	rVB3	2037	4621	0.43%	0.053%
65	10.799	1591	1593	1597	rVB3	438	543	0.05%	0.006%
66	10.964	1616	1620	1626	rVB2	1947	2675	0.25%	0.031%
67	11.006	1626	1627	1629	rBV	226	118	0.01%	0.001%
68	11.092	1637	1641	1649	rVB3	1262	2059	0.19%	0.024%
69	11.189	1651	1657	1671	rVV	447984	562743	52.72%	6.433%
70	11.311	1674	1677	1682	rVB2	1322	1876	0.18%	0.021%
71	11.366	1684	1686	1688	rBV2	127	153	0.01%	0.002%
72	11.451	1695	1700	1706	rVB	1873	2226	0.21%	0.025%
73	11.549	1712	1716	1718	rBV2	124	163	0.02%	0.002%
74	11.671	1734	1736	1738	rBV2	125	112	0.01%	0.001%
75	11.750	1745	1749	1754	rBV4	1470	2271	0.21%	0.026%
76	11.860	1766	1767	1769	rBV	121	92	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040966.D
 Acq On : 11 Apr 2024 10:00
 Operator : JC/MD
 Sample : VX0411WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK667

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.969	1781	1785	1788	rBV3	2767	3373	0.32%	0.039%
78	12.018	1788	1793	1807	rVV	742400	931959	87.31%	10.654%
79	12.317	1837	1842	1853	rBV	746724	913741	85.60%	10.446%
80	12.585	1884	1886	1888	rVB	194	131	0.01%	0.001%
81	12.622	1890	1892	1893	rBV	221	87	0.01%	0.001%
82	12.671	1898	1900	1903	rBV	128	117	0.01%	0.001%
83	12.762	1911	1915	1920	rVB2	2374	3291	0.31%	0.038%
84	12.884	1932	1935	1936	rBV	150	110	0.01%	0.001%
85	12.902	1936	1938	1939	rVV	146	84	0.01%	0.001%
86	12.951	1942	1946	1948	rVV2	470	597	0.06%	0.007%
87	13.116	1969	1973	1979	rVB	2494	3291	0.31%	0.038%
88	13.384	2016	2017	2019	rBV	182	150	0.01%	0.002%
89	13.433	2023	2025	2026	rVV	160	88	0.01%	0.001%
90	13.506	2036	2037	2041	rBV2	132	154	0.01%	0.002%
91	13.555	2043	2045	2046	rBV2	118	111	0.01%	0.001%
92	13.591	2047	2051	2055	rBV3	3157	4398	0.41%	0.050%
93	13.689	2066	2067	2068	rBV	193	98	0.01%	0.001%
94	13.780	2076	2082	2088	rBV	4523	6231	0.58%	0.071%
95	13.963	2107	2112	2119	rBV2	3560	4913	0.46%	0.056%
96	14.036	2122	2124	2126	rBV2	275	238	0.02%	0.003%
97	14.128	2135	2139	2146	rVB2	2340	3273	0.31%	0.037%
98	14.195	2148	2150	2155	rBV2	175	226	0.02%	0.003%
99	14.634	2218	2222	2223	rBV2	218	223	0.02%	0.003%
100	14.993	2279	2281	2282	rBV	364	186	0.02%	0.002%



Sum of corrected areas: 8747415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040966.D
Acq On : 11 Apr 2024 10:00
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK667

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

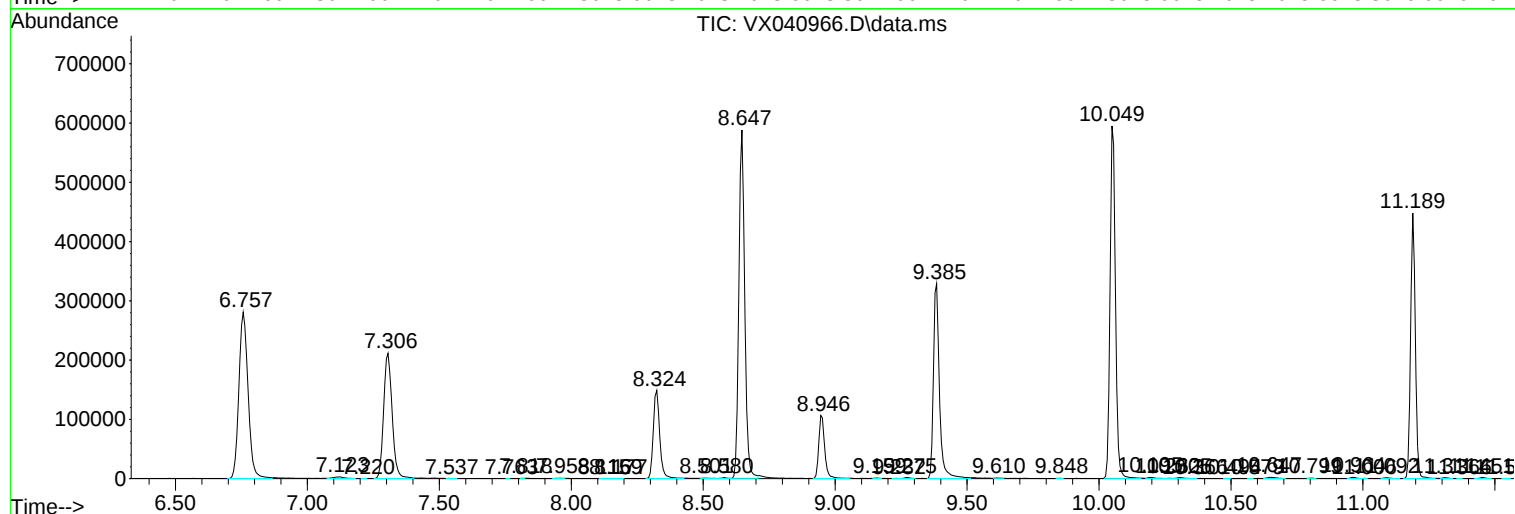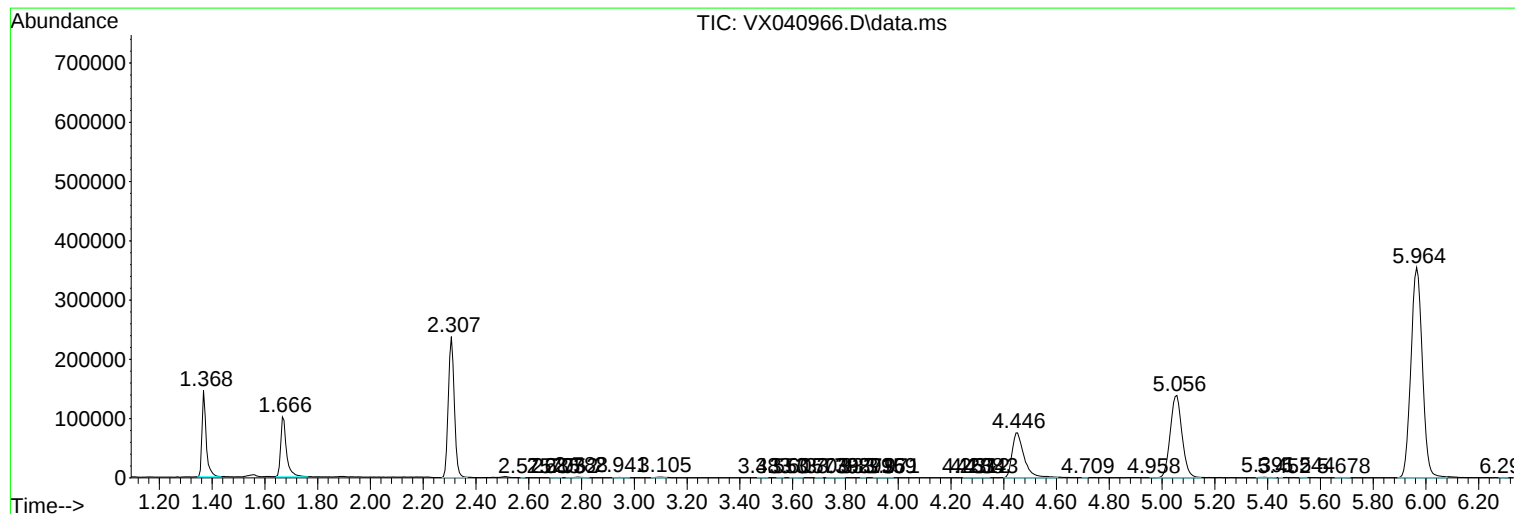

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040966.D
Acq On : 11 Apr 2024 10:00
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK667

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040966.D
Acq On : 11 Apr 2024 10:00
Operator : JC/MD
Sample : VX0411WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK667

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc