

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040967.D
 Acq On : 11 Apr 2024 10:32
 Operator : JC/MD
 Sample : P2048-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX040967.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	141944	151686	14.84%	1.789%
2	1.666	91	95	114	rVB	95052	145222	14.20%	1.713%
3	2.307	194	200	208	rBV	226769	352407	34.47%	4.156%
4	2.428	218	220	222	rBV3	233	236	0.02%	0.003%
5	2.709	264	266	268	rVB3	215	179	0.02%	0.002%
6	2.727	268	269	272	rBV	129	126	0.01%	0.001%
7	2.782	275	278	289	rVB6	516	1177	0.12%	0.014%
8	2.947	299	305	312	rVB3	1057	2646	0.26%	0.031%
9	3.093	325	329	332	rBV3	571	756	0.07%	0.009%
10	3.136	335	336	340	rBV2	97	141	0.01%	0.002%
11	3.245	351	354	356	rBV	164	150	0.01%	0.002%
12	3.447	385	387	390	rVB2	134	120	0.01%	0.001%
13	3.971	472	473	475	rVB	203	144	0.01%	0.002%
14	4.014	478	480	485	rVV2	195	328	0.03%	0.004%
15	4.056	485	487	492	rVV2	158	298	0.03%	0.004%
16	4.111	495	496	499	rVB2	239	151	0.01%	0.002%
17	4.209	509	512	515	rBV2	125	196	0.02%	0.002%
18	4.446	542	551	567	rBV	67086	206667	20.21%	2.437%
19	4.794	606	608	614	rBV2	350	546	0.05%	0.006%
20	5.050	636	650	666	rBV	136730	427799	41.84%	5.045%
21	5.269	684	686	691	rVB2	184	184	0.02%	0.002%
22	5.373	700	703	704	rBV	486	453	0.04%	0.005%
23	5.532	727	729	730	rBV2	290	280	0.03%	0.003%
24	5.660	749	750	752	rBV2	180	145	0.01%	0.002%
25	5.757	765	766	769	rVB	145	121	0.01%	0.001%
26	5.855	779	782	785	rBV2	180	207	0.02%	0.002%
27	5.964	788	800	820	rBV2	342069	1022373	100.00%	12.056%
28	6.233	842	844	846	rBV3	220	186	0.02%	0.002%
29	6.306	854	856	860	rBV2	185	255	0.02%	0.003%
30	6.342	860	862	865	rVB2	205	169	0.02%	0.002%
31	6.379	866	868	871	rVB2	179	120	0.01%	0.001%
32	6.464	880	882	886	rBV2	267	419	0.04%	0.005%
33	6.531	891	893	895	rVV	256	247	0.02%	0.003%
34	6.550	895	896	900	rVB	268	278	0.03%	0.003%
35	6.757	921	930	951	rBV	279233	667107	65.25%	7.867%
36	7.117	983	989	998	rVB6	1568	4602	0.45%	0.054%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040967.D
 Acq On : 11 Apr 2024 10:32
 Operator : JC/MD
 Sample : P2048-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCOR70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.239	1005	1009	1011	rBV2	184	244	0.02%	0.003%
38	7.306	1011	1020	1033	rBV	205382	452322	44.24%	5.334%
39	7.476	1044	1048	1056	rVB4	477	1011	0.10%	0.012%
40	7.574	1061	1064	1066	rBV	209	140	0.01%	0.002%
41	7.598	1066	1068	1069	rBV2	145	123	0.01%	0.001%
42	7.799	1097	1101	1103	rBV2	129	160	0.02%	0.002%
43	7.842	1105	1108	1111	rBV3	264	369	0.04%	0.004%
44	7.946	1122	1125	1127	rBV2	585	605	0.06%	0.007%
45	8.141	1154	1157	1159	rBV	126	131	0.01%	0.002%
46	8.324	1181	1187	1202	rBV	141518	235628	23.05%	2.779%
47	8.574	1225	1228	1232	rBV3	410	471	0.05%	0.006%
48	8.647	1233	1240	1263	rVV	556227	883428	86.41%	10.418%
49	8.946	1284	1289	1308	rBV	103633	157932	15.45%	1.862%
50	9.141	1318	1321	1324	rVB2	140	205	0.02%	0.002%
51	9.275	1337	1343	1350	rBV	18748	29425	2.88%	0.347%
52	9.385	1355	1361	1378	rBV	298097	465286	45.51%	5.487%
53	9.683	1408	1410	1411	rBV	188	152	0.01%	0.002%
54	9.848	1435	1437	1444	rVB2	331	368	0.04%	0.004%
55	9.952	1451	1454	1455	rBV2	127	146	0.01%	0.002%
56	10.049	1465	1470	1488	rBV	577230	831518	81.33%	9.806%
57	10.189	1492	1493	1500	rVB2	783	1188	0.12%	0.014%
58	10.305	1509	1512	1516	rVB3	711	1062	0.10%	0.013%
59	10.439	1532	1534	1536	rBV	153	126	0.01%	0.001%
60	10.598	1558	1560	1561	rBV2	148	136	0.01%	0.002%
61	10.647	1564	1568	1570	rBV3	497	588	0.06%	0.007%
62	10.750	1583	1585	1586	rBV2	205	144	0.01%	0.002%
63	10.805	1589	1594	1595	rBV2	205	211	0.02%	0.002%
64	10.964	1615	1620	1624	rBV3	449	655	0.06%	0.008%
65	11.092	1637	1641	1646	rVB2	1725	2548	0.25%	0.030%
66	11.189	1652	1657	1672	rVV	420774	526048	51.45%	6.203%
67	11.311	1672	1677	1683	rVB	25159	35792	3.50%	0.422%
68	11.360	1683	1685	1687	rBV2	163	147	0.01%	0.002%
69	11.457	1697	1701	1706	rVB2	524	885	0.09%	0.010%
70	11.567	1718	1719	1722	rVB2	239	154	0.02%	0.002%
71	11.604	1722	1725	1728	rBV2	181	270	0.03%	0.003%
72	11.707	1740	1742	1746	rVB2	497	473	0.05%	0.006%
73	11.750	1746	1749	1753	rBV2	675	926	0.09%	0.011%
74	11.927	1777	1778	1781	rBV2	207	189	0.02%	0.002%
75	11.976	1781	1786	1788	rBV4	1237	1556	0.15%	0.018%
76	12.018	1788	1793	1805	rBV	723746	915161	89.51%	10.792%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040967.D
 Acq On : 11 Apr 2024 10:32
 Operator : JC/MD
 Sample : P2048-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MCOR70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.219	1822	1826	1837	rBV2	10495	24530	2.40%	0.289%
78	12.317	1837	1842	1853	rVB	725984	890519	87.10%	10.502%
79	12.762	1909	1915	1919	rBV	7532	9641	0.94%	0.114%
80	12.817	1923	1924	1926	rBV	217	157	0.02%	0.002%
81	12.860	1926	1931	1937	rVB3	2126	3393	0.33%	0.040%
82	12.914	1937	1940	1942	rBV2	302	380	0.04%	0.004%
83	13.024	1956	1958	1961	rVB	103	119	0.01%	0.001%
84	13.079	1965	1967	1969	rBV2	170	185	0.02%	0.002%
85	13.116	1969	1973	1978	rVV3	1147	1524	0.15%	0.018%
86	13.268	1994	1998	2000	rBV2	187	234	0.02%	0.003%
87	13.439	2024	2026	2029	rBV2	179	143	0.01%	0.002%
88	13.481	2029	2033	2035	rBV2	145	189	0.02%	0.002%
89	13.591	2047	2051	2057	rVB4	1878	2433	0.24%	0.029%
90	13.731	2072	2074	2078	rBV2	126	169	0.02%	0.002%
91	13.780	2078	2082	2088	rVV2	1448	2106	0.21%	0.025%
92	13.963	2109	2112	2117	rVB3	1508	1909	0.19%	0.023%
93	14.073	2128	2130	2132	rVB	234	169	0.02%	0.002%
94	14.103	2132	2135	2136	rBV	365	364	0.04%	0.004%
95	14.134	2136	2140	2145	rVB	3277	4604	0.45%	0.054%
96	14.396	2181	2183	2185	rBV3	180	187	0.02%	0.002%
97	14.707	2232	2234	2235	rBV	202	135	0.01%	0.002%
98	14.823	2251	2253	2254	rBV	258	154	0.02%	0.002%
99	14.926	2268	2270	2272	rBV2	377	314	0.03%	0.004%
100	16.139	2468	2469	2472	rBV3	347	269	0.03%	0.003%




Sum of corrected areas: 8479871

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040967.D
Acq On : 11 Apr 2024 10:32
Operator : JC/MD
Sample : P2048-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

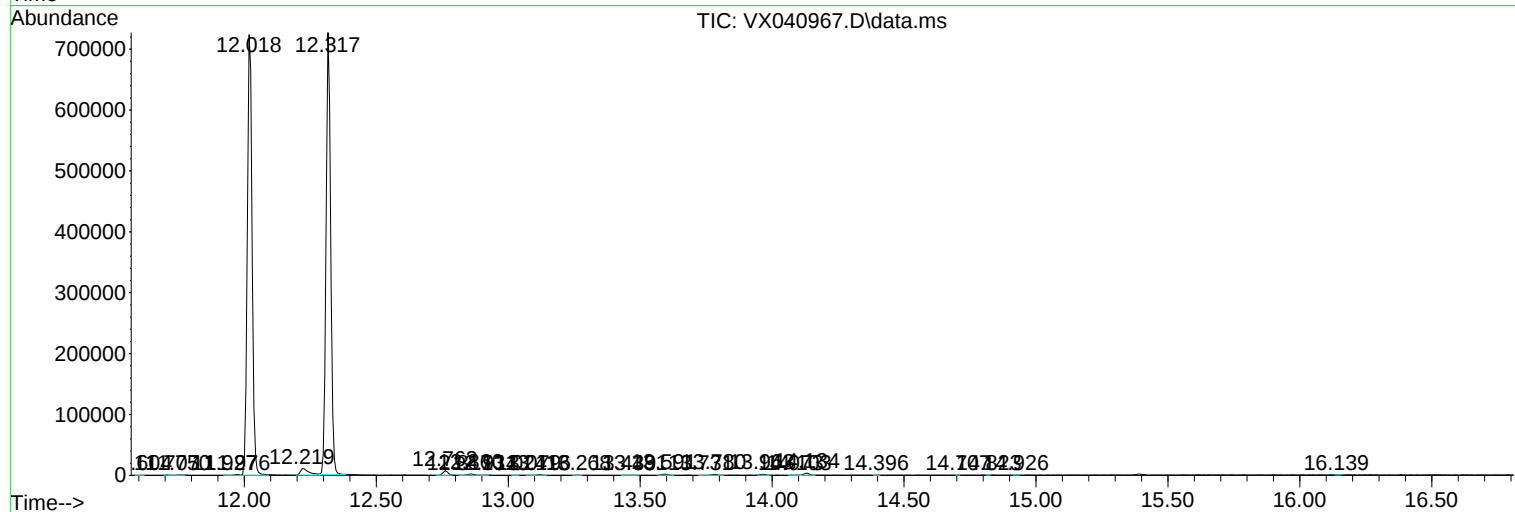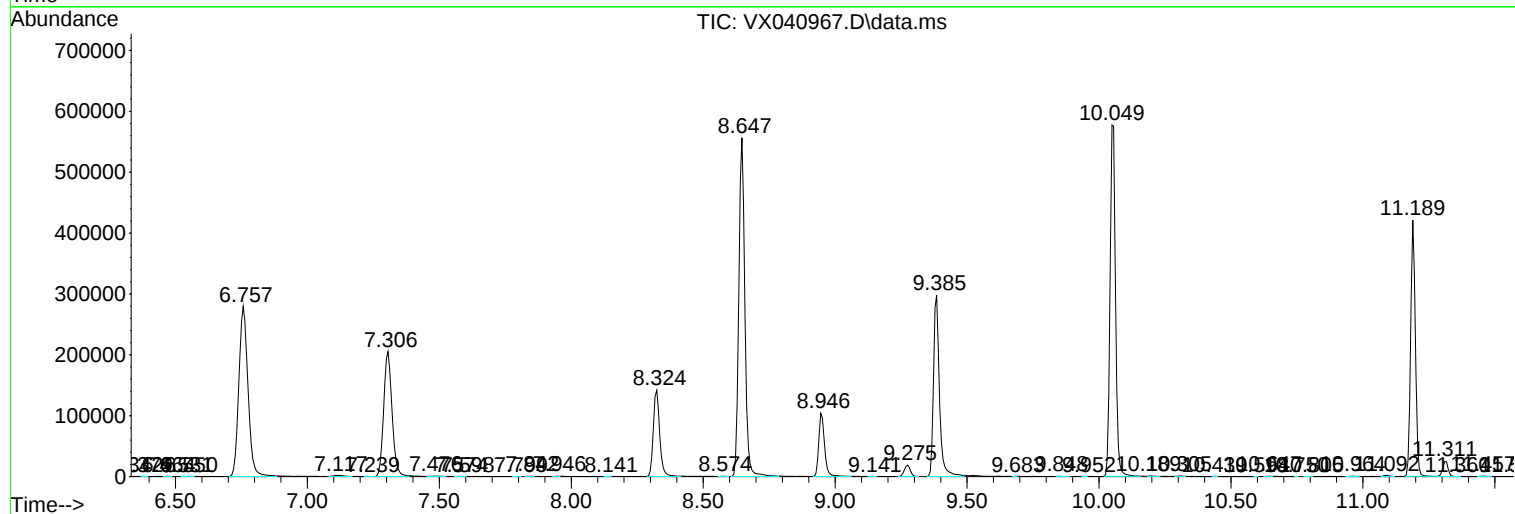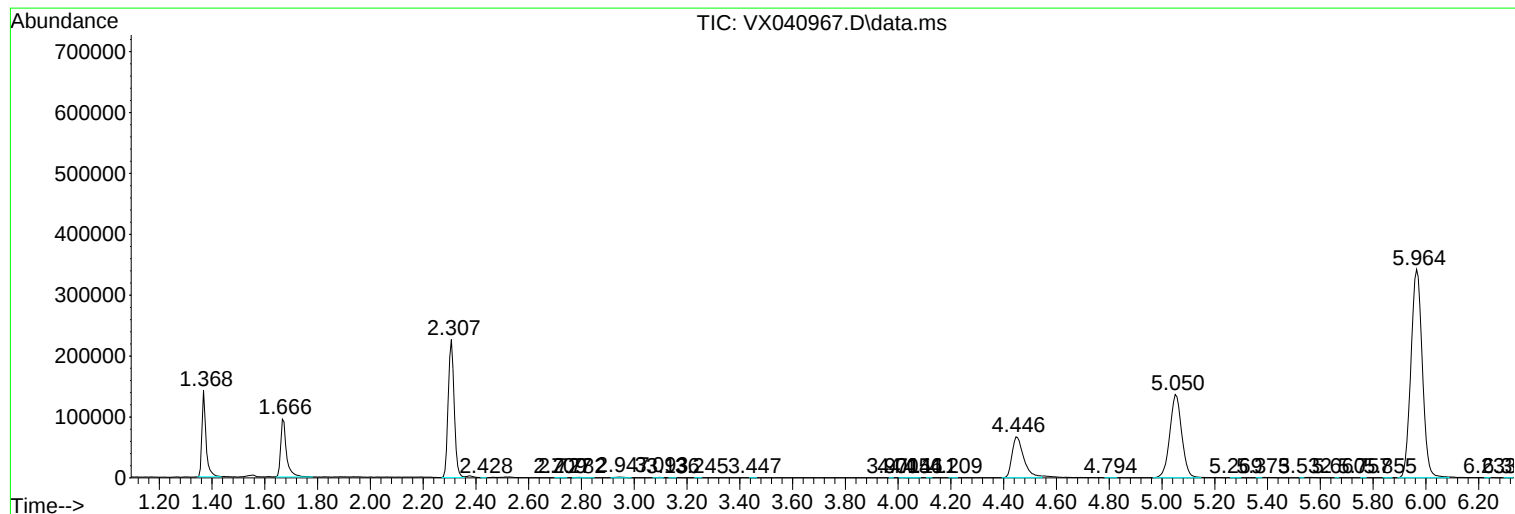

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040967.D
Acq On : 11 Apr 2024 10:32
Operator : JC/MD
Sample : P2048-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040967.D
Acq On : 11 Apr 2024 10:32
Operator : JC/MD
Sample : P2048-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc