

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040969.D
 Acq On : 11 Apr 2024 11:18
 Operator : JC/MD
 Sample : P2048-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	27	29	32	rBV2	1124	1343	0.12%	0.016%
2	1.301	32	35	40	rVV3	1784	3088	0.29%	0.037%
3	1.368	43	46	57	rVB	136323	154907	14.40%	1.853%
4	1.672	91	96	113	rVB	97515	147564	13.72%	1.765%
5	2.306	194	200	208	rBV	237323	372537	34.63%	4.457%
6	2.380	208	212	222	rVB	11512	19603	1.82%	0.235%
7	2.471	223	227	230	rBV2	434	602	0.06%	0.007%
8	2.703	260	265	267	rBV2	337	470	0.04%	0.006%
9	2.788	275	279	286	rBV3	716	1081	0.10%	0.013%
10	2.953	300	306	313	rVV2	617	1385	0.13%	0.017%
11	3.099	329	330	331	rBV	273	145	0.01%	0.002%
12	3.611	412	414	416	rBV	125	112	0.01%	0.001%
13	3.770	437	440	441	rBV	126	121	0.01%	0.001%
14	3.788	441	443	447	rVB2	156	129	0.01%	0.002%
15	4.312	528	529	532	rBV2	175	163	0.02%	0.002%
16	4.452	543	552	583	rBV	70411	228171	21.21%	2.730%
17	4.946	631	633	635	rBV	138	126	0.01%	0.002%
18	5.056	637	651	669	rBV	143794	447979	41.65%	5.360%
19	5.263	684	685	689	rVB2	185	158	0.01%	0.002%
20	5.300	689	691	693	rVB2	158	127	0.01%	0.002%
21	5.403	702	708	713	rVB4	583	1575	0.15%	0.019%
22	5.477	718	720	722	rVB2	156	121	0.01%	0.001%
23	5.556	728	733	734	rBV2	534	767	0.07%	0.009%
24	5.684	749	754	755	rBV3	274	349	0.03%	0.004%
25	5.733	760	762	765	rBV2	128	149	0.01%	0.002%
26	5.970	789	801	819	rBV2	360357	1075633	100.00%	12.869%
27	6.293	852	854	856	rBV	164	180	0.02%	0.002%
28	6.434	874	877	879	rVV2	179	169	0.02%	0.002%
29	6.531	890	893	894	rBV2	140	121	0.01%	0.001%
30	6.696	917	920	921	rBV	123	131	0.01%	0.002%
31	6.763	921	931	946	rBV	254229	616086	57.28%	7.371%
32	7.117	982	989	996	rBV8	2005	4771	0.44%	0.057%
33	7.171	996	998	1002	rVB3	272	299	0.03%	0.004%
34	7.306	1011	1020	1038	rBV	214548	474832	44.14%	5.681%
35	7.476	1046	1048	1051	rBV2	837	808	0.08%	0.010%
36	7.848	1107	1109	1112	rBV2	168	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040969.D
 Acq On : 11 Apr 2024 11:18
 Operator : JC/MD
 Sample : P2048-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.891	1115	1116	1119	rBV	227	213	0.02%	0.003%
38	7.952	1124	1126	1133	rVV2	638	781	0.07%	0.009%
39	8.074	1144	1146	1148	rVB	153	113	0.01%	0.001%
40	8.226	1166	1171	1173	rBV	167	182	0.02%	0.002%
41	8.324	1181	1187	1203	rBV	146662	245839	22.86%	2.941%
42	8.507	1212	1217	1223	rBV3	462	877	0.08%	0.010%
43	8.647	1233	1240	1261	rBV	559199	909863	84.59%	10.886%
44	8.952	1284	1290	1301	rVV	105939	159864	14.86%	1.913%
45	9.134	1319	1320	1322	rBV2	156	138	0.01%	0.002%
46	9.275	1334	1343	1350	rBV	10032	15261	1.42%	0.183%
47	9.384	1355	1361	1382	rBV	313761	488813	45.44%	5.848%
48	9.744	1419	1420	1424	rVB2	323	236	0.02%	0.003%
49	9.787	1424	1427	1428	rBV	246	297	0.03%	0.004%
50	9.982	1457	1459	1463	rVB2	144	199	0.02%	0.002%
51	10.055	1465	1471	1491	rBV	535714	750616	69.78%	8.981%
52	10.207	1492	1496	1498	rVB4	663	888	0.08%	0.011%
53	10.311	1509	1513	1517	rVB3	960	1361	0.13%	0.016%
54	10.592	1558	1559	1562	rVV	136	138	0.01%	0.002%
55	10.622	1562	1564	1565	rVV2	195	124	0.01%	0.001%
56	10.646	1565	1568	1570	rVV2	487	753	0.07%	0.009%
57	10.695	1574	1576	1579	rVB2	163	128	0.01%	0.002%
58	10.896	1607	1609	1613	rVB2	160	227	0.02%	0.003%
59	10.939	1615	1616	1617	rVV	205	129	0.01%	0.002%
60	10.963	1617	1620	1625	rVB2	553	881	0.08%	0.011%
61	11.000	1625	1626	1628	rBV	206	113	0.01%	0.001%
62	11.024	1628	1630	1632	rBV2	139	129	0.01%	0.002%
63	11.091	1637	1641	1647	rVB	2172	2808	0.26%	0.034%
64	11.189	1652	1657	1670	rVV	410520	526401	48.94%	6.298%
65	11.311	1670	1677	1683	rVB	15459	20701	1.92%	0.248%
66	11.451	1697	1700	1709	rBV	641	901	0.08%	0.011%
67	11.628	1725	1729	1731	rBV	213	249	0.02%	0.003%
68	11.646	1731	1732	1737	rVB2	115	130	0.01%	0.002%
69	11.707	1737	1742	1746	rBV3	491	553	0.05%	0.007%
70	11.756	1746	1750	1753	rBV2	598	972	0.09%	0.012%
71	11.860	1765	1767	1770	rBV	223	154	0.01%	0.002%
72	11.896	1770	1773	1776	rVB2	143	162	0.02%	0.002%
73	11.933	1776	1779	1781	rBV	286	209	0.02%	0.003%
74	11.969	1781	1785	1788	rBV2	1219	1513	0.14%	0.018%
75	12.018	1788	1793	1803	rBV	609017	785625	73.04%	9.399%
76	12.225	1822	1827	1837	rBV2	5034	11759	1.09%	0.141%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040969.D
 Acq On : 11 Apr 2024 11:18
 Operator : JC/MD
 Sample : P2048-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1854	rVB	674028	850998	79.12%	10.182%
78	12.536	1876	1878	1879	rBV2	178	113	0.01%	0.001%
79	12.762	1911	1915	1919	rVB	3537	4559	0.42%	0.055%
80	12.859	1925	1931	1937	rVB3	2206	3078	0.29%	0.037%
81	12.933	1941	1943	1944	rBV	150	130	0.01%	0.002%
82	13.115	1970	1973	1977	rBV2	778	861	0.08%	0.010%
83	13.176	1981	1983	1986	rVB2	104	112	0.01%	0.001%
84	13.201	1986	1987	1991	rBV	196	178	0.02%	0.002%
85	13.341	2007	2010	2012	rBV2	109	111	0.01%	0.001%
86	13.506	2035	2037	2040	rBV2	122	138	0.01%	0.002%
87	13.591	2047	2051	2056	rVB3	1453	1815	0.17%	0.022%
88	13.786	2078	2083	2089	rBV2	776	1178	0.11%	0.014%
89	13.853	2092	2094	2095	rVB	277	124	0.01%	0.001%
90	13.871	2095	2097	2098	rBV2	280	179	0.02%	0.002%
91	13.932	2105	2107	2109	rBV	266	178	0.02%	0.002%
92	13.963	2109	2112	2117	rVB2	1031	1181	0.11%	0.014%
93	14.048	2122	2126	2127	rBV2	222	253	0.02%	0.003%
94	14.127	2135	2139	2144	rBV	2949	4098	0.38%	0.049%
95	14.621	2218	2220	2221	rBV2	277	162	0.02%	0.002%
96	14.640	2221	2223	2225	rBV2	188	178	0.02%	0.002%
97	14.883	2262	2263	2264	rBV	278	132	0.01%	0.002%
98	14.975	2276	2278	2280	rBV2	259	158	0.01%	0.002%
99	15.389	2343	2346	2352	rVB5	1031	1761	0.16%	0.021%
100	16.066	2455	2457	2459	rBV2	357	287	0.03%	0.003%


Sum of corrected areas: 8358267

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040969.D
Acq On : 11 Apr 2024 11:18
Operator : JC/MD
Sample : P2048-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

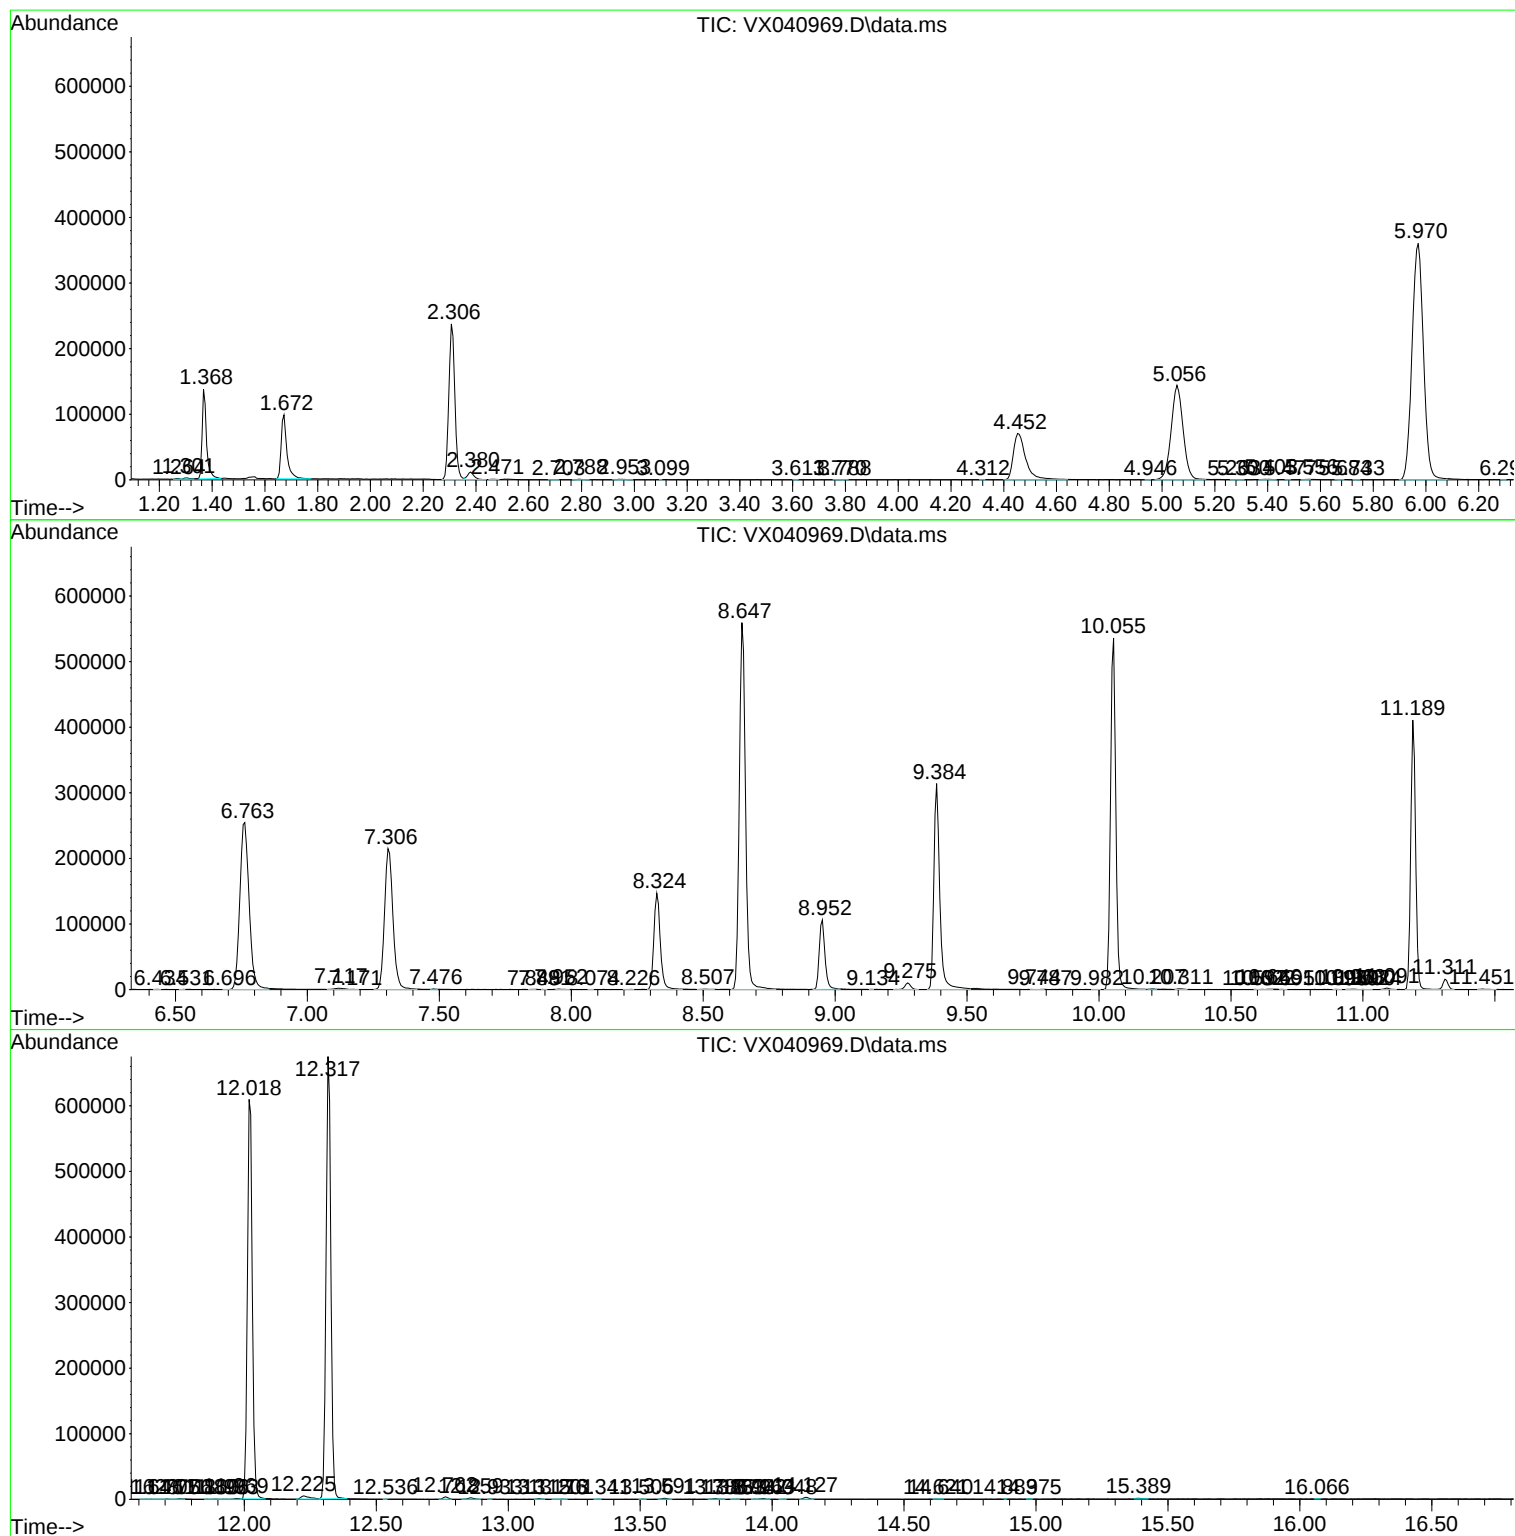

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040969.D
Acq On : 11 Apr 2024 11:18
Operator : JC/MD
Sample : P2048-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040969.D
Acq On : 11 Apr 2024 11:18
Operator : JC/MD
Sample : P2048-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc