

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040970.D
 Acq On : 11 Apr 2024 11:41
 Operator : JC/MD
 Sample : P2048-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX040970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	142870	155258	14.41%	1.806%
2	1.673	91	96	109	rBV	97916	149901	13.91%	1.743%
3	2.307	194	200	208	rBV	236535	368026	34.15%	4.280%
4	2.380	208	212	221	rVB	8223	14057	1.30%	0.163%
5	2.520	231	235	243	rVB6	931	2228	0.21%	0.026%
6	2.648	254	256	257	rBV	156	123	0.01%	0.001%
7	2.697	262	264	267	rVB	199	157	0.01%	0.002%
8	2.788	276	279	284	rVB3	593	920	0.09%	0.011%
9	2.843	286	288	292	rBV	185	173	0.02%	0.002%
10	2.880	292	294	296	rBV2	126	154	0.01%	0.002%
11	2.934	300	303	304	rBV2	633	760	0.07%	0.009%
12	3.093	327	329	332	rBV2	242	269	0.02%	0.003%
13	3.117	332	333	336	rVB	337	209	0.02%	0.002%
14	3.245	352	354	355	rBV	198	164	0.02%	0.002%
15	3.306	361	364	365	rBV2	122	121	0.01%	0.001%
16	3.325	365	367	369	rVV2	110	119	0.01%	0.001%
17	3.361	371	373	376	rBV2	125	163	0.02%	0.002%
18	3.404	378	380	382	rBV2	147	161	0.01%	0.002%
19	3.538	401	402	405	rBV	120	94	0.01%	0.001%
20	3.703	426	429	430	rBV2	105	108	0.01%	0.001%
21	4.038	483	484	487	rBV2	104	138	0.01%	0.002%
22	4.233	515	516	518	rBV2	152	113	0.01%	0.001%
23	4.361	535	537	539	rBV2	114	126	0.01%	0.001%
24	4.453	544	552	577	rBV	73550	230331	21.37%	2.679%
25	4.727	595	597	598	rBV2	204	119	0.01%	0.001%
26	4.800	607	609	611	rBV2	263	248	0.02%	0.003%
27	4.928	629	630	635	rBV2	233	224	0.02%	0.003%
28	5.056	637	651	667	rBV	139646	446987	41.48%	5.198%
29	5.391	699	706	708	rBV2	836	1702	0.16%	0.020%
30	5.477	717	720	723	rBV2	228	266	0.02%	0.003%
31	5.562	726	734	738	rBV4	1078	2582	0.24%	0.030%
32	5.641	746	747	749	rBV	160	114	0.01%	0.001%
33	5.684	749	754	757	rVV2	348	416	0.04%	0.005%
34	5.971	789	801	818	rBV2	359658	1077685	100.00%	12.533%
35	6.361	864	865	869	rVV	153	141	0.01%	0.002%
36	6.416	873	874	877	rBV2	150	105	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040970.D
 Acq On : 11 Apr 2024 11:41
 Operator : JC/MD
 Sample : P2048-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.550	892	896	897	rBV2	152	198	0.02%	0.002%
38	6.696	918	920	921	rBV	131	106	0.01%	0.001%
39	6.763	921	931	953	rBV	267555	652936	60.59%	7.593%
40	7.062	978	980	981	rBV	289	162	0.02%	0.002%

41	7.117	984	989	999	rVB6	1817	4411	0.41%	0.051%
42	7.239	1004	1009	1012	rBV4	390	870	0.08%	0.010%
43	7.306	1012	1020	1038	rBV	215194	471995	43.80%	5.489%
44	7.470	1044	1047	1048	rBV2	339	303	0.03%	0.004%
45	7.617	1069	1071	1074	rBV	130	108	0.01%	0.001%

46	7.812	1101	1103	1104	rBV	129	93	0.01%	0.001%
47	7.921	1118	1121	1122	rBV2	152	122	0.01%	0.001%
48	7.946	1122	1125	1131	rBV3	504	862	0.08%	0.010%
49	8.031	1138	1139	1141	rBV	139	96	0.01%	0.001%
50	8.153	1157	1159	1160	rBV	244	143	0.01%	0.002%

51	8.263	1173	1177	1180	rBV2	92	142	0.01%	0.002%
52	8.324	1181	1187	1200	rBV	148073	245150	22.75%	2.851%
53	8.482	1211	1213	1214	rBV2	231	115	0.01%	0.001%
54	8.647	1234	1240	1259	rBV	589660	929081	86.21%	10.804%
55	8.866	1273	1276	1278	rVB2	229	183	0.02%	0.002%

56	8.952	1284	1290	1305	rBV	108708	164562	15.27%	1.914%
57	9.275	1338	1343	1351	rVB	9641	14110	1.31%	0.164%
58	9.385	1356	1361	1381	rBV	338872	507023	47.05%	5.896%
59	9.726	1415	1417	1419	rBV2	273	333	0.03%	0.004%
60	10.055	1465	1471	1487	rBV	566917	807071	74.89%	9.386%

61	10.311	1509	1513	1519	rVB2	1189	1740	0.16%	0.020%
62	10.372	1521	1523	1525	rVV	168	137	0.01%	0.002%
63	10.403	1527	1528	1530	rBV	136	88	0.01%	0.001%
64	10.458	1533	1537	1540	rVV2	158	231	0.02%	0.003%
65	10.647	1565	1568	1570	rBV	531	614	0.06%	0.007%

66	10.707	1576	1578	1582	rVB2	89	98	0.01%	0.001%
67	10.921	1611	1613	1614	rVB	208	112	0.01%	0.001%
68	10.964	1616	1620	1625	rBV2	675	889	0.08%	0.010%
69	11.092	1636	1641	1647	rVB3	2229	3281	0.30%	0.038%
70	11.134	1647	1648	1649	rBV	191	89	0.01%	0.001%

71	11.189	1652	1657	1670	rVV	435820	549058	50.95%	6.385%
72	11.317	1673	1678	1682	rVB	14105	20190	1.87%	0.235%
73	11.457	1696	1701	1705	rVB2	760	1079	0.10%	0.013%
74	11.488	1705	1706	1709	rBV2	153	190	0.02%	0.002%
75	11.604	1722	1725	1726	rVB	190	167	0.02%	0.002%

76	11.713	1740	1743	1745	rVV3	499	502	0.05%	0.006%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040970.D
 Acq On : 11 Apr 2024 11:41
 Operator : JC/MD
 Sample : P2048-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MC0R85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.762	1747	1751	1758	rVB5	647	1277	0.12%	0.015%
78	11.890	1769	1772	1777	rVB2	168	246	0.02%	0.003%
79	11.927	1777	1778	1779	rBV	262	119	0.01%	0.001%
80	11.976	1783	1786	1788	rVB2	739	708	0.07%	0.008%
81	12.018	1788	1793	1805	rBV	669638	856875	79.51%	9.965%
82	12.226	1823	1827	1837	rBV3	4477	10751	1.00%	0.125%
83	12.317	1837	1842	1855	rVB	714033	878080	81.48%	10.211%
84	12.561	1881	1882	1885	rVB2	228	158	0.01%	0.002%
85	12.725	1907	1909	1910	rVV	250	122	0.01%	0.001%
86	12.762	1910	1915	1919	rVV2	3258	4254	0.39%	0.049%
87	12.860	1928	1931	1936	rVB2	2476	2891	0.27%	0.034%
88	12.945	1943	1945	1949	rBV2	169	187	0.02%	0.002%
89	13.055	1961	1963	1965	rVB	212	176	0.02%	0.002%
90	13.079	1965	1967	1969	rVB2	149	125	0.01%	0.001%
91	13.116	1969	1973	1977	rBV4	969	1349	0.13%	0.016%
92	13.359	2012	2013	2015	rVB	171	103	0.01%	0.001%
93	13.591	2047	2051	2057	rVB	1359	1653	0.15%	0.019%
94	13.780	2078	2082	2086	rBV	843	1152	0.11%	0.013%
95	13.926	2104	2106	2108	rVB	138	107	0.01%	0.001%
96	13.963	2108	2112	2117	rBV2	996	1259	0.12%	0.015%
97	14.006	2117	2119	2120	rBV	243	144	0.01%	0.002%
98	14.128	2135	2139	2144	rBV	3032	3856	0.36%	0.045%
99	14.311	2167	2169	2170	rBV	206	119	0.01%	0.001%
100	14.859	2257	2259	2263	rVB	366	260	0.02%	0.003%


Sum of corrected areas: 8599073

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040970.D
Acq On : 11 Apr 2024 11:41
Operator : JC/MD
Sample : P2048-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

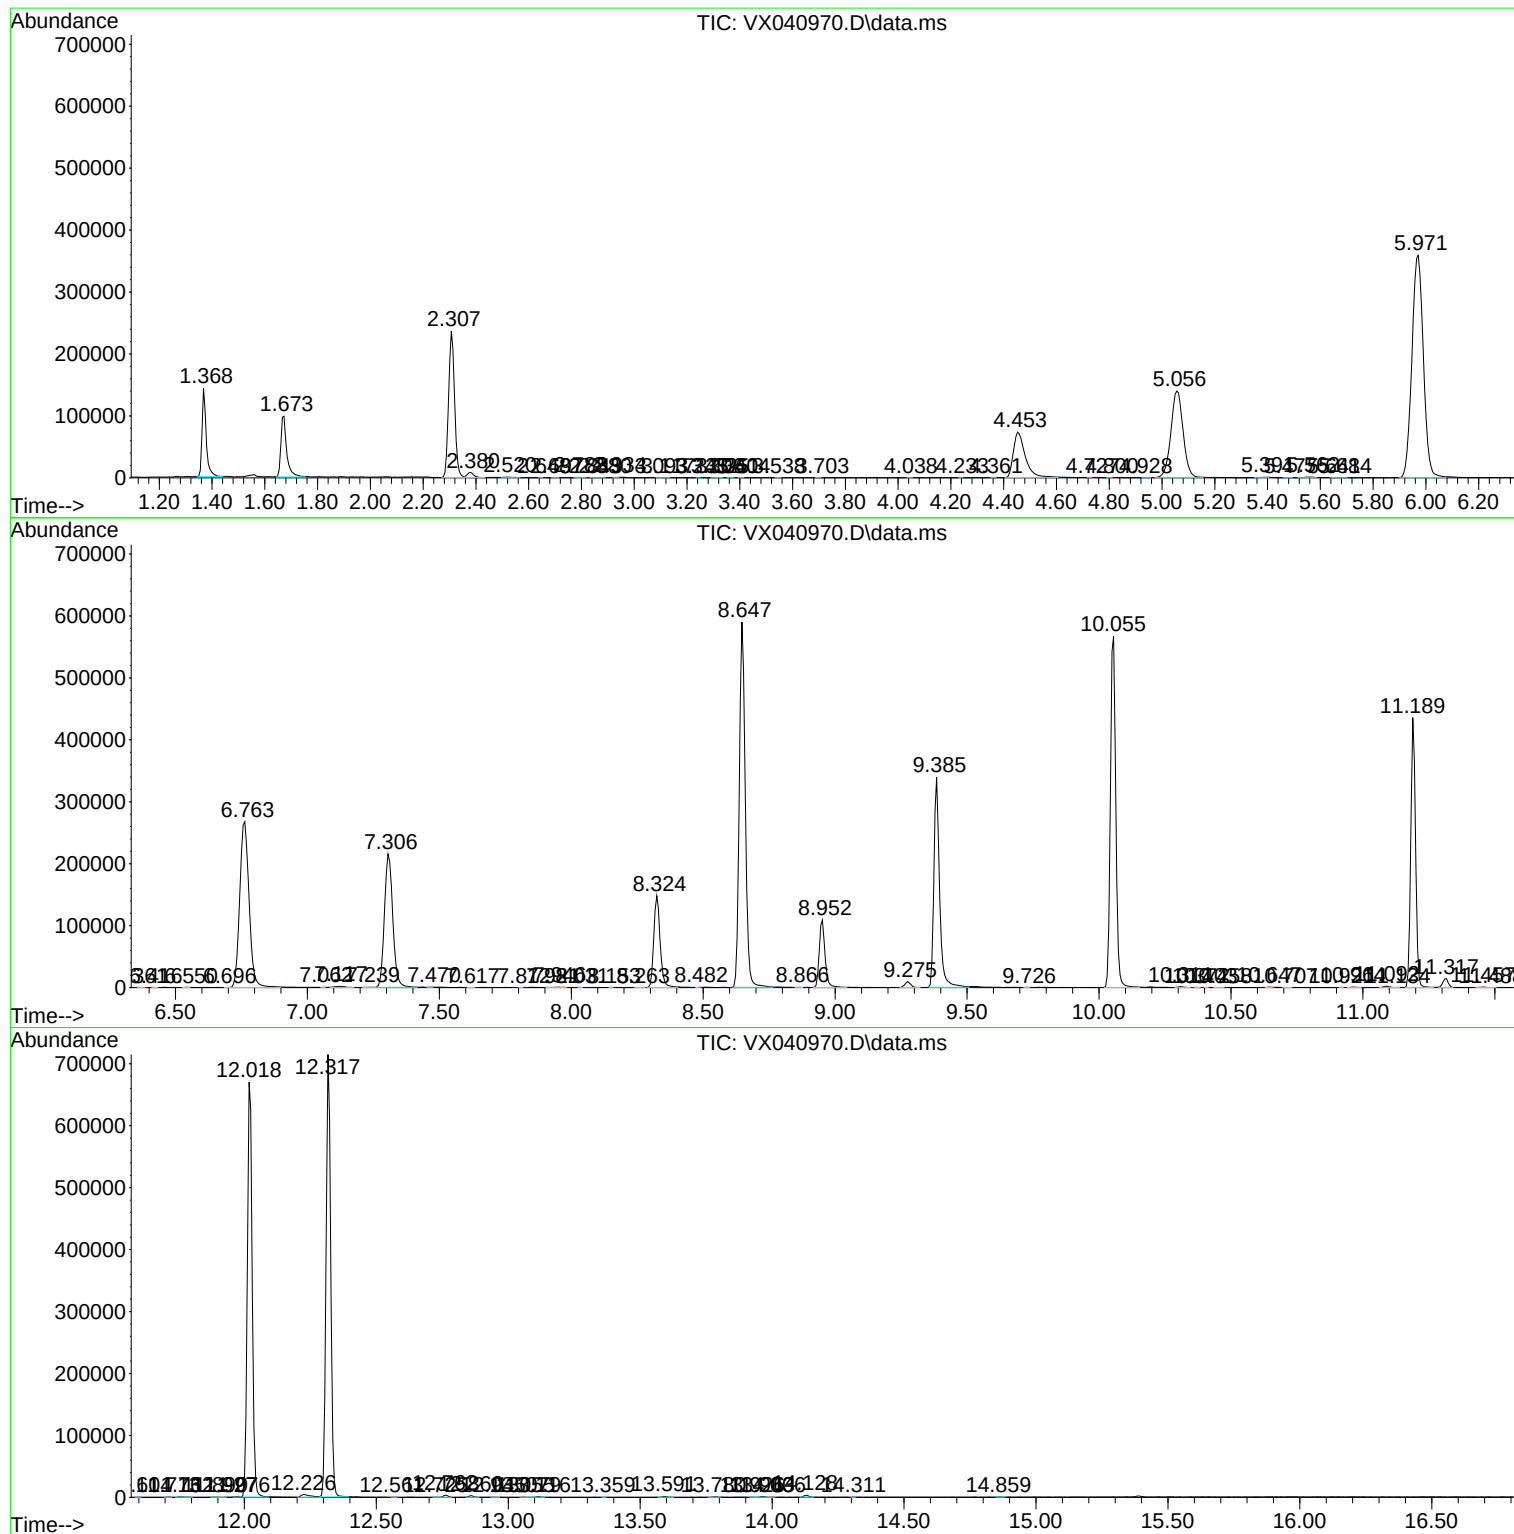

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040970.D
Acq On : 11 Apr 2024 11:41
Operator : JC/MD
Sample : P2048-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040970.D
Acq On : 11 Apr 2024 11:41
Operator : JC/MD
Sample : P2048-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MC0R85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------