

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040971.D
 Acq On : 11 Apr 2024 12:04
 Operator : JC/MD
 Sample : P2048-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

Signal : TIC: VX040971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	138334	149334	14.51%	1.826%
2	1.672	91	96	109	rBV	96000	144133	14.00%	1.762%
3	2.306	194	200	208	rBV	225050	351421	34.15%	4.296%
4	2.380	208	212	218	rVB	5372	8409	0.82%	0.103%
5	2.532	231	237	246	rBV	13863	26215	2.55%	0.320%
6	2.703	263	265	266	rBV	188	147	0.01%	0.002%
7	2.788	276	279	286	rVB4	614	1069	0.10%	0.013%
8	2.873	291	293	295	rVB	181	146	0.01%	0.002%
9	2.947	298	305	313	rVB	2113	4666	0.45%	0.057%
10	3.081	325	327	328	rBV	187	125	0.01%	0.002%
11	3.318	364	366	369	rVB	210	146	0.01%	0.002%
12	3.465	388	390	393	rBV2	80	120	0.01%	0.001%
13	3.544	397	403	405	rVB2	88	133	0.01%	0.002%
14	3.575	405	408	413	rBV2	122	222	0.02%	0.003%
15	3.837	448	451	455	rBV2	124	178	0.02%	0.002%
16	4.081	489	491	493	rBV2	118	129	0.01%	0.002%
17	4.452	544	552	566	rBV	67072	209107	20.32%	2.556%
18	4.904	623	626	628	rVB	203	190	0.02%	0.002%
19	4.928	628	630	633	rBV2	216	211	0.02%	0.003%
20	5.056	638	651	670	rBV	134940	412573	40.09%	5.044%
21	5.391	700	706	714	rVB2	710	1889	0.18%	0.023%
22	5.562	727	734	741	rBV2	802	1898	0.18%	0.023%
23	5.672	749	752	754	rVB2	160	123	0.01%	0.002%
24	5.763	764	767	770	rBV2	151	200	0.02%	0.002%
25	5.885	786	787	789	rBV	161	140	0.01%	0.002%
26	5.970	789	801	825	rBV2	344931	1029198	100.00%	12.582%
27	6.391	869	870	873	rBV	218	206	0.02%	0.003%
28	6.556	895	897	902	rVB2	225	222	0.02%	0.003%
29	6.635	906	910	911	rBV	174	139	0.01%	0.002%
30	6.763	921	931	959	rBV	244288	601546	58.45%	7.354%
31	7.117	984	989	996	rVB5	1777	4189	0.41%	0.051%
32	7.171	996	998	1001	rBV2	137	172	0.02%	0.002%
33	7.306	1012	1020	1039	rBV	203977	451773	43.90%	5.523%
34	7.482	1045	1049	1053	rBV6	495	1008	0.10%	0.012%
35	7.623	1070	1072	1074	rVB2	192	119	0.01%	0.001%
36	7.653	1076	1077	1079	rBV2	123	115	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040971.D
 Acq On : 11 Apr 2024 12:04
 Operator : JC/MD
 Sample : P2048-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CORH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	7.708	1082	1086	1088	rVB	169	191	0.02%	0.002%
38	7.738	1088	1091	1093	rBV	166	185	0.02%	0.002%
39	7.915	1116	1120	1121	rBV2	152	165	0.02%	0.002%
40	7.946	1121	1125	1133	rBV3	485	1108	0.11%	0.014%
41	8.098	1148	1150	1152	rBV2	160	160	0.02%	0.002%
42	8.238	1170	1173	1174	rBV2	198	187	0.02%	0.002%
43	8.324	1181	1187	1200	rBV	140414	234098	22.75%	2.862%
44	8.580	1225	1229	1234	rBV2	352	498	0.05%	0.006%
45	8.647	1234	1240	1259	rVV	542671	876497	85.16%	10.716%
46	8.952	1284	1290	1304	rBV	101437	155835	15.14%	1.905%
47	9.159	1323	1324	1327	rBV2	162	201	0.02%	0.002%
48	9.275	1337	1343	1349	rVB	7983	12296	1.19%	0.150%
49	9.384	1356	1361	1379	rBV	305983	468501	45.52%	5.728%
50	9.604	1395	1397	1399	rBV2	343	286	0.03%	0.003%
51	10.055	1465	1471	1483	rBV	531923	746954	72.58%	9.132%
52	10.256	1502	1504	1508	rVB2	247	279	0.03%	0.003%
53	10.305	1508	1512	1518	rBV4	770	1578	0.15%	0.019%
54	10.427	1530	1532	1533	rBV	208	155	0.02%	0.002%
55	10.500	1541	1544	1546	rVB	238	227	0.02%	0.003%
56	10.531	1546	1549	1550	rBV2	247	188	0.02%	0.002%
57	10.653	1562	1569	1571	rBV2	597	959	0.09%	0.012%
58	10.671	1571	1572	1576	rVV2	388	437	0.04%	0.005%
59	10.732	1580	1582	1585	rVV	245	208	0.02%	0.003%
60	10.774	1585	1589	1591	rVB	235	215	0.02%	0.003%
61	10.817	1595	1596	1599	rVB2	150	136	0.01%	0.002%
62	10.878	1604	1606	1607	rBV	202	148	0.01%	0.002%
63	10.970	1616	1621	1624	rBV4	638	793	0.08%	0.010%
64	11.091	1637	1641	1648	rBV4	1808	2981	0.29%	0.036%
65	11.152	1648	1651	1652	rBV	136	124	0.01%	0.002%
66	11.189	1652	1657	1666	rBV	412002	525499	51.06%	6.424%
67	11.311	1673	1677	1685	rVB	12051	16895	1.64%	0.207%
68	11.451	1696	1700	1706	rVB3	514	856	0.08%	0.010%
69	11.518	1706	1711	1712	rBV	201	243	0.02%	0.003%
70	11.610	1722	1726	1727	rBV	220	205	0.02%	0.003%
71	11.707	1740	1742	1746	rBV3	377	436	0.04%	0.005%
72	11.762	1746	1751	1755	rVB3	530	811	0.08%	0.010%
73	11.829	1760	1762	1766	rBV2	115	167	0.02%	0.002%
74	11.969	1782	1785	1788	rBV2	750	1036	0.10%	0.013%
75	12.018	1788	1793	1805	rBV	651742	822017	79.87%	10.050%
76	12.232	1822	1828	1837	rBV2	4413	10996	1.07%	0.134%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040971.D
 Acq On : 11 Apr 2024 12:04
 Operator : JC/MD
 Sample : P2048-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0RH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1855	rVB	692138	877833	85.29%	10.732%
78	12.597	1886	1888	1891	rVB2	177	164	0.02%	0.002%
79	12.628	1891	1893	1896	rBV	193	205	0.02%	0.003%
80	12.670	1898	1900	1902	rBV	218	159	0.02%	0.002%
81	12.762	1911	1915	1920	rVB3	2714	3745	0.36%	0.046%
82	12.872	1930	1933	1934	rBV2	117	127	0.01%	0.002%
83	12.994	1952	1953	1955	rBV	194	144	0.01%	0.002%
84	13.122	1971	1974	1979	rVB3	805	1028	0.10%	0.013%
85	13.213	1986	1989	1991	rBV	182	171	0.02%	0.002%
86	13.244	1991	1994	1995	rBV	130	136	0.01%	0.002%
87	13.500	2032	2036	2037	rBV3	135	174	0.02%	0.002%
88	13.561	2044	2046	2047	rBV	148	145	0.01%	0.002%
89	13.591	2047	2051	2058	rVB4	987	1747	0.17%	0.021%
90	13.640	2058	2059	2061	rBV	199	141	0.01%	0.002%
91	13.737	2073	2075	2076	rBV	230	124	0.01%	0.002%
92	13.786	2079	2083	2086	rBV2	608	1023	0.10%	0.013%
93	13.920	2103	2105	2106	rBV2	211	148	0.01%	0.002%
94	13.963	2109	2112	2117	rVB3	583	928	0.09%	0.011%
95	14.000	2117	2118	2120	rBV	150	131	0.01%	0.002%
96	14.091	2130	2133	2135	rBV2	297	349	0.03%	0.004%
97	14.128	2135	2139	2145	rVV	2769	3930	0.38%	0.048%
98	14.225	2153	2155	2157	rVB	236	153	0.01%	0.002%
99	14.438	2188	2190	2193	rVB2	274	203	0.02%	0.002%
100	14.701	2230	2233	2236	rBV3	259	364	0.04%	0.004%




Sum of corrected areas: 8179634

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040971.D
Acq On : 11 Apr 2024 12:04
Operator : JC/MD
Sample : P2048-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CORH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

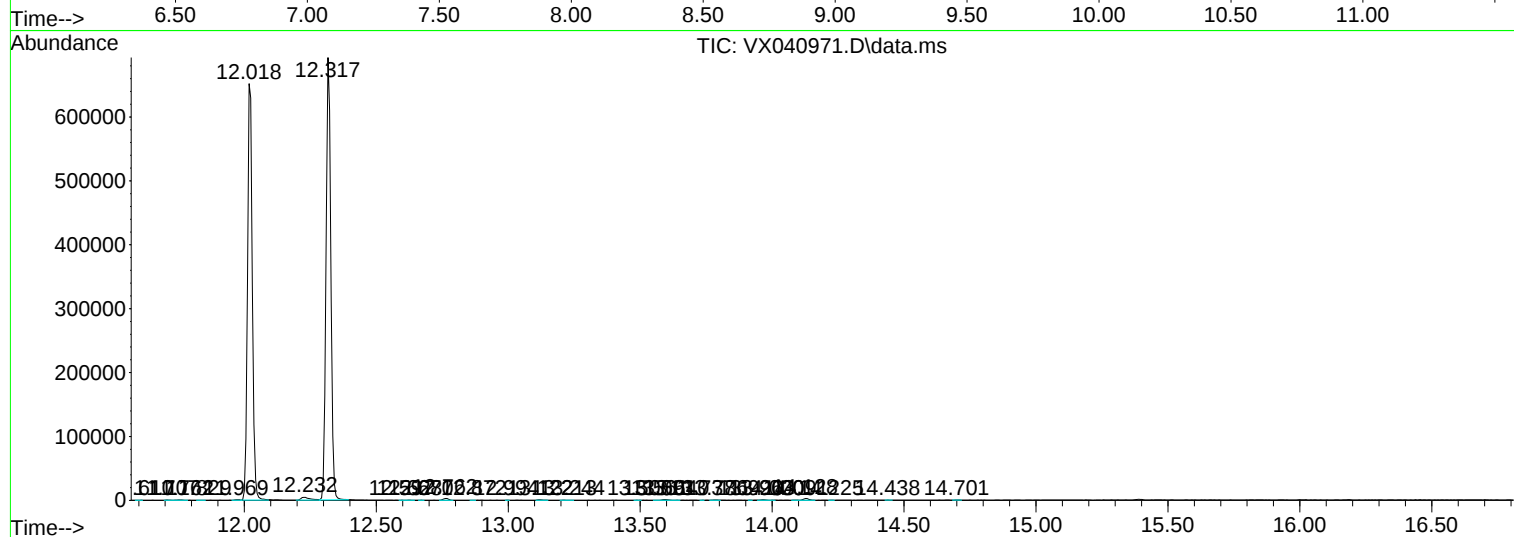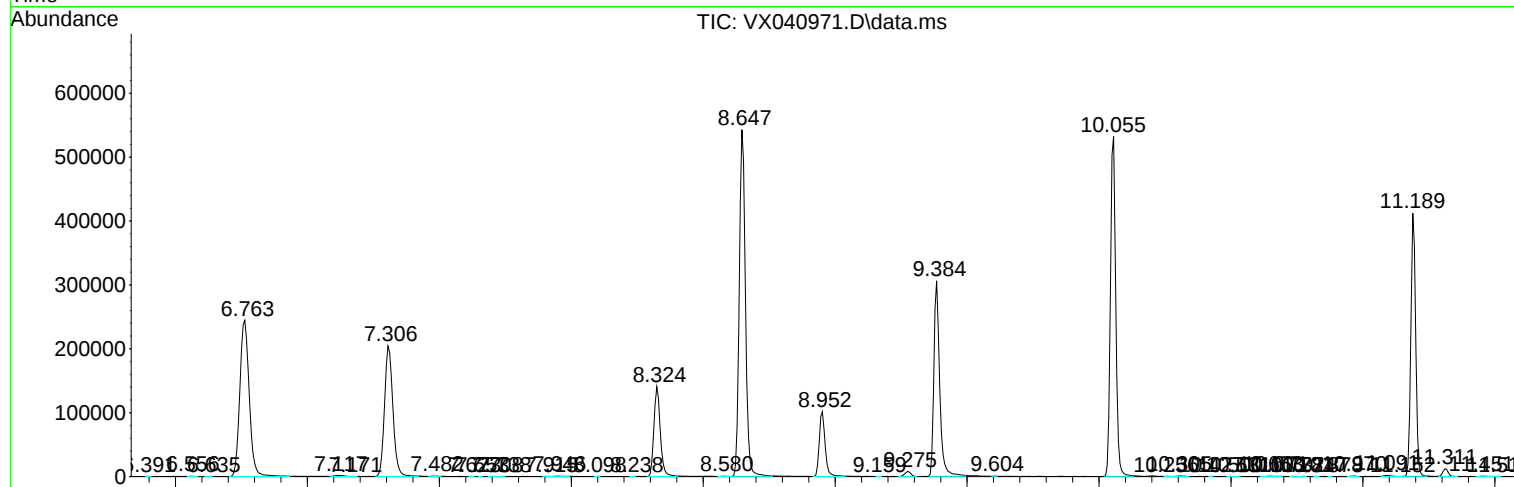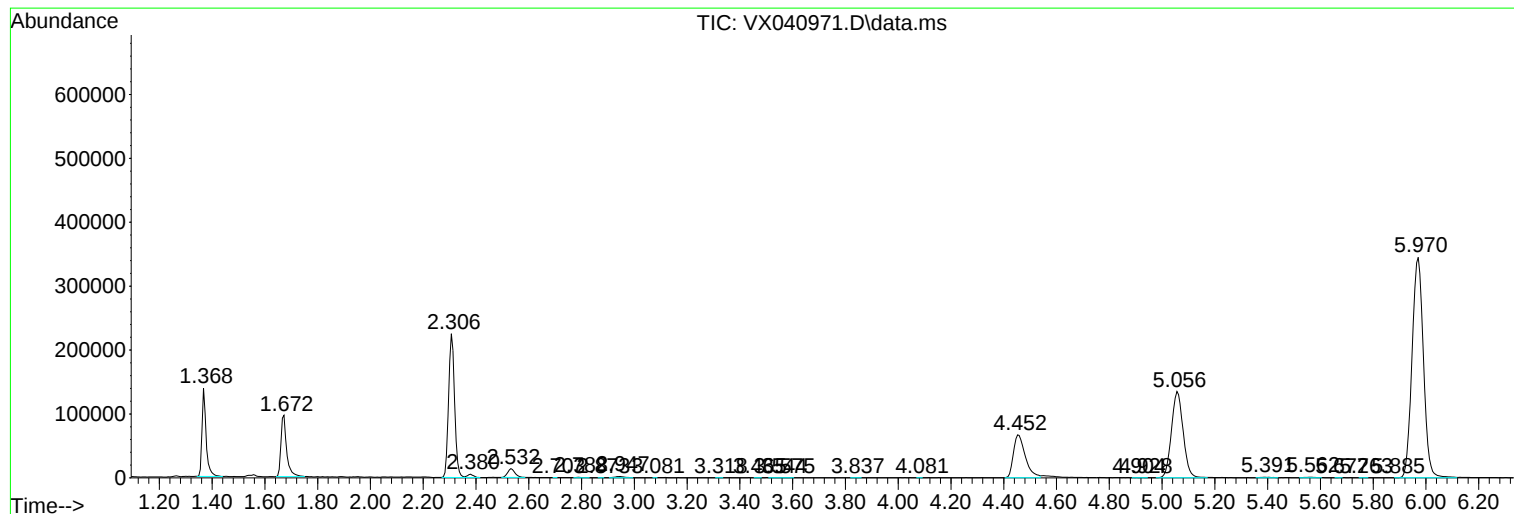

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040971.D
Acq On : 11 Apr 2024 12:04
Operator : JC/MD
Sample : P2048-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040971.D
Acq On : 11 Apr 2024 12:04
Operator : JC/MD
Sample : P2048-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0RH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc