

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040976.D
 Acq On : 11 Apr 2024 14:22
 Operator : JC/MD
 Sample : VIBLK655
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M

Title : VOC Analysis

Signal : TIC: VX040976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	24	28	32	rBV2	3016	5875	0.56%	0.071%
2	1.368	42	46	62	rVB	109929	123198	11.81%	1.493%
3	1.666	91	95	112	rVB	84164	124845	11.97%	1.513%
4	2.306	193	200	210	rBV	185844	288251	27.64%	3.494%
5	2.465	223	226	230	rBV4	578	1084	0.10%	0.013%
6	2.758	272	274	275	rBV	194	112	0.01%	0.001%
7	2.794	275	280	284	rVV2	1527	2927	0.28%	0.035%
8	2.855	287	290	292	rVB2	170	157	0.02%	0.002%
9	2.940	297	304	315	rVB2	3587	8535	0.82%	0.103%
10	3.044	318	321	323	rVB2	219	163	0.02%	0.002%
11	3.111	323	332	338	rBV6	901	2264	0.22%	0.027%
12	3.196	341	346	348	rVB3	186	269	0.03%	0.003%
13	3.343	367	370	371	rBV2	126	119	0.01%	0.001%
14	3.440	383	386	387	rBV2	169	151	0.01%	0.002%
15	3.593	408	411	412	rBV2	166	155	0.01%	0.002%
16	3.690	425	427	429	rVV	132	146	0.01%	0.002%
17	3.709	429	430	433	rVB2	217	210	0.02%	0.003%
18	3.739	433	435	438	rBV	218	249	0.02%	0.003%
19	3.946	465	469	470	rBV	226	153	0.01%	0.002%
20	4.056	486	487	490	rVB	214	124	0.01%	0.002%
21	4.111	493	496	499	rBV2	160	204	0.02%	0.002%
22	4.324	529	531	533	rVB2	158	129	0.01%	0.002%
23	4.355	533	536	537	rBV	162	180	0.02%	0.002%
24	4.452	543	552	567	rBV	78608	245352	23.53%	2.974%
25	5.056	639	651	667	rBV	123849	387001	37.11%	4.691%
26	5.391	700	706	714	rVB4	836	2077	0.20%	0.025%
27	5.464	714	718	722	rBV4	455	859	0.08%	0.010%
28	5.562	727	734	735	rBV2	1082	1722	0.17%	0.021%
29	5.678	748	753	754	rBV3	333	425	0.04%	0.005%
30	5.879	783	786	788	rBV2	129	153	0.01%	0.002%
31	5.970	789	801	808	rBV2	326491	981723	94.15%	11.900%
32	6.318	856	858	859	rVB	245	136	0.01%	0.002%
33	6.379	864	868	871	rBV	258	335	0.03%	0.004%
34	6.556	892	897	898	rBV3	225	274	0.03%	0.003%
35	6.629	908	909	911	rVB2	193	139	0.01%	0.002%
36	6.678	916	917	920	rBV	153	125	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040976.D
 Acq On : 11 Apr 2024 14:22
 Operator : JC/MD
 Sample : VIBLK655
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

37	6.763	922	931	952	rBV	238108	586801	56.27%	7.113%
38	7.123	983	990	997	rVB7	2120	5725	0.55%	0.069%
39	7.306	1011	1020	1039	rBV	197905	437151	41.92%	5.299%
40	7.592	1066	1067	1070	rVB2	241	213	0.02%	0.003%
41	7.629	1070	1073	1075	rBV2	165	206	0.02%	0.002%
42	7.714	1085	1087	1089	rVB2	181	180	0.02%	0.002%
43	7.738	1089	1091	1093	rBV2	134	153	0.01%	0.002%
44	7.818	1103	1104	1105	rBV	196	142	0.01%	0.002%
45	7.946	1122	1125	1127	rBV3	437	458	0.04%	0.006%
46	8.147	1154	1158	1161	rVB	205	230	0.02%	0.003%
47	8.177	1161	1163	1166	rBV	120	119	0.01%	0.001%
48	8.269	1176	1178	1181	rBV2	138	111	0.01%	0.001%
49	8.324	1181	1187	1207	rVV	127429	220978	21.19%	2.679%
50	8.580	1226	1229	1234	rVB3	1128	1700	0.16%	0.021%
51	8.647	1234	1240	1250	rBV	504104	788606	75.63%	9.559%
52	8.891	1279	1280	1284	rVB2	195	119	0.01%	0.001%
53	8.952	1284	1290	1304	rBV	94297	148044	14.20%	1.795%
54	9.165	1321	1325	1330	rVB3	771	1104	0.11%	0.013%
55	9.281	1338	1344	1350	rVB3	1871	2758	0.26%	0.033%
56	9.384	1356	1361	1378	rBV	353599	528322	50.67%	6.404%
57	9.701	1410	1413	1417	rBV2	753	1085	0.10%	0.013%
58	9.933	1449	1451	1453	rBV	228	204	0.02%	0.002%
59	9.970	1456	1457	1459	rVB	222	159	0.02%	0.002%
60	10.000	1461	1462	1465	rVB2	160	165	0.02%	0.002%
61	10.055	1465	1471	1473	rBV	552566	791004	75.86%	9.588%
62	10.274	1504	1507	1508	rBV	293	285	0.03%	0.003%
63	10.305	1508	1512	1519	rVV3	1787	3096	0.30%	0.038%
64	10.384	1522	1525	1528	rBV4	214	350	0.03%	0.004%
65	10.592	1558	1559	1561	rBV2	163	142	0.01%	0.002%
66	10.616	1561	1563	1564	rBV	155	112	0.01%	0.001%
67	10.646	1564	1568	1569	rBV2	1421	1616	0.15%	0.020%
68	10.805	1592	1594	1597	rBV3	400	474	0.05%	0.006%
69	10.963	1615	1620	1625	rBV2	1509	2125	0.20%	0.026%
70	11.055	1633	1635	1636	rVB	220	127	0.01%	0.002%
71	11.085	1636	1640	1650	rBV2	2569	3924	0.38%	0.048%
72	11.189	1652	1657	1664	rBV	418095	544123	52.18%	6.596%
73	11.311	1673	1677	1683	rVB2	1598	2465	0.24%	0.030%
74	11.408	1689	1693	1696	rBV2	125	269	0.03%	0.003%
75	11.457	1696	1701	1707	rVB3	1376	1846	0.18%	0.022%
76	11.713	1740	1743	1745	rVB2	317	287	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
 Data File : VX040976.D
 Acq On : 11 Apr 2024 14:22
 Operator : JC/MD
 Sample : VIBLK655
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
 Title : VOC Analysis

77	11.756	1747	1750	1756	rVB	1669	1815	0.17%	0.022%
78	11.969	1780	1785	1788	rBV	8908	11257	1.08%	0.136%
79	12.024	1788	1794	1804	rVB2	625370	1042748	100.00%	12.640%
80	12.189	1820	1821	1824	rVB2	581	390	0.04%	0.005%
81	12.317	1837	1842	1858	rBV2	643937	908274	87.10%	11.010%
82	12.548	1879	1880	1883	rVB3	204	154	0.01%	0.002%
83	12.762	1910	1915	1919	rBV3	3115	4153	0.40%	0.050%
84	12.859	1927	1931	1933	rBV3	155	203	0.02%	0.002%
85	13.115	1970	1973	1978	rVB2	1516	1929	0.18%	0.023%
86	13.292	1999	2002	2004	rBV2	217	176	0.02%	0.002%
87	13.341	2009	2010	2012	rBV2	122	111	0.01%	0.001%
88	13.402	2018	2020	2022	rBV2	174	165	0.02%	0.002%
89	13.439	2025	2026	2030	rVB	226	177	0.02%	0.002%
90	13.475	2030	2032	2034	rBV	136	135	0.01%	0.002%
91	13.591	2046	2051	2056	rBV2	8567	11443	1.10%	0.139%
92	13.719	2070	2072	2075	rVB	220	210	0.02%	0.003%
93	13.786	2079	2083	2086	rBV3	1151	1658	0.16%	0.020%
94	13.902	2099	2102	2103	rBV3	189	223	0.02%	0.003%
95	13.963	2109	2112	2117	rVB2	1694	2068	0.20%	0.025%
96	14.030	2121	2123	2127	rBV3	168	248	0.02%	0.003%
97	14.127	2134	2139	2143	rBV	3070	4487	0.43%	0.054%
98	14.390	2181	2182	2184	rBV	287	204	0.02%	0.002%
99	15.286	2327	2329	2330	rBV2	432	304	0.03%	0.004%
100	16.505	2527	2529	2530	rBV2	423	233	0.02%	0.003%




Sum of corrected areas: 8249564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040976.D
Acq On : 11 Apr 2024 14:22
Operator : JC/MD
Sample : VIBLK655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

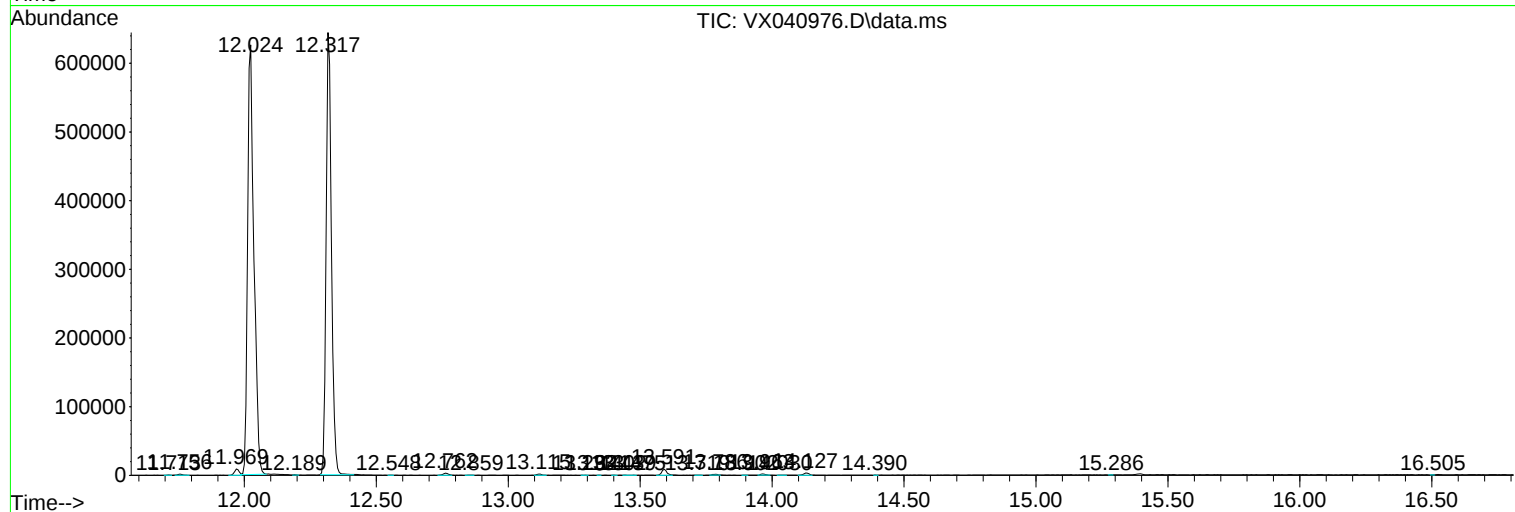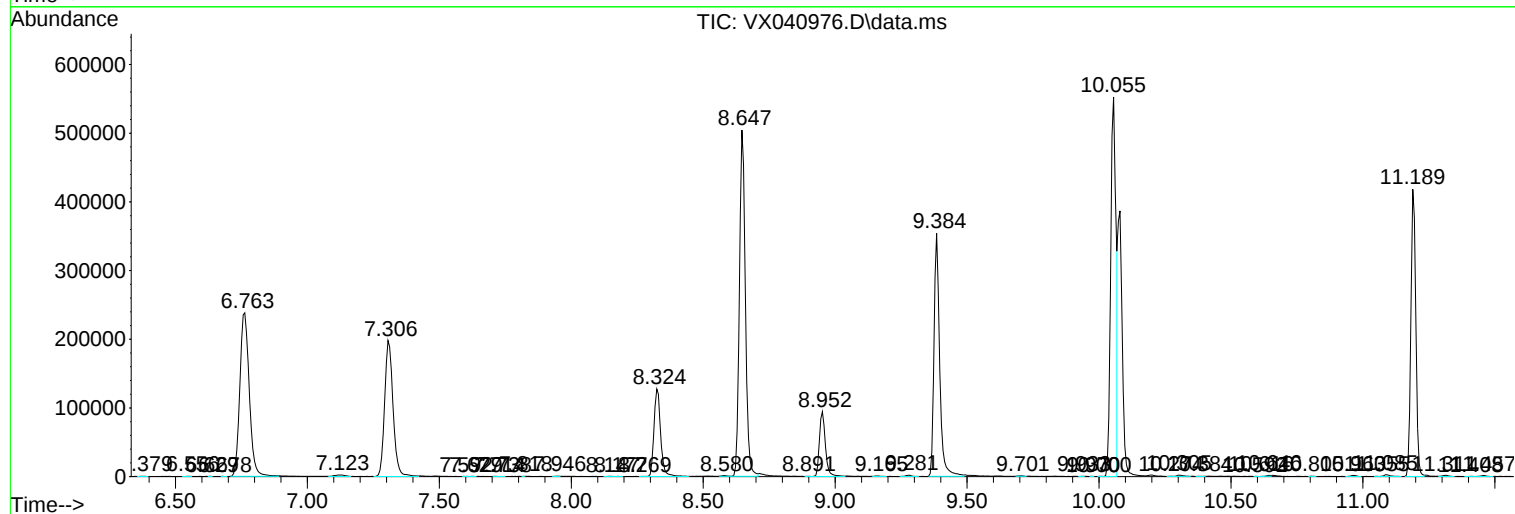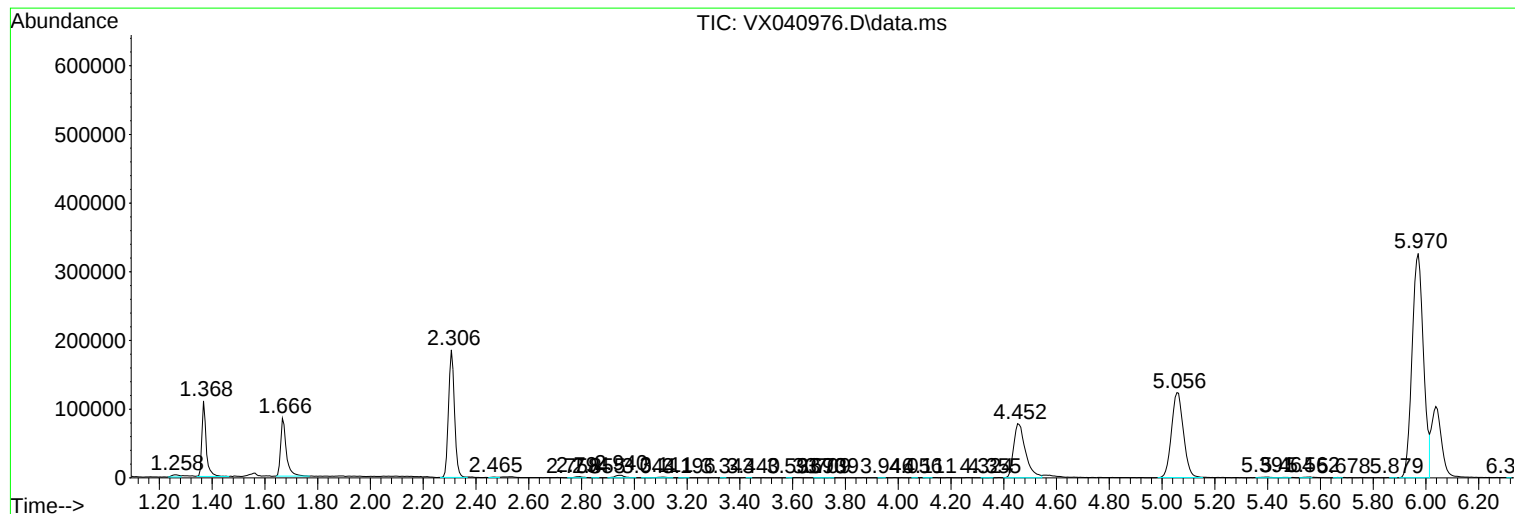

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040976.D
Acq On : 11 Apr 2024 14:22
Operator : JC/MD
Sample : VIBLK655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX041124\
Data File : VX040976.D
Acq On : 11 Apr 2024 14:22
Operator : JC/MD
Sample : VIBLK655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML041024WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
